

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
 Data File : PL065162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 10:46
 Operator : AR\AJ
 Sample : M1579-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:17:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.096	33838280	27121809	11.508	10.922
28)	SA Decachlor...	8.140	9.251	35259850	29771935	12.706	13.554
Target Compounds							
12)	B 4,4'-DDE	5.564	6.470	3407692	3249365	0.948	1.300 #
13)	MA Dieldrin	5.688	0.000	2109800	0	0.570	N.D. #
14)	MA Endrin	5.950	0.000	595833	0	0.174	N.D. #
17)	MA 4,4'-DDT	6.311	0.000	3352535	0	1.203	N.D. #
20)	A Methoxychlor	6.841f	0.000	277413	0	0.176	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
Data File : PL065162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 10:46
Operator : AR\AJ
Sample : M1579-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:17:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

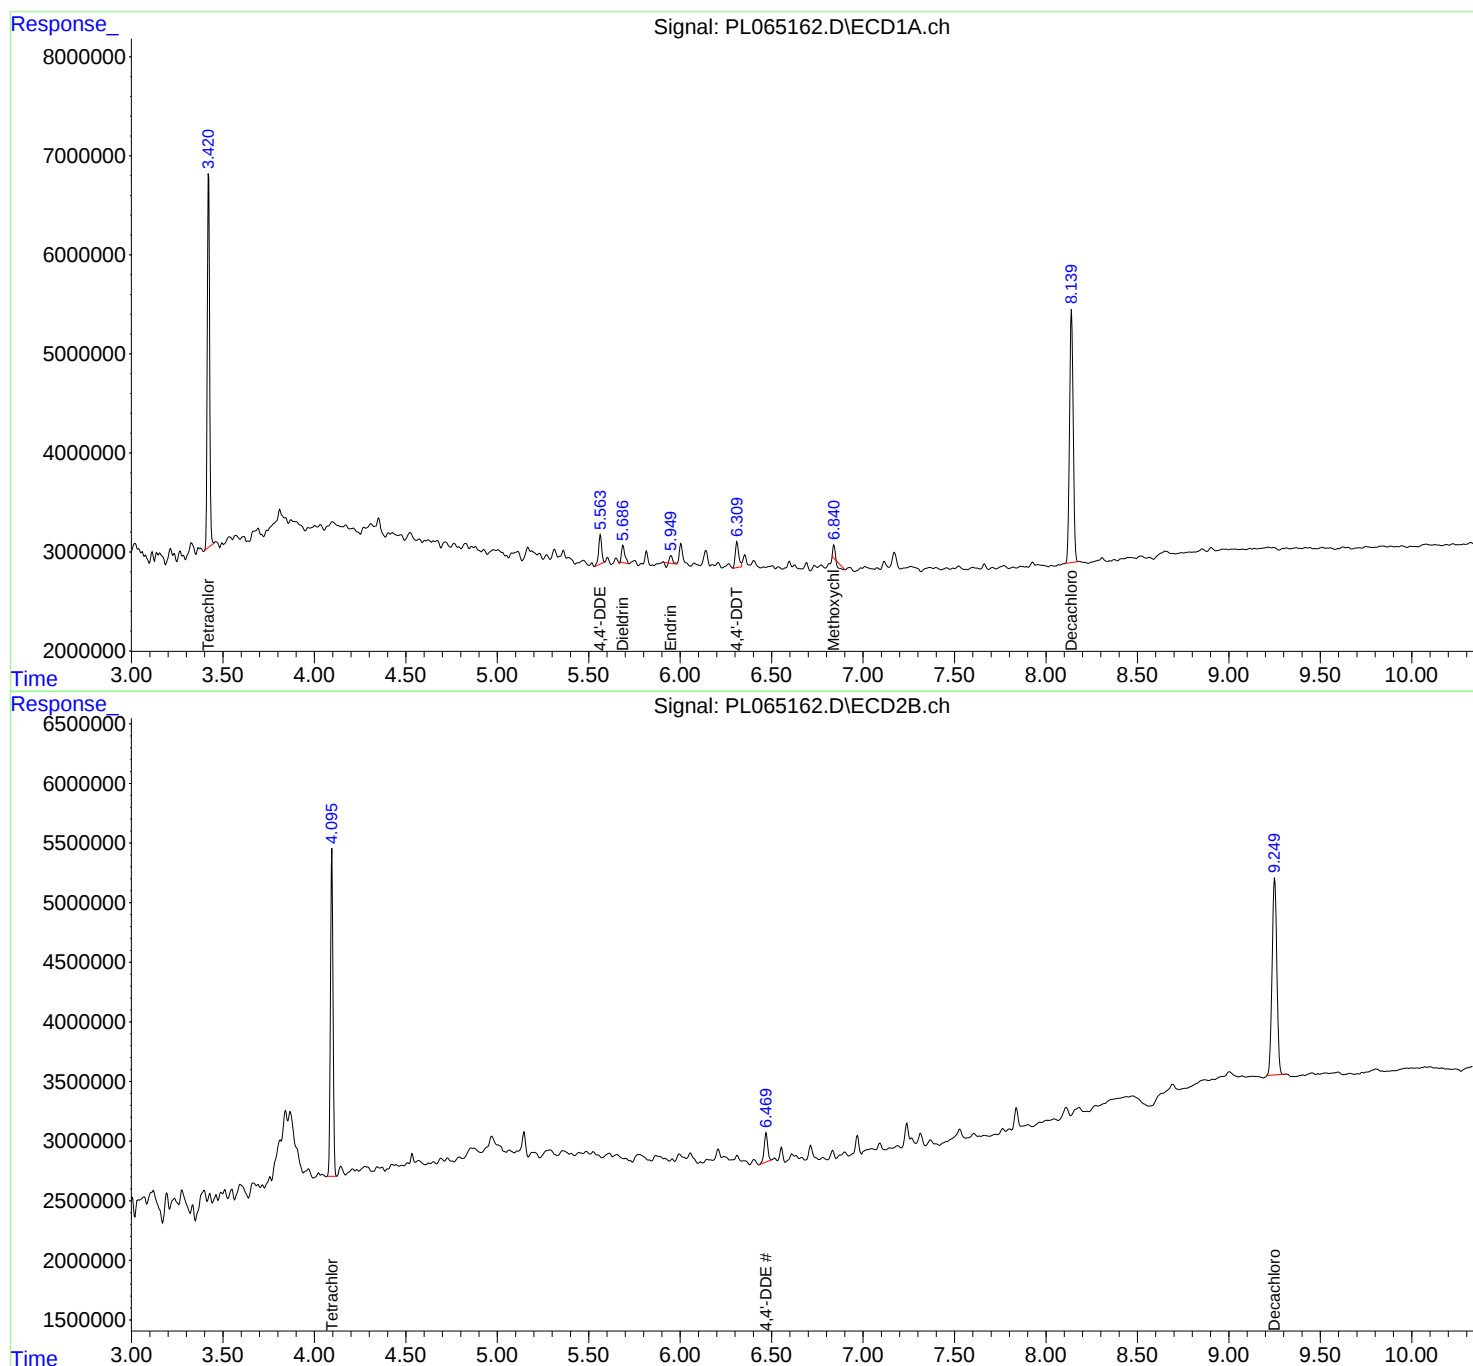


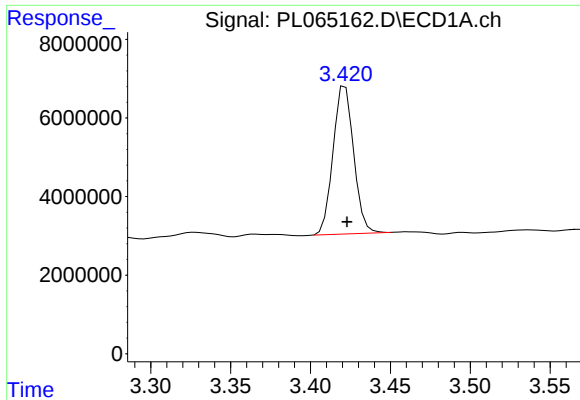

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.001 min
Response: 33838280
Conc: 11.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

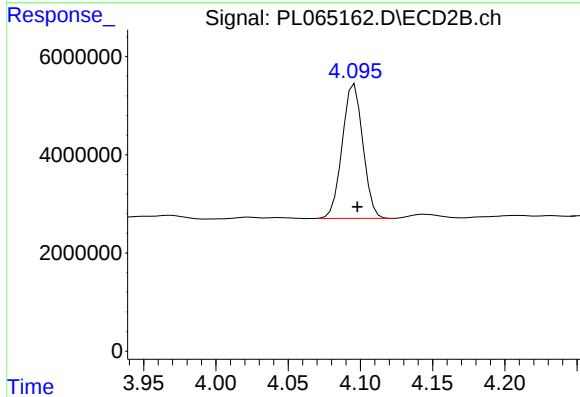


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.002 min
Response: 27121809
Conc: 10.92 ng/ml

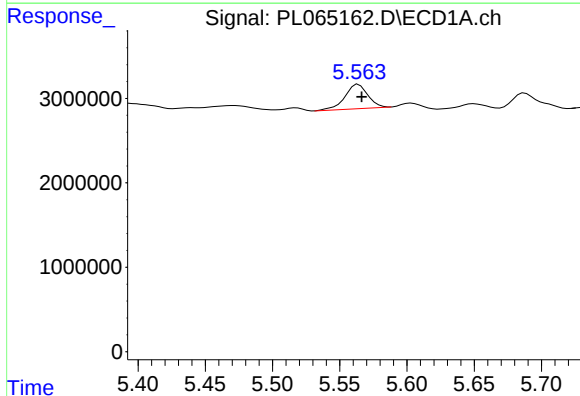


#12 4,4'-DDE

R.T.: 5.564 min
Delta R.T.: -0.003 min
Response: 3407692
Conc: 0.95 ng/ml

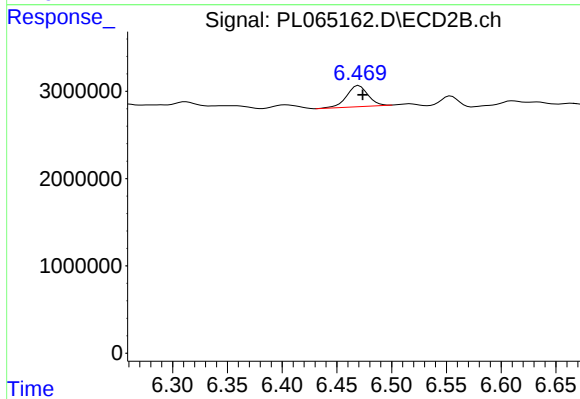

#12 4,4'-DDE


R.T.: 6.470 min
Delta R.T.: -0.004 min
Response: 3249365
Conc: 1.30 ng/ml

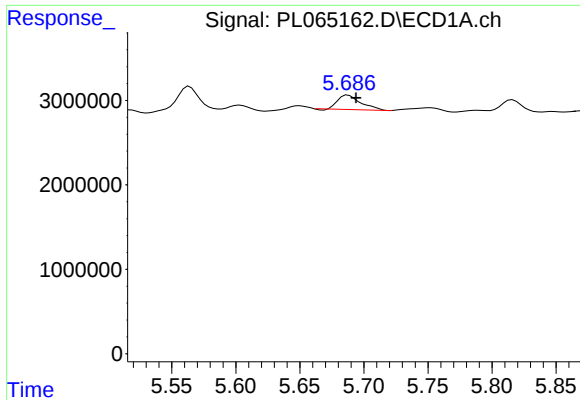

#13 Dieldrin


R.T.: 5.688 min
Delta R.T.: -0.006 min
Response: 2109800
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

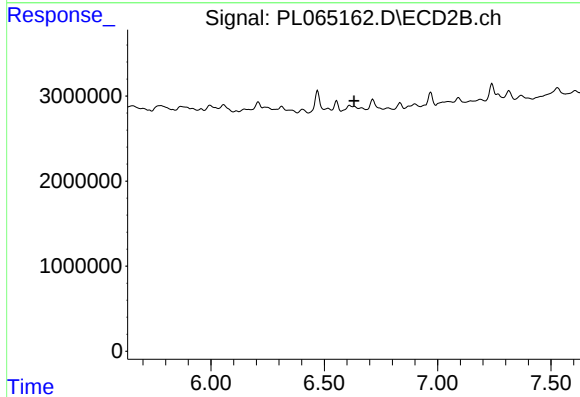


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

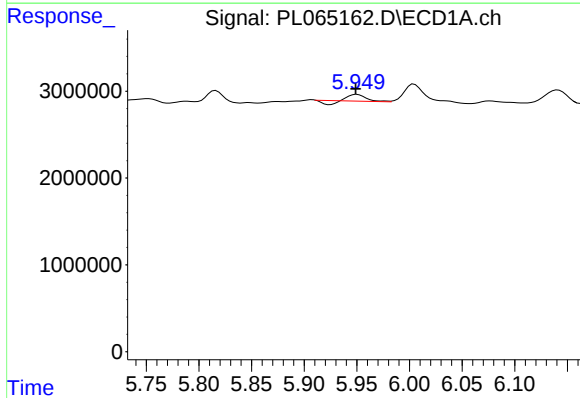


#14 Endrin

R.T.: 5.950 min
Delta R.T.: 0.001 min
Response: 595833
Conc: 0.17 ng/ml

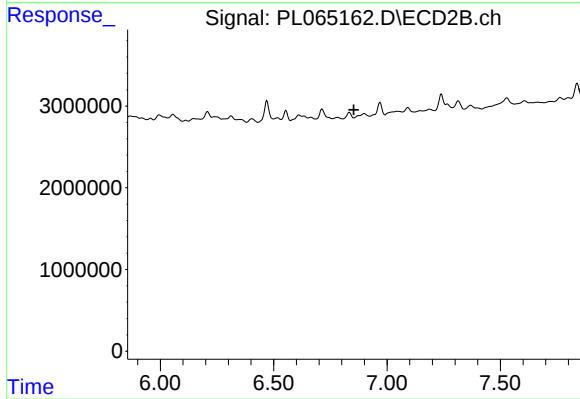

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

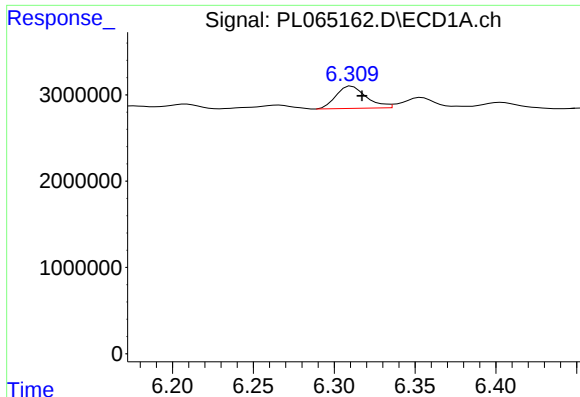

#17 4,4'-DDT


R.T.: 6.311 min
Delta R.T.: -0.006 min
Response: 3352535
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

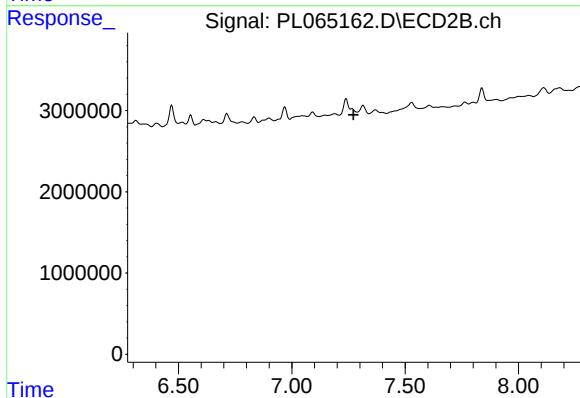


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.273 min
Response: 0
Conc: N.D.

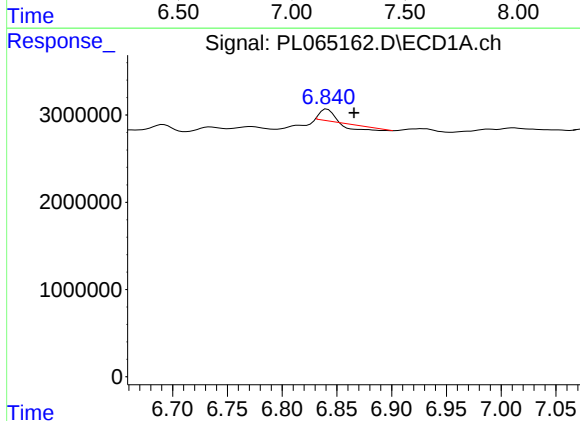


#20 Methoxychlor

R.T.: 6.841 min
Delta R.T.: -0.025 min
Response: 277413
Conc: 0.18 ng/ml

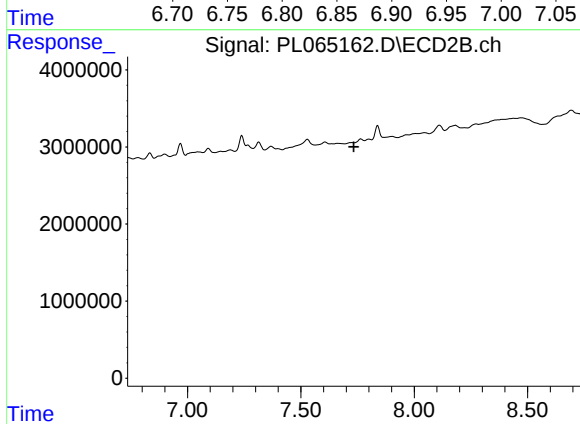

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.734 min
Response: 0
Conc: N.D.

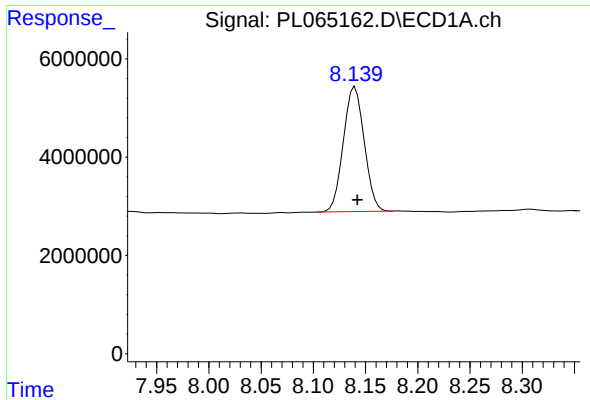

#28 Decachlorobiphenyl

R.T.: 8.140 min
Delta R.T.: -0.002 min
Response: 35259850
Conc: 12.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

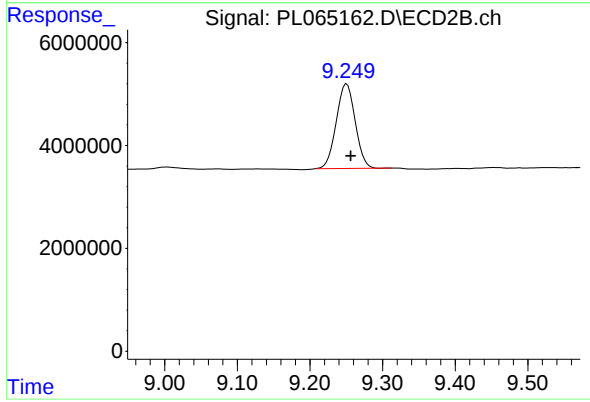

#28 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.005 min
Response: 29771935
Conc: 13.55 ng/ml