

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
 Data File : PL065172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 13:38
 Operator : AR\AJ
 Sample : M1601-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:20:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.096	38138799	30260166	12.970	12.186
28)	SA Decachlor...	8.138	9.250	31187934	24200985	11.238	11.018
Target Compounds							
4)	MA Heptachlor	4.440	0.000	1139459	0	0.259	N.D. #
5)	MB Aldrin	4.653f	0.000	1147555	0	0.281	N.D. #
6)	B beta-BHC	0.000	4.979	0	7667378	N.D.	5.015 #
9)	A Endosulfan I	5.465	0.000	4125679	0	1.154	N.D. #
10)	B gamma-Chl...	5.340	0.000	6700992	0	1.711	N.D. #
12)	B 4,4'-DDE	5.563	6.469	7406097	7436748	2.061	2.975 #
23)	Chlordane-1	4.279	0.000	7301502	0	57.285	N.D. #
25)	Chlordane-3	5.340	0.000	6700992	0	16.797	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
Data File : PL065172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 13:38
Operator : AR\AJ
Sample : M1601-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:20:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

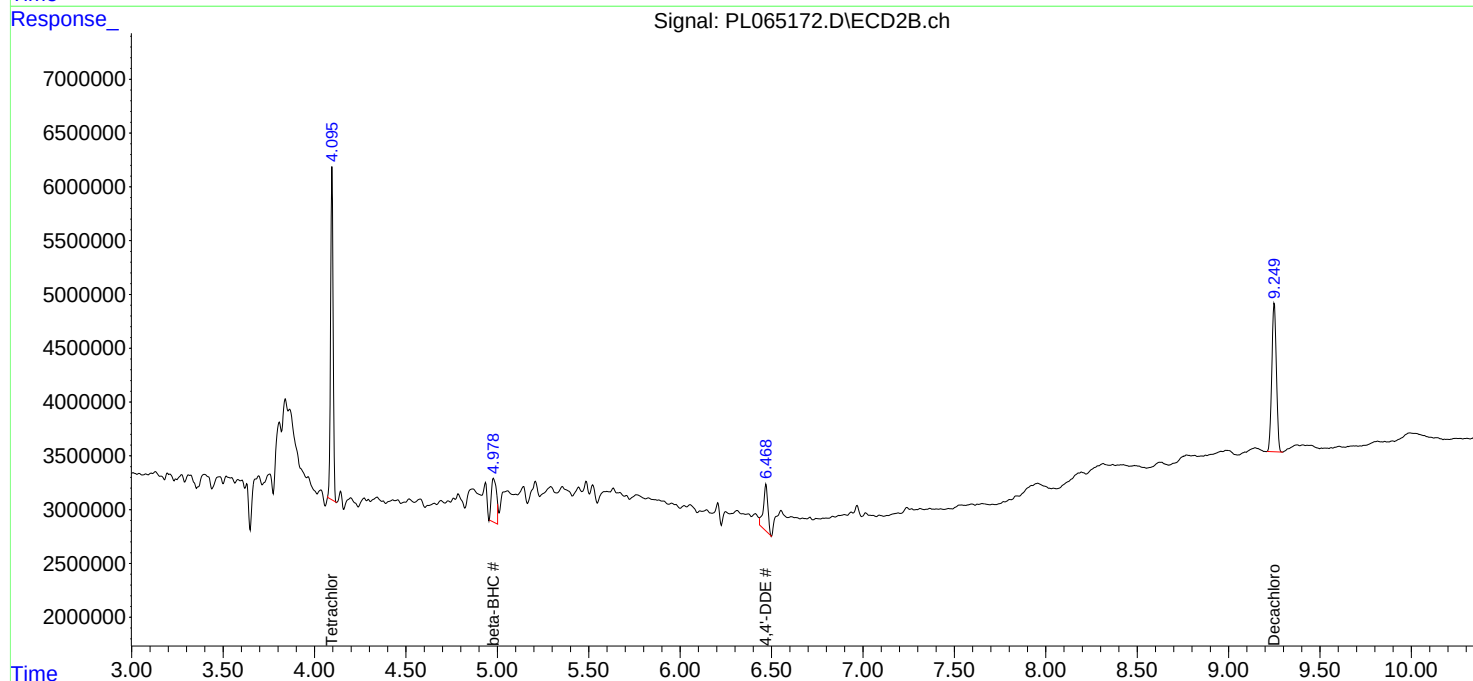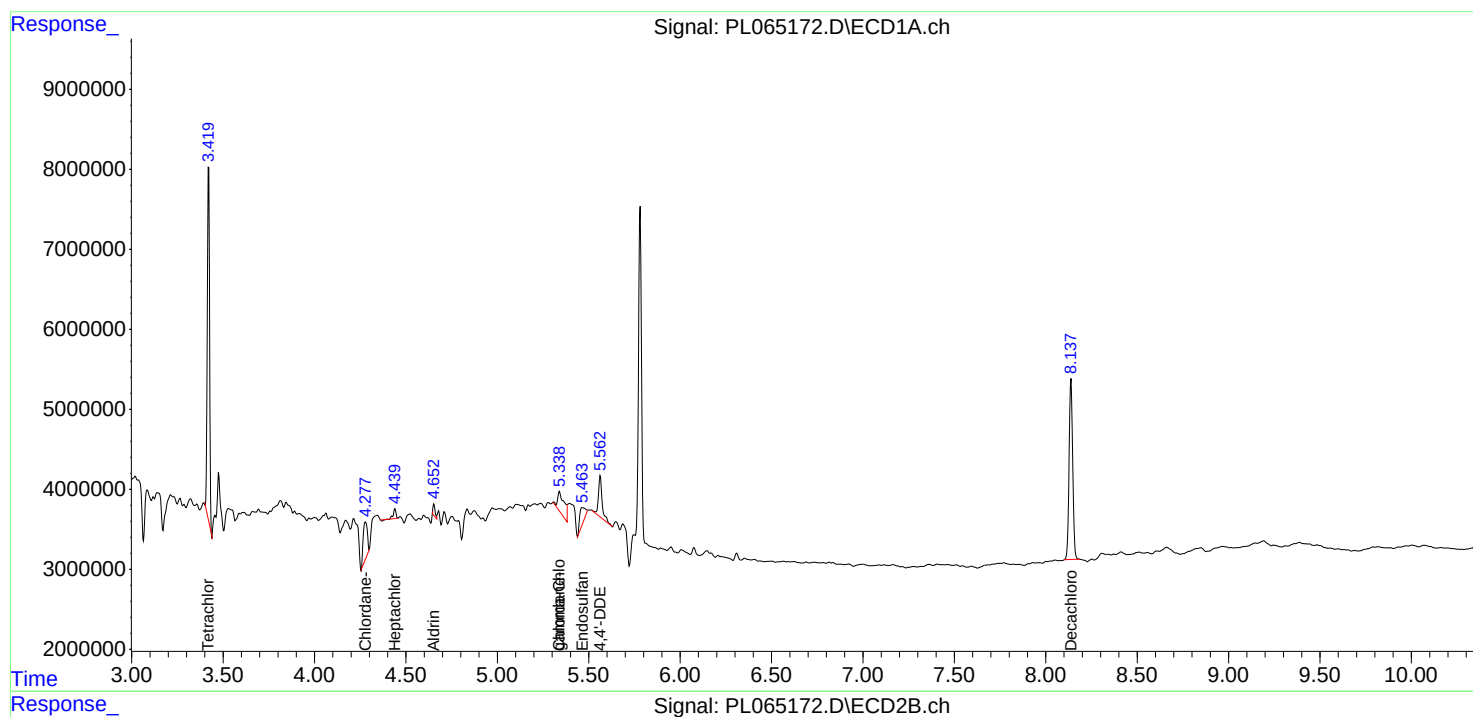


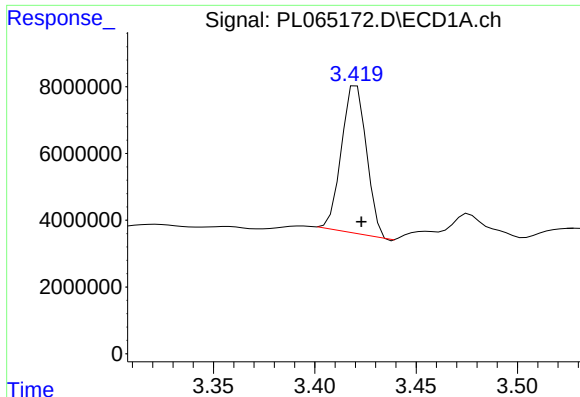

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: -0.002 min
Response: 38138799
Conc: 12.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

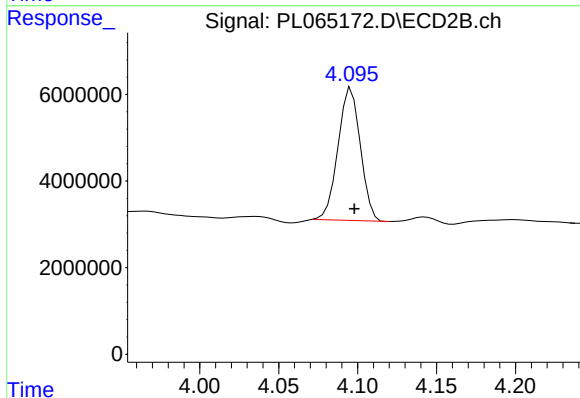


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.002 min
Response: 30260166
Conc: 12.19 ng/ml

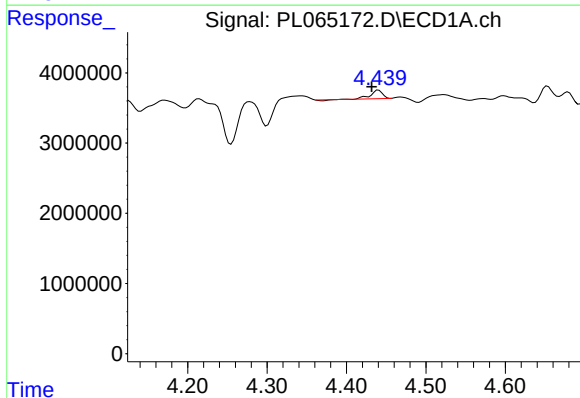


#4 Heptachlor

R.T.: 4.440 min
Delta R.T.: 0.009 min
Response: 1139459
Conc: 0.26 ng/ml

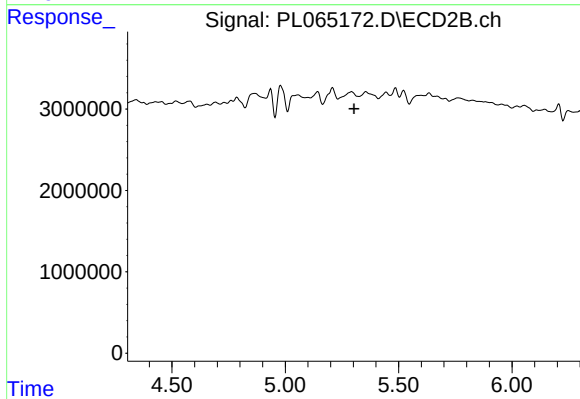

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.304 min
Response: 0
Conc: N.D.

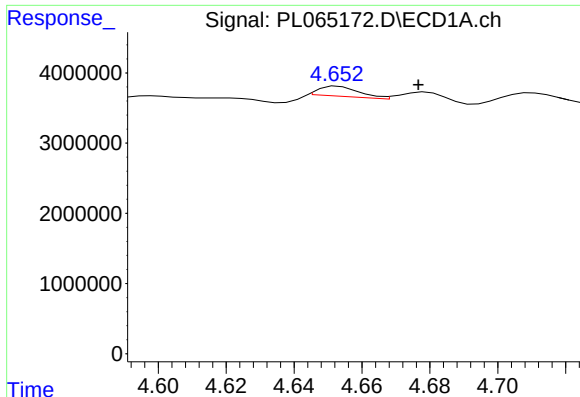

#5 Aldrin


R.T.: 4.653 min
Delta R.T.: -0.023 min
Response: 1147555
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

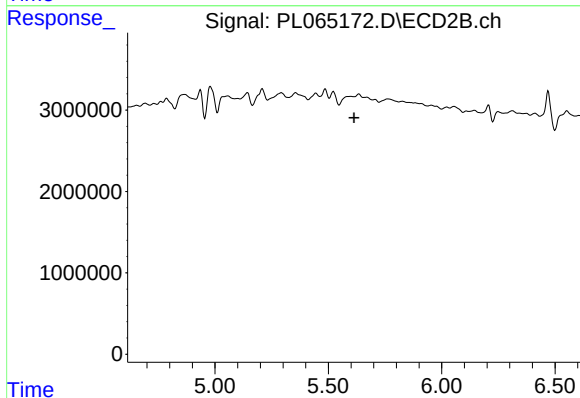


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.614 min
Response: 0
Conc: N.D.

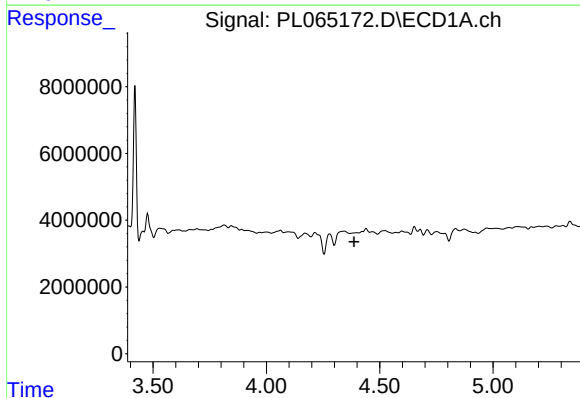


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.386 min
Response: 0
Conc: N.D.

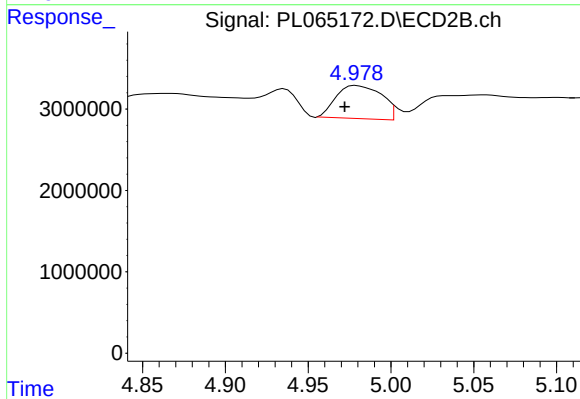

#6 beta-BHC


R.T.: 4.979 min
Delta R.T.: 0.007 min
Response: 7667378
Conc: 5.01 ng/ml

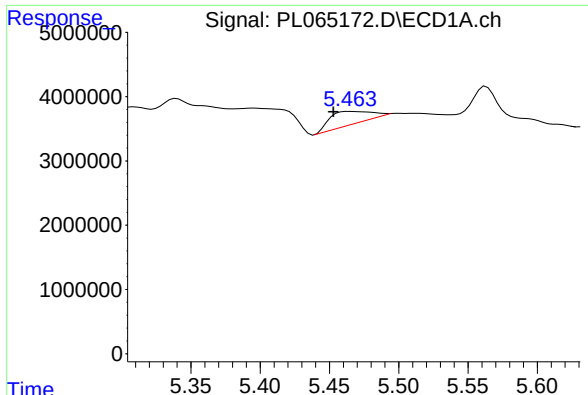

#9 Endosulfan I


R.T.: 5.465 min
Delta R.T.: 0.012 min
Response: 4125679
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

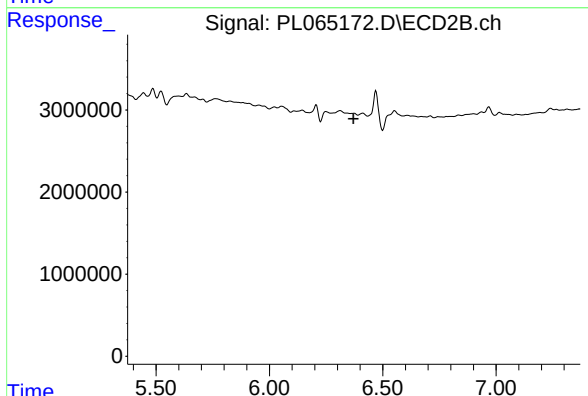


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.371 min
Response: 0
Conc: N.D.

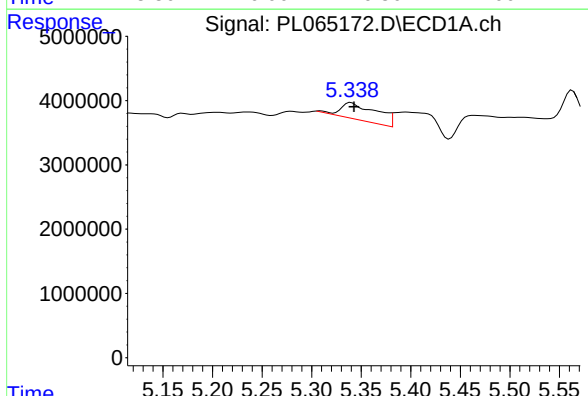


#10 gamma-Chlordane

R.T.: 5.340 min
Delta R.T.: -0.003 min
Response: 6700992
Conc: 1.71 ng/ml

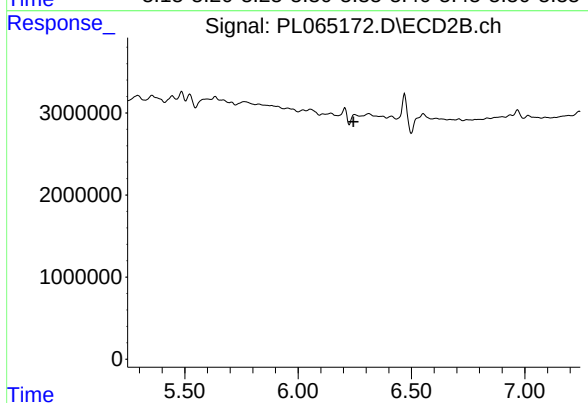

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

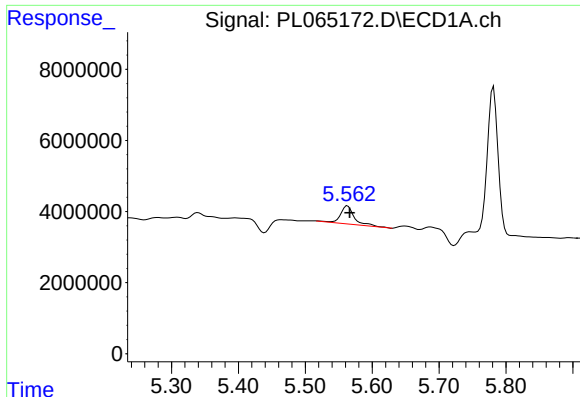

#12 4,4'-DDE


R.T.: 5.563 min
Delta R.T.: -0.003 min
Response: 7406097
Conc: 2.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

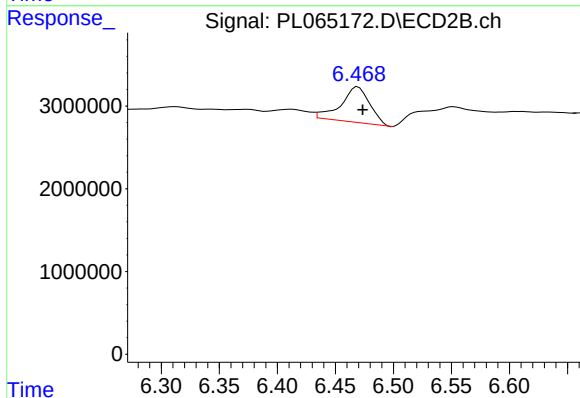


#12 4,4'-DDE

R.T.: 6.469 min
Delta R.T.: -0.004 min
Response: 7436748
Conc: 2.97 ng/ml

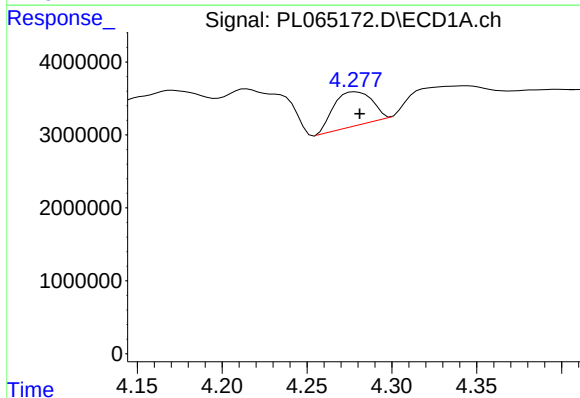


#23 Chlordane-1

R.T.: 4.279 min
Delta R.T.: -0.002 min
Response: 7301502
Conc: 57.28 ng/ml

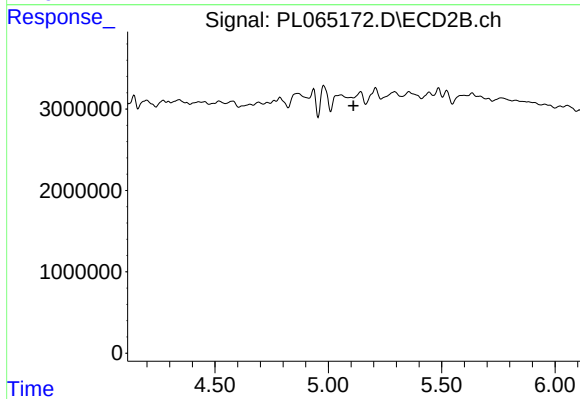

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.112 min
Response: 0
Conc: N.D.

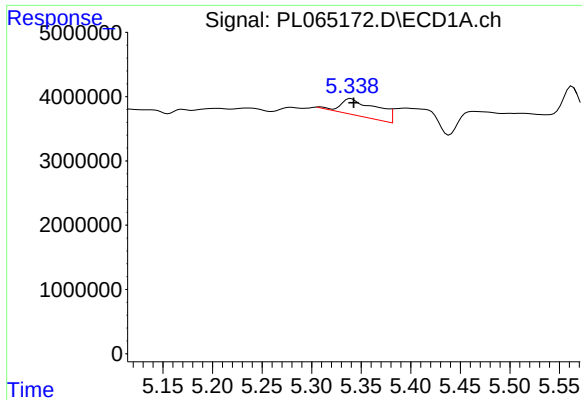

#25 Chlordane-3


R.T.: 5.340 min
Delta R.T.: -0.003 min
Response: 6700992
Conc: 16.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

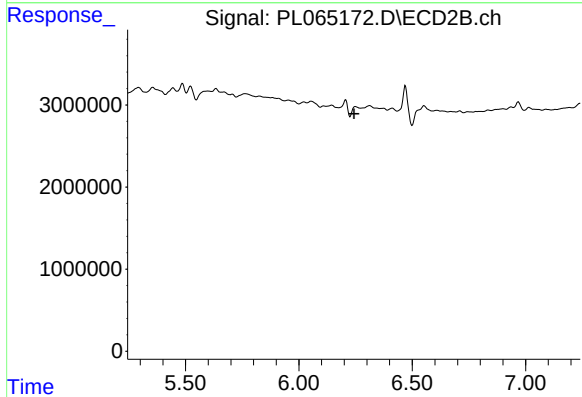


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.244 min
Response: 0
Conc: N.D.

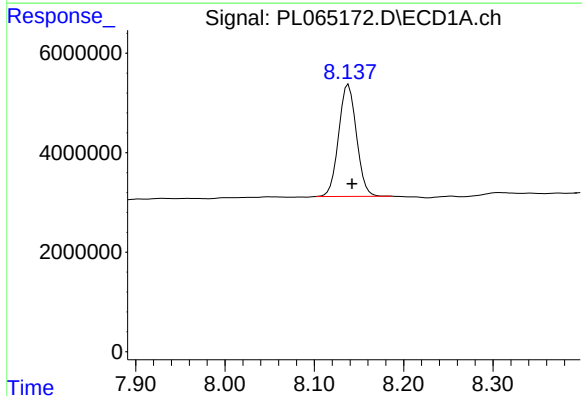

#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: -0.004 min
Response: 31187934
Conc: 11.24 ng/ml

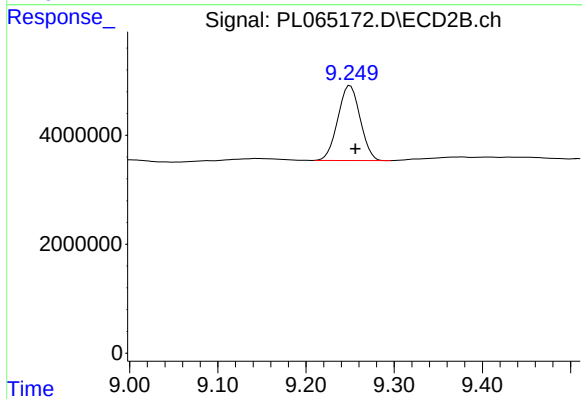

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 24200985
Conc: 11.02 ng/ml