

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
 Data File : PL065174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 14:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:20:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	4.096	49025541	42266568	16.673	17.021
28)	SA Decachlor...	8.136	9.248	62443327	52986527	22.501	24.123
Target Compounds							
6)	B beta-BHC	4.390	4.968	-1348720	3954857	N.D.	2.587
12)	B 4,4'-DDE	0.000	6.482	0	21541295	N.D.	8.617 #
13)	MA Dieldrin	5.690	0.000	19596594	0	5.298	N.D. #
14)	MA Endrin	5.970f	0.000	6472964	0	1.886	N.D. #
23)	Chlordane-1	0.000	5.137f	0	9277790	N.D.	88.897 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
Data File : PL065174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 14:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:20:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

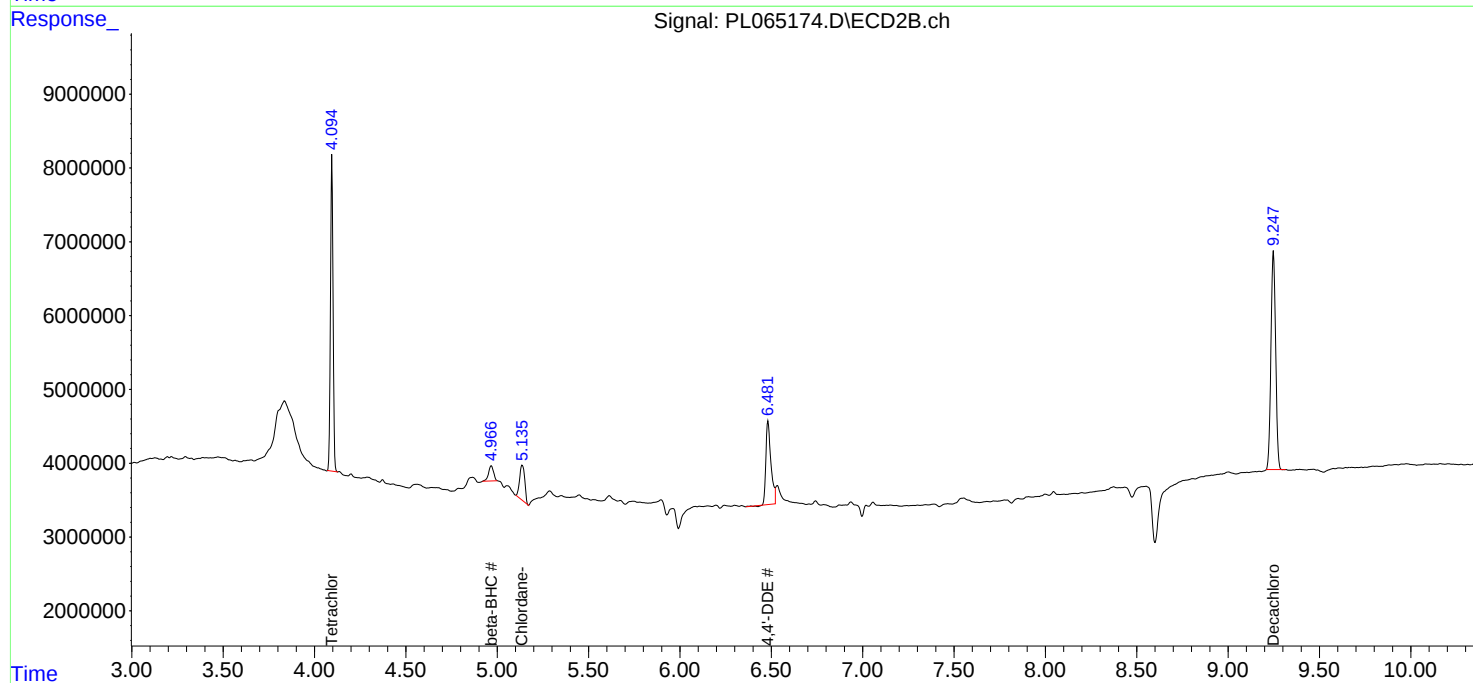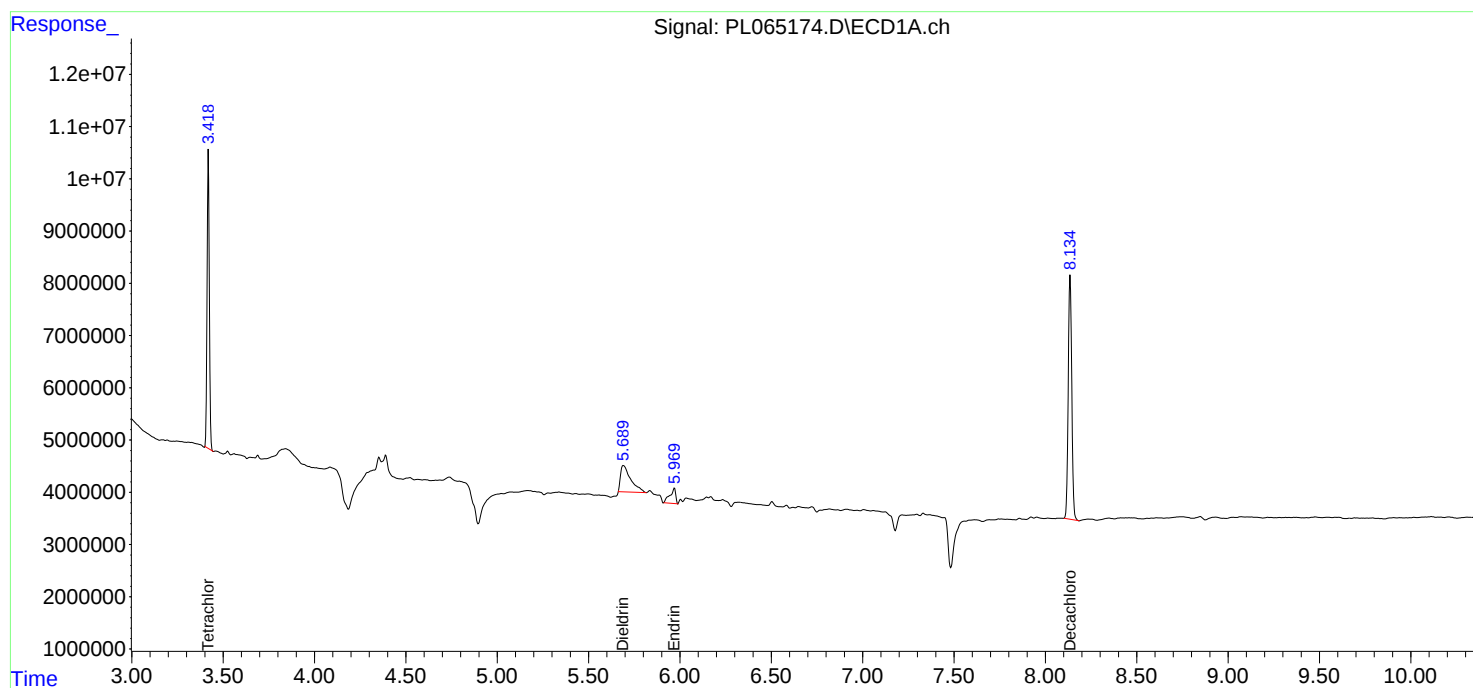


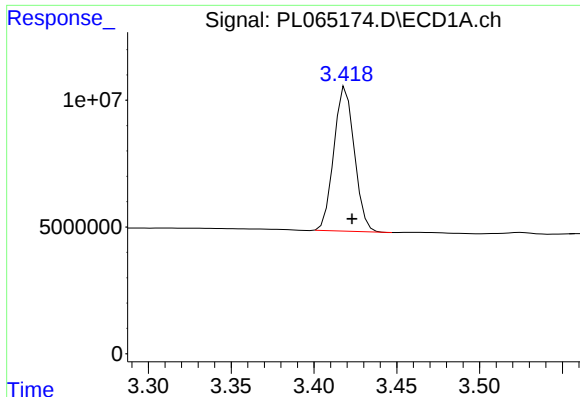

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: -0.004 min
Response: 49025541
Conc: 16.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

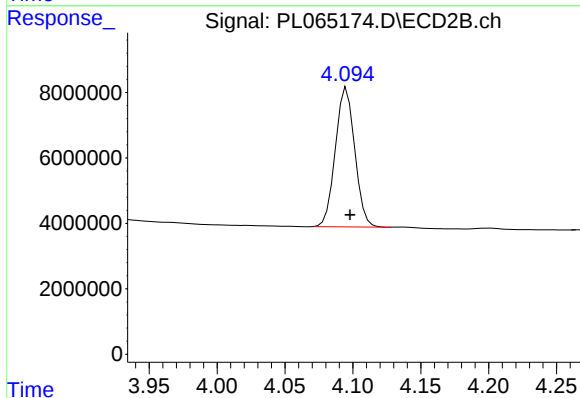


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.002 min
Response: 42266568
Conc: 17.02 ng/ml

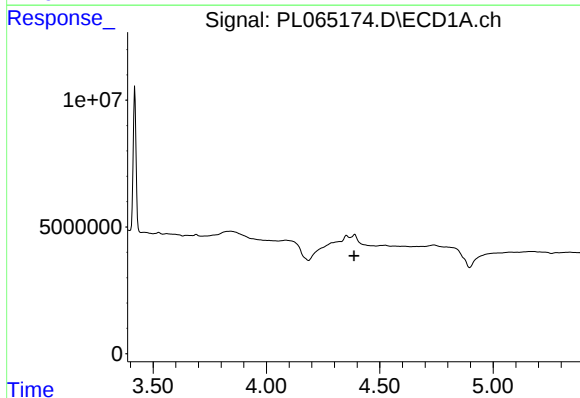


#6 beta-BHC

R.T.: 4.390 min
Delta R.T.: 0.003 min
Response: -1348720
Conc: N.D.

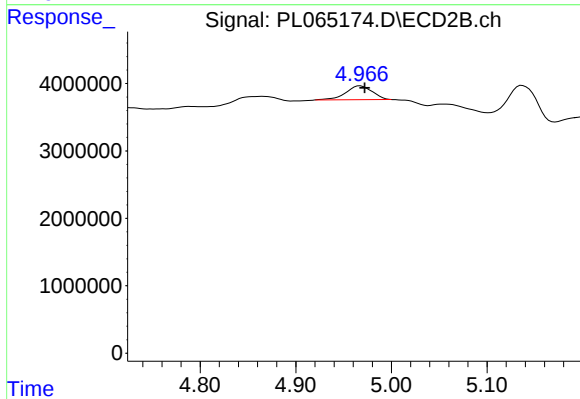

#6 beta-BHC


R.T.: 4.968 min
Delta R.T.: -0.004 min
Response: 3954857
Conc: 2.59 ng/ml

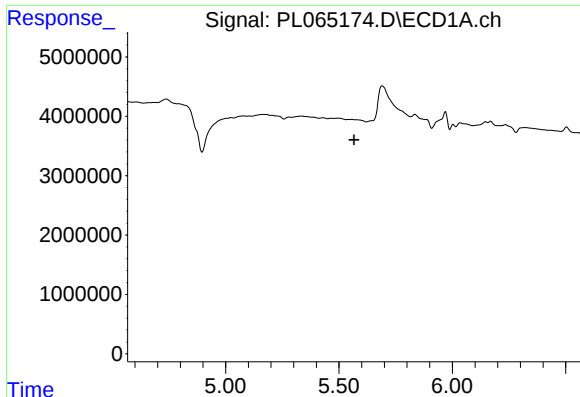

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

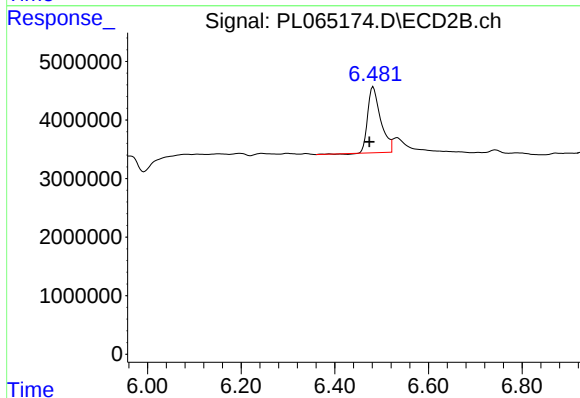


#12 4,4'-DDE

R.T.: 6.482 min
Delta R.T.: 0.008 min
Response: 21541295
Conc: 8.62 ng/ml

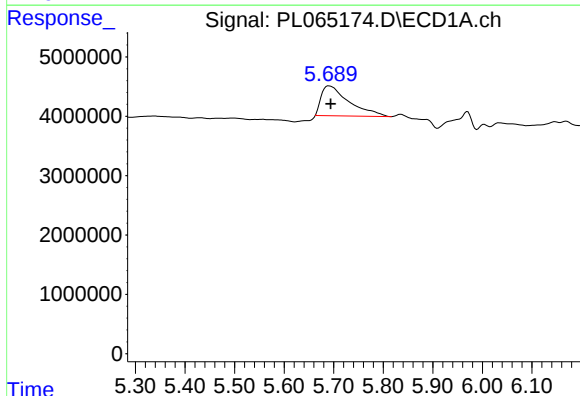


#13 Dieldrin

R.T.: 5.690 min
Delta R.T.: -0.004 min
Response: 19596594
Conc: 5.30 ng/ml

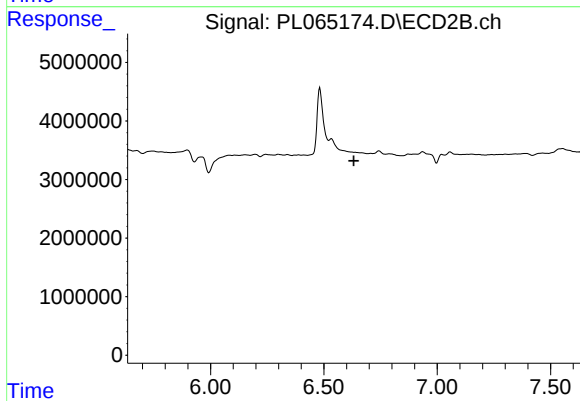

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.632 min
Response: 0
Conc: N.D.

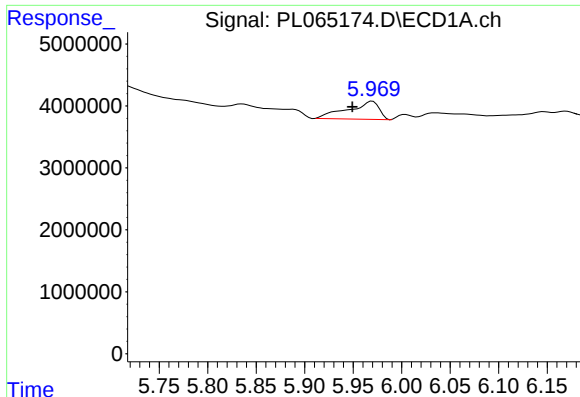

#14 Endrin


R.T.: 5.970 min
Delta R.T.: 0.021 min
Response: 6472964
Conc: 1.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

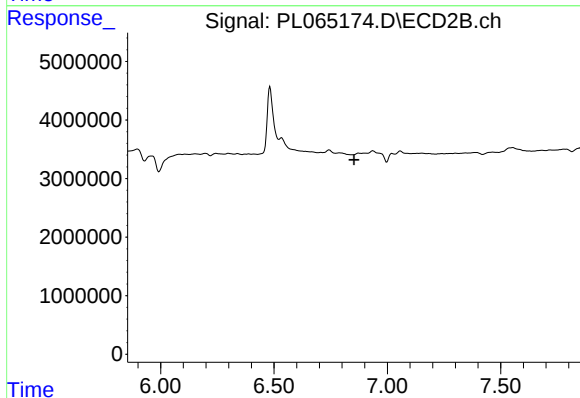


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

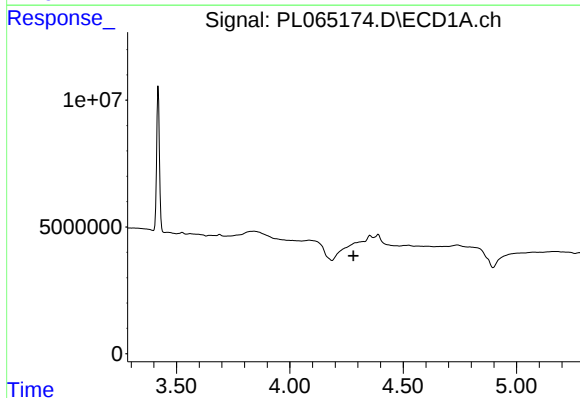


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.281 min
Response: 0
Conc: N.D.

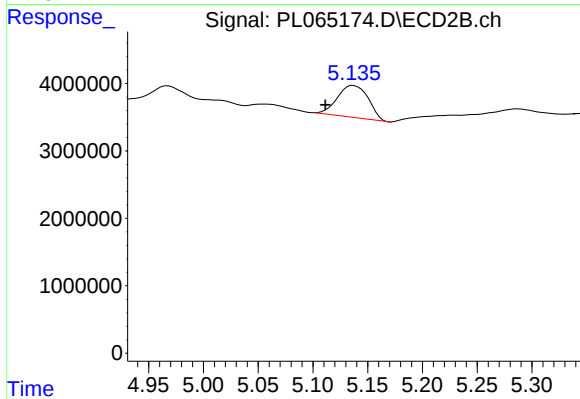

#23 Chlordane-1


R.T.: 5.137 min
Delta R.T.: 0.025 min
Response: 9277790
Conc: 88.90 ng/ml

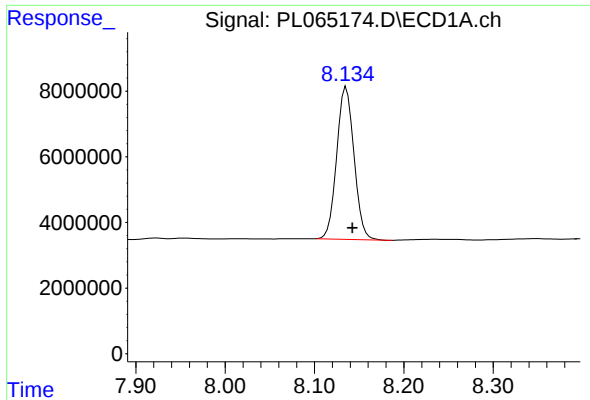

#28 Decachlorobiphenyl

R.T.: 8.136 min
Delta R.T.: -0.007 min
Response: 62443327
Conc: 22.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

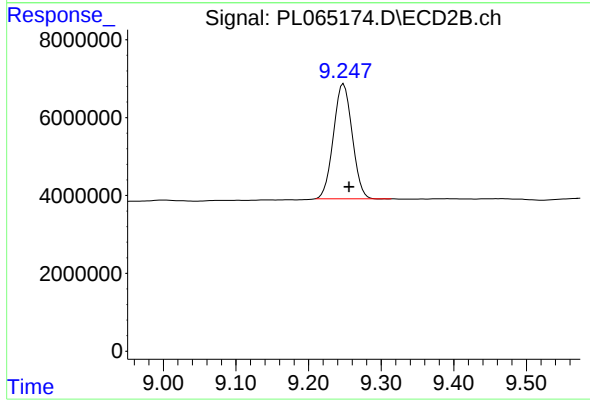

#28 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: -0.008 min
Response: 52986527
Conc: 24.12 ng/ml