

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
 Data File : PL065178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 16:58
 Operator : AR\AJ
 Sample : M1599-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:21:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.096	5192357	4246623	1.766	1.710
28)	SA Decachlor...	8.141	9.250	7232312	6065059	2.606	2.761
Target Compounds							
6)	B beta-BHC	0.000	4.974	0	4321448	N.D.	2.826 #
14)	MA Endrin	5.954	0.000	1665782	0	0.485	N.D. #
23)	Chlordane-1	4.286	0.000	4106107	0	32.215	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
Data File : PL065178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 16:58
Operator : AR\AJ
Sample : M1599-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:21:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

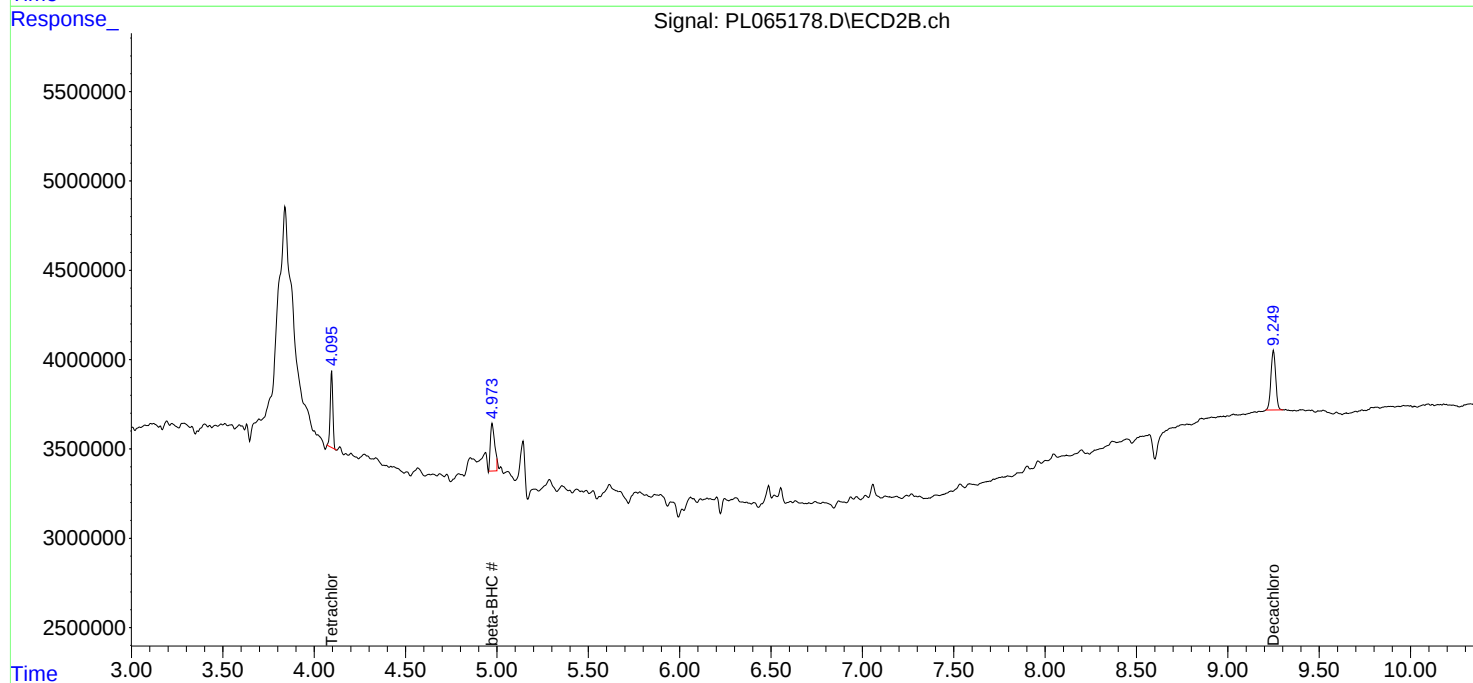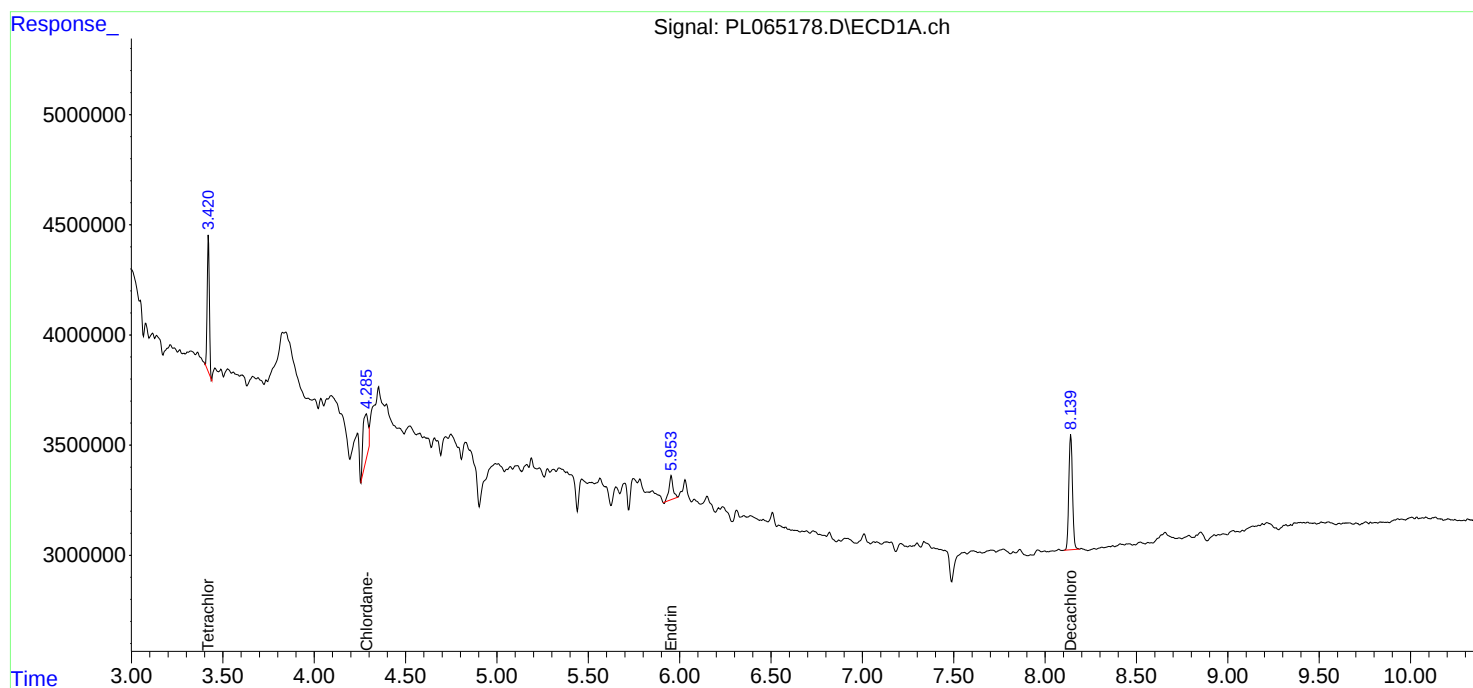


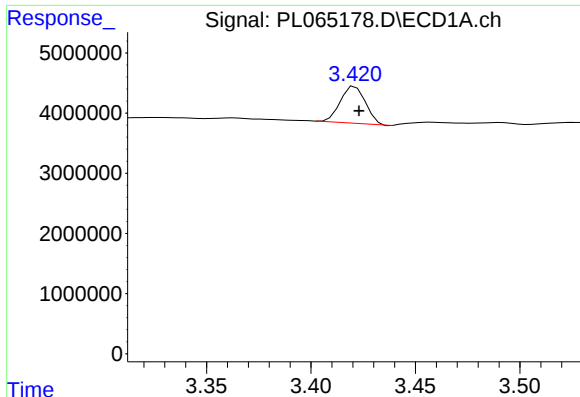

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: -0.002 min
Response: 5192357
Conc: 1.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

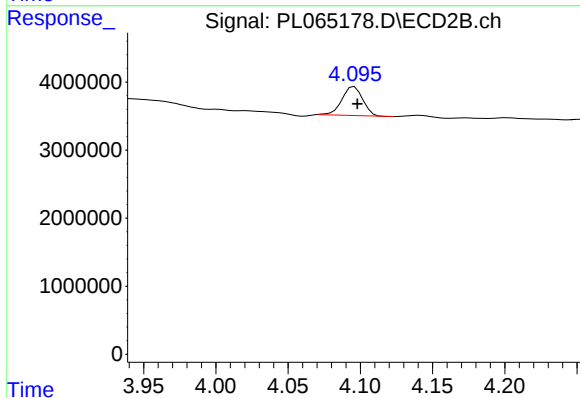


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.002 min
Response: 4246623
Conc: 1.71 ng/ml

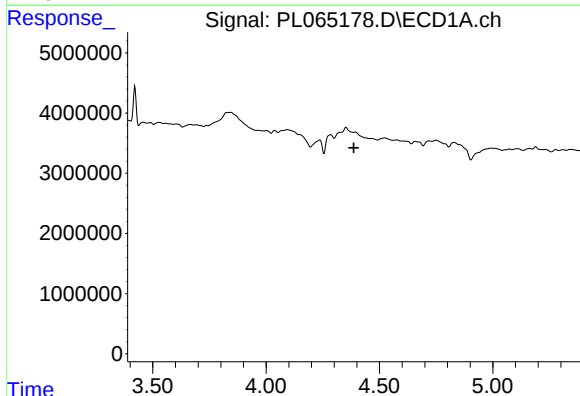


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.386 min
Response: 0
Conc: N.D.

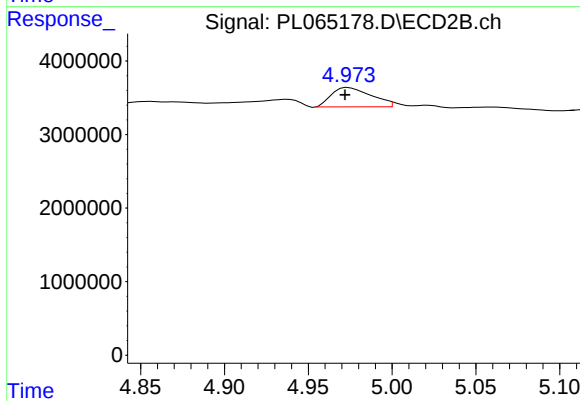

#6 beta-BHC


R.T.: 4.974 min
Delta R.T.: 0.002 min
Response: 4321448
Conc: 2.83 ng/ml

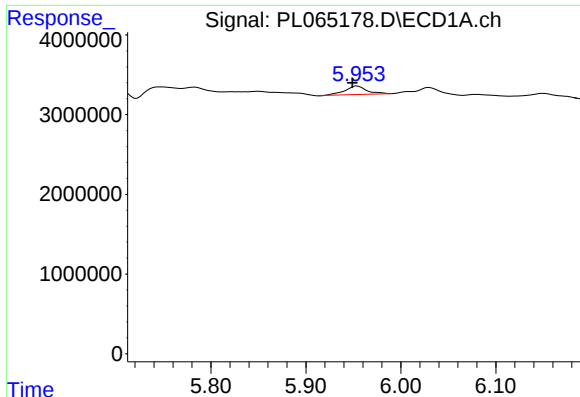

#14 Endrin


R.T.: 5.954 min
Delta R.T.: 0.005 min
Response: 1665782
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

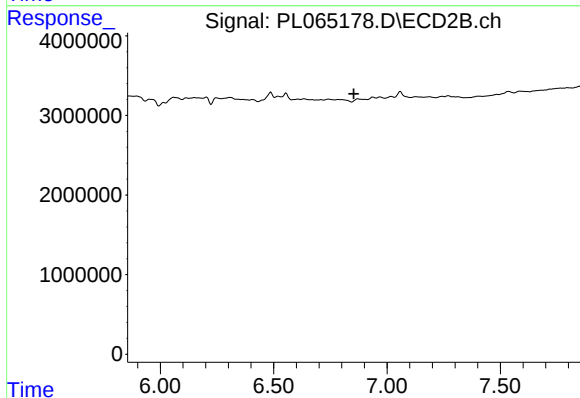


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

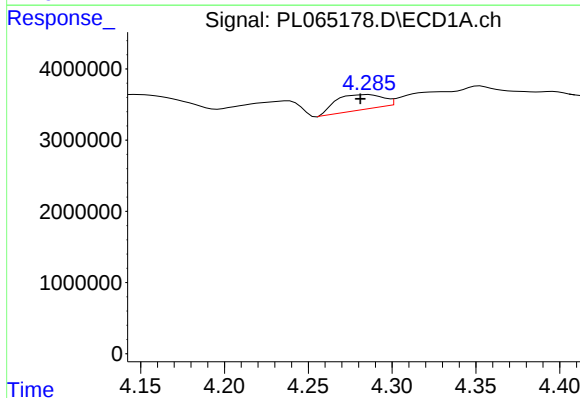


#23 Chlordane-1

R.T.: 4.286 min
Delta R.T.: 0.005 min
Response: 4106107
Conc: 32.21 ng/ml

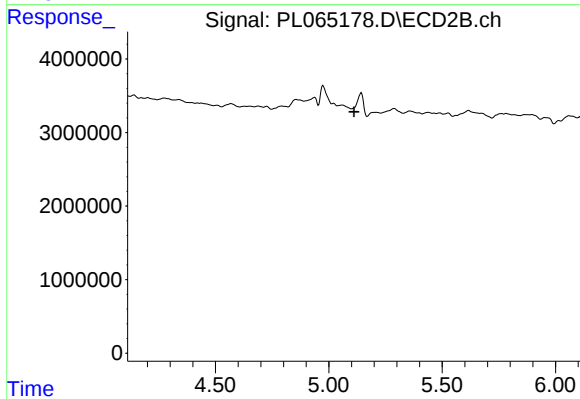

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

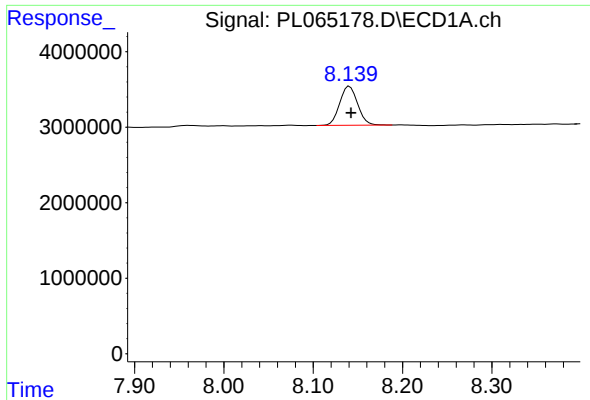

#28 Decachlorobiphenyl

R.T.: 8.141 min
Delta R.T.: -0.002 min
Response: 7232312
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

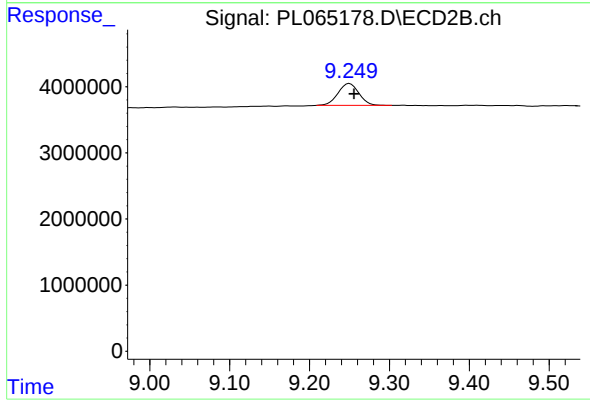

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 6065059
Conc: 2.76 ng/ml