

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
 Data File : PL065181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 17:41
 Operator : AR\AJ
 Sample : M1601-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:22:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.096	37477914	31263653	12.746	12.590
28)	SA Decachlor...	8.138	9.250	41250894	36651559	14.865	16.686
Target Compounds							
4)	MA Heptachlor	4.441	0.000	1352529	0	0.307	N.D. #
6)	B beta-BHC	0.000	4.979	0	9106694	N.D.	5.956 #
9)	A Endosulfan I	5.464	0.000	7332509	0	2.050	N.D. #
10)	B gamma-Chl...	5.340	0.000	6221502	0	1.589	N.D. #
12)	B 4,4'-DDE	5.563	6.470	15013709	7658484	4.177	3.063 #
13)	MA Dieldrin	5.690	0.000	5210730	0	1.409	N.D. #
17)	MA 4,4'-DDT	6.310	0.000	1142586	0	0.410	N.D. #
23)	Chlordane-1	4.279	0.000	7393885	0	58.010	N.D. #
25)	Chlordane-3	5.340	0.000	6221502	0	15.595	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
Data File : PL065181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 17:41
Operator : AR\AJ
Sample : M1601-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:22:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

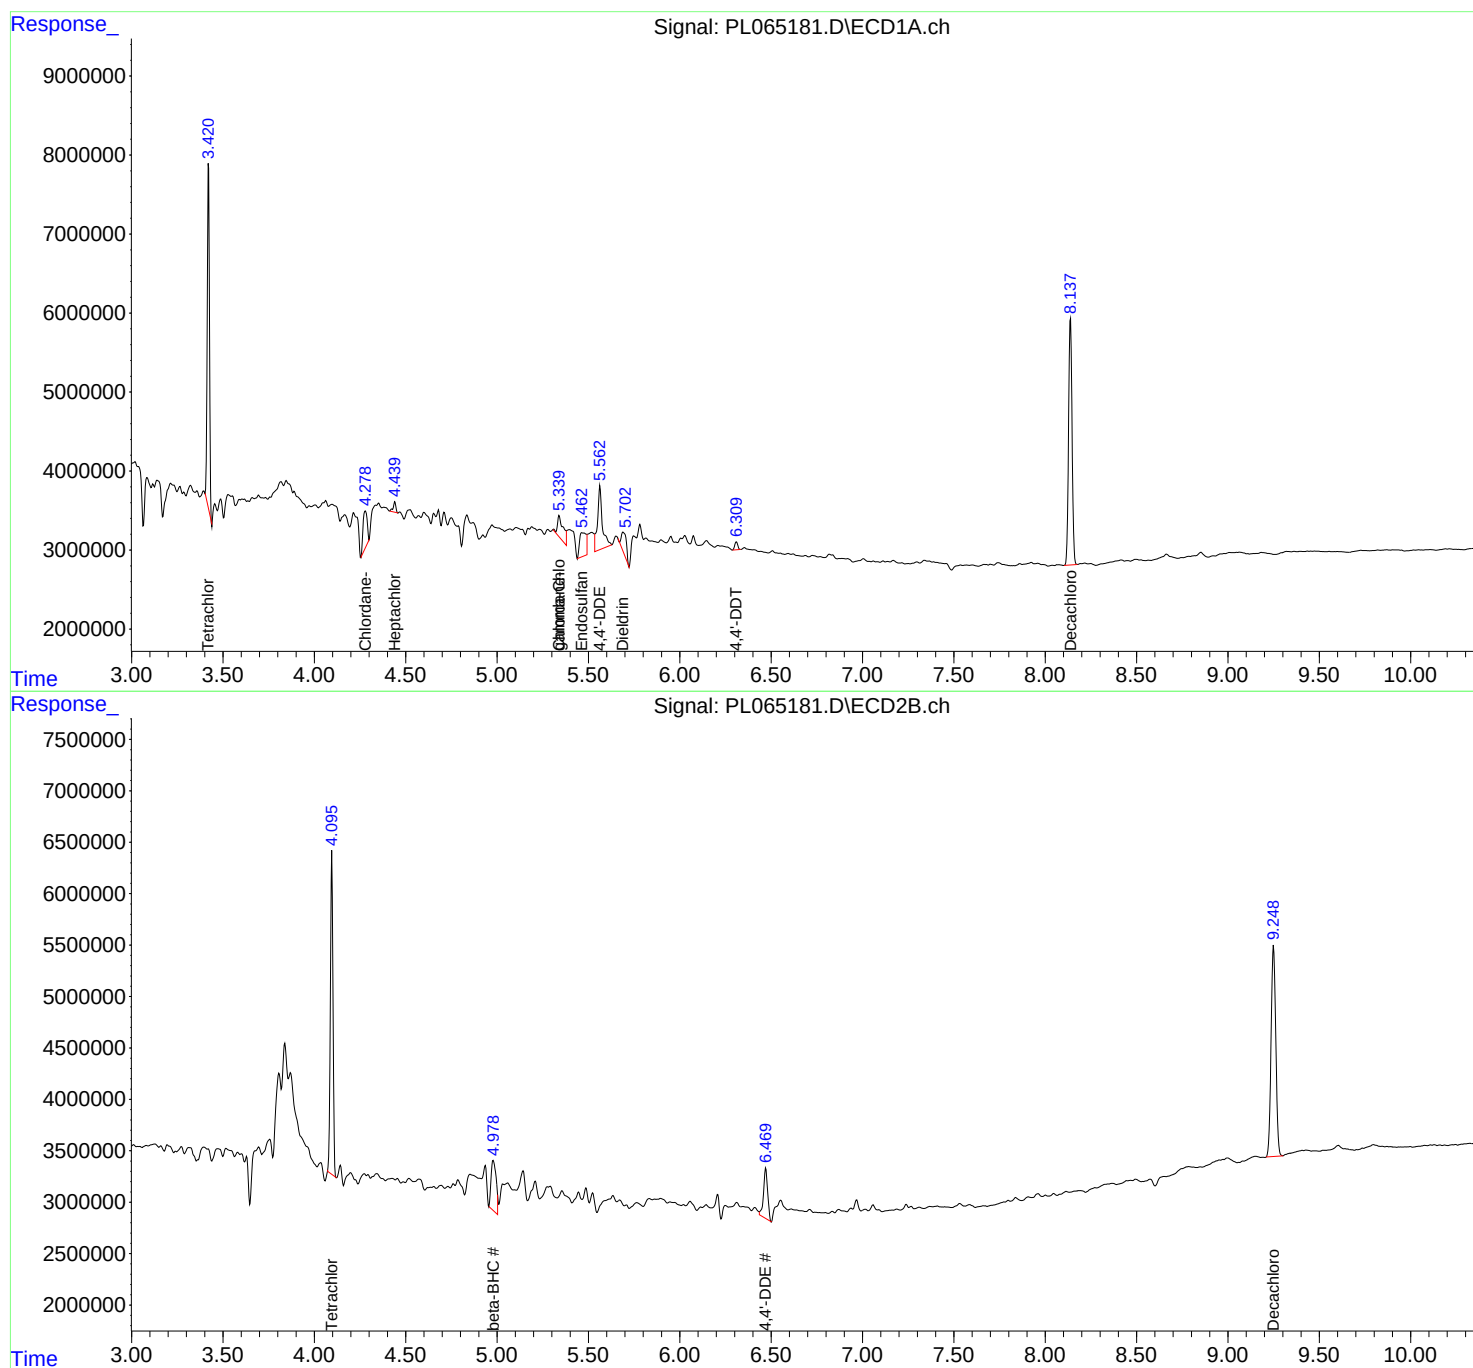


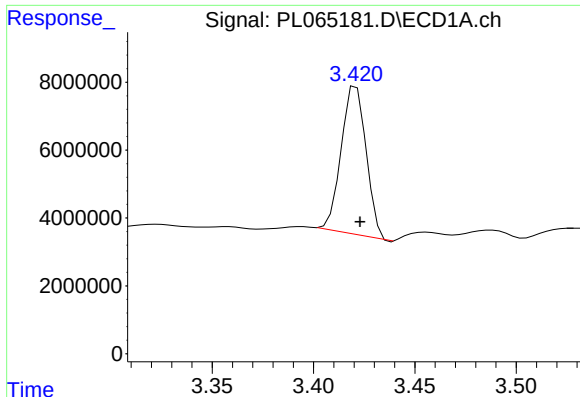

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: -0.002 min
Response: 37477914
Conc: 12.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

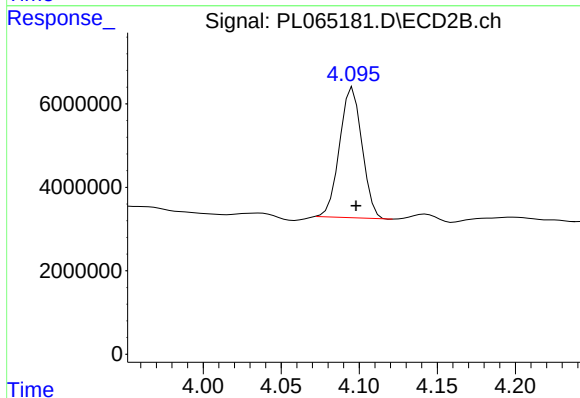


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.002 min
Response: 31263653
Conc: 12.59 ng/ml

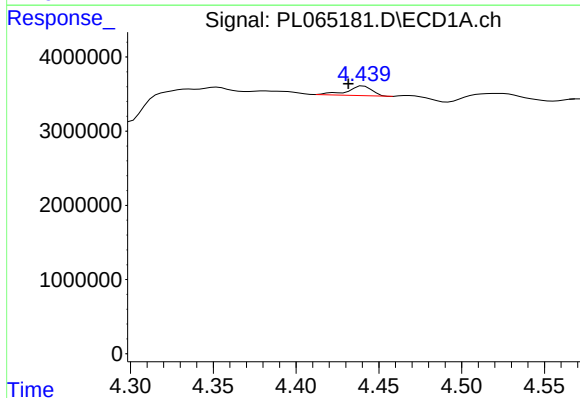


#4 Heptachlor

R.T.: 4.441 min
Delta R.T.: 0.009 min
Response: 1352529
Conc: 0.31 ng/ml

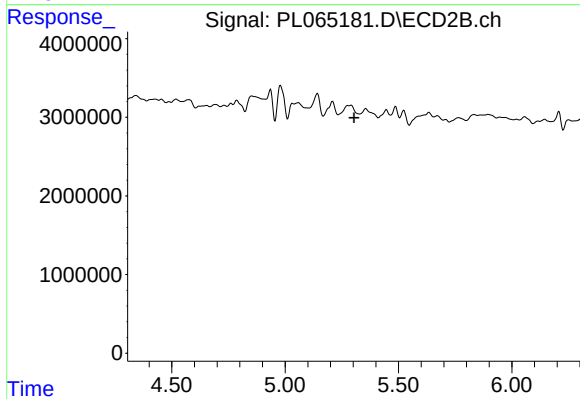

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.304 min
Response: 0
Conc: N.D.

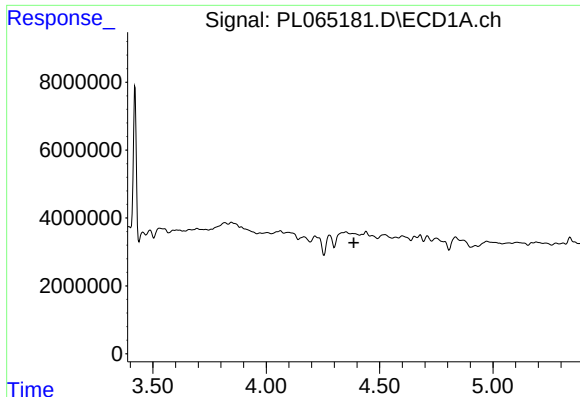

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

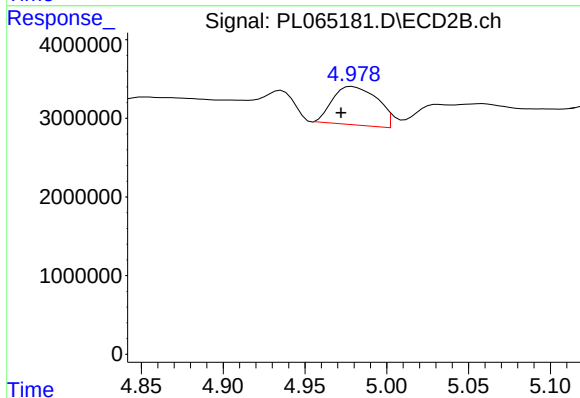


#6 beta-BHC

R.T.: 4.979 min
Delta R.T.: 0.007 min
Response: 9106694
Conc: 5.96 ng/ml

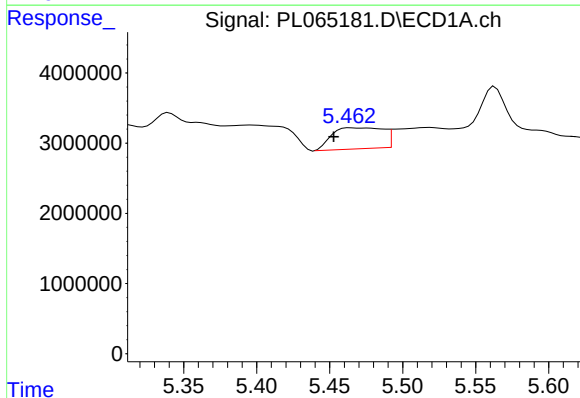


#9 Endosulfan I

R.T.: 5.464 min
Delta R.T.: 0.012 min
Response: 7332509
Conc: 2.05 ng/ml

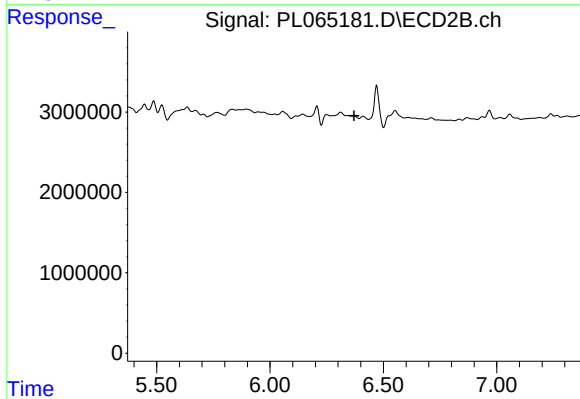

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.371 min
Response: 0
Conc: N.D.

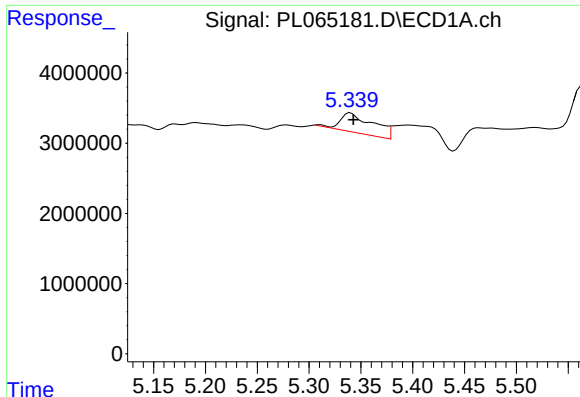

#10 gamma-Chlordane


R.T.: 5.340 min
Delta R.T.: -0.003 min
Response: 6221502
Conc: 1.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

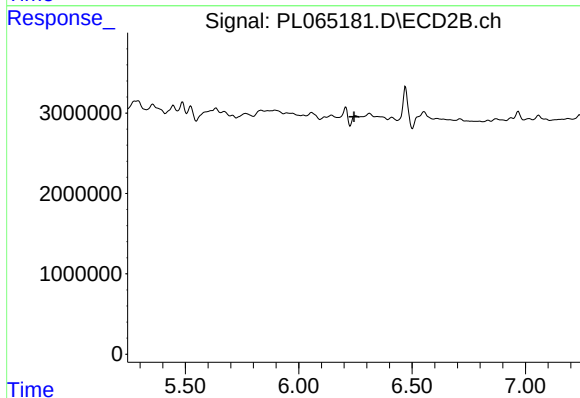


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

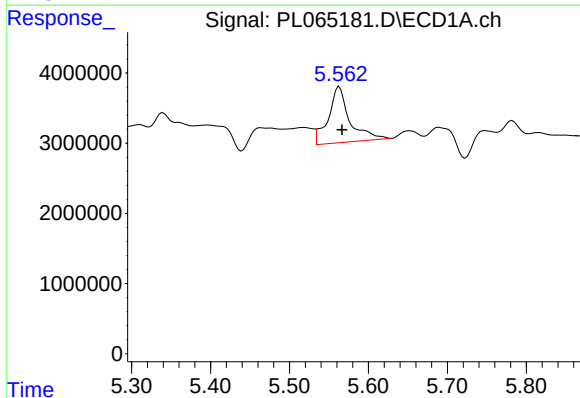


#12 4,4'-DDE

R.T.: 5.563 min
Delta R.T.: -0.003 min
Response: 15013709
Conc: 4.18 ng/ml

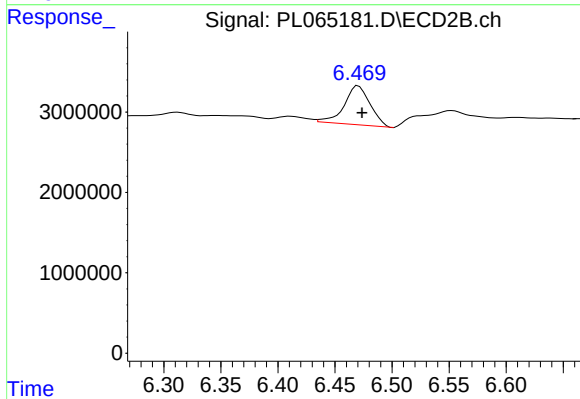

#12 4,4'-DDE


R.T.: 6.470 min
Delta R.T.: -0.003 min
Response: 7658484
Conc: 3.06 ng/ml

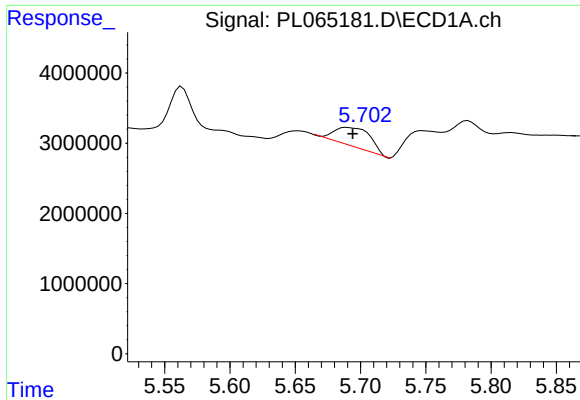

#13 Dieldrin


R.T.: 5.690 min
Delta R.T.: -0.004 min
Response: 5210730
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

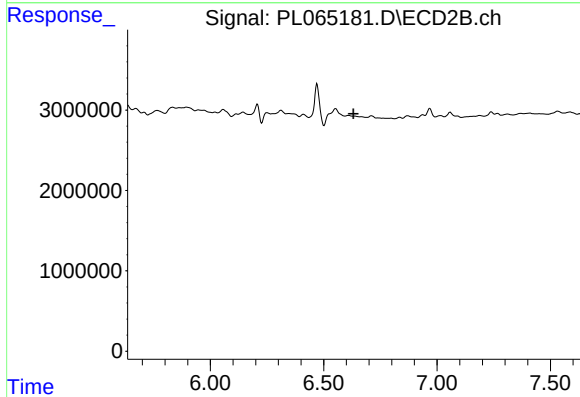


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

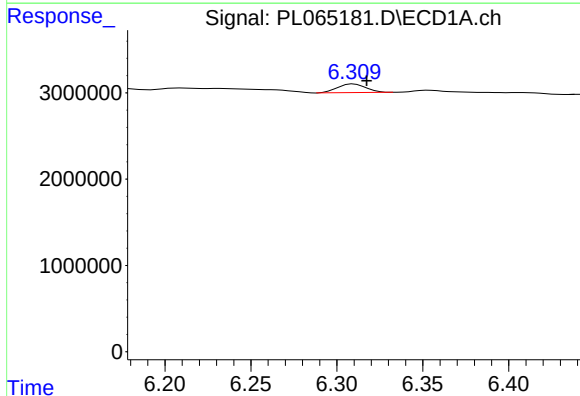


#17 4,4'-DDT

R.T.: 6.310 min
Delta R.T.: -0.007 min
Response: 1142586
Conc: 0.41 ng/ml

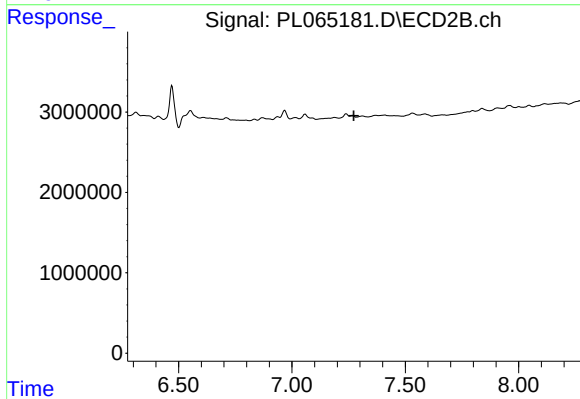

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.273 min
Response: 0
Conc: N.D.

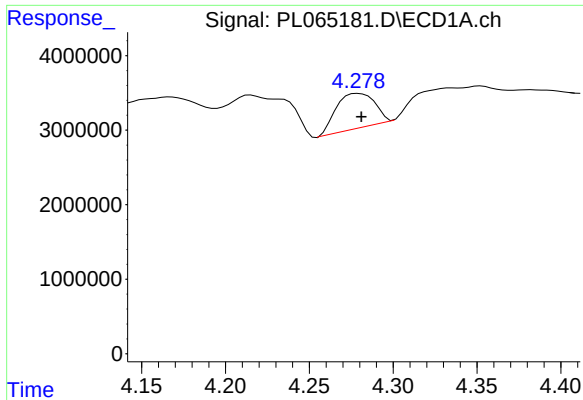

#23 Chlordane-1


R.T.: 4.279 min
Delta R.T.: -0.002 min
Response: 7393885
Conc: 58.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

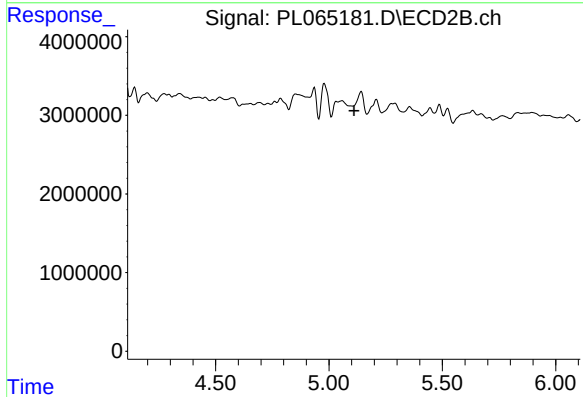


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

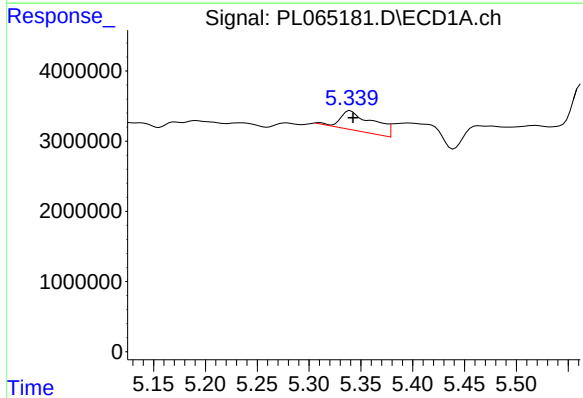


#25 Chlordane-3

R.T.: 5.340 min
Delta R.T.: -0.003 min
Response: 6221502
Conc: 15.60 ng/ml

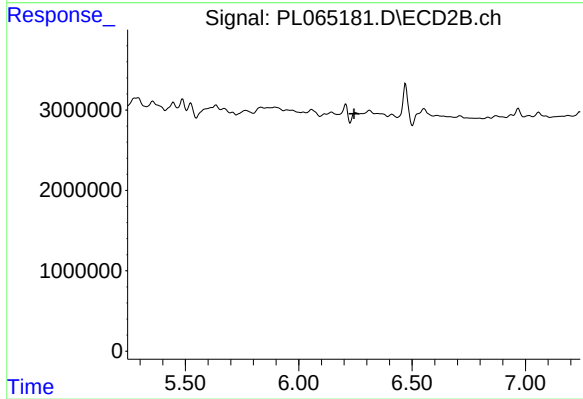

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.244 min
Response: 0
Conc: N.D.

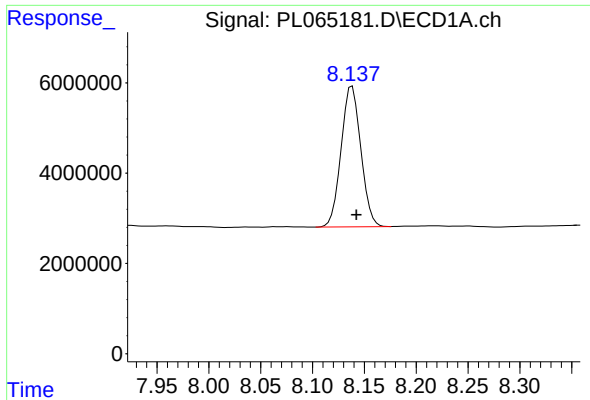

#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: -0.004 min
Response: 41250894
Conc: 14.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

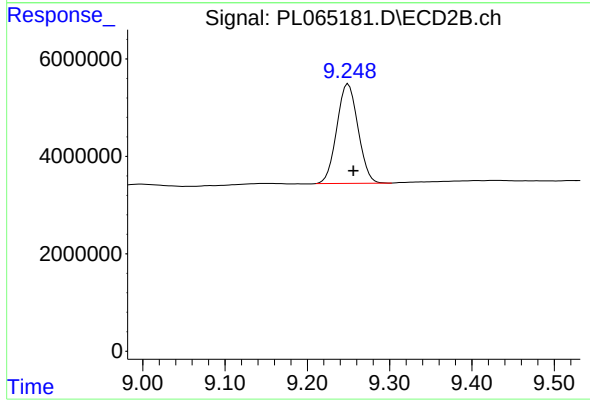

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 36651559
Conc: 16.69 ng/ml