

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
 Data File : PL065182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 17:56
 Operator : AR\AJ
 Sample : M1602-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:22:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.096	37419701	32720935	12.726	13.177
28)	SA Decachlor...	8.138	9.249	42455088	38332908	15.299	17.452
Target Compounds							
6)	B beta-BHC	0.000	4.976	0	3917914	N.D.	2.562 #
10)	B gamma-Chl...	5.362f	0.000	814073	0	0.208	N.D. #
23)	Chlordane-1	4.286	0.000	4330562	0	33.976	N.D. #
25)	Chlordane-3	5.362f	0.000	814073	0	2.041	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
Data File : PL065182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 17:56
Operator : AR\AJ
Sample : M1602-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:22:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

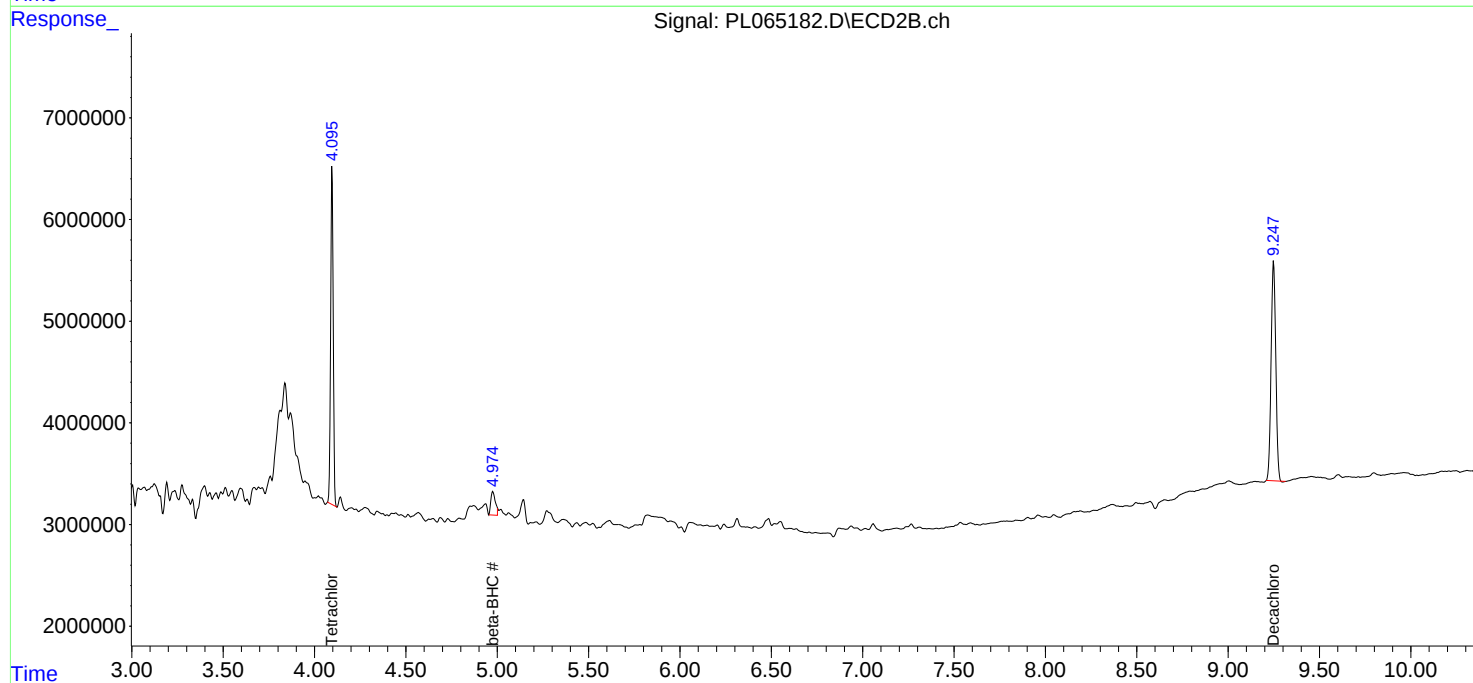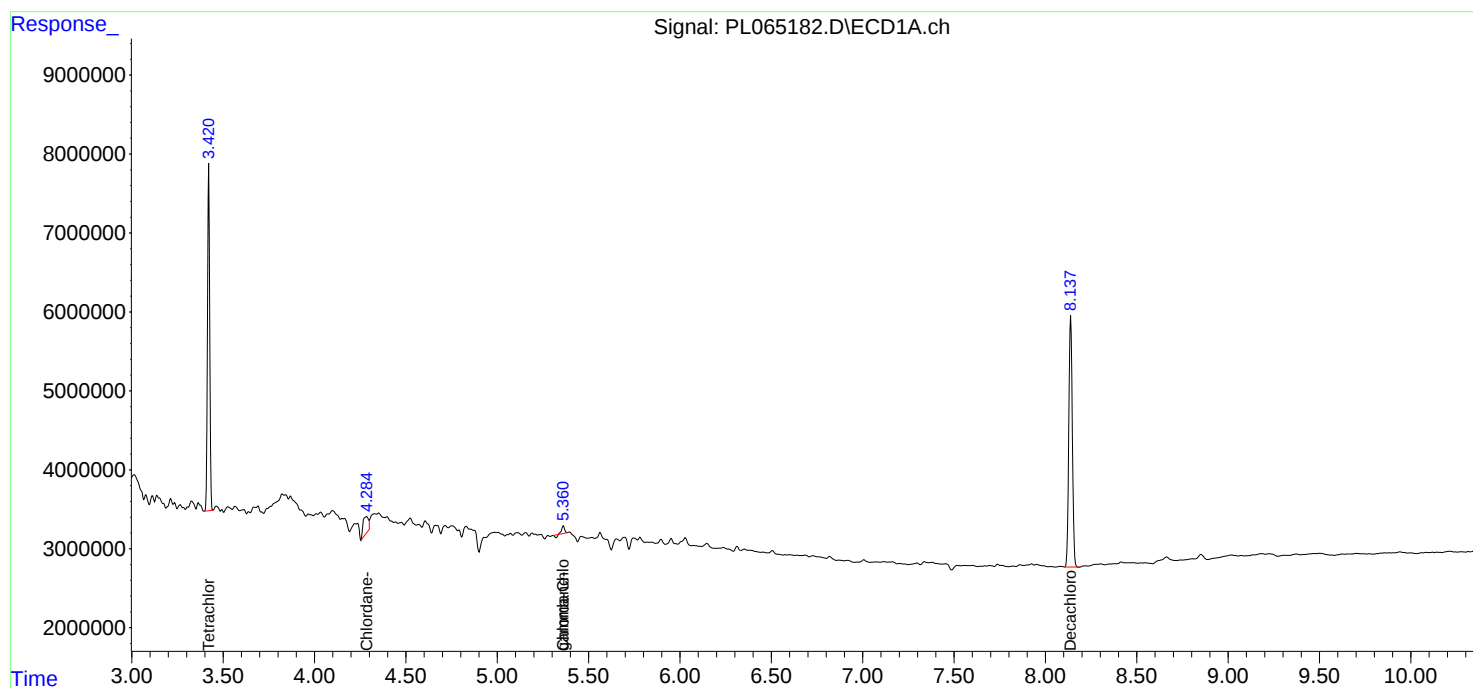


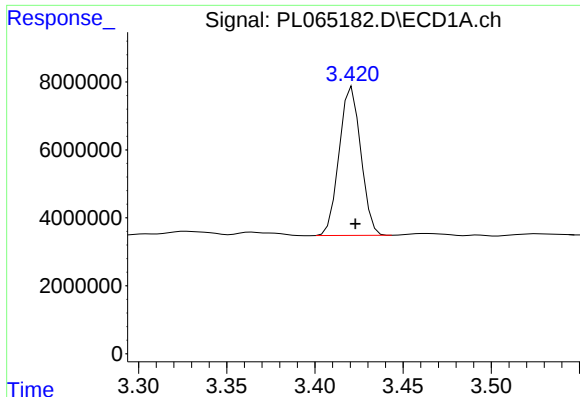

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: -0.002 min
Response: 37419701
Conc: 12.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

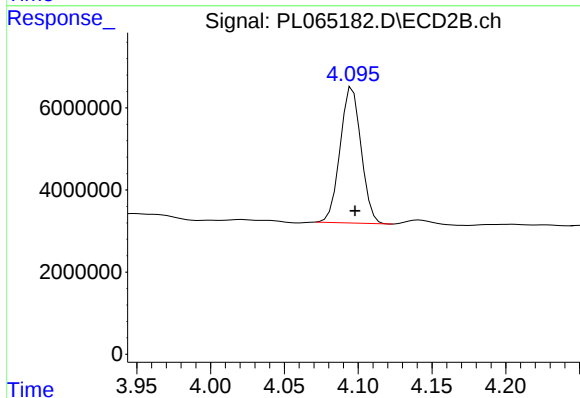


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.002 min
Response: 32720935
Conc: 13.18 ng/ml

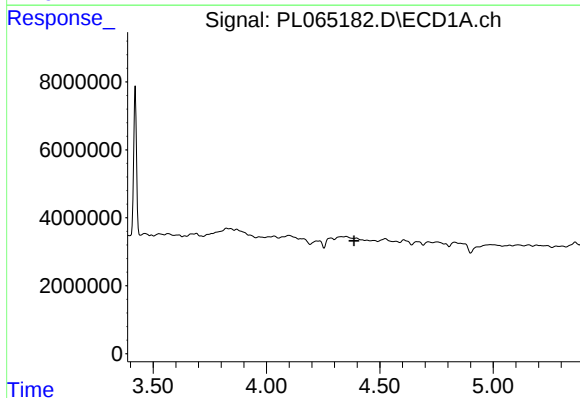


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.386 min
Response: 0
Conc: N.D.

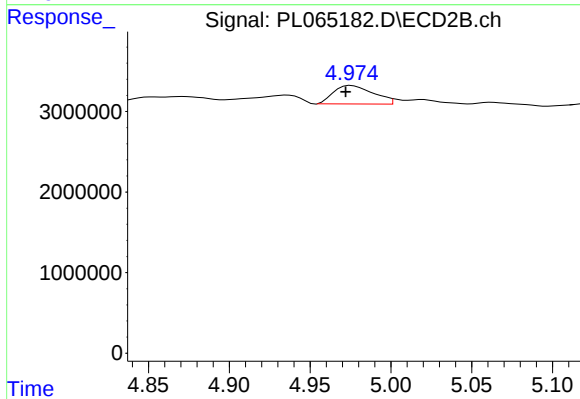

#6 beta-BHC


R.T.: 4.976 min
Delta R.T.: 0.004 min
Response: 3917914
Conc: 2.56 ng/ml

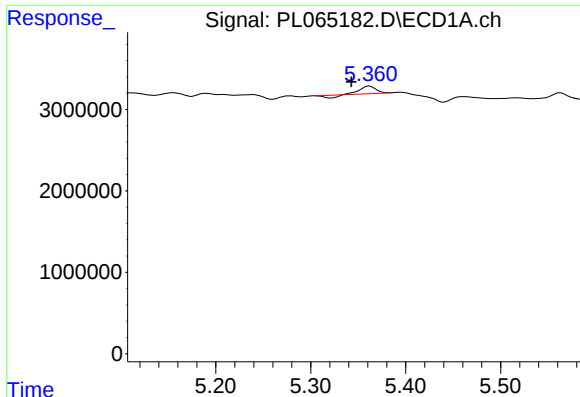

#10 gamma-Chlordane


R.T.: 5.362 min
Delta R.T.: 0.019 min
Response: 814073
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

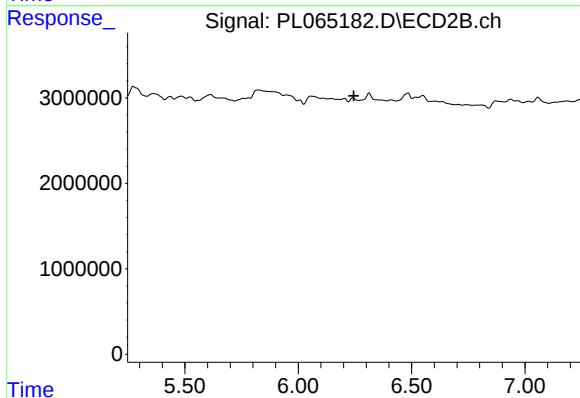


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

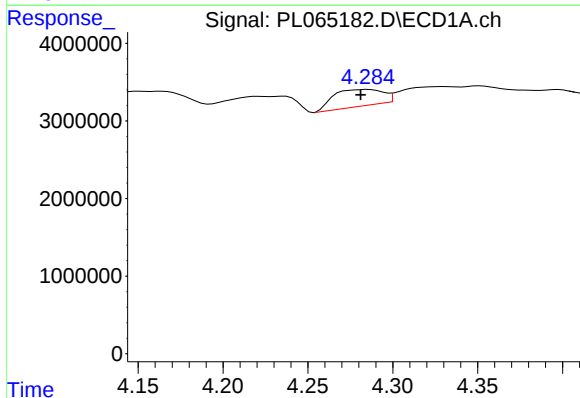


#23 Chlordane-1

R.T.: 4.286 min
Delta R.T.: 0.004 min
Response: 4330562
Conc: 33.98 ng/ml

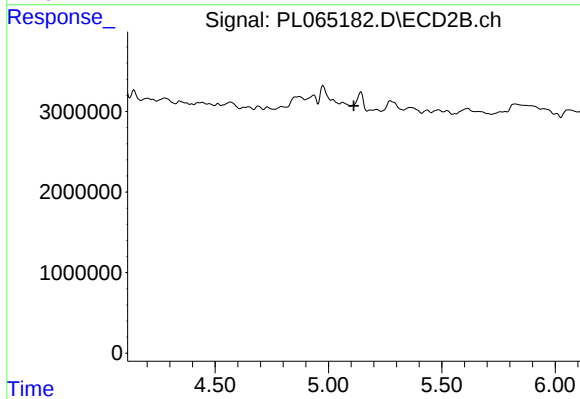

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

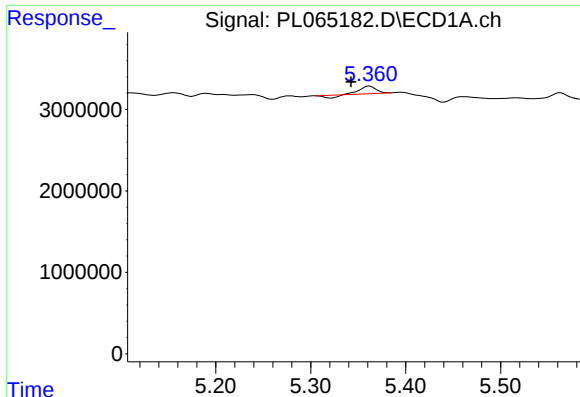

#25 Chlordane-3


R.T.: 5.362 min
Delta R.T.: 0.020 min
Response: 814073
Conc: 2.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

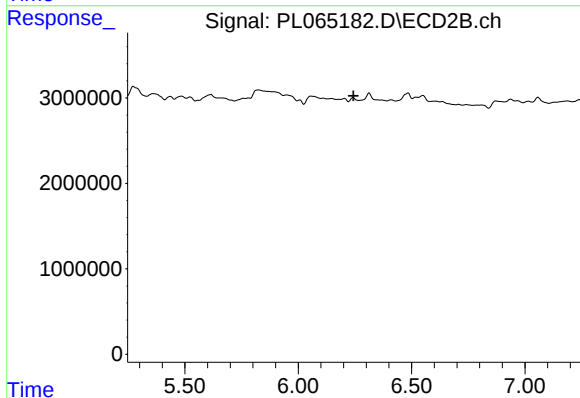


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.244 min
Response: 0
Conc: N.D.

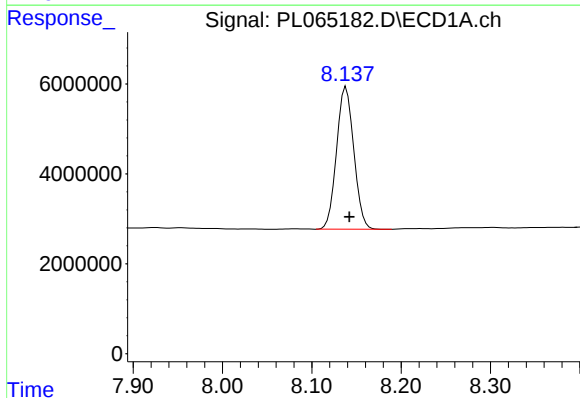

#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: -0.004 min
Response: 42455088
Conc: 15.30 ng/ml

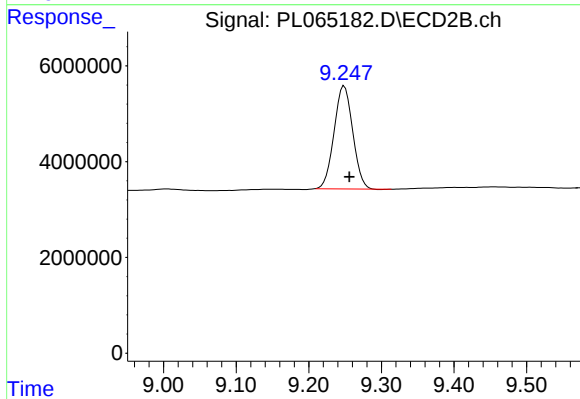

#28 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: -0.007 min
Response: 38332908
Conc: 17.45 ng/ml