

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
 Data File : PL065172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 13:38
 Operator : AR\AJ
 Sample : M1601-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BIN-3

Manual Integrations
 APPROVED

Ankita
 3/10/2021 10:14:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:20:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.096	38138799	30260166	12.970	12.186
28)	SA Decachlor...	8.138	9.250	31187934	24200985	11.238	11.018
Target Compounds							
12)	B 4,4'-DDE	5.563	6.468	7406097	3956381	2.061	1.583m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
Data File : PL065172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 13:38
Operator : AR\AJ
Sample : M1601-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BIN-3


Manual Integrations
APPROVED

Ankita
3/10/2021 10:14:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:20:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

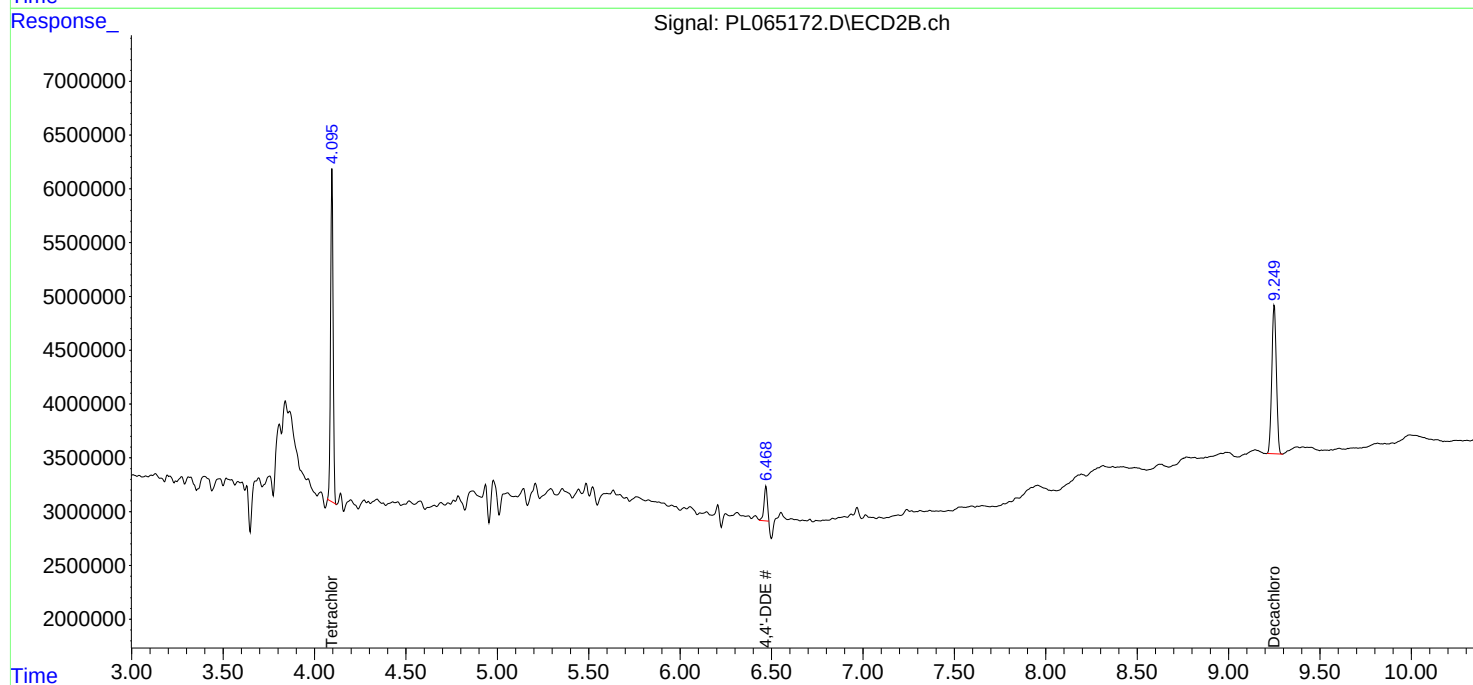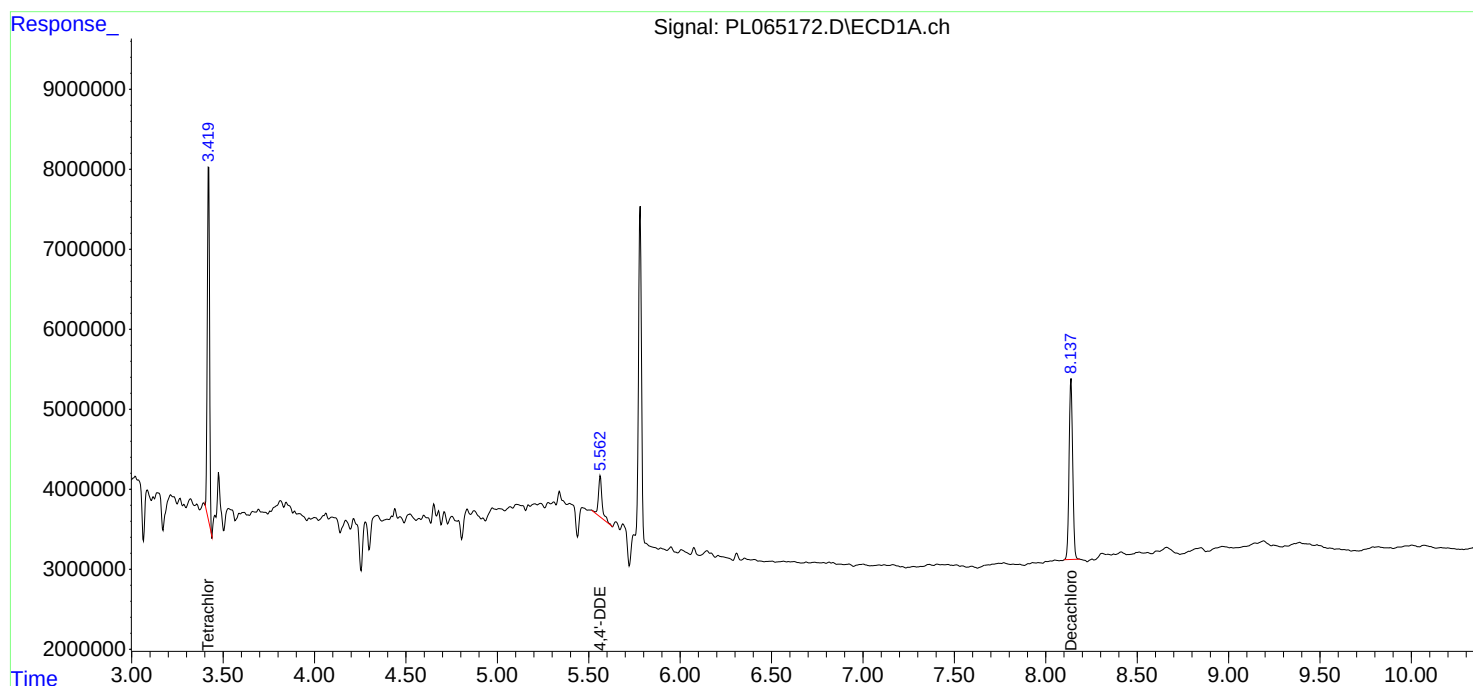

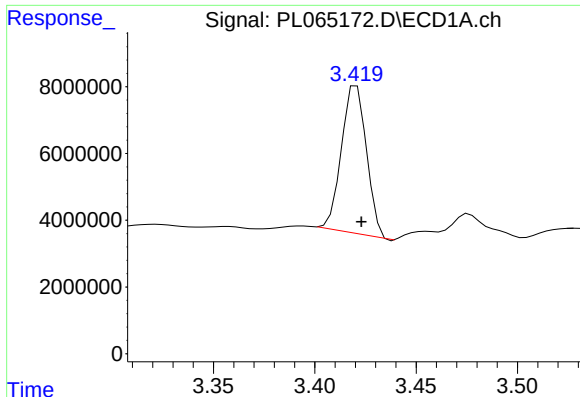


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: -0.002 min
Response: 38138799
Conc: 12.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
BIN-3


Manual Integrations
APPROVED

Ankita
3/10/2021 10:14:02 AM

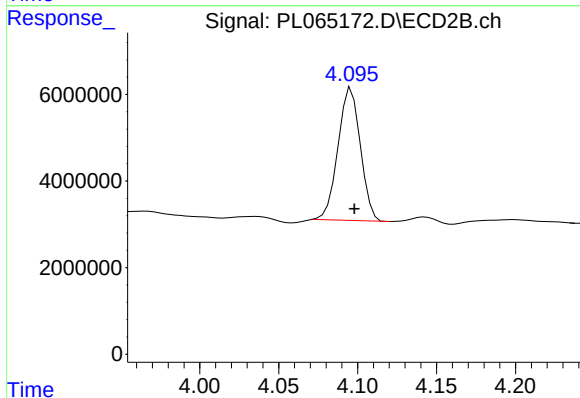


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.002 min
Response: 30260166
Conc: 12.19 ng/ml

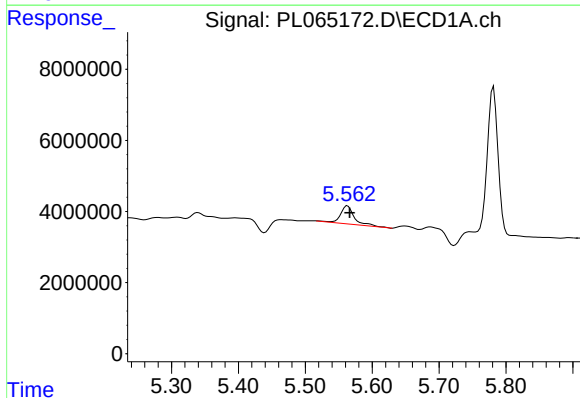


#12 4,4'-DDE

R.T.: 5.563 min
Delta R.T.: -0.003 min
Response: 7406097
Conc: 2.06 ng/ml

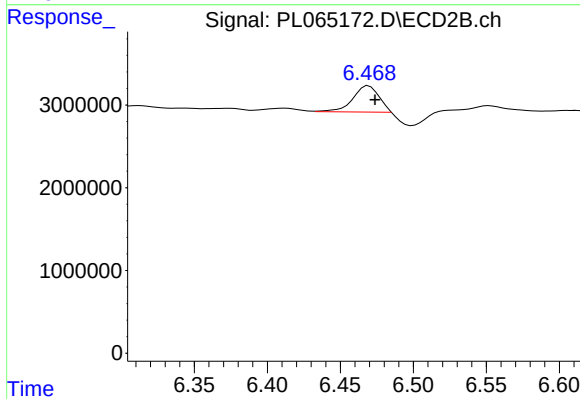

#12 4,4'-DDE

R.T.: 6.468 min
Delta R.T.: -0.006 min
Response: 3956381
Conc: 1.58 ng/ml m

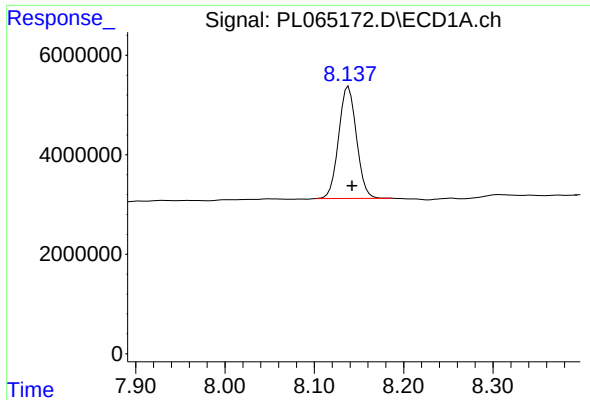


#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: -0.004 min
Response: 31187934
Conc: 11.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
BIN-3

Manual Integrations
APPROVED

Ankita
3/10/2021 10:14:02 AM

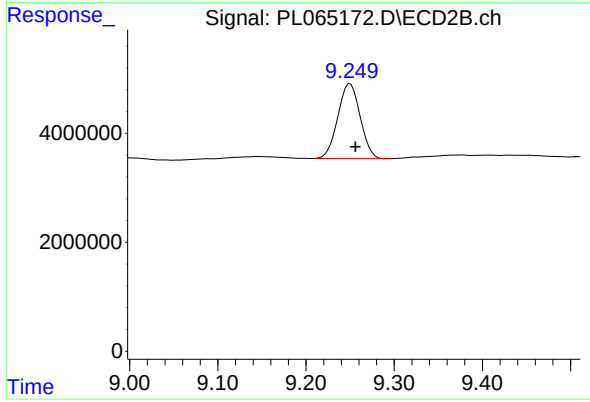

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 24200985
Conc: 11.02 ng/ml