

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
 Data File : PL065181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 17:41
 Operator : AR\AJ
 Sample : M1601-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BIN-3

Manual Integrations
 APPROVED

Ankita
 3/10/2021 10:14:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:22:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.096	37477914	31263653	12.746	12.590
28)	SA Decachlor...	8.138	9.250	41250894	36651559	14.865	16.686
Target Compounds							
12)	B 4,4'-DDE	5.562	6.469	7296266	5806849	2.030m	2.323m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
Data File : PL065181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 17:41
Operator : AR\AJ
Sample : M1601-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BIN-3


Manual Integrations
APPROVED

Ankita
3/10/2021 10:14:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:22:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

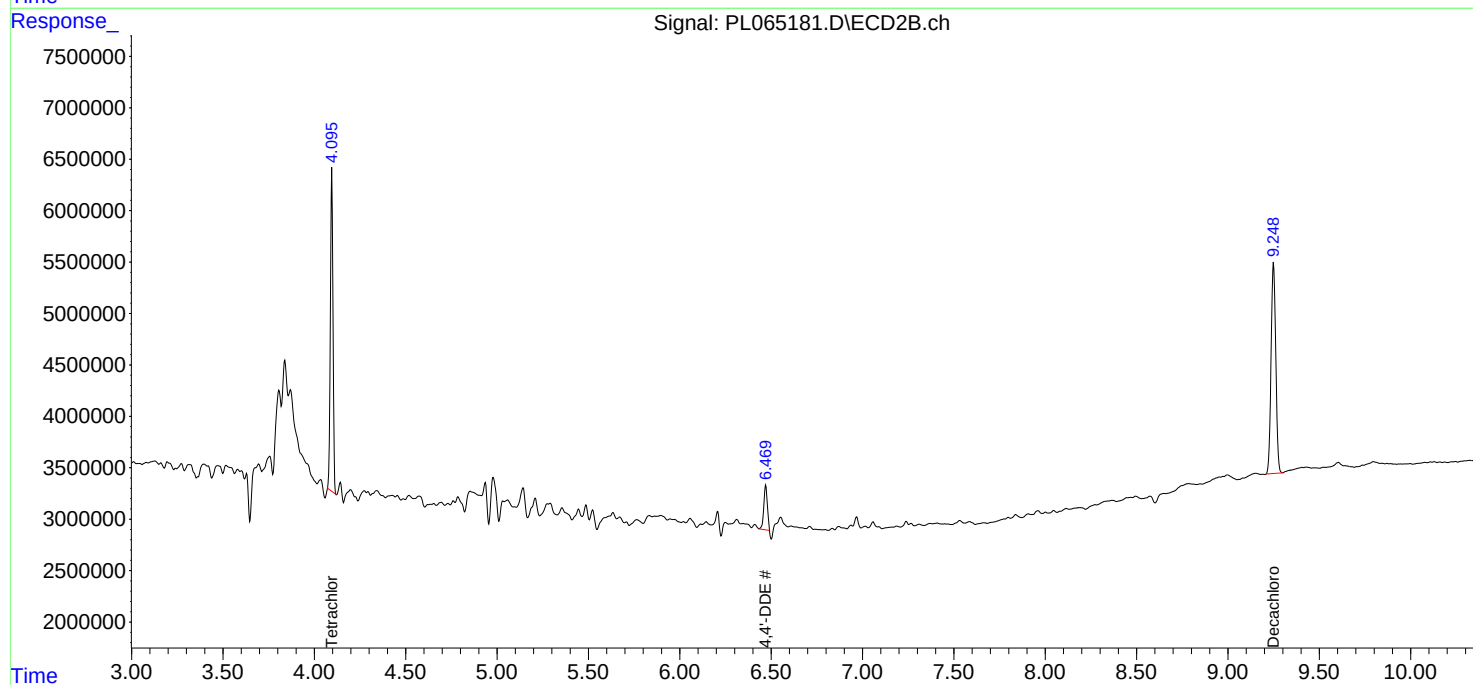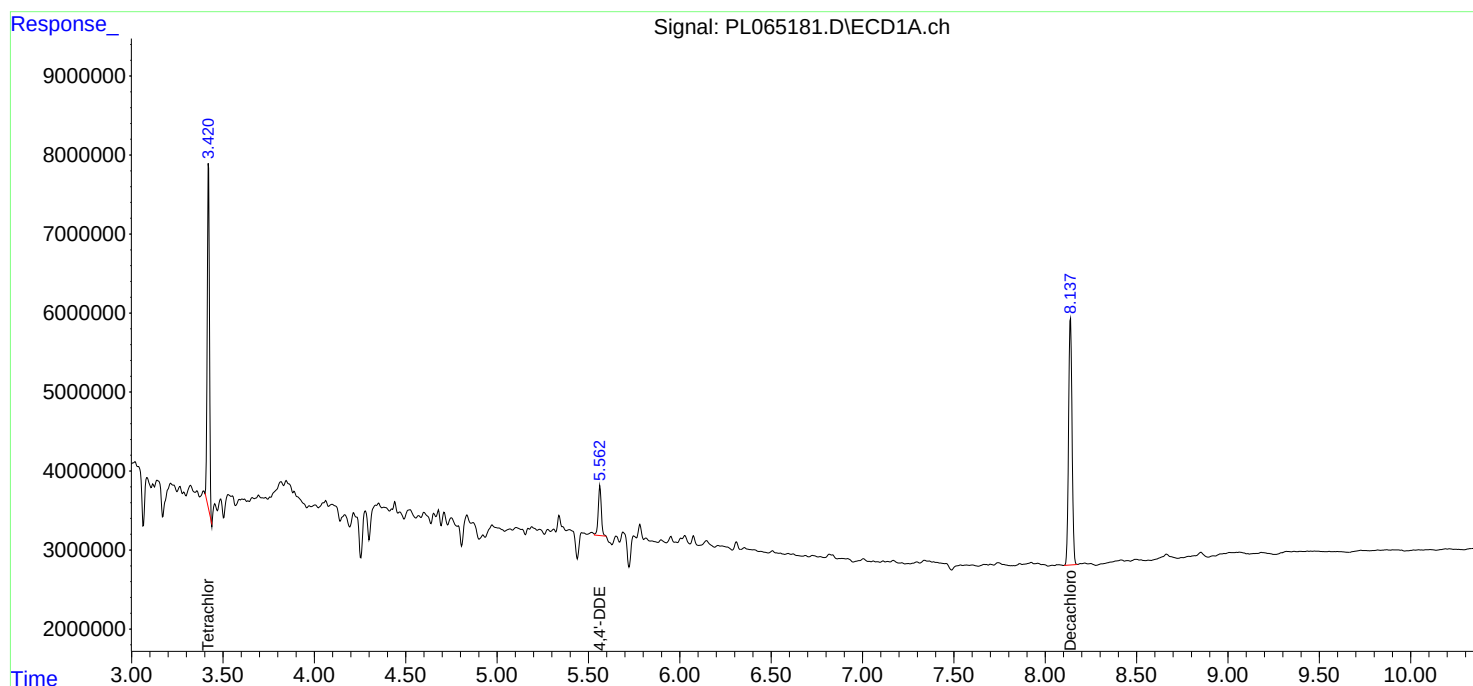

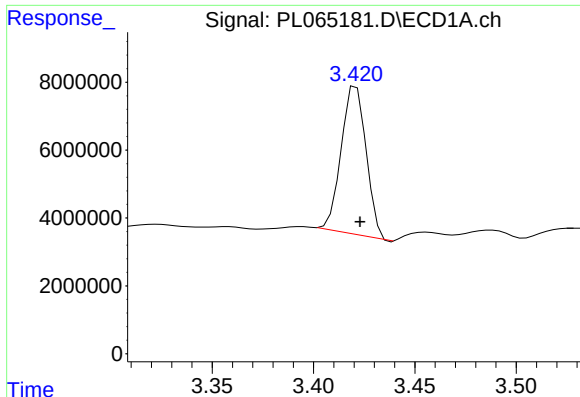


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: -0.002 min
Response: 37477914
Conc: 12.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
BIN-3


Manual Integrations
APPROVED

Ankita
3/10/2021 10:14:09 AM

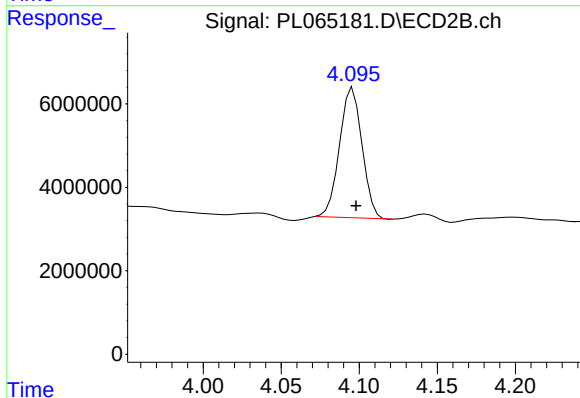


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.002 min
Response: 31263653
Conc: 12.59 ng/ml

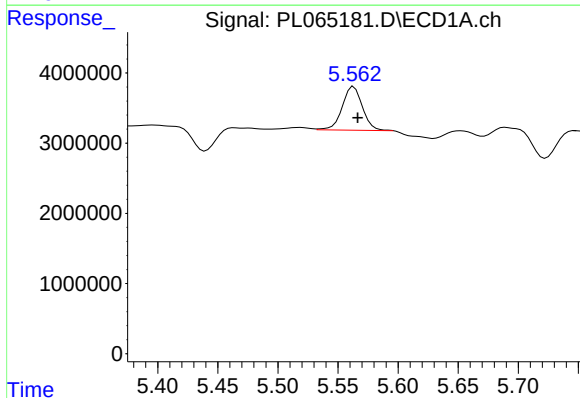


#12 4,4'-DDE

R.T.: 5.562 min
Delta R.T.: -0.005 min
Response: 7296266
Conc: 2.03 ng/ml m

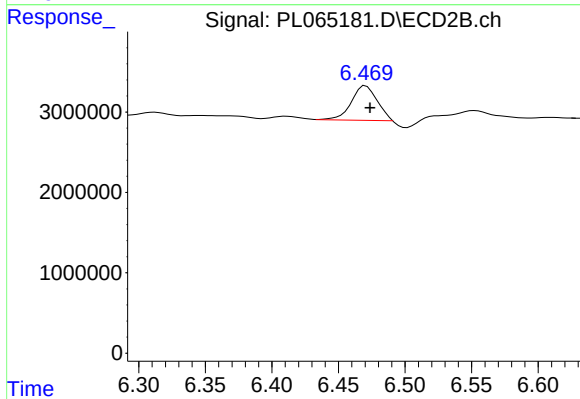

#12 4,4'-DDE

R.T.: 6.469 min
Delta R.T.: -0.005 min
Response: 5806849
Conc: 2.32 ng/ml m

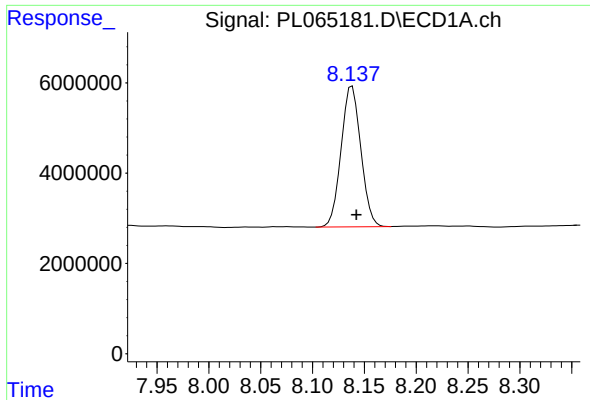


#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: -0.004 min
Response: 41250894
Conc: 14.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
BIN-3

Manual Integrations
APPROVED

Ankita
3/10/2021 10:14:09 AM

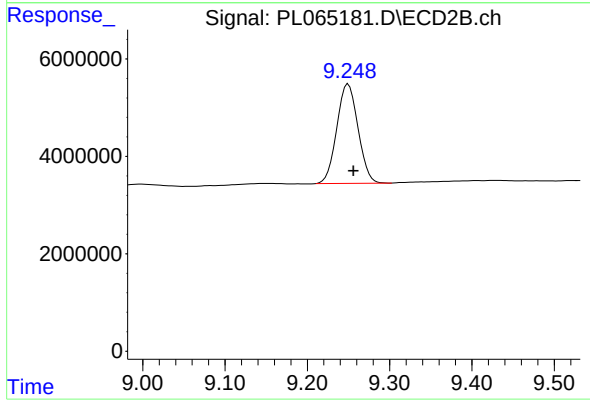

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 36651559
Conc: 16.69 ng/ml