

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040723\
 Data File : PL081886.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2023 08:55
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 22:02:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.331	2.654	105.4E6	109.8E6	45.304	55.002
28)	SA Decachlor...	8.751	7.771	73682280	89374306	41.172	45.065
Target Compounds							
23)	Chlordane-1	4.475	3.641	47795772	35822166	480.753	465.072
24)	Chlordane-2	5.001	4.216	48813570	41544082	469.019	444.712
25)	Chlordane-3	5.706	4.843	177.1E6	120.3E6	447.091	477.673
26)	Chlordane-4	5.787	4.904	221.9E6	124.1E6	463.774	473.805
27)	Chlordane-5	6.628	5.571	35413325	28237306	417.040	423.090



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040723\
Data File : PL081886.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2023 08:55
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 22:02:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

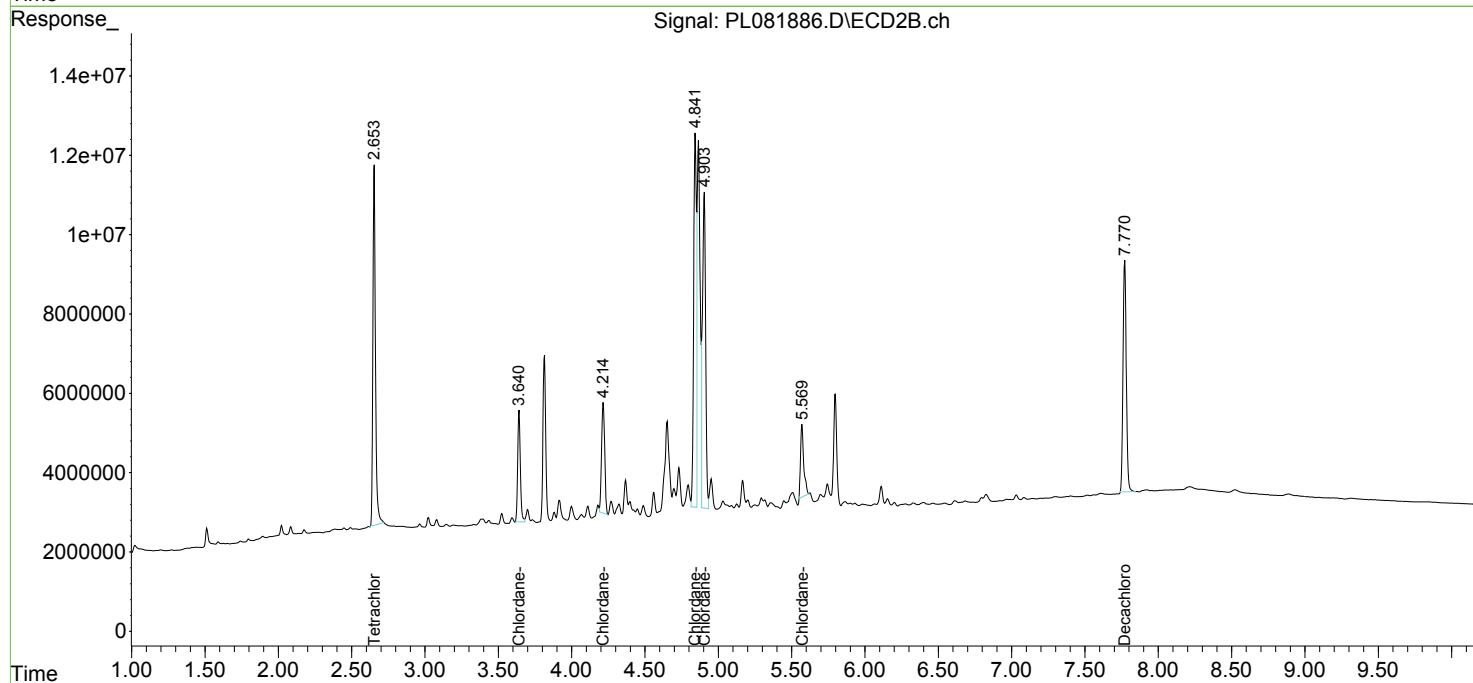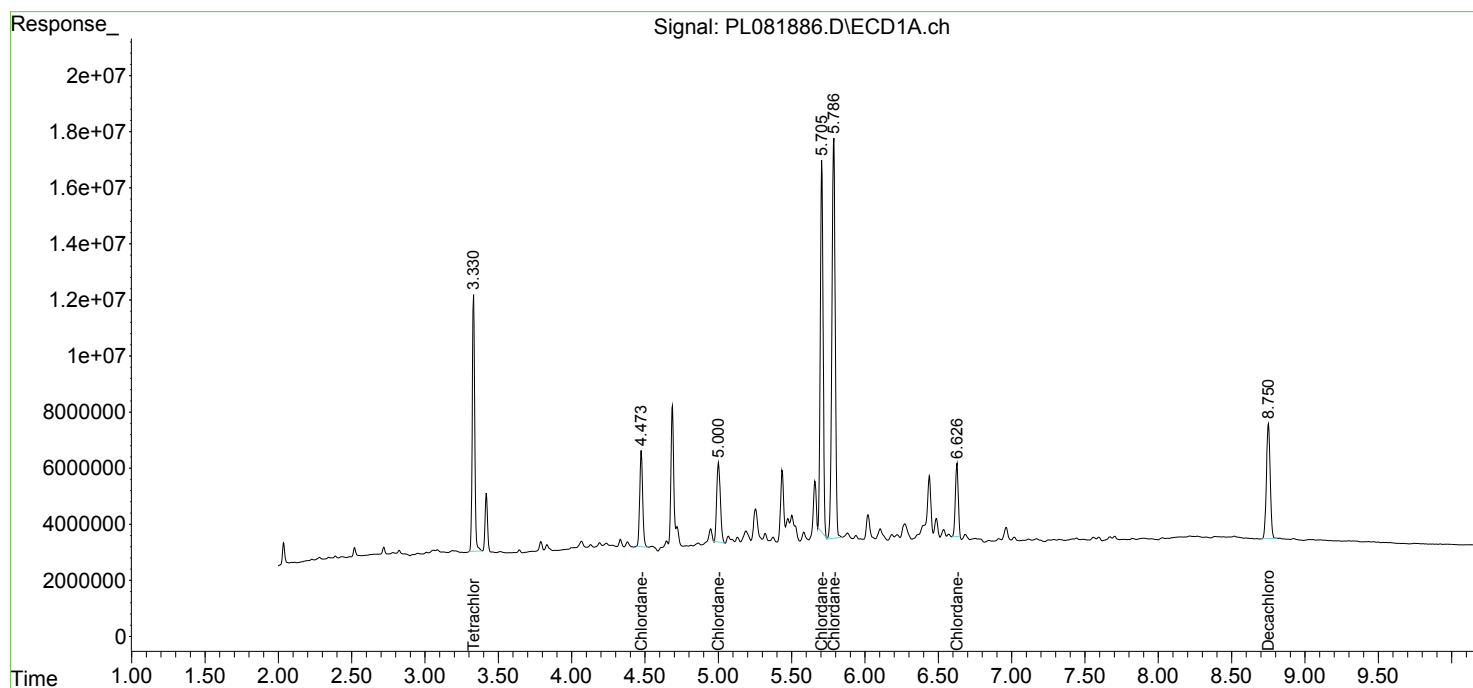


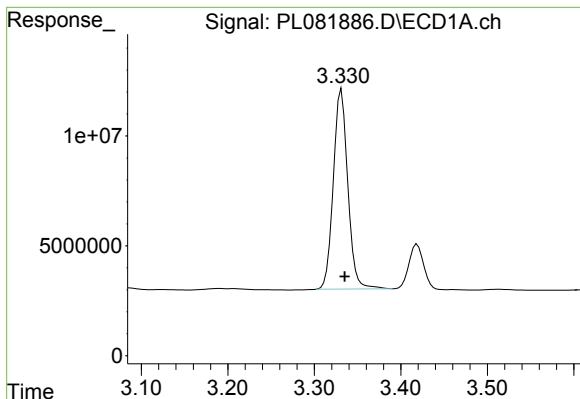

#1 Tetrachloro-m-xylene


R.T.: 3.331 min
Delta R.T.: -0.004 min
Response: 105372542
Conc: 45.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

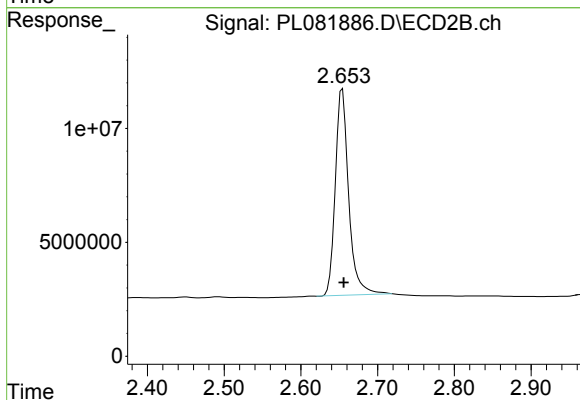


#1 Tetrachloro-m-xylene

R.T.: 2.654 min
Delta R.T.: -0.002 min
Response: 109792192
Conc: 55.00 ng/ml

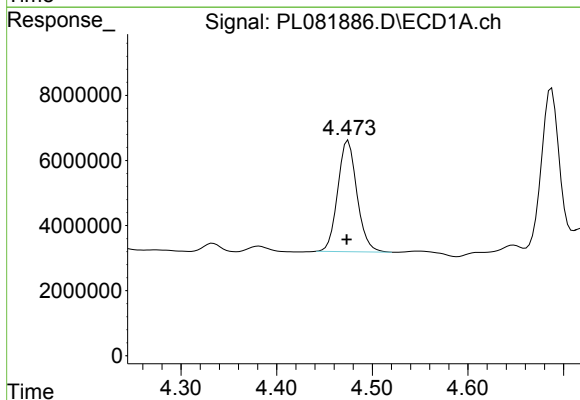


#23 Chlordane-1

R.T.: 4.475 min
Delta R.T.: 0.002 min
Response: 47795772
Conc: 480.75 ng/ml

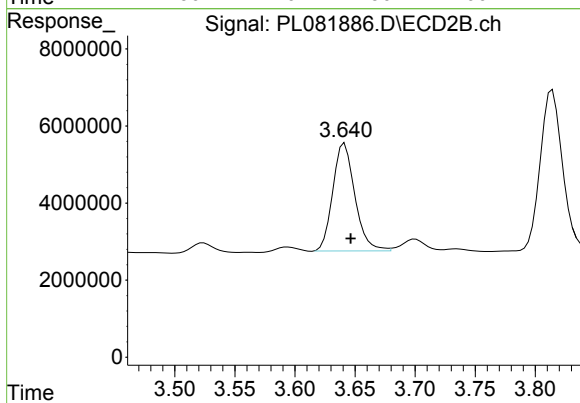

#23 Chlordane-1


R.T.: 3.641 min
Delta R.T.: -0.005 min
Response: 35822166
Conc: 465.07 ng/ml

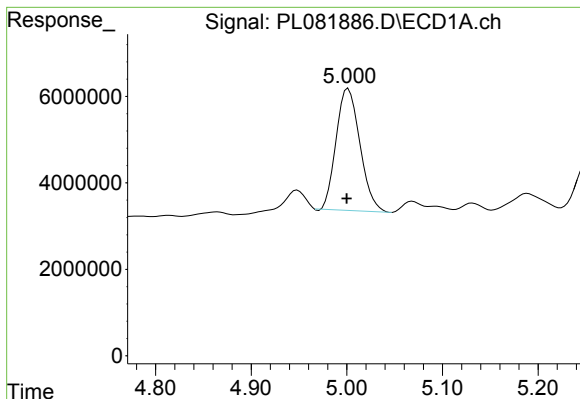

#24 Chlordane-2


R.T.: 5.001 min
Delta R.T.: 0.002 min
Response: 48813570
Conc: 469.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

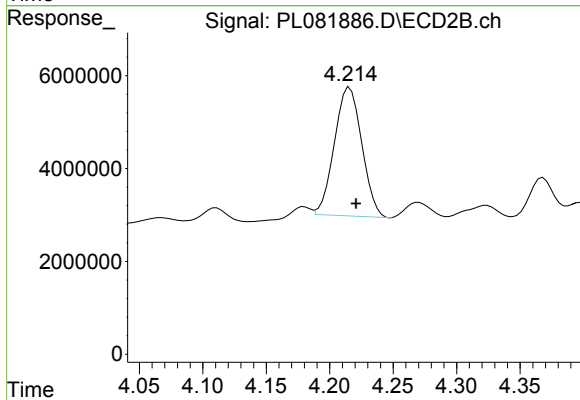


#24 Chlordane-2

R.T.: 4.216 min
Delta R.T.: -0.005 min
Response: 41544082
Conc: 444.71 ng/ml

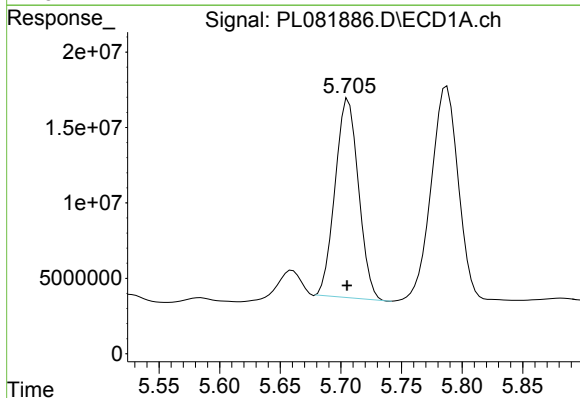


#25 Chlordane-3

R.T.: 5.706 min
Delta R.T.: 0.001 min
Response: 177098580
Conc: 447.09 ng/ml

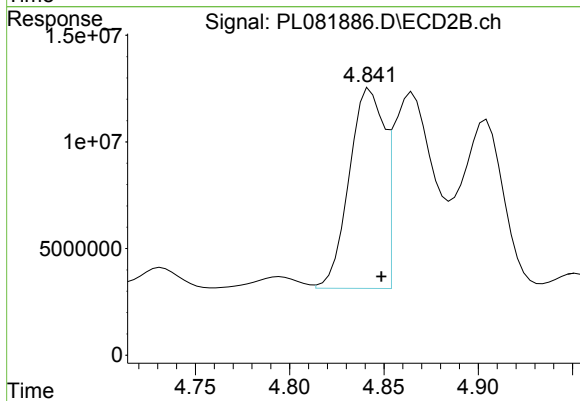

#25 Chlordane-3


R.T.: 4.843 min
Delta R.T.: -0.006 min
Response: 120312062
Conc: 477.67 ng/ml

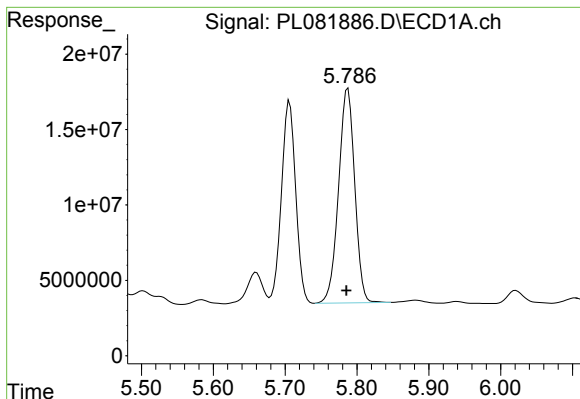

#26 Chlordane-4


R.T.: 5.787 min
Delta R.T.: 0.002 min
Response: 221943814
Conc: 463.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

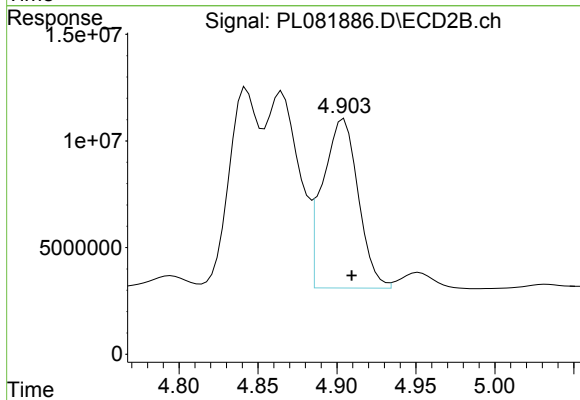


#26 Chlordane-4

R.T.: 4.904 min
Delta R.T.: -0.005 min
Response: 124104848
Conc: 473.80 ng/ml

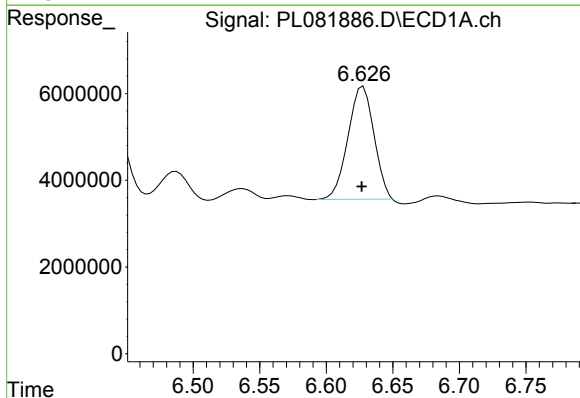


#27 Chlordane-5

R.T.: 6.628 min
Delta R.T.: 0.001 min
Response: 35413325
Conc: 417.04 ng/ml

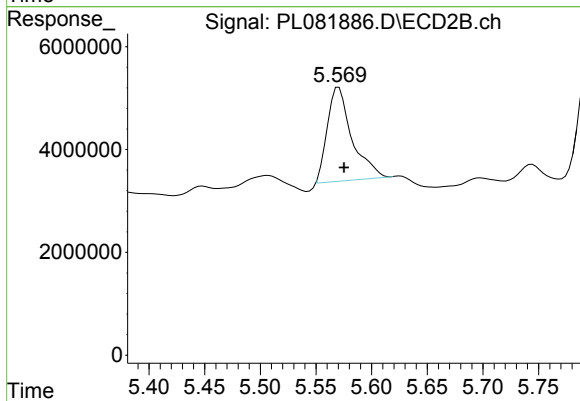

#27 Chlordane-5


R.T.: 5.571 min
Delta R.T.: -0.005 min
Response: 28237306
Conc: 423.09 ng/ml

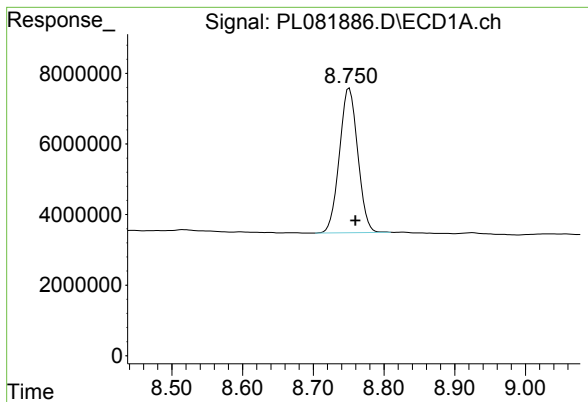

#28 Decachlorobiphenyl

R.T.: 8.751 min
Delta R.T.: -0.009 min
Response: 73682280
Conc: 41.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

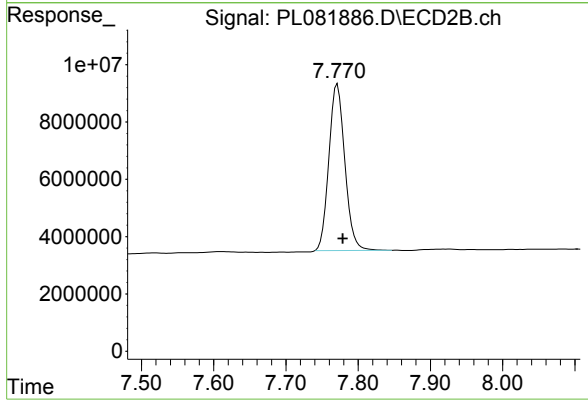

#28 Decachlorobiphenyl

R.T.: 7.771 min
Delta R.T.: -0.007 min
Response: 89374306
Conc: 45.06 ng/ml