

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040723\
 Data File : PL081927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 08:36
 Operator : AR\AJ
 Sample : 02224-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU3-FC-BACKFILL-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 12:43:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	2.655	38149569	33057362	16.402	16.561
28)	SA Decachlor...	8.749	7.771	29996876	35228426	16.761	17.763

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040723\
Data File : PL081927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 08:36
Operator : AR\AJ
Sample : 02224-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OU3-FC-BACKFILL-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 12:43:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

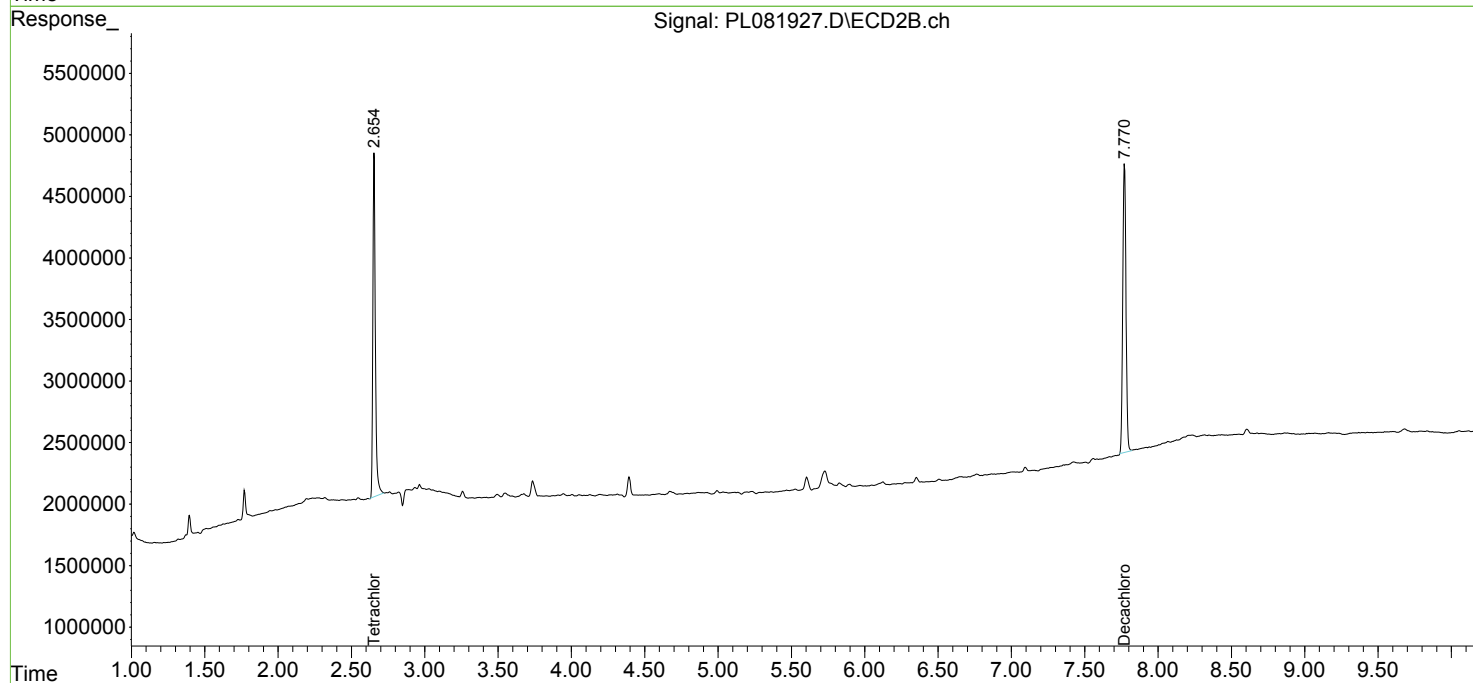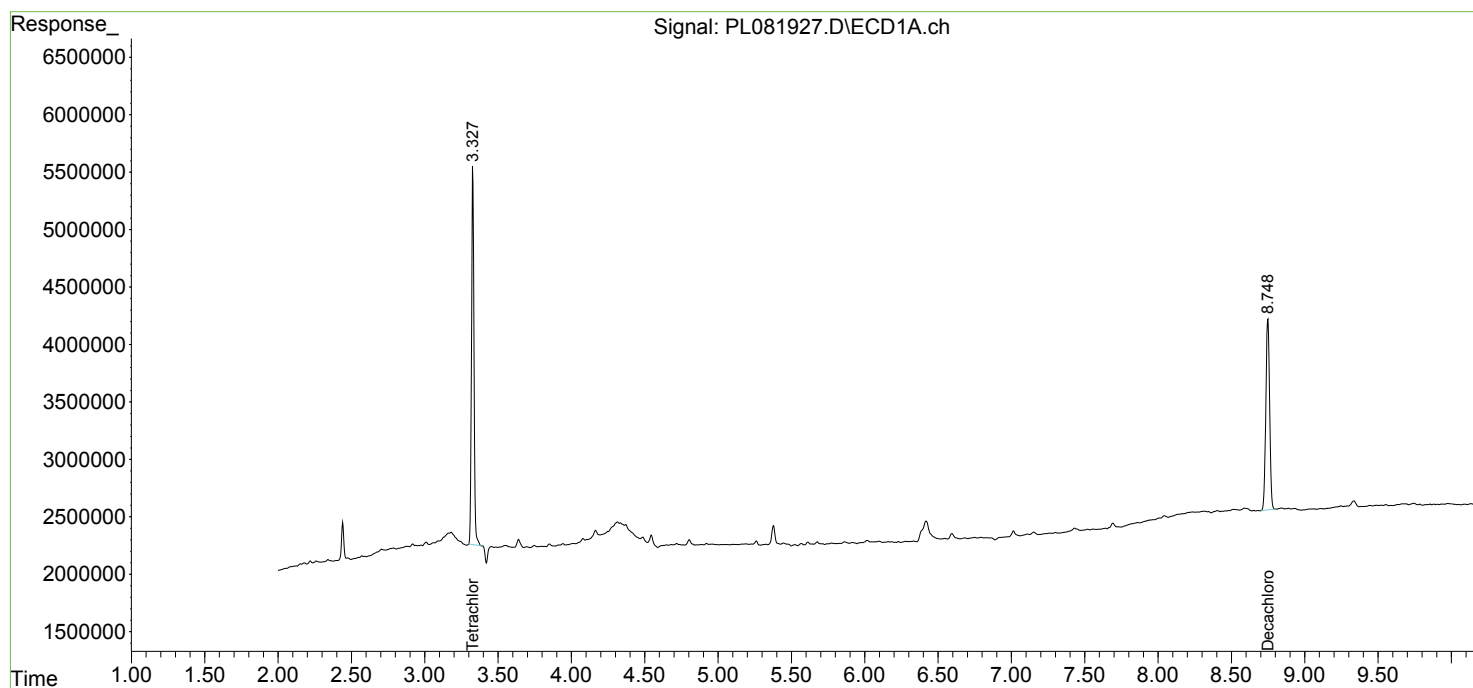


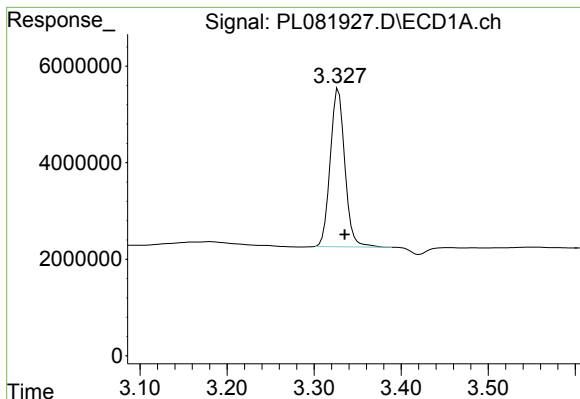

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: -0.007 min
Response: 38149569
Conc: 16.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU3-FC-BACKFILL-02

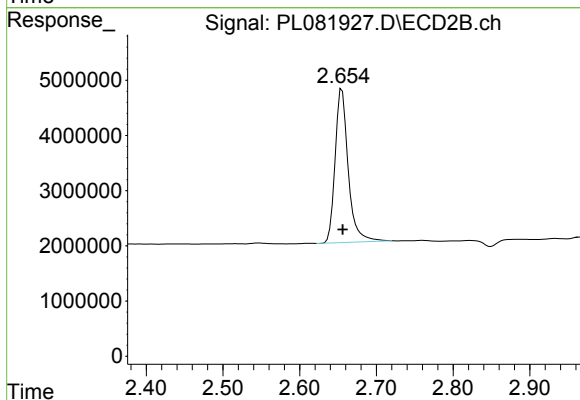


#1 Tetrachloro-m-xylene

R.T.: 2.655 min
Delta R.T.: 0.000 min
Response: 33057362
Conc: 16.56 ng/ml

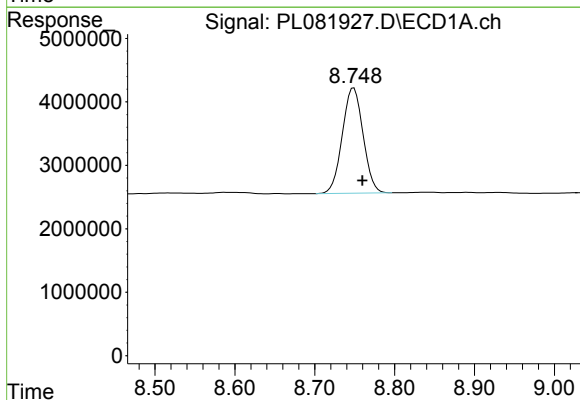

#28 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.011 min
Response: 29996876
Conc: 16.76 ng/ml

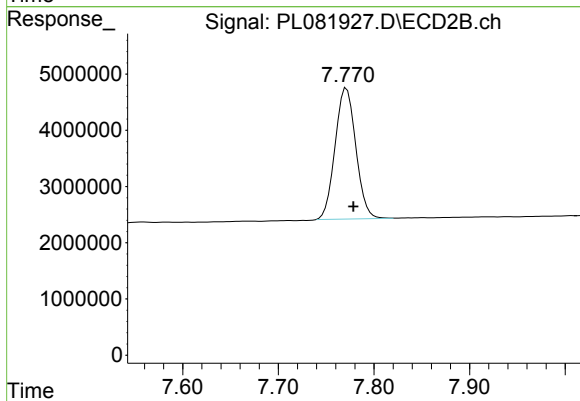

#28 Decachlorobiphenyl

R.T.: 7.771 min
Delta R.T.: -0.007 min
Response: 35228426
Conc: 17.76 ng/ml