

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 09:01
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 01:52:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	0.000	5.350f	0	3397309	N.D.	0.610 #
6) B	beta-BHC	0.000	5.034	0	15021414	N.D.	1.745 #
7) B	delta-BHC	0.000	5.251	0	1823025	N.D.	0.355 #
15) B	Endosulfa...	0.000	7.125	0	503610	N.D.	0.144 #
18) B	Endrin al...	0.000	7.262	0	568520	N.D.	0.203 #
21) B	Endrin ke...	0.000	7.973	0	1662530	N.D.	0.452 #
22)	Mirex	0.000	8.443f	0	254907	N.D.	0.090 #
23)	Chlordane-1	4.321	5.200f	3526797	3948508	30.850	22.966 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 09:01
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 01:52:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

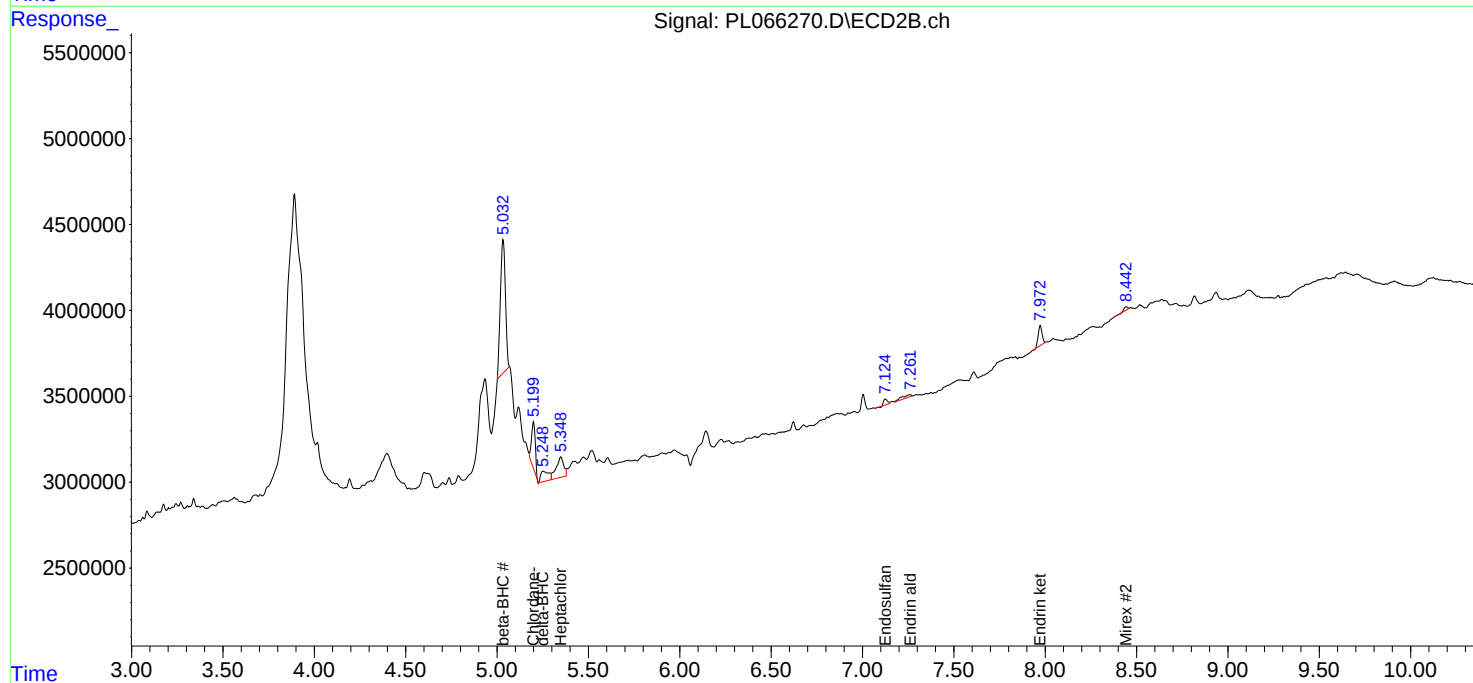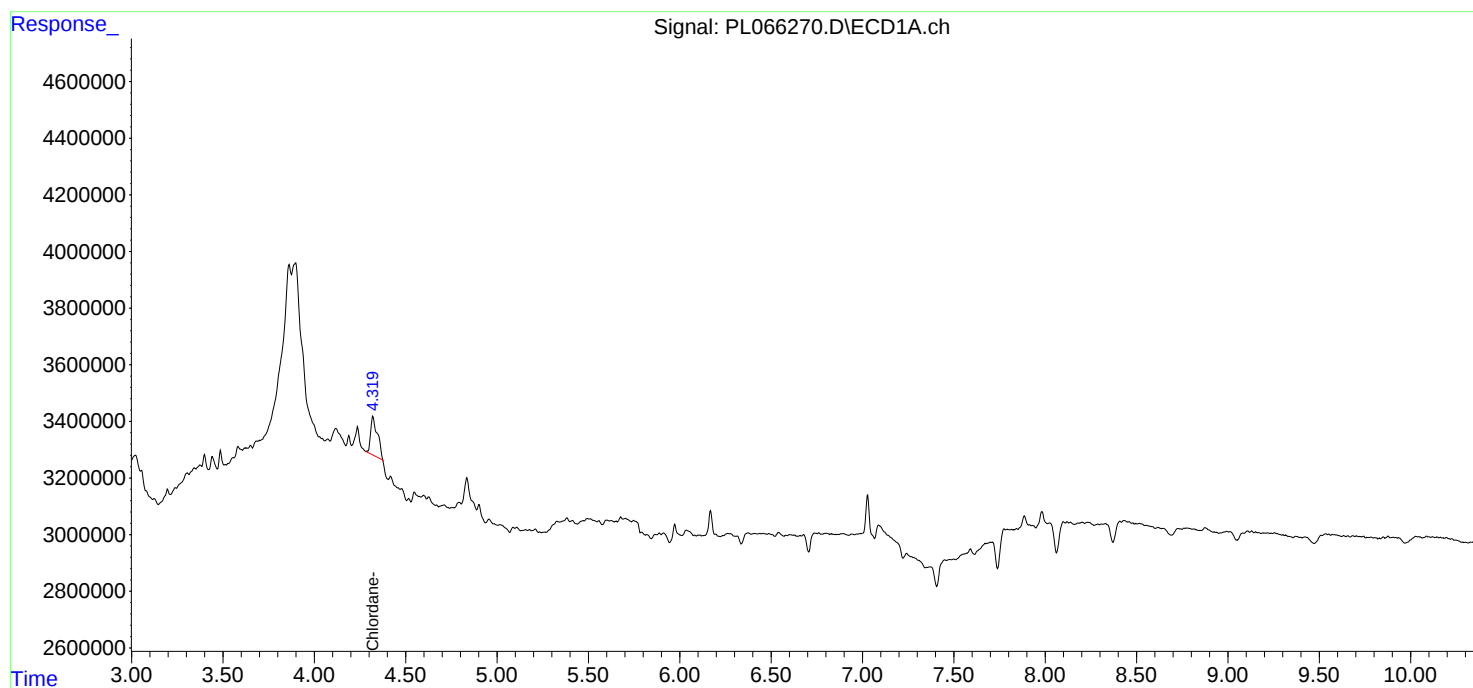


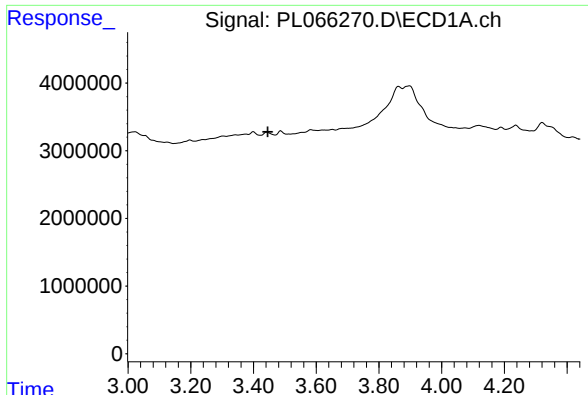

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

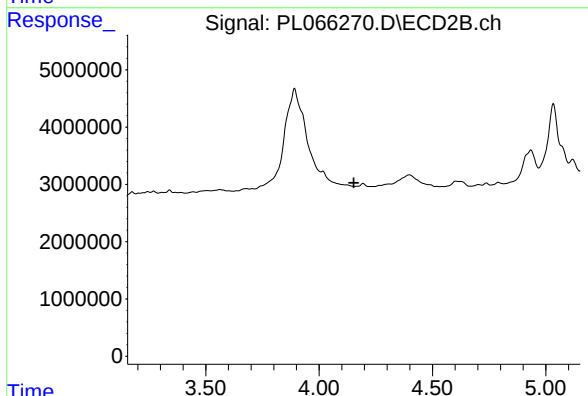


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

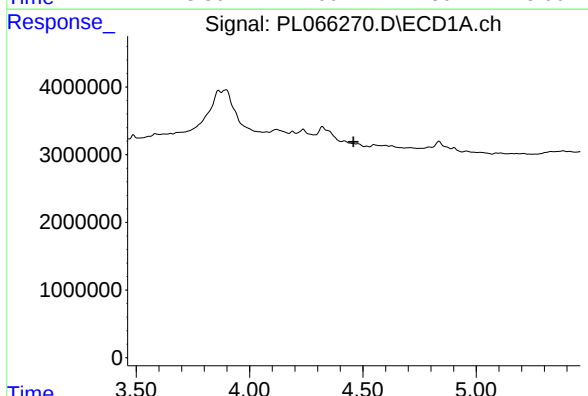


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

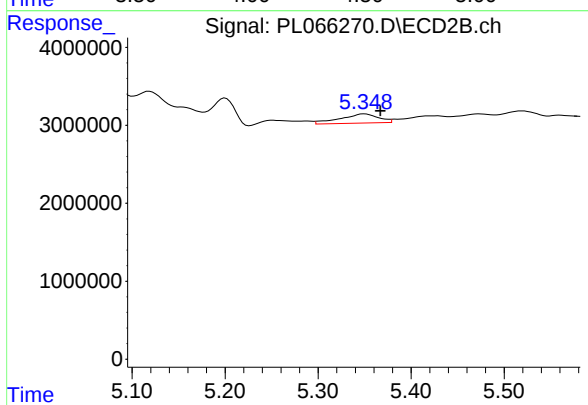

#4 Heptachlor


R.T.: 5.350 min
Delta R.T.: -0.017 min
Response: 3397309
Conc: 0.61 ng/ml

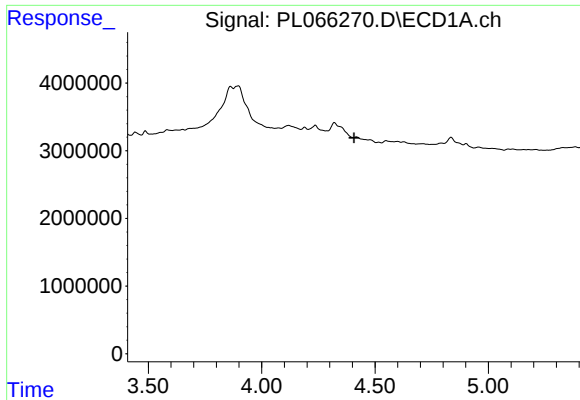

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

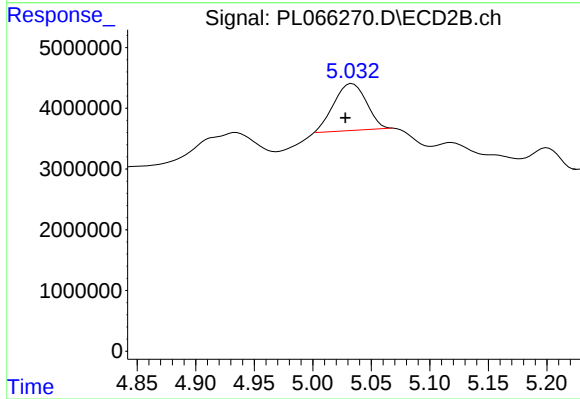


#6 beta-BHC

R.T.: 5.034 min
Delta R.T.: 0.006 min
Response: 15021414
Conc: 1.74 ng/ml

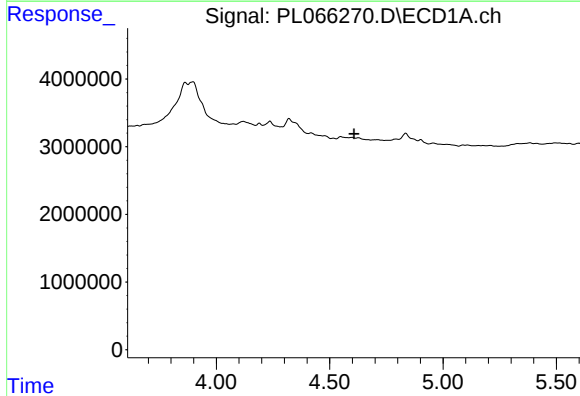


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.608 min
Response: 0
Conc: N.D.

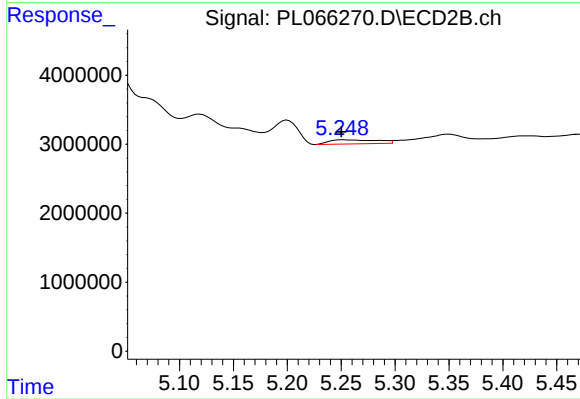

#7 delta-BHC


R.T.: 5.251 min
Delta R.T.: 0.001 min
Response: 1823025
Conc: 0.35 ng/ml

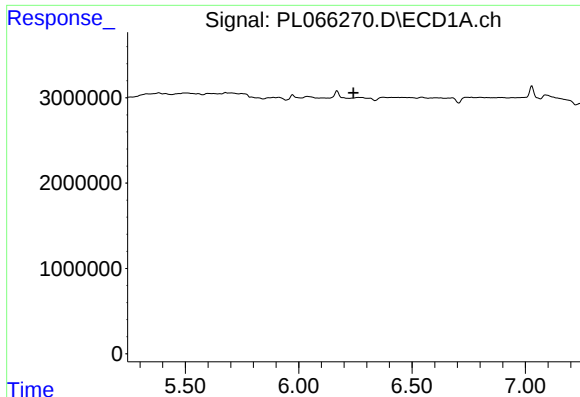

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

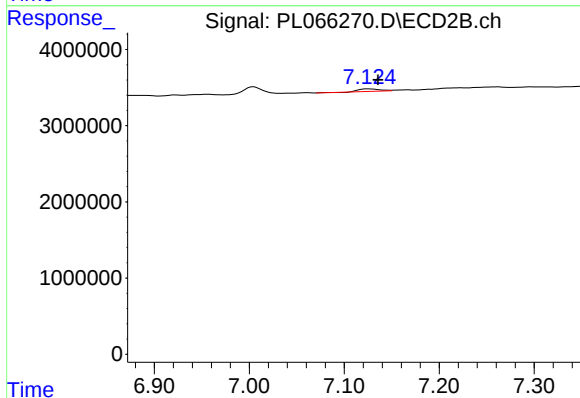


#15 Endosulfan II

R.T.: 7.125 min
Delta R.T.: -0.010 min
Response: 503610
Conc: 0.14 ng/ml

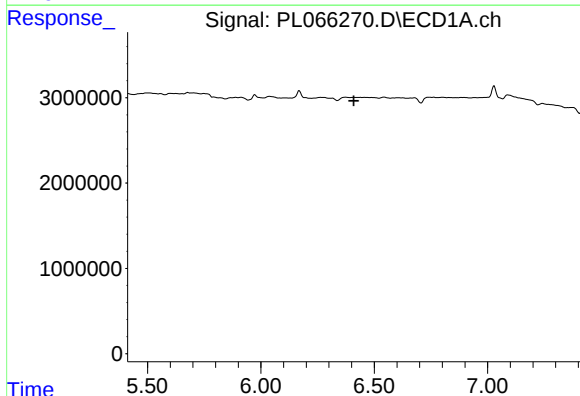


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

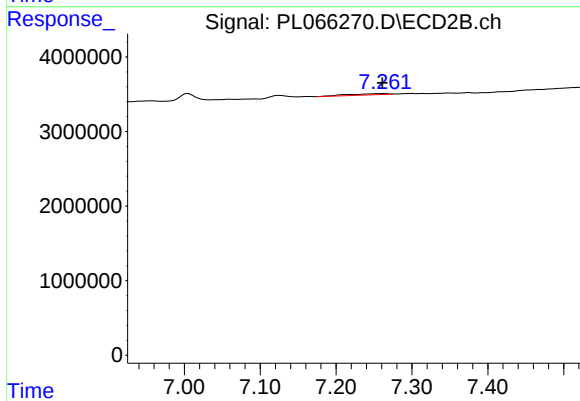

#18 Endrin aldehyde


R.T.: 7.262 min
Delta R.T.: 0.001 min
Response: 568520
Conc: 0.20 ng/ml

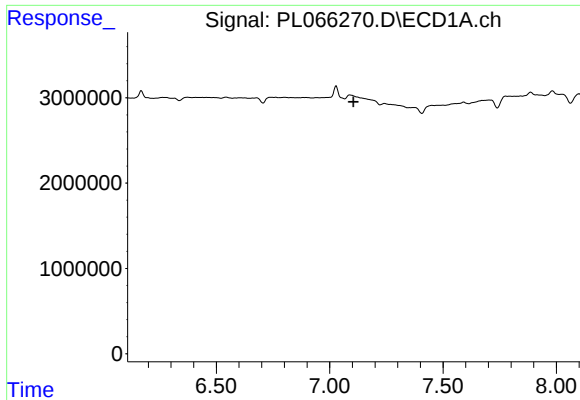

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

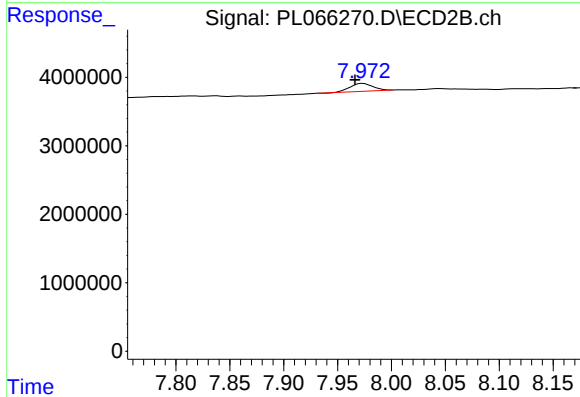


#21 Endrin ketone

R.T.: 7.973 min
Delta R.T.: 0.007 min
Response: 1662530
Conc: 0.45 ng/ml

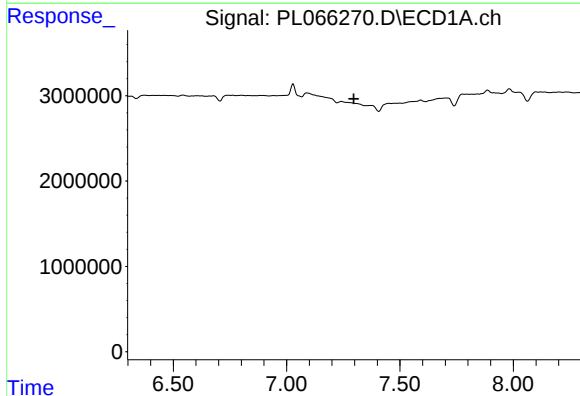


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.296 min
Response: 0
Conc: N.D.

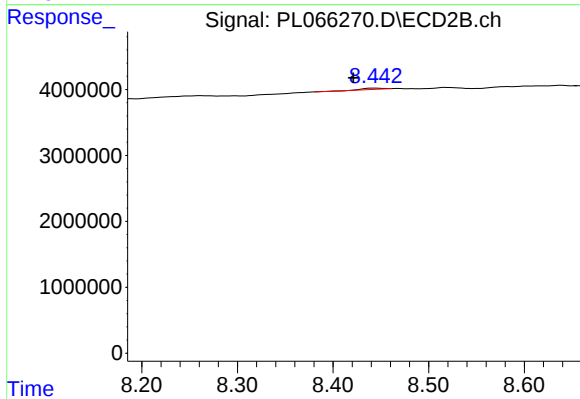

#22 Mirex


R.T.: 8.443 min
Delta R.T.: 0.022 min
Response: 254907
Conc: 0.09 ng/ml

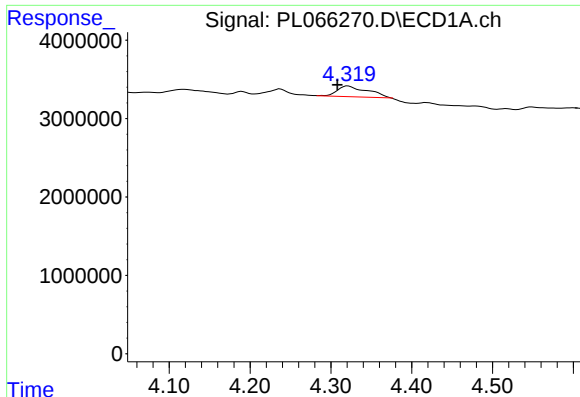

#23 Chlordane-1


R.T.: 4.321 min
Delta R.T.: 0.013 min
Response: 3526797
Conc: 30.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

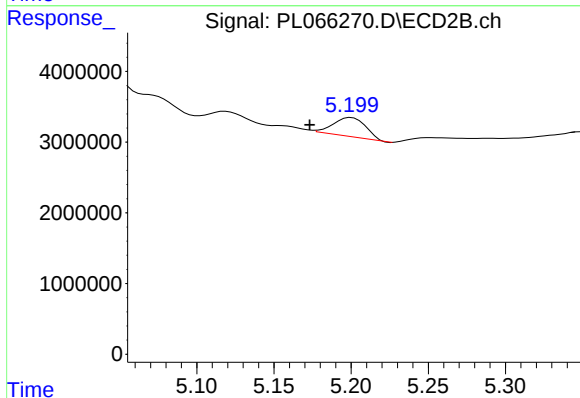


#23 Chlordane-1

R.T.: 5.200 min
Delta R.T.: 0.027 min
Response: 3948508
Conc: 22.97 ng/ml

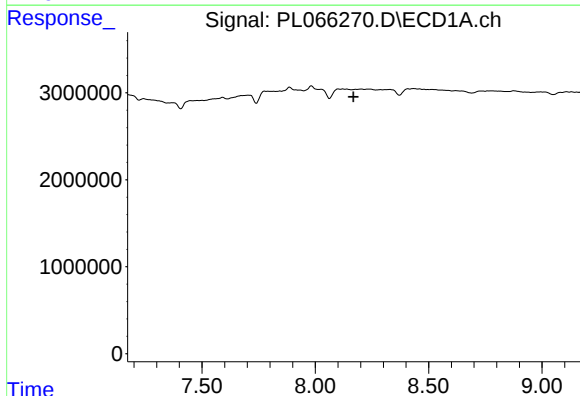

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.169 min
Response: 0
Conc: N.D.

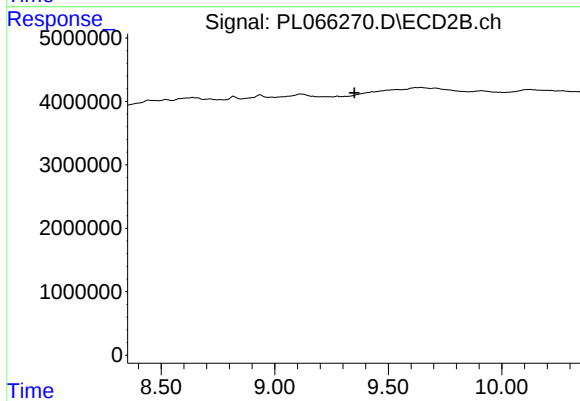

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.351 min
Response: 0
Conc: N.D.