

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 09:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 01:52:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.153	48825473	80452788	19.183	20.000
28)	SA Decachlor...	8.167	9.352	50233416	62509037	21.060	19.140
Target Compounds							
2)	A alpha-BHC	3.870	0.000	2296027	0	0.558	N.D. #
4)	MA Heptachlor	0.000	5.351f	0	3160201	N.D.	0.568 #
6)	B beta-BHC	0.000	5.034	0	15898424	N.D.	2.129 #
14)	MA Endrin	0.000	6.946f	0	12976555	N.D.	4.016 #
15)	B Endosulfa...	0.000	7.123	0	1828463	N.D.	0.525 #
17)	MA 4,4'-DDT	0.000	7.341	0	352211	N.D.	0.104 #
21)	B Endrin ke...	0.000	7.973	0	1864564	N.D.	0.507 #
23)	Chlordane-1	4.331f	0.000	3318826	0	29.031	N.D. #
27)	Chlordane-5	0.000	7.194	0	1451036	N.D.	10.826 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 09:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 01:52:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

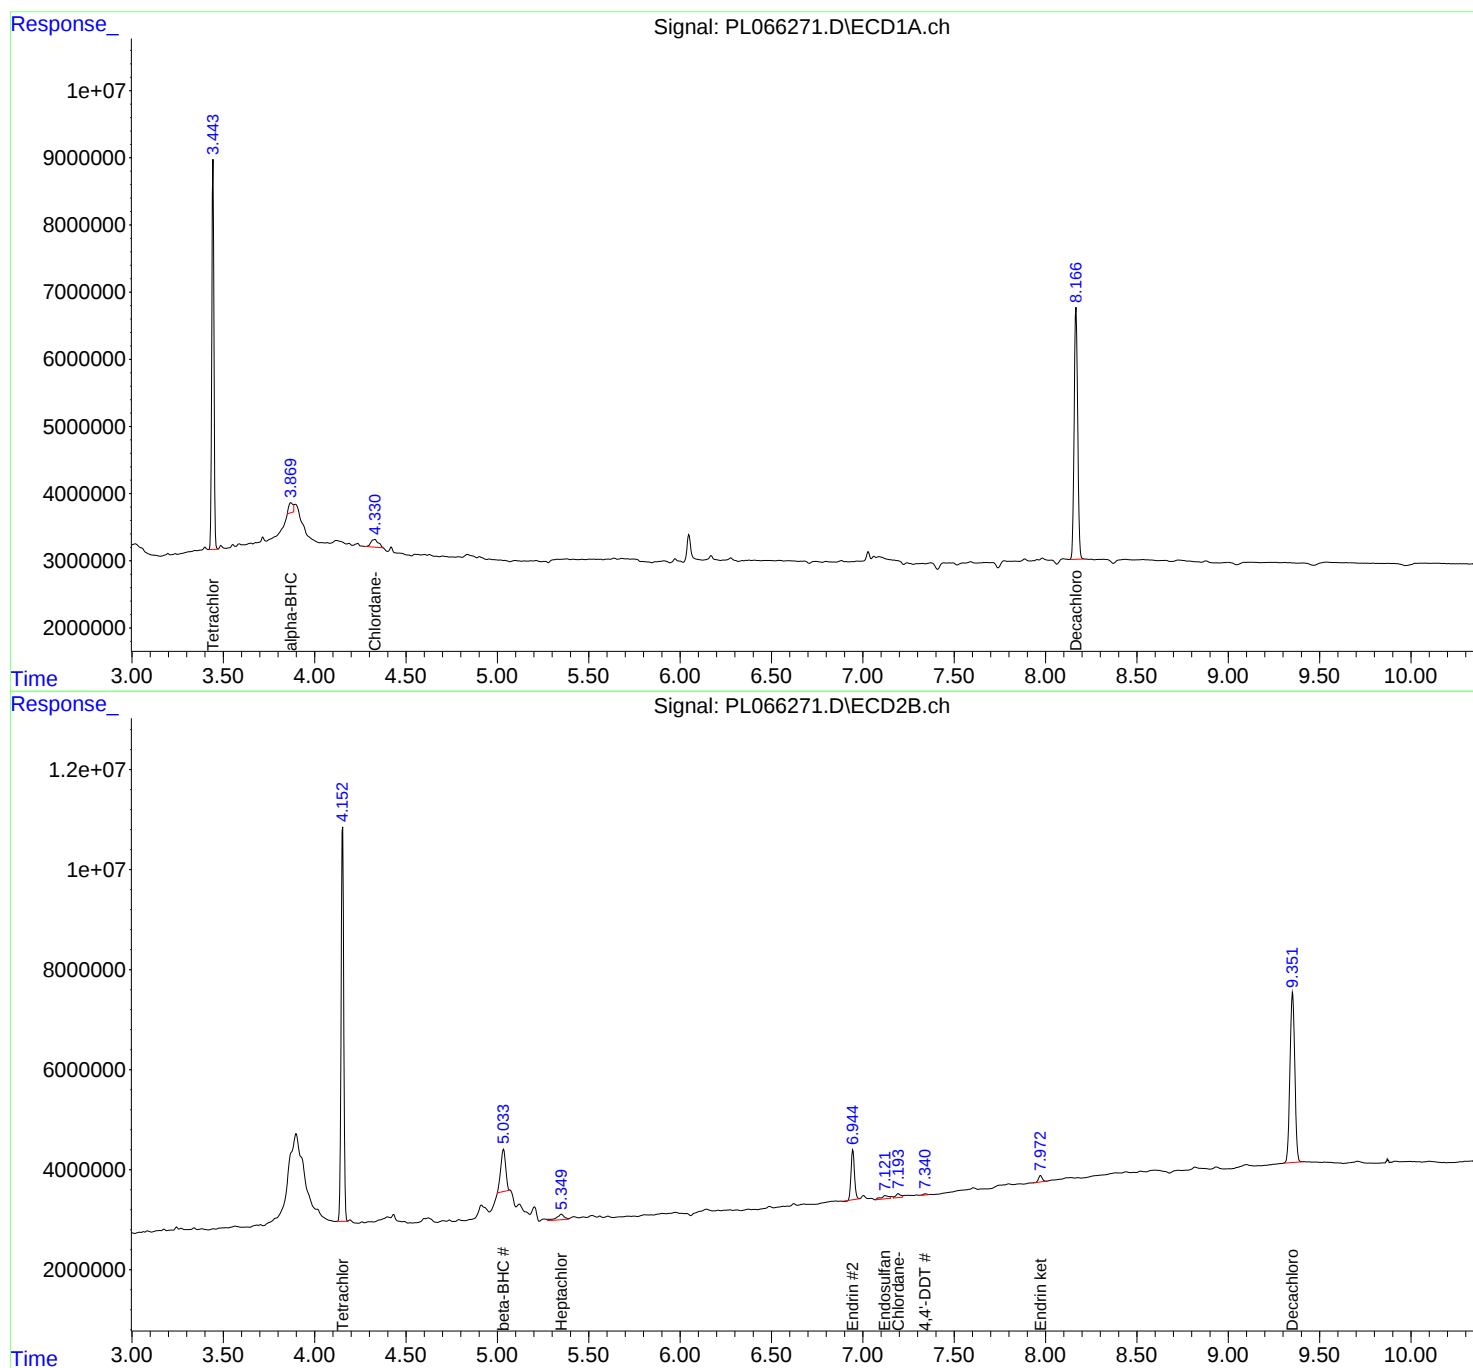


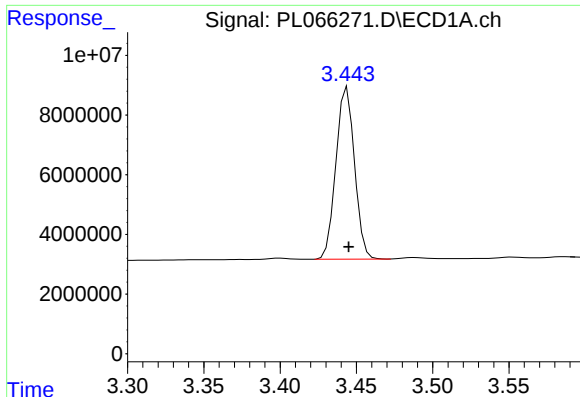

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 48825473
Conc: 19.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

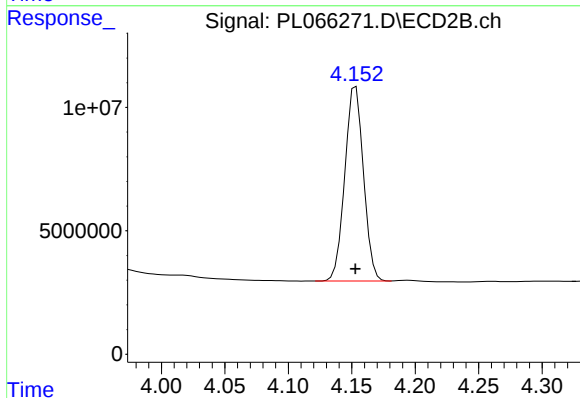


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 80452788
Conc: 20.00 ng/ml

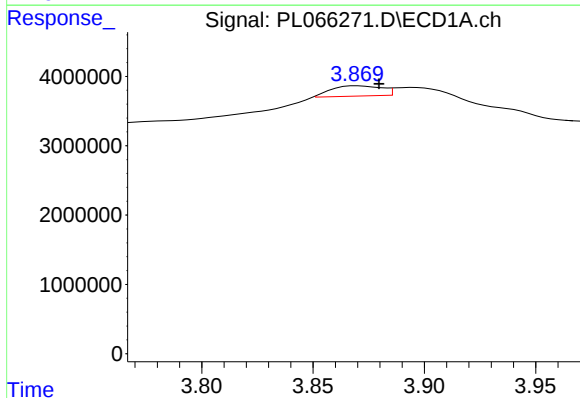


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: -0.010 min
Response: 2296027
Conc: 0.56 ng/ml

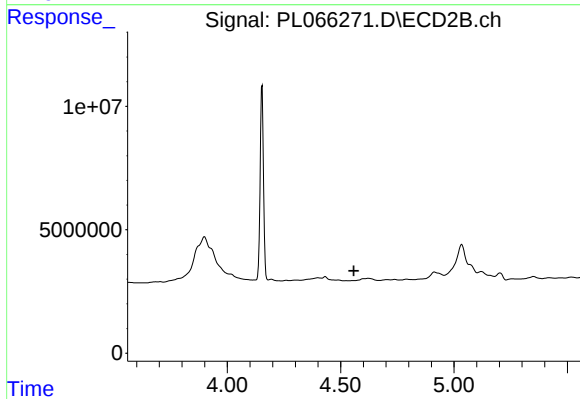

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.558 min
Response: 0
Conc: N.D.

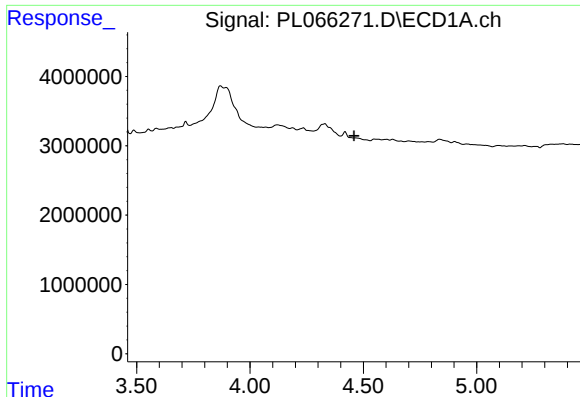

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

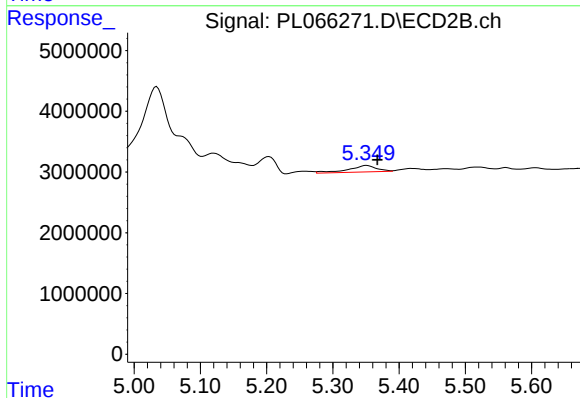


#4 Heptachlor

R.T.: 5.351 min
Delta R.T.: -0.016 min
Response: 3160201
Conc: 0.57 ng/ml

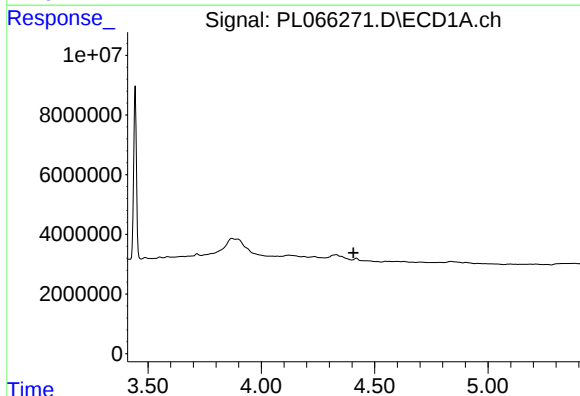


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.407 min
Response: 0
Conc: N.D.

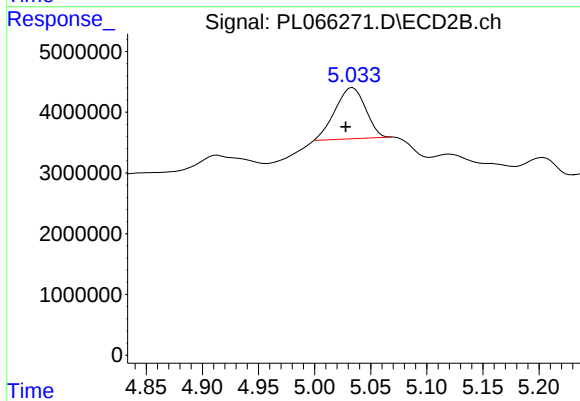

#6 beta-BHC


R.T.: 5.034 min
Delta R.T.: 0.006 min
Response: 15898424
Conc: 2.13 ng/ml

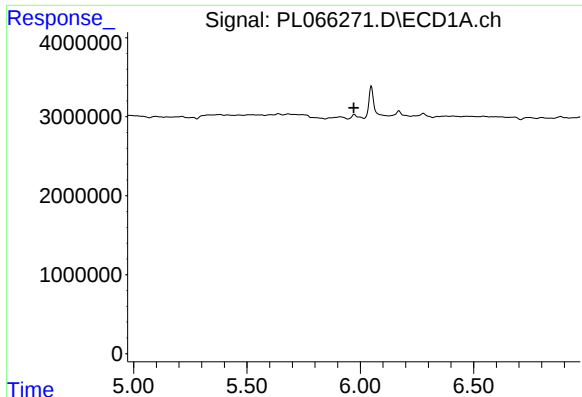

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

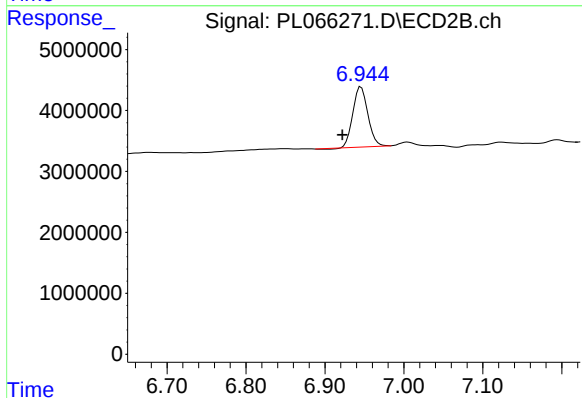


#14 Endrin

R.T.: 6.946 min
Delta R.T.: 0.024 min
Response: 12976555
Conc: 4.02 ng/ml

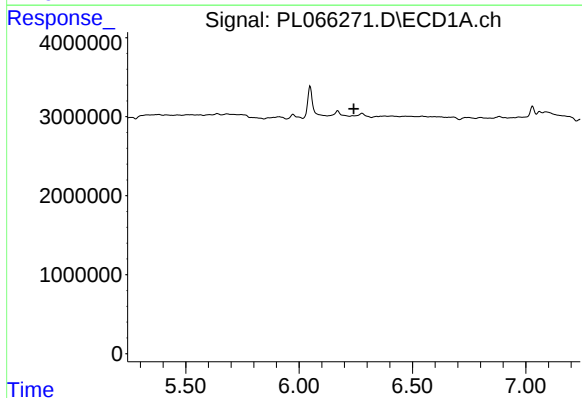


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

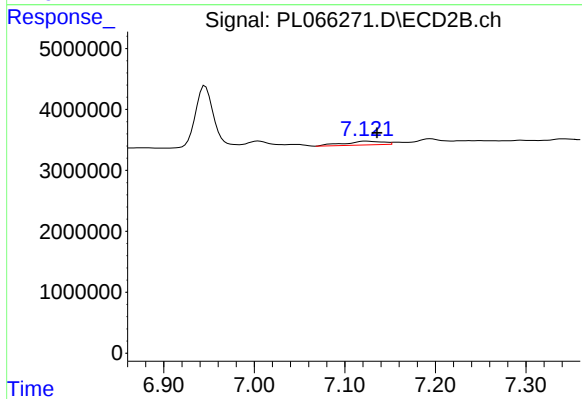

#15 Endosulfan II


R.T.: 7.123 min
Delta R.T.: -0.013 min
Response: 1828463
Conc: 0.52 ng/ml

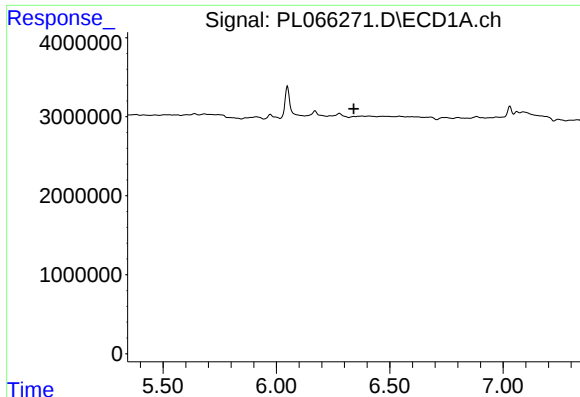

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

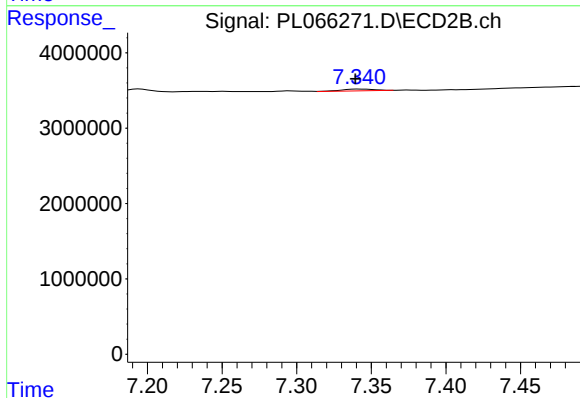


#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: 0.002 min
Response: 352211
Conc: 0.10 ng/ml

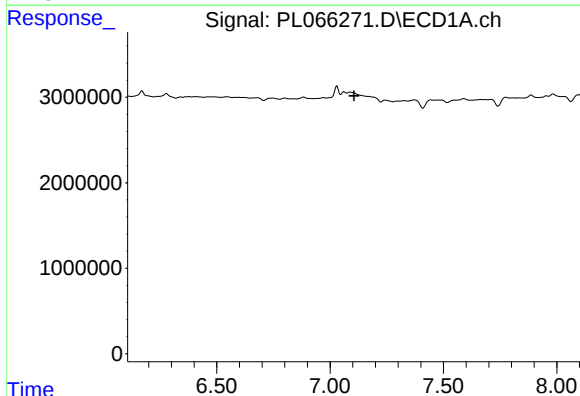


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

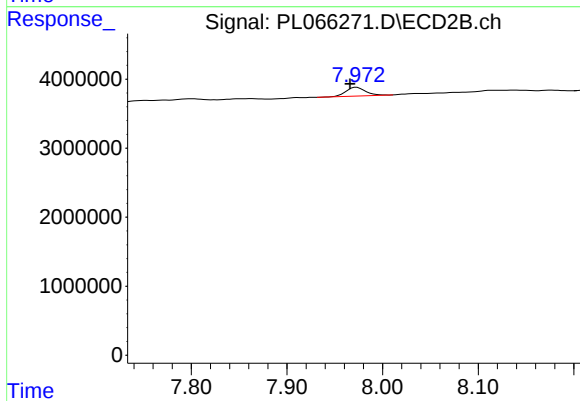

#21 Endrin ketone


R.T.: 7.973 min
Delta R.T.: 0.007 min
Response: 1864564
Conc: 0.51 ng/ml

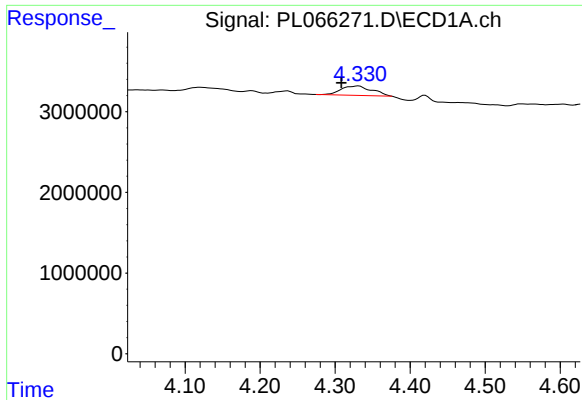

#23 Chlordane-1


R.T.: 4.331 min
Delta R.T.: 0.023 min
Response: 3318826
Conc: 29.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

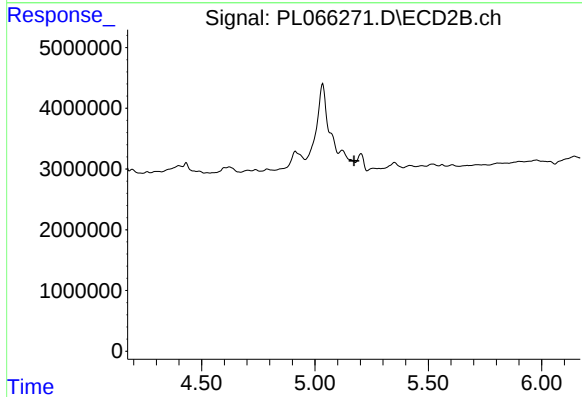


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.173 min
Response: 0
Conc: N.D.

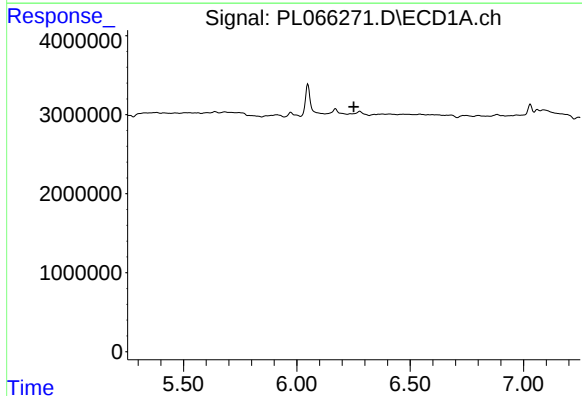


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

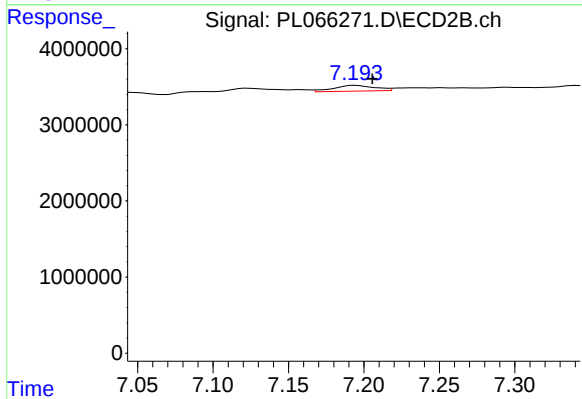

#27 Chlordane-5


R.T.: 7.194 min
Delta R.T.: -0.011 min
Response: 1451036
Conc: 10.83 ng/ml

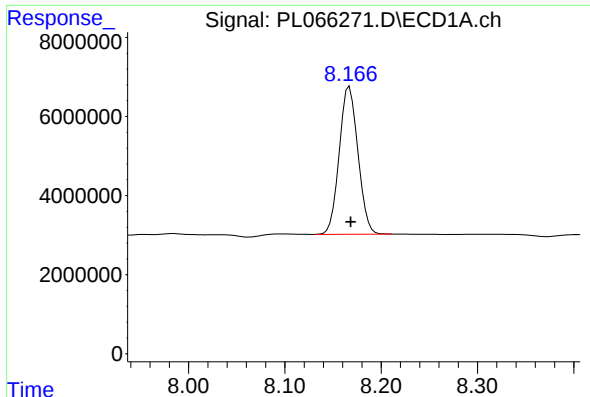

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: -0.001 min
Response: 50233416
Conc: 21.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

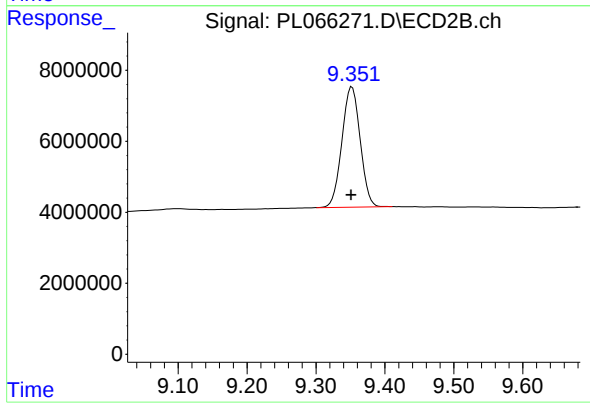

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.002 min
Response: 62509037
Conc: 19.14 ng/ml