

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066278.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 11:05
 Operator : AR\AJ
 Sample : PB135803BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 01:55:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.154	49495235	82702558	19.446	20.560
28)	SA Decachlor...	8.171	9.356	52272004	67945605	21.915	20.805
Target Compounds							
2)	A alpha-BHC	0.000	4.554	0	596789	N.D.	0.103 #
4)	MA Heptachlor	0.000	5.341f	0	2559745	N.D.	0.460 #
7)	B delta-BHC	0.000	5.255	0	1119831	N.D.	0.218 #
15)	B Endosulfa...	0.000	7.124	0	1963884	N.D.	0.563 #
17)	MA 4,4'-DDT	0.000	7.354	0	275609	N.D.	0.081 #
18)	B Endrin al...	0.000	7.264	0	2442051	N.D.	0.873 #
21)	B Endrin ke...	0.000	7.974	0	2980254	N.D.	0.810 #
23)	Chlordane-1	4.290f	5.187	2226491	2898078	19.476	16.856



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066278.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 11:05
Operator : AR\AJ
Sample : PB135803BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 01:55:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

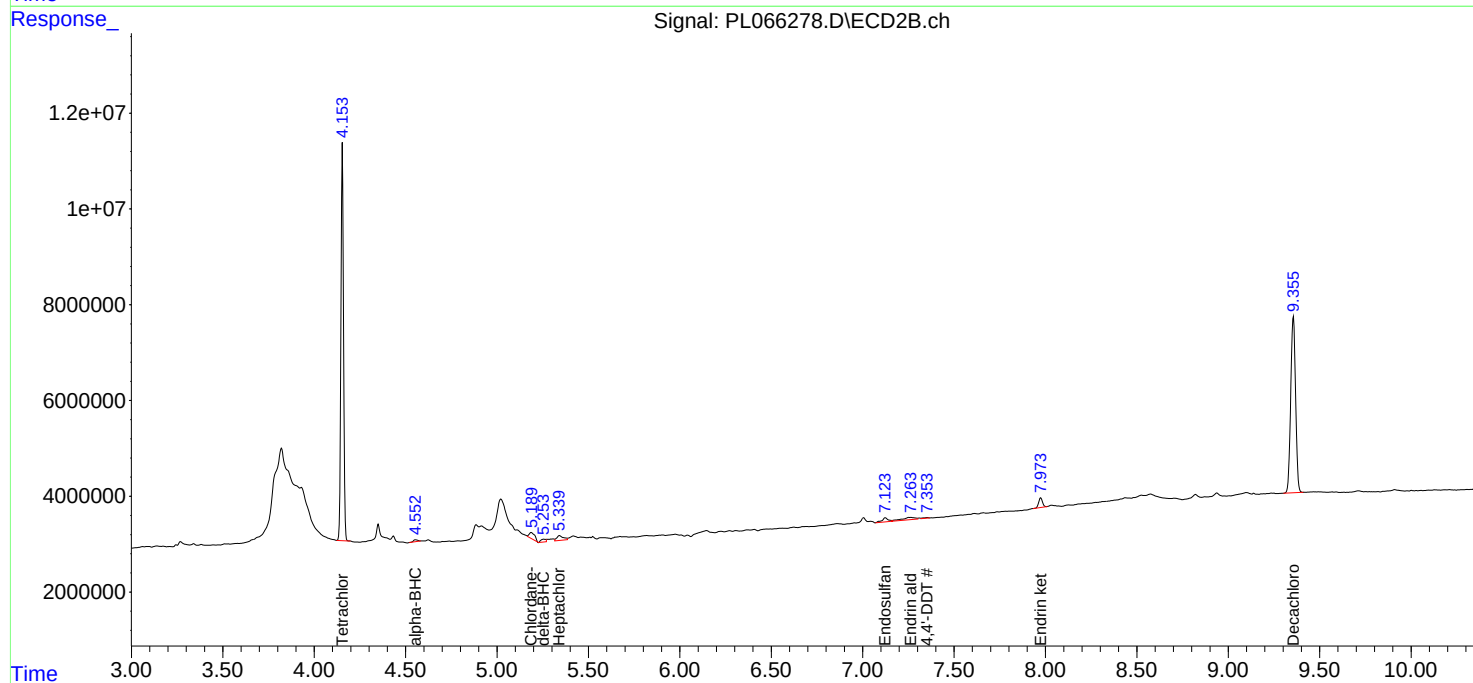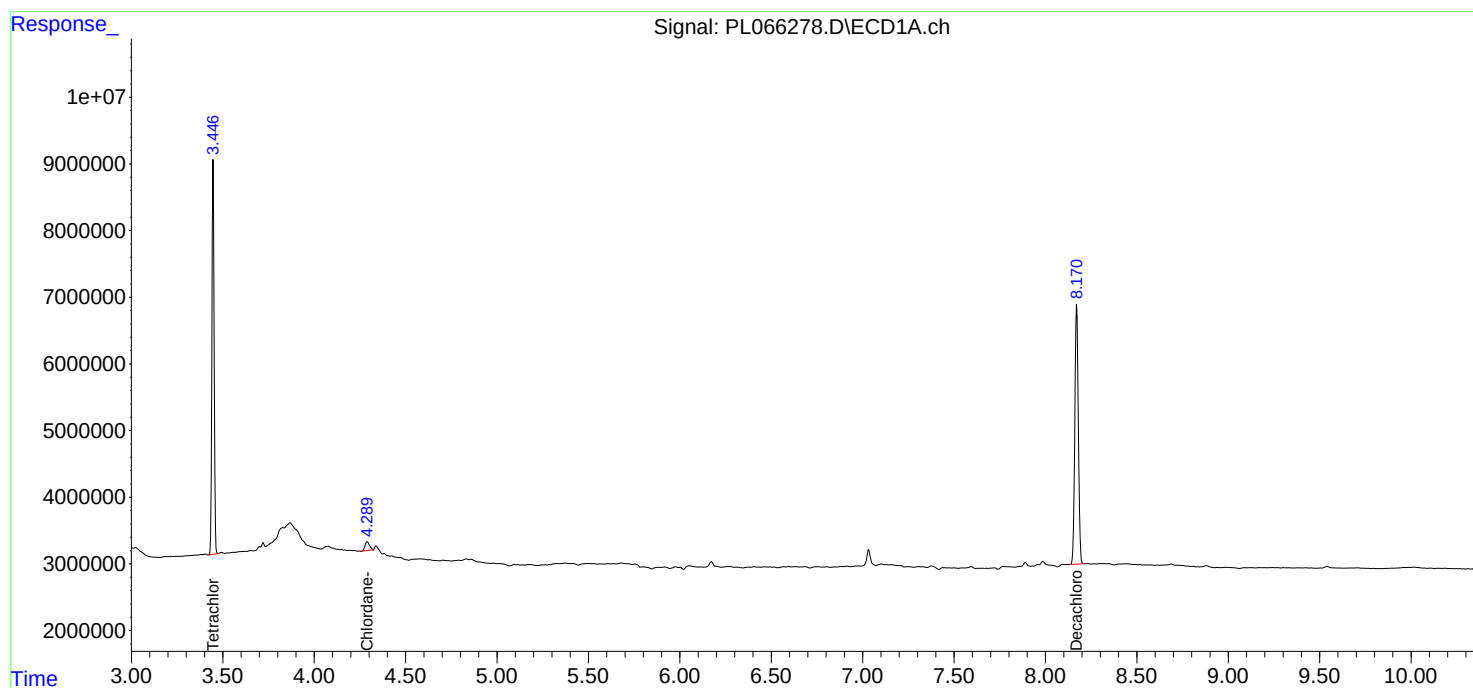


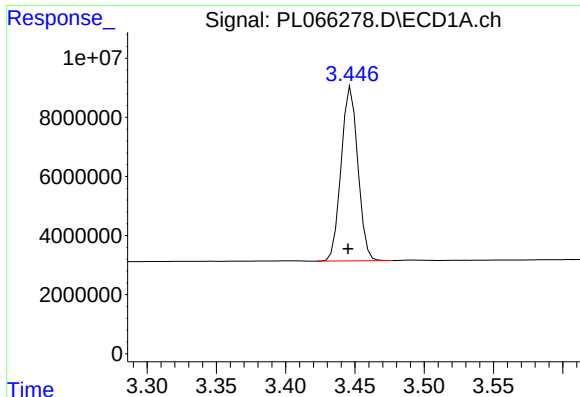

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: 0.002 min
Response: 49495235
Conc: 19.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

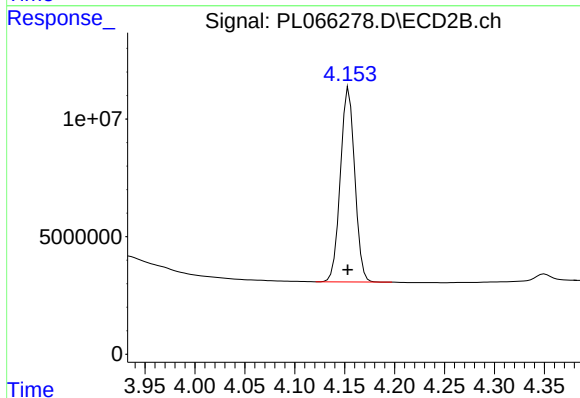


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 82702558
Conc: 20.56 ng/ml

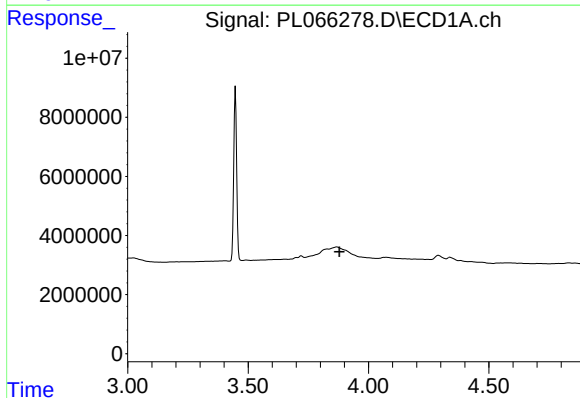


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.880 min
Response: 0
Conc: N.D.

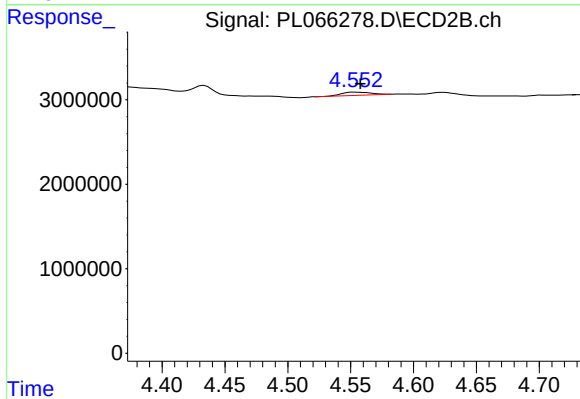

#2 alpha-BHC


R.T.: 4.554 min
Delta R.T.: -0.004 min
Response: 596789
Conc: 0.10 ng/ml

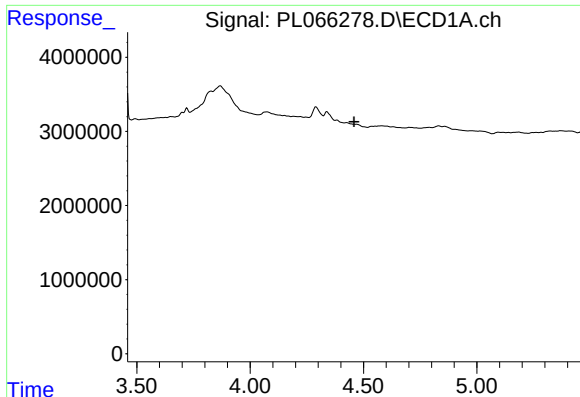

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

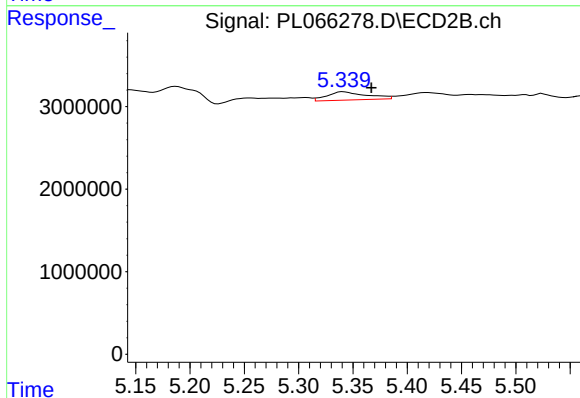


#4 Heptachlor

R.T.: 5.341 min
Delta R.T.: -0.026 min
Response: 2559745
Conc: 0.46 ng/ml

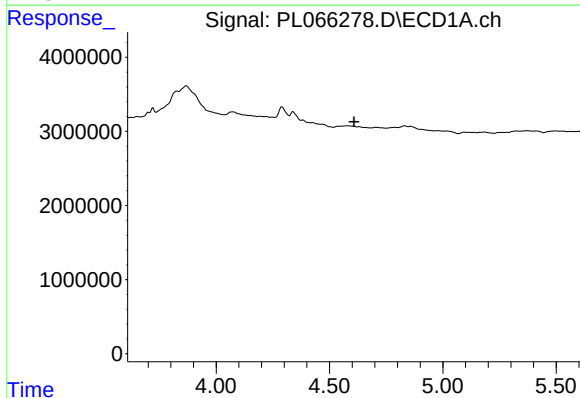


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.608 min
Response: 0
Conc: N.D.

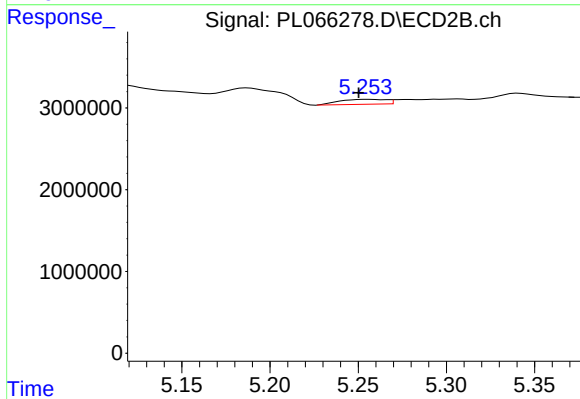

#7 delta-BHC


R.T.: 5.255 min
Delta R.T.: 0.005 min
Response: 1119831
Conc: 0.22 ng/ml

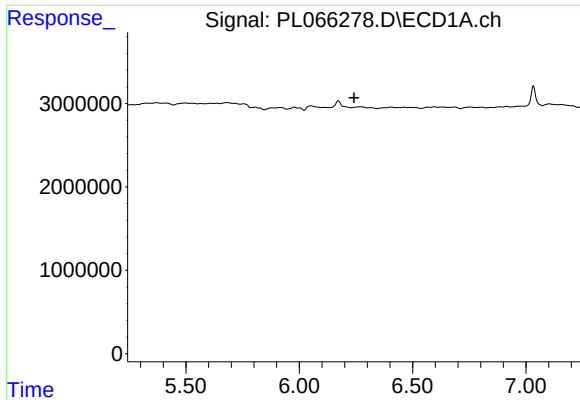

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

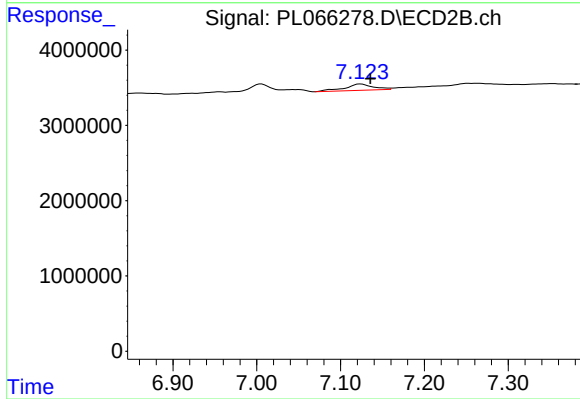


#15 Endosulfan II

R.T.: 7.124 min
Delta R.T.: -0.011 min
Response: 1963884
Conc: 0.56 ng/ml

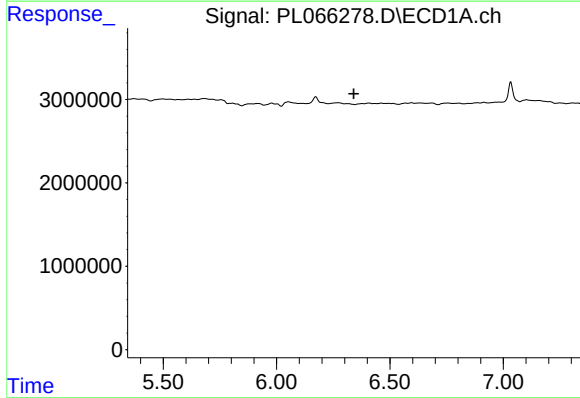


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

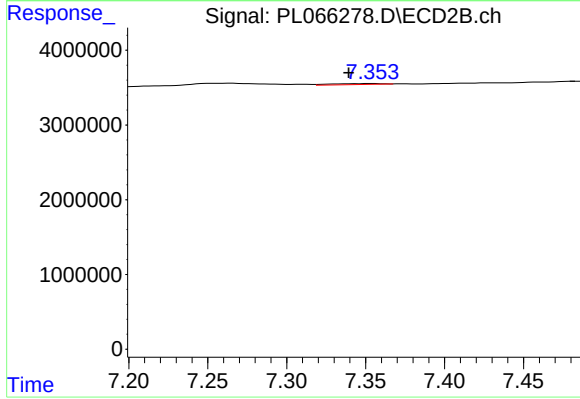

#17 4,4'-DDT


R.T.: 7.354 min
Delta R.T.: 0.015 min
Response: 275609
Conc: 0.08 ng/ml

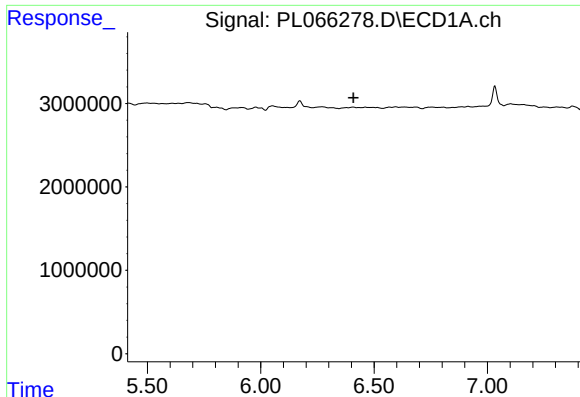

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

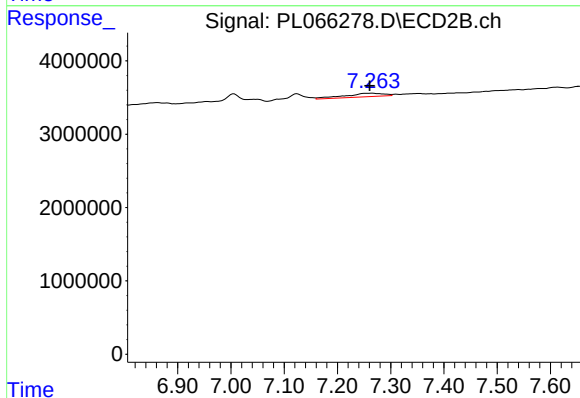


#18 Endrin aldehyde

R.T.: 7.264 min
Delta R.T.: 0.003 min
Response: 2442051
Conc: 0.87 ng/ml

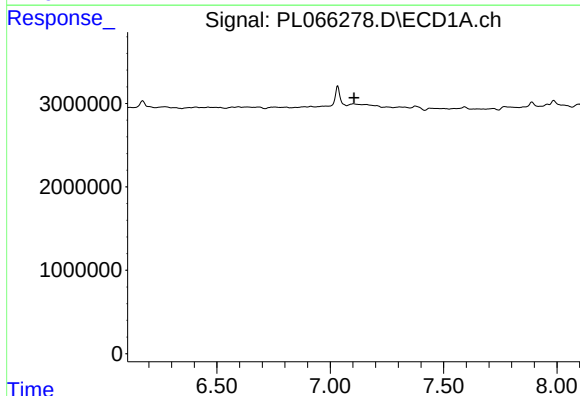


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

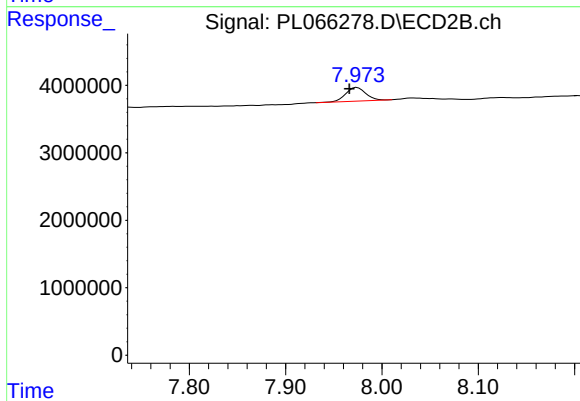

#21 Endrin ketone


R.T.: 7.974 min
Delta R.T.: 0.008 min
Response: 2980254
Conc: 0.81 ng/ml

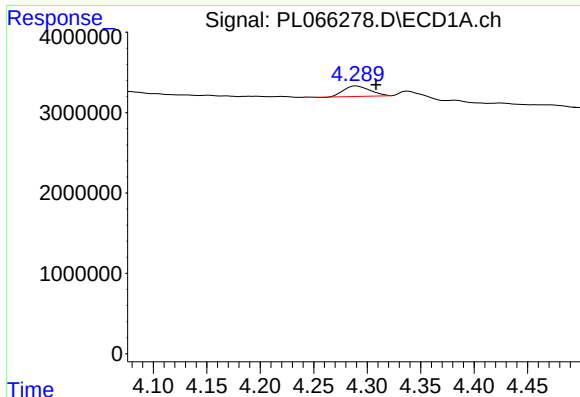

#23 Chlordane-1


R.T.: 4.290 min
Delta R.T.: -0.018 min
Response: 2226491
Conc: 19.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

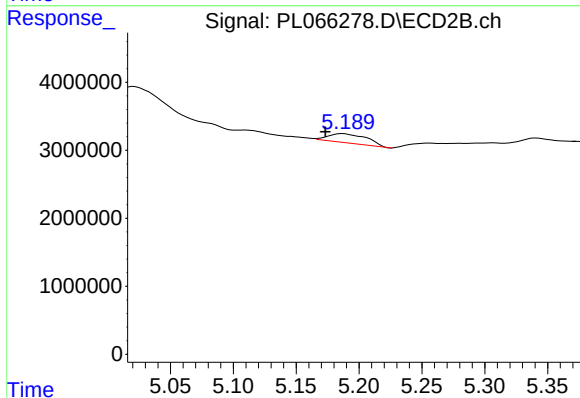


#23 Chlordane-1

R.T.: 5.187 min
Delta R.T.: 0.014 min
Response: 2898078
Conc: 16.86 ng/ml

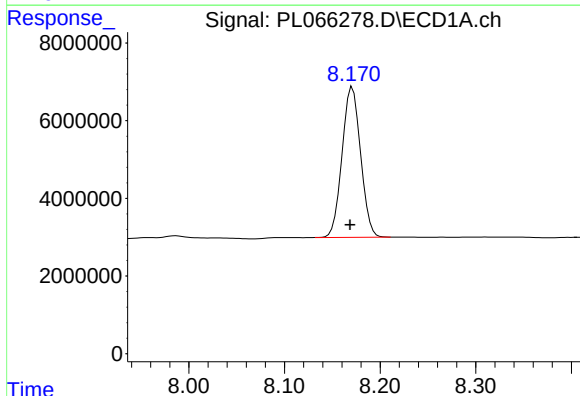

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.003 min
Response: 52272004
Conc: 21.91 ng/ml

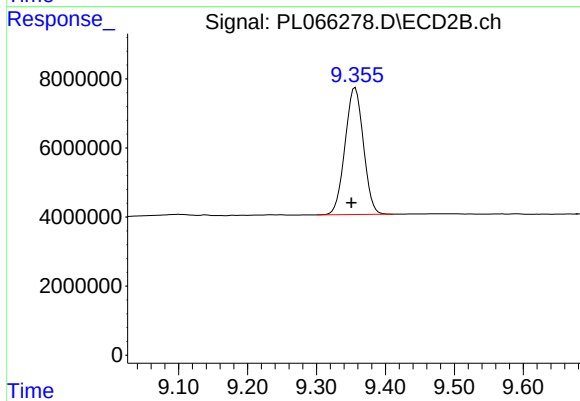

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.005 min
Response: 67945605
Conc: 20.80 ng/ml