

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 17:00
 Operator : AR\AJ
 Sample : PB135821BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:08:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.452	4.155	41098067	69678266	16.147	17.322
28)	SA Decachlor...	8.178	9.359	44797639	58840197	18.781	18.017
Target Compounds							
4)	MA Heptachlor	0.000	5.374	0	5011517	N.D.	0.900 #
7)	B delta-BHC	0.000	5.261	0	3948607	N.D.	0.768 #
14)	MA Endrin	0.000	6.950f	0	66172	N.D.	0.020 #
15)	B Endosulfa...	0.000	7.121	0	4036768	N.D.	1.158 #
17)	MA 4,4'-DDT	0.000	7.346	0	1826804	N.D.	0.539 #
18)	B Endrin al...	0.000	7.244f	0	509181	N.D.	0.182 #
21)	B Endrin ke...	0.000	7.974	0	7642480	N.D.	2.077 #
22)	Mirex	0.000	8.438f	0	1229185	N.D.	0.434 #
24)	Chlordane-2	0.000	5.639	0	2165074	N.D.	12.306 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 17:00
Operator : AR\AJ
Sample : PB135821BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:08:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

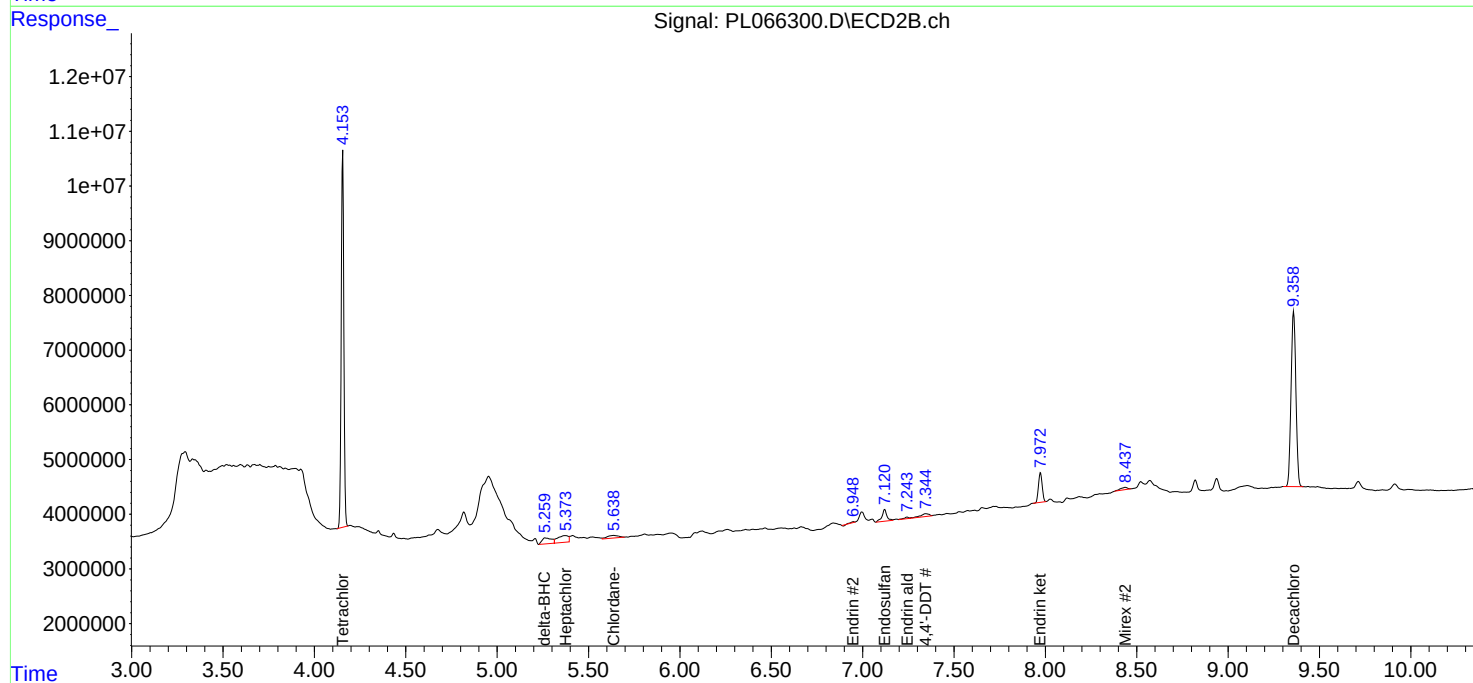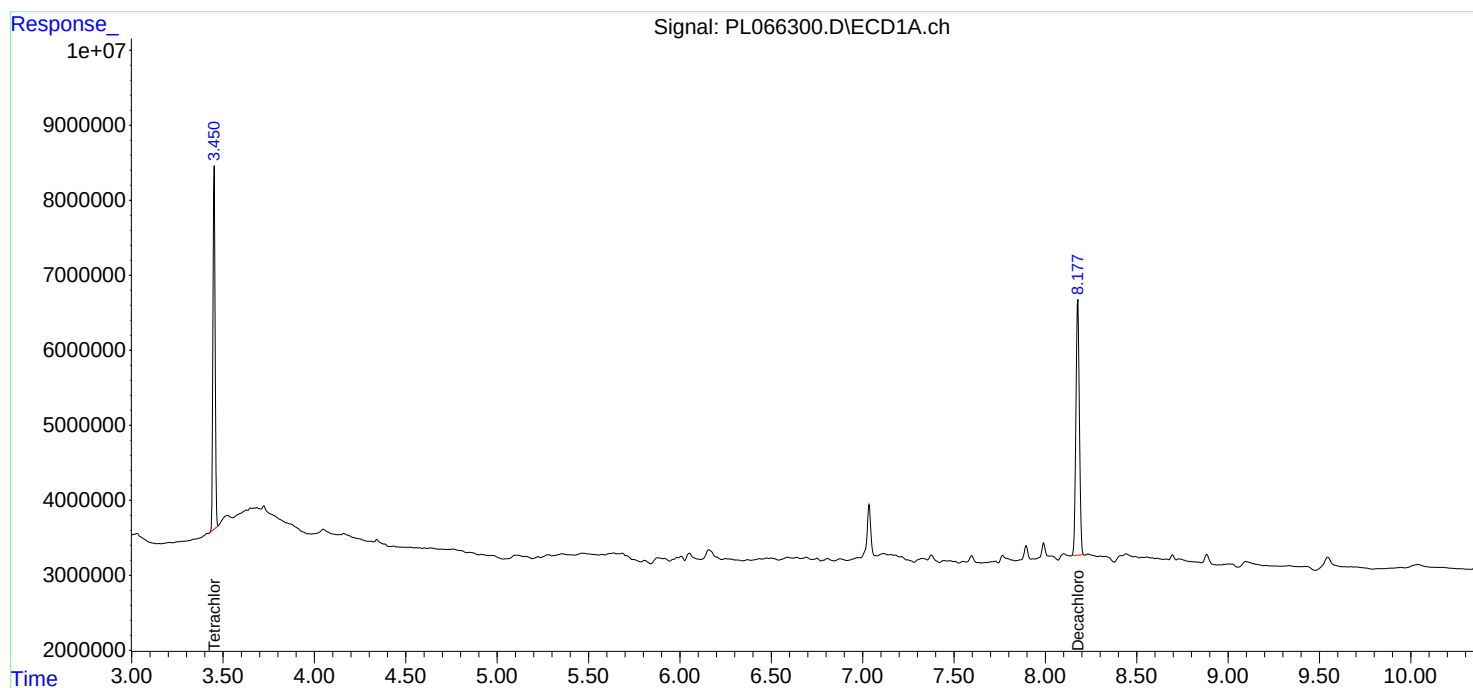


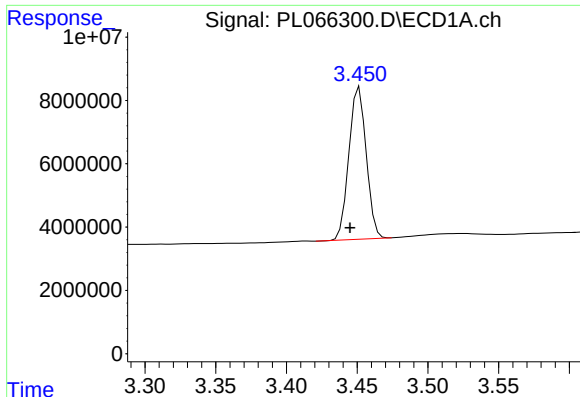

#1 Tetrachloro-m-xylene


R.T.: 3.452 min
Delta R.T.: 0.007 min
Response: 41098067
Conc: 16.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

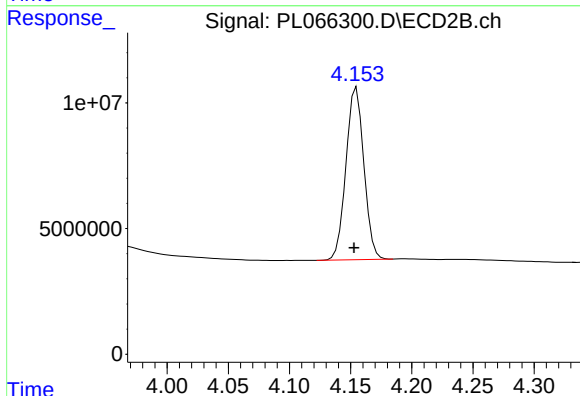


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 69678266
Conc: 17.32 ng/ml

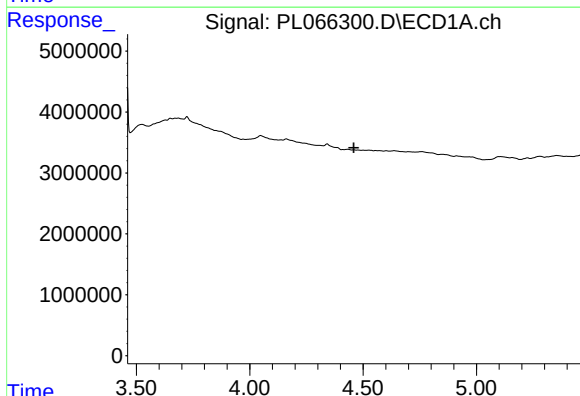


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

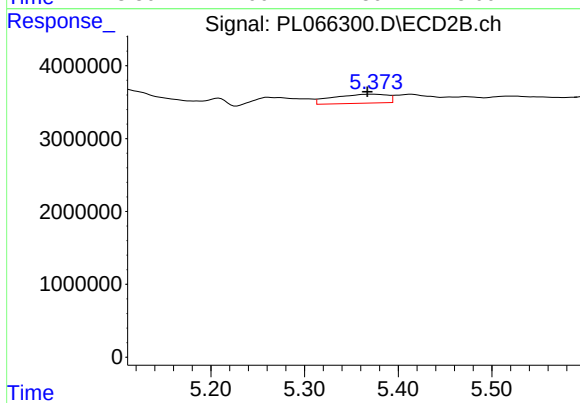

#4 Heptachlor


R.T.: 5.374 min
Delta R.T.: 0.007 min
Response: 5011517
Conc: 0.90 ng/ml

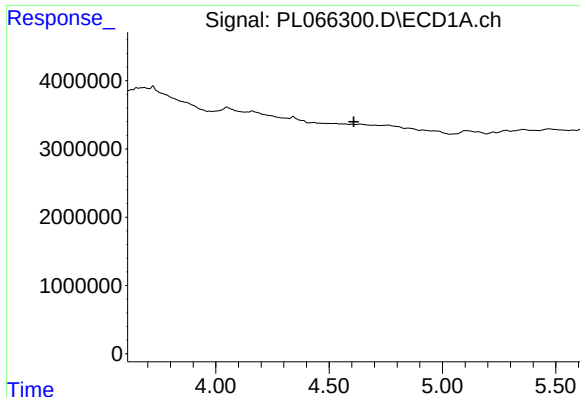

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

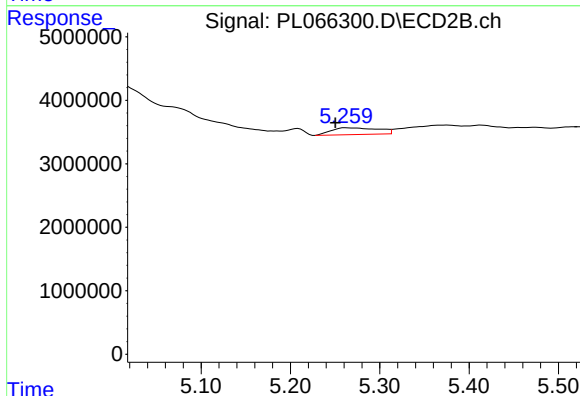


#7 delta-BHC

R.T.: 5.261 min
Delta R.T.: 0.011 min
Response: 3948607
Conc: 0.77 ng/ml

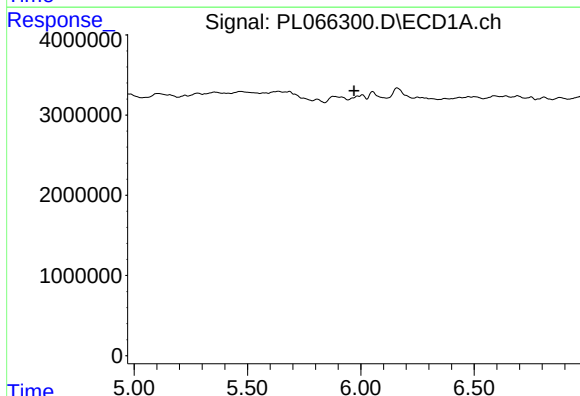


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

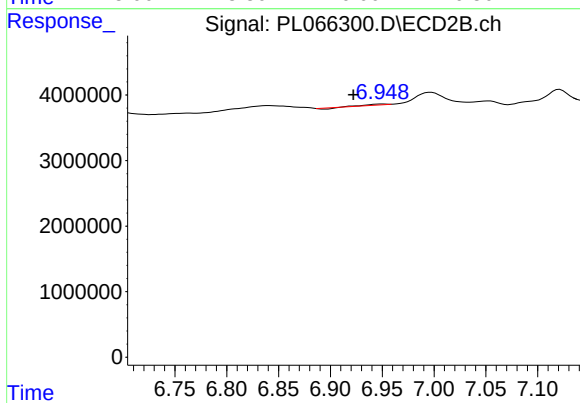

#14 Endrin


R.T.: 6.950 min
Delta R.T.: 0.028 min
Response: 66172
Conc: 0.02 ng/ml

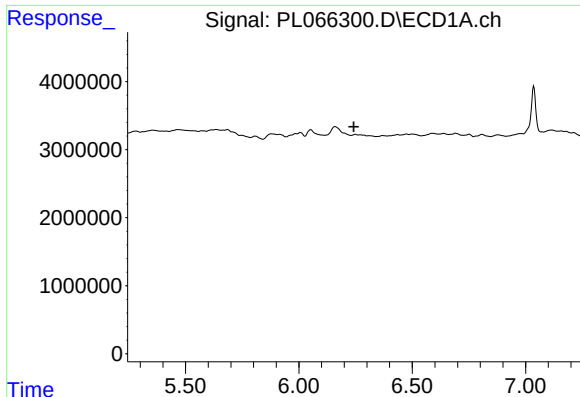

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

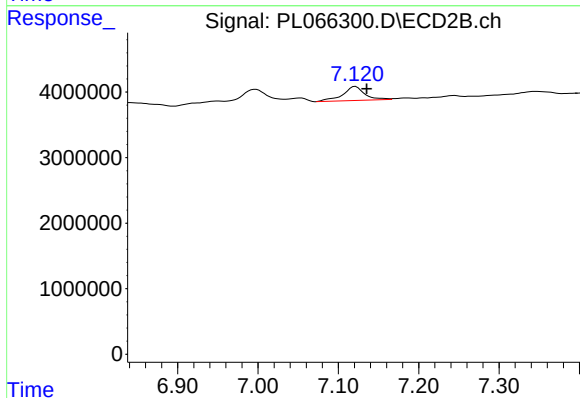


#15 Endosulfan II

R.T.: 7.121 min
Delta R.T.: -0.014 min
Response: 4036768
Conc: 1.16 ng/ml

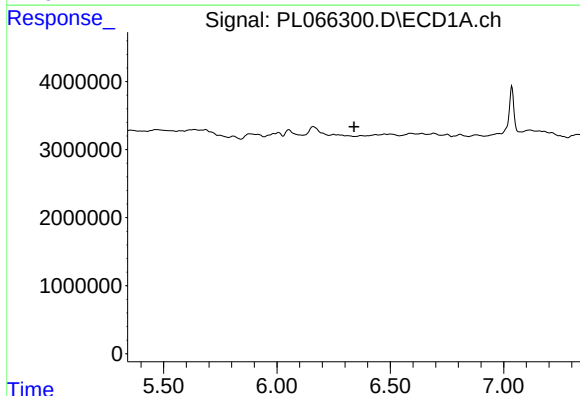


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

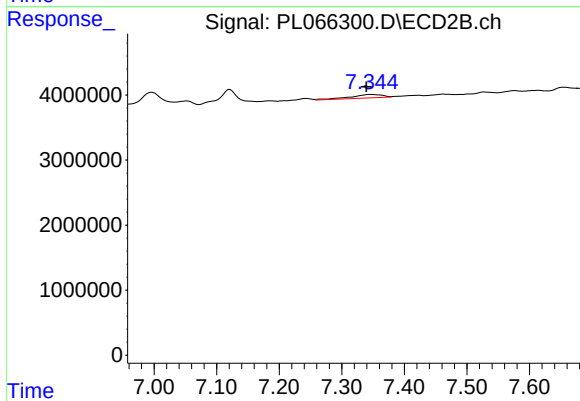

#17 4,4'-DDT


R.T.: 7.346 min
Delta R.T.: 0.006 min
Response: 1826804
Conc: 0.54 ng/ml

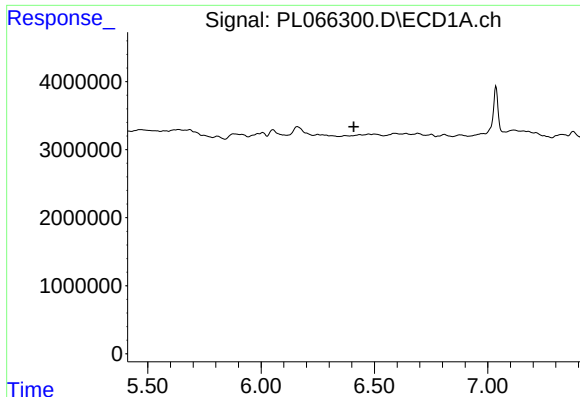

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

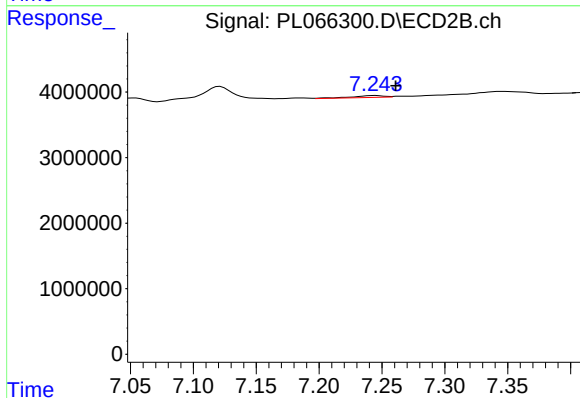


#18 Endrin aldehyde

R.T.: 7.244 min
Delta R.T.: -0.017 min
Response: 509181
Conc: 0.18 ng/ml

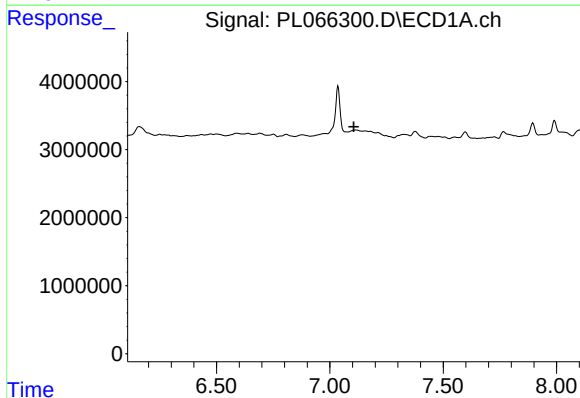


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

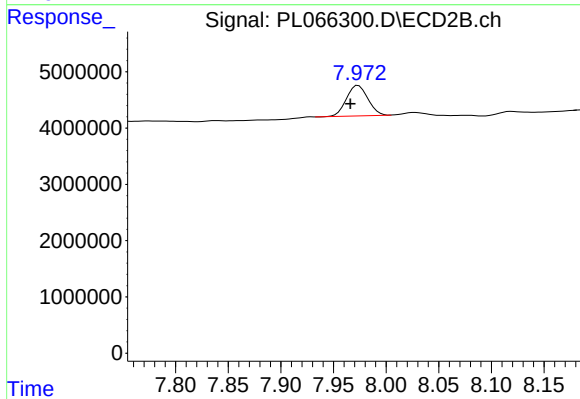

#21 Endrin ketone


R.T.: 7.974 min
Delta R.T.: 0.007 min
Response: 7642480
Conc: 2.08 ng/ml

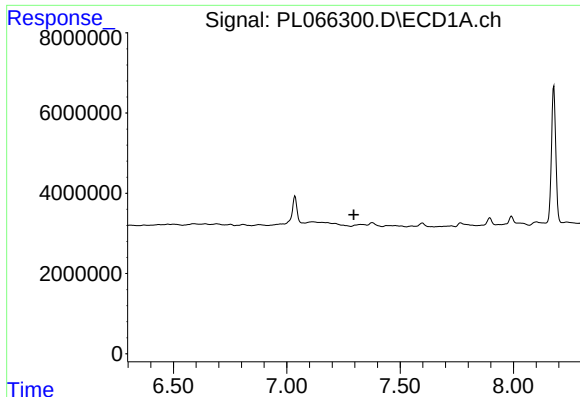

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

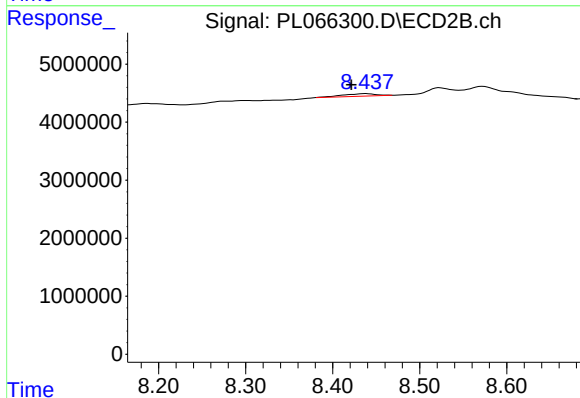


#22 Mirex

R.T.: 8.438 min
Delta R.T.: 0.017 min
Response: 1229185
Conc: 0.43 ng/ml

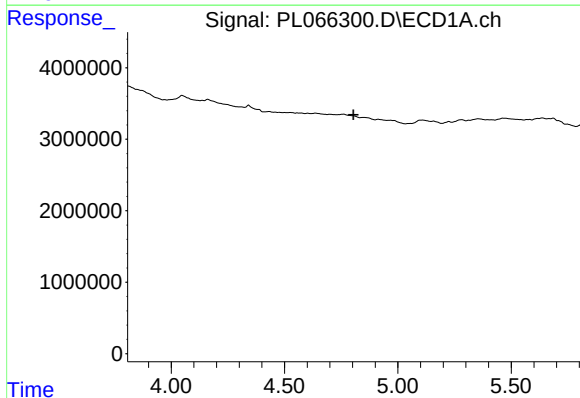


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.805 min
Response: 0
Conc: N.D.

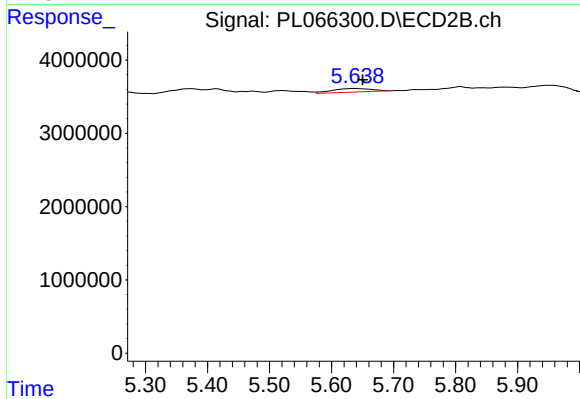

#24 Chlordane-2


R.T.: 5.639 min
Delta R.T.: -0.011 min
Response: 2165074
Conc: 12.31 ng/ml

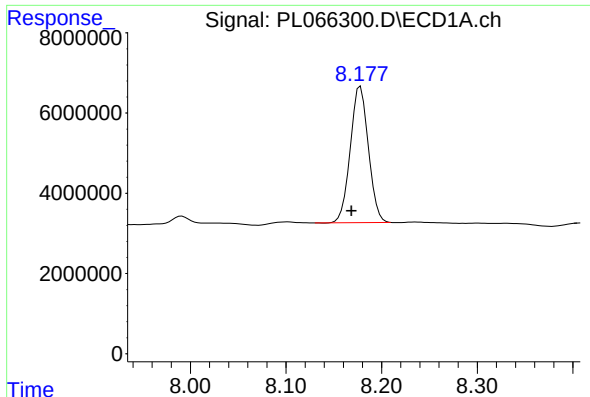

#28 Decachlorobiphenyl

R.T.: 8.178 min
Delta R.T.: 0.009 min
Response: 44797639
Conc: 18.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

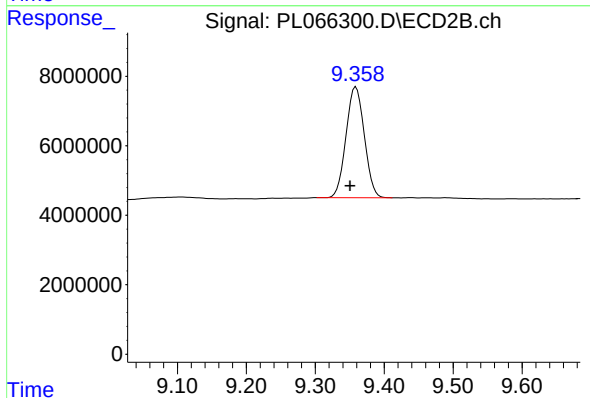

#28 Decachlorobiphenyl

R.T.: 9.359 min
Delta R.T.: 0.008 min
Response: 58840197
Conc: 18.02 ng/ml