

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 19:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:12:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.154	46904352	79056340	18.428	19.653
28)	SA Decachlor...	8.168	9.354	50246613	65039799	21.065	19.915
Target Compounds							
4)	MA Heptachlor	0.000	5.352	0	2488280	N.D.	0.447 #
5)	MB Aldrin	0.000	5.670	0	148610	N.D.	0.030 #
15)	B Endosulfa...	0.000	7.125	0	1951650	N.D.	0.560 #
17)	MA 4,4'-DDT	0.000	7.346	0	897533	N.D.	0.265 #
18)	B Endrin al...	0.000	7.259	0	873317	N.D.	0.312 #
21)	B Endrin ke...	0.000	7.974	0	1306919	N.D.	0.355 #
22)	Mirex	0.000	8.438f	0	601694	N.D.	0.213 #
23)	Chlordane-1	4.332f	0.000	2786708	0	24.376	N.D. #
24)	Chlordane-2	0.000	5.670f	0	148610	N.D.	0.845 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 19:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:12:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

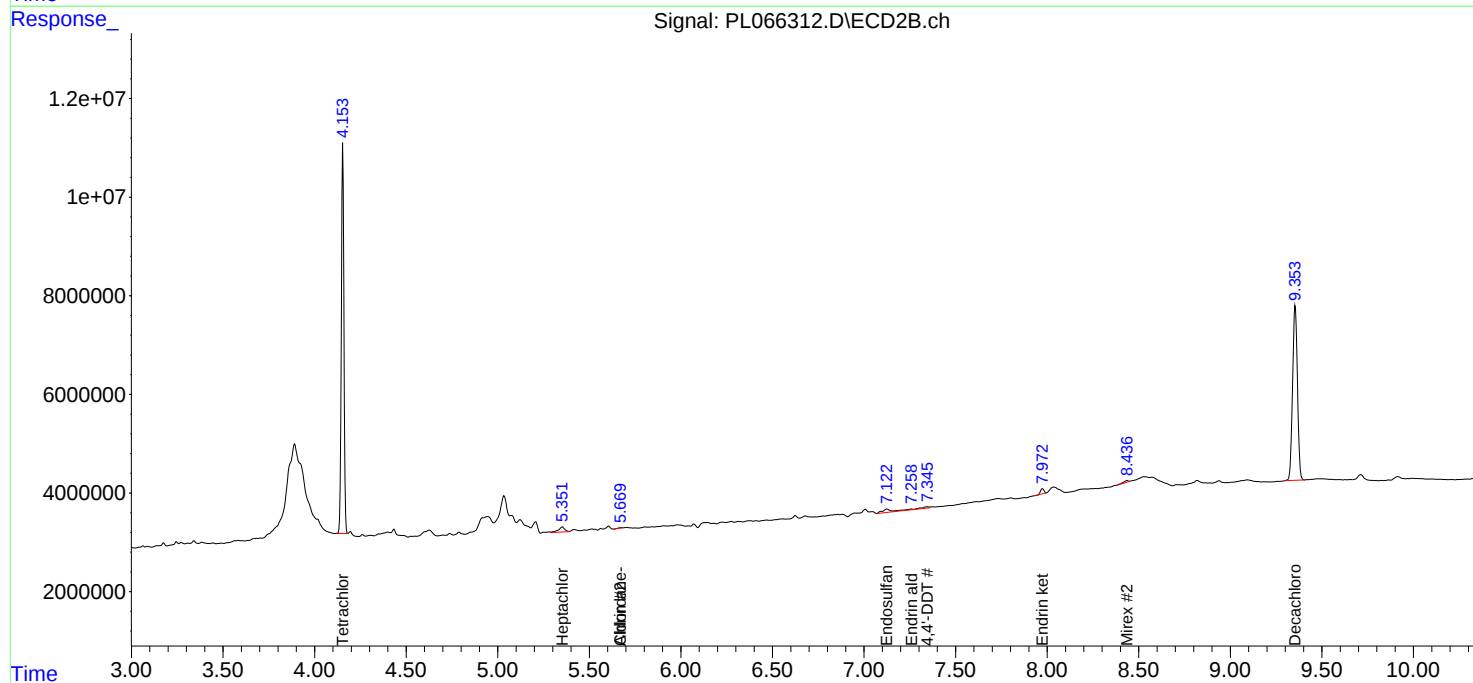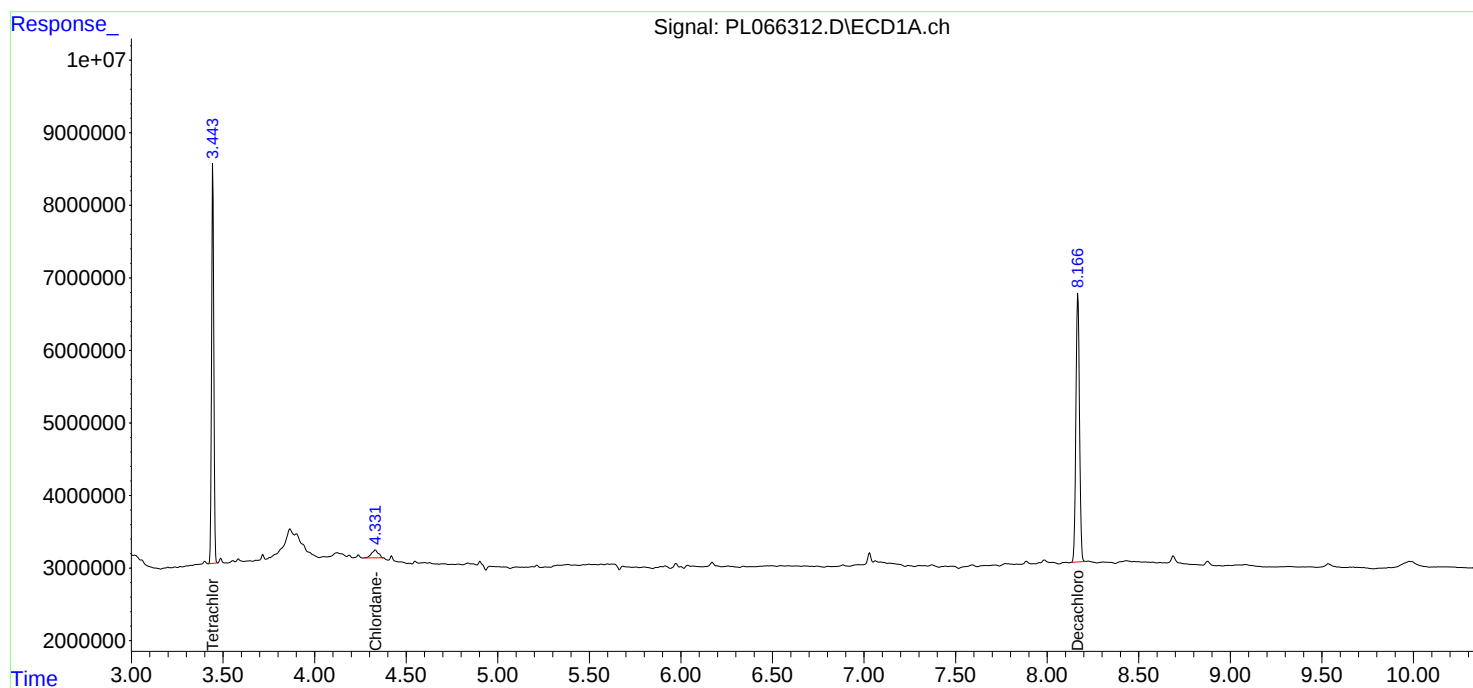


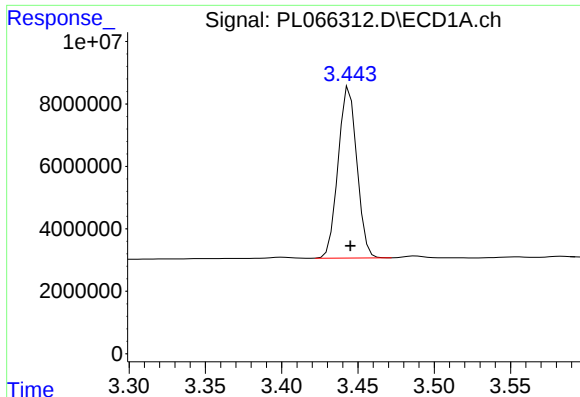

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 46904352
Conc: 18.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

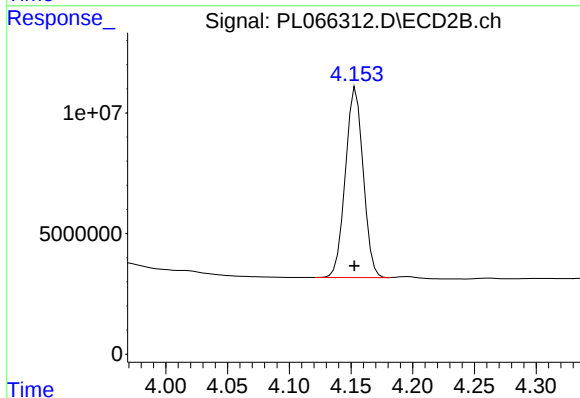


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 79056340
Conc: 19.65 ng/ml

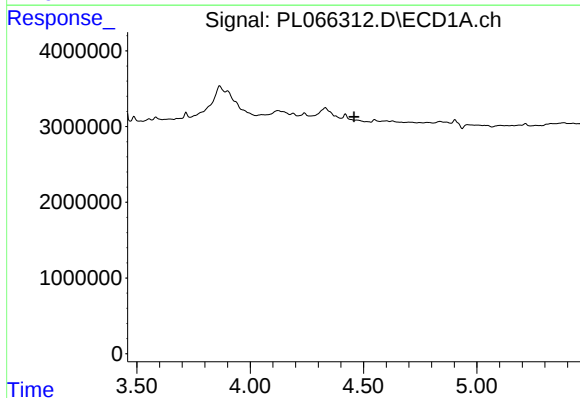


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

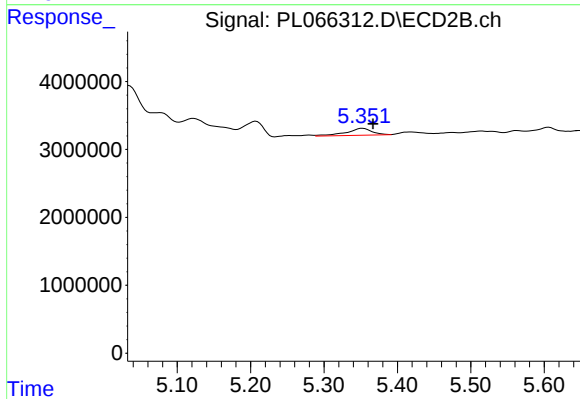

#4 Heptachlor


R.T.: 5.352 min
Delta R.T.: -0.015 min
Response: 2488280
Conc: 0.45 ng/ml

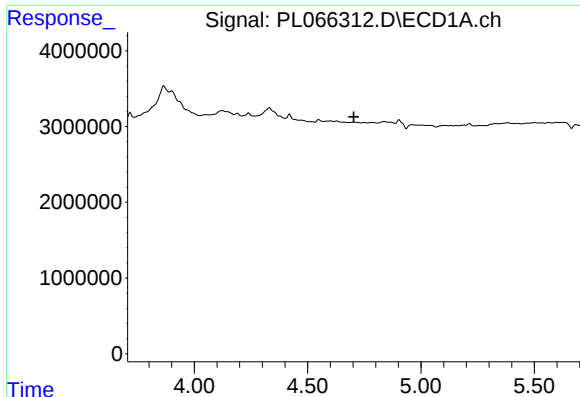

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

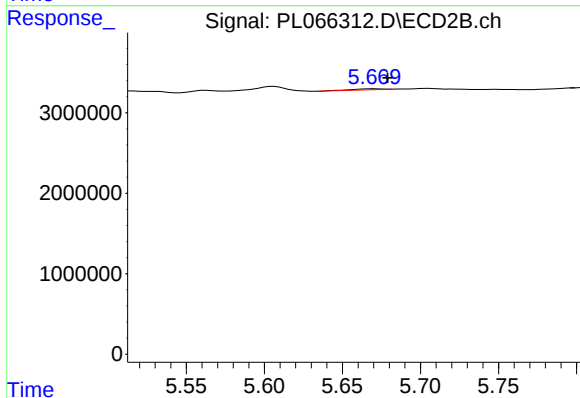


#5 Aldrin

R.T.: 5.670 min
Delta R.T.: -0.009 min
Response: 148610
Conc: 0.03 ng/ml

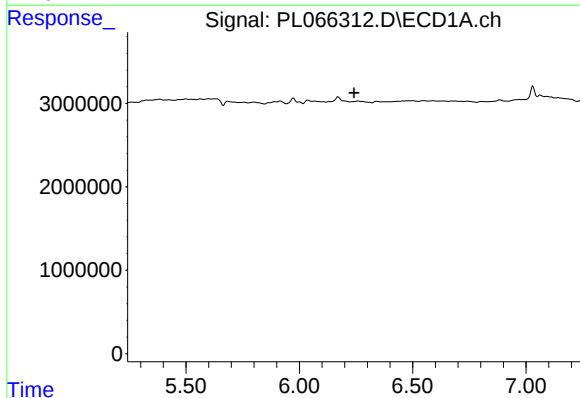


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

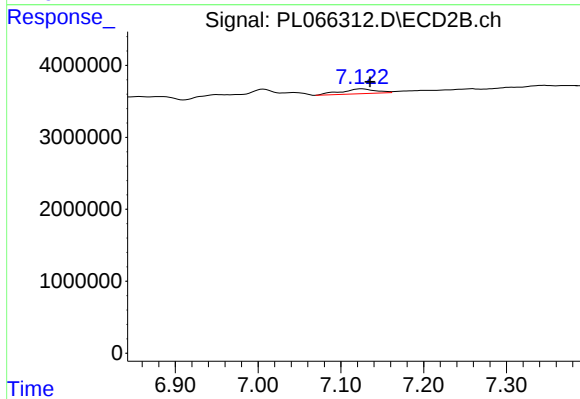

#15 Endosulfan II


R.T.: 7.125 min
Delta R.T.: -0.011 min
Response: 1951650
Conc: 0.56 ng/ml

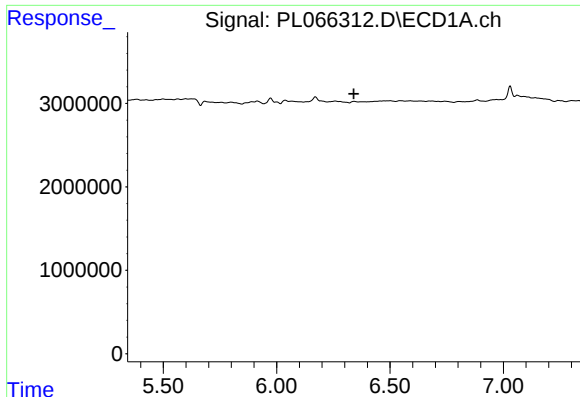

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

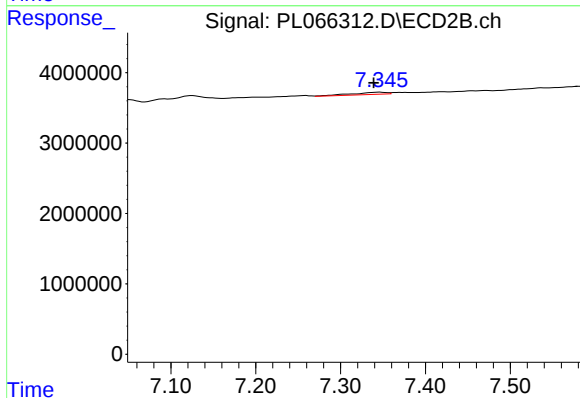


#17 4,4'-DDT

R.T.: 7.346 min
Delta R.T.: 0.007 min
Response: 897533
Conc: 0.26 ng/ml

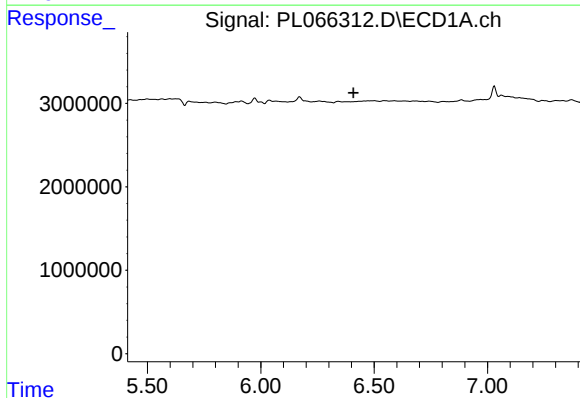


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

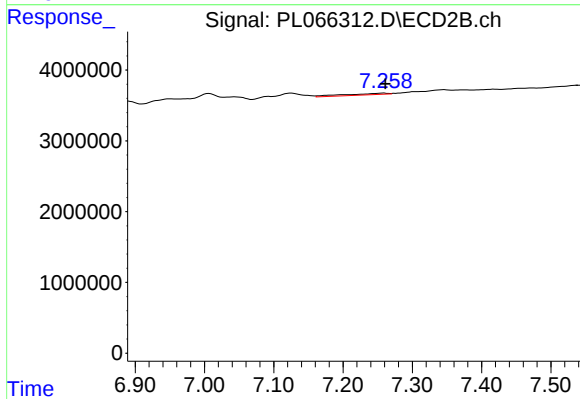

#18 Endrin aldehyde


R.T.: 7.259 min
Delta R.T.: -0.002 min
Response: 873317
Conc: 0.31 ng/ml

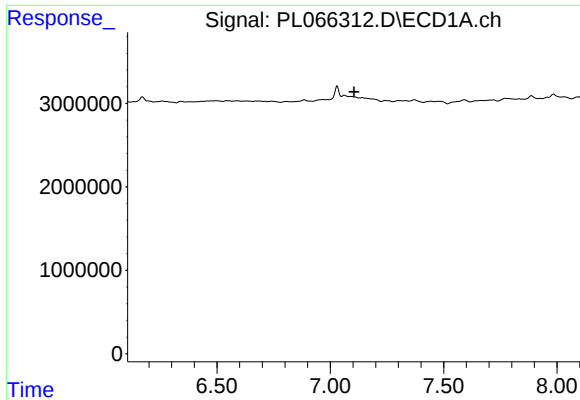

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

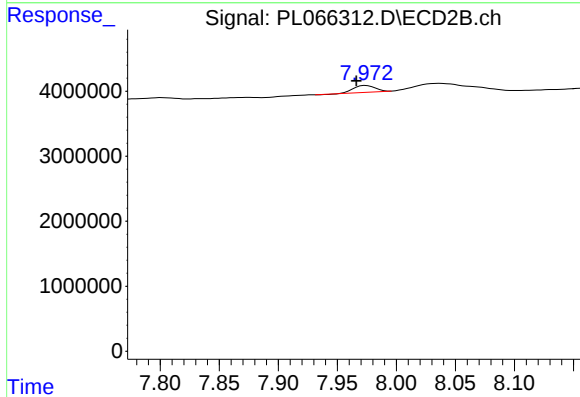


#21 Endrin ketone

R.T.: 7.974 min
Delta R.T.: 0.008 min
Response: 1306919
Conc: 0.36 ng/ml

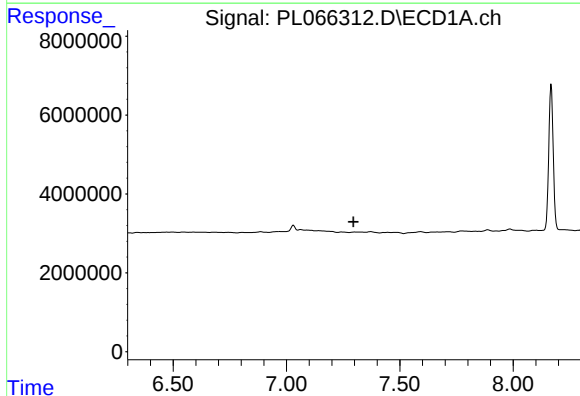


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.296 min
Response: 0
Conc: N.D.

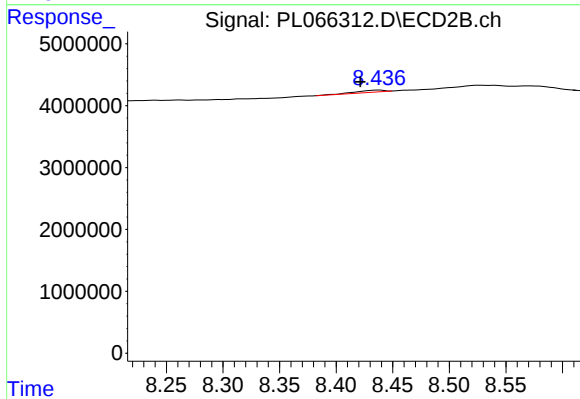

#22 Mirex


R.T.: 8.438 min
Delta R.T.: 0.017 min
Response: 601694
Conc: 0.21 ng/ml

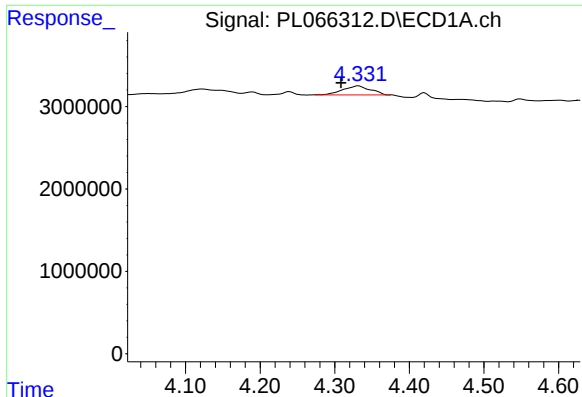

#23 Chlordane-1


R.T.: 4.332 min
Delta R.T.: 0.024 min
Response: 2786708
Conc: 24.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

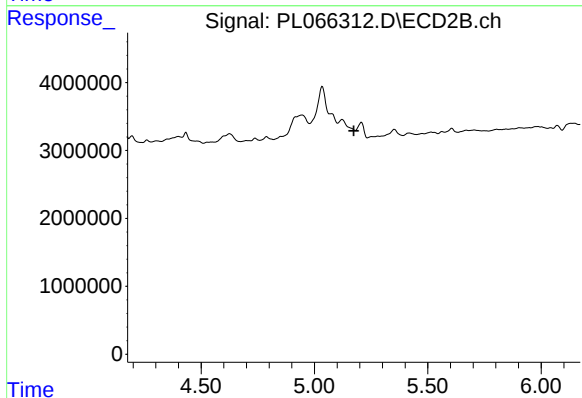


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.173 min
Response: 0
Conc: N.D.

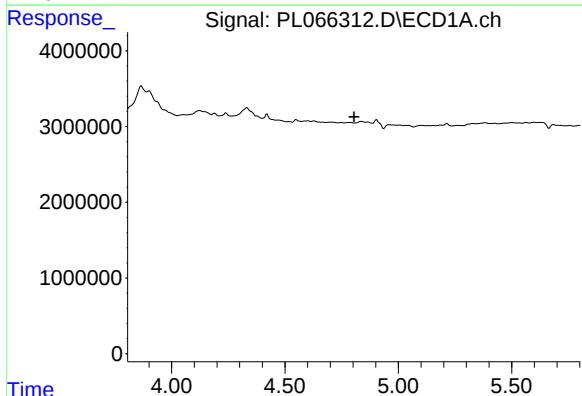


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.805 min
Response: 0
Conc: N.D.

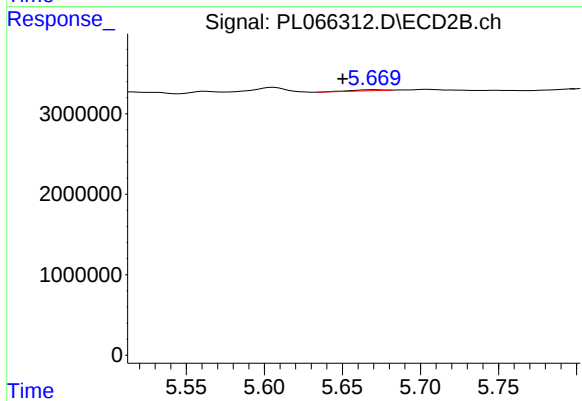

#24 Chlordane-2


R.T.: 5.670 min
Delta R.T.: 0.020 min
Response: 148610
Conc: 0.84 ng/ml

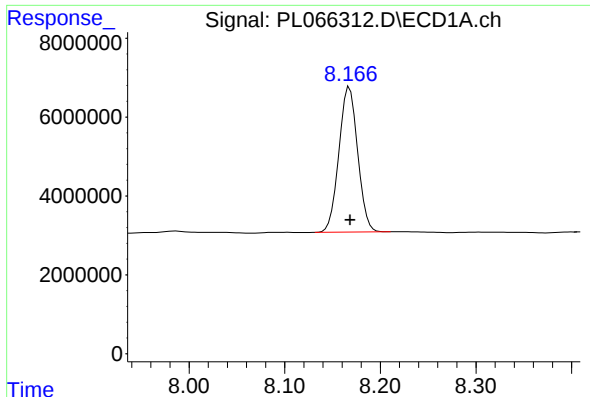

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 50246613
Conc: 21.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

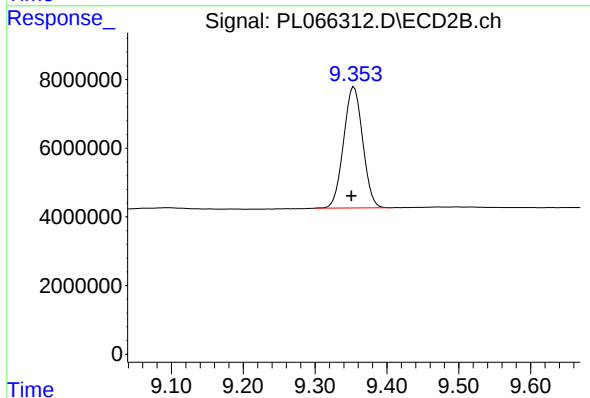

#28 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: 0.004 min
Response: 65039799
Conc: 19.91 ng/ml