

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 23:13
 Operator : AR\AJ
 Sample : PB135839BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:16:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.155	48246635	81532942	18.955	20.269
28)	SA Decachlor...	8.167	9.354	48197525	66592912	20.206	20.390
Target Compounds							
4)	MA Heptachlor	0.000	5.354	0	3034446	N.D.	0.545 #
5)	MB Aldrin	0.000	5.671	0	151208	N.D.	0.030 #
8)	B Heptachlo...	0.000	6.046f	0	54409	N.D.	0.012 #
15)	B Endosulfa...	0.000	7.125	0	1722310	N.D.	0.494 #
21)	B Endrin ke...	0.000	7.974	0	1939372	N.D.	0.527 #
22)	Mirex	0.000	8.437f	0	183031	N.D.	0.065 #
23)	Chlordane-1	4.330f	0.000	2430721	0	21.262	N.D. #
24)	Chlordane-2	0.000	5.671f	0	151208	N.D.	0.859 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 23:13
Operator : AR\AJ
Sample : PB135839BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:16:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

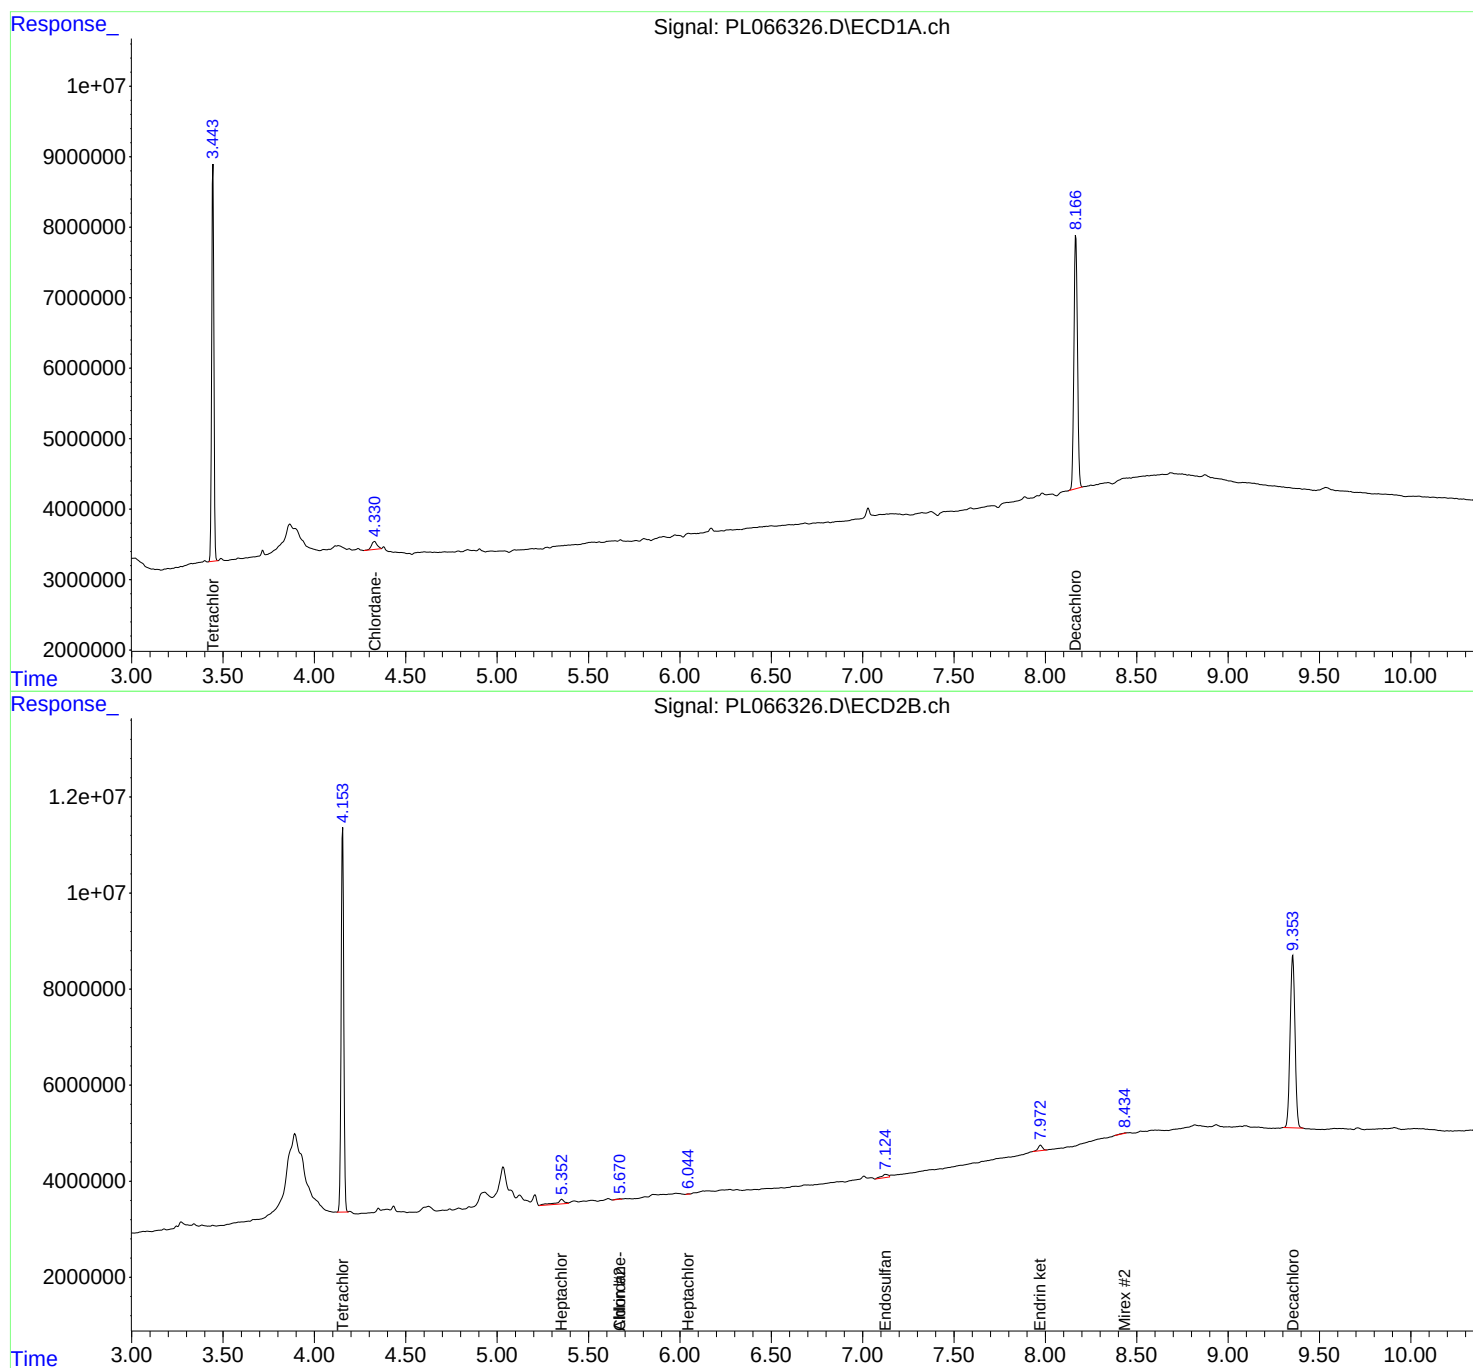


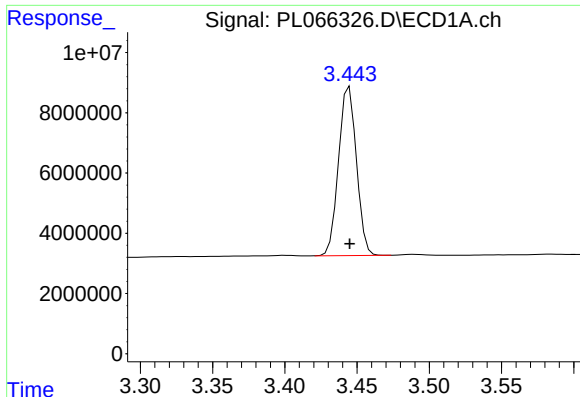

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 48246635
Conc: 18.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

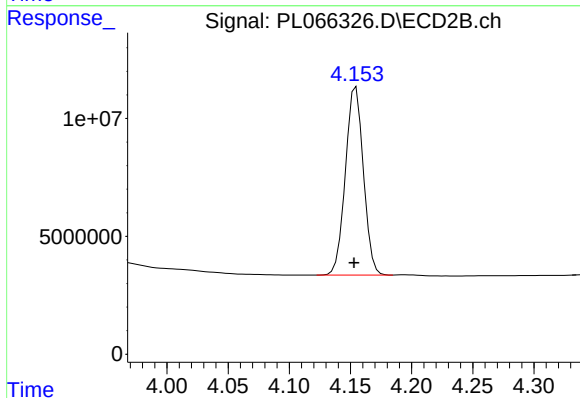


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 81532942
Conc: 20.27 ng/ml

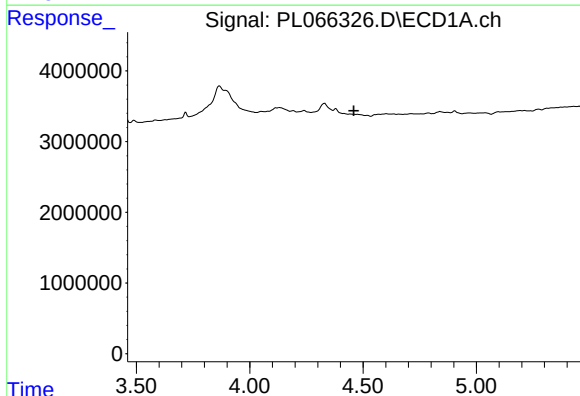


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

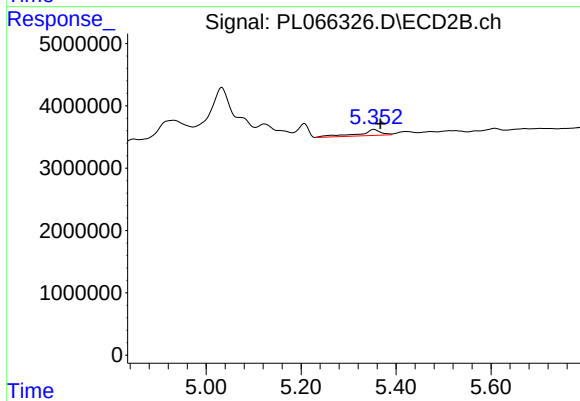

#4 Heptachlor


R.T.: 5.354 min
Delta R.T.: -0.013 min
Response: 3034446
Conc: 0.55 ng/ml

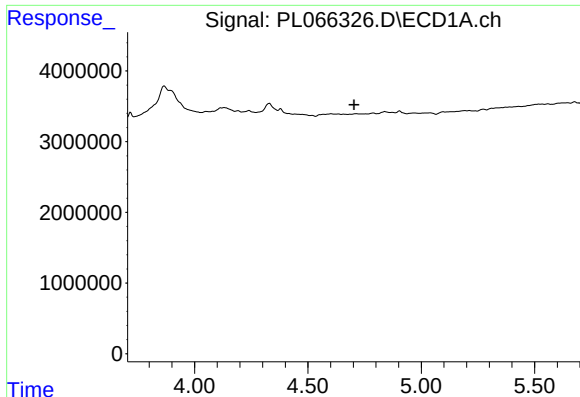

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

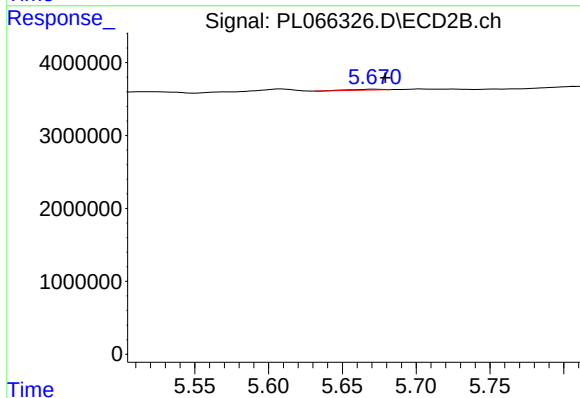


#5 Aldrin

R.T.: 5.671 min
Delta R.T.: -0.008 min
Response: 151208
Conc: 0.03 ng/ml

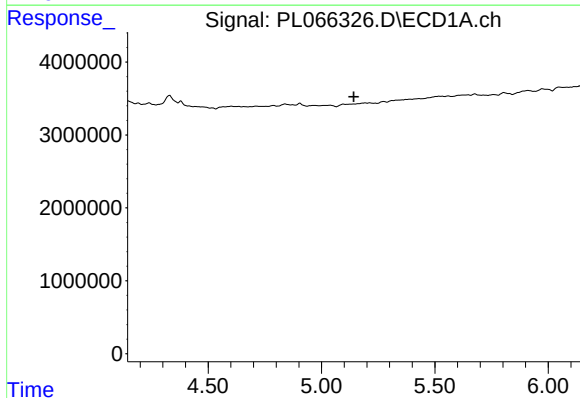


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.143 min
Response: 0
Conc: N.D.

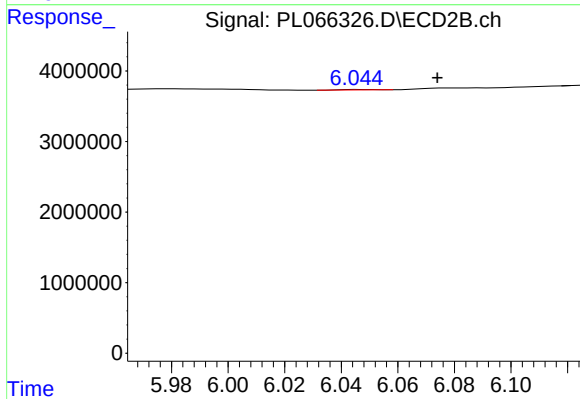

#8 Heptachlor epoxide


R.T.: 6.046 min
Delta R.T.: -0.028 min
Response: 54409
Conc: 0.01 ng/ml

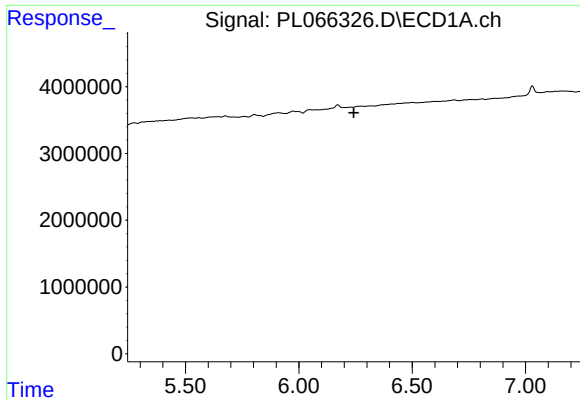

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

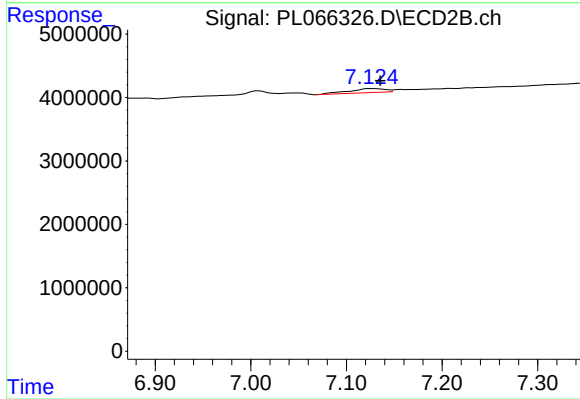


#15 Endosulfan II

R.T.: 7.125 min
Delta R.T.: -0.010 min
Response: 1722310
Conc: 0.49 ng/ml

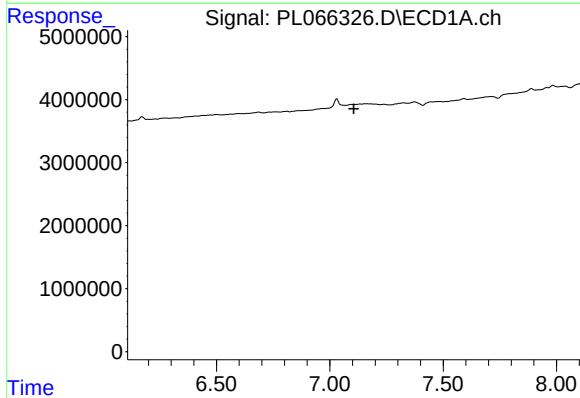


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

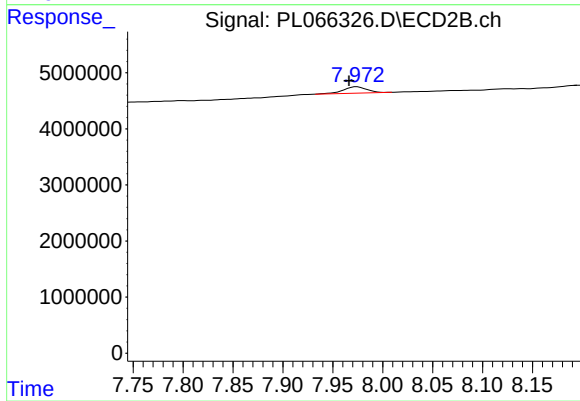

#21 Endrin ketone


R.T.: 7.974 min
Delta R.T.: 0.008 min
Response: 1939372
Conc: 0.53 ng/ml

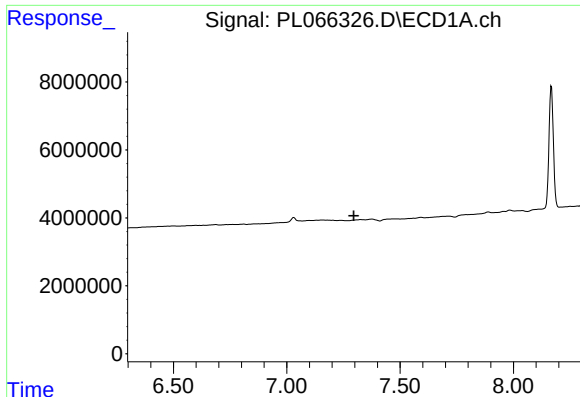

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

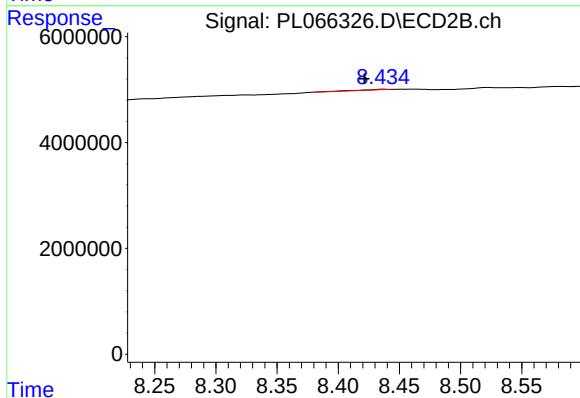


#22 Mirex

R.T.: 8.437 min
Delta R.T.: 0.016 min
Response: 183031
Conc: 0.06 ng/ml

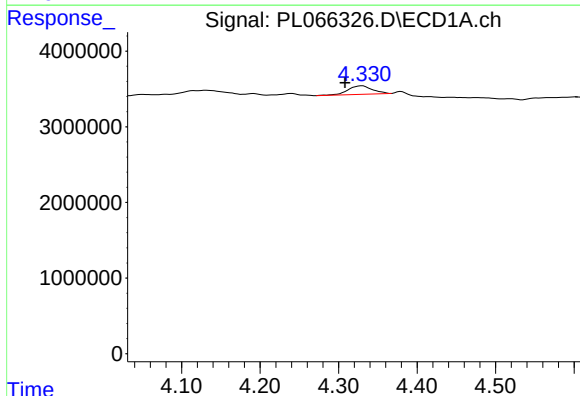


#23 Chlordane-1

R.T.: 4.330 min
Delta R.T.: 0.022 min
Response: 2430721
Conc: 21.26 ng/ml

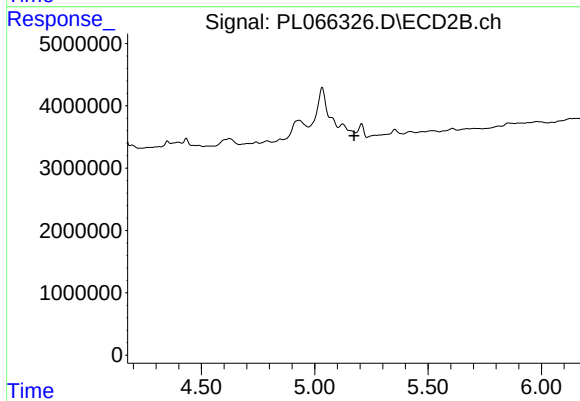

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.173 min
Response: 0
Conc: N.D.

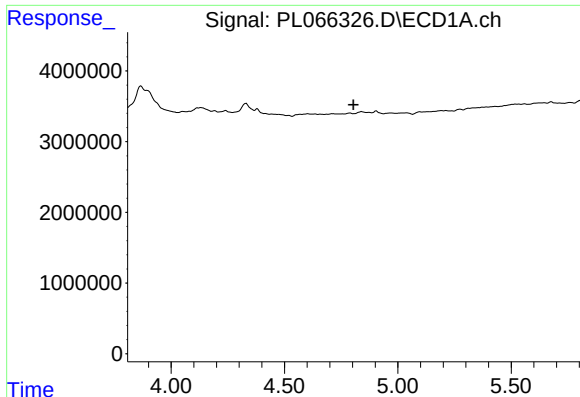

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.805 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

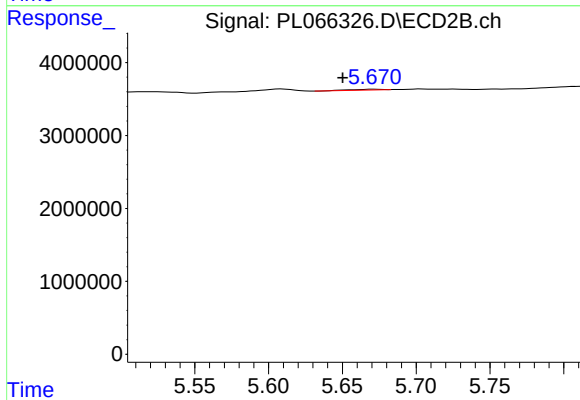


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.021 min
Response: 151208
Conc: 0.86 ng/ml

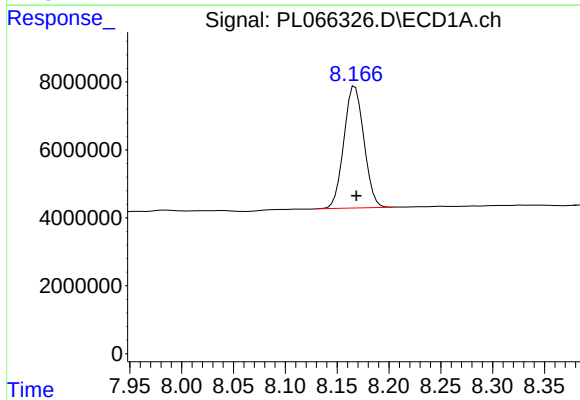

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: -0.001 min
Response: 48197525
Conc: 20.21 ng/ml

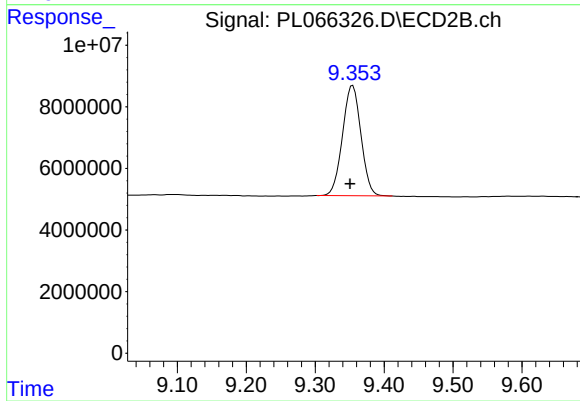

#28 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: 0.004 min
Response: 66592912
Conc: 20.39 ng/ml