

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 00:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:17:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.154	47330345	77615131	18.595	19.295
28)	SA Decachlor...	8.168	9.354	47646286	63471655	19.975	19.435
Target Compounds							
4)	MA Heptachlor	0.000	5.353	0	2410260	N.D.	0.433 #
8)	B Heptachlo...	0.000	6.068	0	8216477	N.D.	1.779 #
12)	B 4,4'-DDE	0.000	6.553	0	322567	N.D.	0.078 #
14)	MA Endrin	5.974	0.000	1159266	0	0.332	N.D. #
15)	B Endosulfa...	0.000	7.128	0	2197658	N.D.	0.630 #
17)	MA 4,4'-DDT	0.000	7.343	0	539448	N.D.	0.159 #
18)	B Endrin al...	0.000	7.257	0	989818	N.D.	0.354 #
21)	B Endrin ke...	0.000	7.973	0	1832631	N.D.	0.498 #
23)	Chlordane-1	4.332f	0.000	2589044	0	22.647	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 00:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:17:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

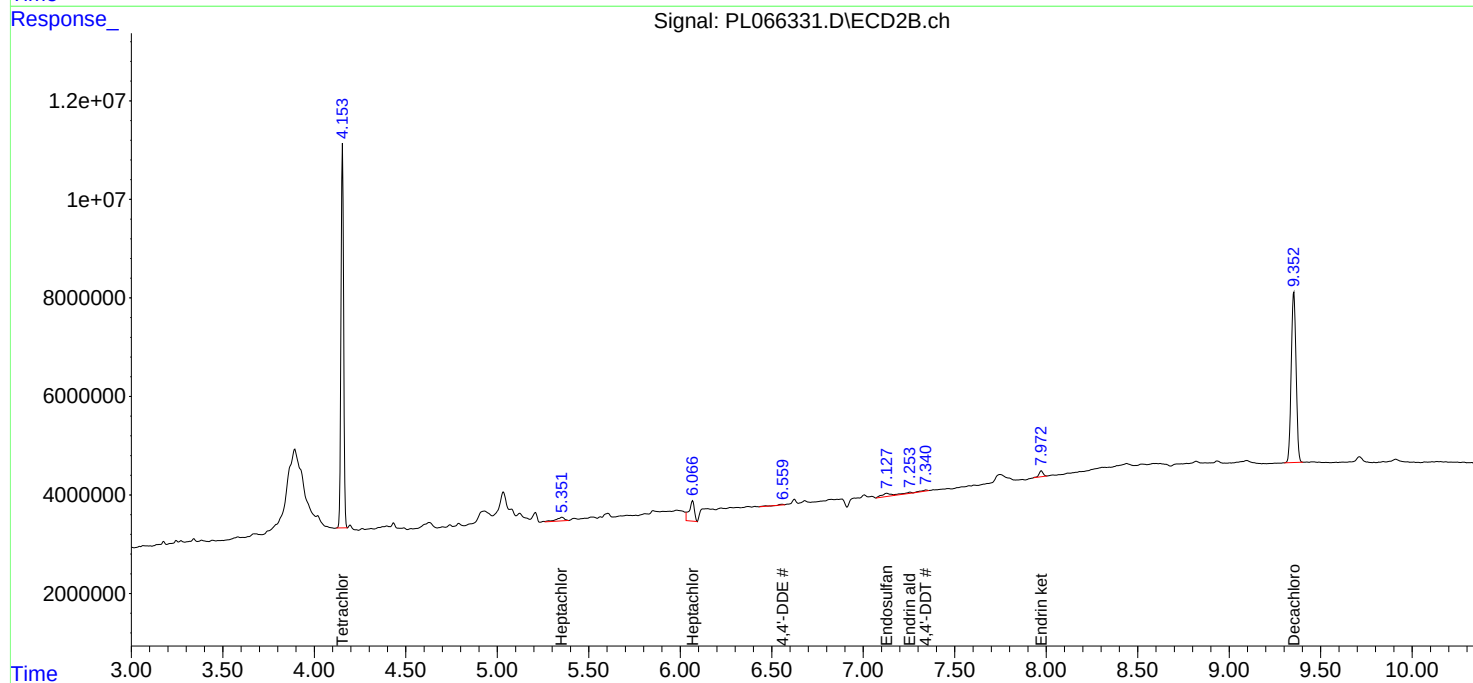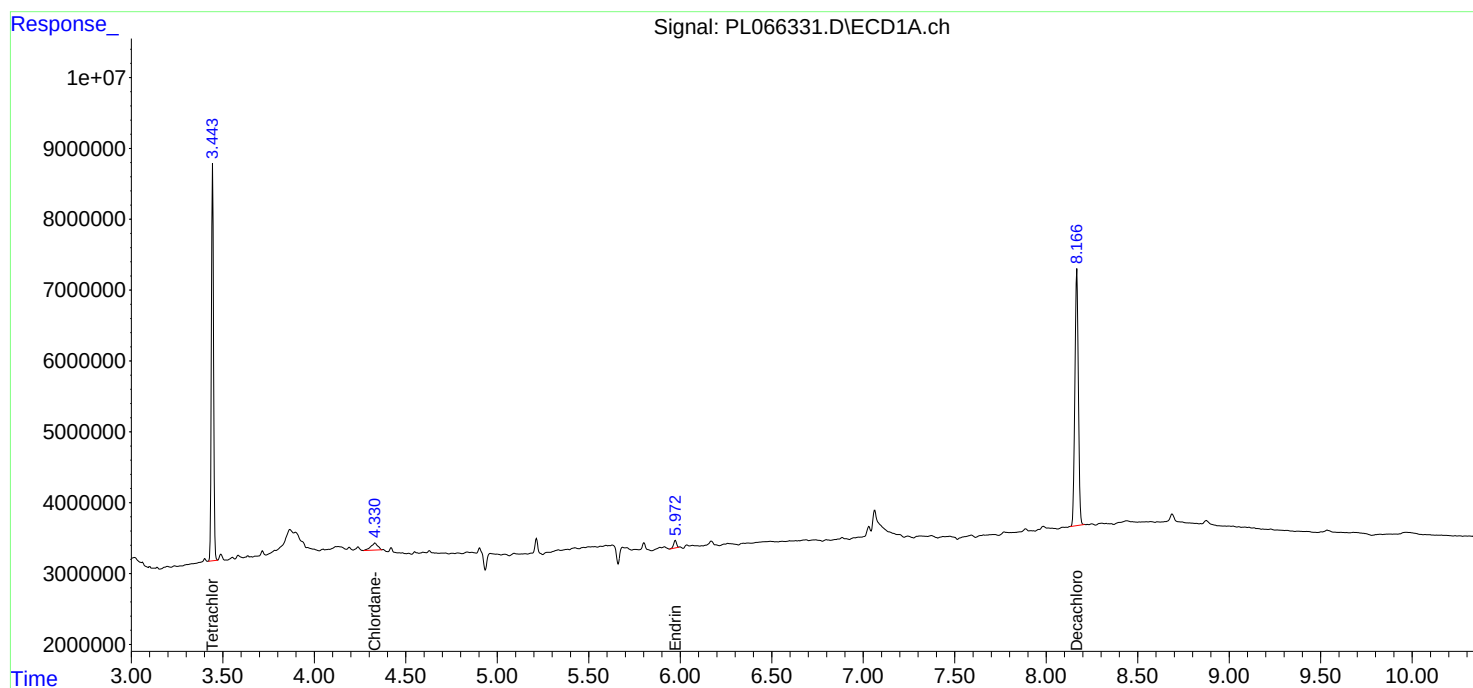


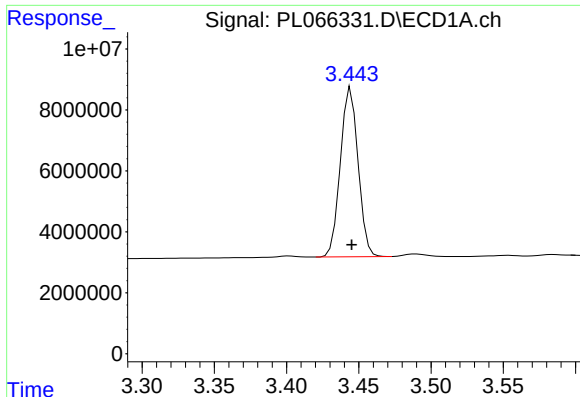

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 47330345
Conc: 18.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

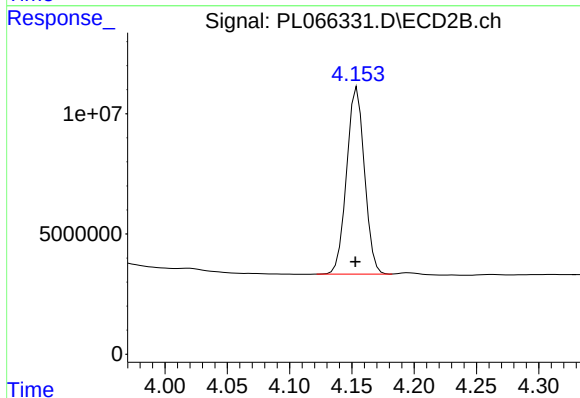


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 77615131
Conc: 19.29 ng/ml

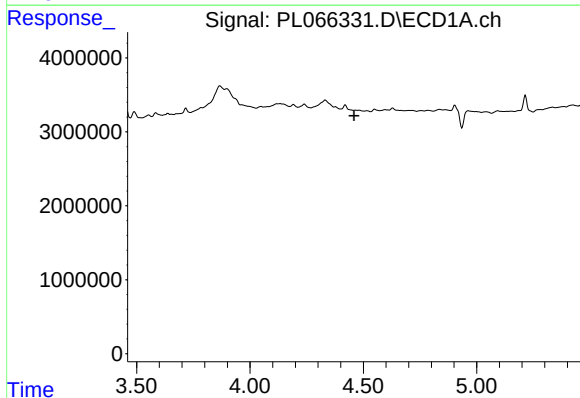


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

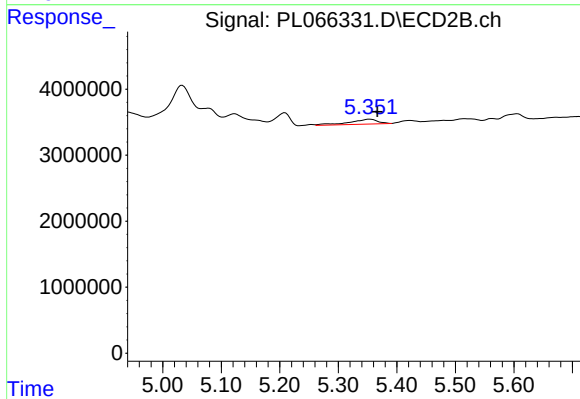

#4 Heptachlor


R.T.: 5.353 min
Delta R.T.: -0.014 min
Response: 2410260
Conc: 0.43 ng/ml

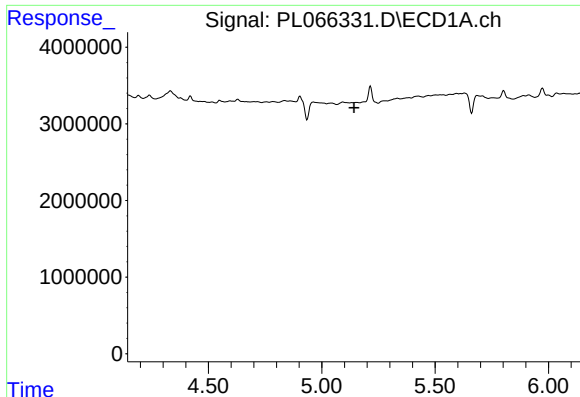

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.143 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

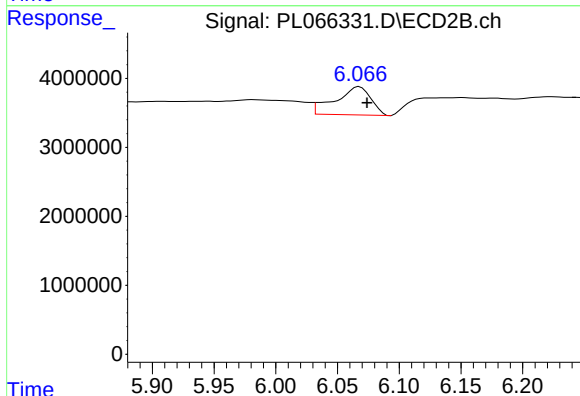


#8 Heptachlor epoxide

R.T.: 6.068 min
Delta R.T.: -0.006 min
Response: 8216477
Conc: 1.78 ng/ml

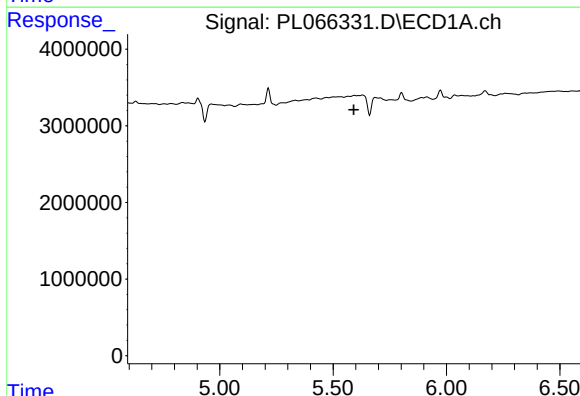


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.591 min
Response: 0
Conc: N.D.

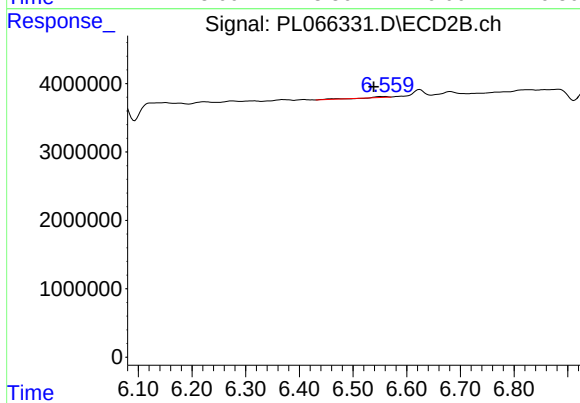

#12 4,4'-DDE


R.T.: 6.553 min
Delta R.T.: 0.014 min
Response: 322567
Conc: 0.08 ng/ml

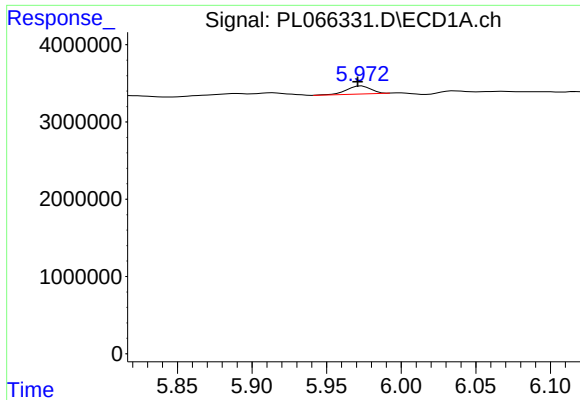

#14 Endrin


R.T.: 5.974 min
Delta R.T.: 0.003 min
Response: 1159266
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

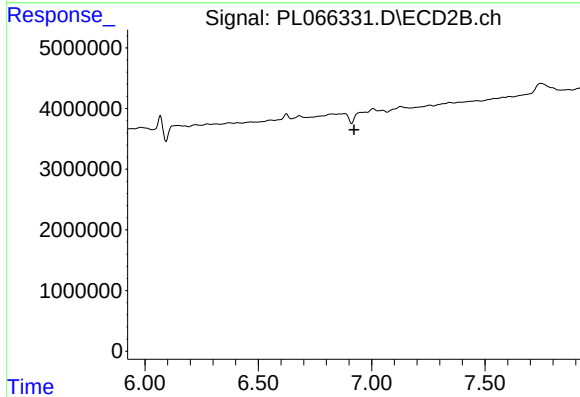


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

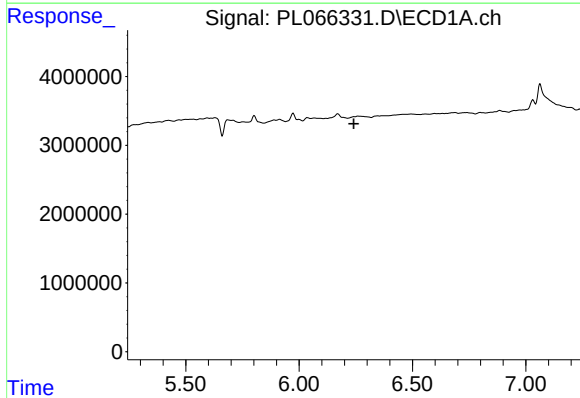


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

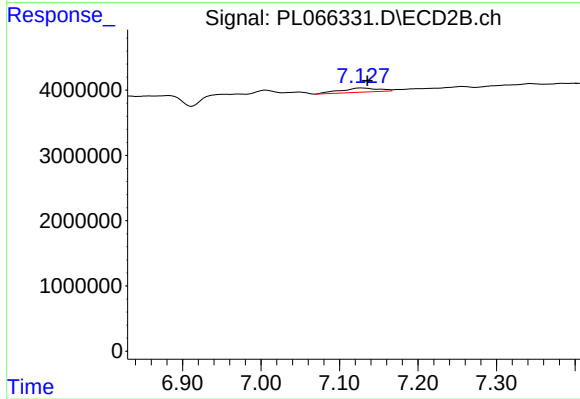

#15 Endosulfan II


R.T.: 7.128 min
Delta R.T.: -0.007 min
Response: 2197658
Conc: 0.63 ng/ml

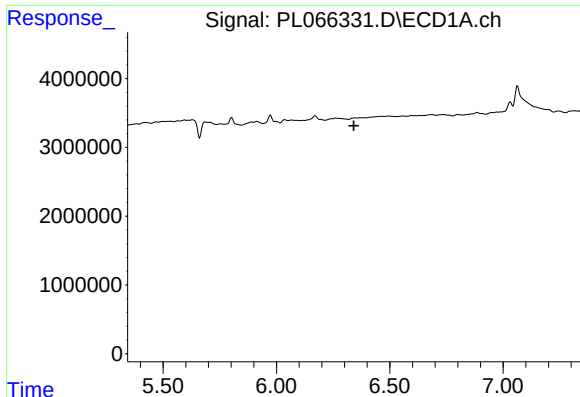

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

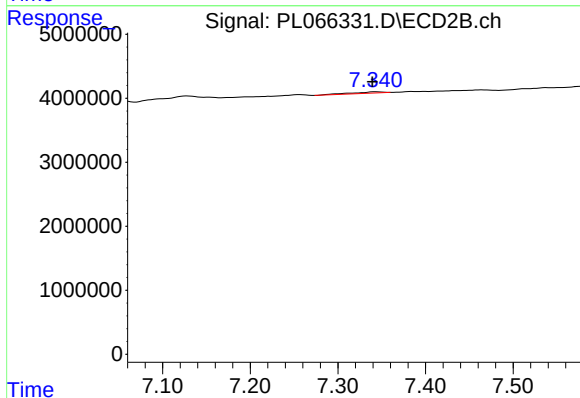


#17 4,4'-DDT

R.T.: 7.343 min
Delta R.T.: 0.003 min
Response: 539448
Conc: 0.16 ng/ml

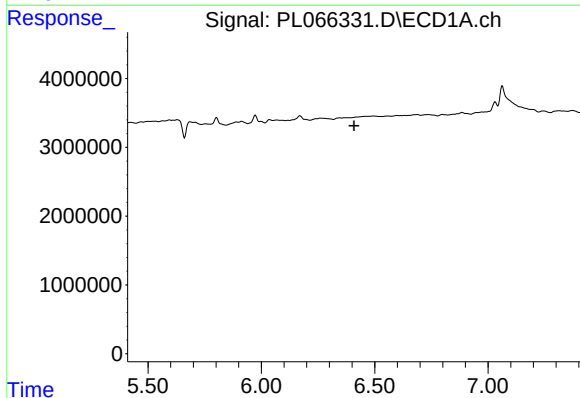


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

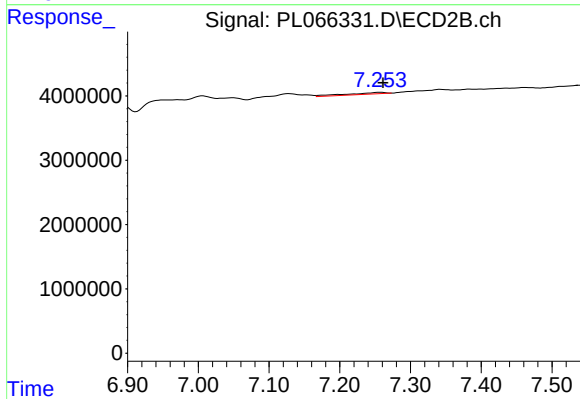

#18 Endrin aldehyde


R.T.: 7.257 min
Delta R.T.: -0.004 min
Response: 989818
Conc: 0.35 ng/ml

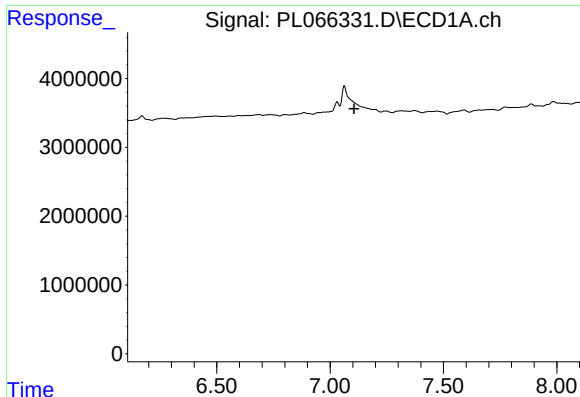

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

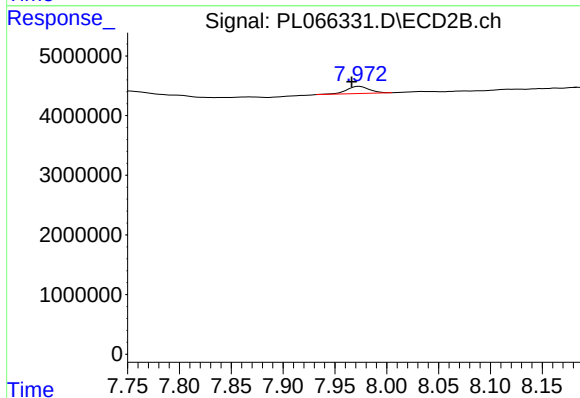


#21 Endrin ketone

R.T.: 7.973 min
Delta R.T.: 0.007 min
Response: 1832631
Conc: 0.50 ng/ml

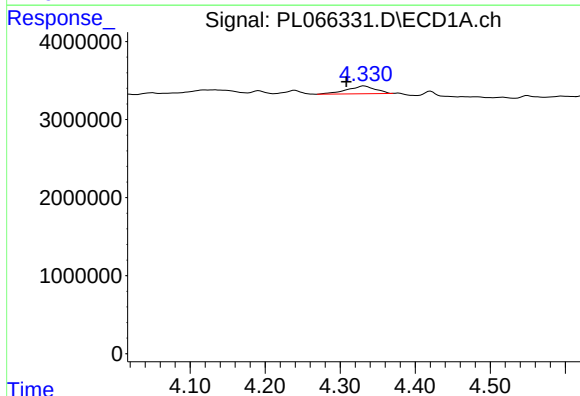


#23 Chlordane-1

R.T.: 4.332 min
Delta R.T.: 0.024 min
Response: 2589044
Conc: 22.65 ng/ml

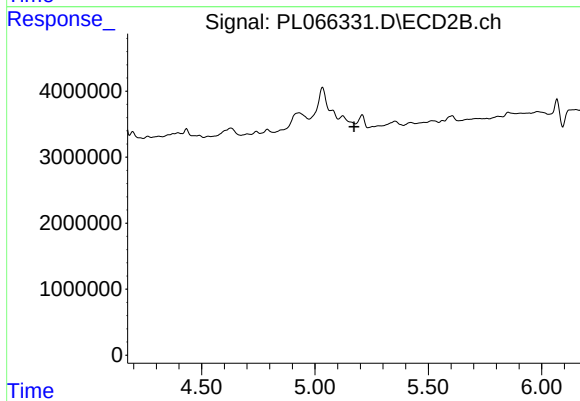

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.173 min
Response: 0
Conc: N.D.

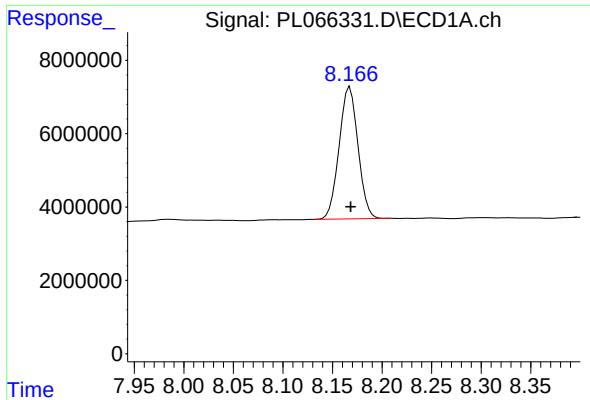

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 47646286
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

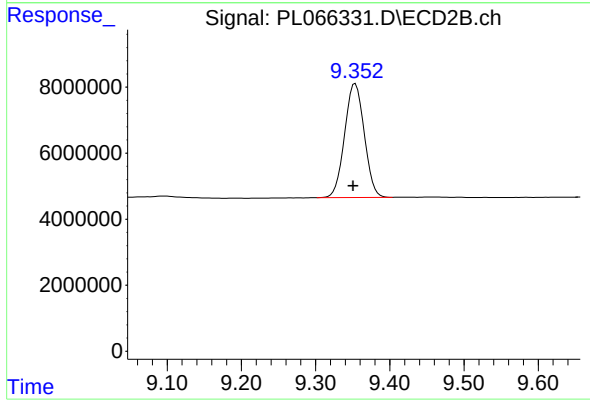

#28 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: 0.003 min
Response: 63471655
Conc: 19.43 ng/ml