

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 12:18
 Operator : AR\AJ
 Sample : M2063-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP2-2-4

Manual Integrations
 APPROVED

Ankita
 4/20/2021 4:24:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 01:57:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.153	32901576	54408868	12.927	13.526
28)	SA Decachlor...	8.168	9.353	36880151	47489140	15.462	14.541
Target Compounds							
12)	B 4,4'-DDE	5.589	6.538	2747145	3853329	0.736m	0.931m#
17)	MA 4,4'-DDT	6.337	7.339	4535212	2696129	1.423	0.795m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 12:18
Operator : AR\AJ
Sample : M2063-07
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP2-2-4


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 01:57:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

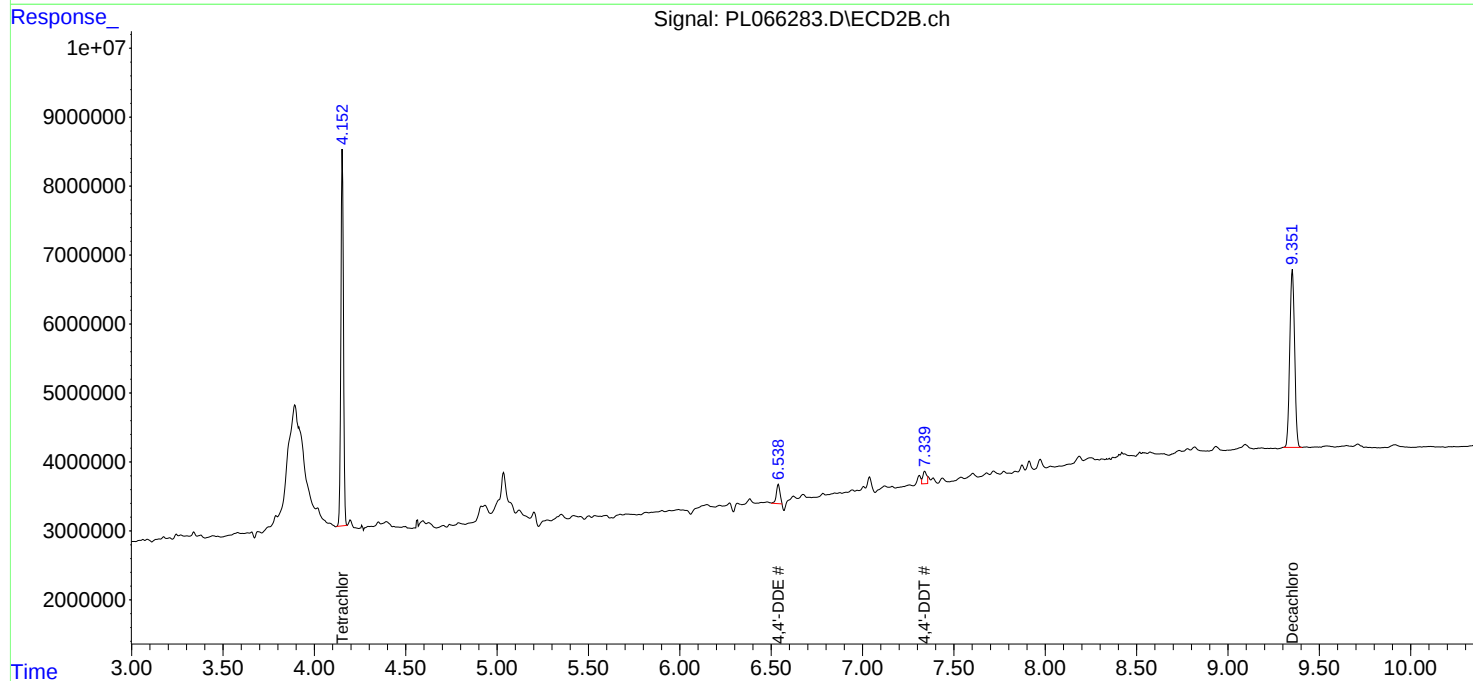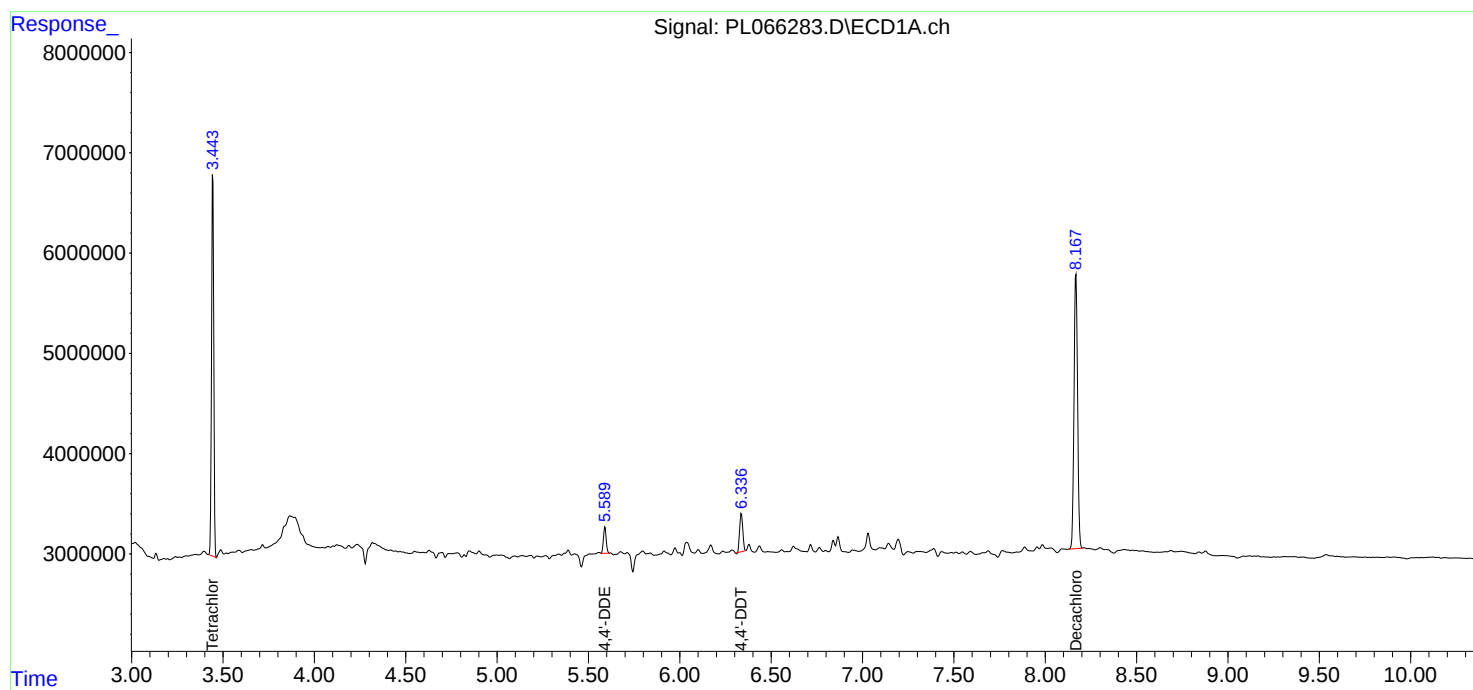

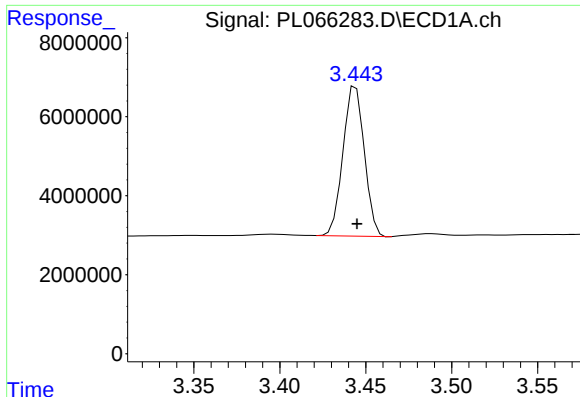


#1 Tetrachloro-m-xylene

R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 32901576
Conc: 12.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP2-2-4


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:34 PM

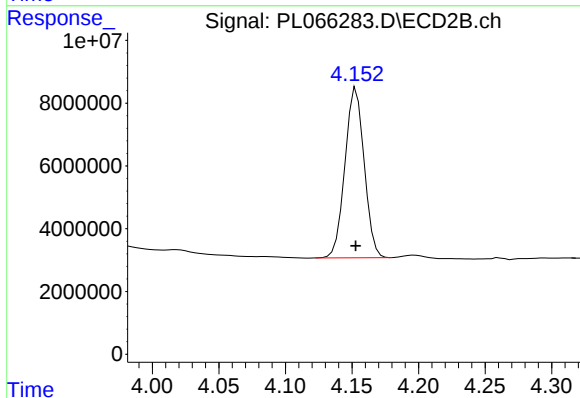


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 54408868
Conc: 13.53 ng/ml

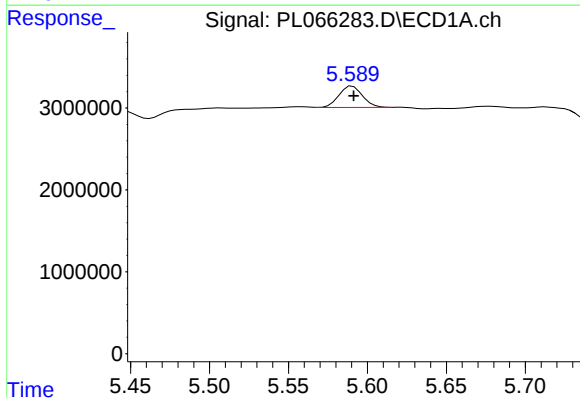


#12 4,4'-DDE

R.T.: 5.589 min
Delta R.T.: -0.002 min
Response: 2747145
Conc: 0.74 ng/ml m

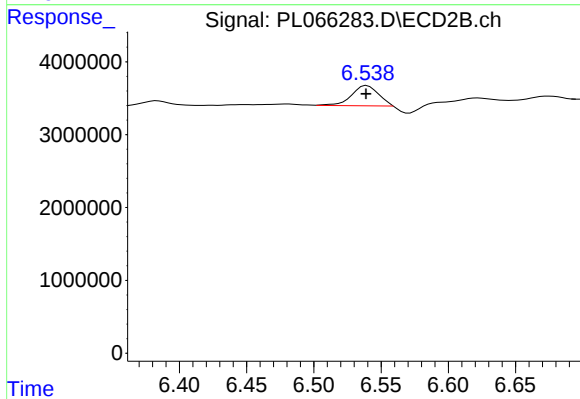

#12 4,4'-DDE

R.T.: 6.538 min
Delta R.T.: 0.000 min
Response: 3853329
Conc: 0.93 ng/ml m

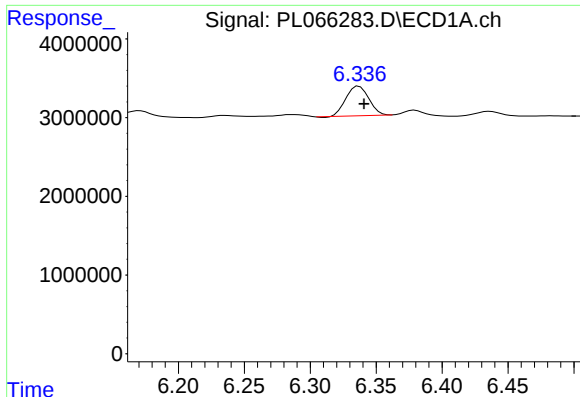


#17 4,4'-DDT

R.T.: 6.337 min
Delta R.T.: -0.004 min
Response: 4535212
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP2-2-4


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:34 PM

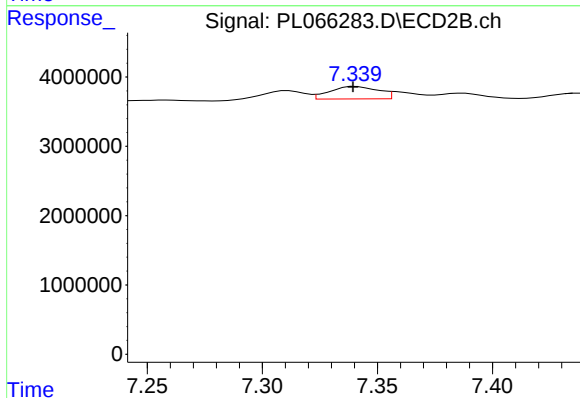


#17 4,4'-DDT

R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 2696129
Conc: 0.79 ng/ml m

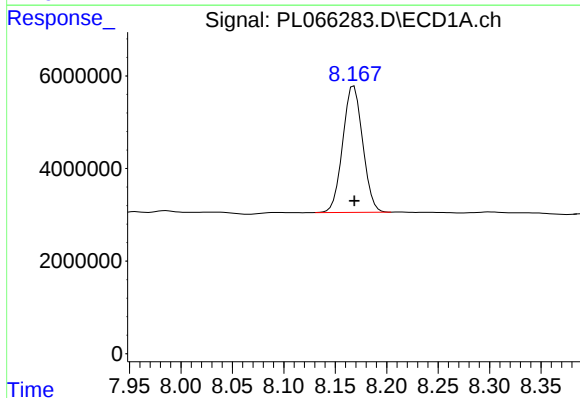

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 36880151
Conc: 15.46 ng/ml

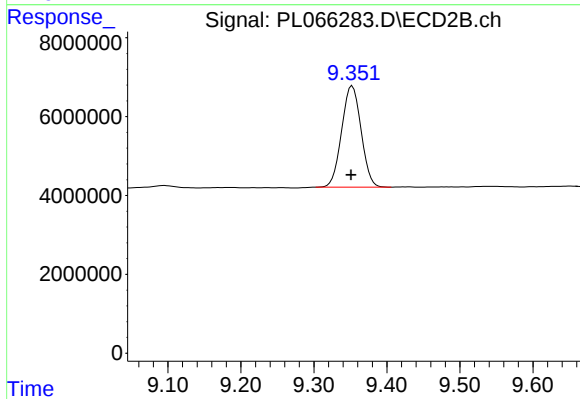

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.002 min
Response: 47489140
Conc: 14.54 ng/ml