

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL041921\  
Data File : PL066286.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 19 Apr 2021 13:00  
Operator : AR\AJ  
Sample : M2075-01  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
TP-1-S

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 20 01:58:00 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL041421.M  
Quant Title : GC Extractables  
QLast Update : Wed Apr 14 15:37:20 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.444 | 4.153 | 50973748 | 85893332 | 20.027 | 21.353 |
| 28)                         | SA Decachlor... | 8.168 | 9.353 | 51094604 | 66778891 | 21.421 | 20.447 |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL041921\  
Data File : PL066286.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 19 Apr 2021 13:00  
Operator : AR\AJ  
Sample : M2075-01  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
TP-1-S

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 20 01:58:00 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL041421.M  
Quant Title : GC Extractables  
QLast Update : Wed Apr 14 15:37:20 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

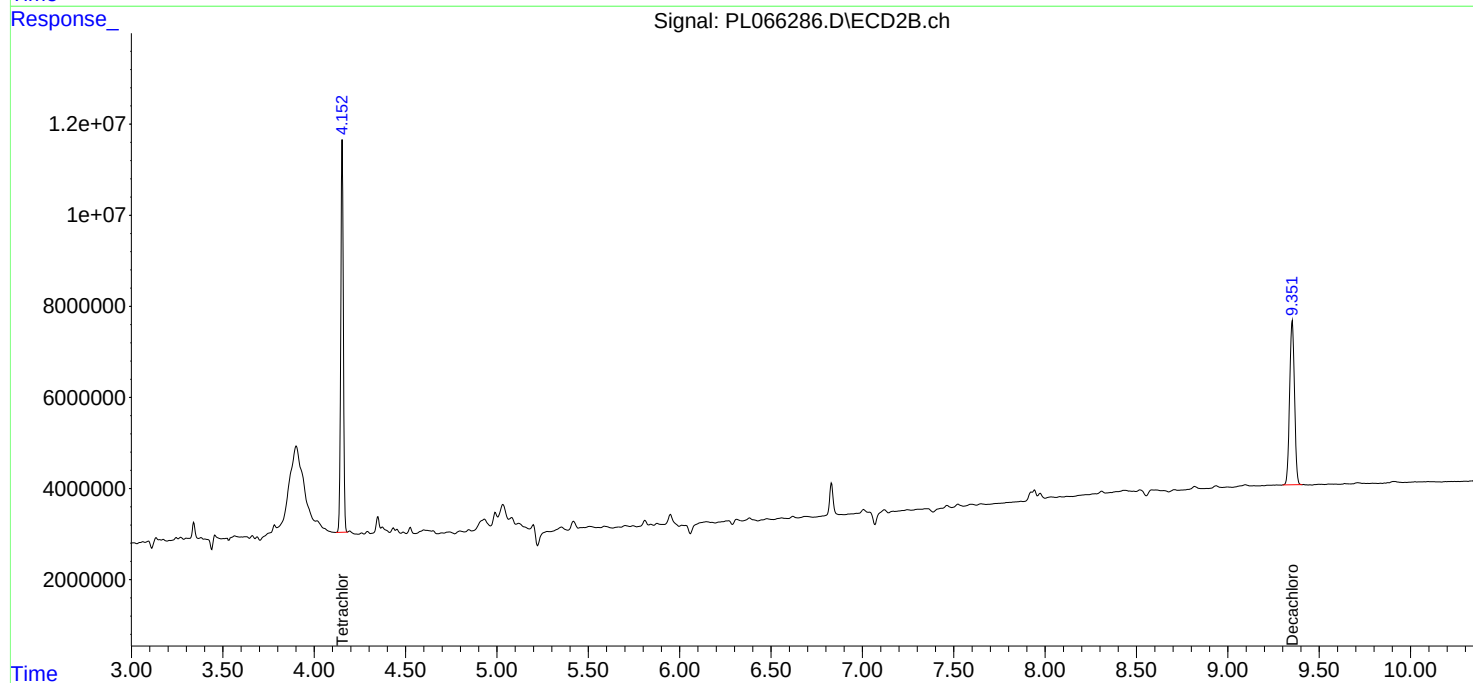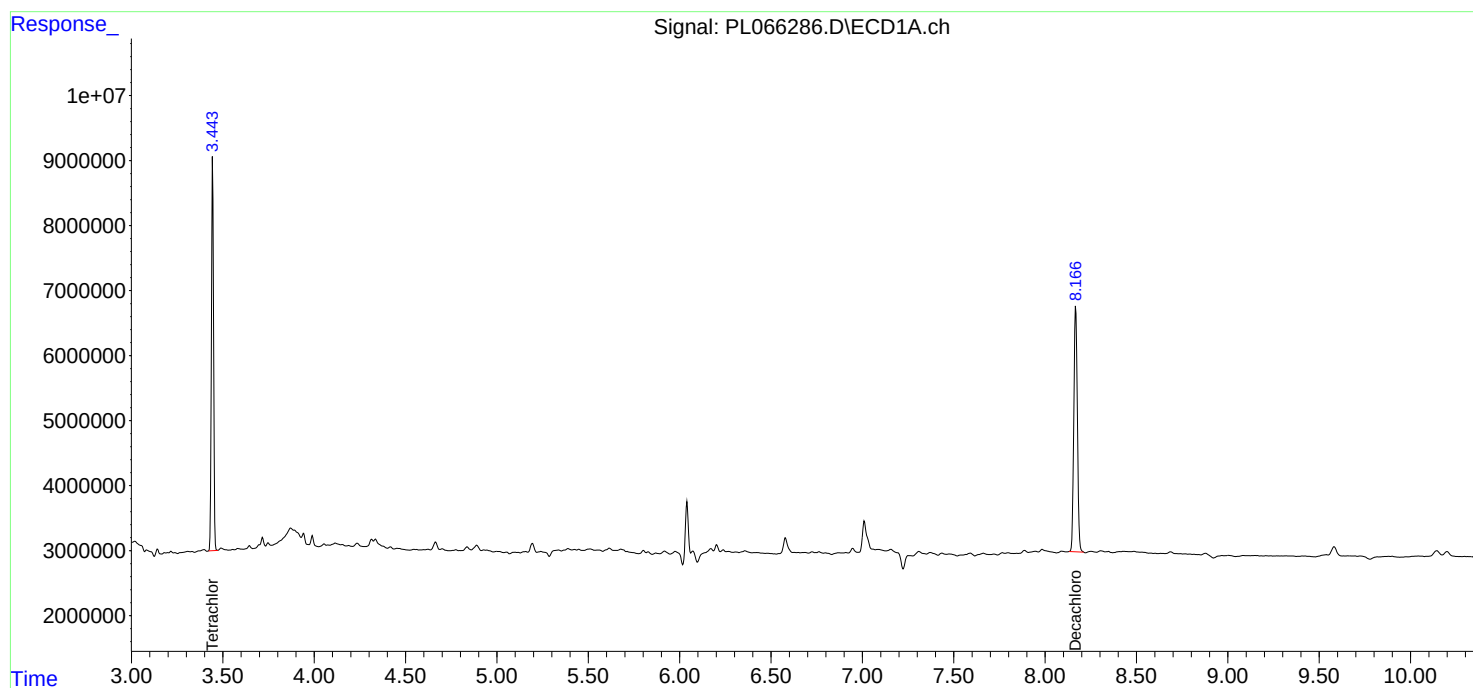


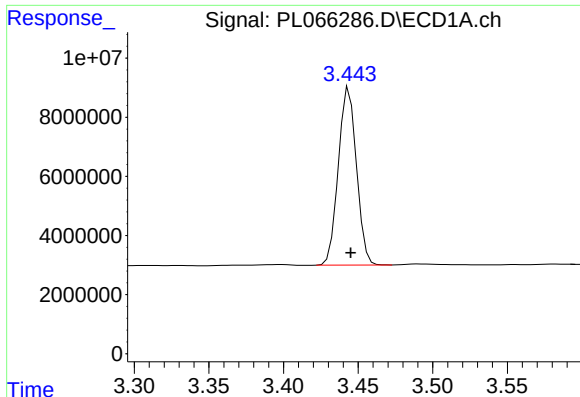

#1 Tetrachloro-m-xylene


R.T.: 3.444 min  
Delta R.T.: 0.000 min  
Response: 50973748  
Conc: 20.03 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
TP-1-S

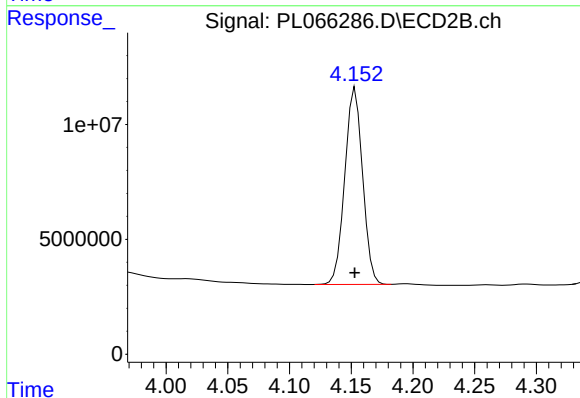


#1 Tetrachloro-m-xylene

R.T.: 4.153 min  
Delta R.T.: 0.000 min  
Response: 85893332  
Conc: 21.35 ng/ml

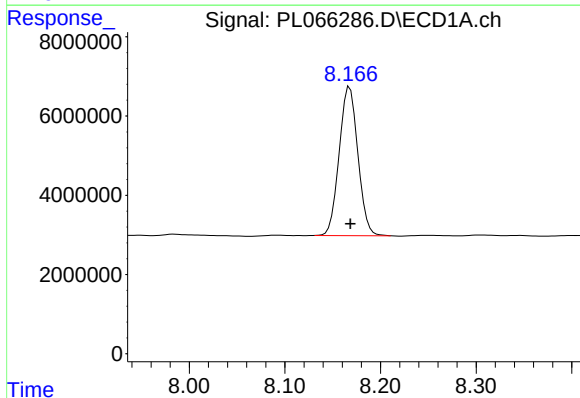

#28 Decachlorobiphenyl

R.T.: 8.168 min  
Delta R.T.: 0.000 min  
Response: 51094604  
Conc: 21.42 ng/ml

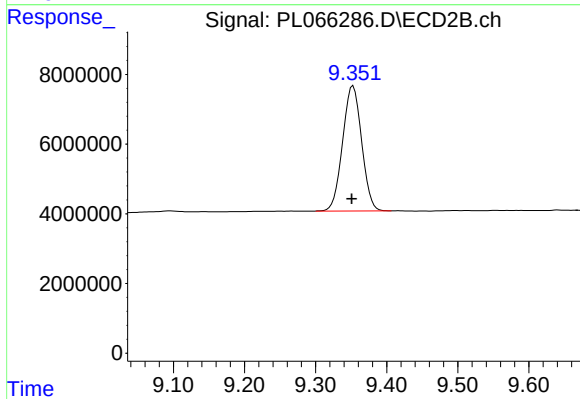

#28 Decachlorobiphenyl

R.T.: 9.353 min  
Delta R.T.: 0.002 min  
Response: 66778891  
Conc: 20.45 ng/ml