

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066296.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 15:45
 Operator : AR\AJ
 Sample : M2075-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-S

Manual Integrations
 APPROVED

Ankita
 4/20/2021 4:24:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:00:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.177f	50184277	80907962	19.717m	20.114
28)	SA Decachlor...	8.169	9.376f	41904890	57316402	17.568	17.550m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066296.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 15:45
Operator : AR\AJ
Sample : M2075-19
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-6-S


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:00:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

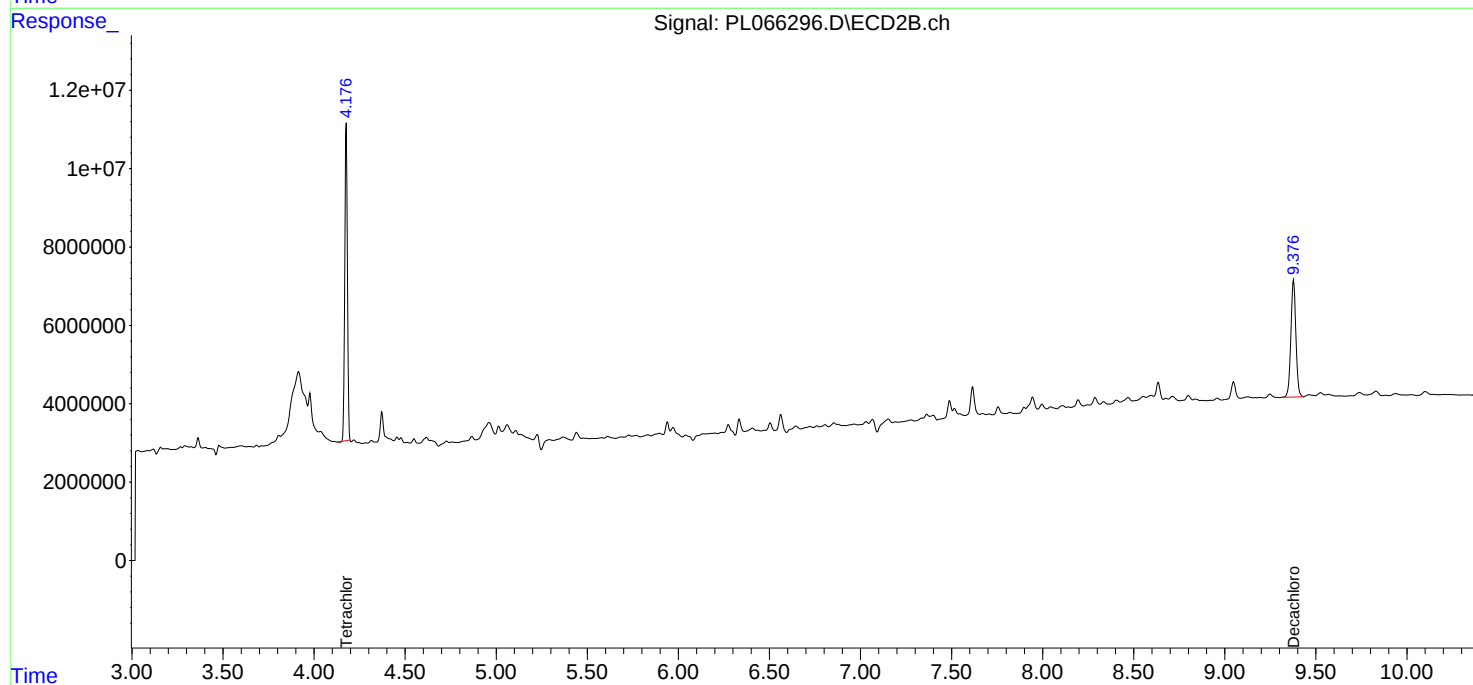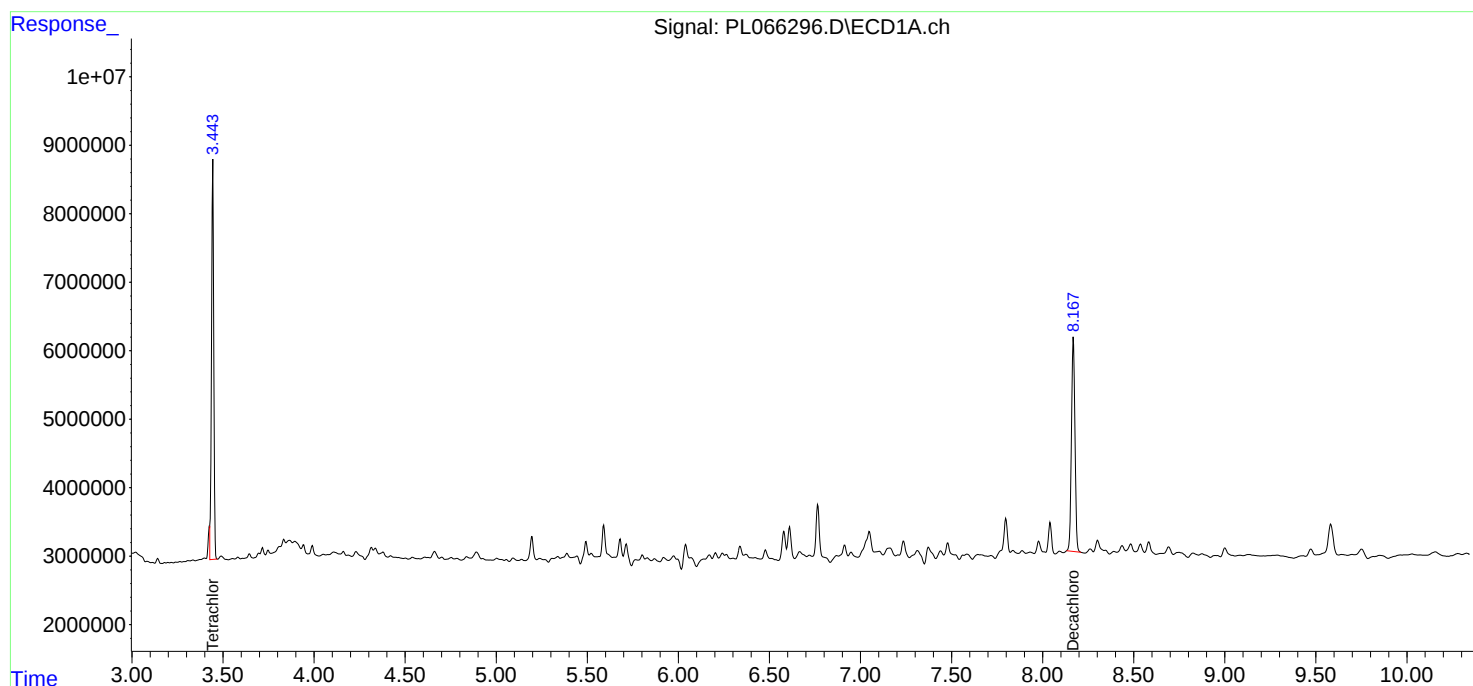

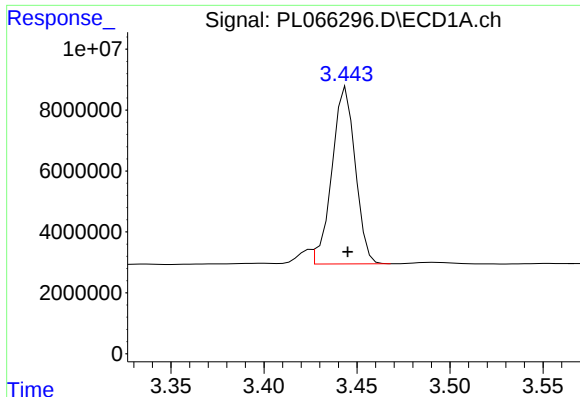


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.002 min
Response: 50184277
Conc: 19.72 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-6-S


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:38 PM

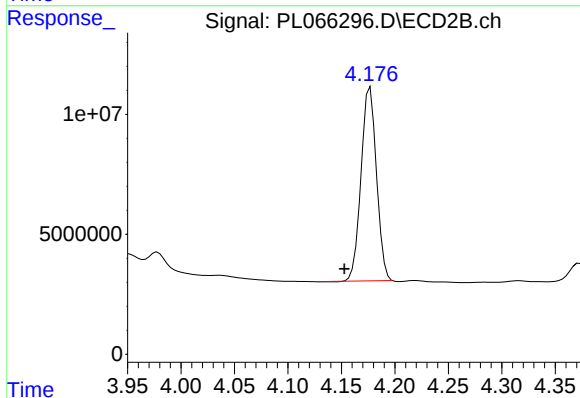


#1 Tetrachloro-m-xylene

R.T.: 4.177 min
Delta R.T.: 0.024 min
Response: 80907962
Conc: 20.11 ng/ml

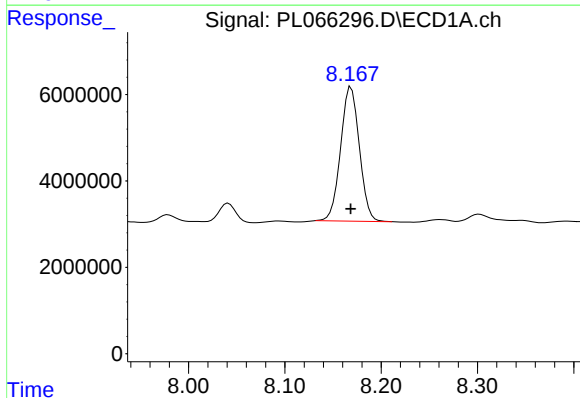

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 41904890
Conc: 17.57 ng/ml

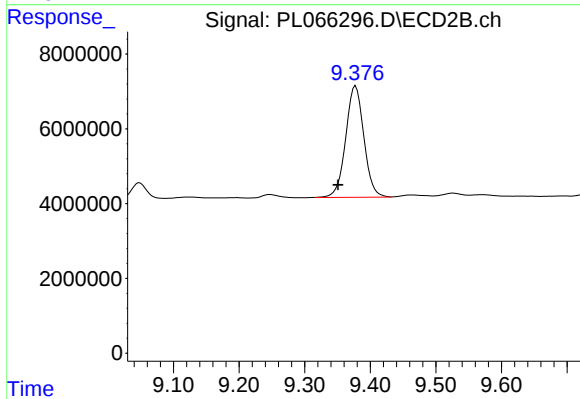

#28 Decachlorobiphenyl

R.T.: 9.376 min
Delta R.T.: 0.026 min
Response: 57316402
Conc: 17.55 ng/ml m