

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 17:28
 Operator : AR\AJ
 Sample : M2076-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-13-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/20/2021 4:24:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:09:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.154	29340087	48103944	11.527	11.959
28)	SA Decachlor...	8.169	9.355	38221152	48946454	16.024	14.987
Target Compounds							
12)	B 4,4'-DDE	5.591	6.539	5027380	5032653	1.348	1.216
17)	MA 4,4'-DDT	6.339	7.339	2228512	1937204	0.699	0.571m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 17:28
Operator : AR\AJ
Sample : M2076-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-13-0-2.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:09:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

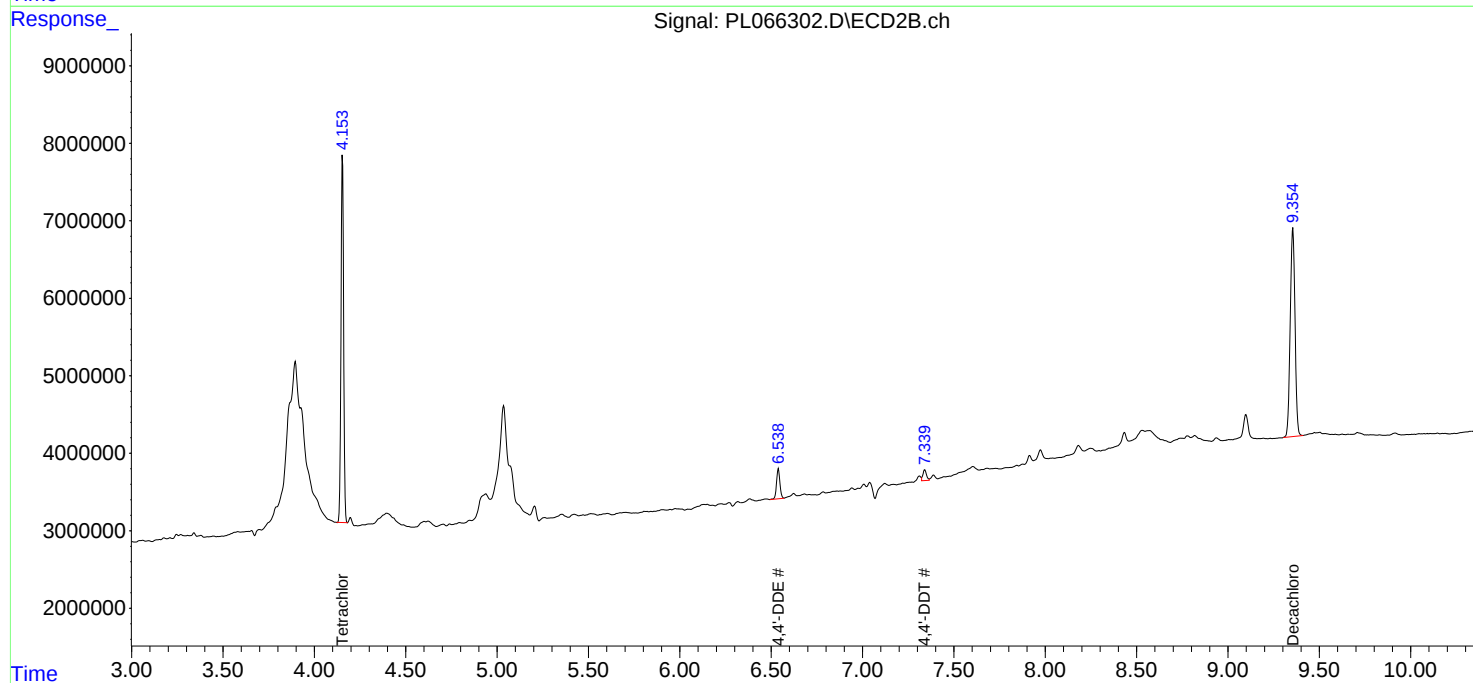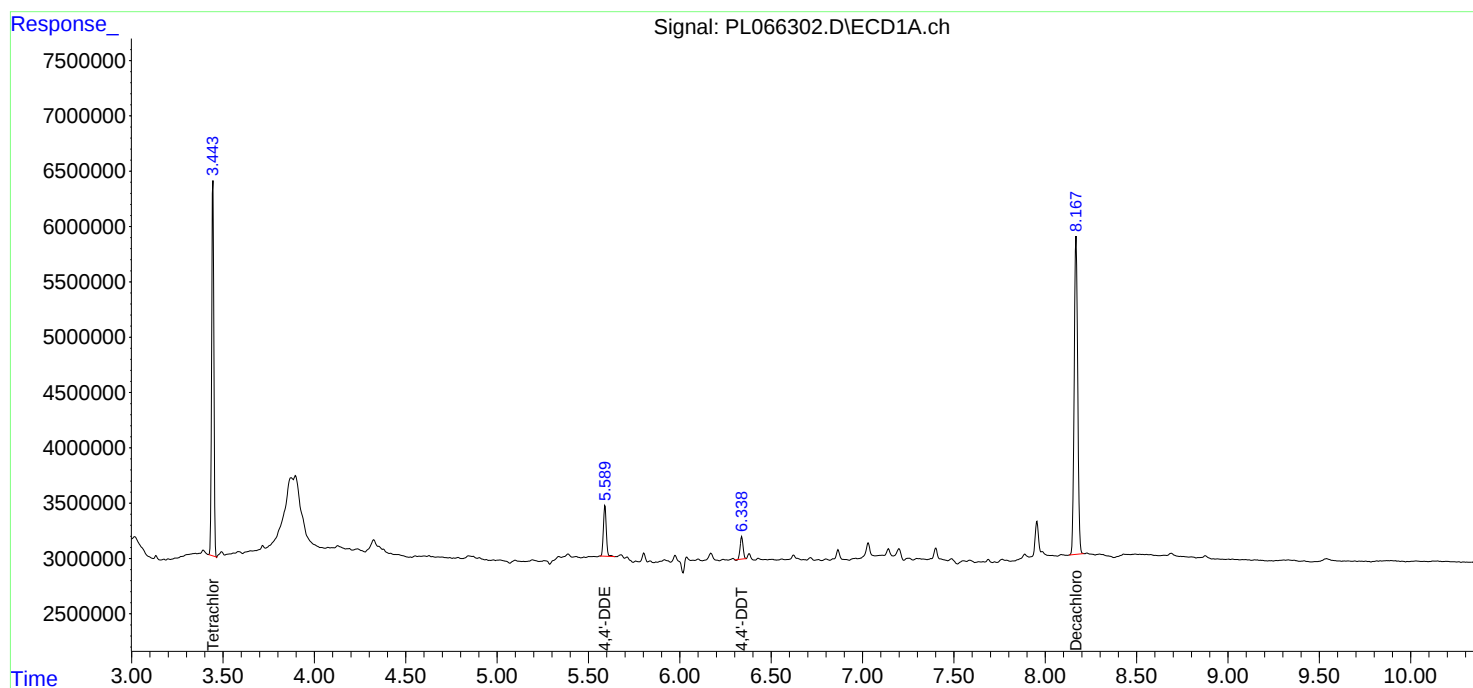

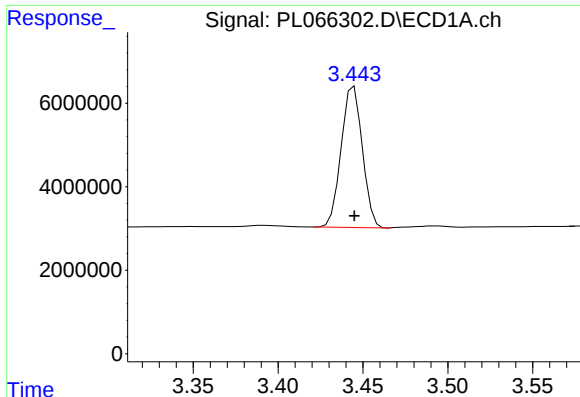


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 29340087
Conc: 11.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-13-0-2.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:40 PM

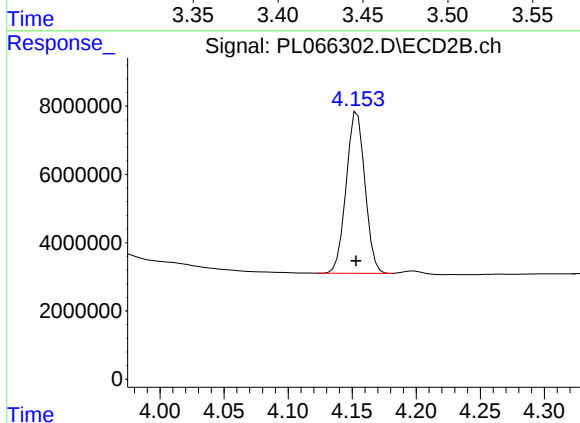


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 48103944
Conc: 11.96 ng/ml

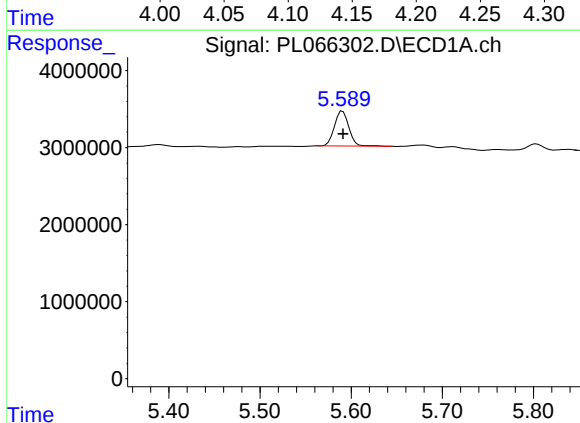


#12 4,4'-DDE

R.T.: 5.591 min
Delta R.T.: 0.000 min
Response: 5027380
Conc: 1.35 ng/ml

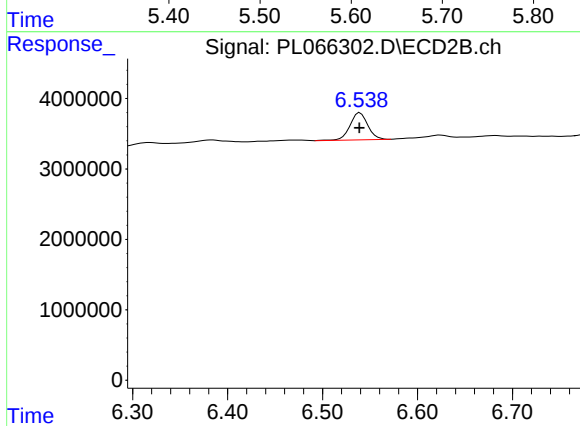

#12 4,4'-DDE

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 5032653
Conc: 1.22 ng/ml

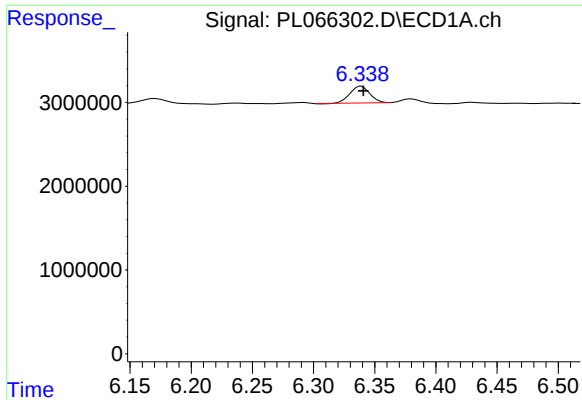


#17 4,4'-DDT

R.T.: 6.339 min
Delta R.T.: -0.002 min
Response: 2228512
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-13-0-2.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:40 PM

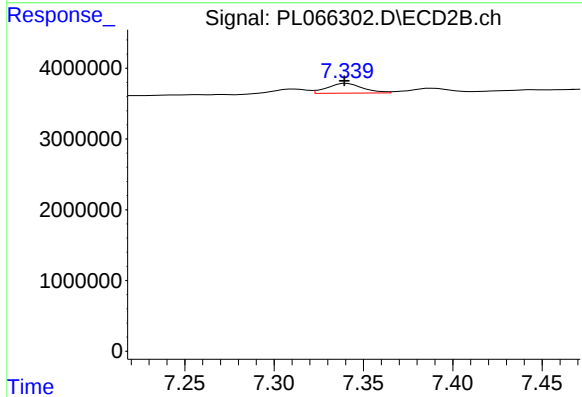


#17 4,4'-DDT

R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 1937204
Conc: 0.57 ng/ml m

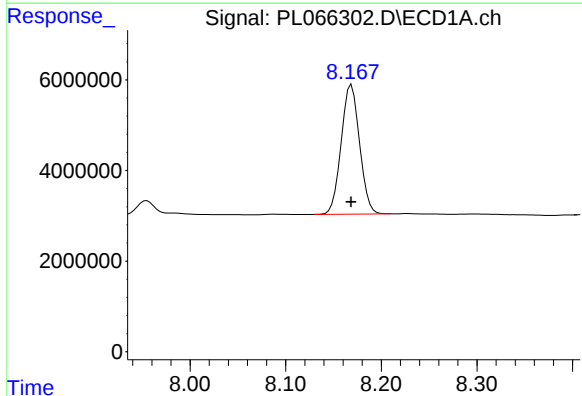

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 38221152
Conc: 16.02 ng/ml

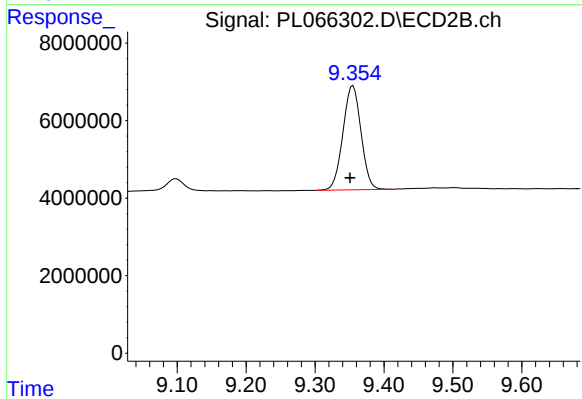

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.004 min
Response: 48946454
Conc: 14.99 ng/ml