

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 18:54
 Operator : AR\AJ
 Sample : M2076-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-15-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/20/2021 4:24:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:11:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.154	49551610	84045725	19.468	20.894
28)	SA Decachlor...	8.167	9.353	52033412	69448570	21.814	21.265
Target Compounds							
12)	B 4,4'-DDE	5.590	6.539	33001859	33669839	8.847	8.135
17)	MA 4,4'-DDT	6.338	7.339	16322222	13803627	5.121m	4.069m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 18:54
Operator : AR\AJ
Sample : M2076-07
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-15-0-2.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:11:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

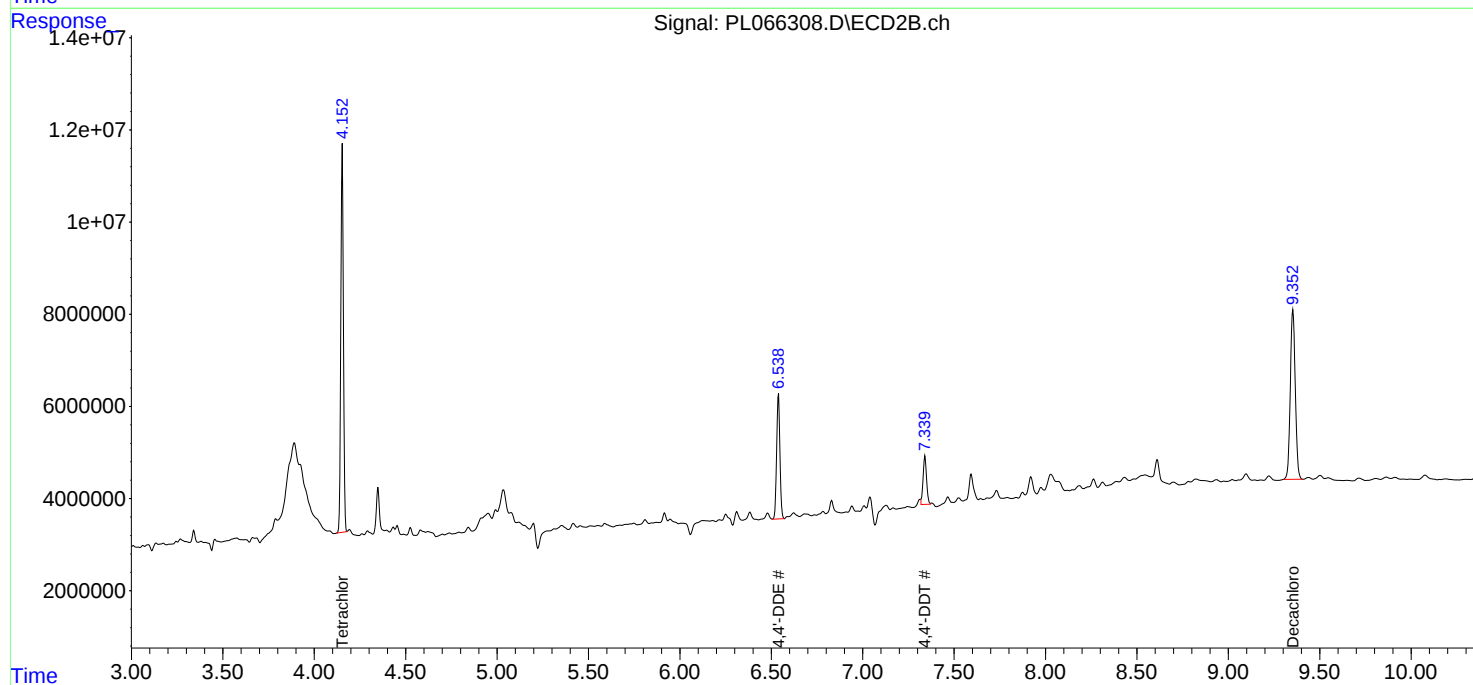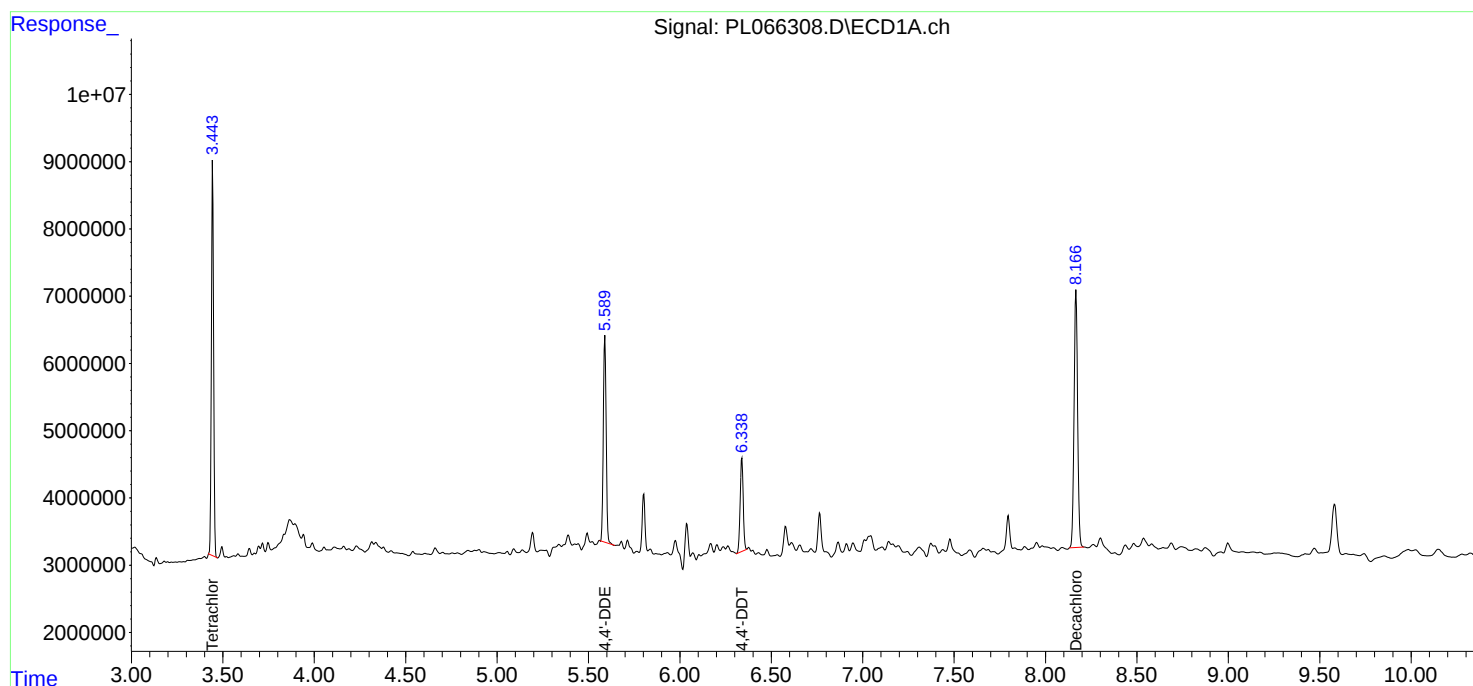

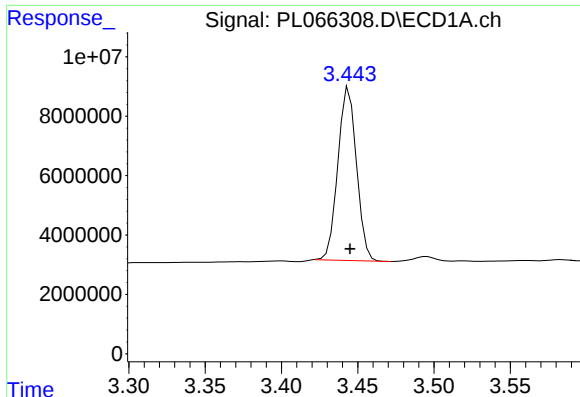


#1 Tetrachloro-m-xylene

R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 49551610
Conc: 19.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-15-0-2.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:44 PM

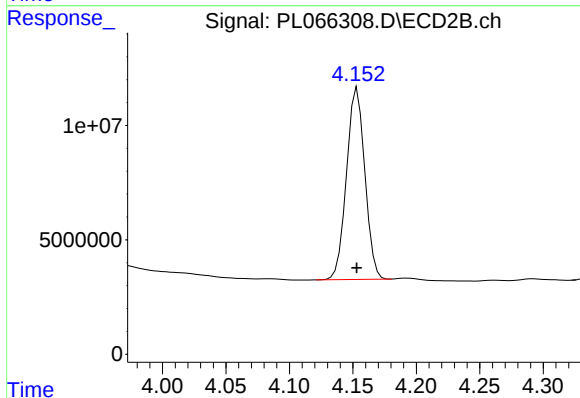


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 84045725
Conc: 20.89 ng/ml

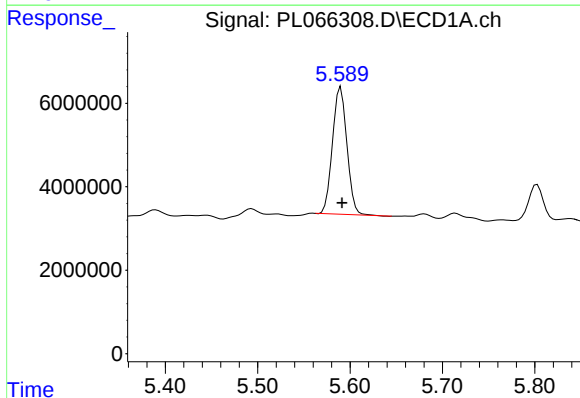


#12 4,4'-DDE

R.T.: 5.590 min
Delta R.T.: -0.001 min
Response: 33001859
Conc: 8.85 ng/ml

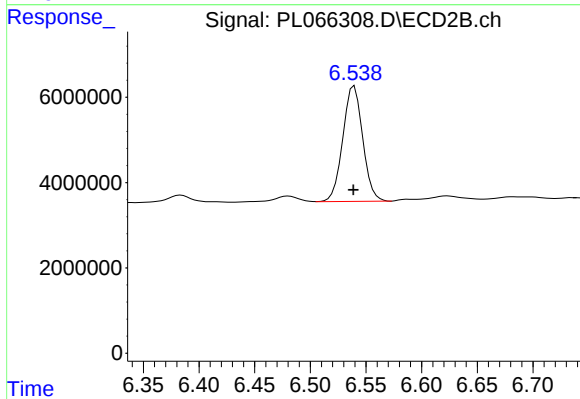

#12 4,4'-DDE

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 33669839
Conc: 8.13 ng/ml

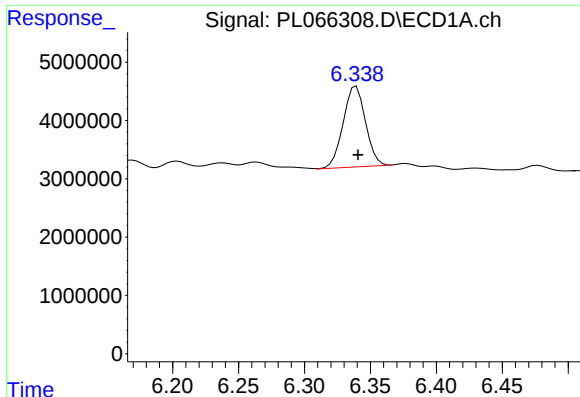


#17 4,4'-DDT

R.T.: 6.338 min
Delta R.T.: -0.003 min
Response: 16322222
Conc: 5.12 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-15-0-2.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:44 PM

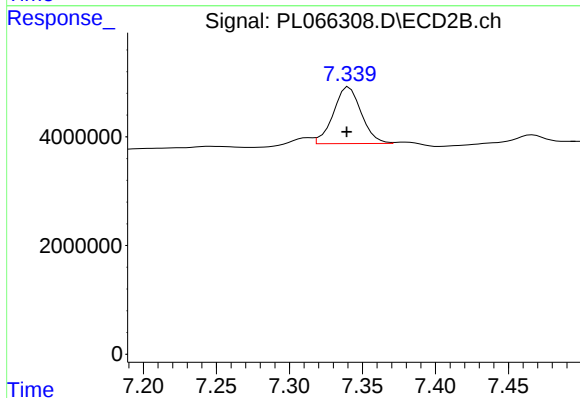


#17 4,4'-DDT

R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 13803627
Conc: 4.07 ng/ml m

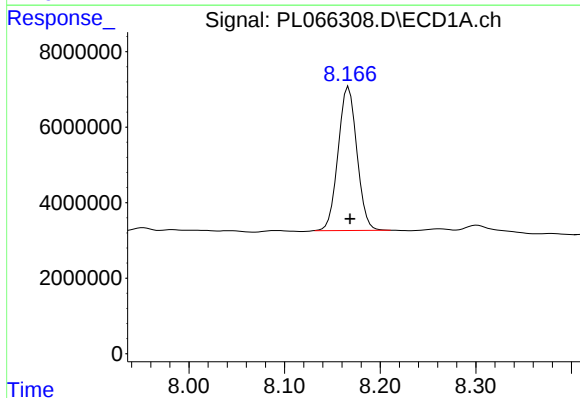

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: -0.001 min
Response: 52033412
Conc: 21.81 ng/ml

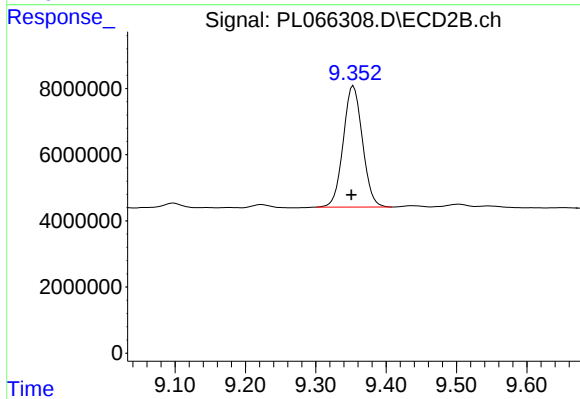

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.003 min
Response: 69448570
Conc: 21.26 ng/ml