

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 20:35
 Operator : AR\AJ
 Sample : M2076-13
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-17-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/20/2021 4:24:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:13:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.154	50125649	82899586	19.694	20.609
28)	SA Decachlor...	8.168	9.355	47663334	63780077	19.982	19.529
Target Compounds							
12)	B 4,4'-DDE	5.591	6.540	31320442	30473082	8.397	7.362
17)	MA 4,4'-DDT	6.338	7.339	20188680	25941249	6.334m	7.647m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 20:35
Operator : AR\AJ
Sample : M2076-13
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-17-0-2.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:13:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

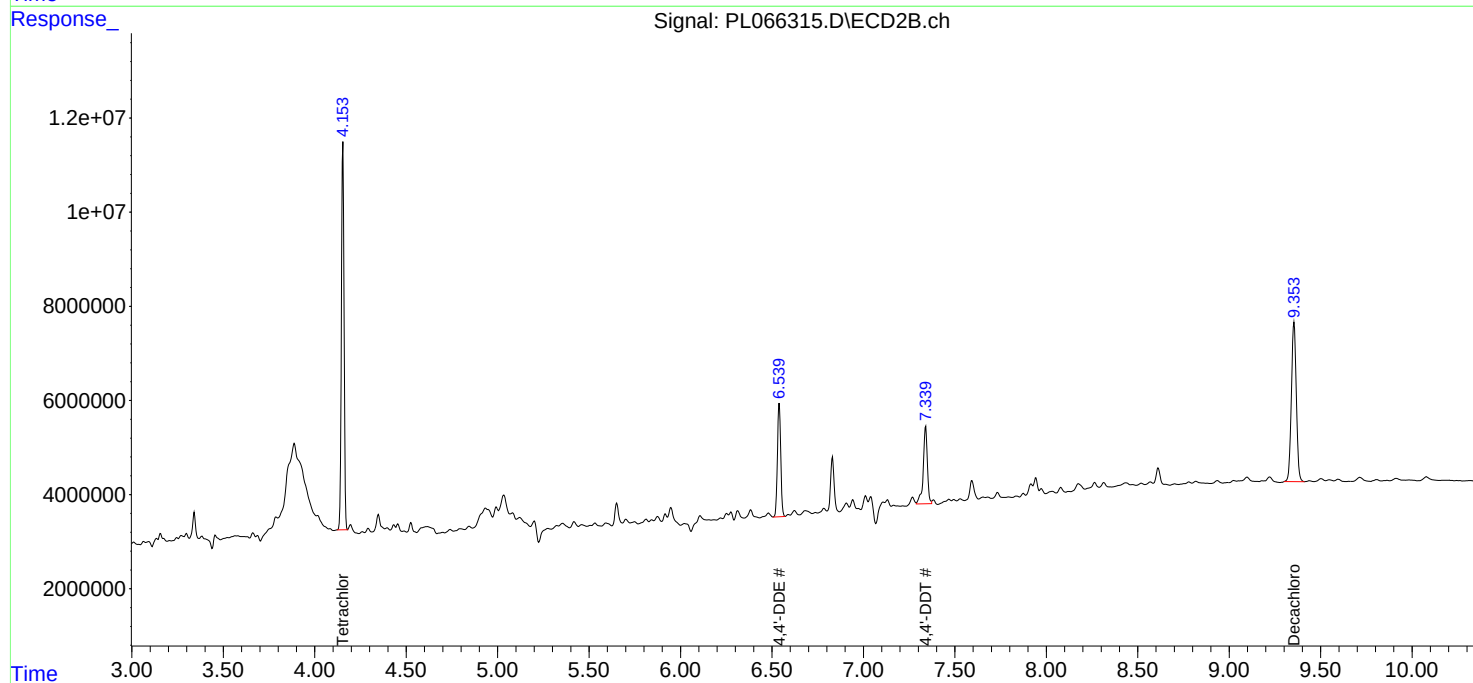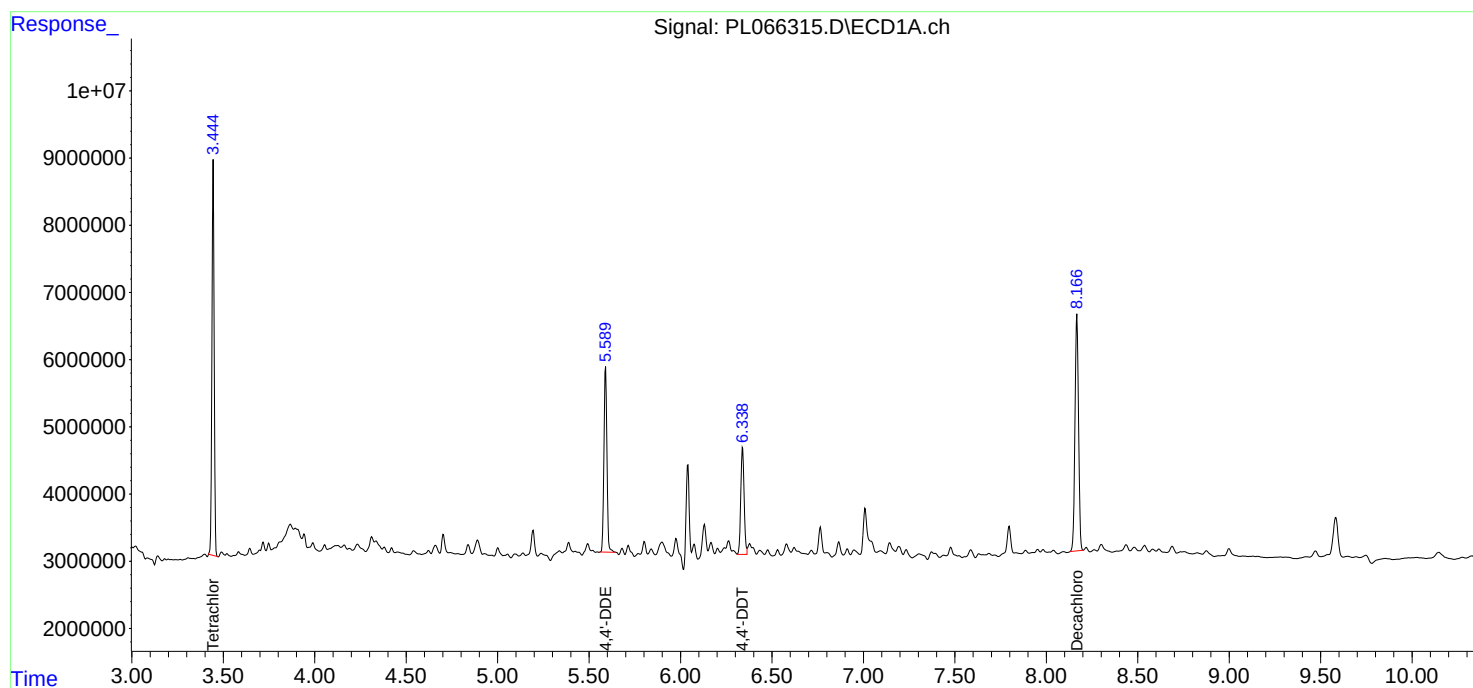

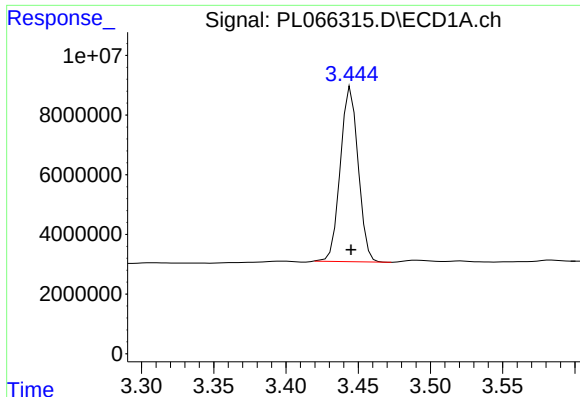


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 50125649
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-17-0-2.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:56 PM

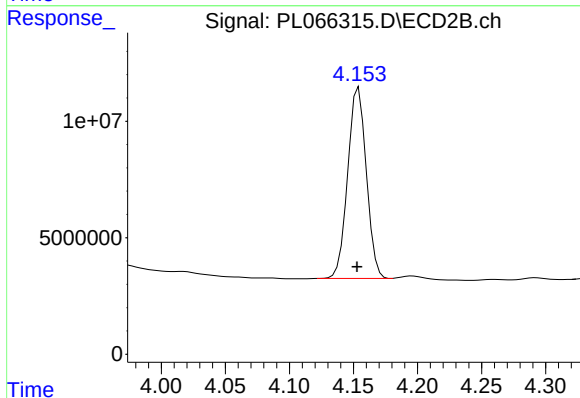


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 82899586
Conc: 20.61 ng/ml

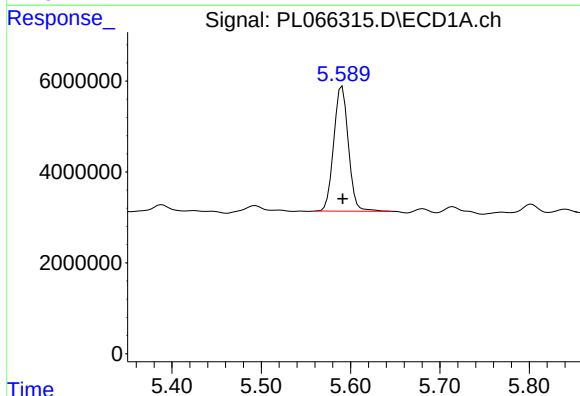


#12 4,4'-DDE

R.T.: 5.591 min
Delta R.T.: 0.000 min
Response: 31320442
Conc: 8.40 ng/ml

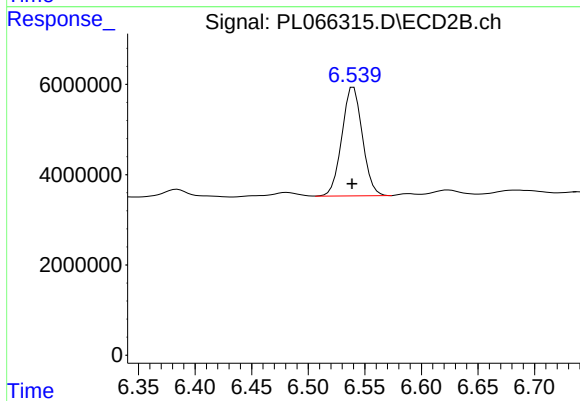

#12 4,4'-DDE

R.T.: 6.540 min
Delta R.T.: 0.001 min
Response: 30473082
Conc: 7.36 ng/ml

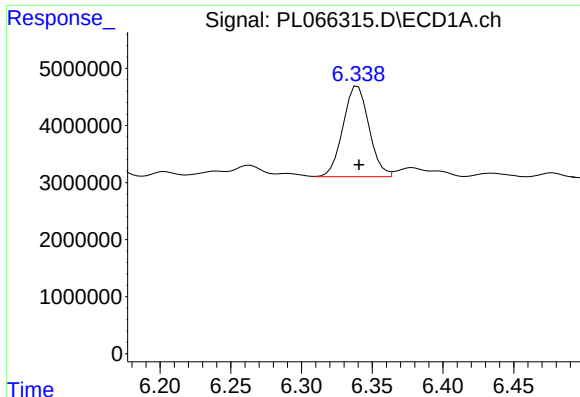


#17 4,4'-DDT

R.T.: 6.338 min
Delta R.T.: -0.002 min
Response: 20188680
Conc: 6.33 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-17-0-2.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:24:56 PM

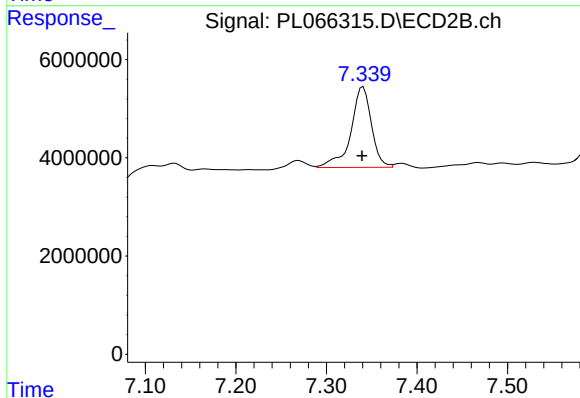


#17 4,4'-DDT

R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 25941249
Conc: 7.65 ng/ml m

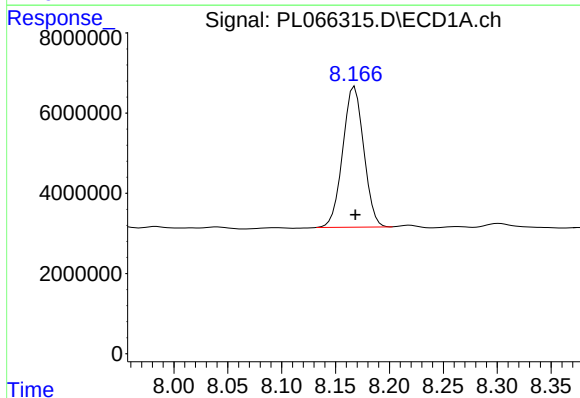

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 47663334
Conc: 19.98 ng/ml

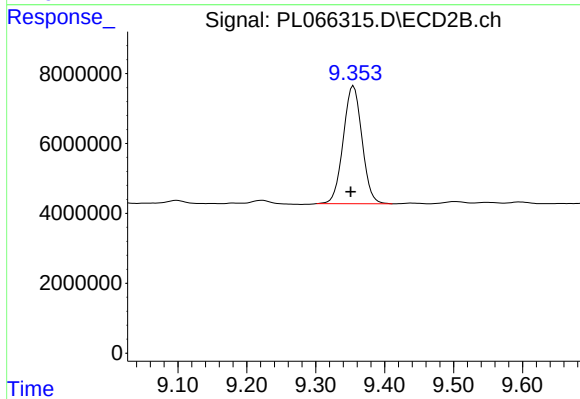

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.004 min
Response: 63780077
Conc: 19.53 ng/ml