

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
 Data File : PL066322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2021 22:15
 Operator : AR\AJ
 Sample : M2077-04
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-20-14.5-15.0

Manual Integrations
 APPROVED

Ankita
 4/20/2021 4:25:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 02:15:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.152	29991368	39187324	11.783	9.742m
28)	SA Decachlor...	8.167	9.354	36313032	53064580	15.224	16.248

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041921\
Data File : PL066322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2021 22:15
Operator : AR\AJ
Sample : M2077-04
Misc :
ALS Vial : 48 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampled :
SB-20-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:25:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 02:15:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

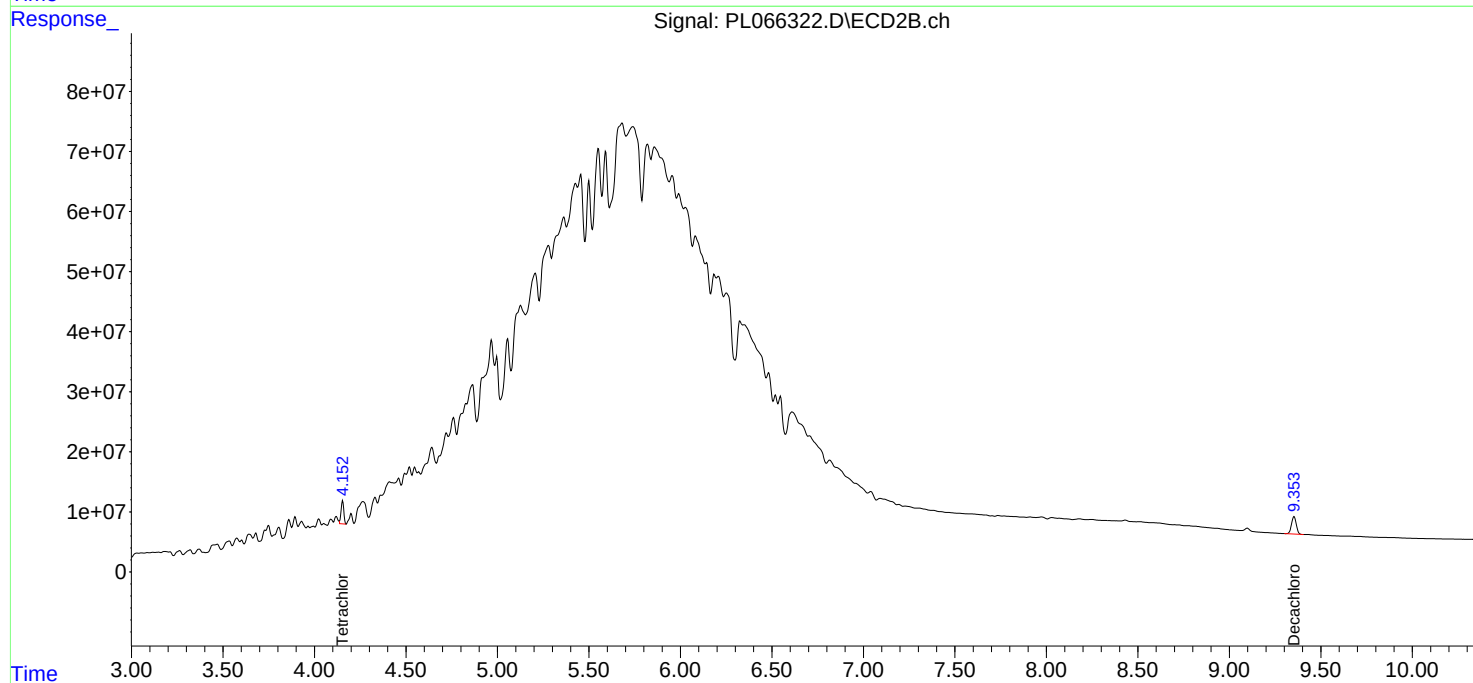

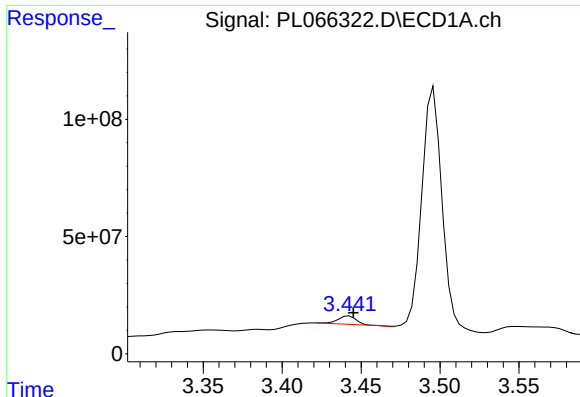


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.002 min
Response: 29991368
Conc: 11.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-20-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/20/2021 4:25:02 PM

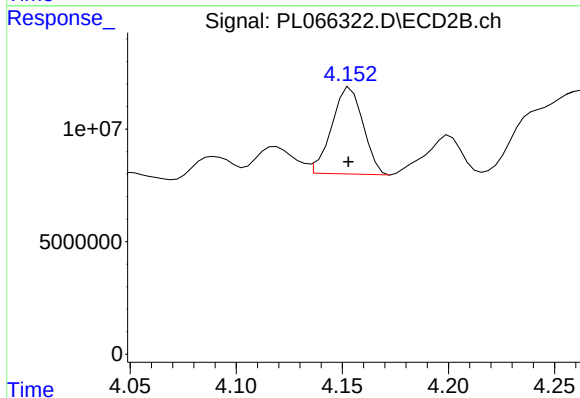


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: 0.000 min
Response: 39187324
Conc: 9.74 ng/ml m

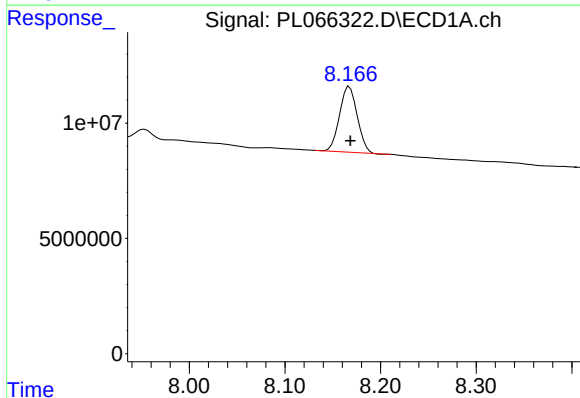

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: -0.001 min
Response: 36313032
Conc: 15.22 ng/ml

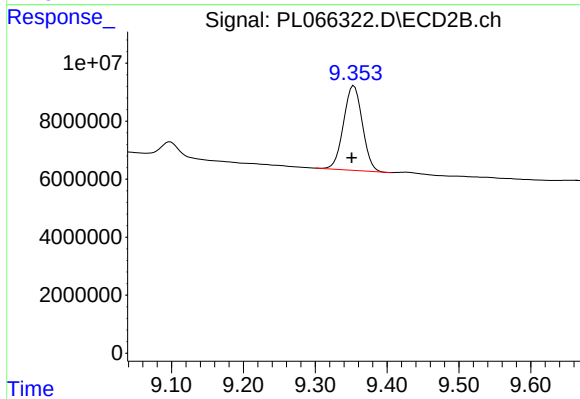

#28 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: 0.003 min
Response: 53064580
Conc: 16.25 ng/ml