

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
 Data File : PL066386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 11:47
 Operator : AR\AJ
 Sample : M2090-03RE 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SEDGWICK-COMP-1RE

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:52:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 18:12:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.442	4.153	8392412	12737831	3.297m	3.167
28) SA Decachlor...	8.168	9.355	8379017	11514404	3.513	3.526

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
Data File : PL066386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 11:47
Operator : AR\AJ
Sample : M2090-03RE 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SEDGWICK-COMP-1RE


Manual Integrations
APPROVED

Ankita
4/22/2021 2:52:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 18:12:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

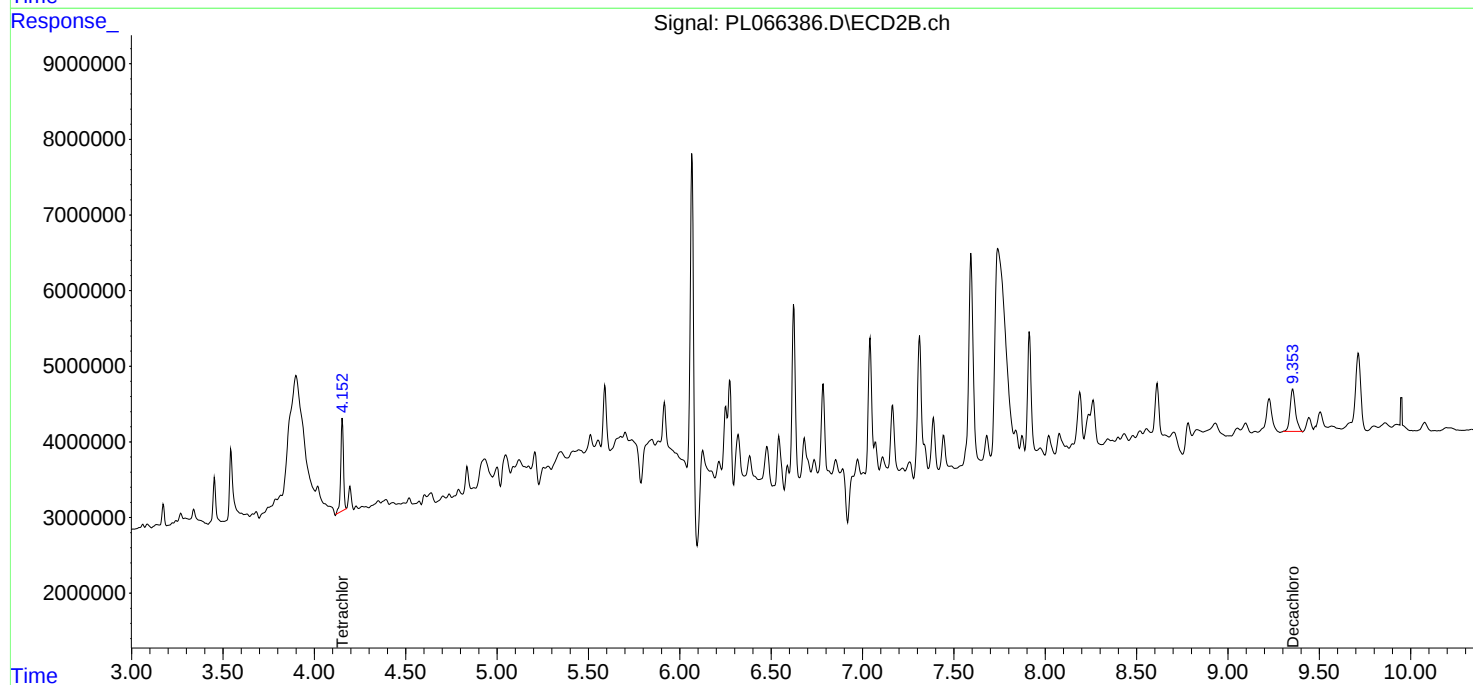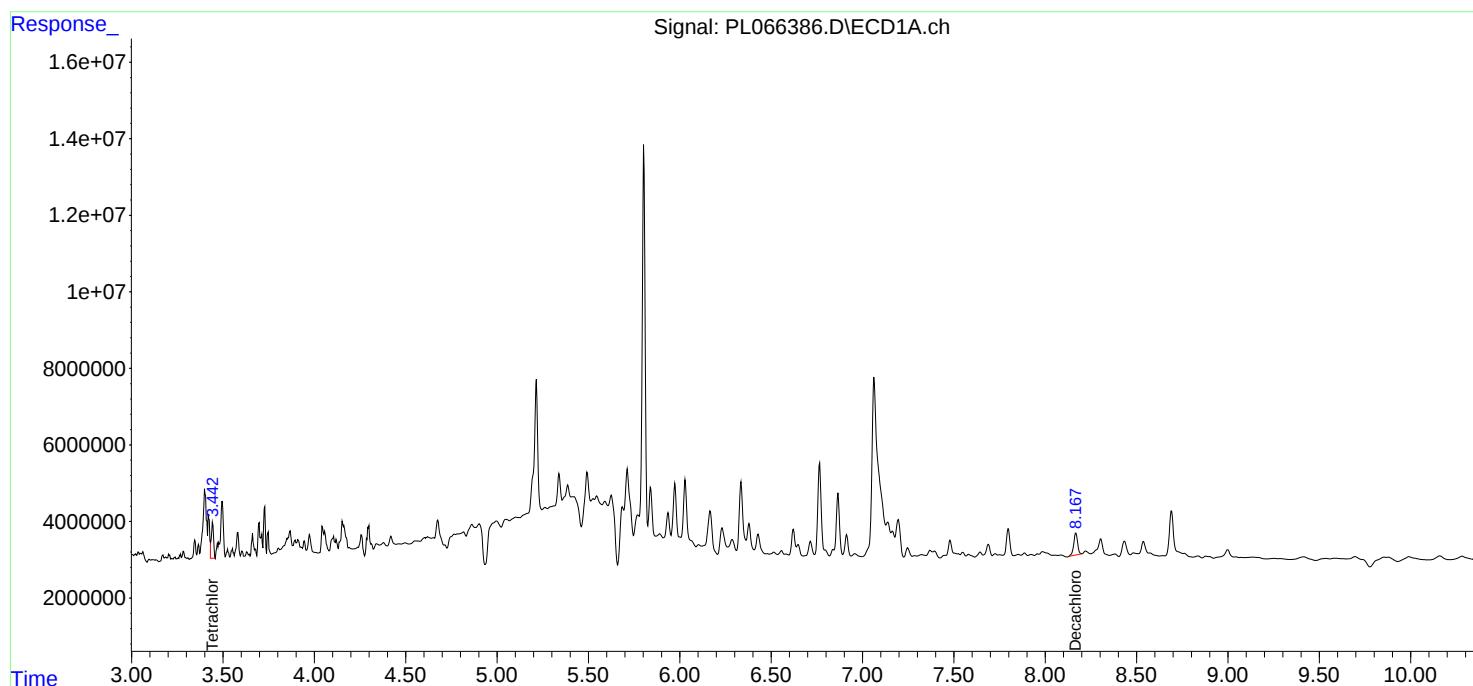

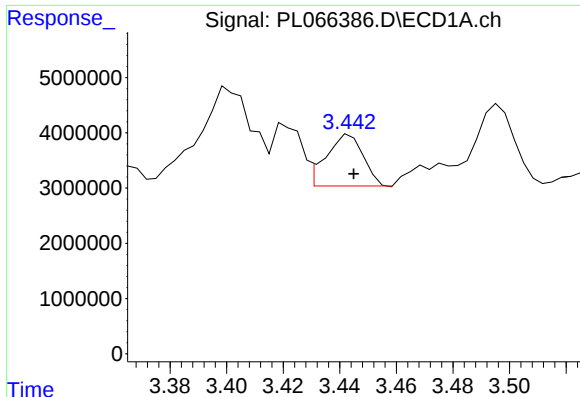


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: -0.003 min
Response: 8392412
Conc: 3.30 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SEDGWICK-COMP-1RE


Manual Integrations
APPROVED

Ankita
4/22/2021 2:52:33 PM

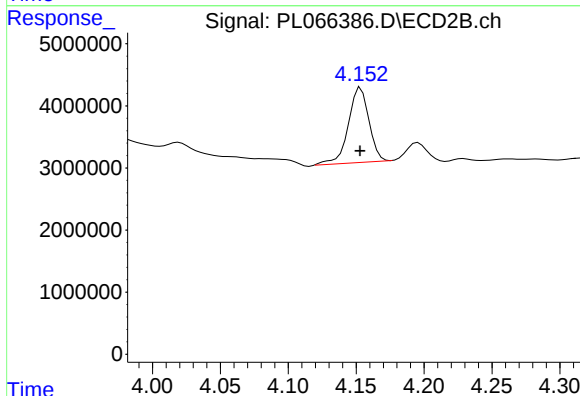


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 12737831
Conc: 3.17 ng/ml

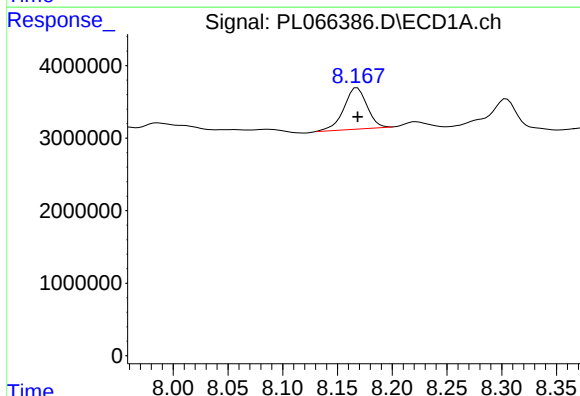

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 8379017
Conc: 3.51 ng/ml

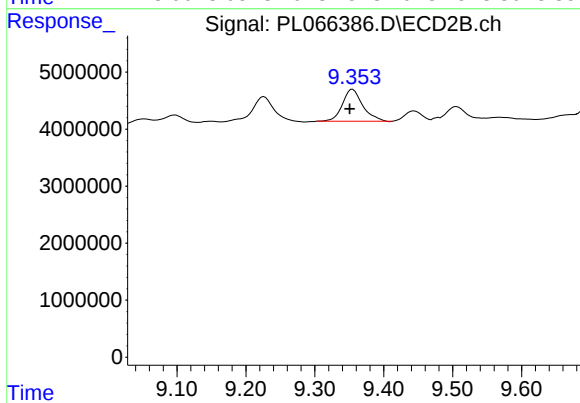

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.004 min
Response: 11514404
Conc: 3.53 ng/ml