

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
 Data File : PL066391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 14:25
 Operator : AR\AJ
 Sample : M2098-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-01-042021

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:52:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 18:13:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.154	29616065	48232403	11.636	11.990
28)	SA Decachlor...	8.177	9.360	29248933	43302295	12.262	13.259
Target Compounds							
12)	B 4,4'-DDE	5.598	6.542	1455192	2942156	0.390m	0.711 #
17)	MA 4,4'-DDT	6.343	7.341	491721	737825	0.154m	0.217m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
Data File : PL066391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 14:25
Operator : AR\AJ
Sample : M2098-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
HR-01-042021


Manual Integrations
APPROVED

Ankita
4/22/2021 2:52:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 18:13:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

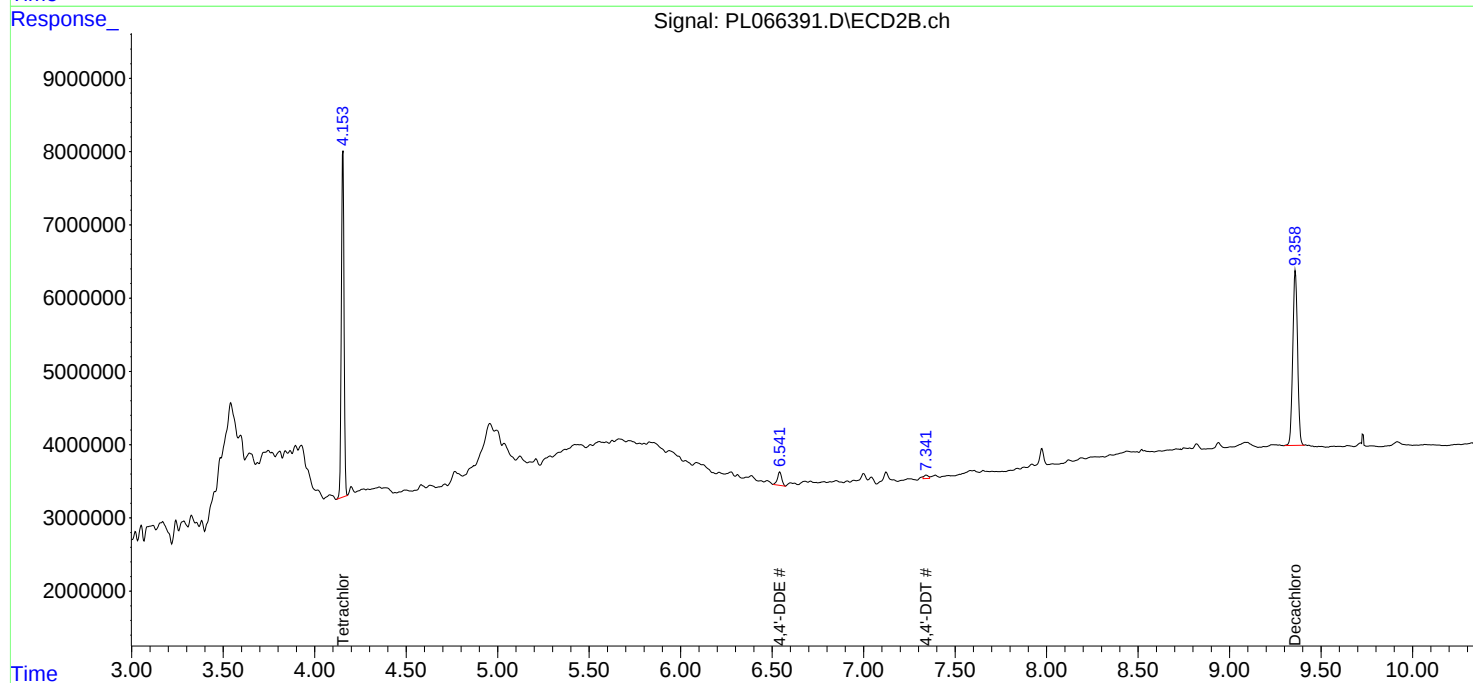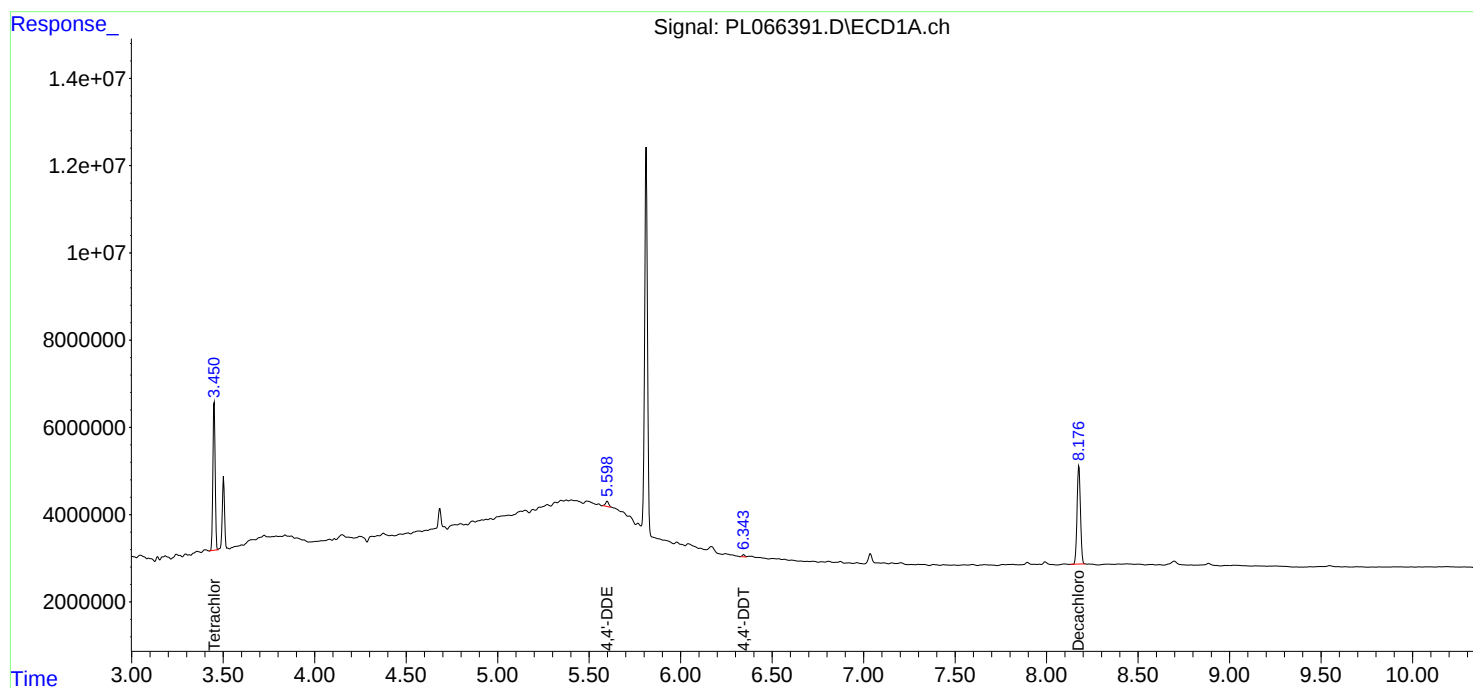

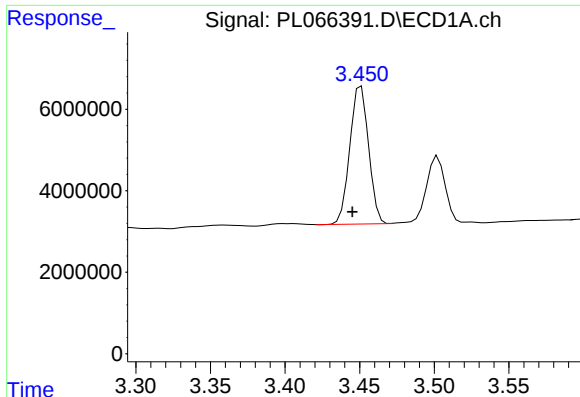


#1 Tetrachloro-m-xylene

R.T.: 3.451 min
Delta R.T.: 0.006 min
Response: 29616065
Conc: 11.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-042021


Manual Integrations
APPROVED

Ankita
4/22/2021 2:52:39 PM

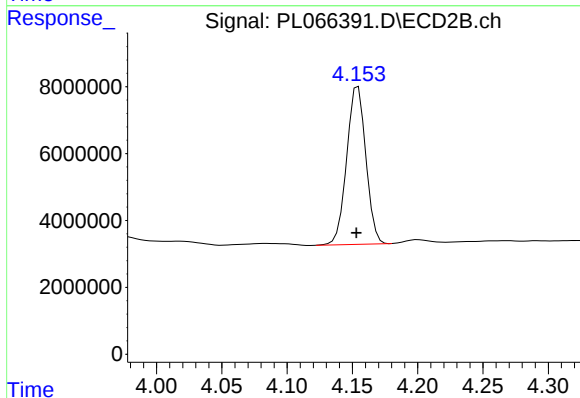


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 48232403
Conc: 11.99 ng/ml

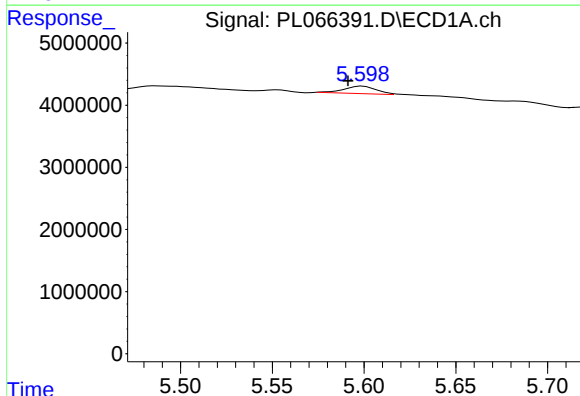


#12 4,4'-DDE

R.T.: 5.598 min
Delta R.T.: 0.007 min
Response: 1455192
Conc: 0.39 ng/ml m

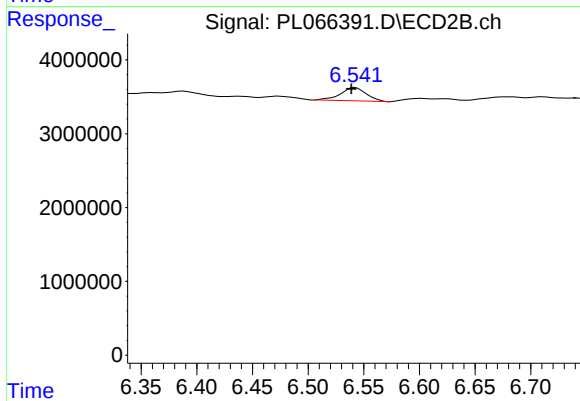

#12 4,4'-DDE

R.T.: 6.542 min
Delta R.T.: 0.003 min
Response: 2942156
Conc: 0.71 ng/ml

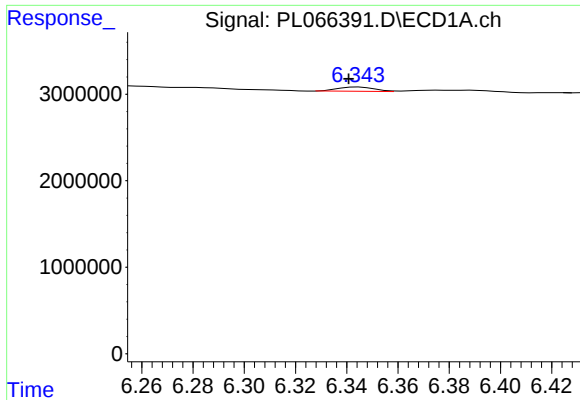


#17 4,4'-DDT

R.T.: 6.343 min
Delta R.T.: 0.003 min
Response: 491721
Conc: 0.15 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HR-01-042021


Manual Integrations
APPROVED

Ankita
4/22/2021 2:52:39 PM

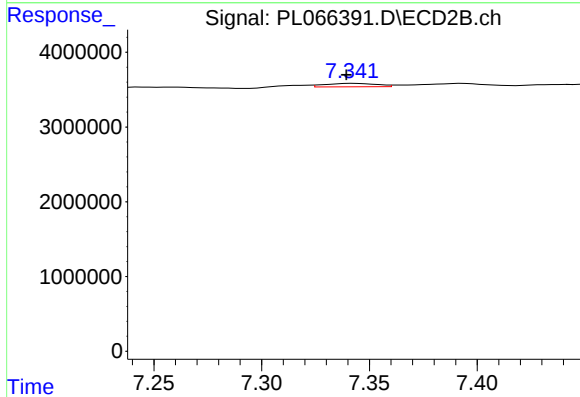


#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: 0.001 min
Response: 737825
Conc: 0.22 ng/ml m

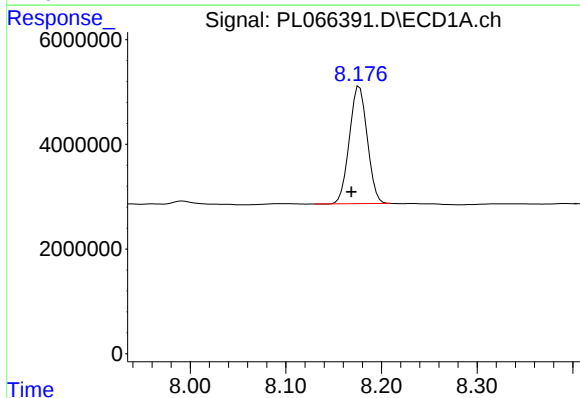

#28 Decachlorobiphenyl

R.T.: 8.177 min
Delta R.T.: 0.008 min
Response: 29248933
Conc: 12.26 ng/ml

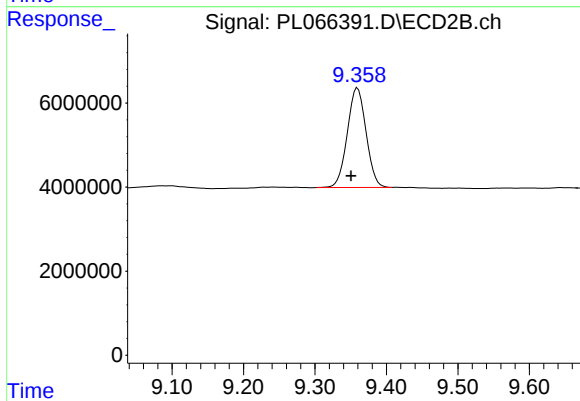

#28 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: 0.009 min
Response: 43302295
Conc: 13.26 ng/ml