

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
 Data File : PL066409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 19:15
 Operator : AR\AJ
 Sample : M2111-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-2

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:53:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 06:06:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.154	71010994	81781960	27.899m	20.331 #
28)	SA Decachlor...	8.168	9.354	39944772	52716954	16.746	16.142

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
Data File : PL066409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 19:15
Operator : AR\AJ
Sample : M2111-02
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
S-2


Manual Integrations
APPROVED

Ankita
4/22/2021 2:53:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 06:06:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

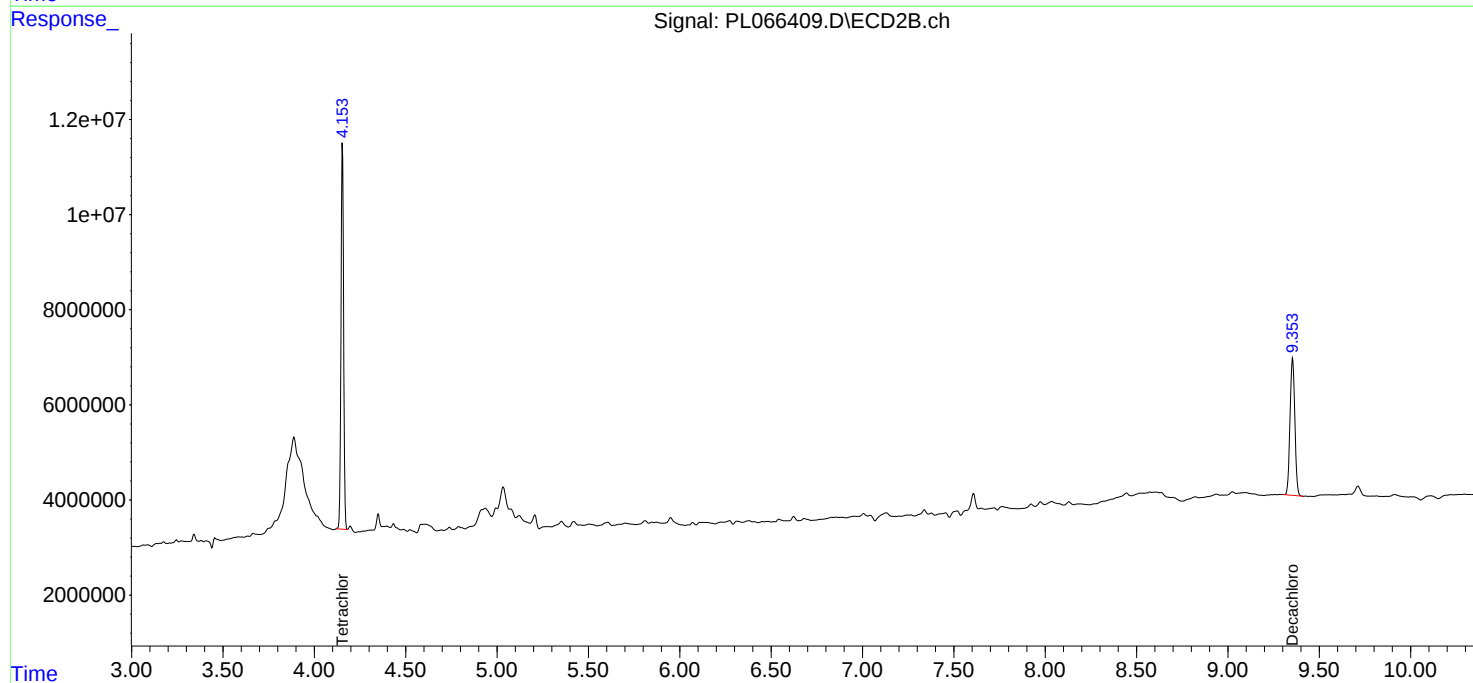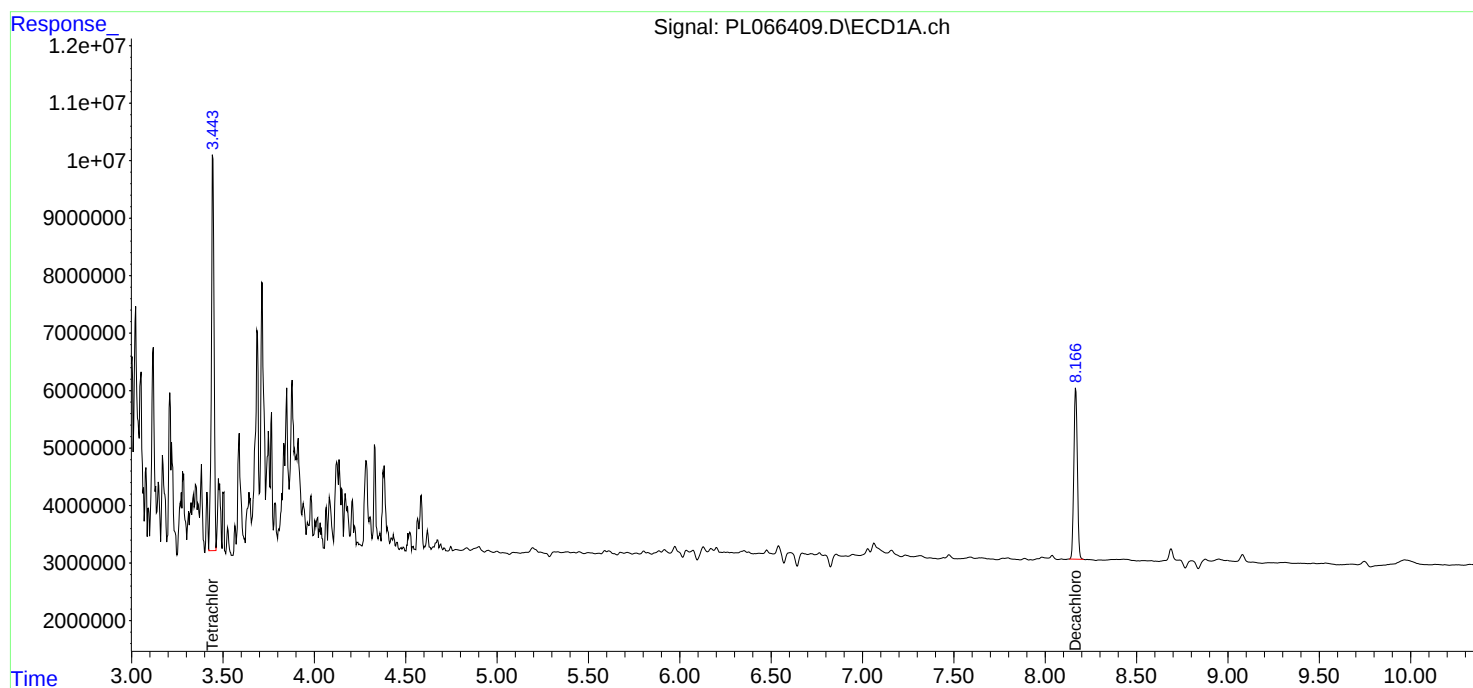

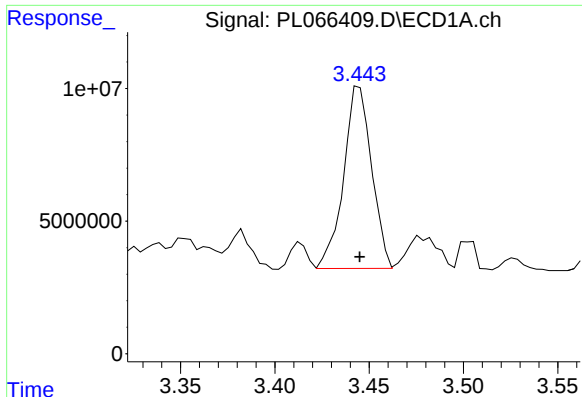

#1 Tetrachloro-m-xylene

R.T.: 3.443 min

Delta R.T.: -0.002 min


Response: 71010994

Conc: 27.90 ng/ml m

Instrument :
ECD_L
ClientSampleId :
S-2

Manual Integrations
APPROVED

Ankita
4/22/2021 2:53:22 PM

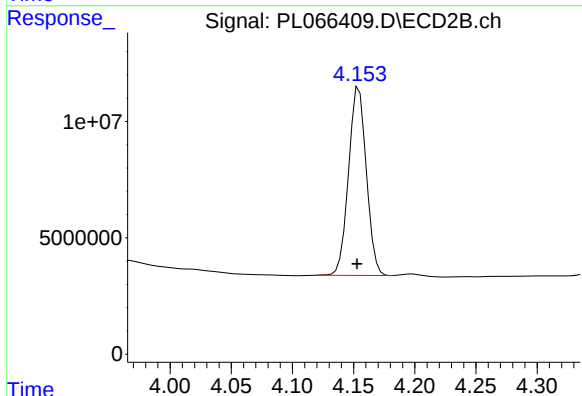


#1 Tetrachloro-m-xylene

R.T.: 4.154 min

Delta R.T.: 0.002 min

Response: 81781960

Conc: 20.33 ng/ml

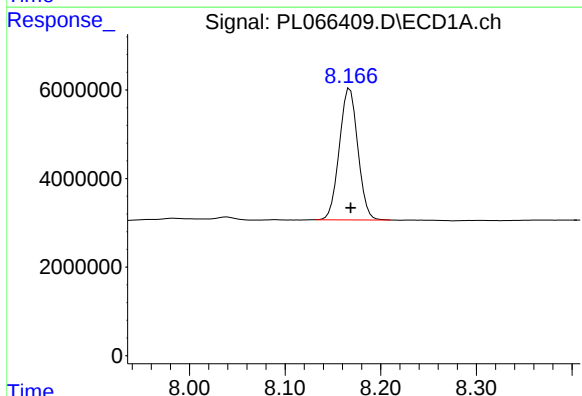


#28 Decachlorobiphenyl

R.T.: 8.168 min

Delta R.T.: 0.000 min

Response: 39944772

Conc: 16.75 ng/ml

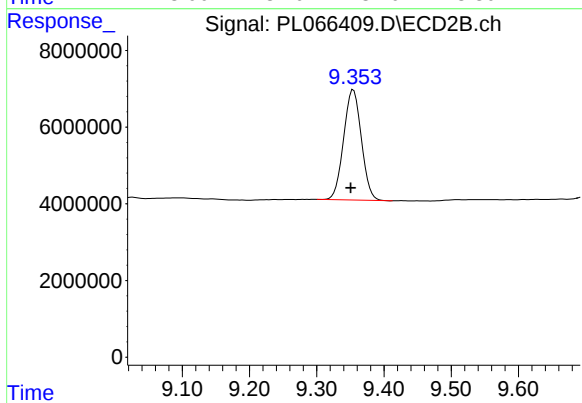

#28 Decachlorobiphenyl

R.T.: 9.354 min

Delta R.T.: 0.004 min

Response: 52716954

Conc: 16.14 ng/ml