

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
 Data File : PL066411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 19:43
 Operator : AR\AJ
 Sample : M2111-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-4

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:53:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 06:06:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.154	48916434	79644696	19.219	19.799
28)	SA Decachlor...	8.168	9.354	39537495	57927999	16.576	17.737
Target Compounds							
17)	MA 4,4'-DDT	6.336	7.338	1684229	1789261	0.528m	0.527m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
Data File : PL066411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 19:43
Operator : AR\AJ
Sample : M2111-04
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
S-4


Manual Integrations
APPROVED

Ankita
4/22/2021 2:53:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 06:06:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

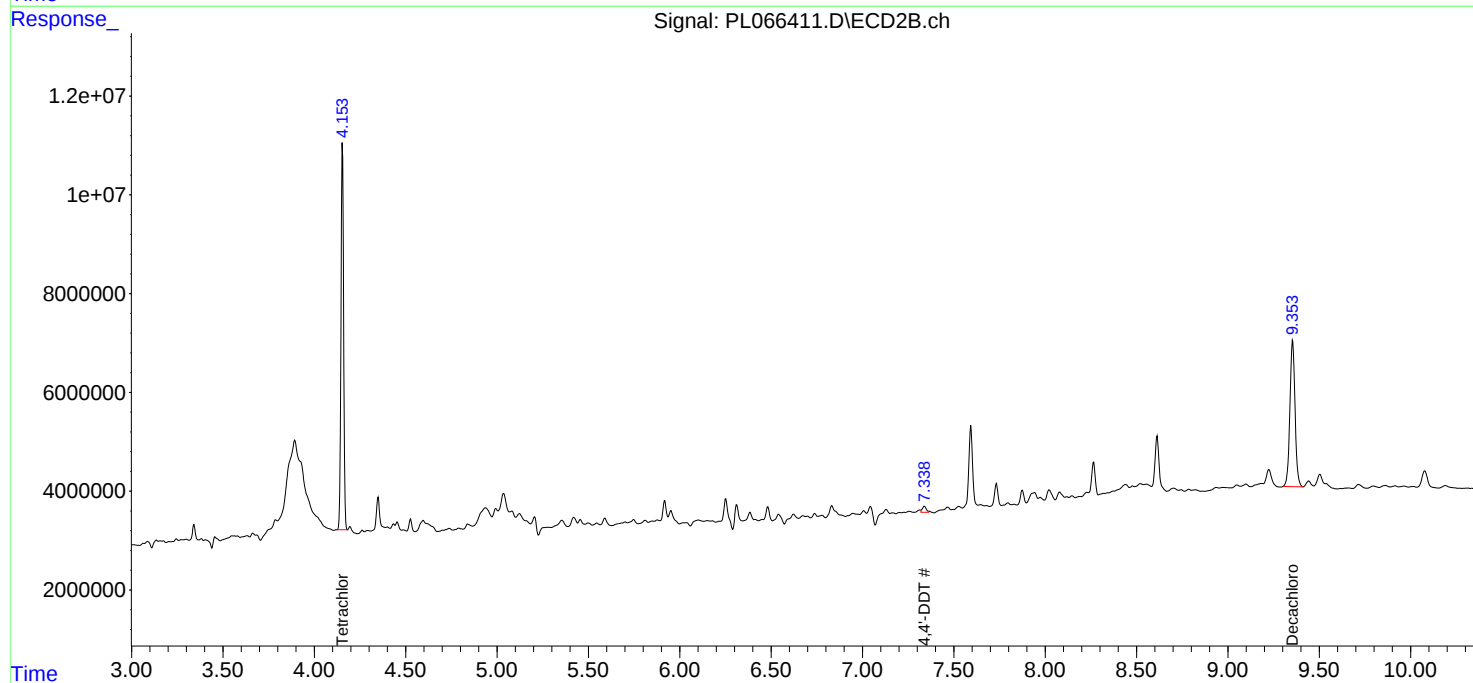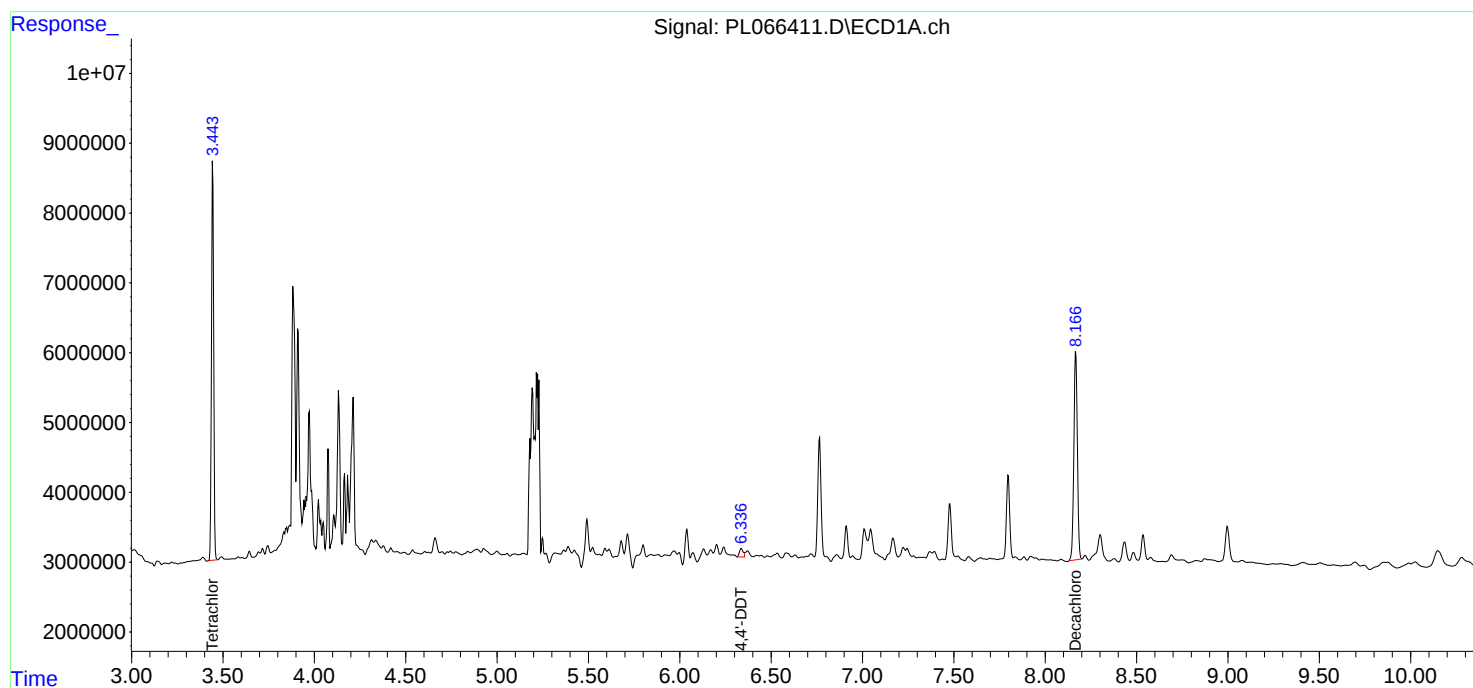

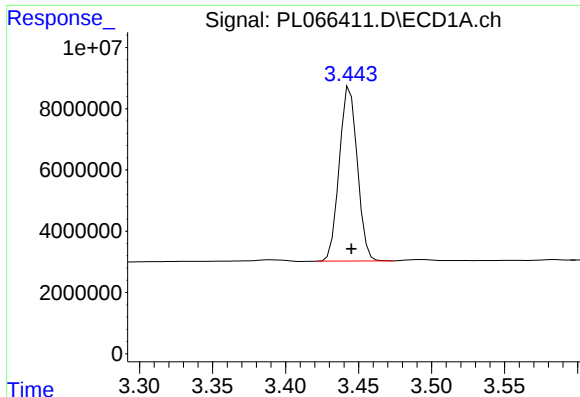


#1 Tetrachloro-m-xylene

R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 48916434
Conc: 19.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-4


Manual Integrations
APPROVED

Ankita
4/22/2021 2:53:26 PM

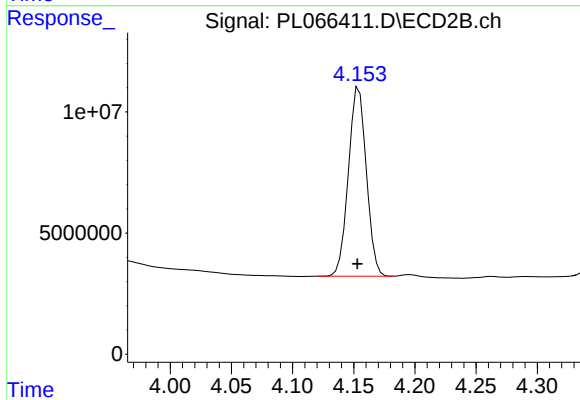


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 79644696
Conc: 19.80 ng/ml

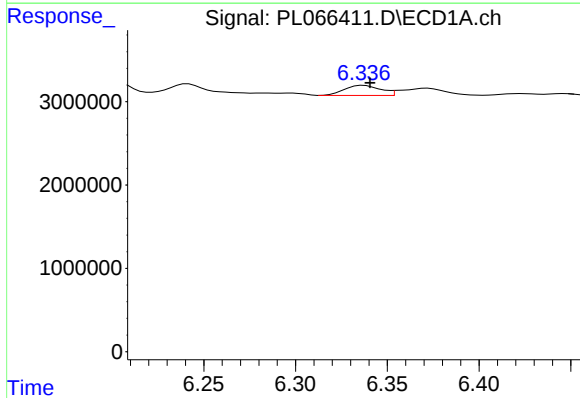


#17 4,4'-DDT

R.T.: 6.336 min
Delta R.T.: -0.005 min
Response: 1684229
Conc: 0.53 ng/ml m

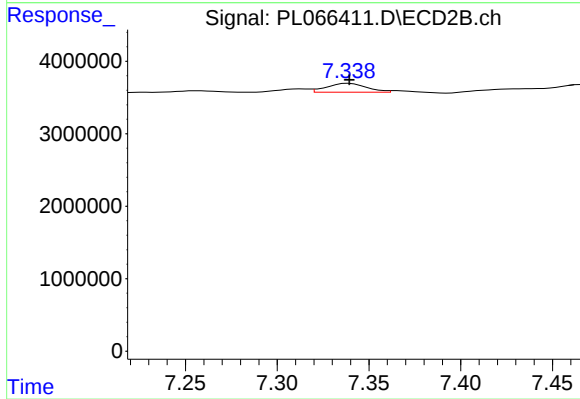

#17 4,4'-DDT

R.T.: 7.338 min
Delta R.T.: -0.002 min
Response: 1789261
Conc: 0.53 ng/ml m

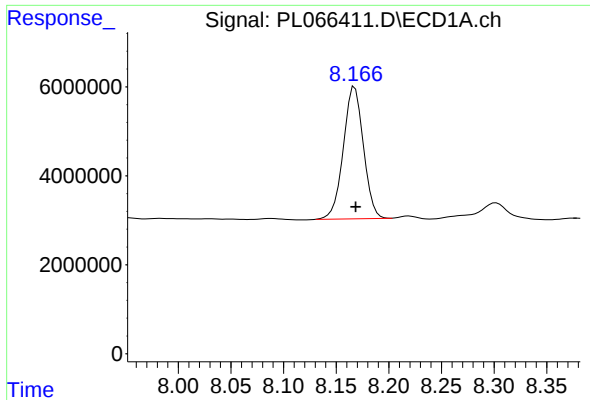


#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 39537495
Conc: 16.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-4

Manual Integrations
APPROVED

Ankita
4/22/2021 2:53:26 PM

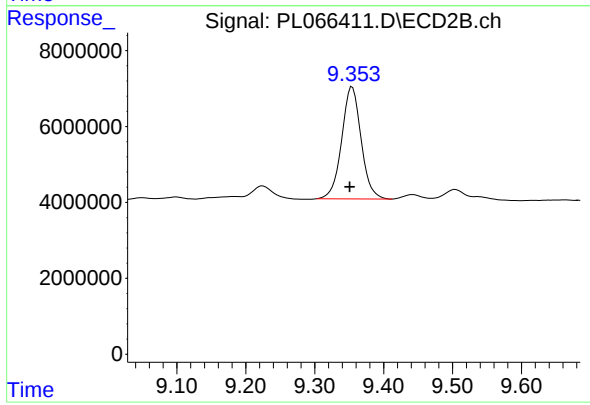

#28 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: 0.004 min
Response: 57927999
Conc: 17.74 ng/ml