

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
 Data File : PL066413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 20:12
 Operator : AR\AJ
 Sample : M2111-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-10

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:53:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 06:07:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.154	47220885	80027764	18.552m	19.895
28)	SA Decachlor...	8.167	9.356	37303009	51941664	15.639	15.904
Target Compounds							
12)	B 4,4'-DDE	5.591	6.542	155.9E6	183.1E6	41.783	44.226
16)	A 4,4'-DDD	6.102	7.040	1636698	5248377	0.497	1.534 #
17)	MA 4,4'-DDT	6.339	7.341	32551677	35052832	10.213	10.333m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
Data File : PL066413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 20:12
Operator : AR\AJ
Sample : M2111-06
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
S-10


Manual Integrations
APPROVED

Ankita
4/22/2021 2:53:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 06:07:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

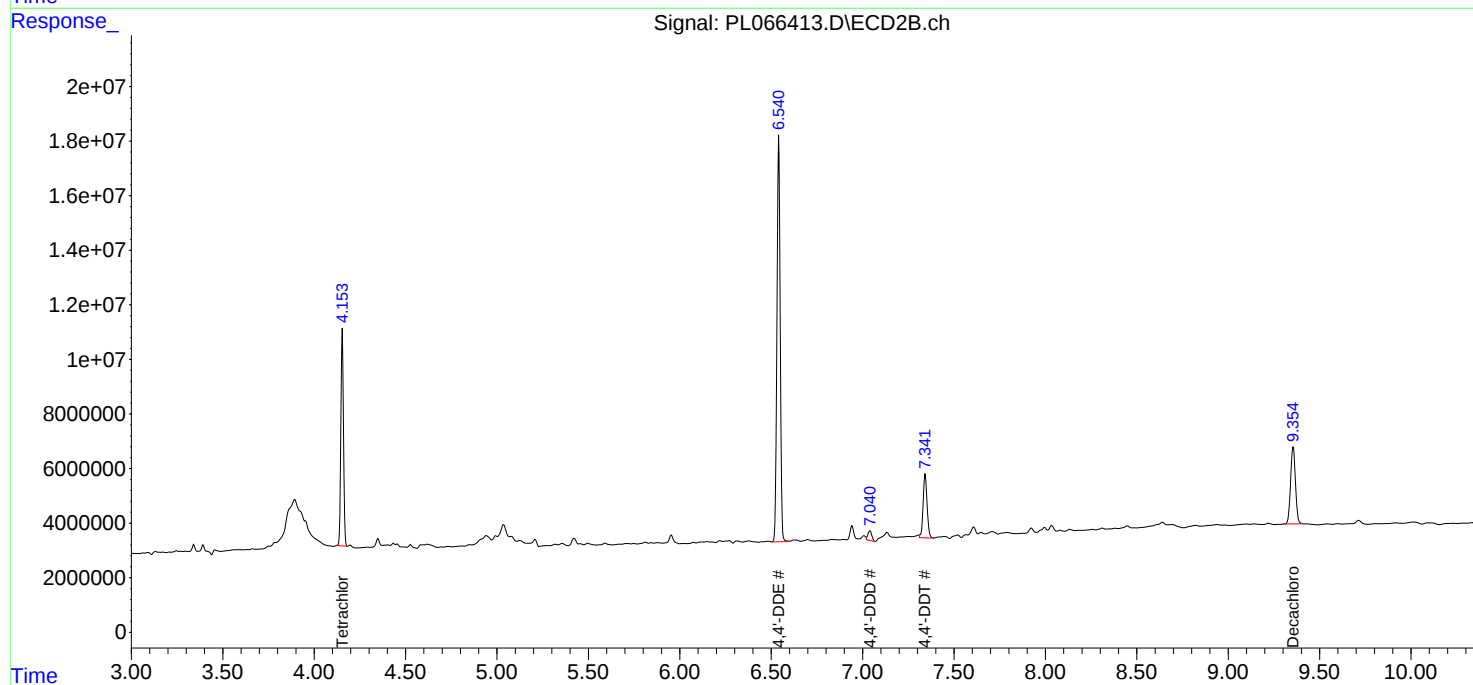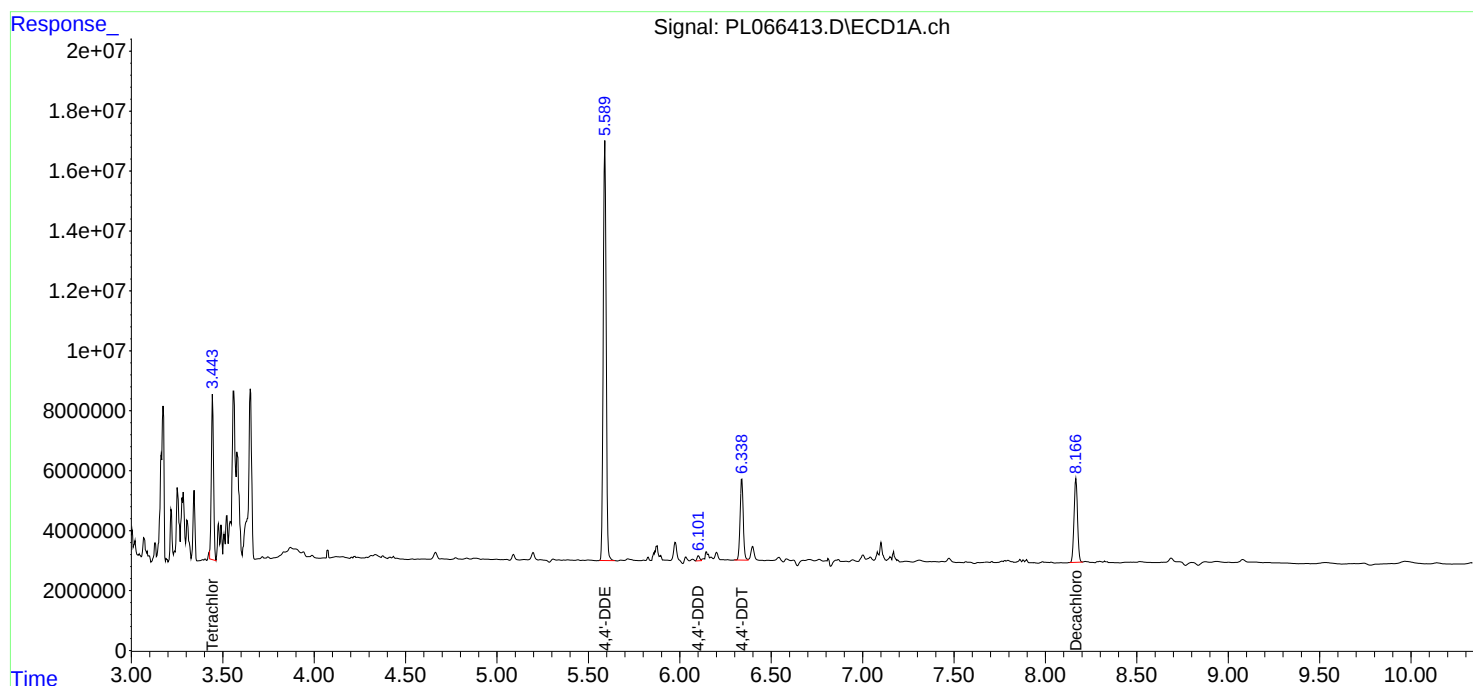

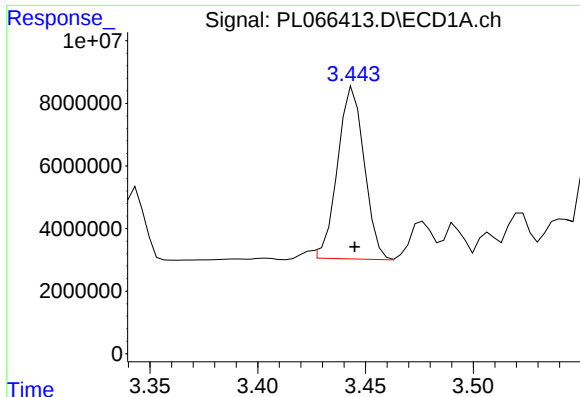


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.002 min
Response: 47220885
Conc: 18.55 ng/ml m

Instrument :
ECD_L
ClientSampleId :
S-10


Manual Integrations
APPROVED

Ankita
4/22/2021 2:53:29 PM

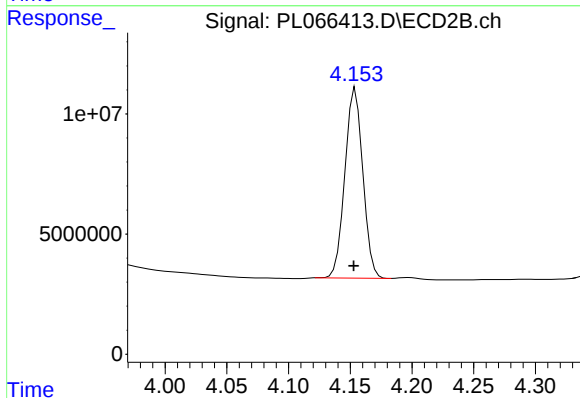


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 80027764
Conc: 19.89 ng/ml

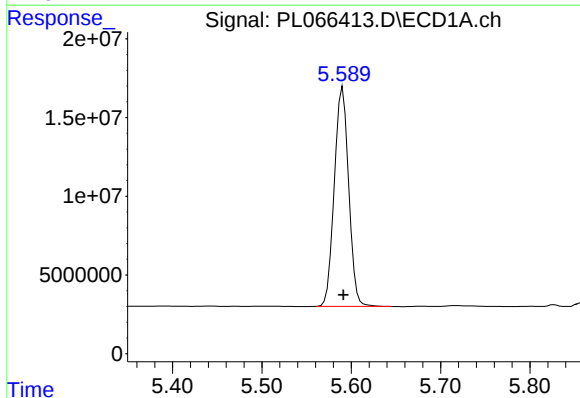


#12 4,4'-DDE

R.T.: 5.591 min
Delta R.T.: 0.000 min
Response: 155855726
Conc: 41.78 ng/ml

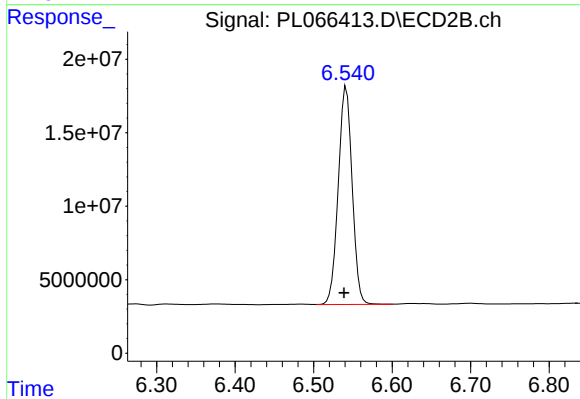

#12 4,4'-DDE

R.T.: 6.542 min
Delta R.T.: 0.003 min
Response: 183056815
Conc: 44.23 ng/ml

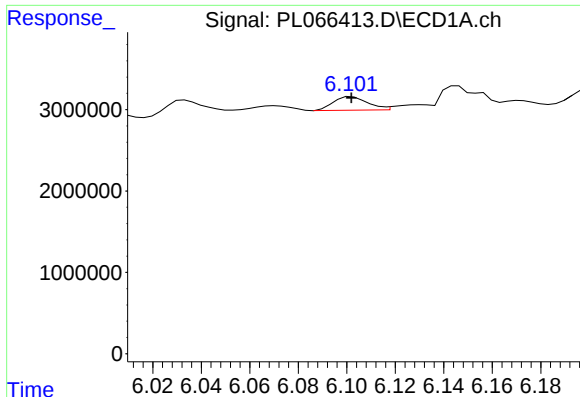


#16 4,4'-DDD

R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 1636698
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-10


Manual Integrations
APPROVED

Ankita
4/22/2021 2:53:29 PM

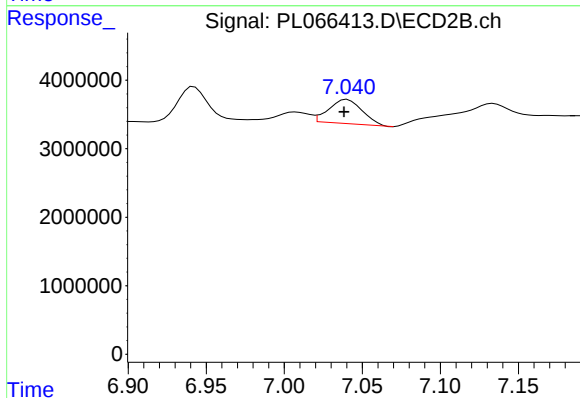


#16 4,4'-DDD

R.T.: 7.040 min
Delta R.T.: 0.002 min
Response: 5248377
Conc: 1.53 ng/ml

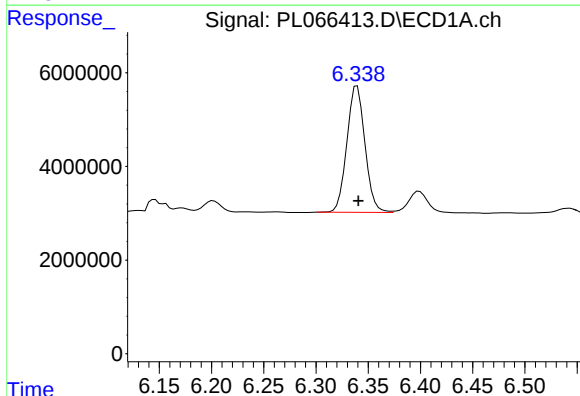


#17 4,4'-DDT

R.T.: 6.339 min
Delta R.T.: -0.001 min
Response: 32551677
Conc: 10.21 ng/ml

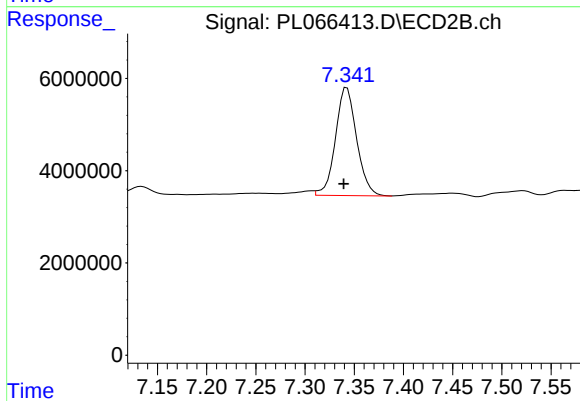

#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: 0.002 min
Response: 35052832
Conc: 10.33 ng/ml m

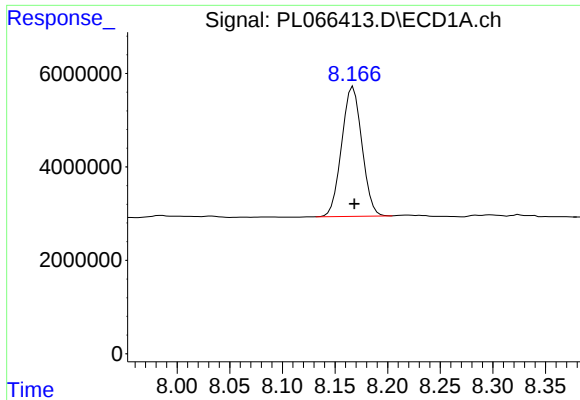


#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: -0.001 min
Response: 37303009
Conc: 15.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-10

Manual Integrations
APPROVED

Ankita
4/22/2021 2:53:29 PM

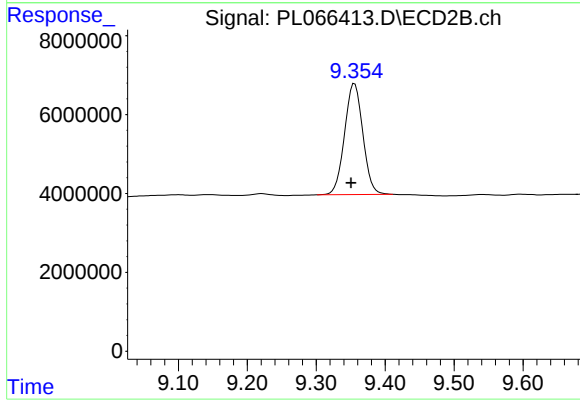

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.005 min
Response: 51941664
Conc: 15.90 ng/ml