

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
 Data File : PL075230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2022 07:10
 Operator : AR\AJ
 Sample : N2930-04
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:15:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.642	5011099	12940161	8.526	8.169
28)	SA Decachlor...	11.641	10.391	5227926	12178767	9.750	8.875
Target Compounds							
7)	B delta-BHC	0.000	6.410	0	196368	N.D.	0.092 #
9)	A Endosulfan I	8.511f	0.000	91311	0	0.145	N.D. #
12)	B 4,4'-DDE	0.000	7.631	0	182306	N.D.	0.112 #
13)	MA Dieldrin	0.000	7.767	0	431110	N.D.	0.248 #
14)	MA Endrin	0.000	8.071f	0	575839	N.D.	0.370 #
16)	A 4,4'-DDD	9.204	0.000	455423	0	0.921	N.D. #
17)	MA 4,4'-DDT	0.000	8.468	0	1110136	N.D.	0.776 #
19)	B Endosulfa...	0.000	8.778	0	320720	N.D.	0.214 #
20)	A Methoxychlor	0.000	9.041f	0	319613	N.D.	0.394 #
21)	B Endrin ke...	10.187f	0.000	116629	0	0.190	N.D. #
27)	Chlordane-5	0.000	8.131	0	1106728	N.D.	21.482 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
Data File : PL075230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2022 07:10
Operator : AR\AJ
Sample : N2930-04
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:15:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

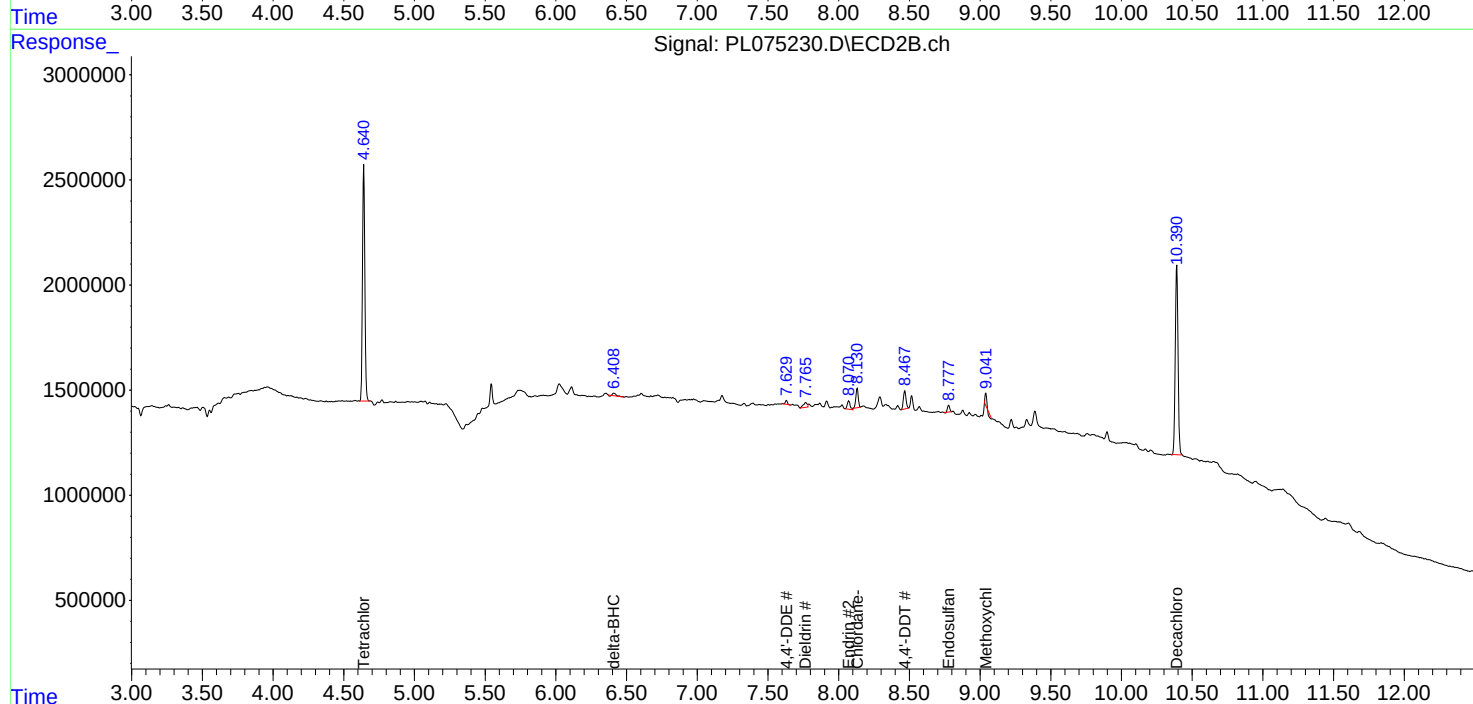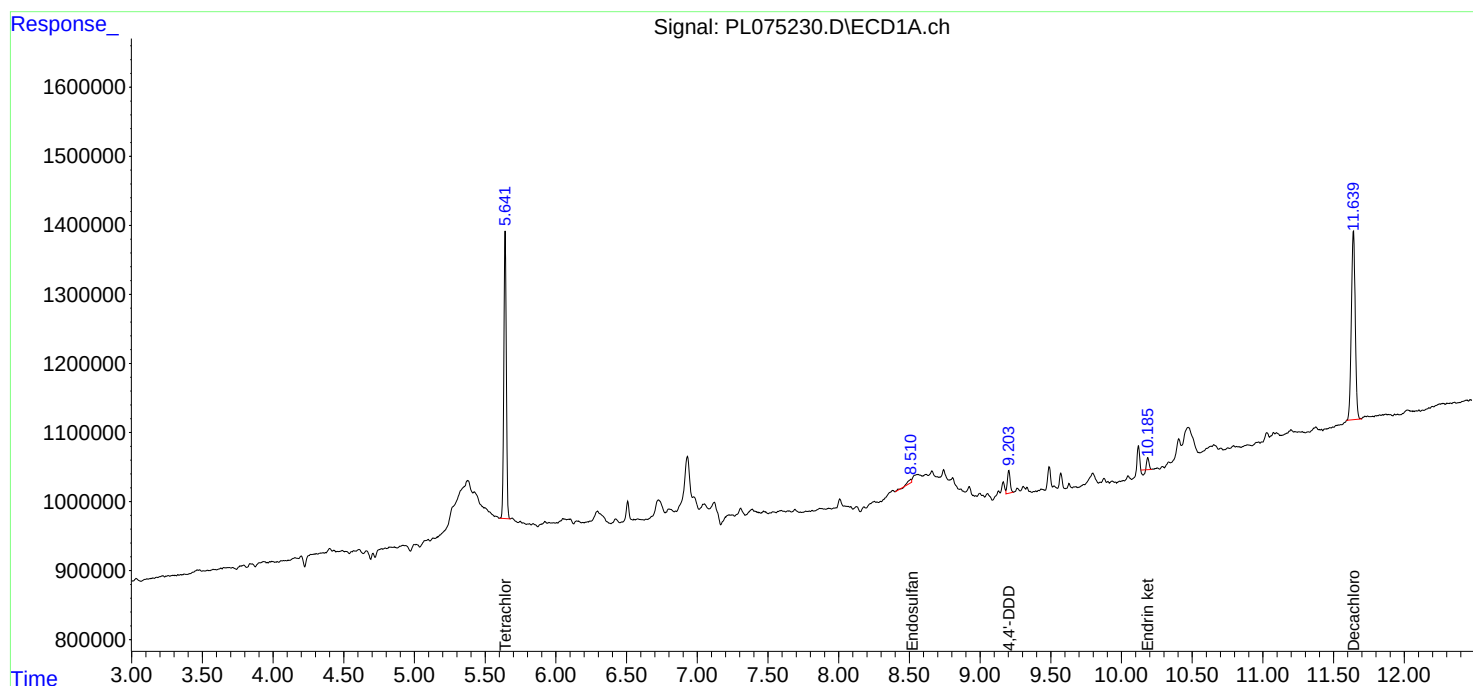


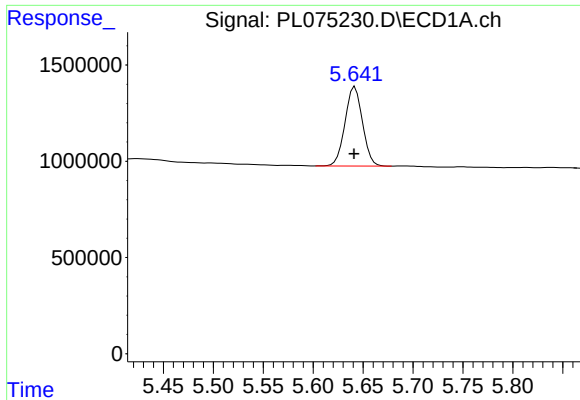

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 5011099
Conc: 8.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

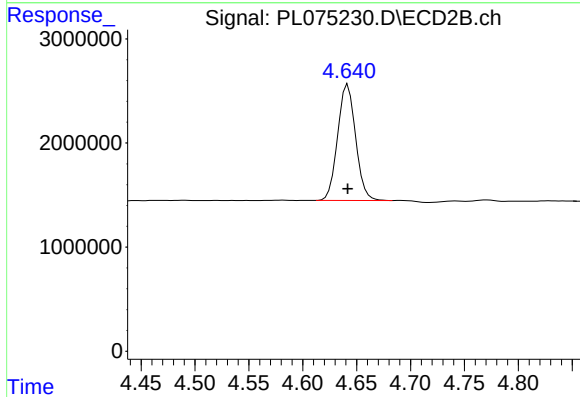


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 12940161
Conc: 8.17 ng/ml

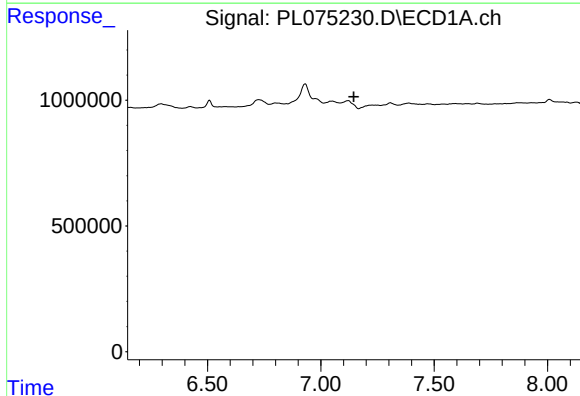


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

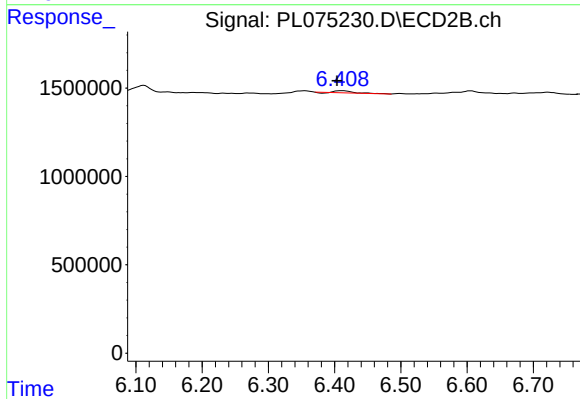

#7 delta-BHC


R.T.: 6.410 min
Delta R.T.: 0.006 min
Response: 196368
Conc: 0.09 ng/ml

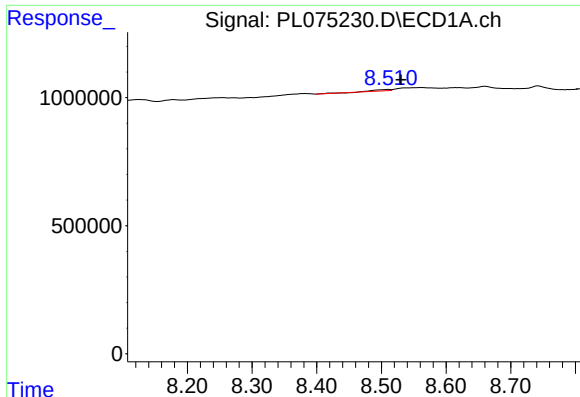

#9 Endosulfan I


R.T.: 8.511 min
Delta R.T.: -0.019 min
Response: 91311
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

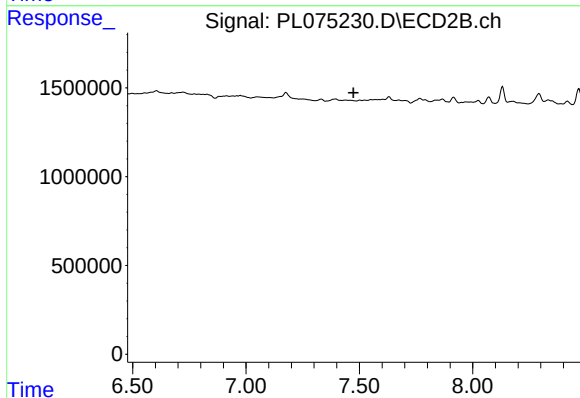


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.475 min
Response: 0
Conc: N.D.

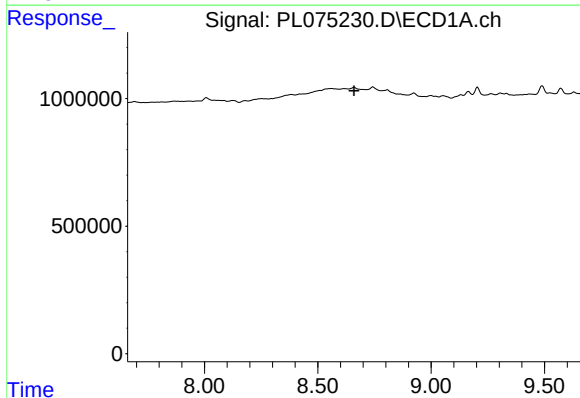


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 8.660 min
Response: 0
Conc: N.D.

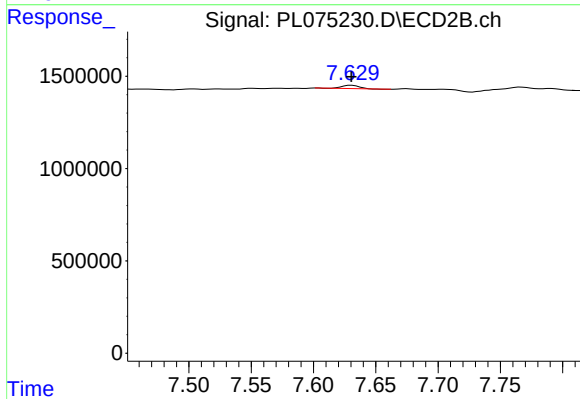

#12 4,4'-DDE


R.T.: 7.631 min
Delta R.T.: 0.000 min
Response: 182306
Conc: 0.11 ng/ml

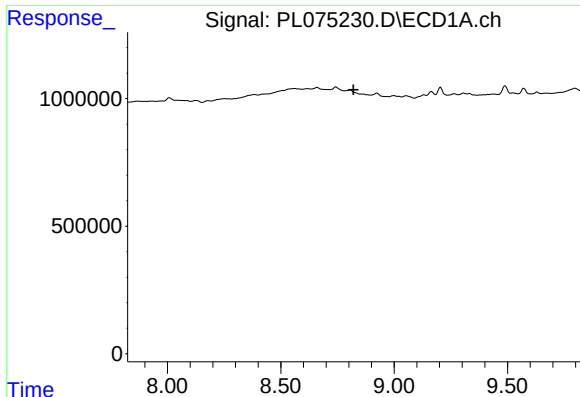

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

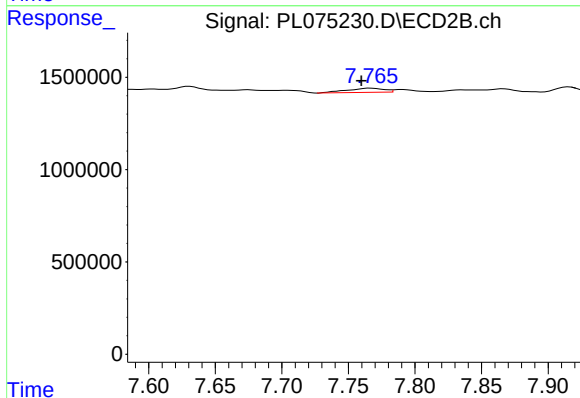


#13 Dieldrin

R.T.: 7.767 min
Delta R.T.: 0.007 min
Response: 431110
Conc: 0.25 ng/ml

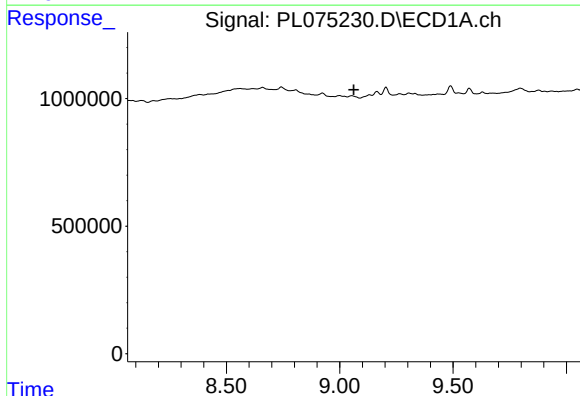


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

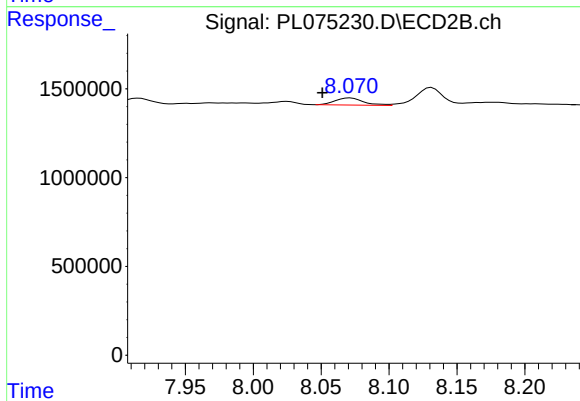

#14 Endrin


R.T.: 8.071 min
Delta R.T.: 0.021 min
Response: 575839
Conc: 0.37 ng/ml

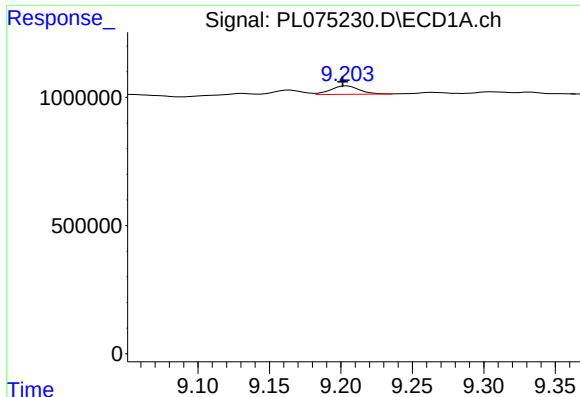

#16 4,4'-DDD


R.T.: 9.204 min
Delta R.T.: 0.003 min
Response: 455423
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

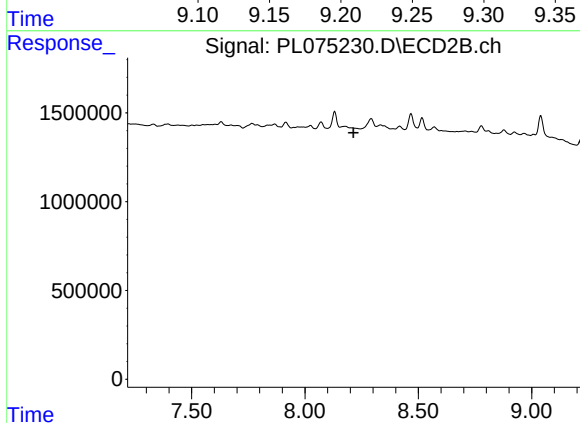


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.215 min
Response: 0
Conc: N.D.

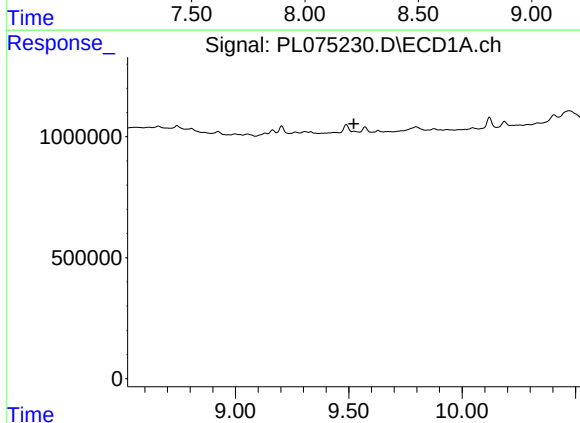


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

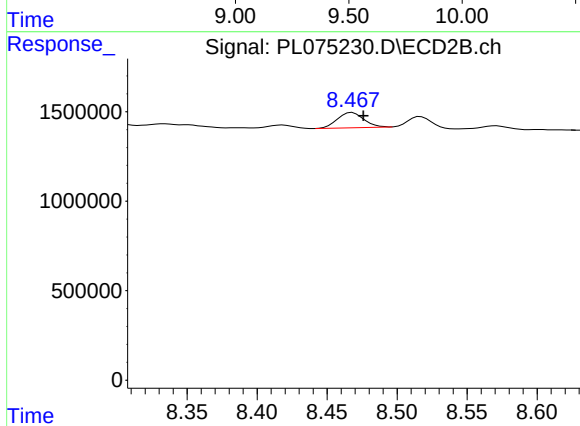

#17 4,4'-DDT


R.T.: 8.468 min
Delta R.T.: -0.008 min
Response: 1110136
Conc: 0.78 ng/ml

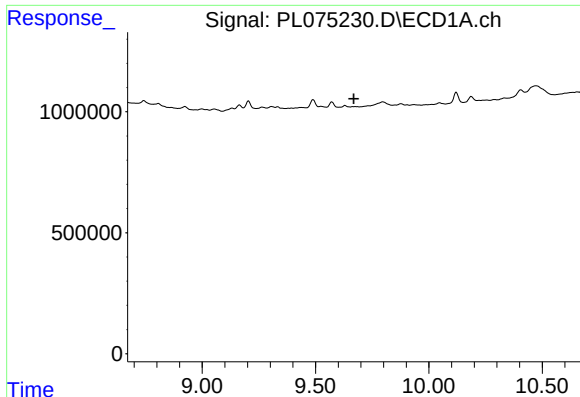

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

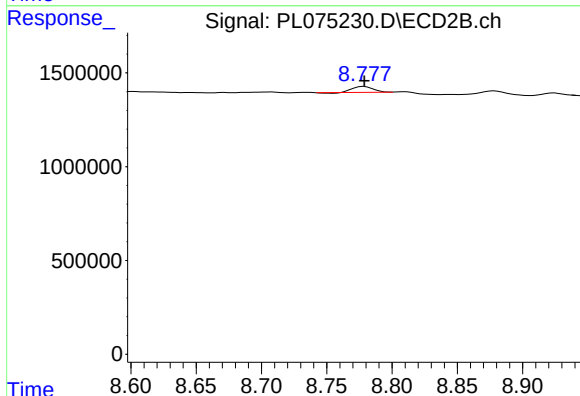


#19 Endosulfan Sulfate

R.T.: 8.778 min
Delta R.T.: 0.000 min
Response: 320720
Conc: 0.21 ng/ml

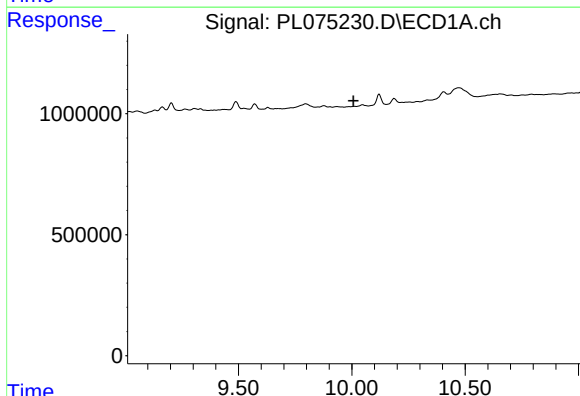


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 10.008 min
Response: 0
Conc: N.D.

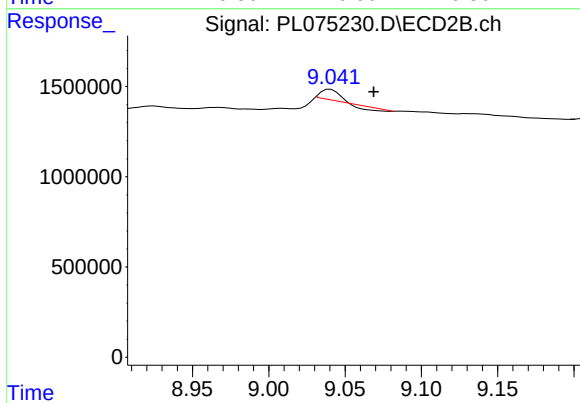

#20 Methoxychlor


R.T.: 9.041 min
Delta R.T.: -0.028 min
Response: 319613
Conc: 0.39 ng/ml

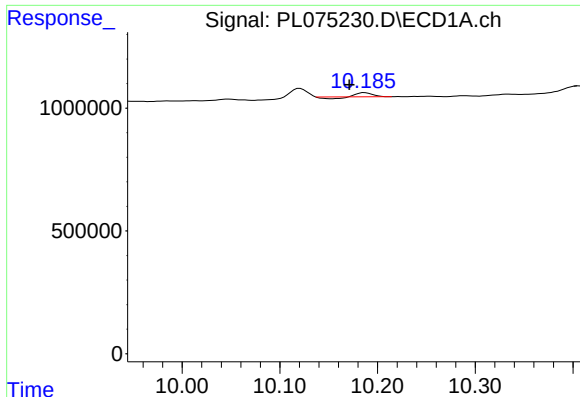

#21 Endrin ketone


R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 116629
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

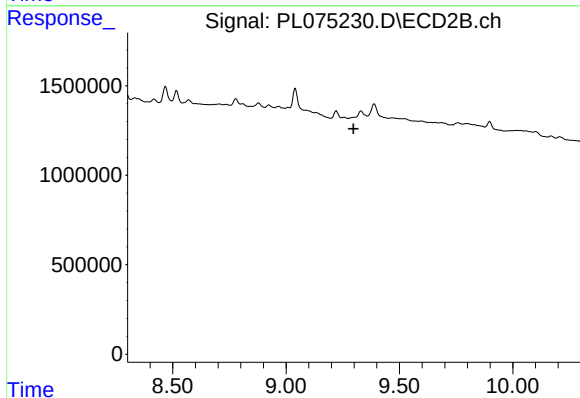


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

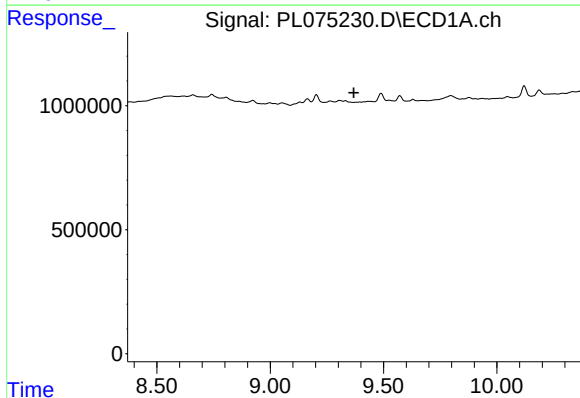


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.369 min
Response: 0
Conc: N.D.

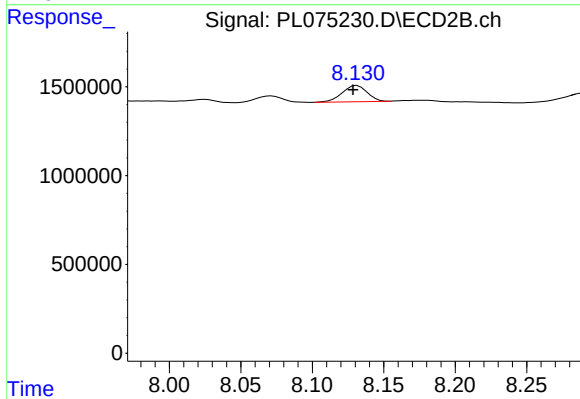

#27 Chlordane-5


R.T.: 8.131 min
Delta R.T.: 0.003 min
Response: 1106728
Conc: 21.48 ng/ml

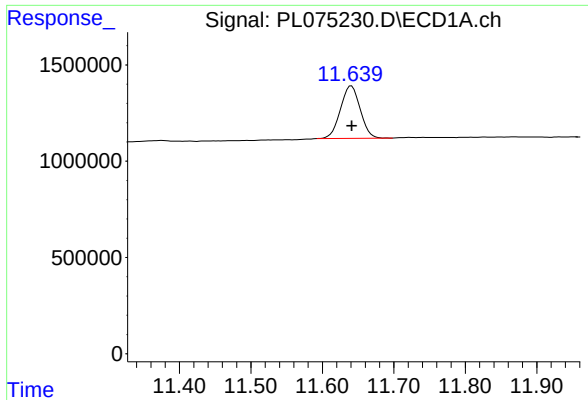

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 5227926
Conc: 9.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

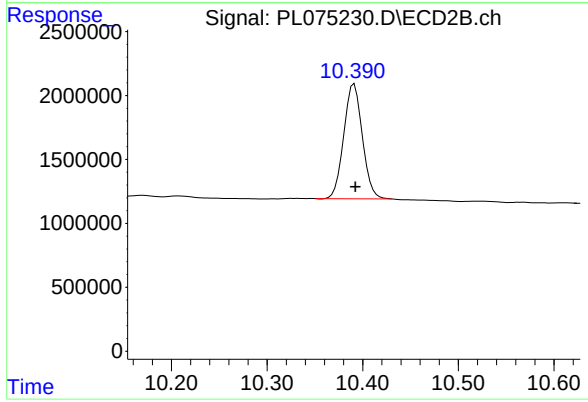

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.001 min
Response: 12178767
Conc: 8.87 ng/ml