

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
 Data File : PL075271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2022 19:36
 Operator : AR\AJ
 Sample : N3072-05
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:26:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.641	13426404	34731773	22.844	21.925
28)	SA Decachlor...	11.639	10.389	12456569	28414518	23.232	20.706
Target Compounds							
7)	B delta-BHC	0.000	6.403	0	228588	N.D.	0.107 #
8)	B Heptachlo...	8.124	0.000	3906854	0	5.723	N.D. #
11)	B alpha-Chl...	0.000	7.395f	0	155057	N.D.	0.085 #
13)	MA Dieldrin	0.000	7.760	0	3255166	N.D.	1.876 #
14)	MA Endrin	0.000	8.071f	0	913184	N.D.	0.587 #
15)	B Endosulfa...	9.302	0.000	210576	0	0.373	N.D. #
19)	B Endosulfa...	0.000	8.776	0	298064	N.D.	0.199 #
21)	B Endrin ke...	10.185	0.000	377533	0	0.615	N.D. #
26)	Chlordane-4	0.000	7.395f	0	155057	N.D.	0.800 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
Data File : PL075271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2022 19:36
Operator : AR\AJ
Sample : N3072-05
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:26:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

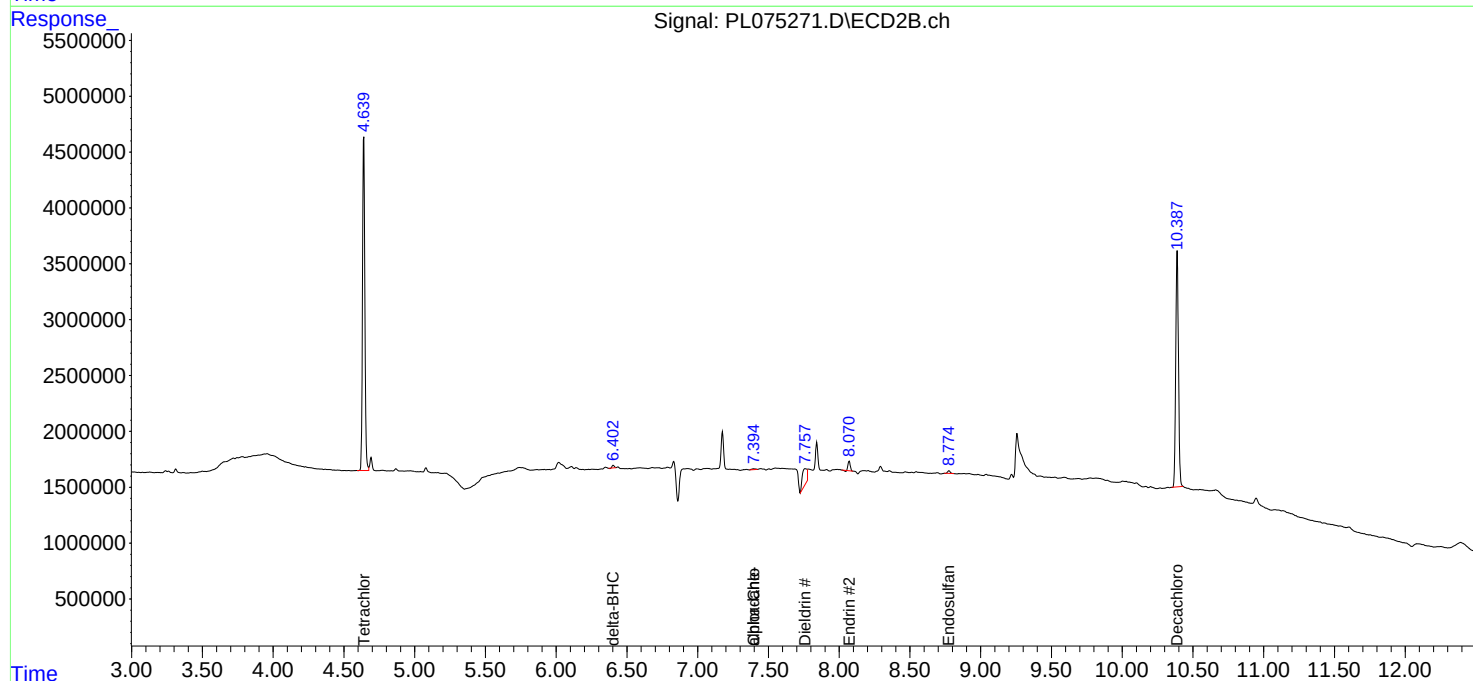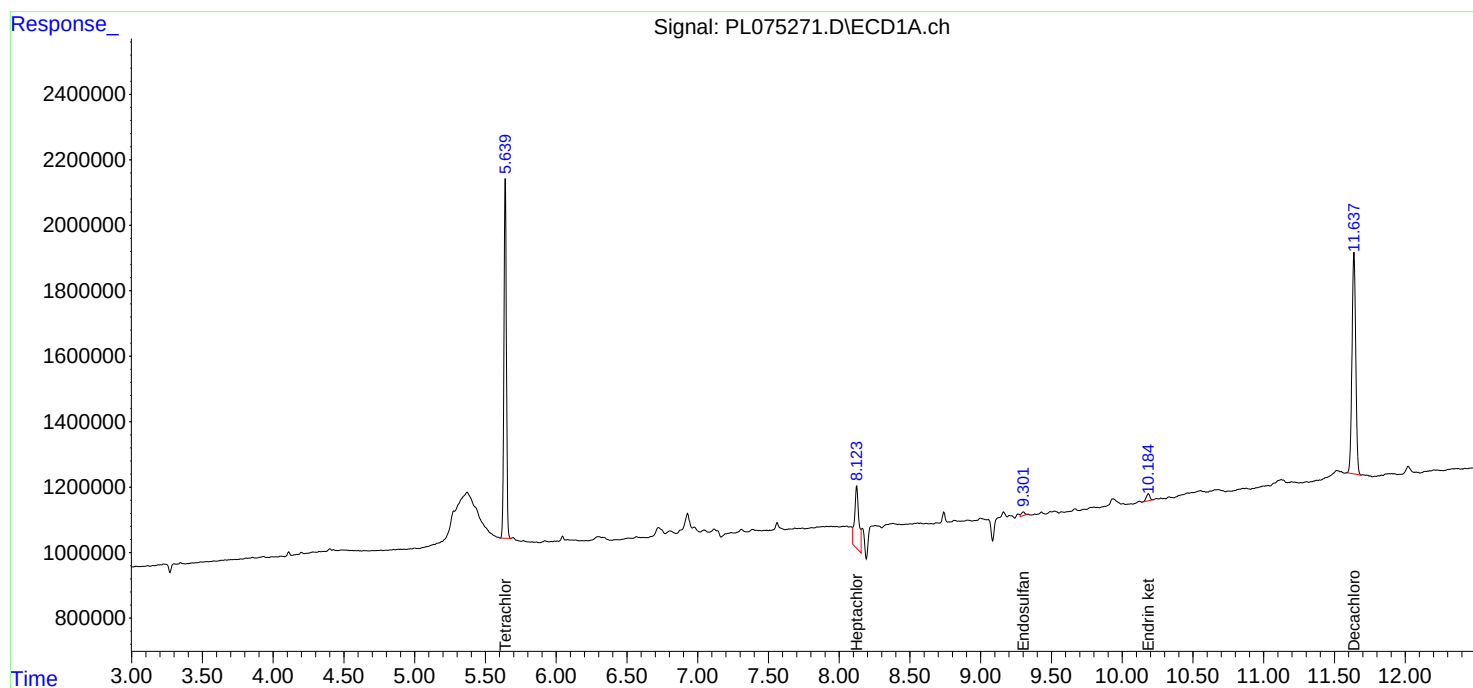


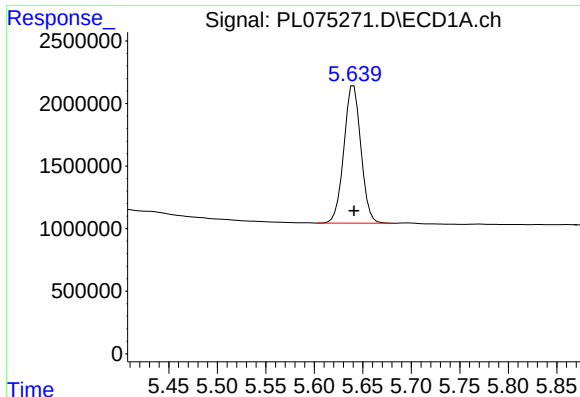

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 13426404
Conc: 22.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

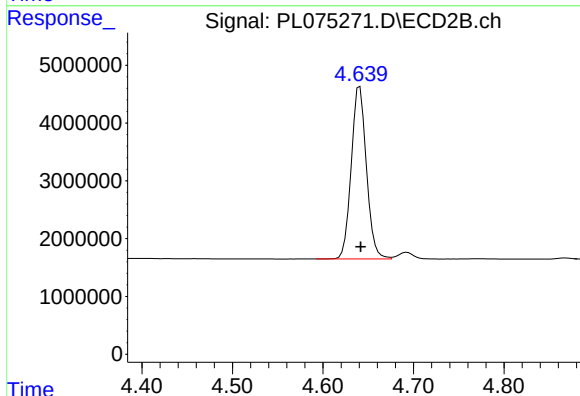


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 34731773
Conc: 21.92 ng/ml

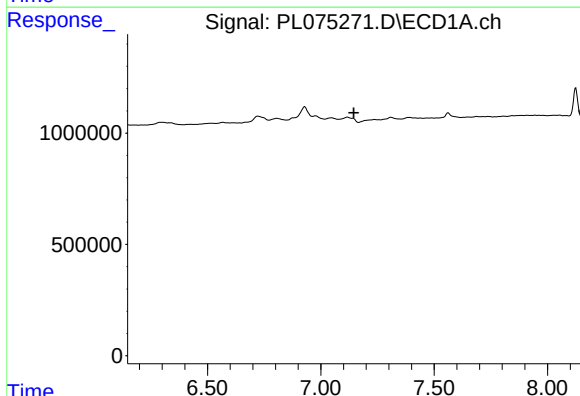


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

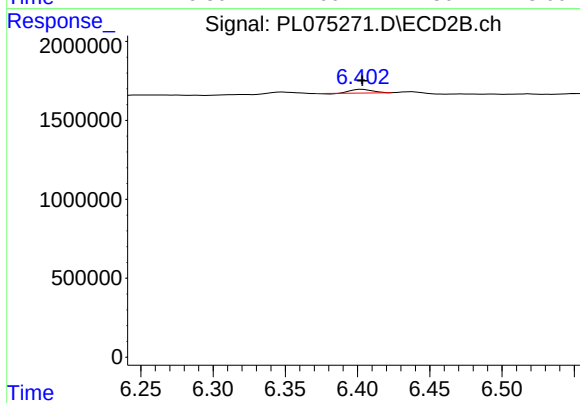

#7 delta-BHC


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 228588
Conc: 0.11 ng/ml

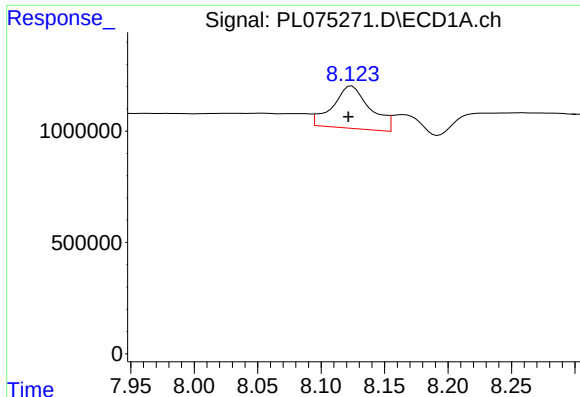

#8 Heptachlor epoxide


R.T.: 8.124 min
Delta R.T.: 0.003 min
Response: 3906854
Conc: 5.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

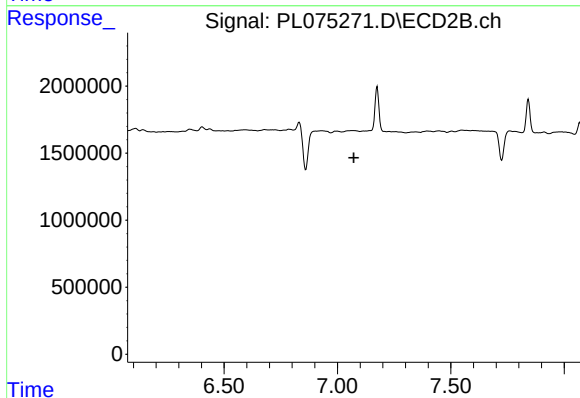


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

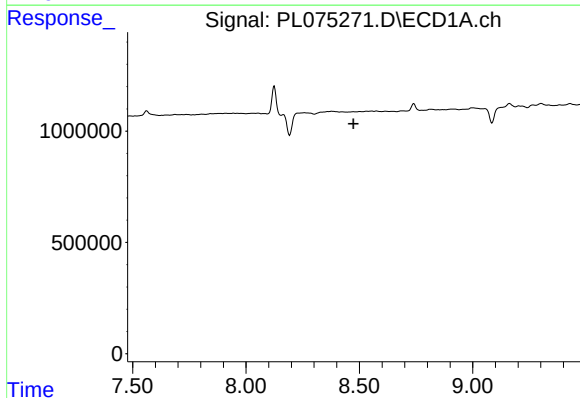


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

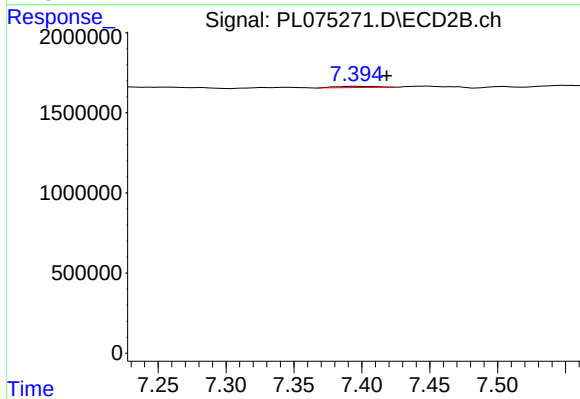

#11 alpha-Chlordane


R.T.: 7.395 min
Delta R.T.: -0.023 min
Response: 155057
Conc: 0.08 ng/ml

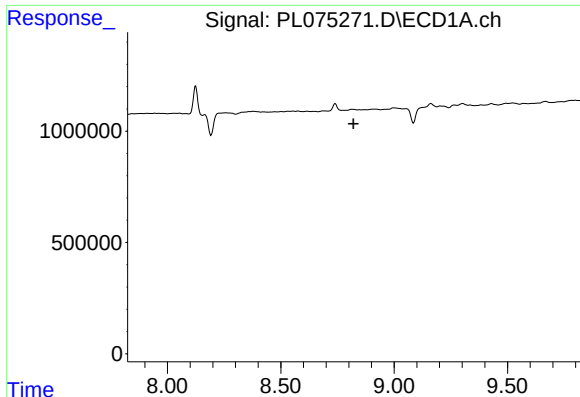

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

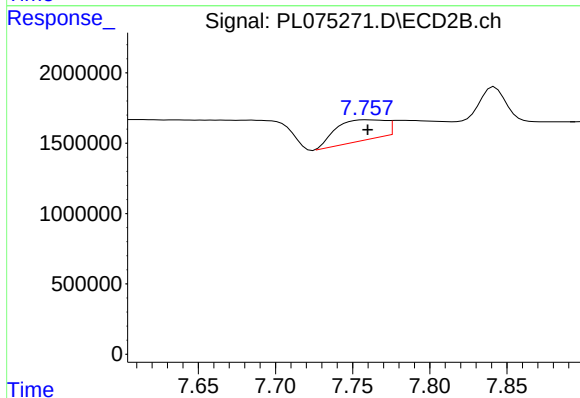


#13 Dieldrin

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 3255166
Conc: 1.88 ng/ml

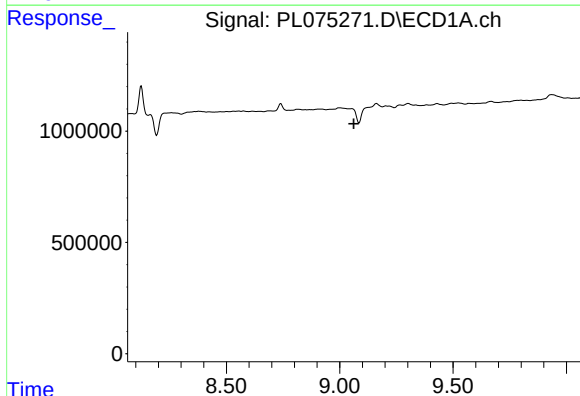


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

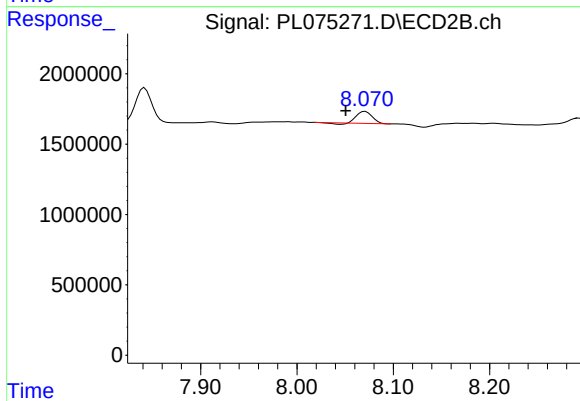

#14 Endrin


R.T.: 8.071 min
Delta R.T.: 0.020 min
Response: 913184
Conc: 0.59 ng/ml

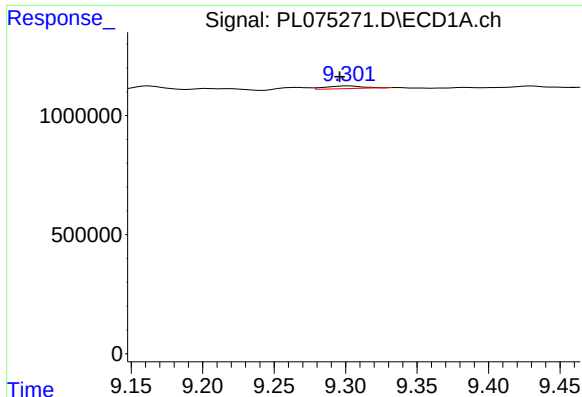

#15 Endosulfan II


R.T.: 9.302 min
Delta R.T.: 0.006 min
Response: 210576
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

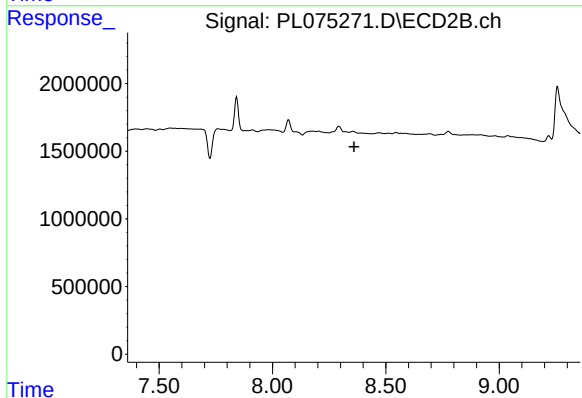


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

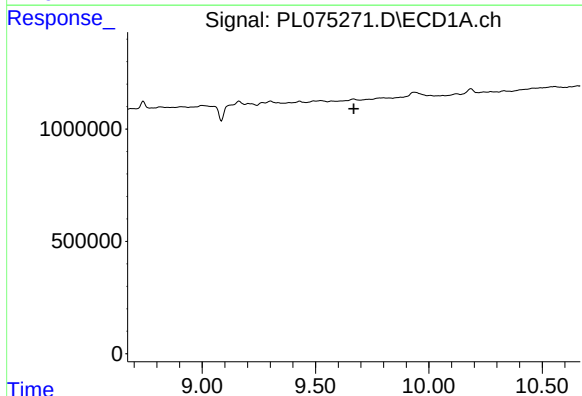


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.669 min
Response: 0
Conc: N.D.

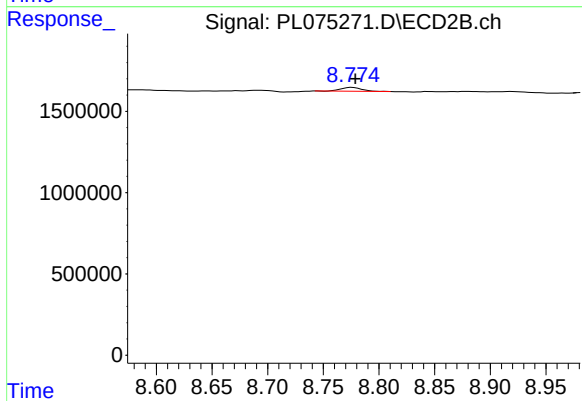

#19 Endosulfan Sulfate


R.T.: 8.776 min
Delta R.T.: -0.003 min
Response: 298064
Conc: 0.20 ng/ml

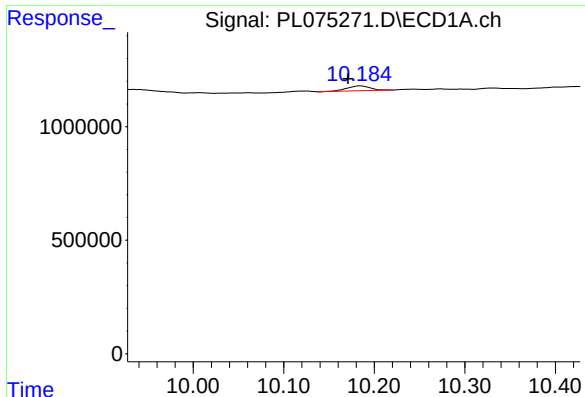

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.014 min
Response: 377533
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

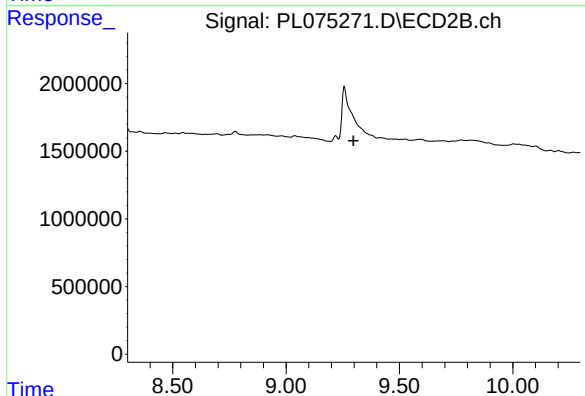


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

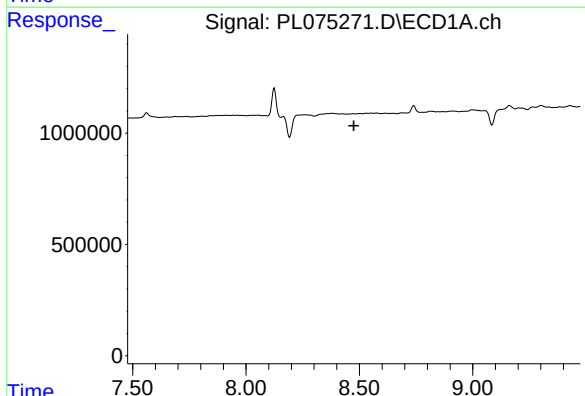


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

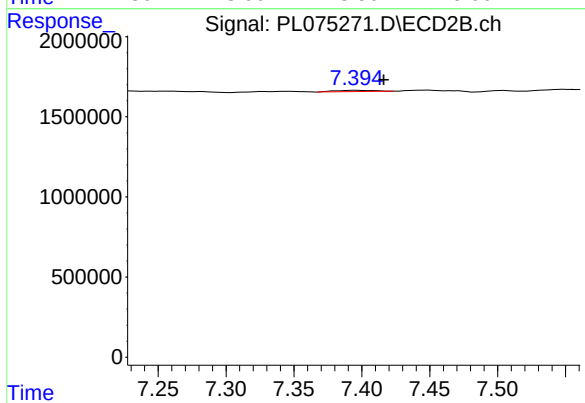

#26 Chlordane-4


R.T.: 7.395 min
Delta R.T.: -0.021 min
Response: 155057
Conc: 0.80 ng/ml

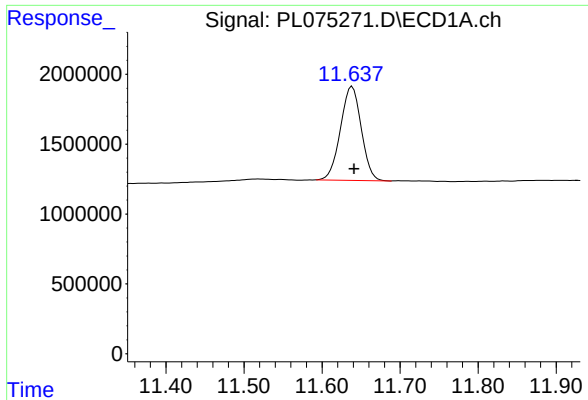

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 12456569
Conc: 23.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

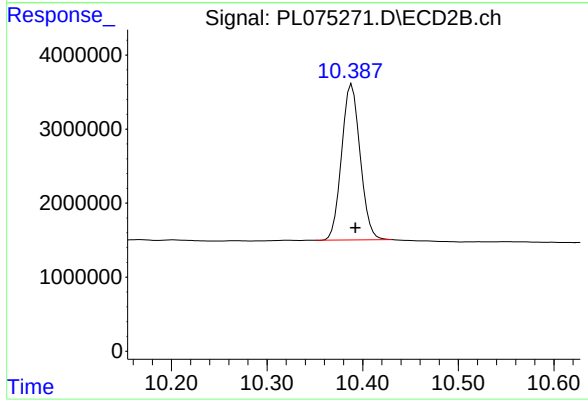

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.004 min
Response: 28414518
Conc: 20.71 ng/ml