

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
 Data File : PL075256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2022 15:27
 Operator : AR\AJ
 Sample : N2932-17MS
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P016-SS005-0006-01MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:22:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.641	6325498	16999316	10.762	10.731
28)	SA Decachlor...	11.638	10.390	7681648	18403775	14.327	13.411
Target Compounds							
12)	B 4,4'-DDE	8.660	7.629	5498582	11346462	9.452	6.967 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
Data File : PL075256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2022 15:27
Operator : AR\AJ
Sample : N2932-17MS
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
P016-SS005-0006-01MS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:22:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

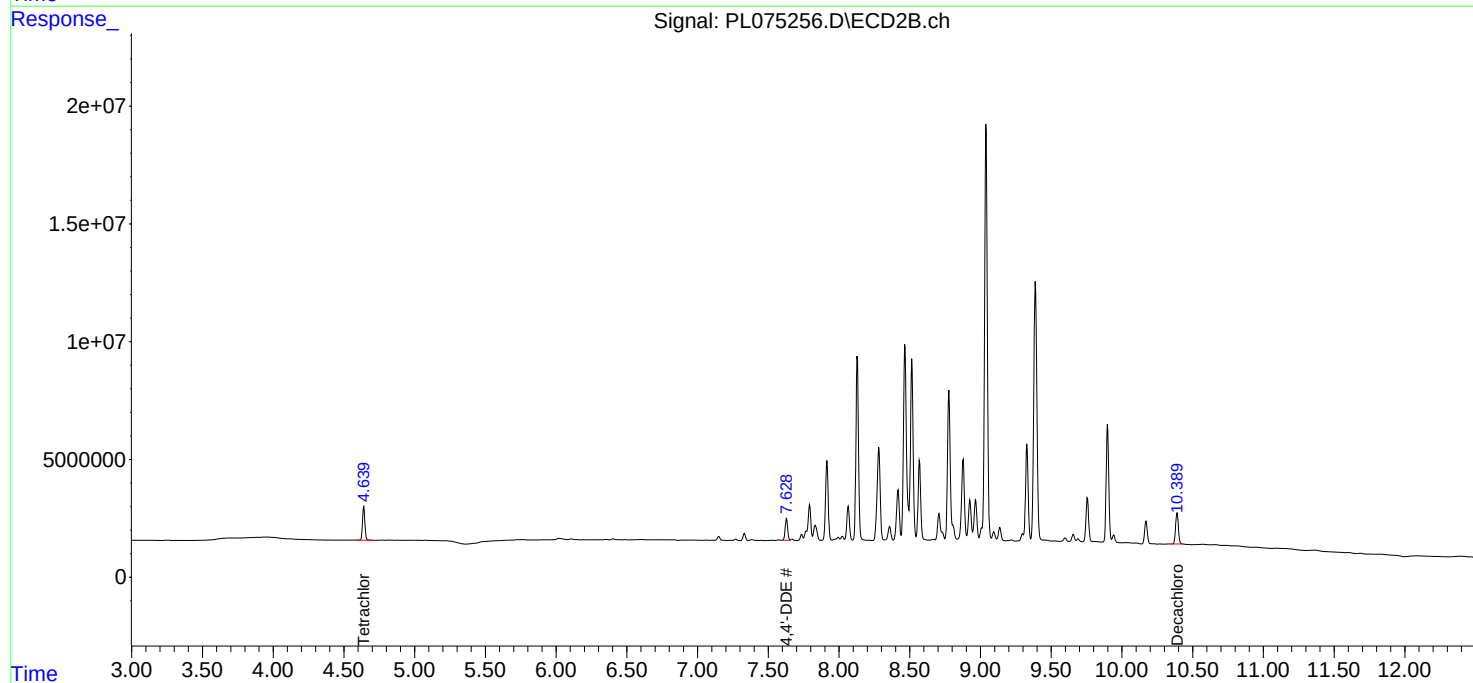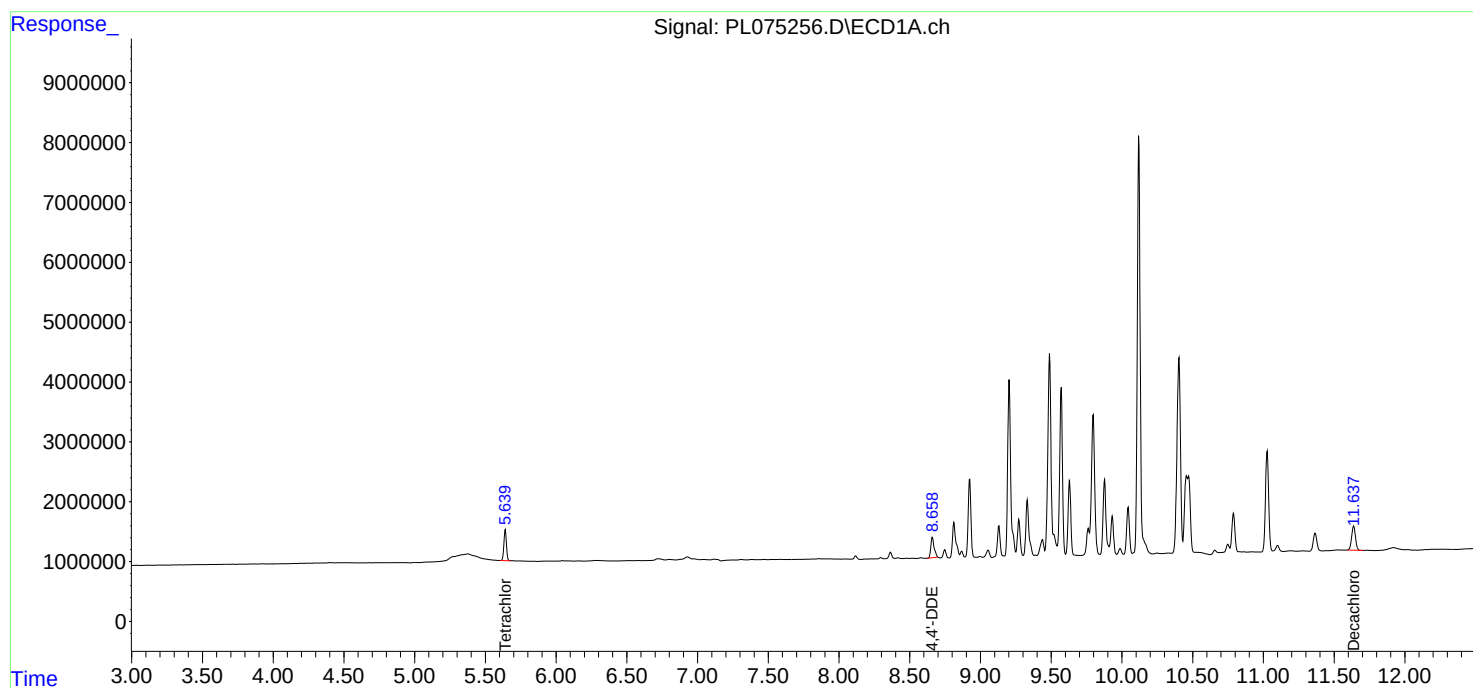


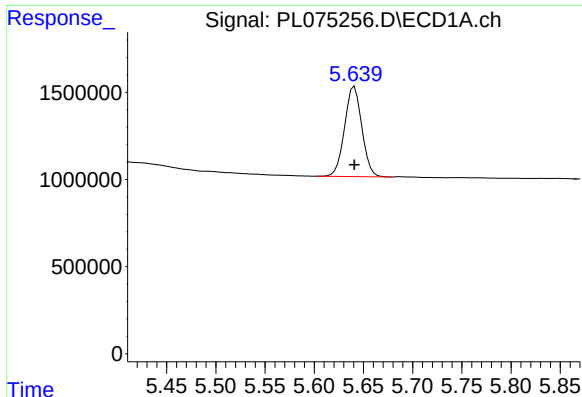

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 6325498
Conc: 10.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
P016-SS005-0006-01MS

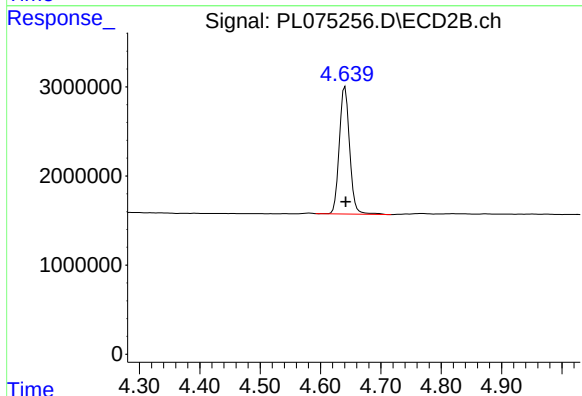


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 16999316
Conc: 10.73 ng/ml

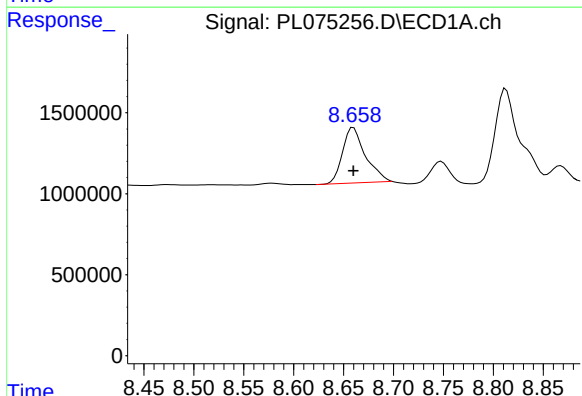


#12 4,4'-DDE

R.T.: 8.660 min
Delta R.T.: 0.000 min
Response: 5498582
Conc: 9.45 ng/ml

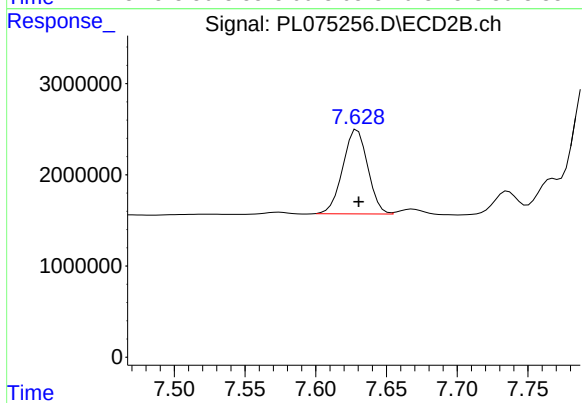

#12 4,4'-DDE


R.T.: 7.629 min
Delta R.T.: -0.001 min
Response: 11346462
Conc: 6.97 ng/ml

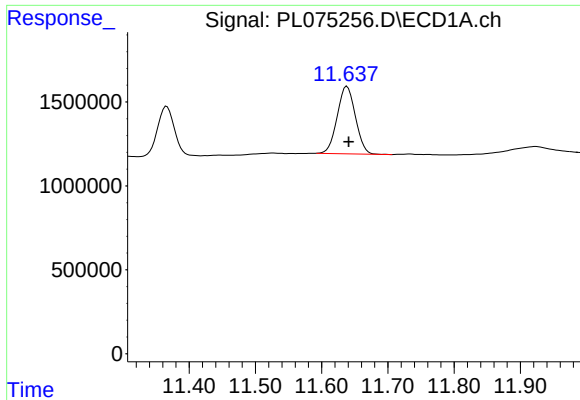

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: -0.003 min
Response: 7681648
Conc: 14.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
P016-SS005-0006-01MS

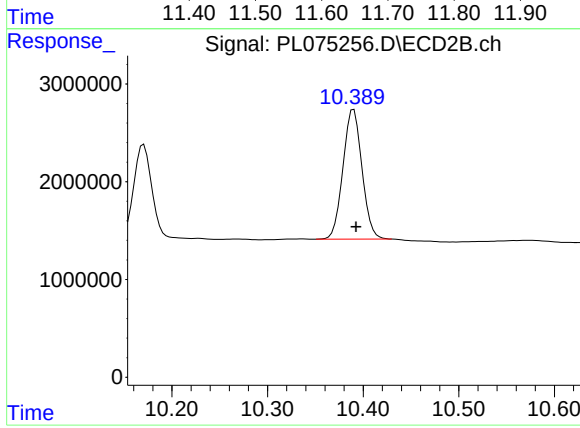

#28 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: -0.002 min
Response: 18403775
Conc: 13.41 ng/ml