

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
 Data File : PL075259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2022 16:17
 Operator : AR\AJ
 Sample : N2932-24
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P023-SS001-0006-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/31/2022
 Supervised By :Ankita Jodhani 05/31/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:23:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.640	11468555	29839171	19.513	18.836
28)	SA Decachlor...	11.636	10.389	7258596	16969015	13.538	12.366
Target Compounds							
12)	B 4,4'-DDE	8.659	7.629	13827184	35811793	23.769	21.988
13)	MA Dieldrin	8.812	7.764	754358	987939	1.190	0.569m#
17)	MA 4,4'-DDT	9.519	8.468	2357090	18878148	4.047m	13.200 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
Data File : PL075259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2022 16:17
Operator : AR\AJ
Sample : N2932-24
Misc :
ALS Vial : 79 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P023-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/31/2022
Supervised By : Ankita Jodhani 05/31/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:23:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

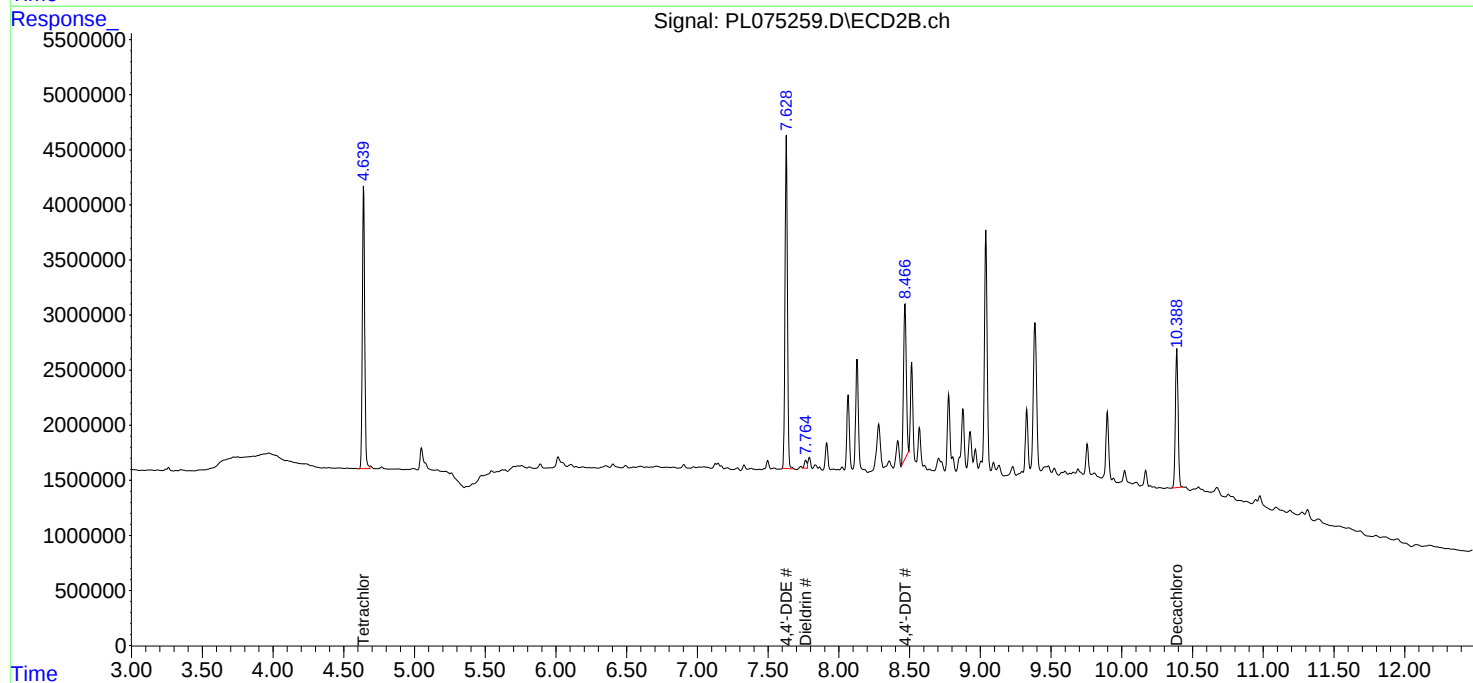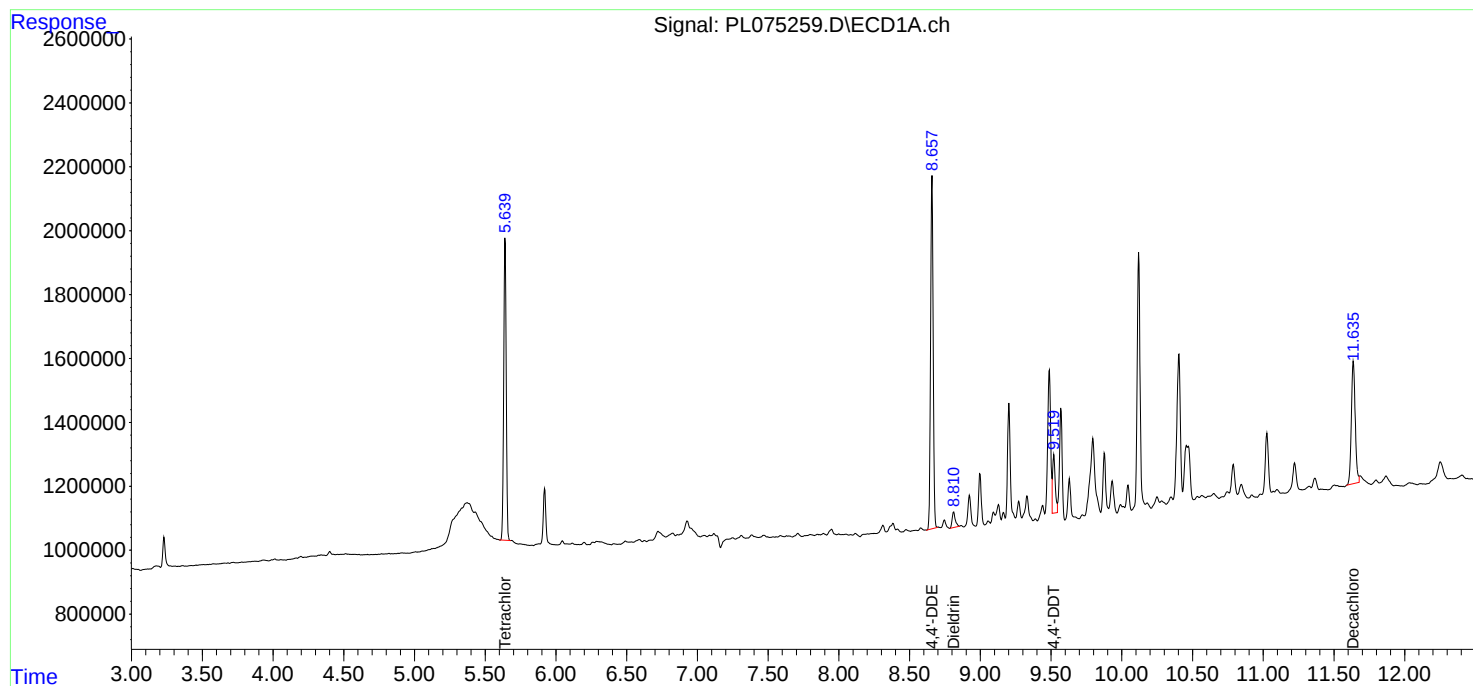

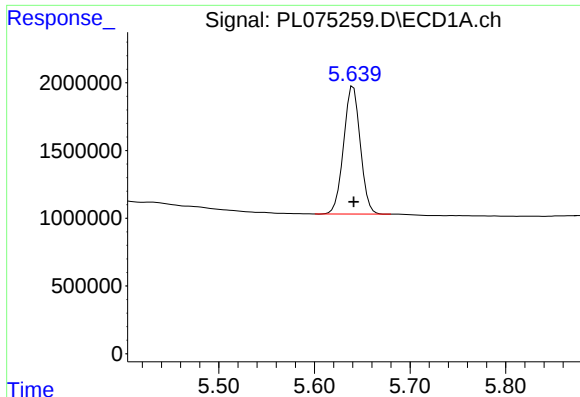


#1 Tetrachloro-m-xylene

R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 11468555
Conc: 19.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
P023-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/31/2022
Supervised By :Ankita Jodhani 05/31/2022

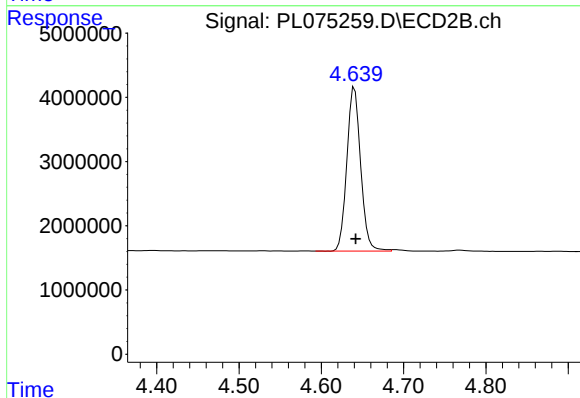


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.001 min
Response: 29839171
Conc: 18.84 ng/ml

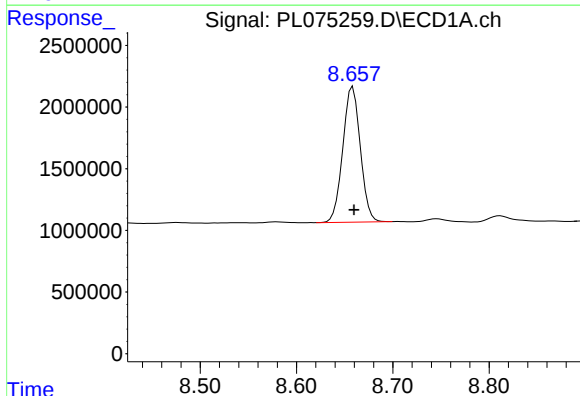


#12 4,4'-DDE

R.T.: 8.659 min
Delta R.T.: -0.001 min
Response: 13827184
Conc: 23.77 ng/ml

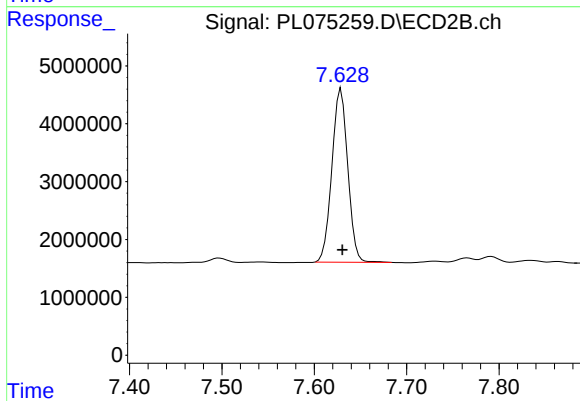

#12 4,4'-DDE

R.T.: 7.629 min
Delta R.T.: -0.001 min
Response: 35811793
Conc: 21.99 ng/ml

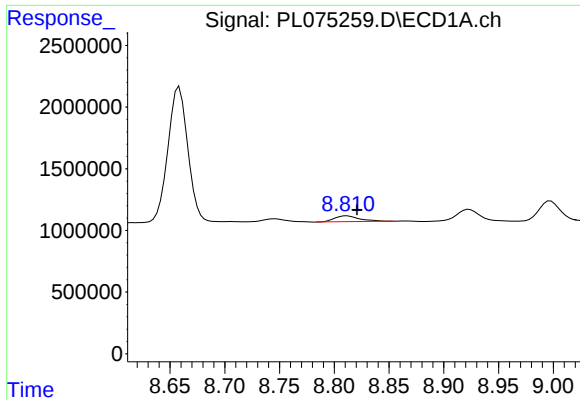


#13 Dieldrin

R.T.: 8.812 min
Delta R.T.: -0.009 min
Response: 754358
Conc: 1.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
P023-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/31/2022
Supervised By :Ankita Jodhani 05/31/2022

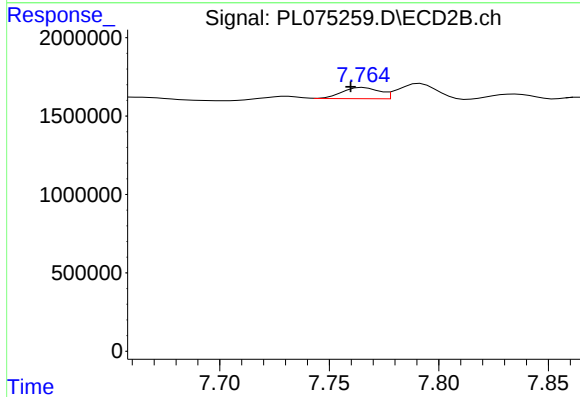


#13 Dieldrin

R.T.: 7.764 min
Delta R.T.: 0.005 min
Response: 987939
Conc: 0.57 ng/ml m

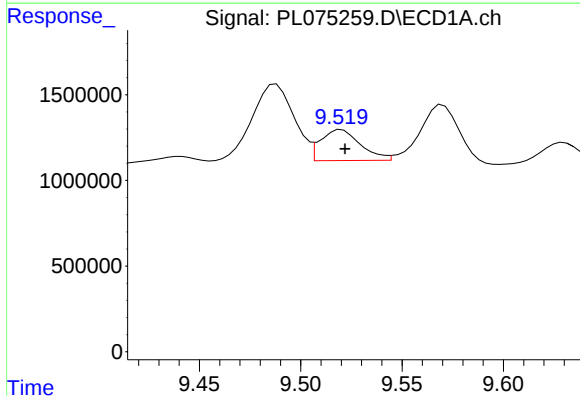


#17 4,4'-DDT

R.T.: 9.519 min
Delta R.T.: -0.003 min
Response: 2357090
Conc: 4.05 ng/ml m

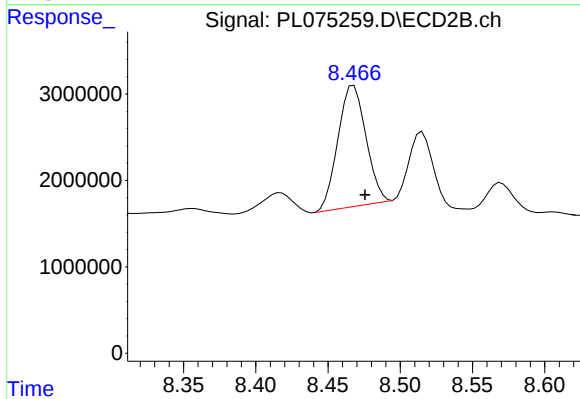

#17 4,4'-DDT

R.T.: 8.468 min
Delta R.T.: -0.008 min
Response: 18878148
Conc: 13.20 ng/ml

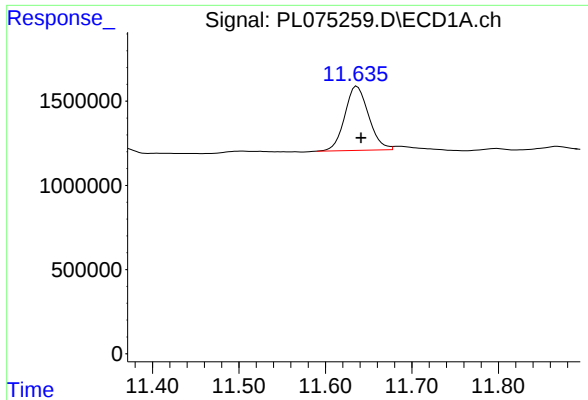


#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: -0.005 min
Response: 7258596
Conc: 13.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
P023-SS001-0006-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/31/2022
Supervised By :Ankita Jodhani 05/31/2022

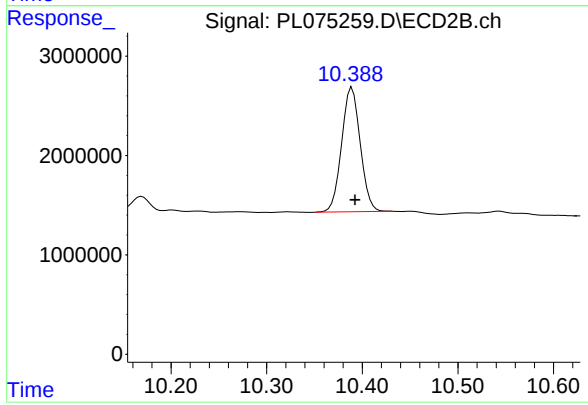

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.003 min
Response: 16969015
Conc: 12.37 ng/ml