

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
 Data File : PL059001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 08:50
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 10:49:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.076	38016655	50377243	20.733	18.600
28)	SA Decachlor...	8.309	9.187	30665380	45247634	18.150	17.164
Target Compounds							
4)	MA Heptachlor	0.000	5.265	0	503675	N.D.	0.131 #
8)	B Heptachlo...	0.000	5.947f	0	562614	N.D.	0.171 #
9)	A Endosulfan I	0.000	6.327	0	931557	N.D.	0.317 #
13)	MA Dieldrin	0.000	6.594	0	1324170	N.D.	0.437 #
14)	MA Endrin	0.000	6.830f	0	215264	N.D.	0.086 #
15)	B Endosulfa...	0.000	7.011	0	629795	N.D.	0.225 #
18)	B Endrin al...	6.534	7.120	505243	87964	0.358	0.037 #
19)	B Endosulfa...	0.000	7.366	0	437171	N.D.	0.166 #
20)	A Methoxychlor	0.000	7.666	0	2420880	N.D.	1.736 #
21)	B Endrin ke...	0.000	7.821	0	3557277	N.D.	1.284 #
27)	Chlordane-5	0.000	7.094	0	294035	N.D.	3.711 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
Data File : PL059001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 08:50
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 10:49:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

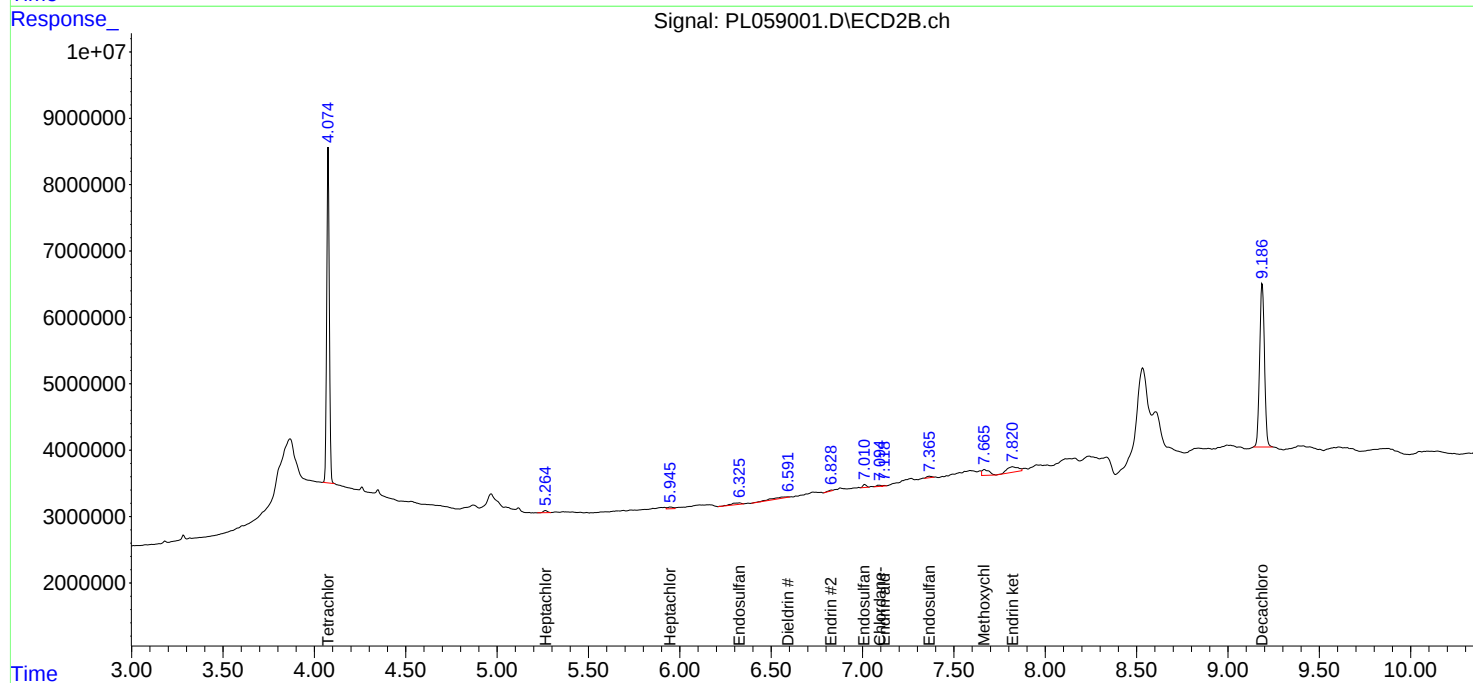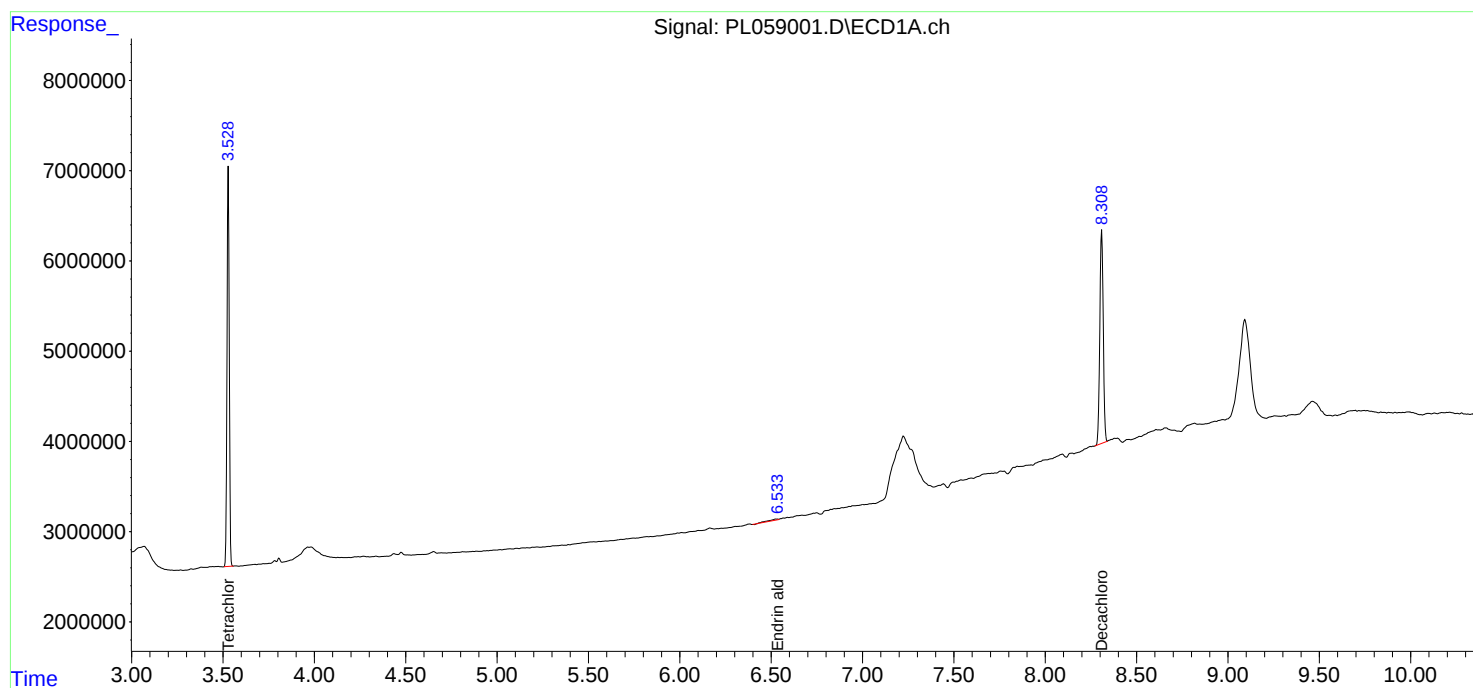


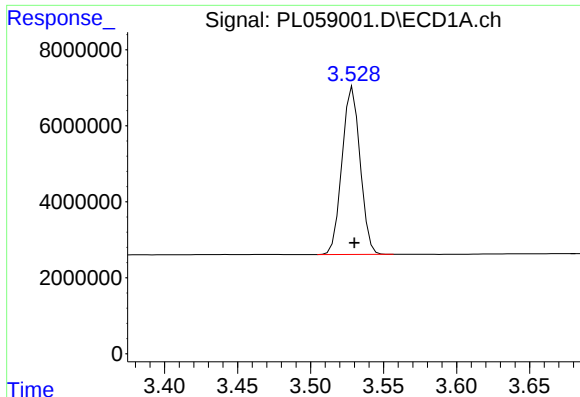

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 38016655
Conc: 20.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

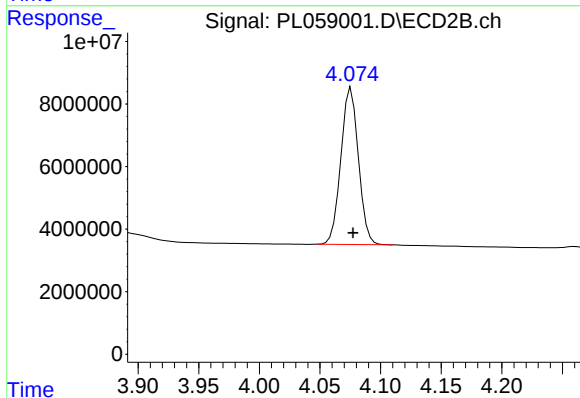


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.002 min
Response: 50377243
Conc: 18.60 ng/ml

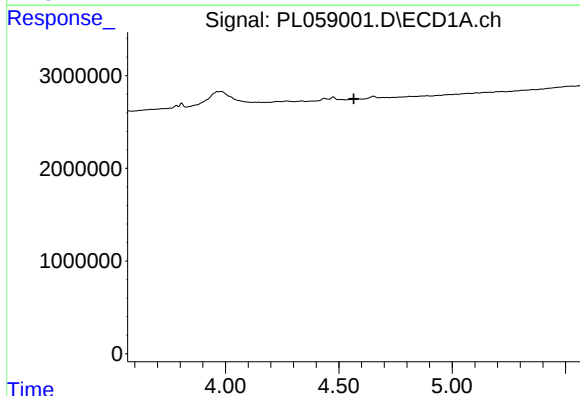


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

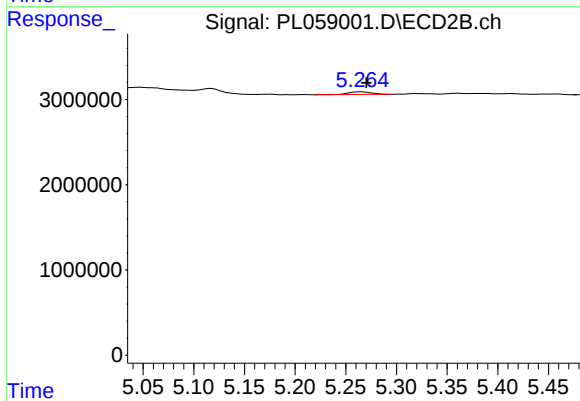

#4 Heptachlor

R.T.: 5.265 min
Delta R.T.: -0.005 min
Response: 503675
Conc: 0.13 ng/ml

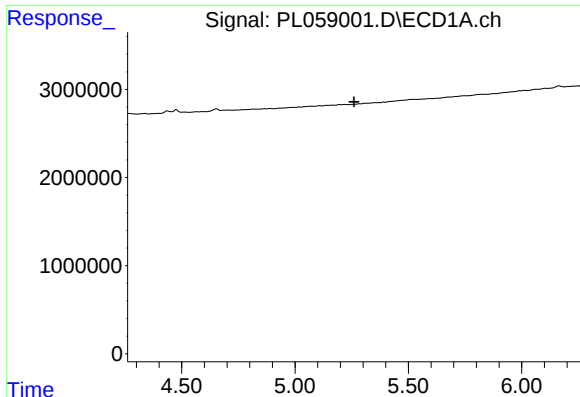


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#8 Heptachlor epoxide

R.T.: 5.947 min
Delta R.T.: -0.019 min
Response: 562614
Conc: 0.17 ng/ml

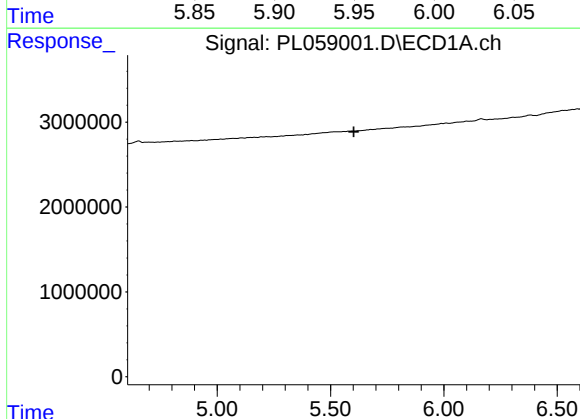


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.603 min
Response: 0
Conc: N.D.

#9 Endosulfan I


R.T.: 6.327 min
Delta R.T.: 0.003 min
Response: 931557
Conc: 0.32 ng/ml

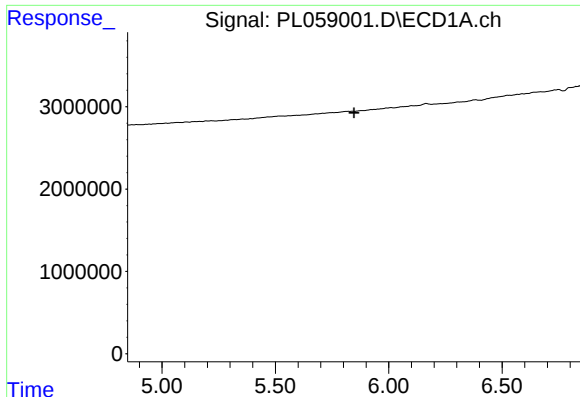

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.847 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

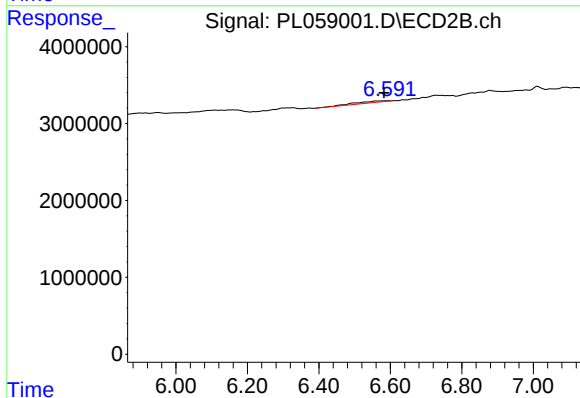


#13 Dieldrin

R.T.: 6.594 min
Delta R.T.: 0.011 min
Response: 1324170
Conc: 0.44 ng/ml

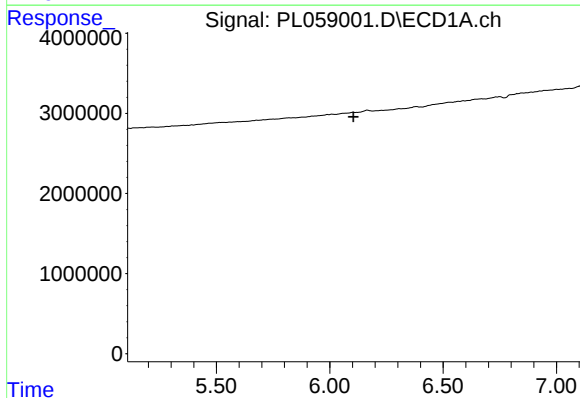


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.105 min
Response: 0
Conc: N.D.

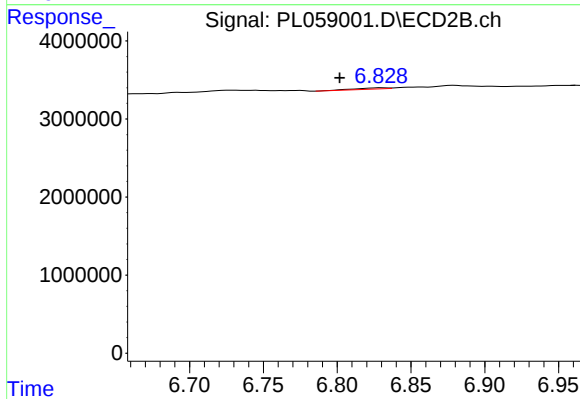

#14 Endrin


R.T.: 6.830 min
Delta R.T.: 0.029 min
Response: 215264
Conc: 0.09 ng/ml

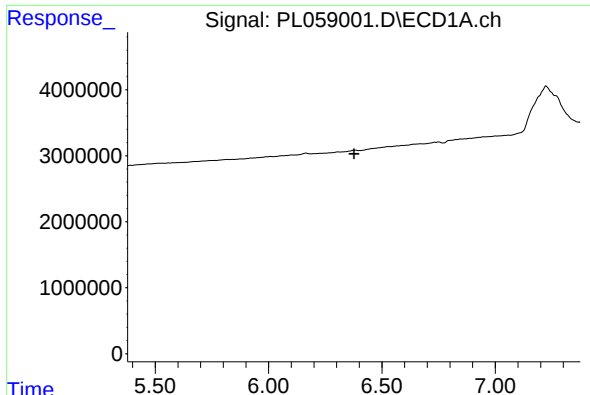

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

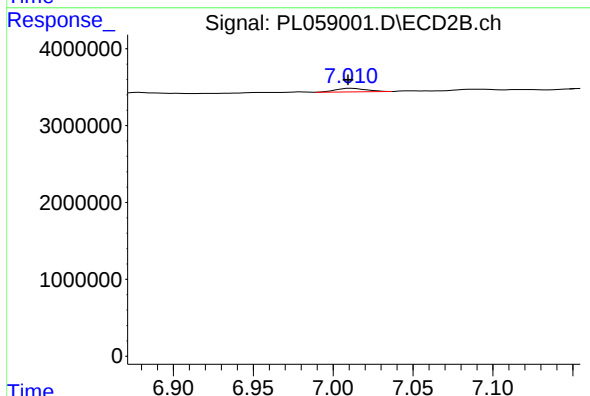


#15 Endosulfan II

R.T.: 7.011 min
Delta R.T.: 0.002 min
Response: 629795
Conc: 0.22 ng/ml

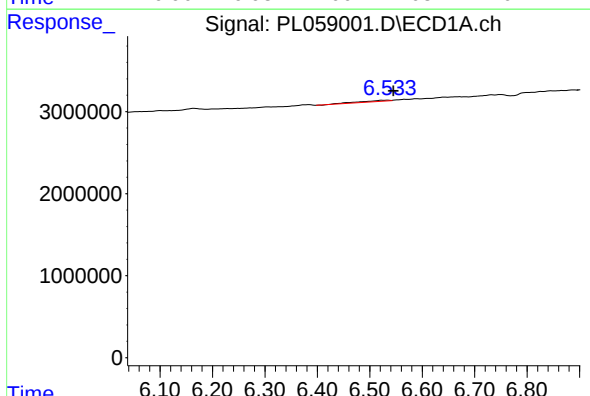


#18 Endrin aldehyde

R.T.: 6.534 min
Delta R.T.: -0.011 min
Response: 505243
Conc: 0.36 ng/ml

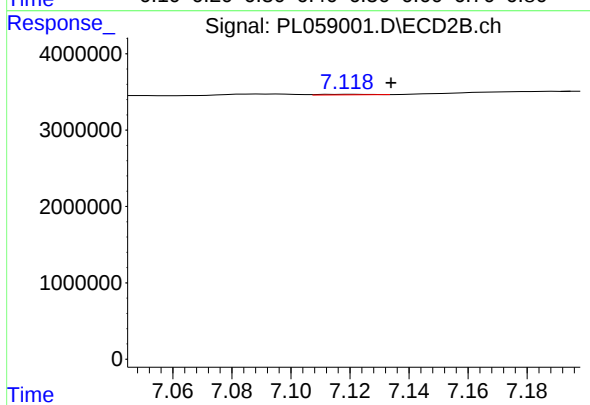

#18 Endrin aldehyde


R.T.: 7.120 min
Delta R.T.: -0.013 min
Response: 87964
Conc: 0.04 ng/ml

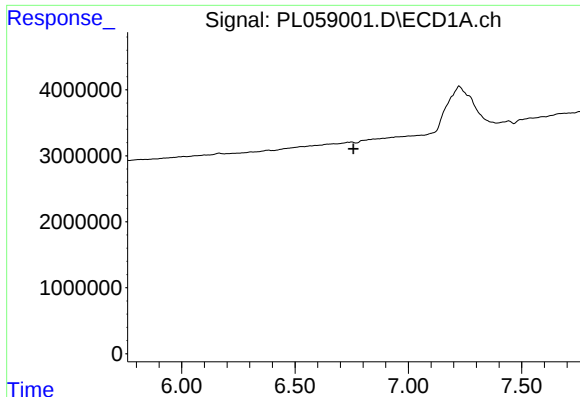

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.758 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

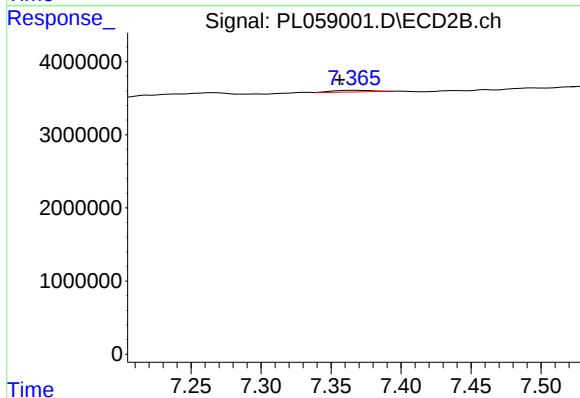


#19 Endosulfan Sulfate

R.T.: 7.366 min
Delta R.T.: 0.010 min
Response: 437171
Conc: 0.17 ng/ml

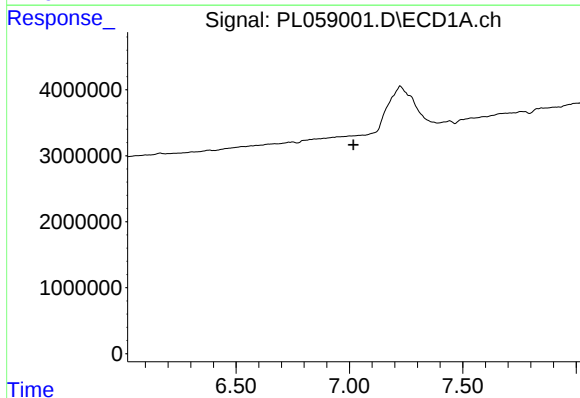


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.018 min
Response: 0
Conc: N.D.

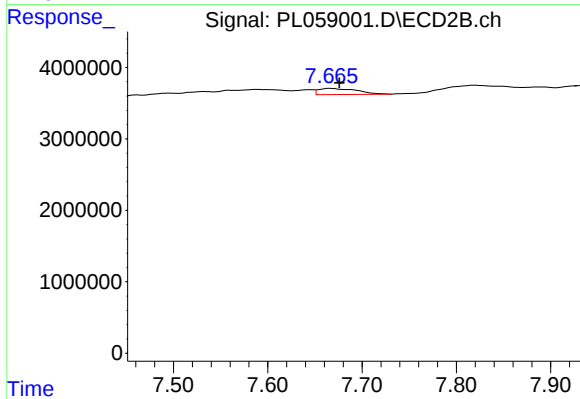

#20 Methoxychlor


R.T.: 7.666 min
Delta R.T.: -0.010 min
Response: 2420880
Conc: 1.74 ng/ml

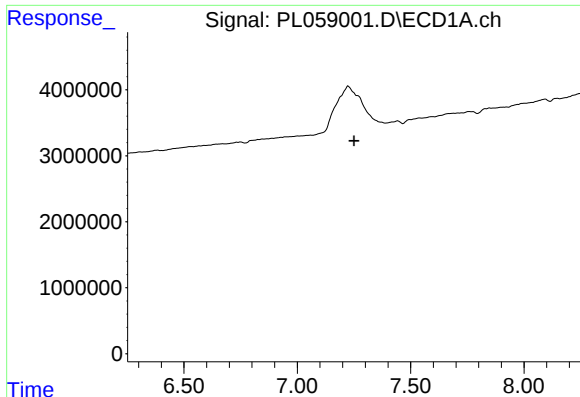

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.251 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

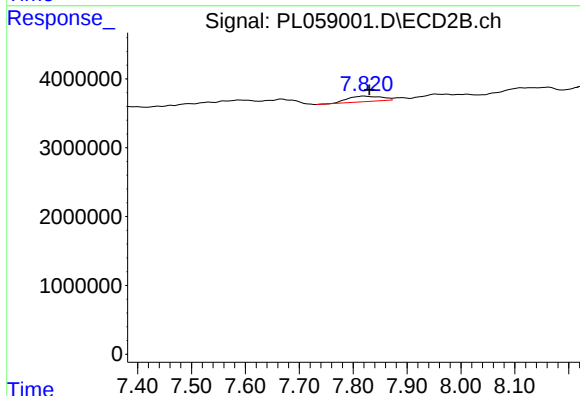


#21 Endrin ketone

R.T.: 7.821 min
Delta R.T.: -0.010 min
Response: 3557277
Conc: 1.28 ng/ml

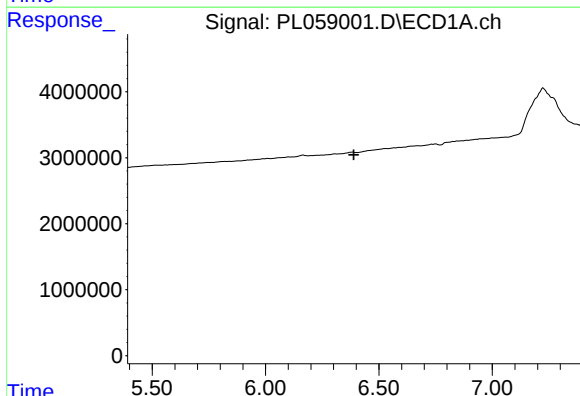


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

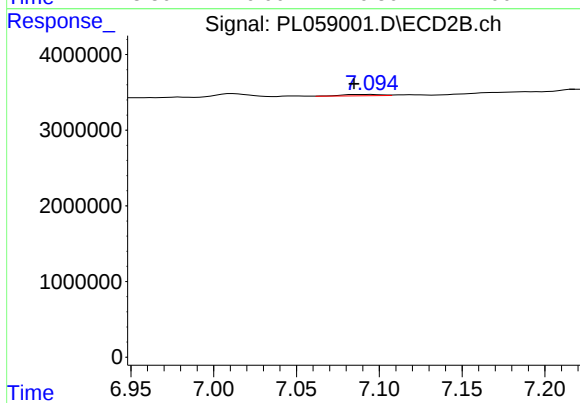

#27 Chlordane-5


R.T.: 7.094 min
Delta R.T.: 0.010 min
Response: 294035
Conc: 3.71 ng/ml

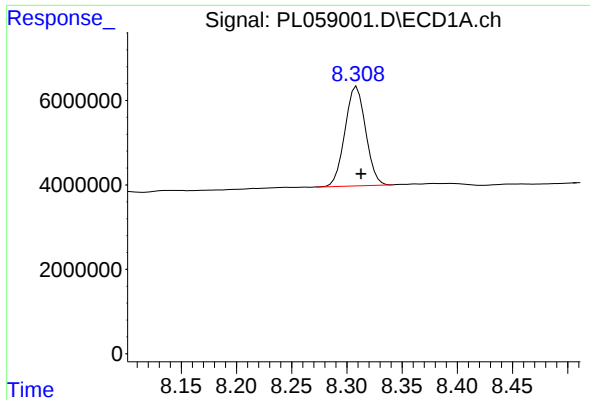

#28 Decachlorobiphenyl

R.T.: 8.309 min
Delta R.T.: -0.004 min
Response: 30665380
Conc: 18.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

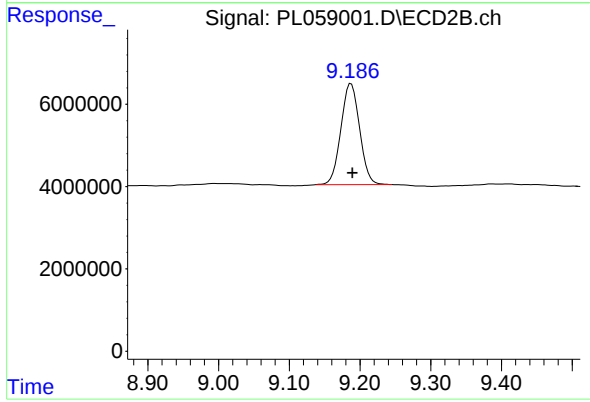

#28 Decachlorobiphenyl

R.T.: 9.187 min
Delta R.T.: -0.002 min
Response: 45247634
Conc: 17.16 ng/ml