

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
 Data File : PL059033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 18:21
 Operator : AJ\MA
 Sample : L2813-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:03:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	4.077	34741255	51232729	18.947	18.916
28)	SA Decachlor...	8.308	9.189	29030384	40387292	17.182	15.320
Target Compounds							
4)	MA Heptachlor	0.000	5.264	0	4020989	N.D.	1.050 #
7)	B delta-BHC	0.000	5.115f	0	6614421	N.D.	1.814 #
8)	B Heptachlo...	0.000	5.991f	0	1585274	N.D.	0.481 #
13)	MA Dieldrin	0.000	6.565f	0	49586	N.D.	0.016 #
15)	B Endosulfa...	0.000	7.012	0	4493622	N.D.	1.603 #
18)	B Endrin al...	0.000	7.130	0	620363	N.D.	0.263 #
20)	A Methoxychlor	7.013	7.677	2306339	4700528	2.704	3.370
21)	B Endrin ke...	0.000	7.815f	0	896171	N.D.	0.323 #
27)	Chlordane-5	0.000	7.079	0	4678755	N.D.	59.057 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
Data File : PL059033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 18:21
Operator : AJ\MA
Sample : L2813-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:03:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

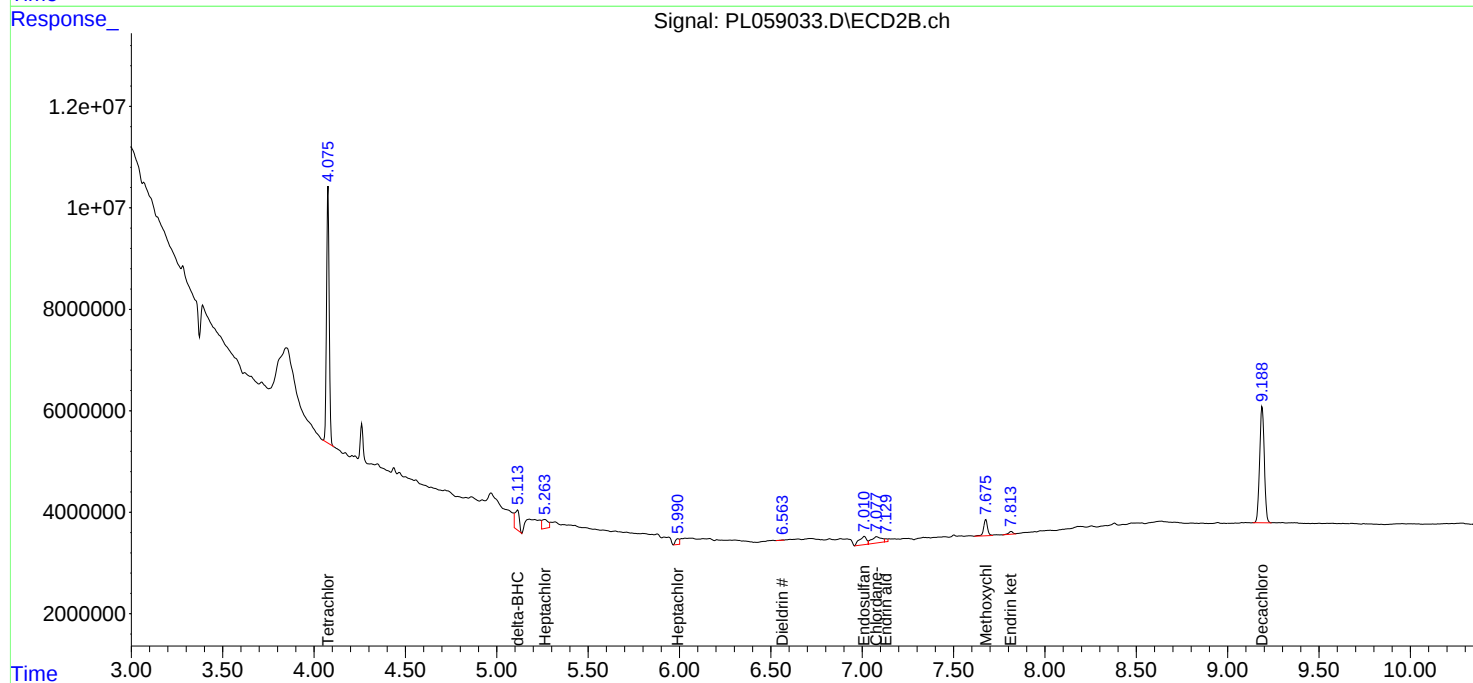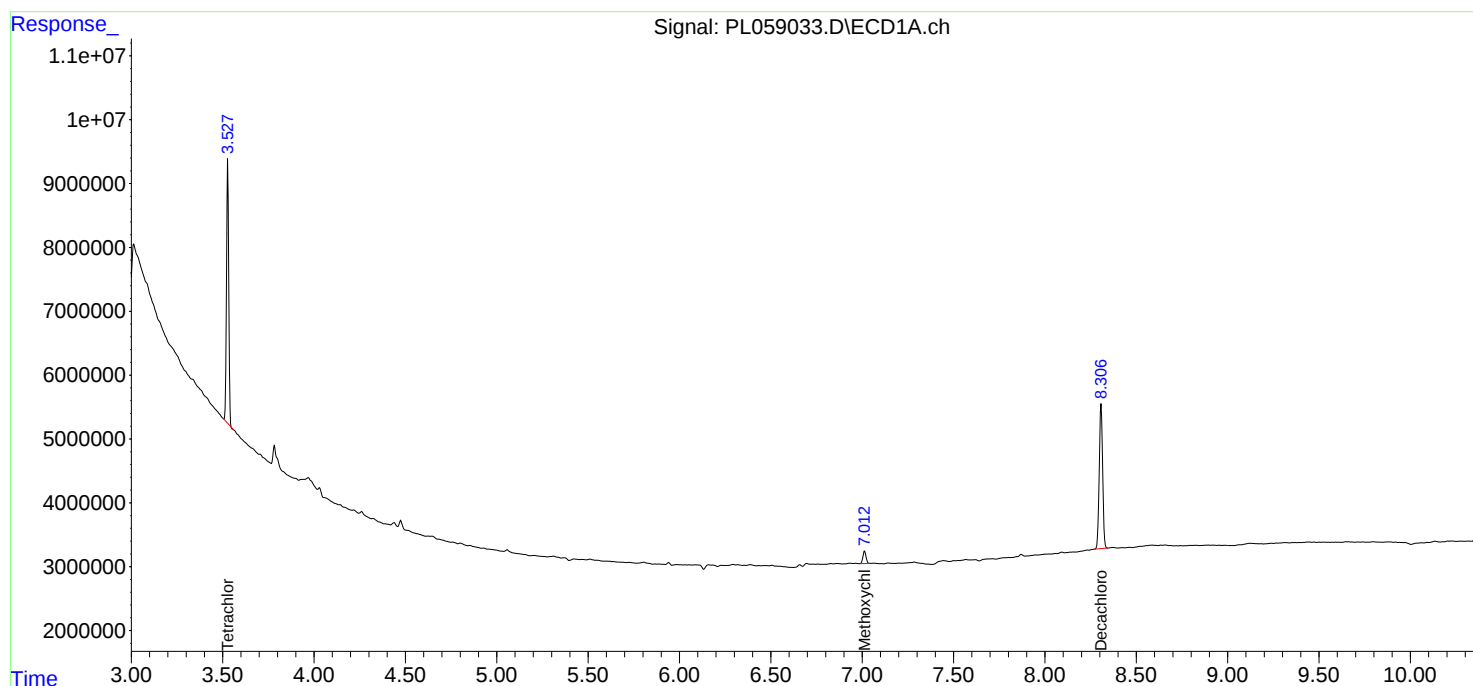


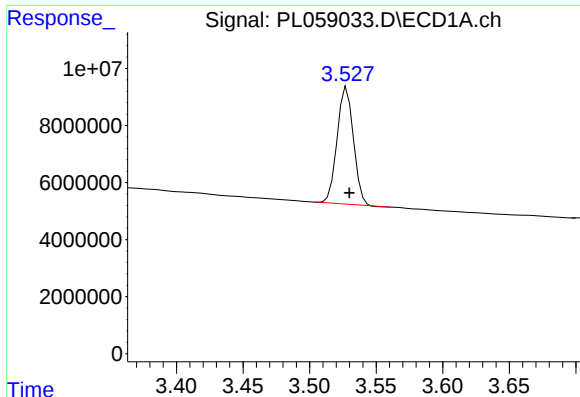

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: -0.002 min
Response: 34741255
Conc: 18.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

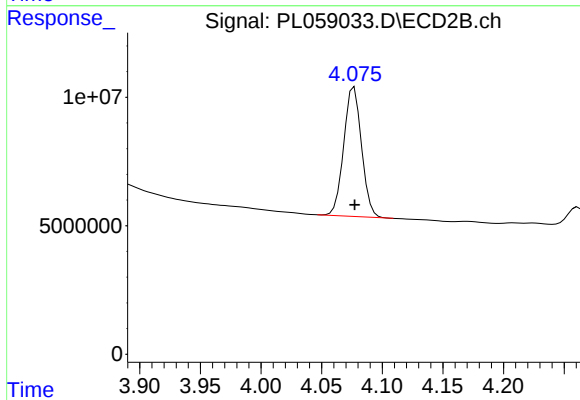


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 51232729
Conc: 18.92 ng/ml

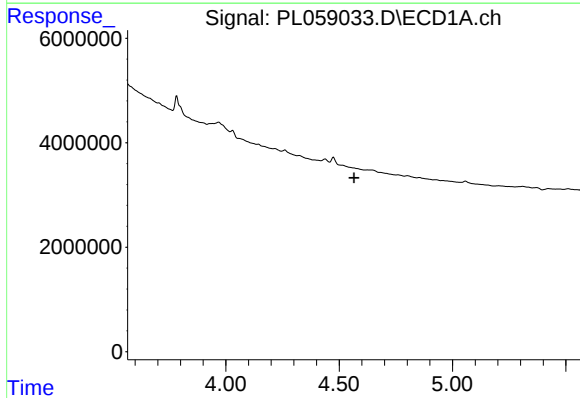


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

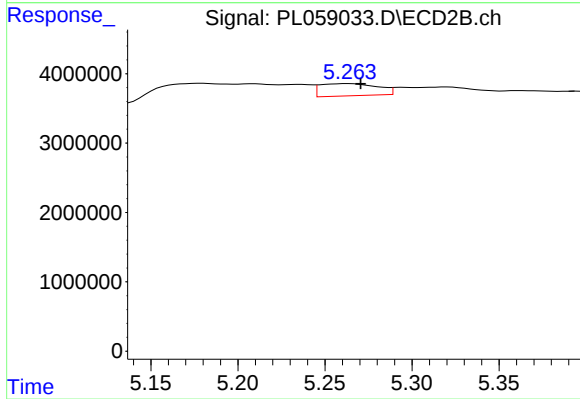

#4 Heptachlor


R.T.: 5.264 min
Delta R.T.: -0.006 min
Response: 4020989
Conc: 1.05 ng/ml

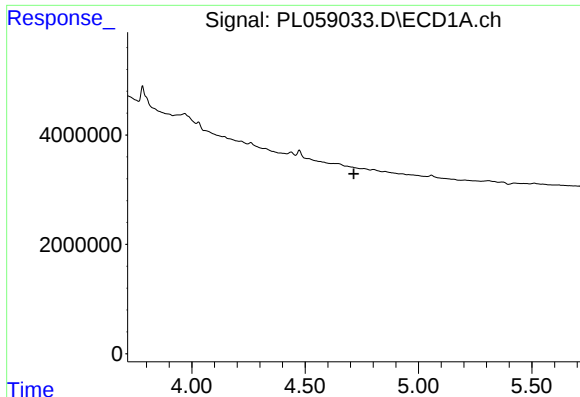

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

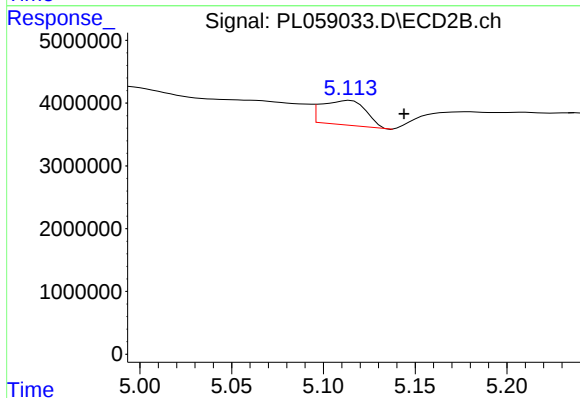


#7 delta-BHC

R.T.: 5.115 min
Delta R.T.: -0.029 min
Response: 6614421
Conc: 1.81 ng/ml

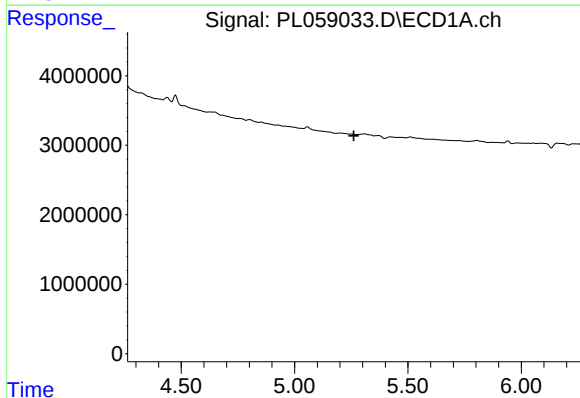


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

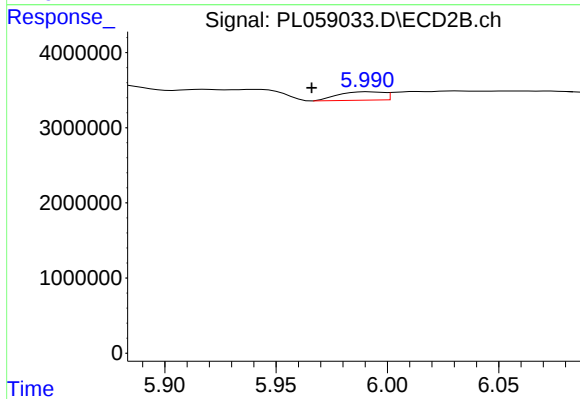

#8 Heptachlor epoxide


R.T.: 5.991 min
Delta R.T.: 0.025 min
Response: 1585274
Conc: 0.48 ng/ml

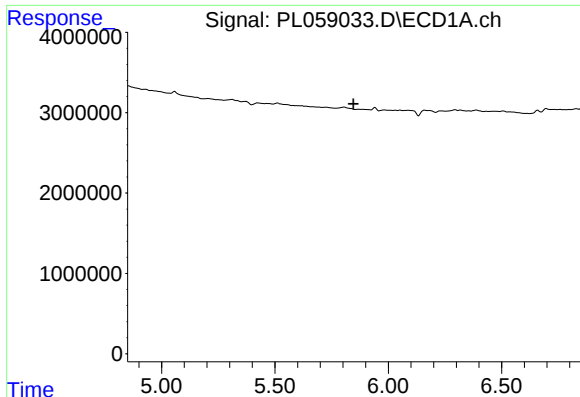

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.847 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

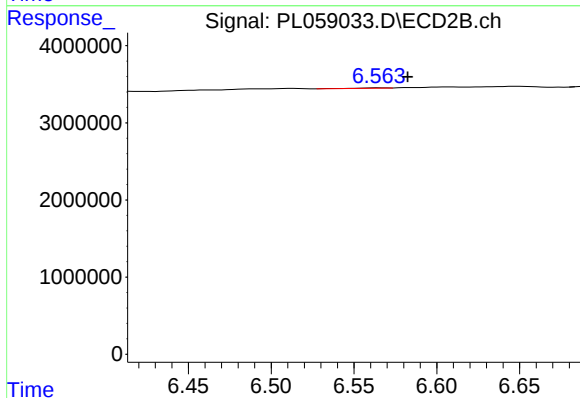


#13 Dieldrin

R.T.: 6.565 min
Delta R.T.: -0.017 min
Response: 49586
Conc: 0.02 ng/ml

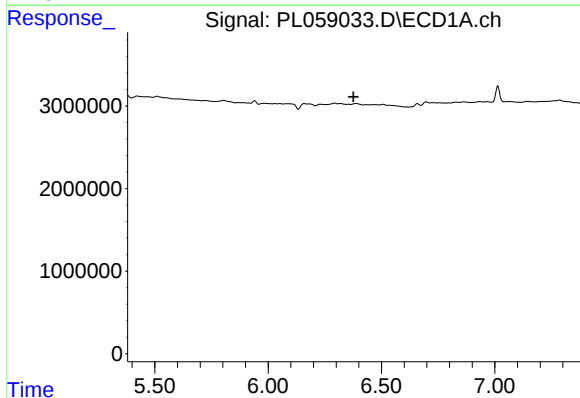


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

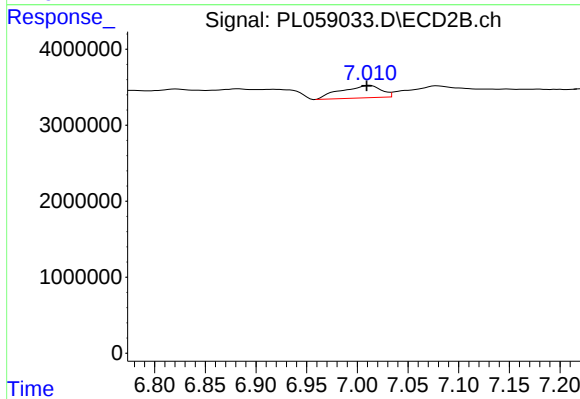

#15 Endosulfan II


R.T.: 7.012 min
Delta R.T.: 0.003 min
Response: 4493622
Conc: 1.60 ng/ml

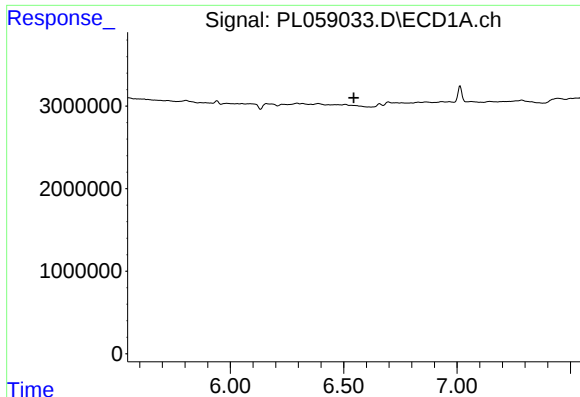

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

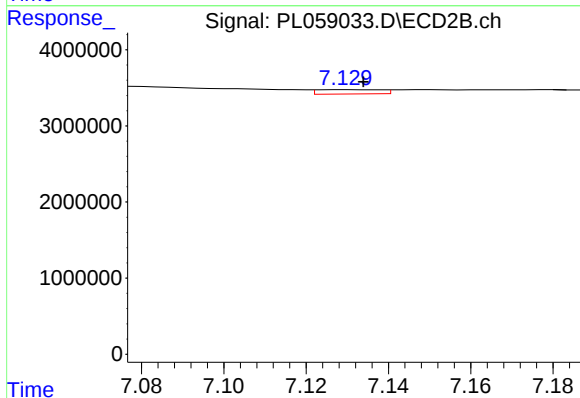


#18 Endrin aldehyde

R.T.: 7.130 min
Delta R.T.: -0.004 min
Response: 620363
Conc: 0.26 ng/ml

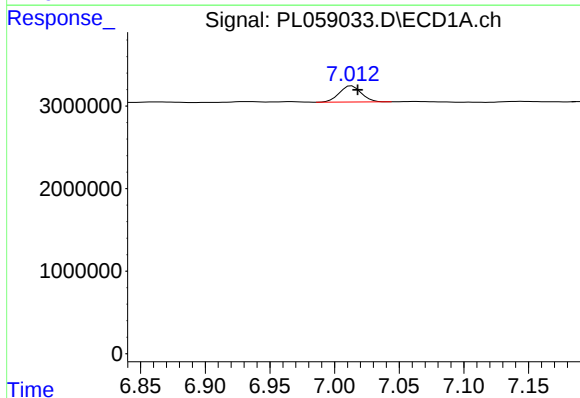


#20 Methoxychlor

R.T.: 7.013 min
Delta R.T.: -0.005 min
Response: 2306339
Conc: 2.70 ng/ml

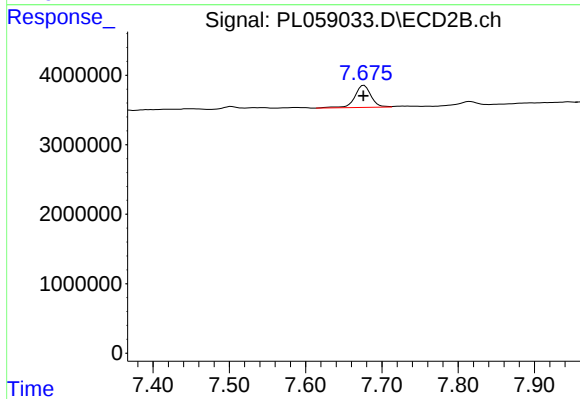

#20 Methoxychlor


R.T.: 7.677 min
Delta R.T.: 0.000 min
Response: 4700528
Conc: 3.37 ng/ml

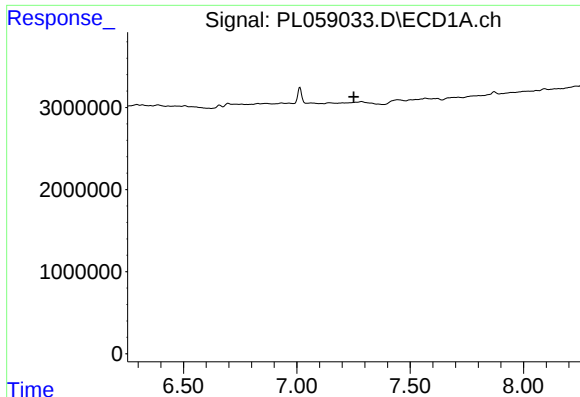

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.251 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

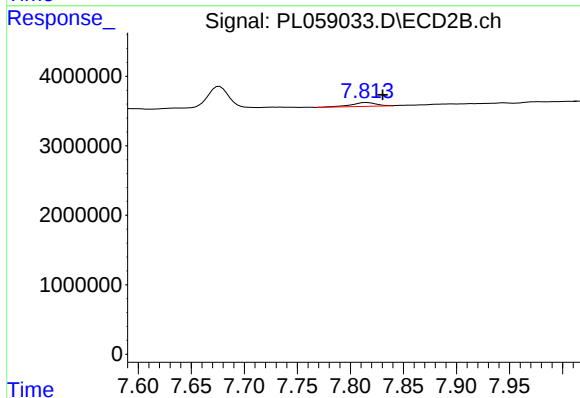


#21 Endrin ketone

R.T.: 7.815 min
Delta R.T.: -0.015 min
Response: 896171
Conc: 0.32 ng/ml

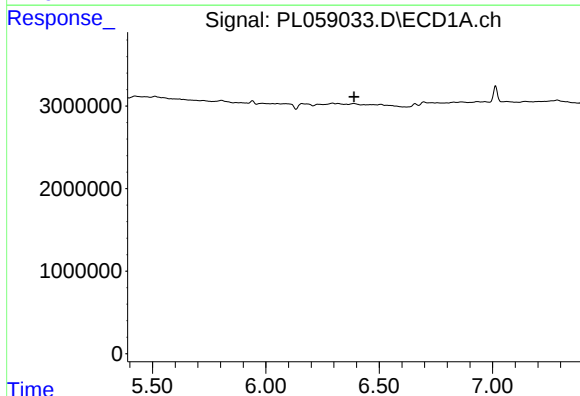


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

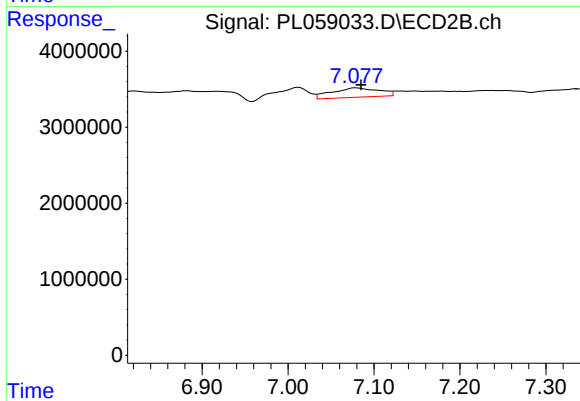

#27 Chlordane-5


R.T.: 7.079 min
Delta R.T.: -0.006 min
Response: 4678755
Conc: 59.06 ng/ml

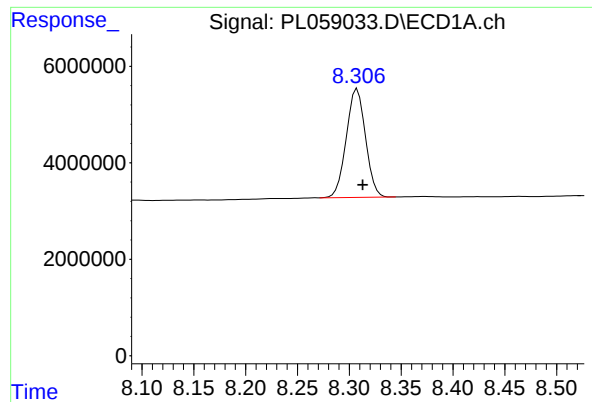

#28 Decachlorobiphenyl

R.T.: 8.308 min
Delta R.T.: -0.005 min
Response: 29030384
Conc: 17.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

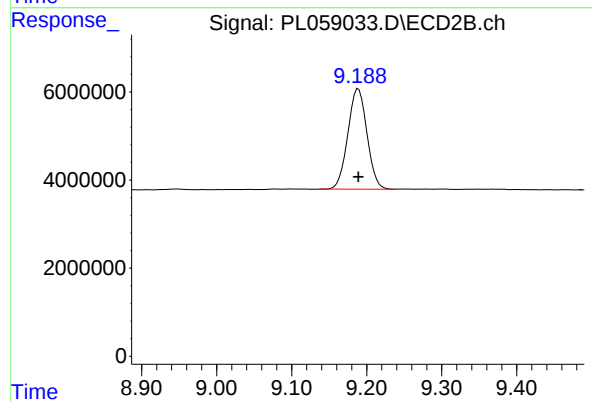

#28 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: 0.000 min
Response: 40387292
Conc: 15.32 ng/ml