

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
 Data File : PL059038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 19:32
 Operator : AJ\MA
 Sample : L2822-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:04:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	4.077	34341030	49776612	18.728	18.379
28)	SA Decachlor...	8.307	9.189	30822182	42341584	18.243	16.062
Target Compounds							
4)	MA Heptachlor	0.000	5.264	0	9870101	N.D.	2.577 #
7)	B delta-BHC	0.000	5.115f	0	5314367	N.D.	1.457 #
10)	B gamma-Chl...	0.000	6.208	0	260025	N.D.	0.079 #
15)	B Endosulfa...	0.000	7.013	0	4603740	N.D.	1.642 #
17)	MA 4,4'-DDT	0.000	7.229	0	542435	N.D.	0.228 #
20)	A Methoxychlor	7.013	7.678	4971842	8638159	5.828	6.194
21)	B Endrin ke...	0.000	7.815f	0	519625	N.D.	0.188 #
25)	Chlordane-3	0.000	6.208	0	260025	N.D.	0.683 #
27)	Chlordane-5	0.000	7.082	0	5248140	N.D.	66.244 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
Data File : PL059038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 19:32
Operator : AJ\MA
Sample : L2822-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:04:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

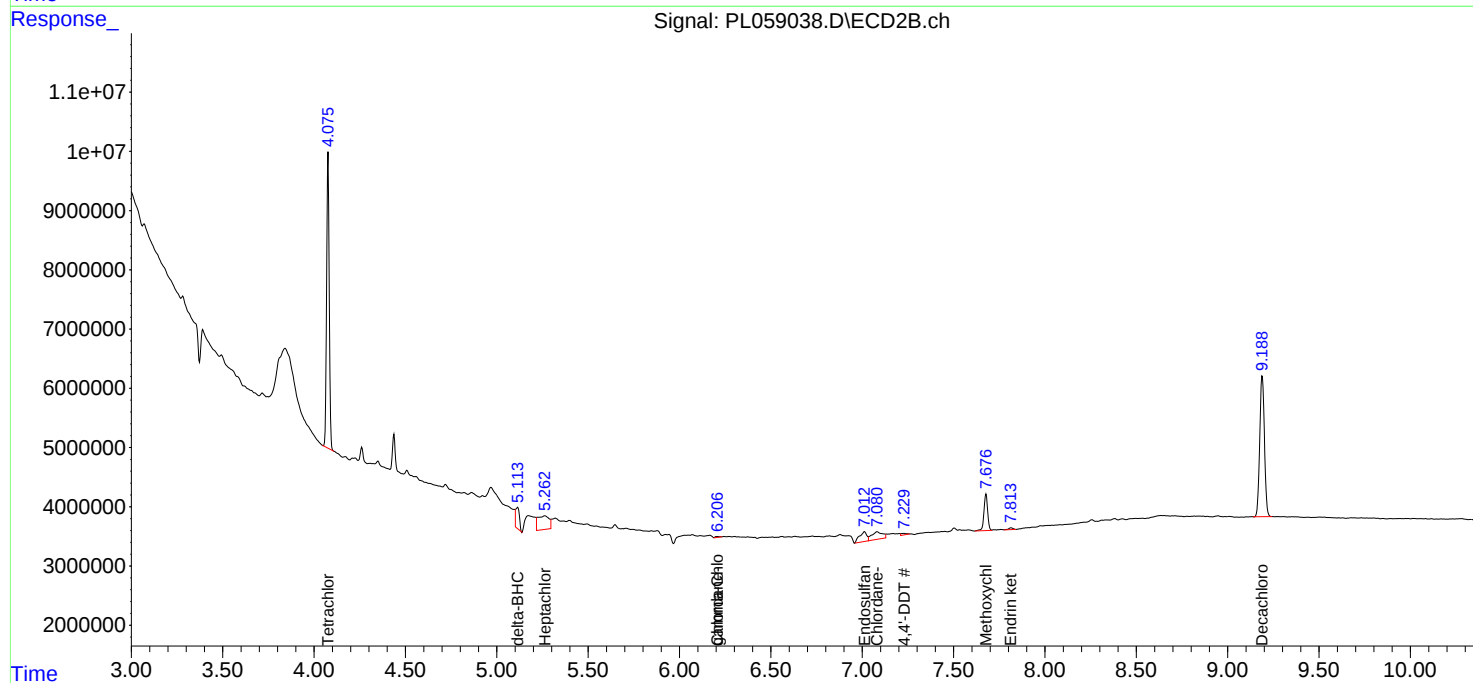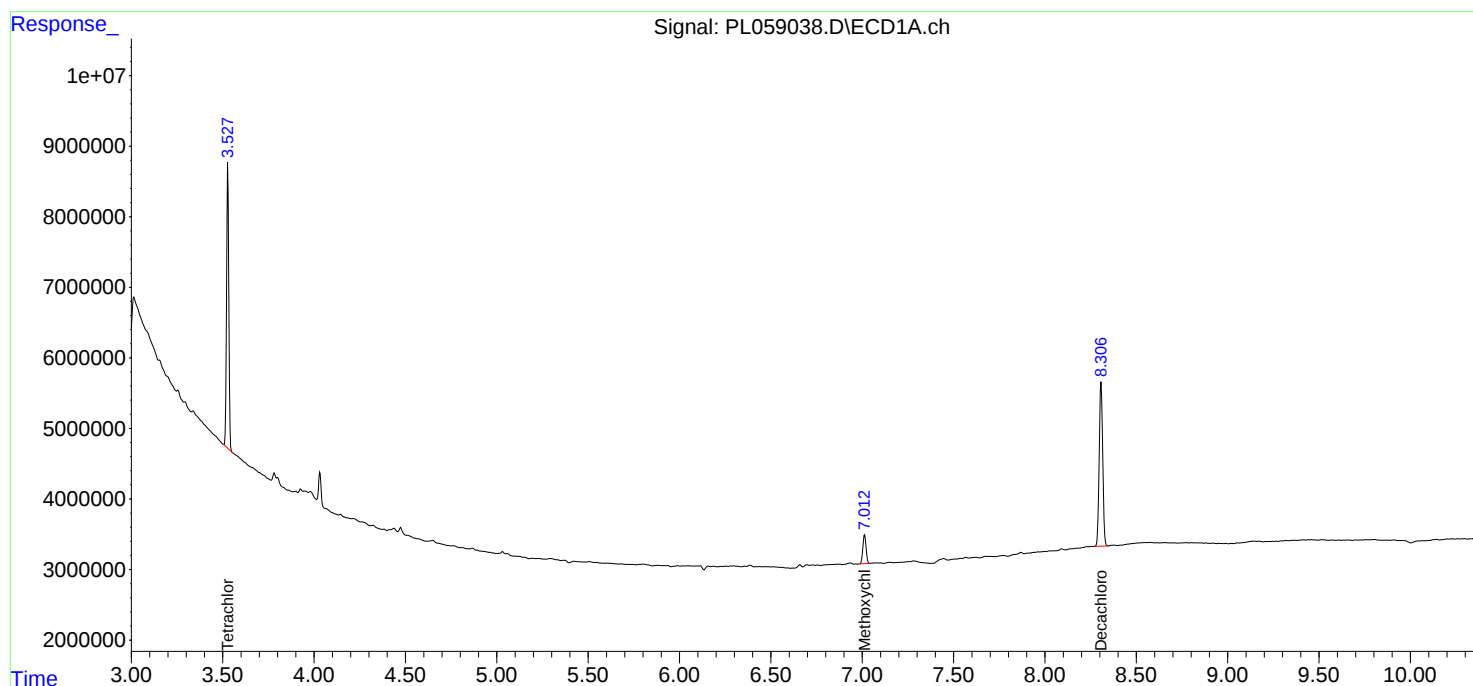


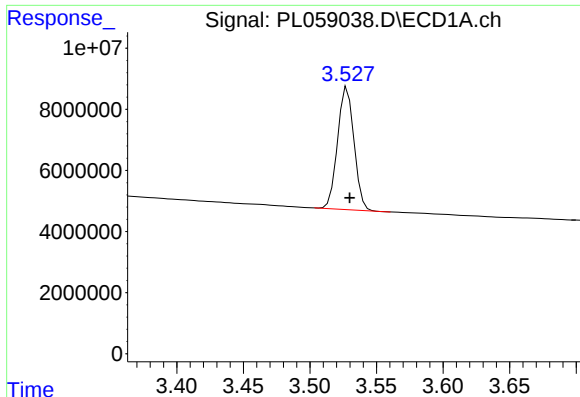

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: -0.002 min
Response: 34341030
Conc: 18.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

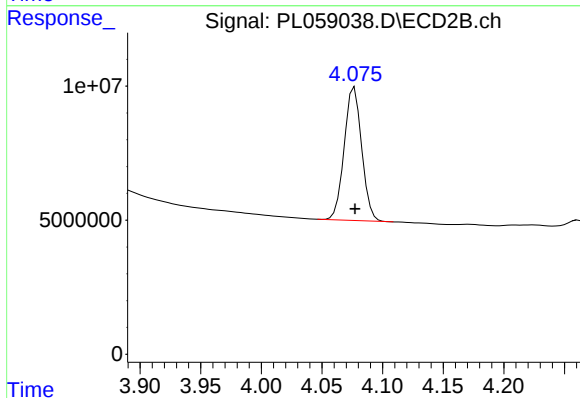


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 49776612
Conc: 18.38 ng/ml

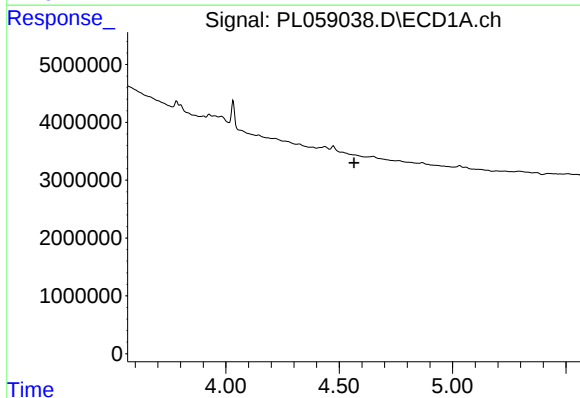


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

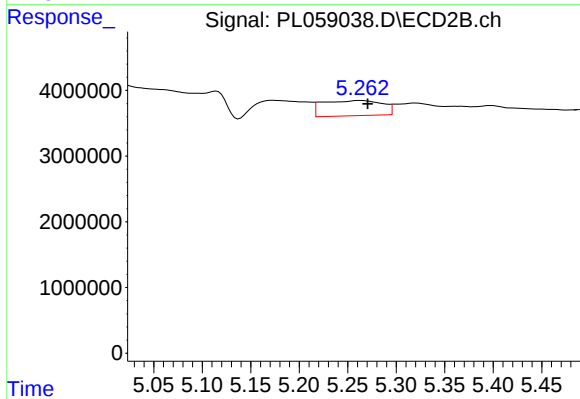

#4 Heptachlor


R.T.: 5.264 min
Delta R.T.: -0.007 min
Response: 9870101
Conc: 2.58 ng/ml

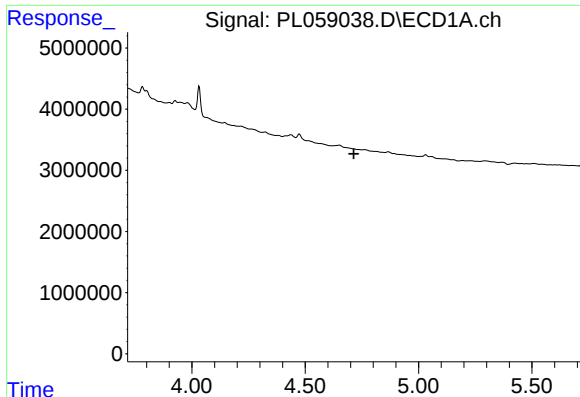

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

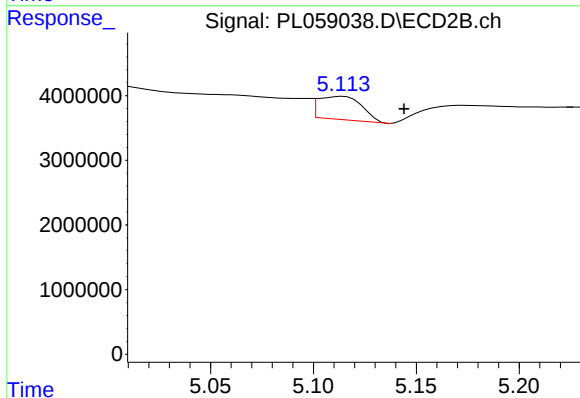


#7 delta-BHC

R.T.: 5.115 min
Delta R.T.: -0.029 min
Response: 5314367
Conc: 1.46 ng/ml

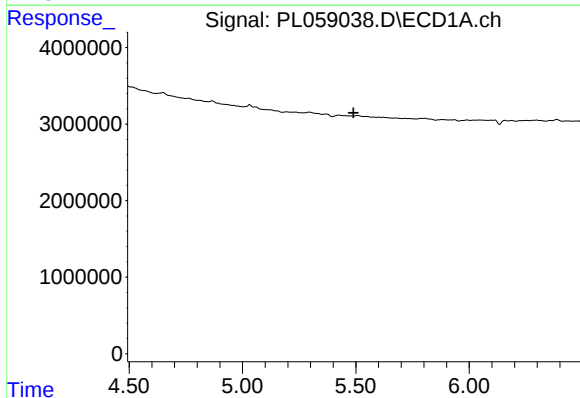


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.490 min
Response: 0
Conc: N.D.

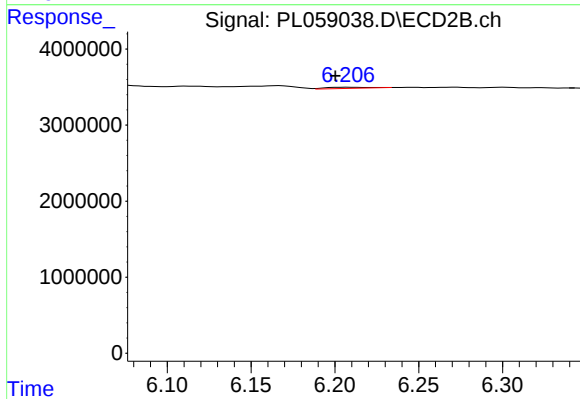

#10 gamma-Chlordane


R.T.: 6.208 min
Delta R.T.: 0.008 min
Response: 260025
Conc: 0.08 ng/ml

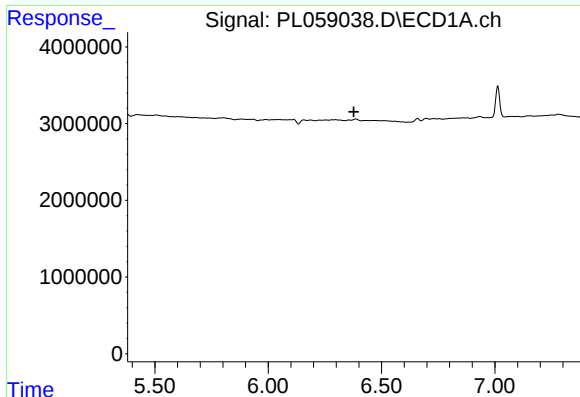

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

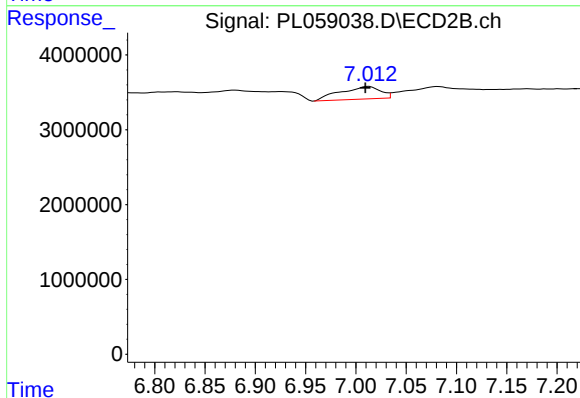


#15 Endosulfan II

R.T.: 7.013 min
Delta R.T.: 0.004 min
Response: 4603740
Conc: 1.64 ng/ml

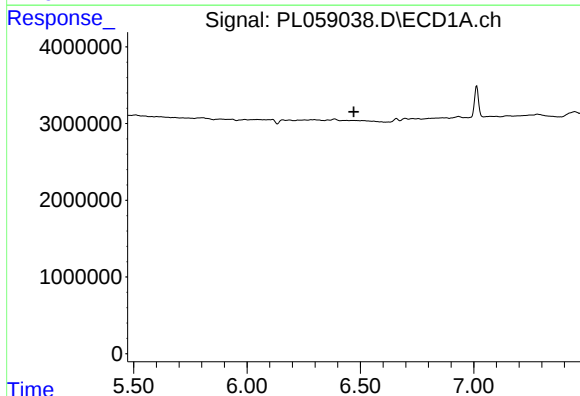


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.471 min
Response: 0
Conc: N.D.

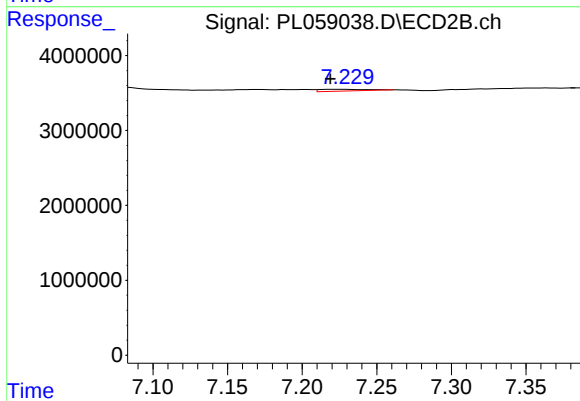

#17 4,4'-DDT


R.T.: 7.229 min
Delta R.T.: 0.011 min
Response: 542435
Conc: 0.23 ng/ml

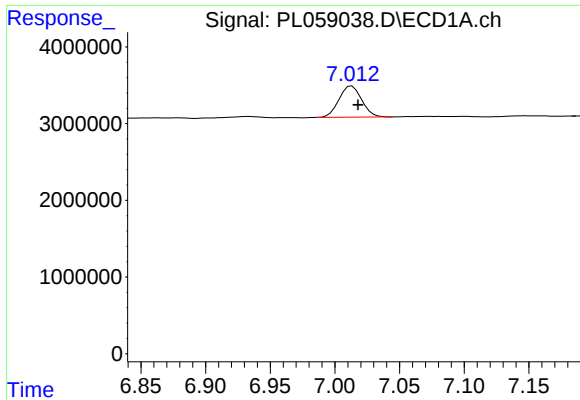

#20 Methoxychlor


R.T.: 7.013 min
Delta R.T.: -0.005 min
Response: 4971842
Conc: 5.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

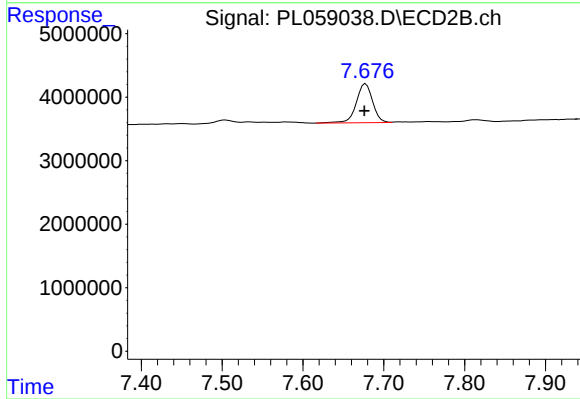


#20 Methoxychlor

R.T.: 7.678 min
Delta R.T.: 0.002 min
Response: 8638159
Conc: 6.19 ng/ml

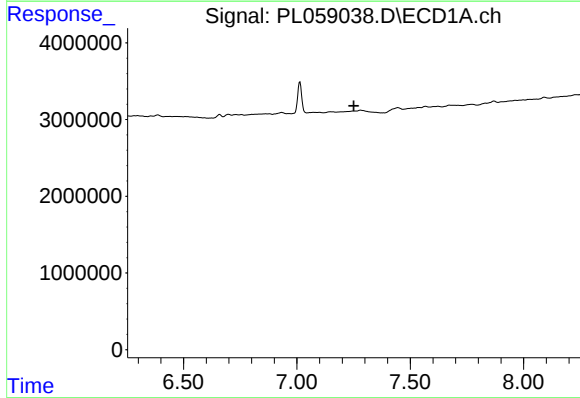


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

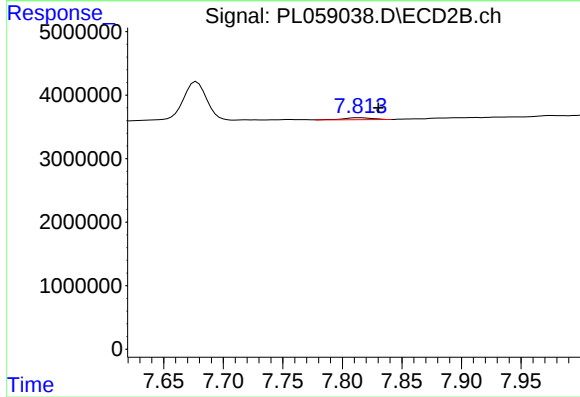

#21 Endrin ketone


R.T.: 7.815 min
Delta R.T.: -0.016 min
Response: 519625
Conc: 0.19 ng/ml

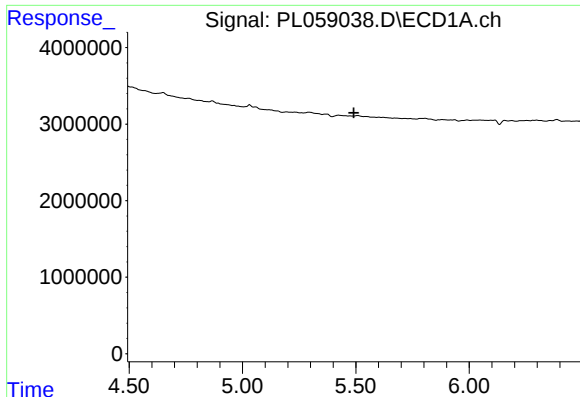

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

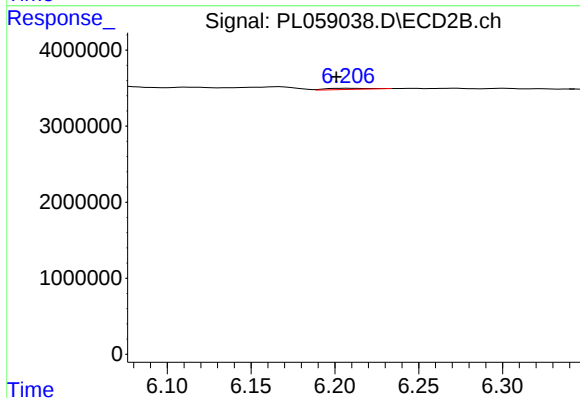


#25 Chlordane-3

R.T.: 6.208 min
Delta R.T.: 0.007 min
Response: 260025
Conc: 0.68 ng/ml

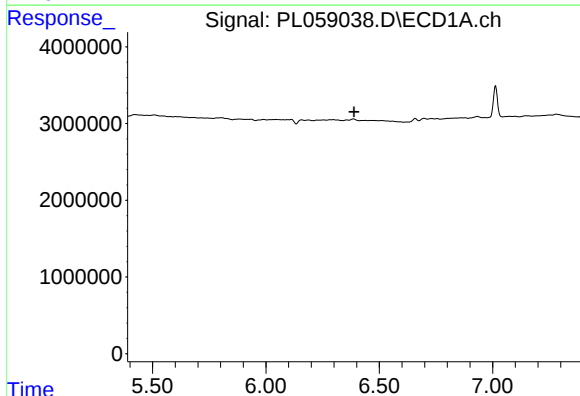


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

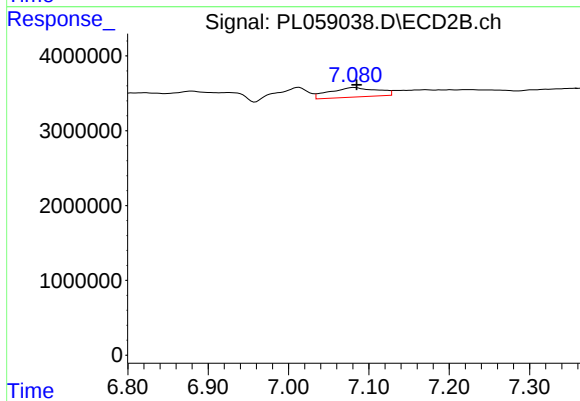

#27 Chlordane-5


R.T.: 7.082 min
Delta R.T.: -0.003 min
Response: 5248140
Conc: 66.24 ng/ml

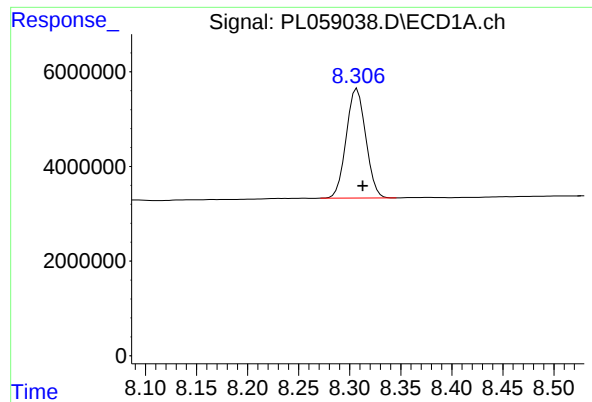

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: -0.006 min
Response: 30822182
Conc: 18.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

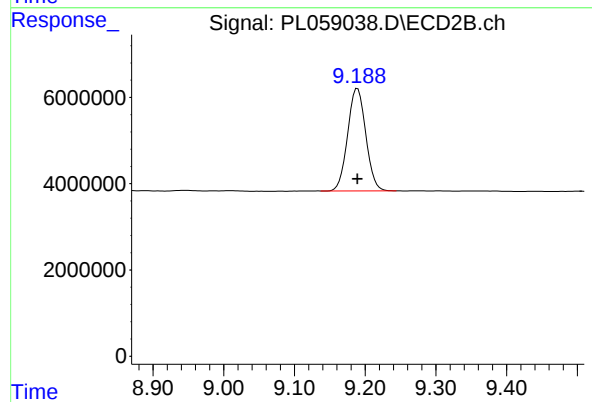

#28 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: 0.000 min
Response: 42341584
Conc: 16.06 ng/ml