

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
 Data File : PL059039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 19:46
 Operator : AJ\MA
 Sample : PB129208BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:05:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	4.077	34759895	50116079	18.957	18.504
28)	SA Decachlor...	8.307	9.190	31795187	44351733	18.819	16.824
Target Compounds							
2)	A alpha-BHC	3.983	0.000	1491485	0	0.549	N.D. #
4)	MA Heptachlor	0.000	5.263	0	2472638	N.D.	0.646 #
8)	B Heptachlo...	0.000	5.992f	0	344682	N.D.	0.105 #
10)	B gamma-Chl...	0.000	6.203	0	199323	N.D.	0.060 #
15)	B Endosulfa...	0.000	7.012	0	2111211	N.D.	0.753 #
17)	MA 4,4'-DDT	0.000	7.211	0	518037	N.D.	0.218 #
20)	A Methoxychlor	0.000	7.672	0	1006475	N.D.	0.722 #
25)	Chlordane-3	0.000	6.203	0	199323	N.D.	0.524 #
27)	Chlordane-5	0.000	7.079	0	2491067	N.D.	31.443 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
Data File : PL059039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 19:46
Operator : AJ\MA
Sample : PB129208BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:05:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

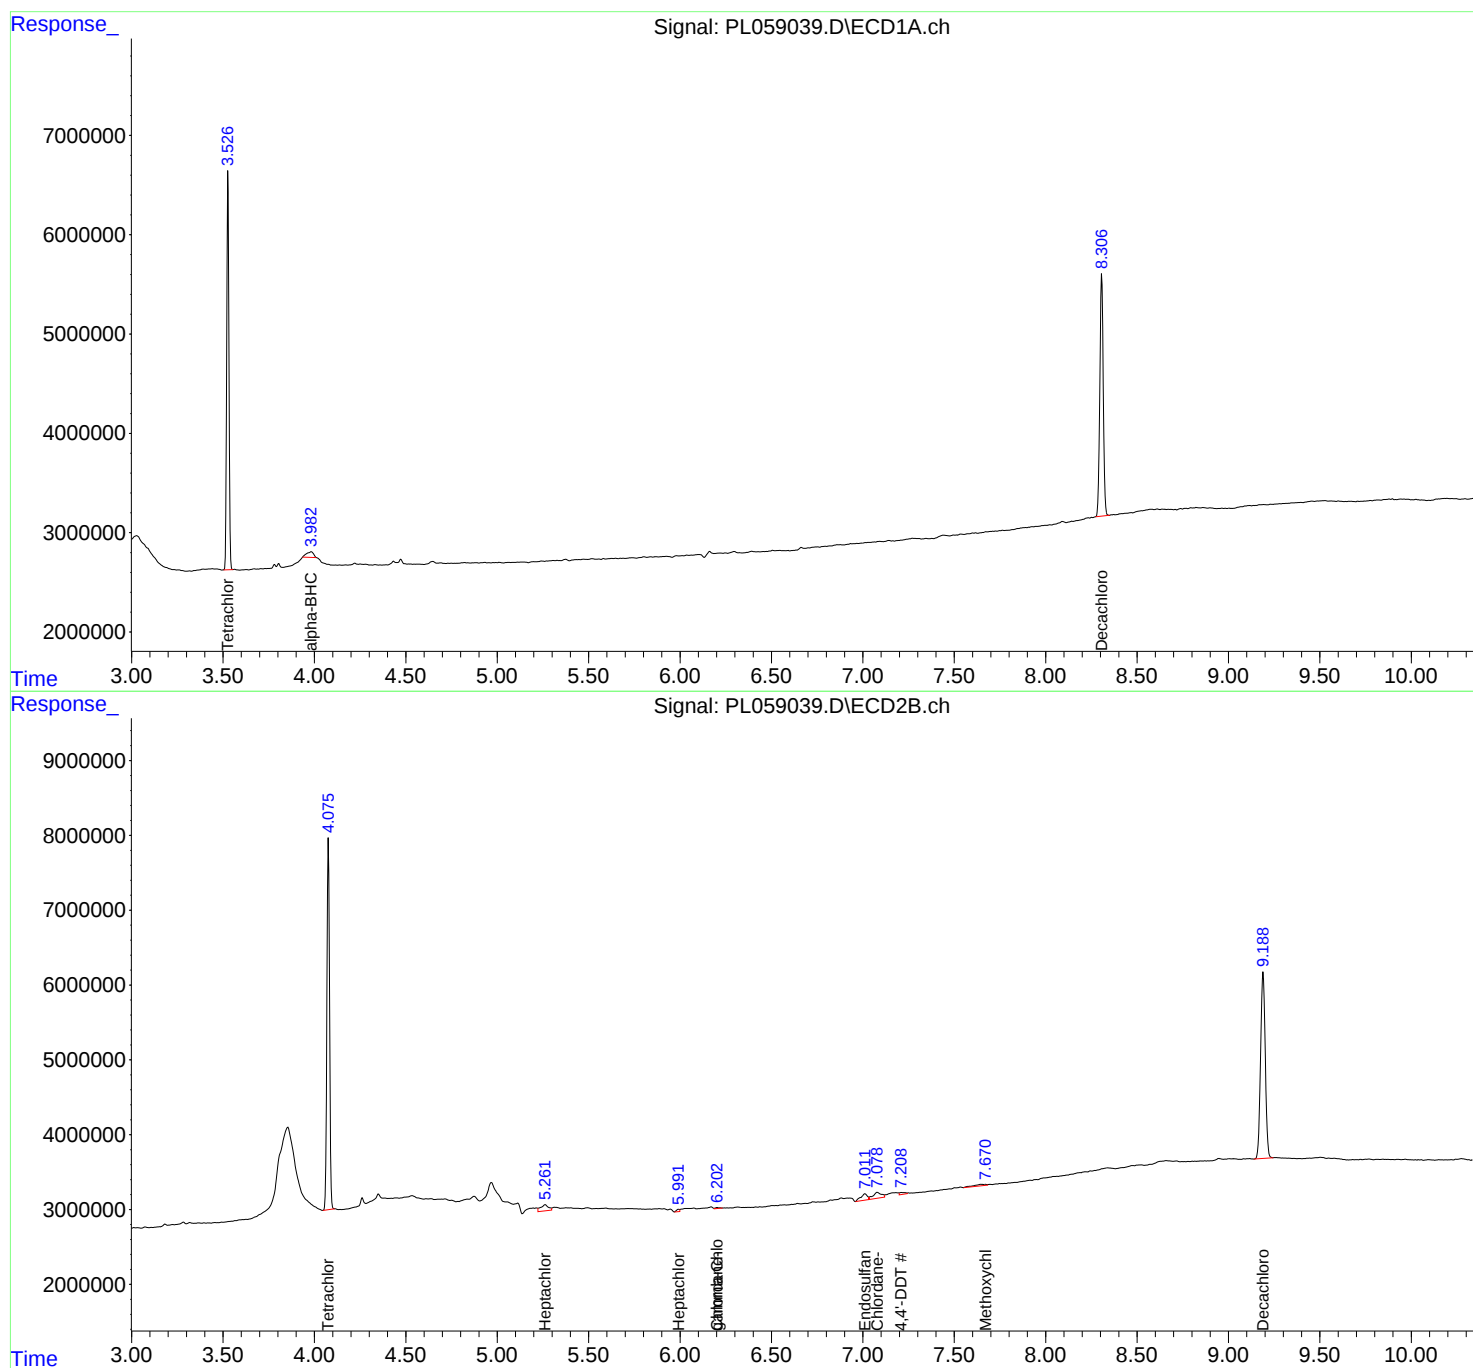


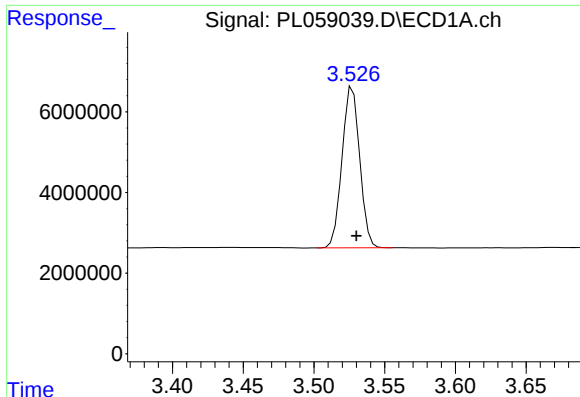

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: -0.003 min
Response: 34759895
Conc: 18.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

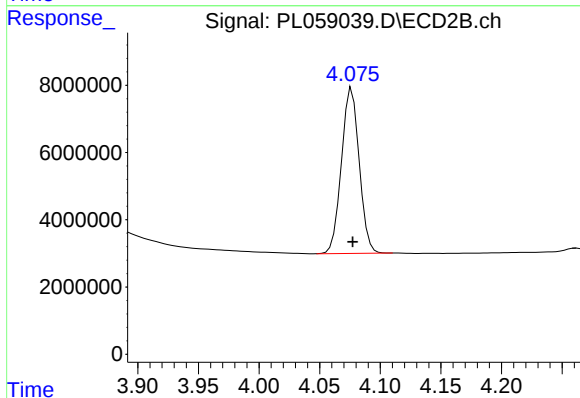


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 50116079
Conc: 18.50 ng/ml

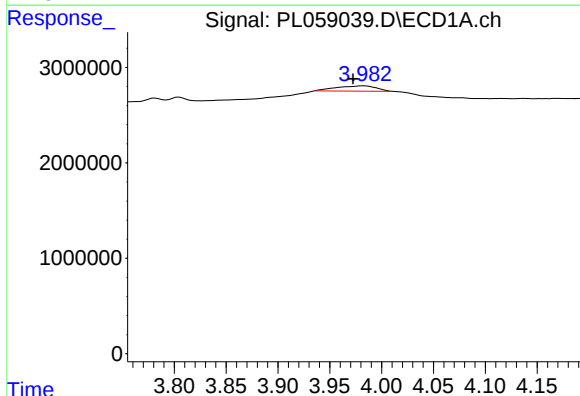


#2 alpha-BHC

R.T.: 3.983 min
Delta R.T.: 0.010 min
Response: 1491485
Conc: 0.55 ng/ml

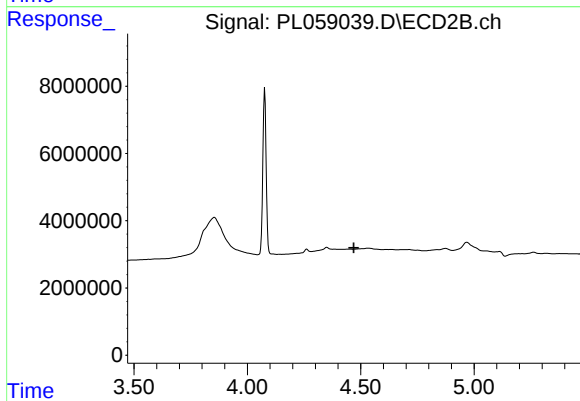

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

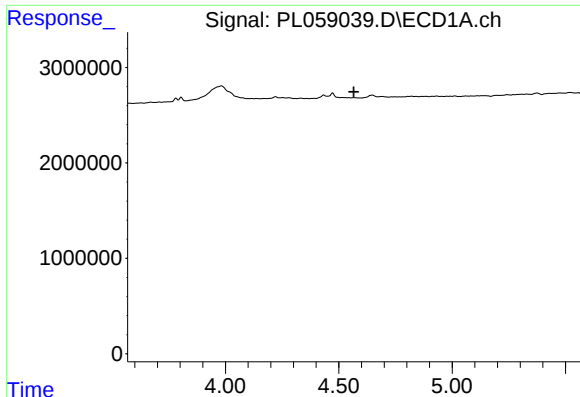

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

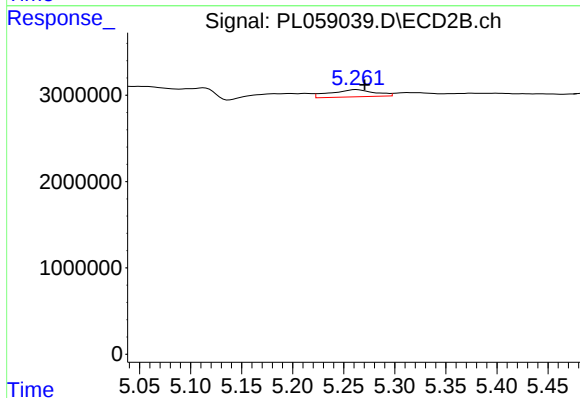


#4 Heptachlor

R.T.: 5.263 min
Delta R.T.: -0.008 min
Response: 2472638
Conc: 0.65 ng/ml

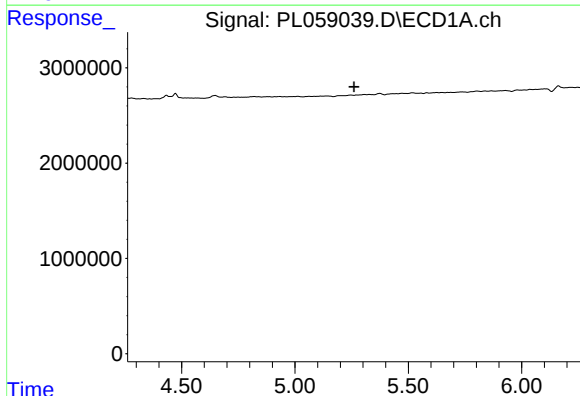


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.261 min
Response: 0
Conc: N.D.

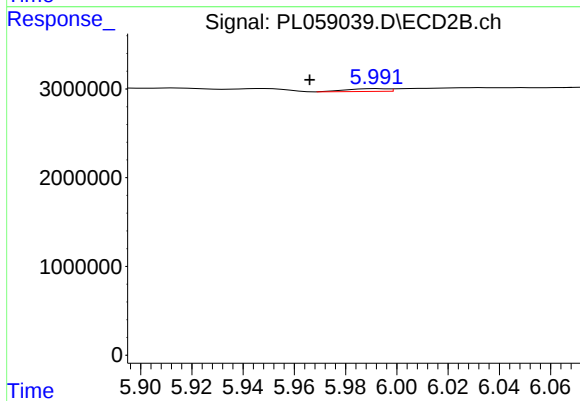

#8 Heptachlor epoxide


R.T.: 5.992 min
Delta R.T.: 0.026 min
Response: 344682
Conc: 0.10 ng/ml

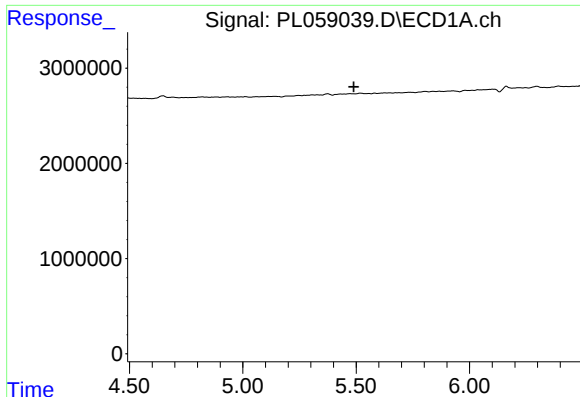

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

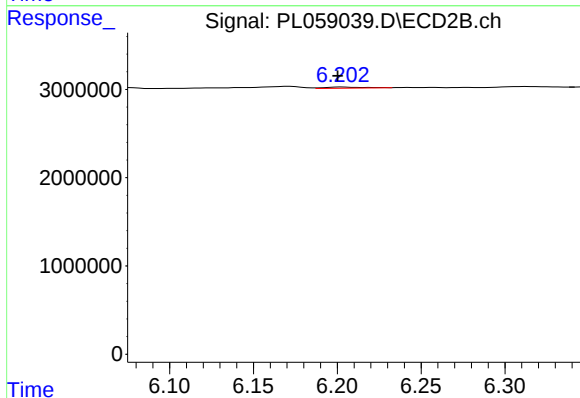


#10 gamma-Chlordane

R.T.: 6.203 min
Delta R.T.: 0.003 min
Response: 199323
Conc: 0.06 ng/ml

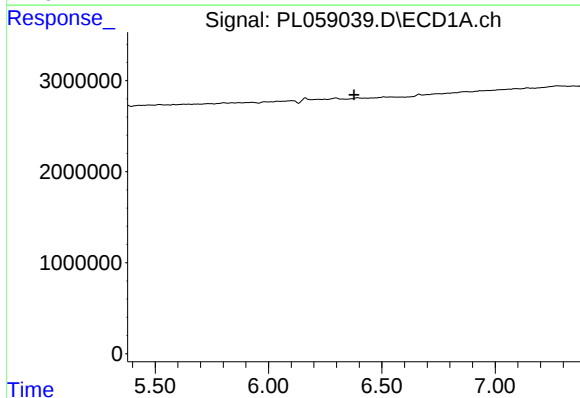


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

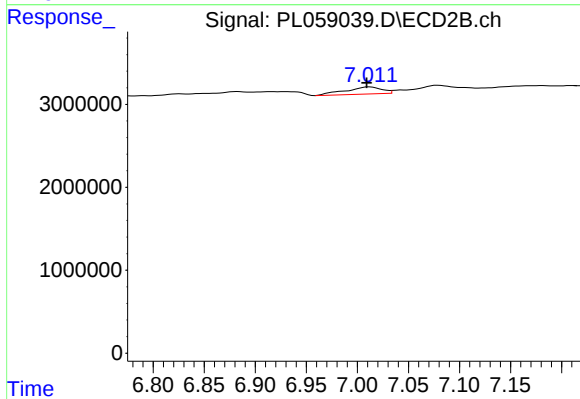

#15 Endosulfan II


R.T.: 7.012 min
Delta R.T.: 0.003 min
Response: 2111211
Conc: 0.75 ng/ml

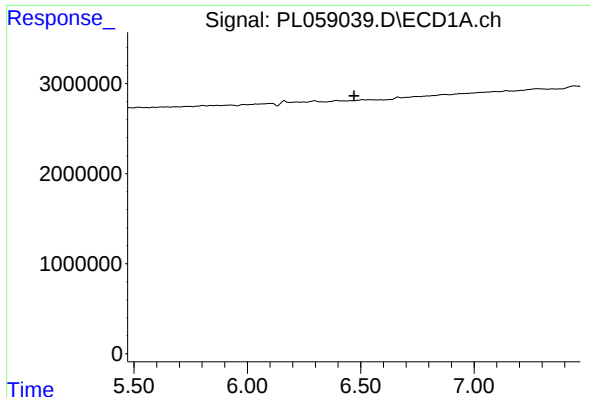

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

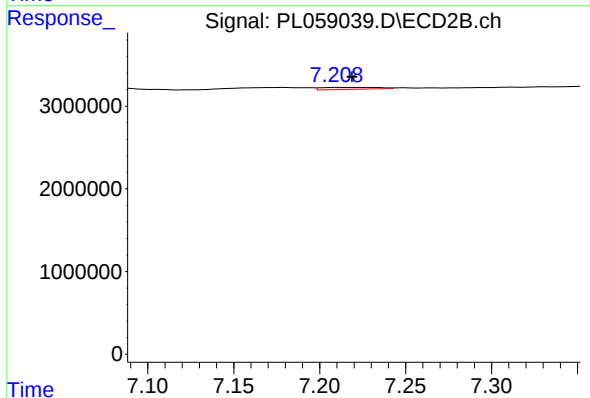


#17 4,4'-DDT

R.T.: 7.211 min
Delta R.T.: -0.008 min
Response: 518037
Conc: 0.22 ng/ml

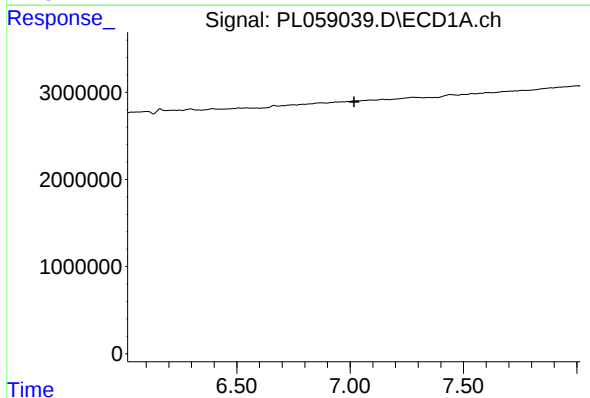


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.018 min
Response: 0
Conc: N.D.

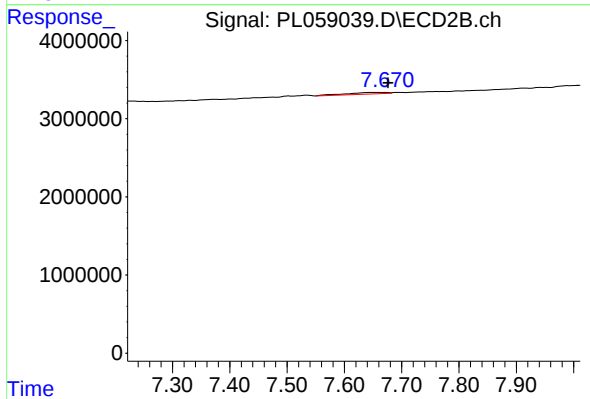

#20 Methoxychlor


R.T.: 7.672 min
Delta R.T.: -0.004 min
Response: 1006475
Conc: 0.72 ng/ml

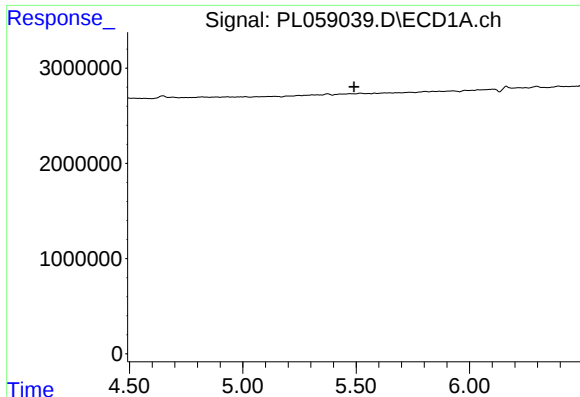

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

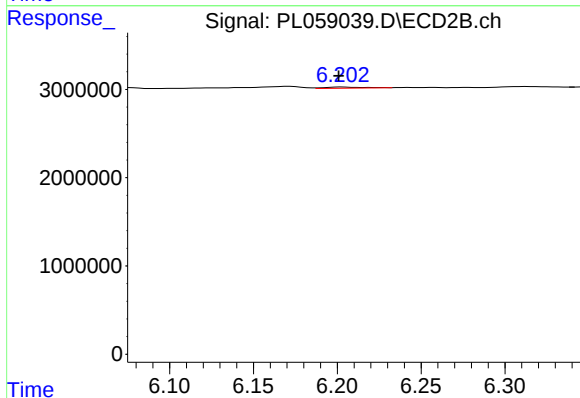


#25 Chlordane-3

R.T.: 6.203 min
Delta R.T.: 0.002 min
Response: 199323
Conc: 0.52 ng/ml

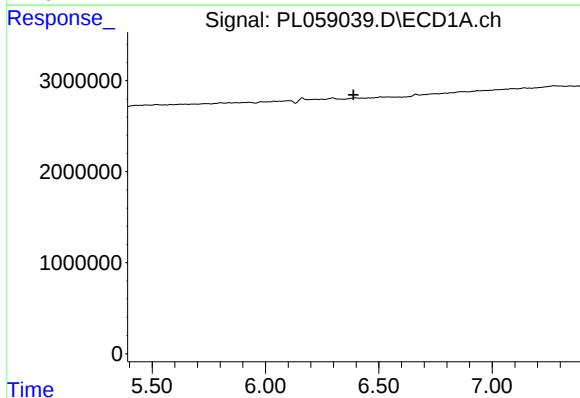


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

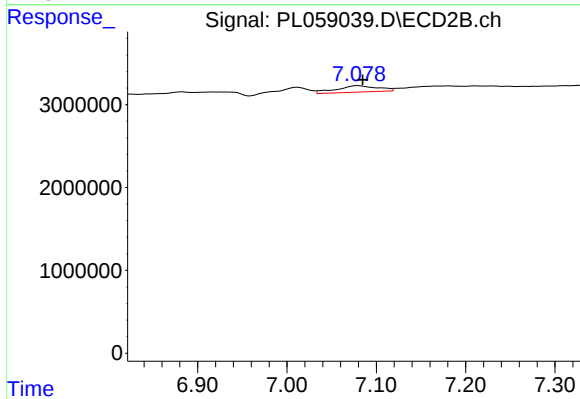

#27 Chlordane-5


R.T.: 7.079 min
Delta R.T.: -0.006 min
Response: 2491067
Conc: 31.44 ng/ml

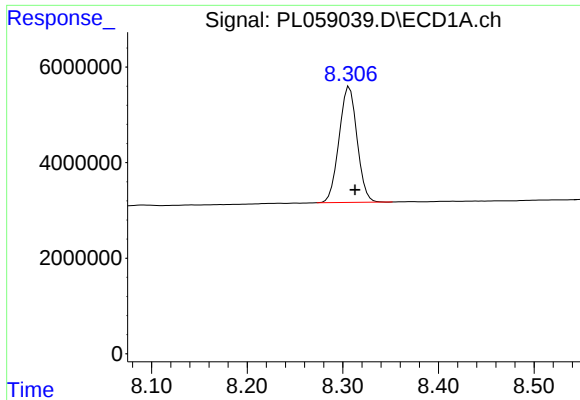

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: -0.006 min
Response: 31795187
Conc: 18.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

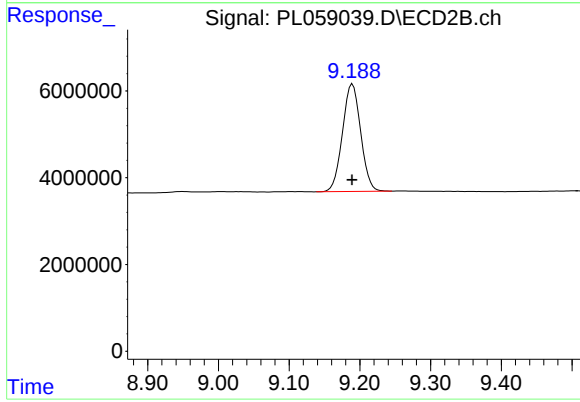

#28 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: 0.000 min
Response: 44351733
Conc: 16.82 ng/ml