

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
 Data File : PL059043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 20:42
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:06:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	4.076	37862878	54450443	20.649	20.104
28)	SA Decachlor...	8.307	9.189	34528942	47024721	20.437	17.838
Target Compounds							
2)	A alpha-BHC	3.982	0.000	1603630	0	0.590	N.D. #
4)	MA Heptachlor	0.000	5.264	0	2825860	N.D.	0.738 #
9)	A Endosulfan I	0.000	6.310	0	240542	N.D.	0.082 #
10)	B gamma-Chl...	0.000	6.204	0	323126	N.D.	0.098 #
11)	B alpha-Chl...	0.000	6.258f	0	217346	N.D.	0.067 #
15)	B Endosulfa...	0.000	7.012	0	962456	N.D.	0.343 #
20)	A Methoxychlor	0.000	7.663	0	206011	N.D.	0.148 #
25)	Chlordane-3	0.000	6.204	0	323126	N.D.	0.849 #
26)	Chlordane-4	0.000	6.258f	0	217346	N.D.	0.477 #
27)	Chlordane-5	0.000	7.079	0	1510643	N.D.	19.068 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
Data File : PL059043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 20:42
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:06:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

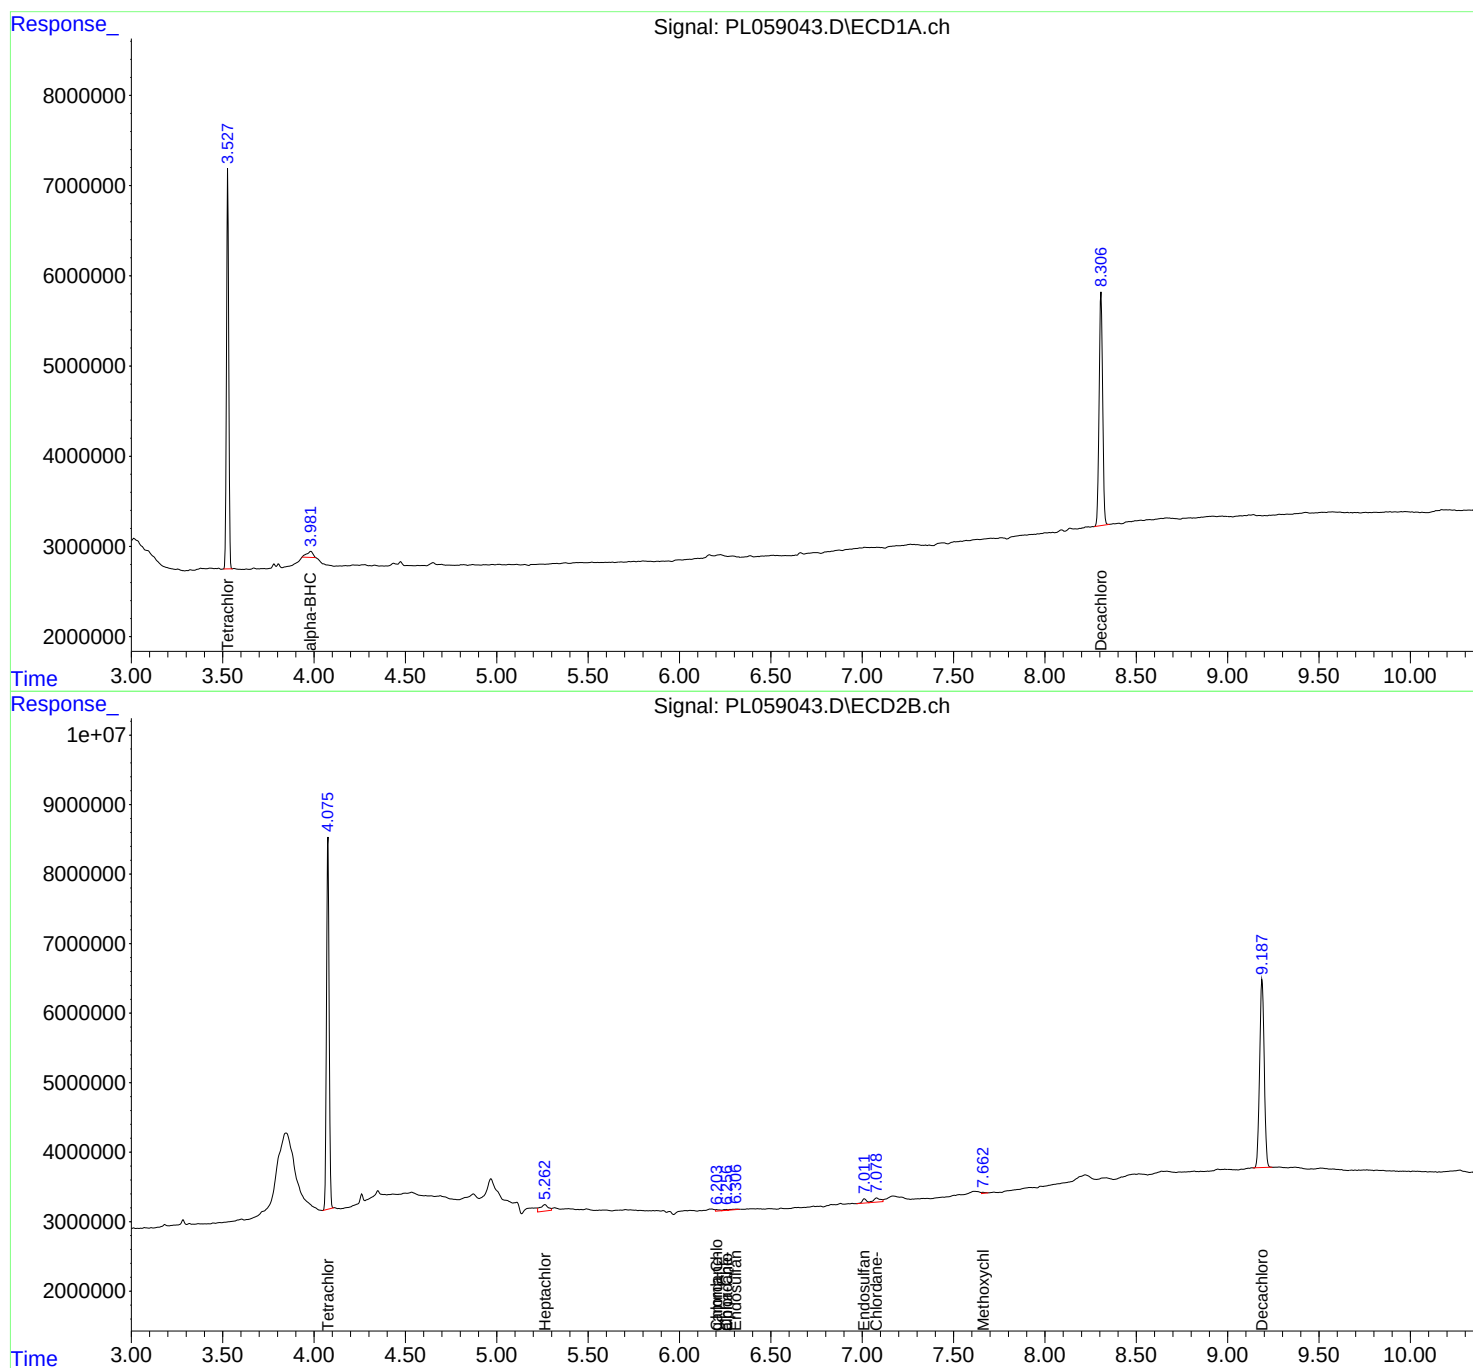


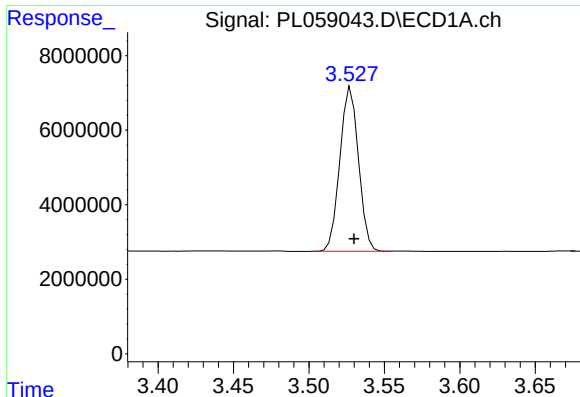

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: -0.002 min
Response: 37862878
Conc: 20.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

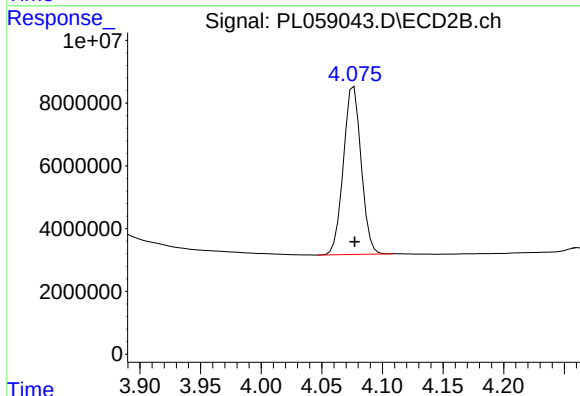


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: 0.000 min
Response: 54450443
Conc: 20.10 ng/ml

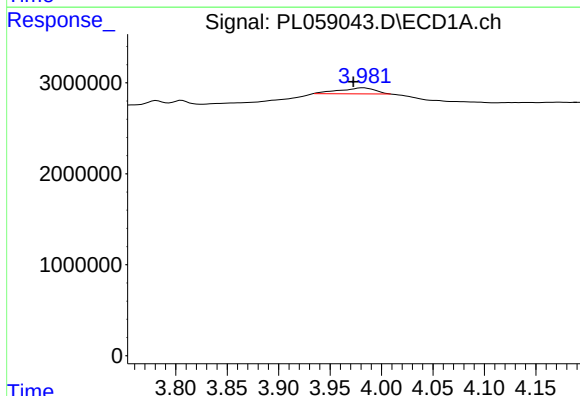


#2 alpha-BHC

R.T.: 3.982 min
Delta R.T.: 0.010 min
Response: 1603630
Conc: 0.59 ng/ml

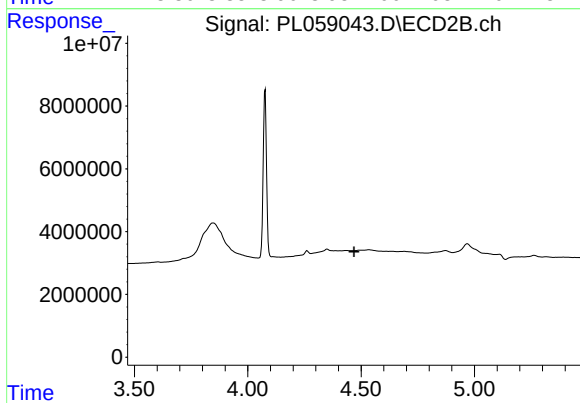

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

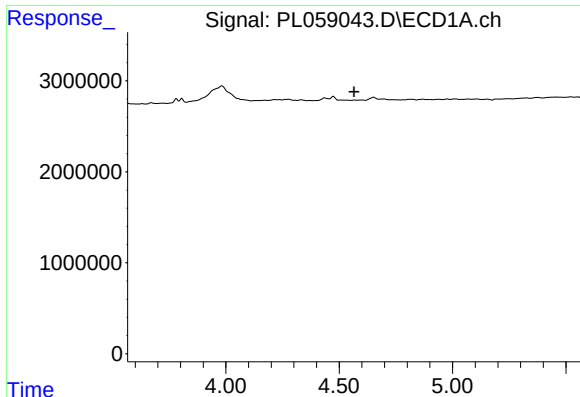

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

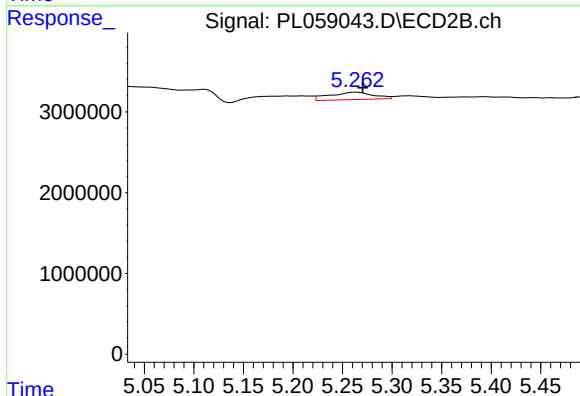


#4 Heptachlor

R.T.: 5.264 min
Delta R.T.: -0.007 min
Response: 2825860
Conc: 0.74 ng/ml

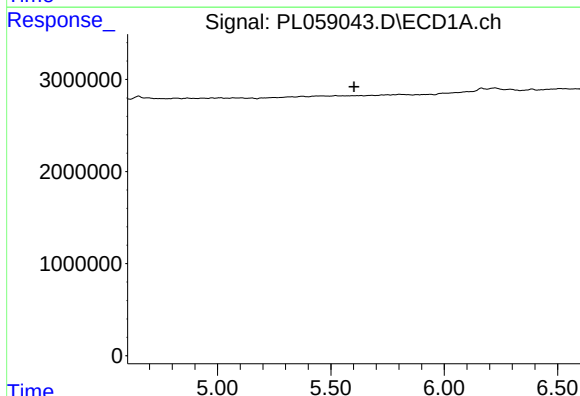


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.603 min
Response: 0
Conc: N.D.

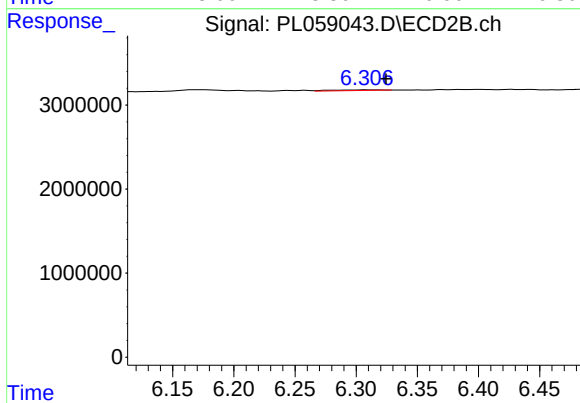

#9 Endosulfan I


R.T.: 6.310 min
Delta R.T.: -0.015 min
Response: 240542
Conc: 0.08 ng/ml

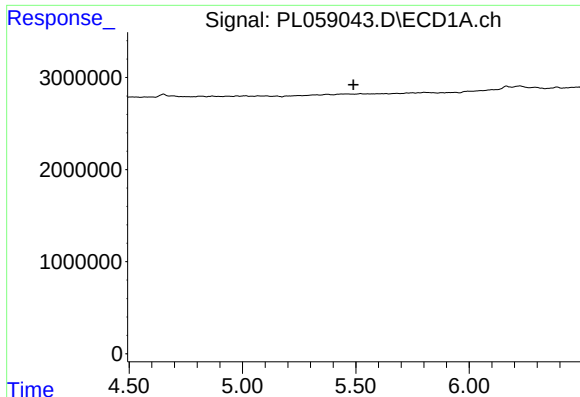

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

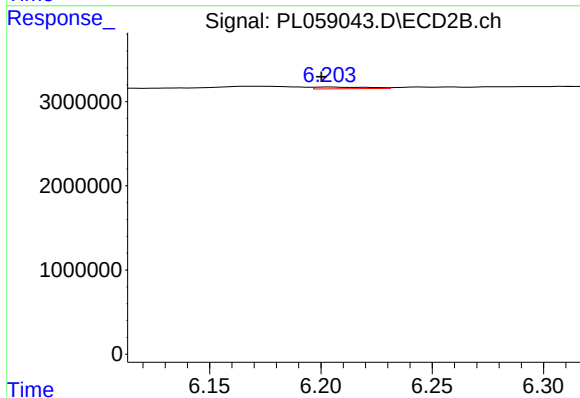


#10 gamma-Chlordane

R.T.: 6.204 min
Delta R.T.: 0.004 min
Response: 323126
Conc: 0.10 ng/ml

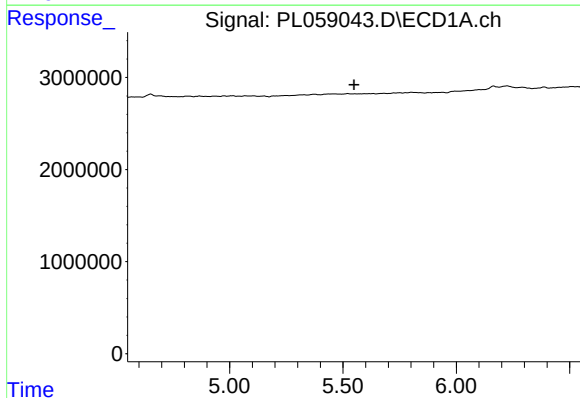


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.549 min
Response: 0
Conc: N.D.

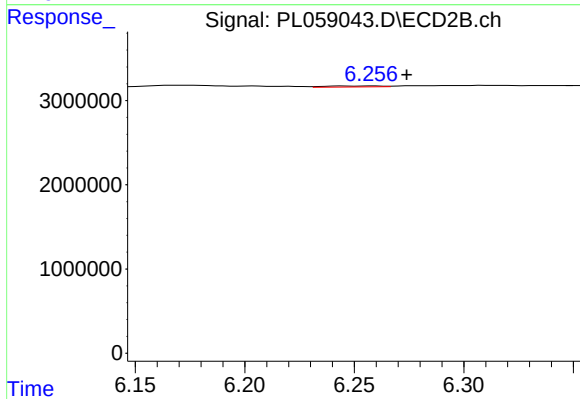

#11 alpha-Chlordane


R.T.: 6.258 min
Delta R.T.: -0.016 min
Response: 217346
Conc: 0.07 ng/ml

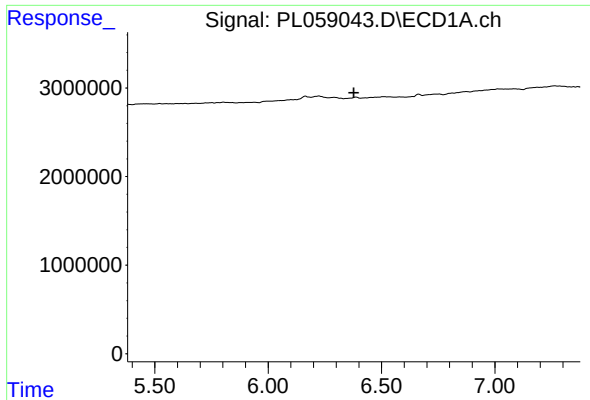

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

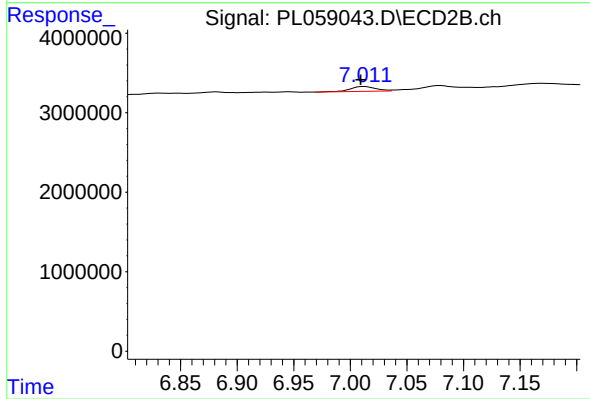


#15 Endosulfan II

R.T.: 7.012 min
Delta R.T.: 0.003 min
Response: 962456
Conc: 0.34 ng/ml

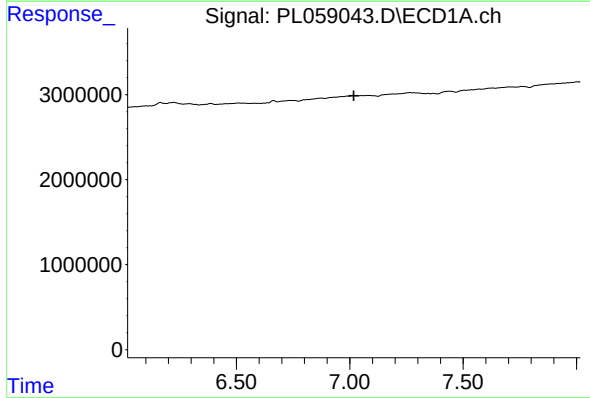


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.018 min
Response: 0
Conc: N.D.

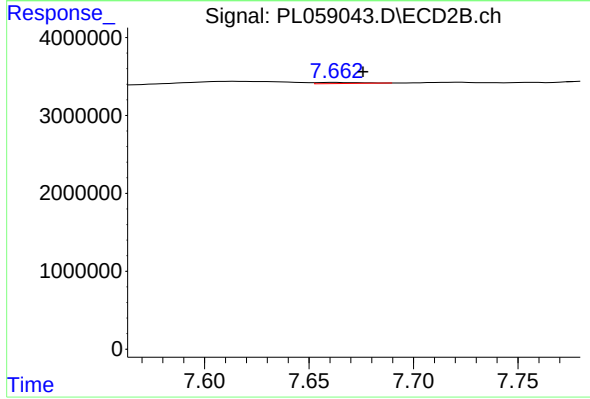

#20 Methoxychlor


R.T.: 7.663 min
Delta R.T.: -0.013 min
Response: 206011
Conc: 0.15 ng/ml

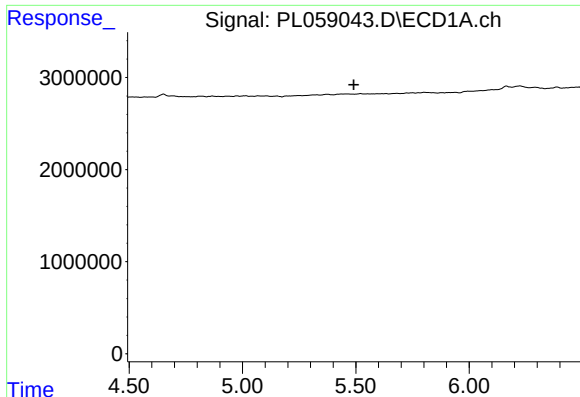

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

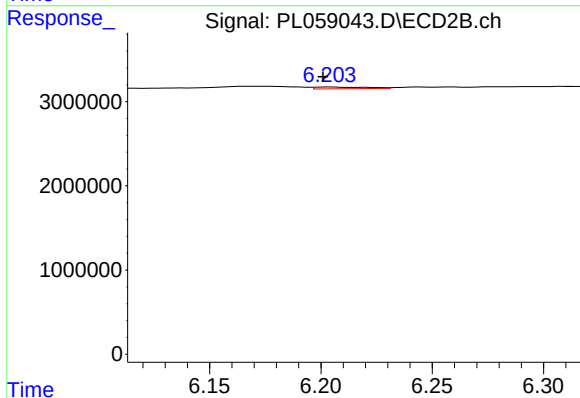


#25 Chlordane-3

R.T.: 6.204 min
Delta R.T.: 0.003 min
Response: 323126
Conc: 0.85 ng/ml

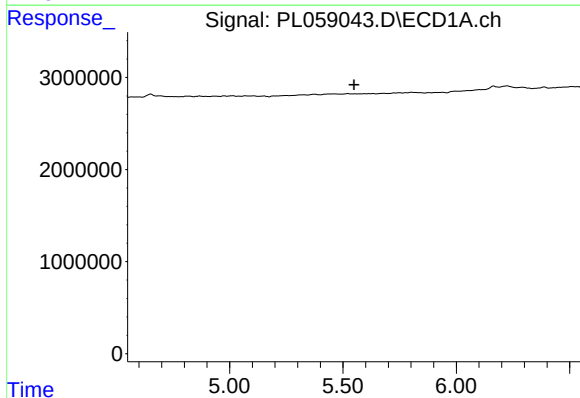


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

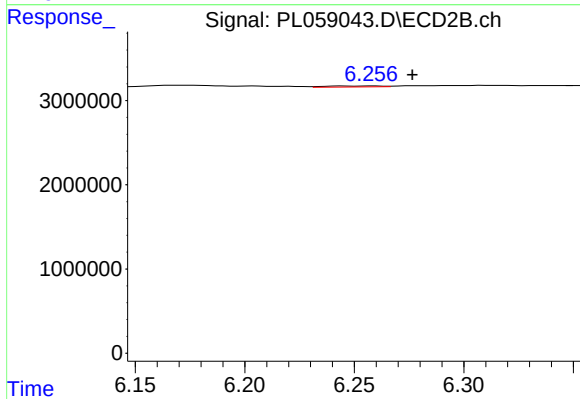

#26 Chlordane-4


R.T.: 6.258 min
Delta R.T.: -0.018 min
Response: 217346
Conc: 0.48 ng/ml

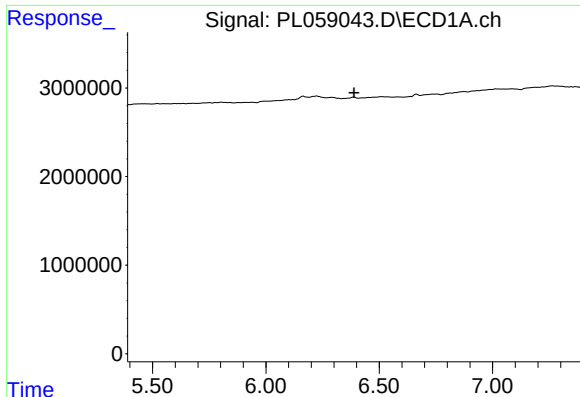

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

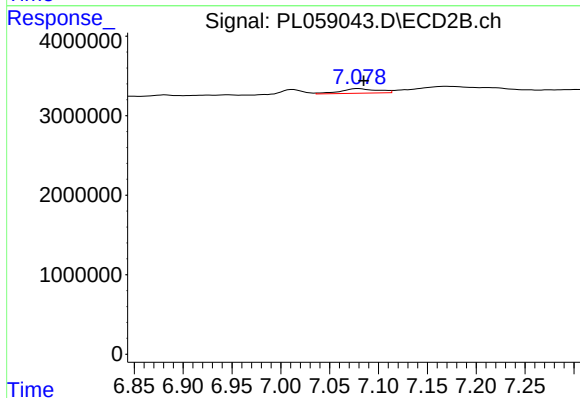


#27 Chlordane-5

R.T.: 7.079 min
Delta R.T.: -0.006 min
Response: 1510643
Conc: 19.07 ng/ml

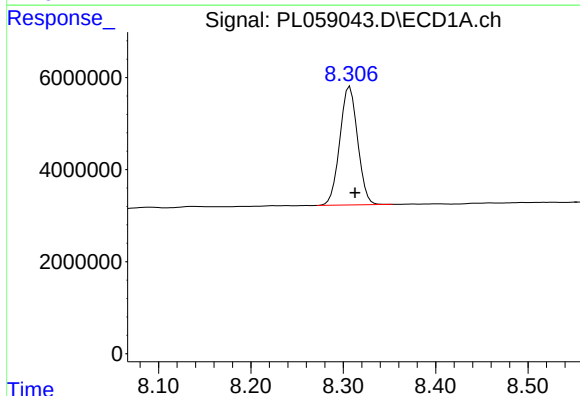

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: -0.006 min
Response: 34528942
Conc: 20.44 ng/ml

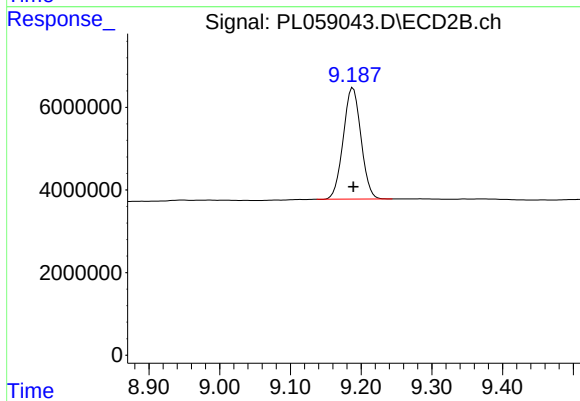

#28 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: 0.000 min
Response: 47024721
Conc: 17.84 ng/ml