

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
 Data File : PL059011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 11:40
 Operator : AJ\MA
 Sample : L2798-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NM87-COMP-2020-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 14:42:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	4.076	21604874	28242756	11.783	10.428
28)	SA Decachlor...	8.307	9.189	15313484	24792704	9.064	9.405
Target Compounds							
11)	B alpha-Chl...	5.544	6.274	2299059	14870583	1.256	4.578m#
12)	B 4,4'-DDE	5.708	6.427	2210149	5125505	1.346	1.796 #
17)	MA 4,4'-DDT	6.464	7.219	2579941	1557397	1.774	0.655 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060120\
Data File : PL059011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 11:40
Operator : AJ\MA
Sample : L2798-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NM87-COMP-2020-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 14:42:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

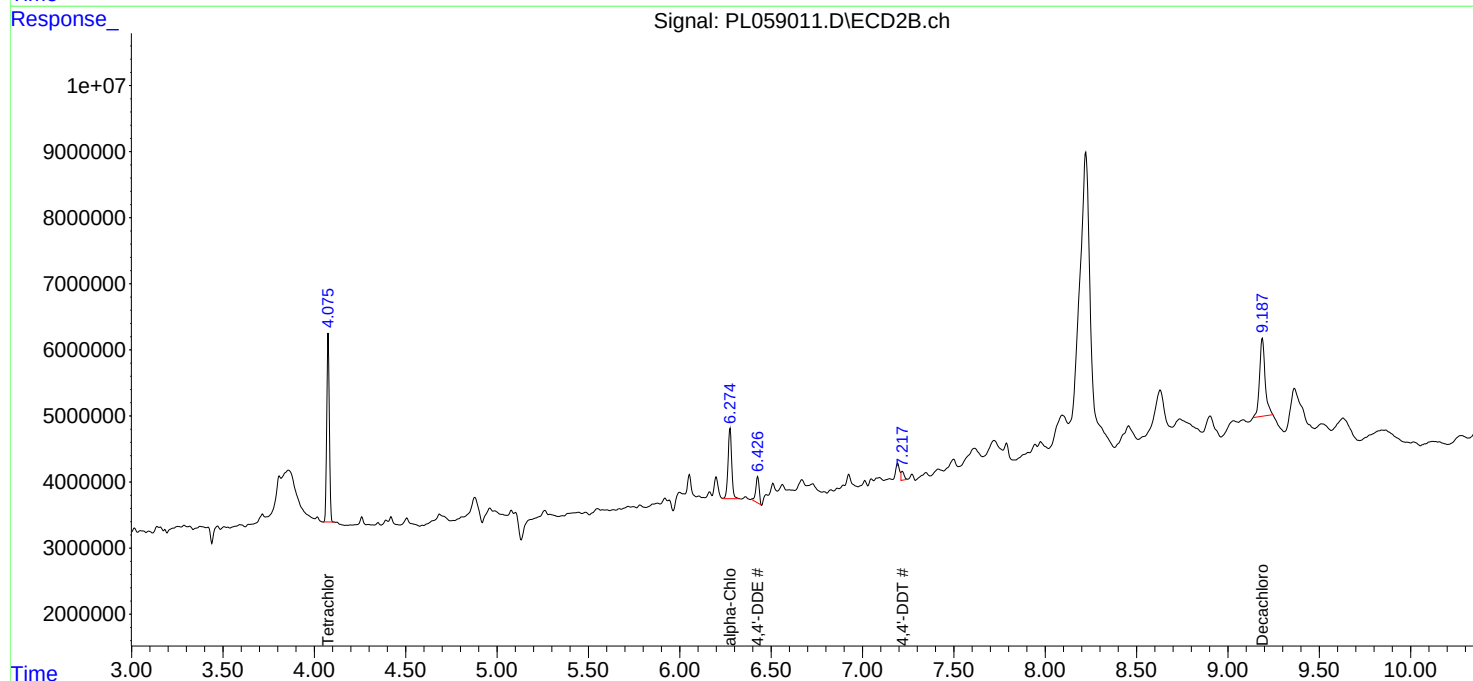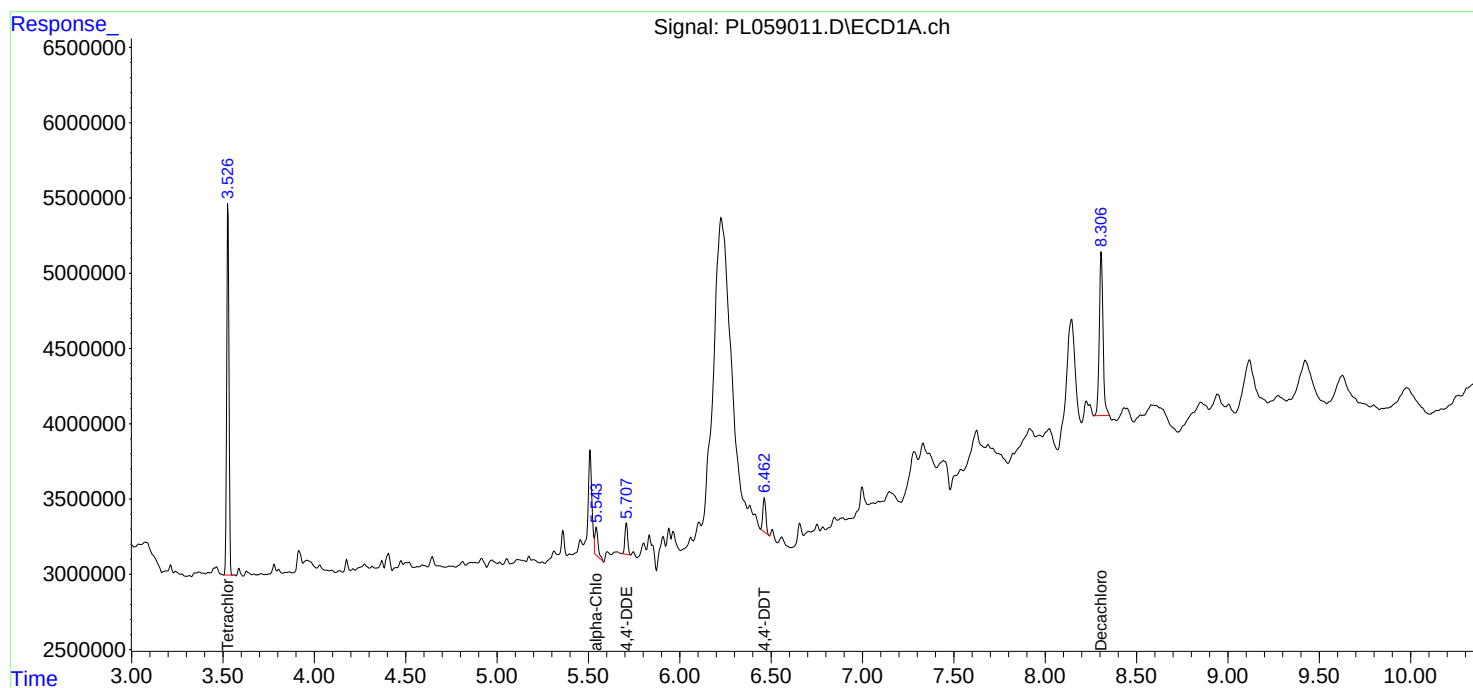


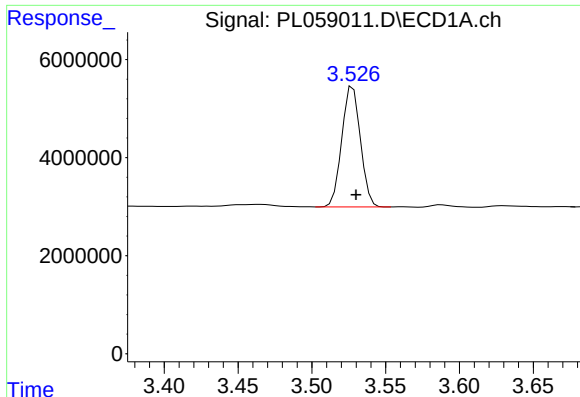

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: -0.002 min
Response: 21604874
Conc: 11.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM87-COMP-2020-0-6

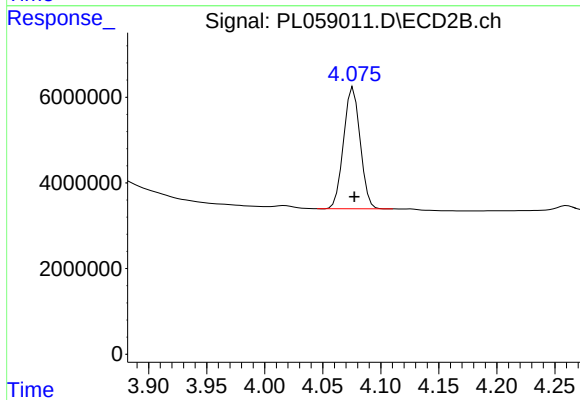


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: 0.000 min
Response: 28242756
Conc: 10.43 ng/ml

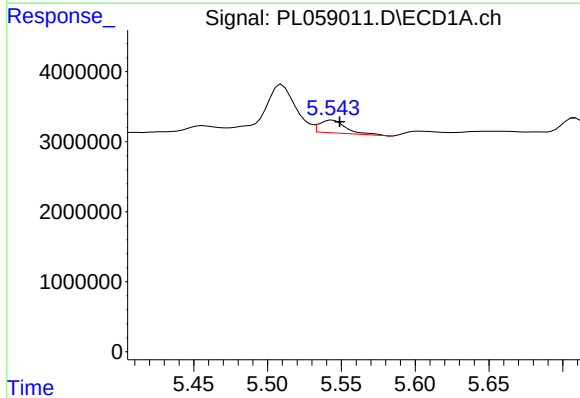


#11 alpha-Chlordane

R.T.: 5.544 min
Delta R.T.: -0.005 min
Response: 2299059
Conc: 1.26 ng/ml

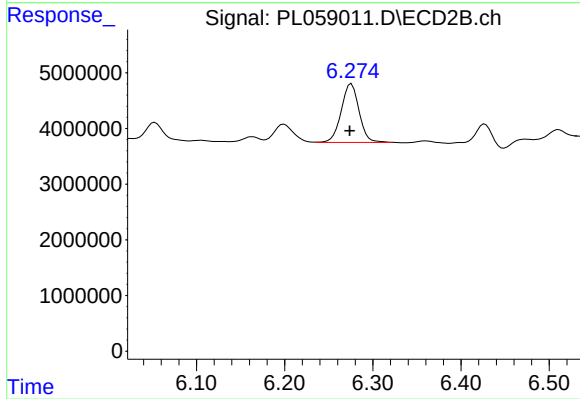

#11 alpha-Chlordane


R.T.: 6.274 min
Delta R.T.: 0.000 min
Response: 14870583
Conc: 4.58 ng/ml m

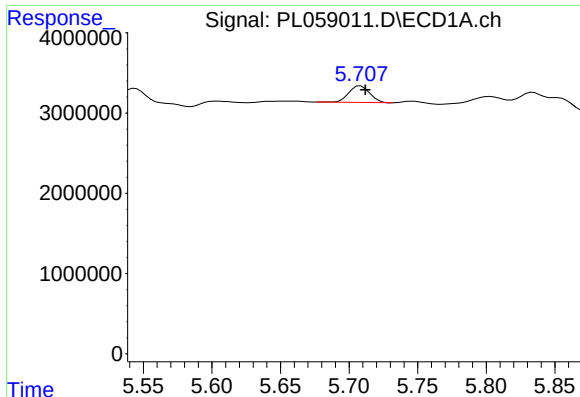

#12 4,4'-DDE


R.T.: 5.708 min
Delta R.T.: -0.004 min
Response: 2210149
Conc: 1.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM87-COMP-2020-0-6

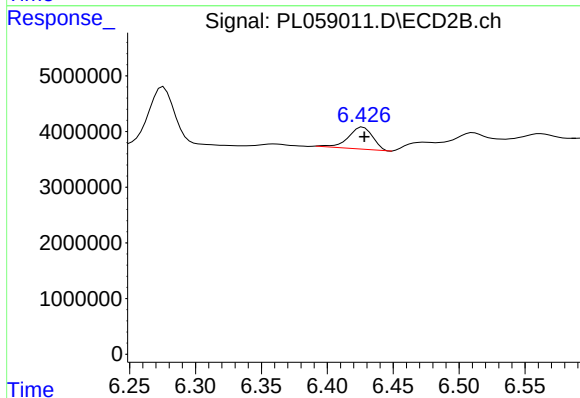


#12 4,4'-DDE

R.T.: 6.427 min
Delta R.T.: 0.000 min
Response: 5125505
Conc: 1.80 ng/ml

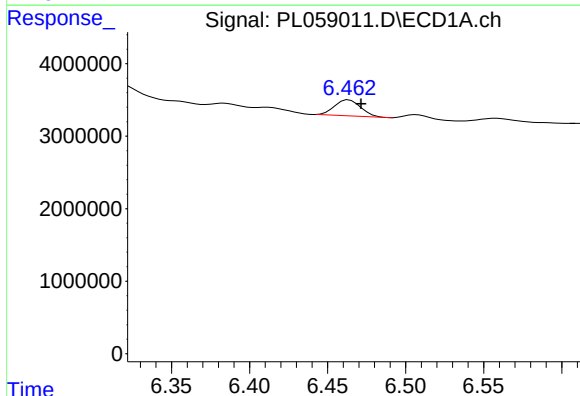


#17 4,4'-DDT

R.T.: 6.464 min
Delta R.T.: -0.008 min
Response: 2579941
Conc: 1.77 ng/ml

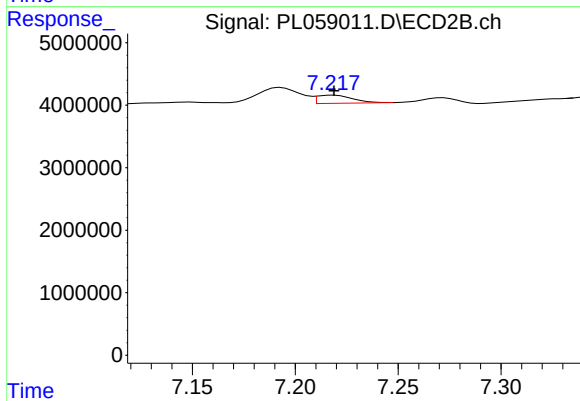

#17 4,4'-DDT


R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 1557397
Conc: 0.65 ng/ml

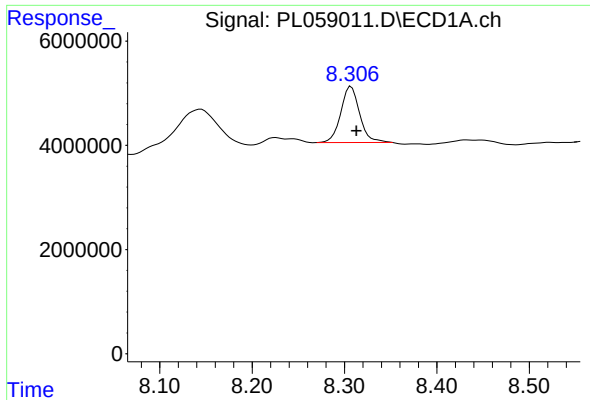

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: -0.006 min
Response: 15313484
Conc: 9.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM87-COMP-2020-0-6

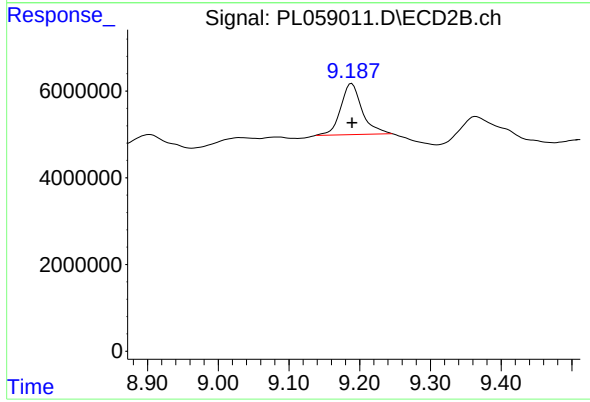

#28 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: 0.000 min
Response: 24792704
Conc: 9.40 ng/ml