

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 09:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 15:51:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.642	12641823	33943039	21.509	21.427
28)	SA Decachlor...	11.640	10.387	12004761	28418001	22.389	20.709
Target Compounds							
7)	B delta-BHC	0.000	6.409	0	409391	N.D.	0.191 #
8)	B Heptachlo...	8.126	0.000	2446643	0	3.584	N.D. #
11)	B alpha-Chl...	0.000	7.396f	0	236175	N.D.	0.129 #
13)	MA Dieldrin	0.000	7.758	0	2812211	N.D.	1.621 #
14)	MA Endrin	0.000	8.070f	0	916995	N.D.	0.589 #
15)	B Endosulfa...	9.307	0.000	172837	0	0.306	N.D. #
17)	MA 4,4'-DDT	9.532	0.000	172382	0	0.296	N.D. #
21)	B Endrin ke...	10.188f	0.000	482448	0	0.786	N.D. #
26)	Chlordane-4	0.000	7.396f	0	236175	N.D.	1.250 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 09:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 15:51:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

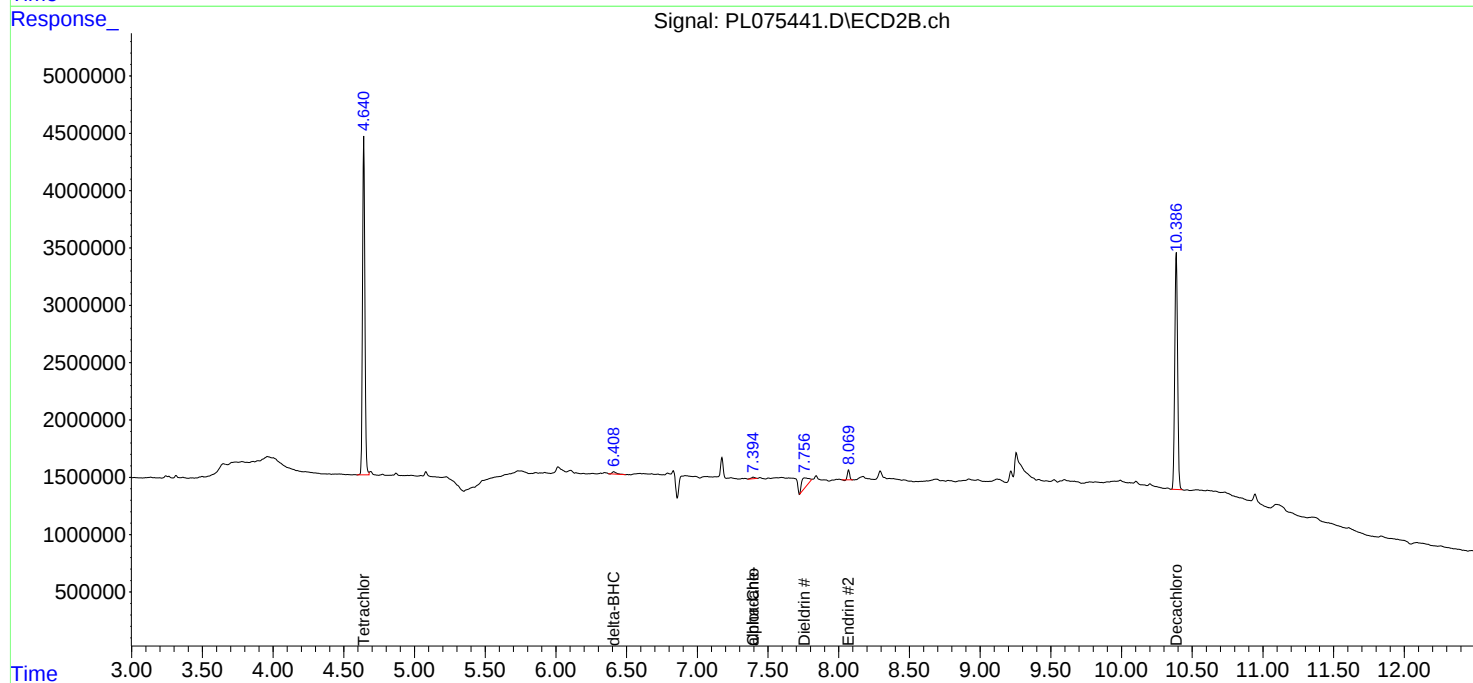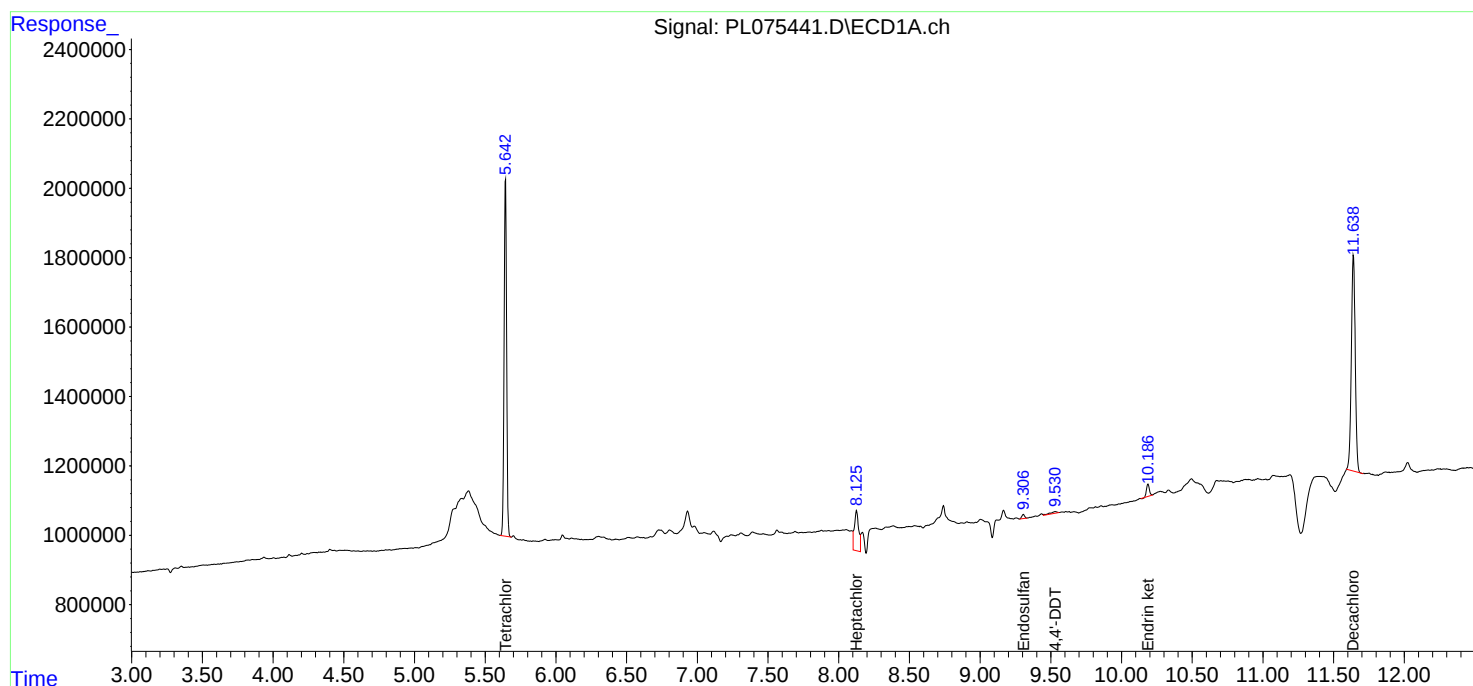


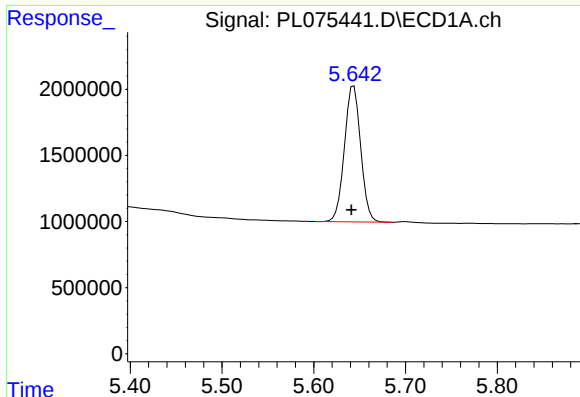

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 12641823
Conc: 21.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

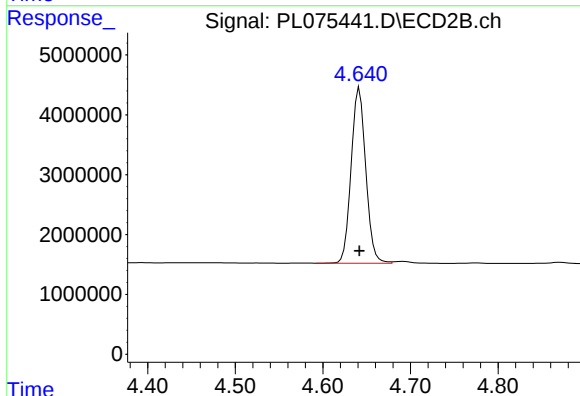


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 33943039
Conc: 21.43 ng/ml

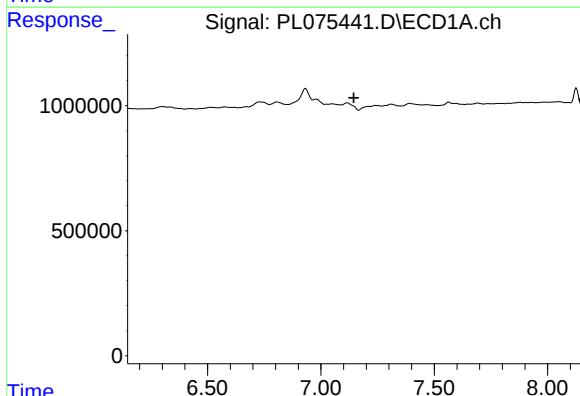


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

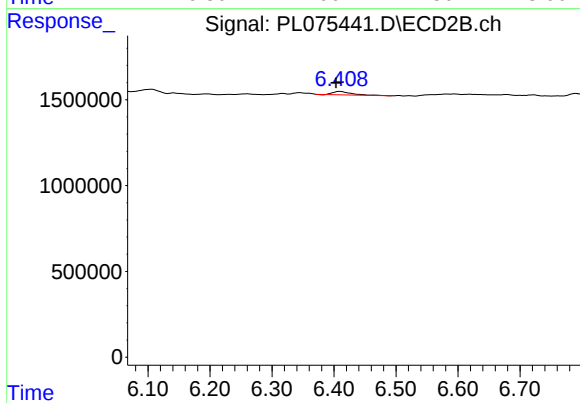

#7 delta-BHC


R.T.: 6.409 min
Delta R.T.: 0.006 min
Response: 409391
Conc: 0.19 ng/ml

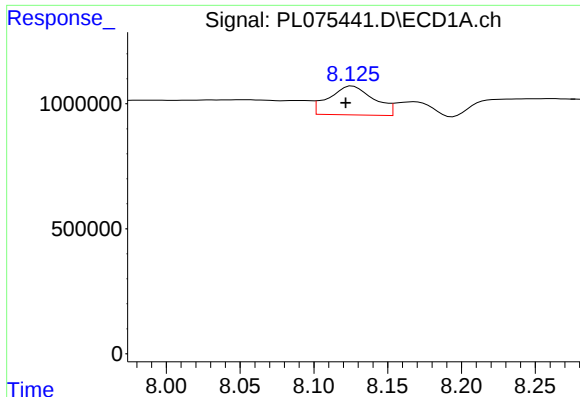

#8 Heptachlor epoxide


R.T.: 8.126 min
Delta R.T.: 0.005 min
Response: 2446643
Conc: 3.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

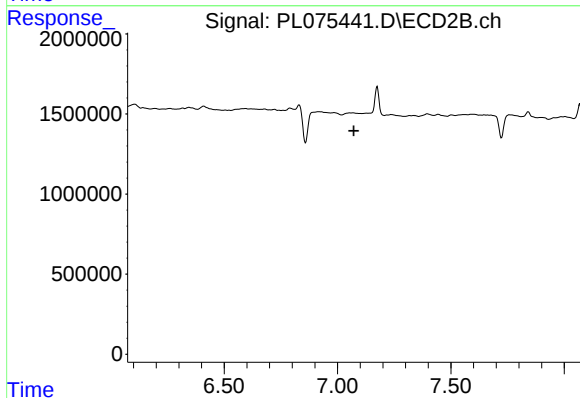


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

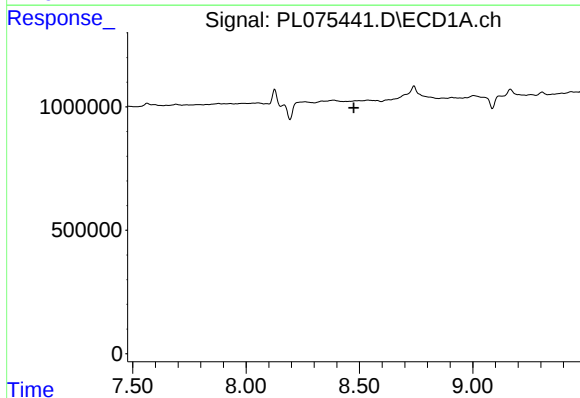


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

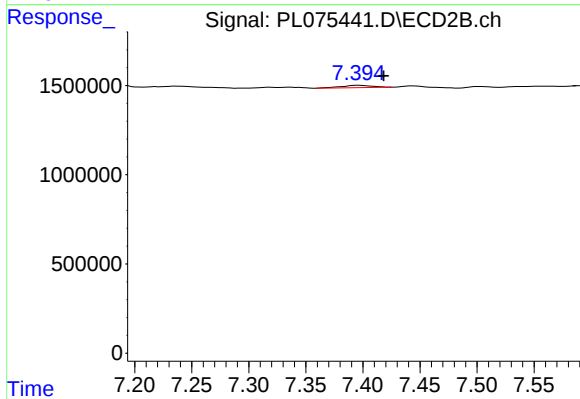

#11 alpha-Chlordane


R.T.: 7.396 min
Delta R.T.: -0.022 min
Response: 236175
Conc: 0.13 ng/ml

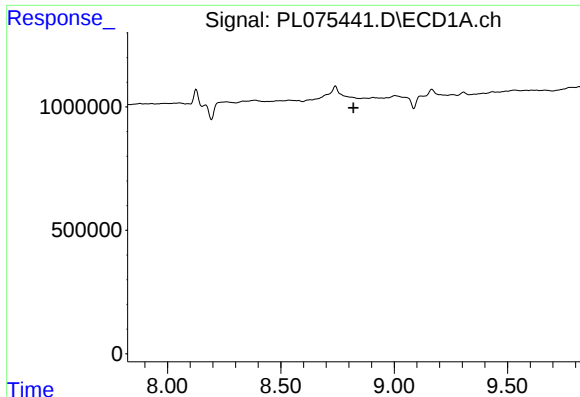

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

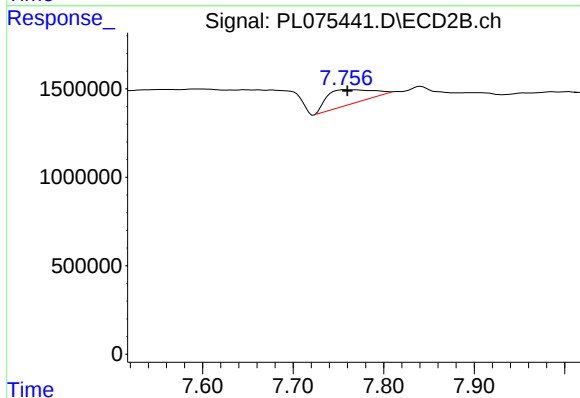


#13 Dieldrin

R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 2812211
Conc: 1.62 ng/ml

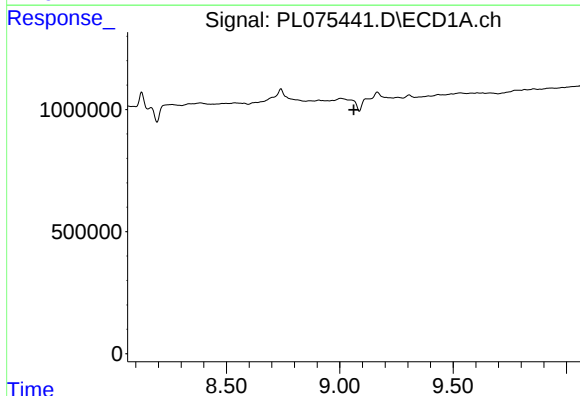


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

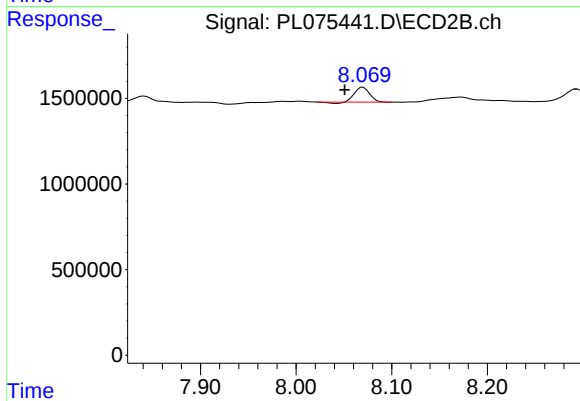

#14 Endrin


R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 916995
Conc: 0.59 ng/ml

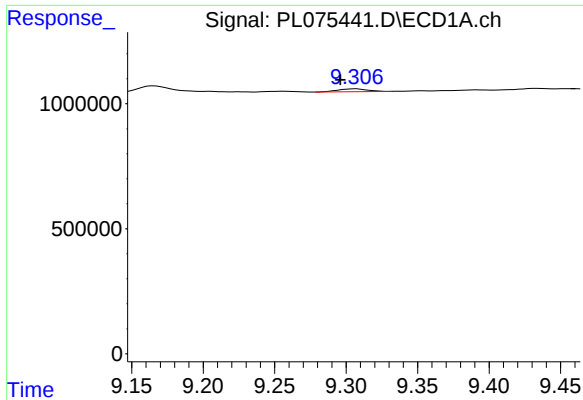

#15 Endosulfan II


R.T.: 9.307 min
Delta R.T.: 0.011 min
Response: 172837
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

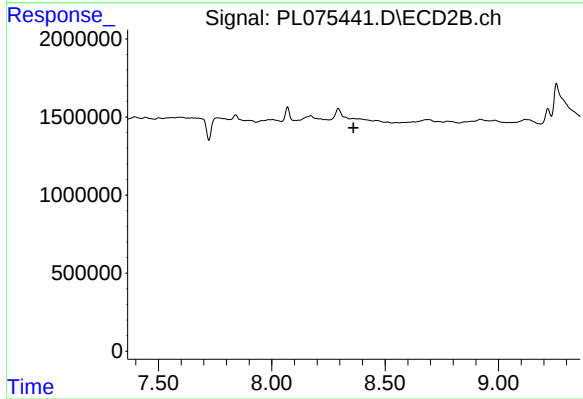


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

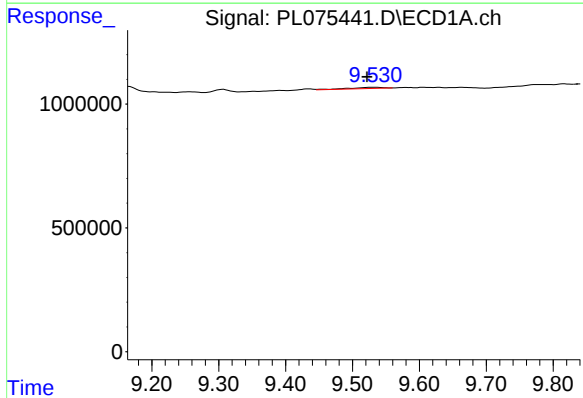


#17 4,4'-DDT

R.T.: 9.532 min
Delta R.T.: 0.010 min
Response: 172382
Conc: 0.30 ng/ml

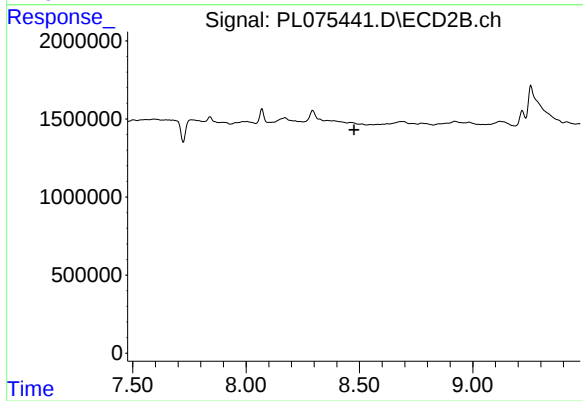

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

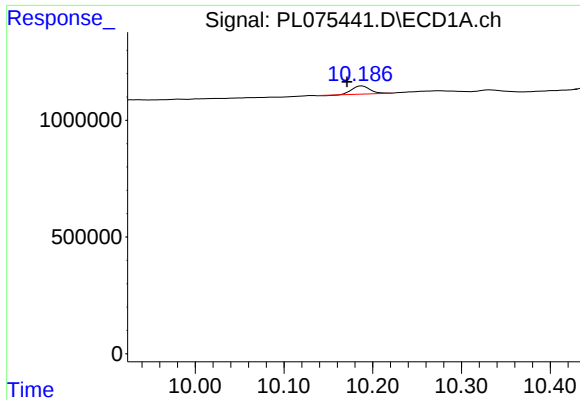

#21 Endrin ketone


R.T.: 10.188 min
Delta R.T.: 0.017 min
Response: 482448
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

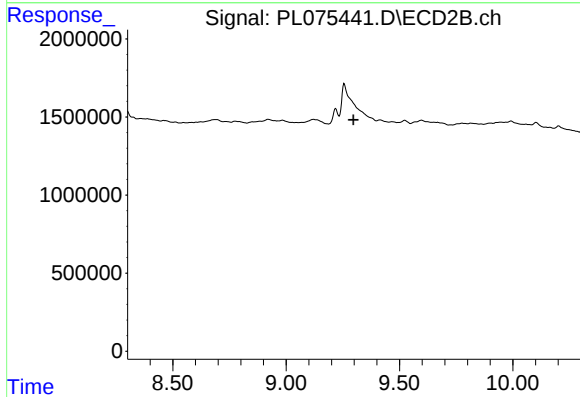


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

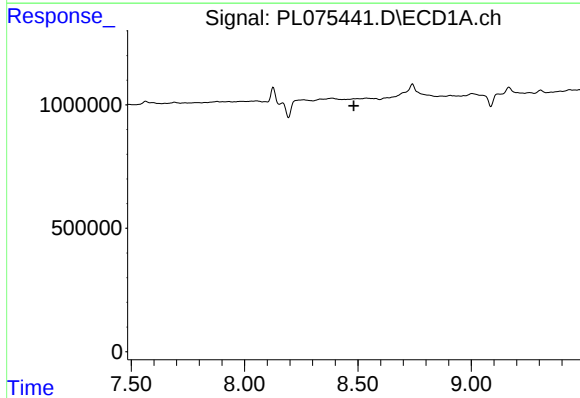


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

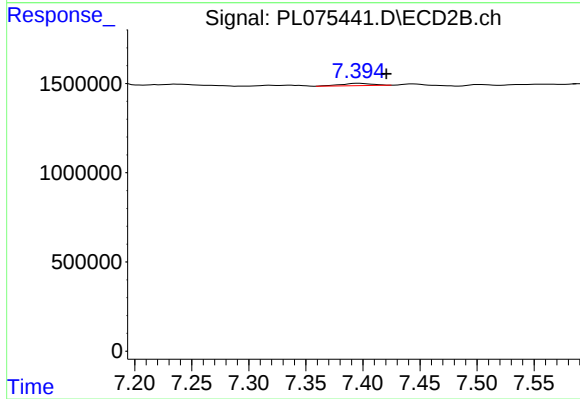

#26 Chlordane-4


R.T.: 7.396 min
Delta R.T.: -0.024 min
Response: 236175
Conc: 1.25 ng/ml

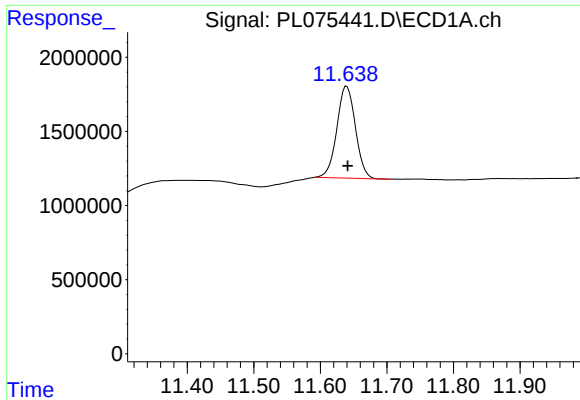

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.001 min
Response: 12004761
Conc: 22.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

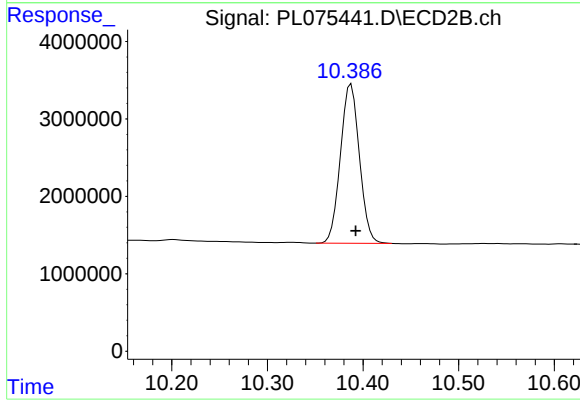

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.005 min
Response: 28418001
Conc: 20.71 ng/ml