

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 10:35
 Operator : AR\AJ
 Sample : N2987-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 15:52:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.651	4.642	11108538	29405849	18.900	18.563
28)	SA Decachlor...	11.647	10.390	9042943	21651596	16.865	15.778
Target Compounds							
8)	B Heptachlo...	8.133	0.000	238646	0	0.350	N.D. #
9)	A Endosulfan I	8.509f	7.467	387841	460279	0.618	0.272 #
10)	B gamma-Chl...	0.000	7.349	0	406220	N.D.	0.221 #
13)	MA Dieldrin	0.000	7.756	0	535382	N.D.	0.309 #
14)	MA Endrin	0.000	8.070f	0	436320	N.D.	0.280 #
15)	B Endosulfa...	9.300	0.000	755643	0	1.339	N.D. #
17)	MA 4,4'-DDT	9.524	8.468	1073207	138522	1.843	0.097 #
19)	B Endosulfa...	9.649f	0.000	486628	0	0.875	N.D. #
21)	B Endrin ke...	10.184	0.000	1657310	0	2.699	N.D. #
25)	Chlordane-3	0.000	7.349	0	406220	N.D.	2.301 #
26)	Chlordane-4	8.509f	0.000	387841	0	3.417	N.D. #
27)	Chlordane-5	0.000	8.131	0	610626	N.D.	12.237 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 10:35
Operator : AR\AJ
Sample : N2987-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 15:52:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

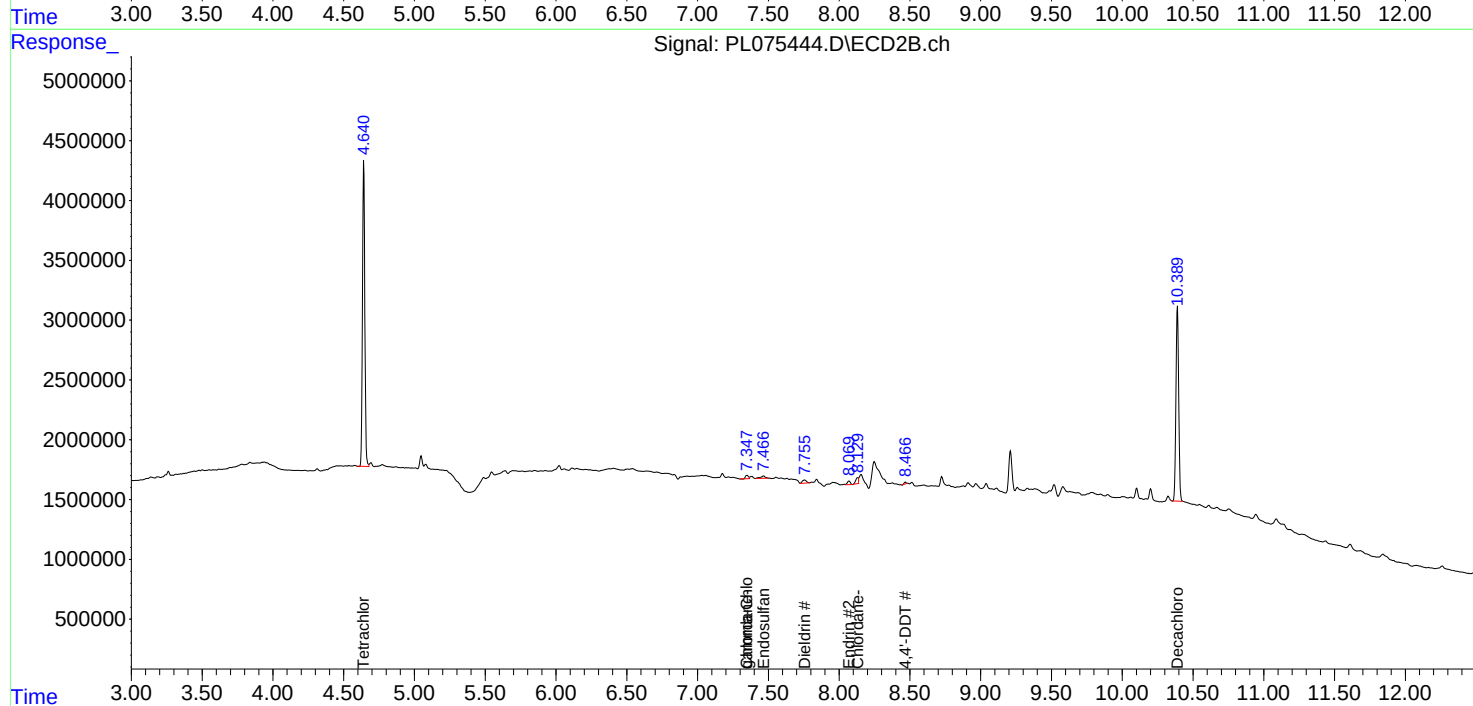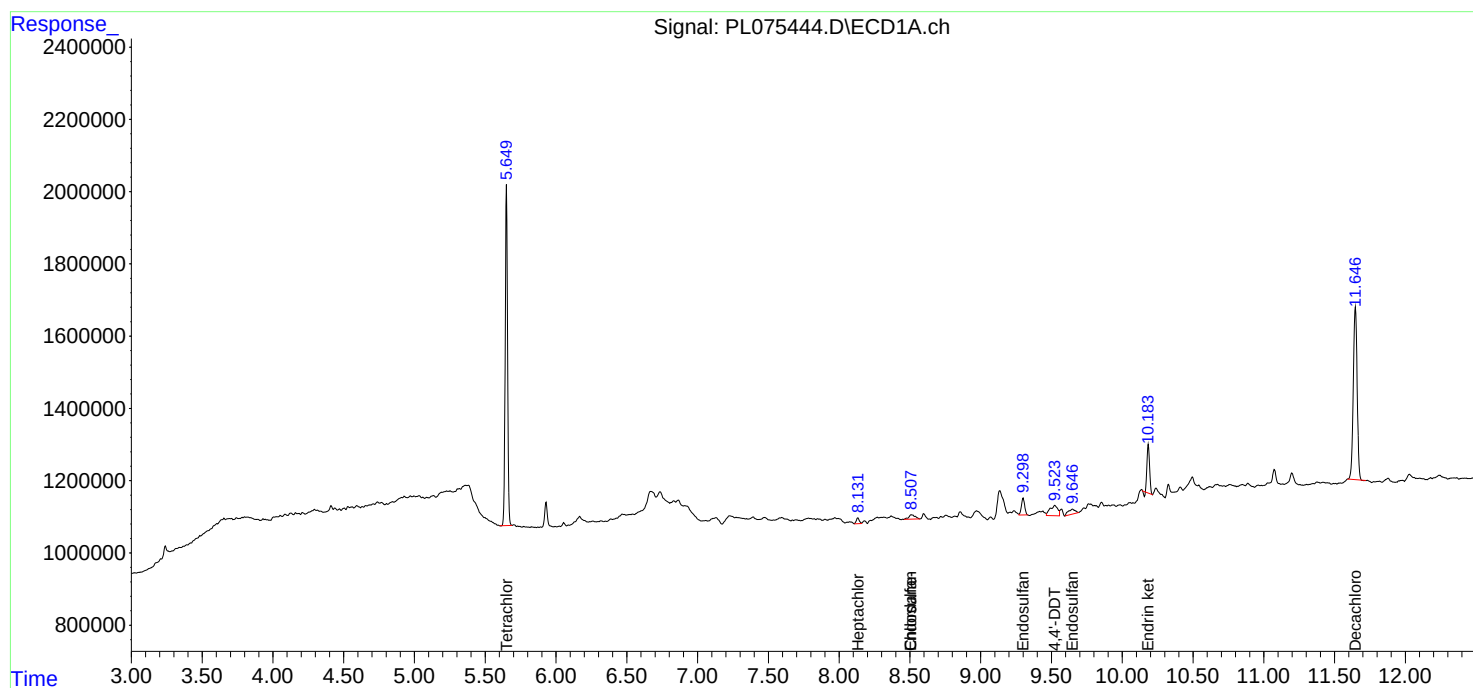


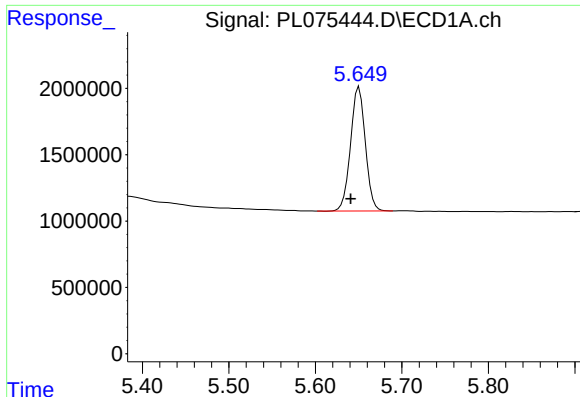

#1 Tetrachloro-m-xylene


R.T.: 5.651 min
Delta R.T.: 0.010 min
Response: 11108538
Conc: 18.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

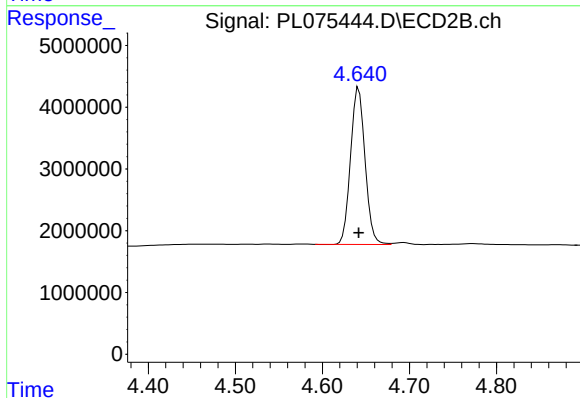


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 29405849
Conc: 18.56 ng/ml

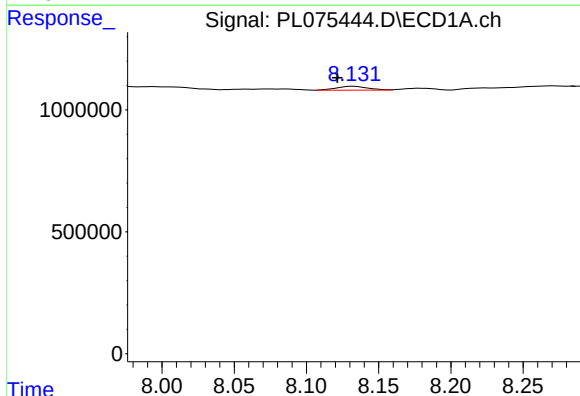


#8 Heptachlor epoxide

R.T.: 8.133 min
Delta R.T.: 0.011 min
Response: 238646
Conc: 0.35 ng/ml

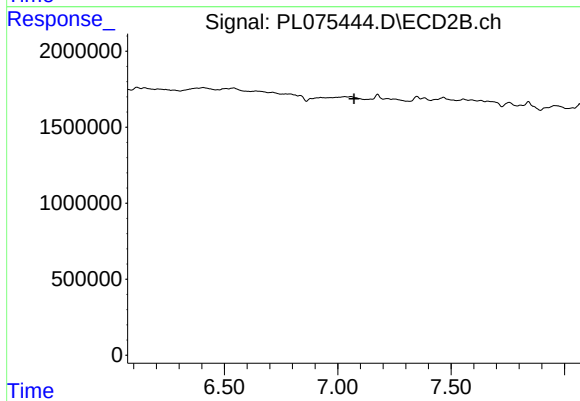

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

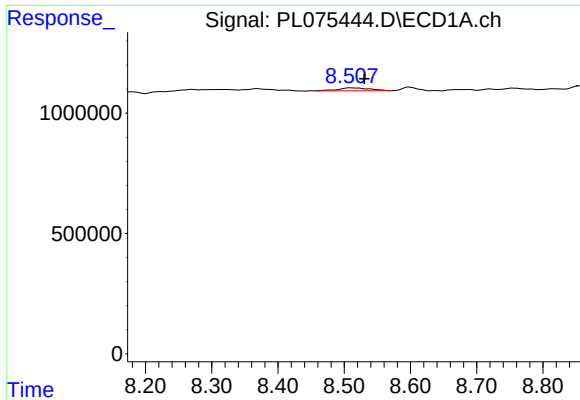

#9 Endosulfan I


R.T.: 8.509 min
Delta R.T.: -0.022 min
Response: 387841
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

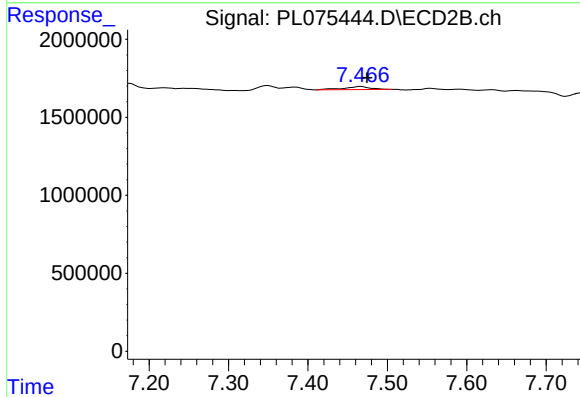


#9 Endosulfan I

R.T.: 7.467 min
Delta R.T.: -0.008 min
Response: 460279
Conc: 0.27 ng/ml

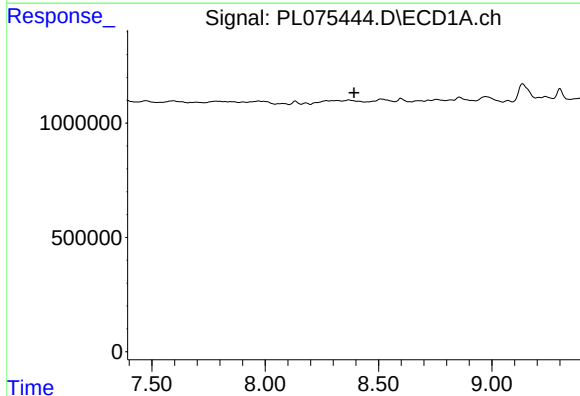


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.392 min
Response: 0
Conc: N.D.

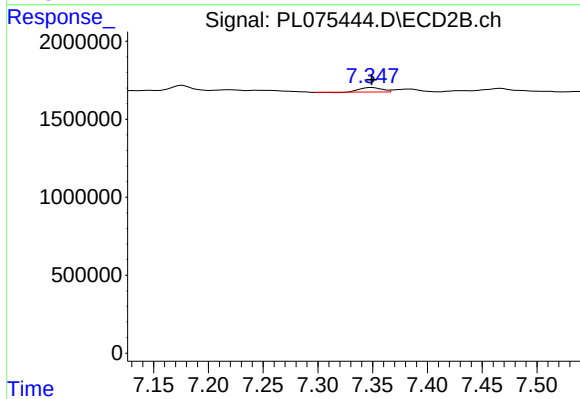

#10 gamma-Chlordane


R.T.: 7.349 min
Delta R.T.: 0.000 min
Response: 406220
Conc: 0.22 ng/ml

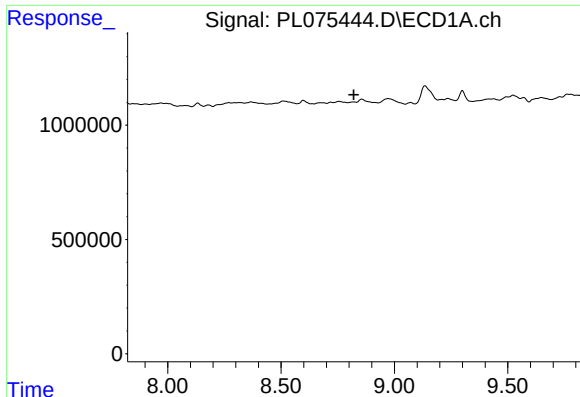

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

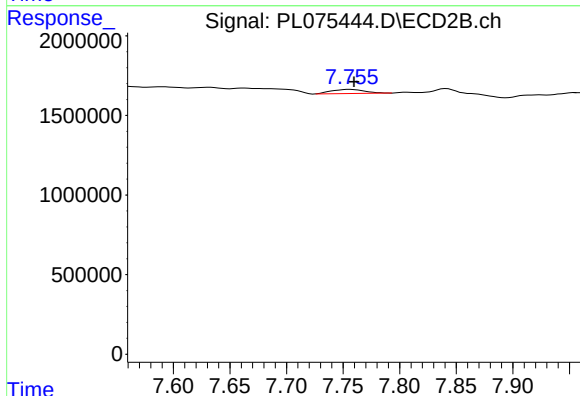


#13 Dieldrin

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 535382
Conc: 0.31 ng/ml

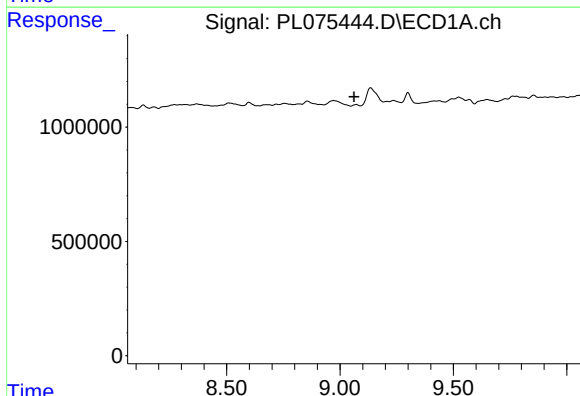


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

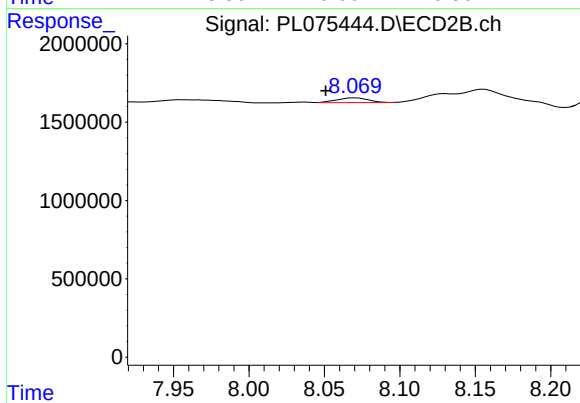

#14 Endrin


R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 436320
Conc: 0.28 ng/ml

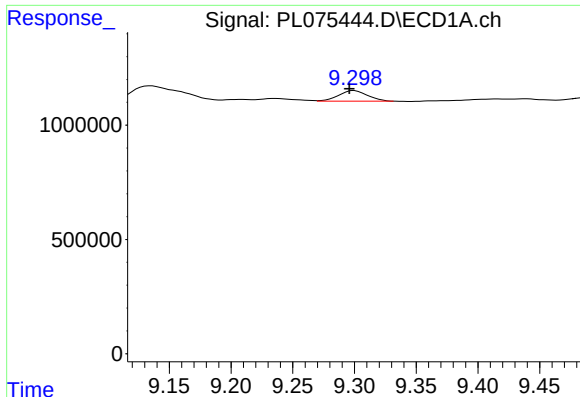

#15 Endosulfan II


R.T.: 9.300 min
Delta R.T.: 0.004 min
Response: 755643
Conc: 1.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

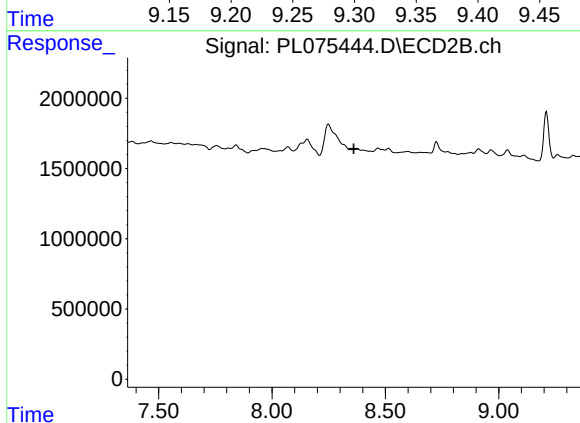


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

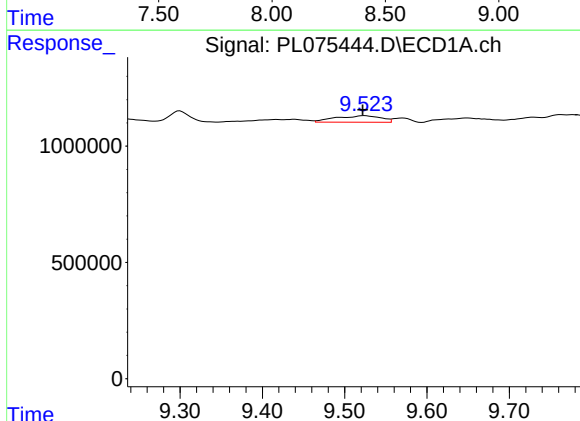


#17 4,4'-DDT

R.T.: 9.524 min
Delta R.T.: 0.002 min
Response: 1073207
Conc: 1.84 ng/ml

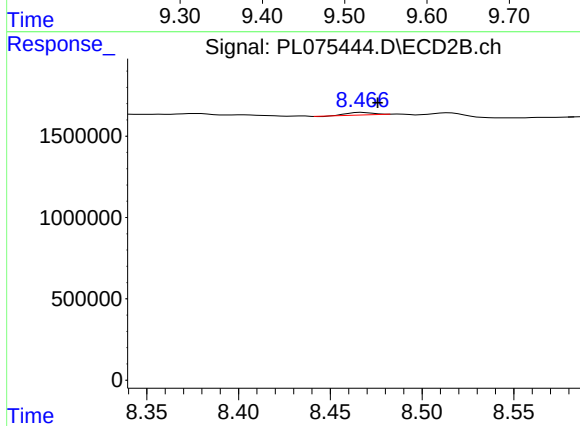

#17 4,4'-DDT


R.T.: 8.468 min
Delta R.T.: -0.008 min
Response: 138522
Conc: 0.10 ng/ml

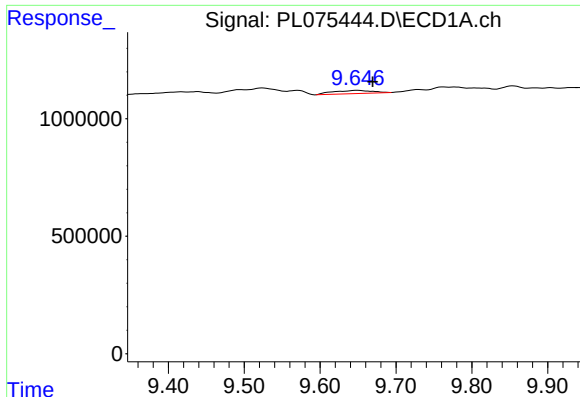

#19 Endosulfan Sulfate


R.T.: 9.649 min
Delta R.T.: -0.020 min
Response: 486628
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

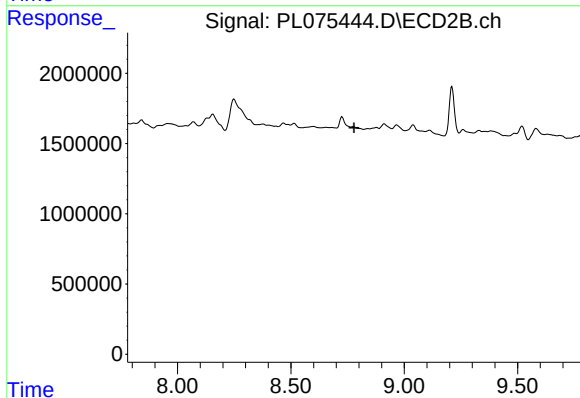


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.779 min
Response: 0
Conc: N.D.

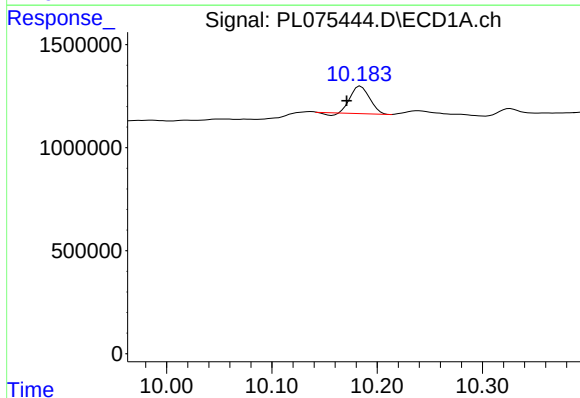


#21 Endrin ketone

R.T.: 10.184 min
Delta R.T.: 0.013 min
Response: 1657310
Conc: 2.70 ng/ml

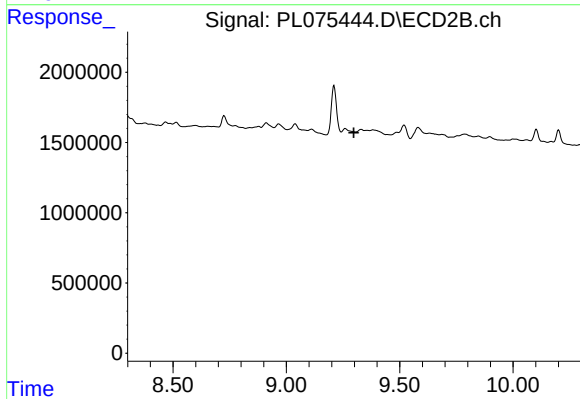

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

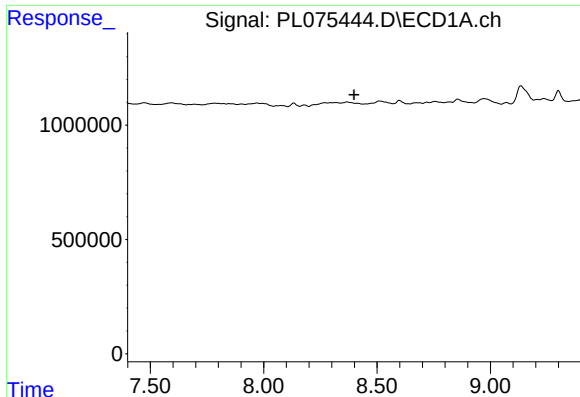

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

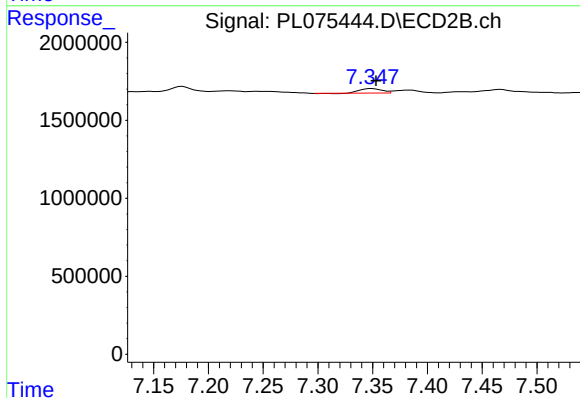


#25 Chlordane-3

R.T.: 7.349 min
Delta R.T.: -0.004 min
Response: 406220
Conc: 2.30 ng/ml

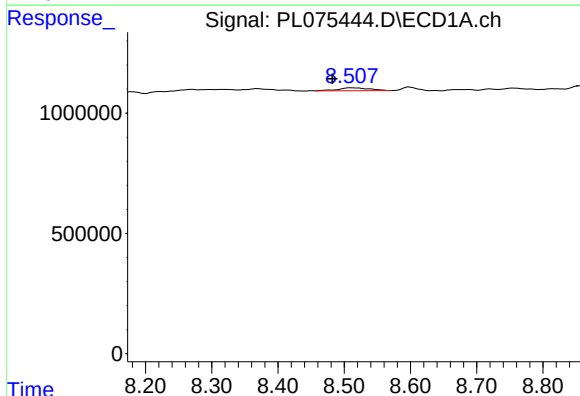


#26 Chlordane-4

R.T.: 8.509 min
Delta R.T.: 0.027 min
Response: 387841
Conc: 3.42 ng/ml

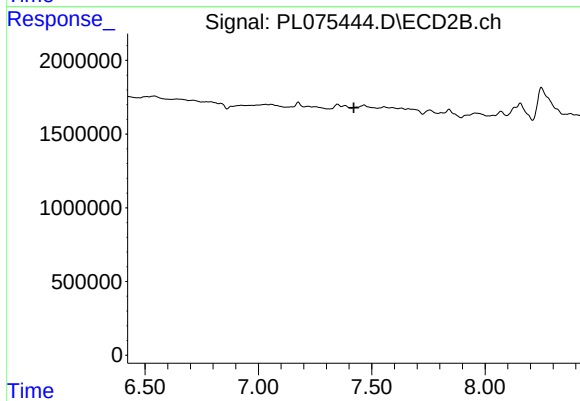

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

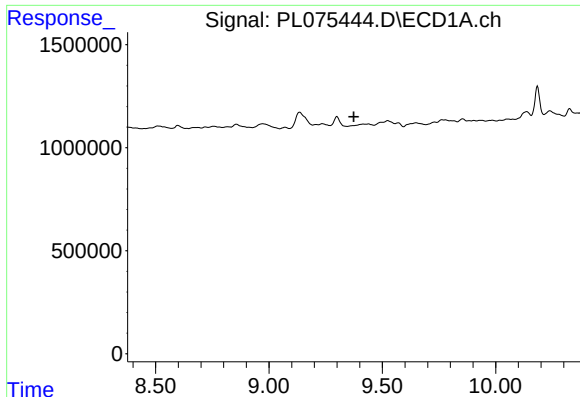

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

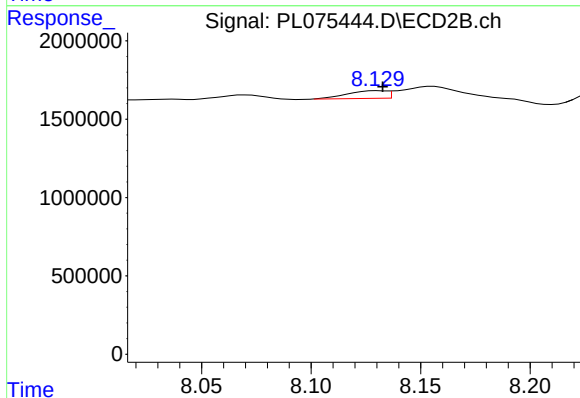


#27 Chlordane-5

R.T.: 8.131 min
Delta R.T.: -0.002 min
Response: 610626
Conc: 12.24 ng/ml

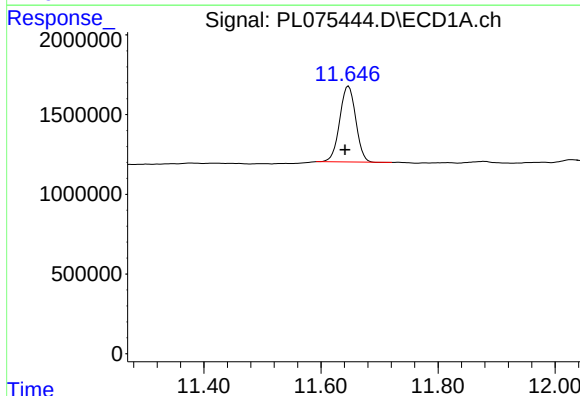

#28 Decachlorobiphenyl

R.T.: 11.647 min
Delta R.T.: 0.006 min
Response: 9042943
Conc: 16.87 ng/ml

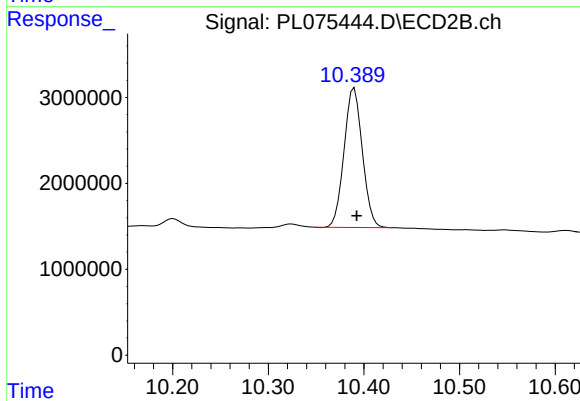

#28 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: -0.002 min
Response: 21651596
Conc: 15.78 ng/ml