

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 11:09
 Operator : AR\AJ
 Sample : N2987-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 15:52:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.641	11486260	30720728	19.543	19.393
28)	SA Decachlor...	11.640	10.387	7087111	17175546	13.218	12.516
Target Compounds							
5)	MB Aldrin	0.000	6.493	0	676437	N.D.	0.351 #
7)	B delta-BHC	0.000	6.412	0	319687	N.D.	0.149 #
11)	B alpha-Chl...	0.000	7.393f	0	246146	N.D.	0.135 #
13)	MA Dieldrin	8.820	7.757	189419	837298	0.299	0.483 #
14)	MA Endrin	0.000	8.068f	0	208709	N.D.	0.134 #
15)	B Endosulfa...	9.306	0.000	254695	0	0.451	N.D. #
17)	MA 4,4'-DDT	0.000	8.465	0	251124	N.D.	0.176 #
19)	B Endosulfa...	9.673	8.772	273691	79077	0.492	0.053 #
21)	B Endrin ke...	10.187f	0.000	123603	0	0.201	N.D. #
22)	Mirex	0.000	9.514f	0	12396	N.D.	0.010 #
26)	Chlordane-4	0.000	7.393f	0	246146	N.D.	1.303 #
27)	Chlordane-5	0.000	8.141	0	654979	N.D.	13.126 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 11:09
Operator : AR\AJ
Sample : N2987-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 15:52:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

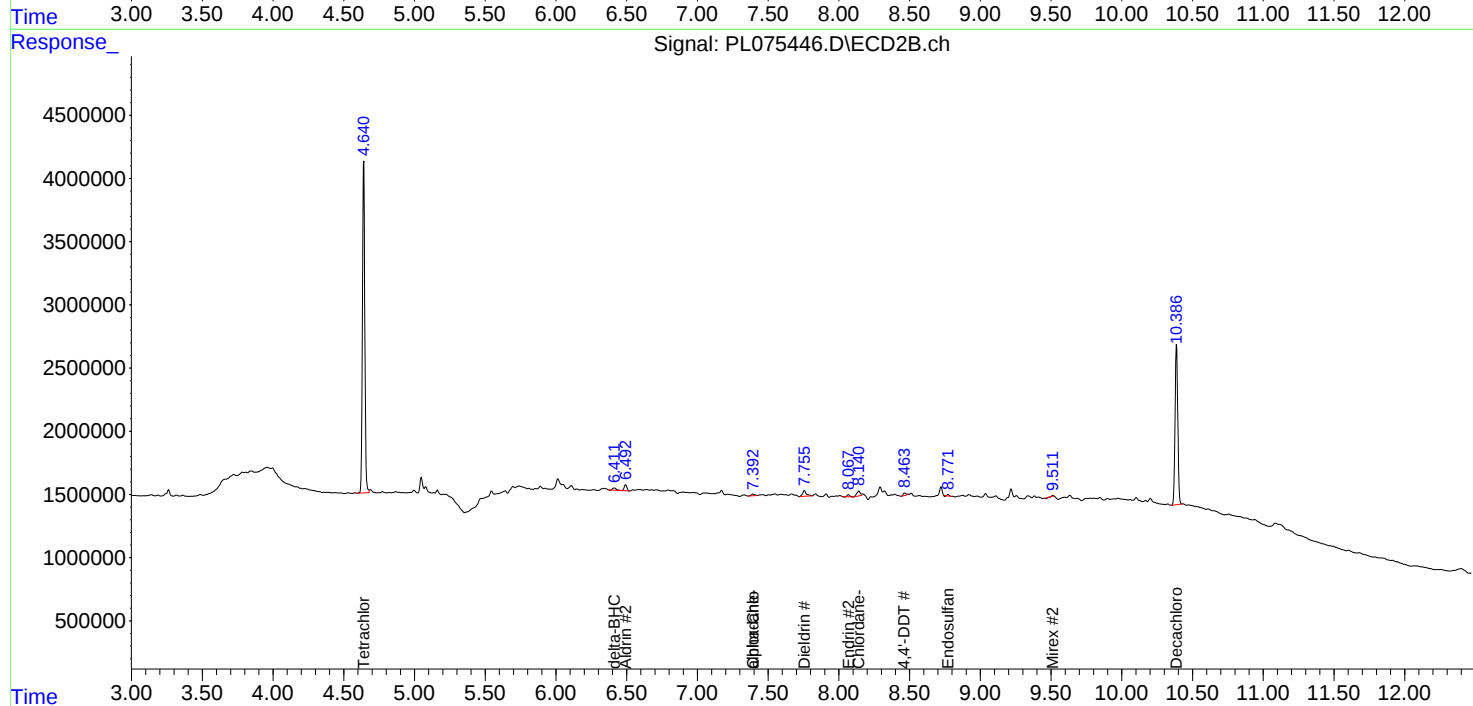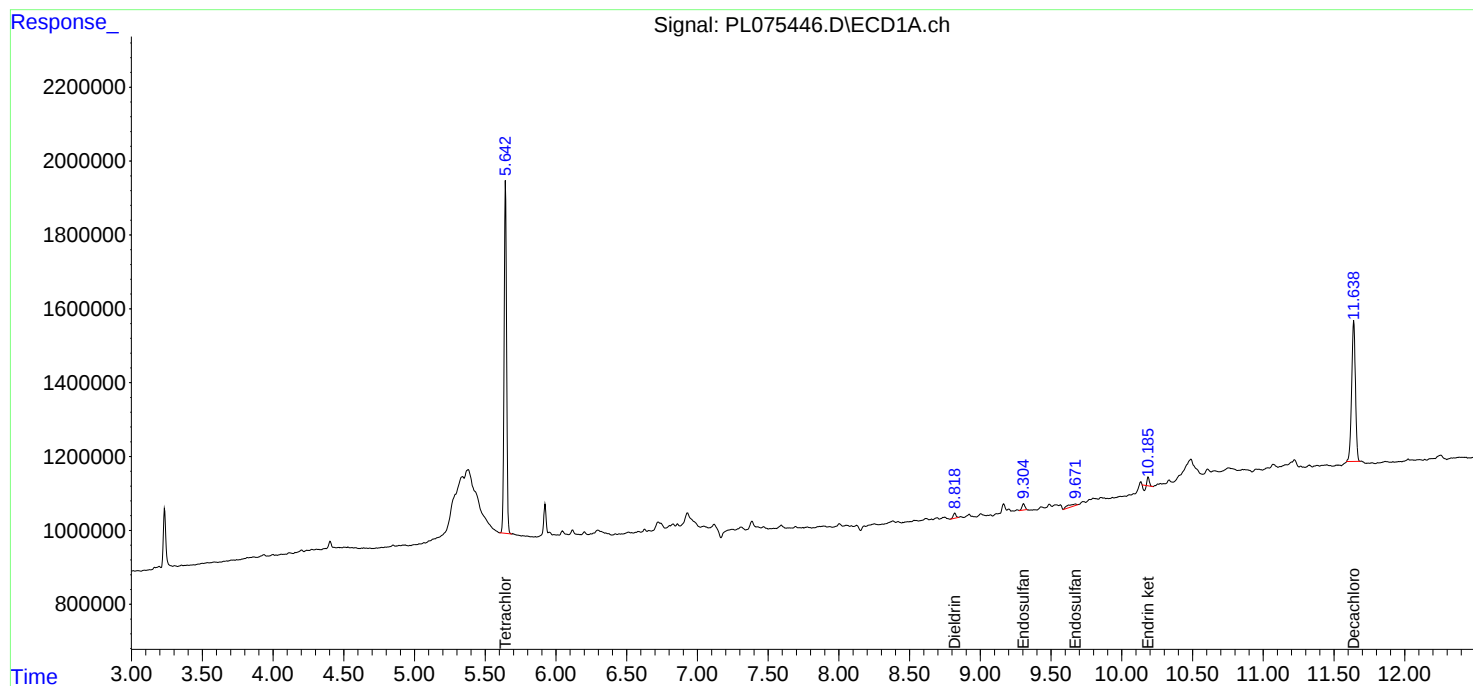


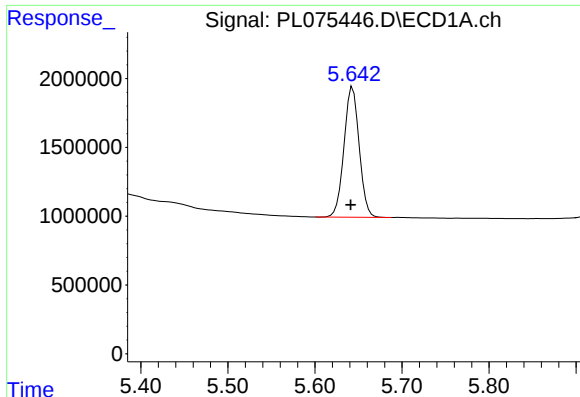

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 11486260
Conc: 19.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

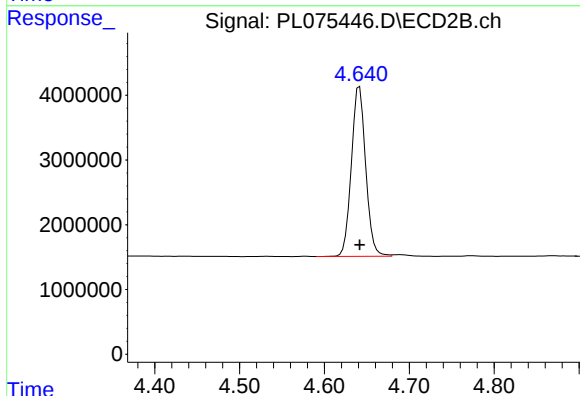


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 30720728
Conc: 19.39 ng/ml

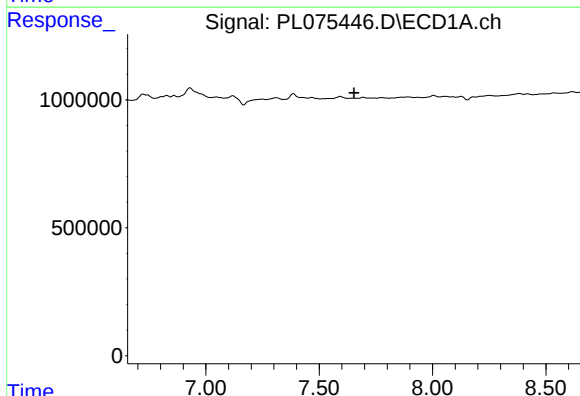


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

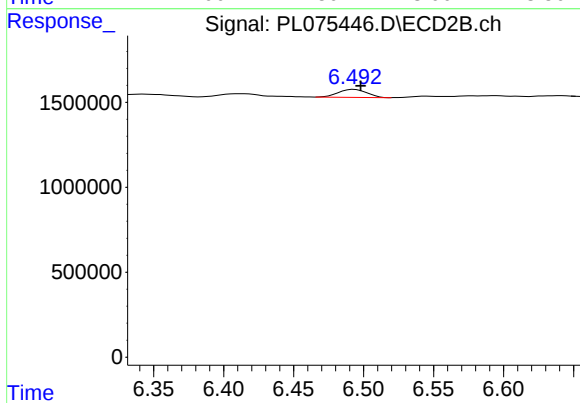

#5 Aldrin


R.T.: 6.493 min
Delta R.T.: -0.005 min
Response: 676437
Conc: 0.35 ng/ml

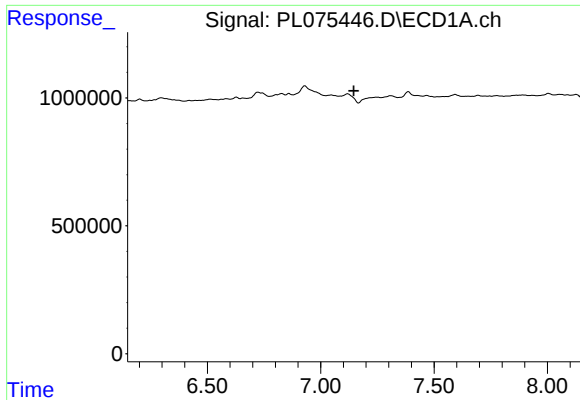

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.146 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

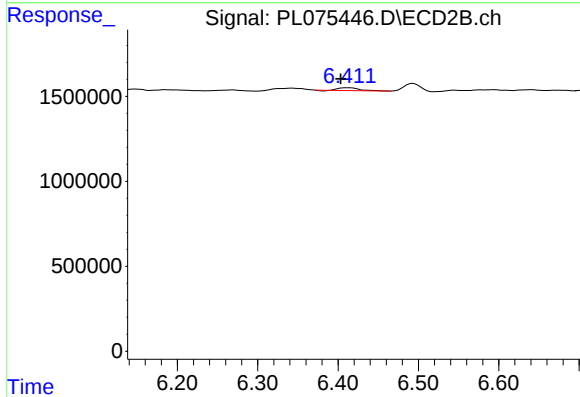


#7 delta-BHC

R.T.: 6.412 min
Delta R.T.: 0.009 min
Response: 319687
Conc: 0.15 ng/ml

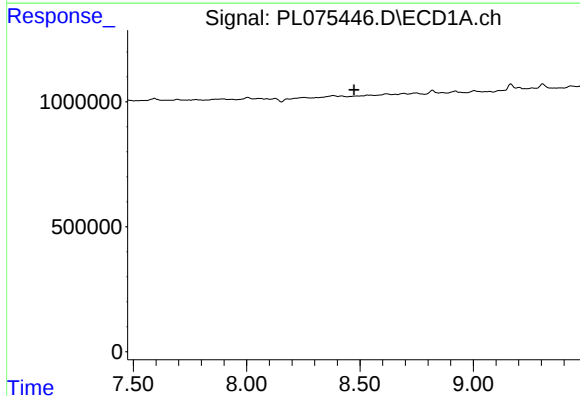


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

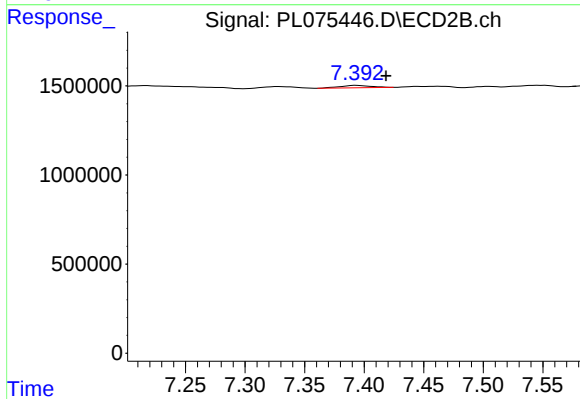

#11 alpha-Chlordane


R.T.: 7.393 min
Delta R.T.: -0.025 min
Response: 246146
Conc: 0.13 ng/ml

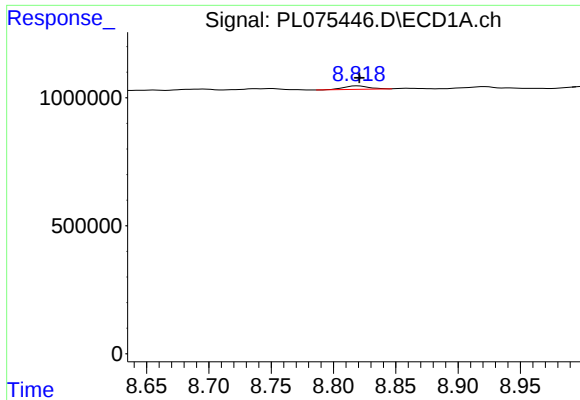

#13 Dieldrin


R.T.: 8.820 min
Delta R.T.: 0.000 min
Response: 189419
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

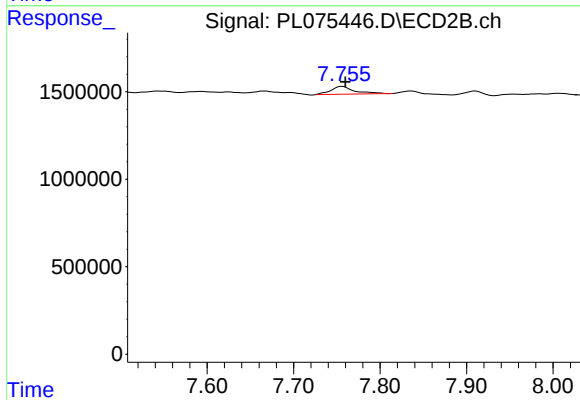


#13 Dieldrin

R.T.: 7.757 min
Delta R.T.: -0.003 min
Response: 837298
Conc: 0.48 ng/ml

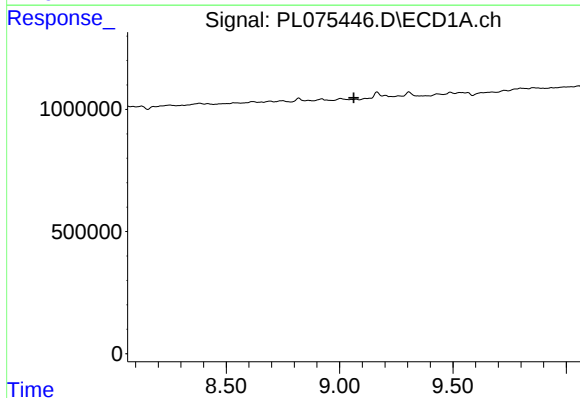


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.062 min
Response: 0
Conc: N.D.

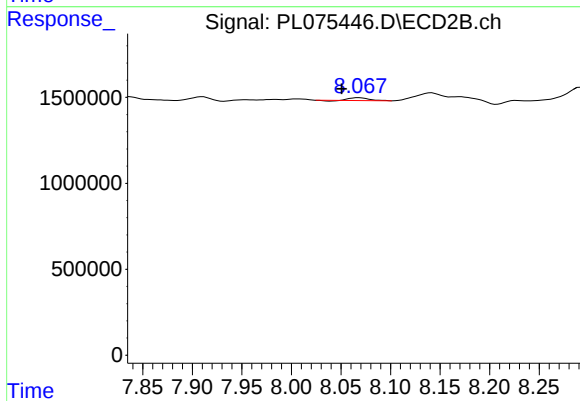

#14 Endrin


R.T.: 8.068 min
Delta R.T.: 0.017 min
Response: 208709
Conc: 0.13 ng/ml

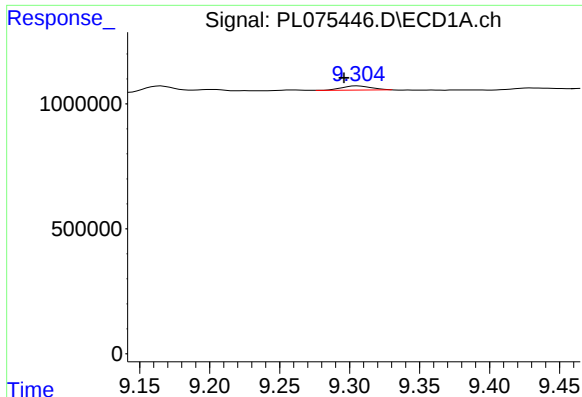

#15 Endosulfan II


R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 254695
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

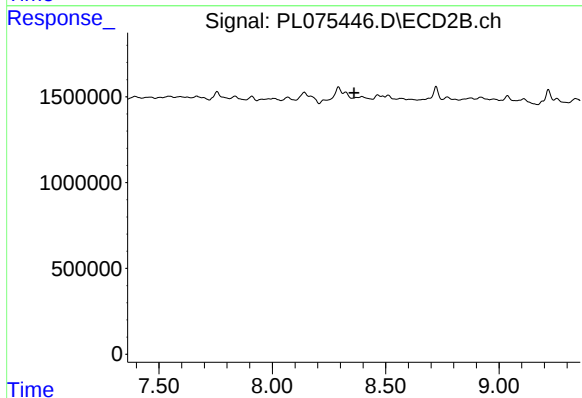


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

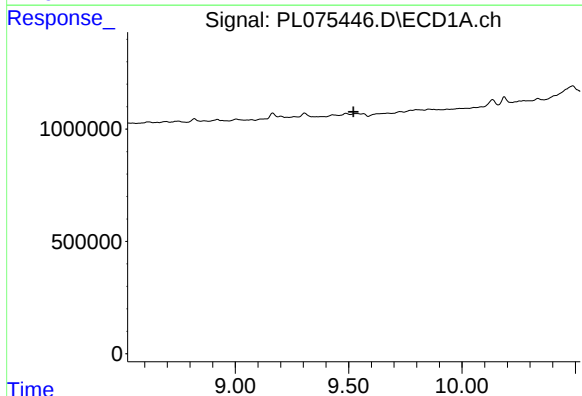


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

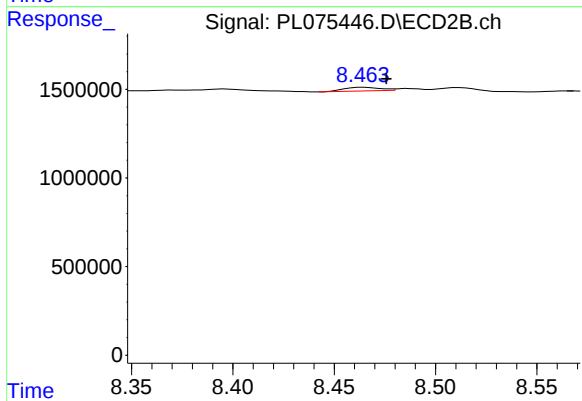

#17 4,4'-DDT


R.T.: 8.465 min
Delta R.T.: -0.011 min
Response: 251124
Conc: 0.18 ng/ml

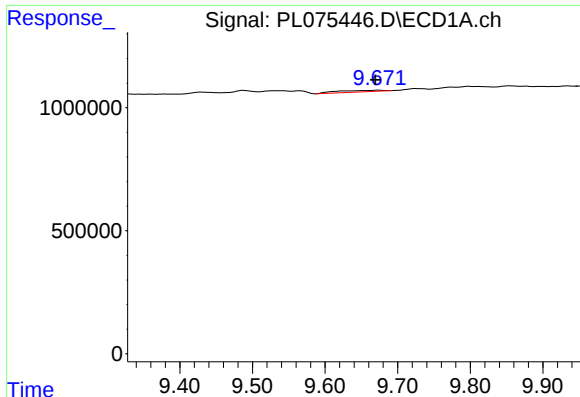

#19 Endosulfan Sulfate


R.T.: 9.673 min
Delta R.T.: 0.004 min
Response: 273691
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

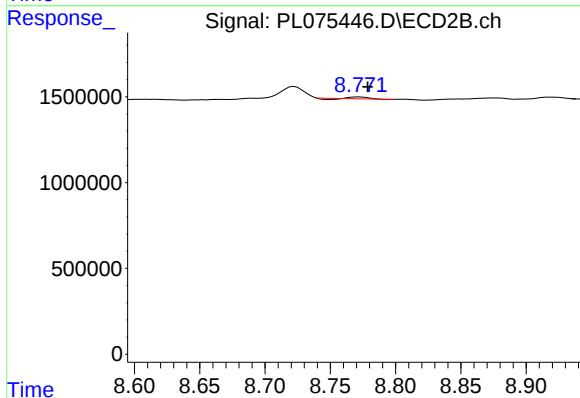


#19 Endosulfan Sulfate

R.T.: 8.772 min
Delta R.T.: -0.006 min
Response: 79077
Conc: 0.05 ng/ml

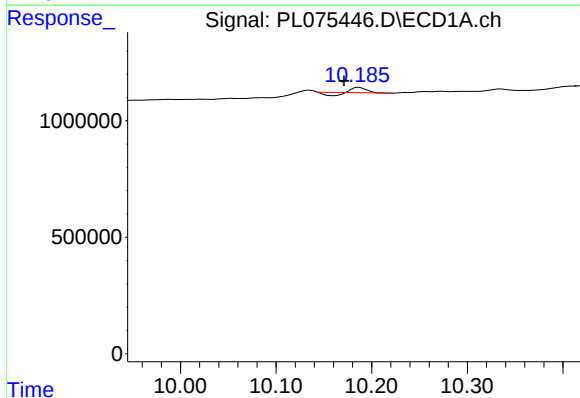


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 123603
Conc: 0.20 ng/ml

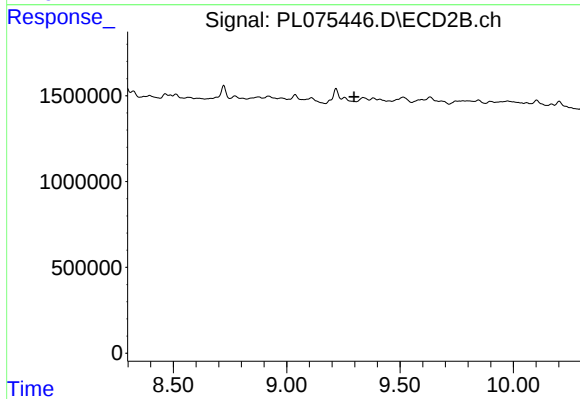

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.298 min
Response: 0
Conc: N.D.

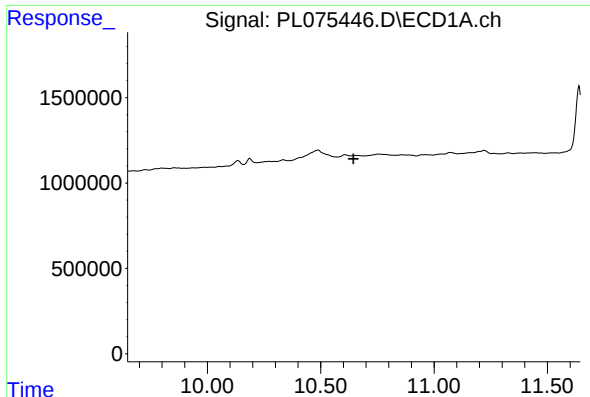

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 10.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

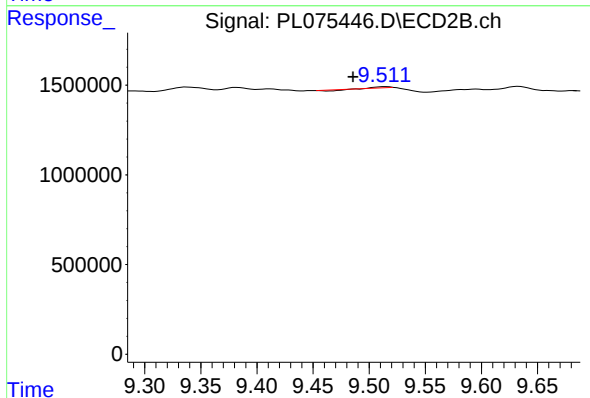


#22 Mirex

R.T.: 9.514 min
Delta R.T.: 0.029 min
Response: 12396
Conc: 0.01 ng/ml

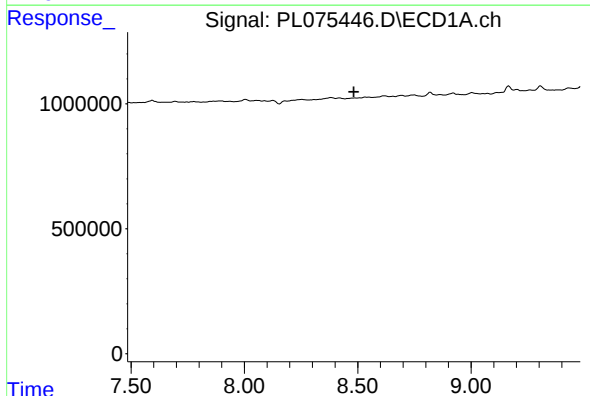


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 8.482 min
Response: 0
Conc: N.D.

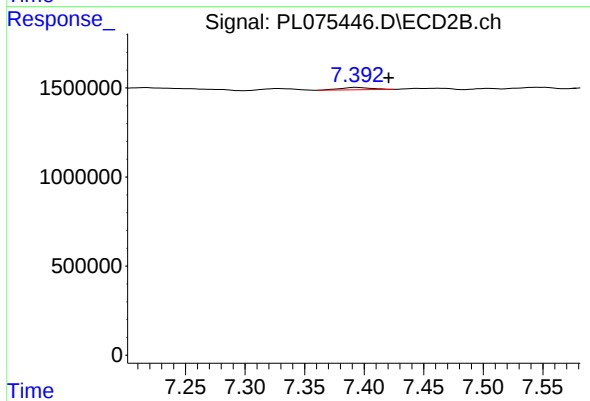

#26 Chlordane-4


R.T.: 7.393 min
Delta R.T.: -0.027 min
Response: 246146
Conc: 1.30 ng/ml

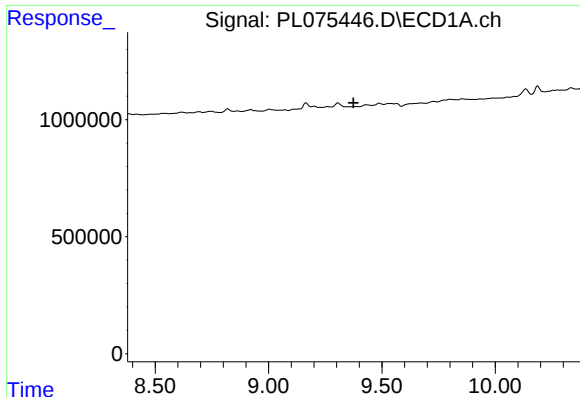

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

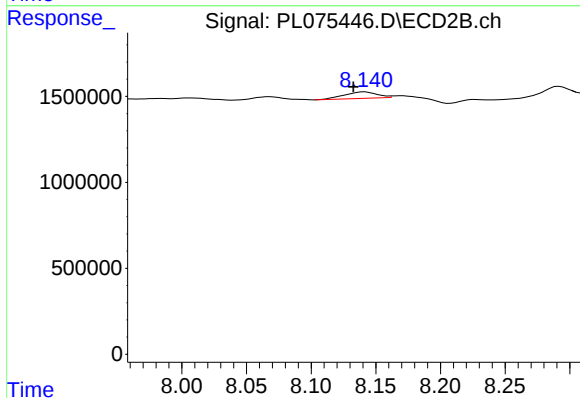


#27 Chlordane-5

R.T.: 8.141 min
Delta R.T.: 0.009 min
Response: 654979
Conc: 13.13 ng/ml

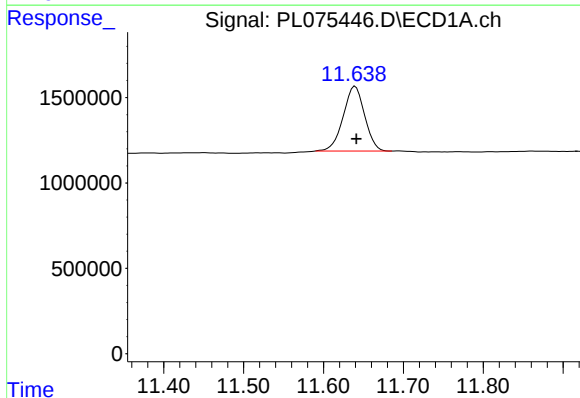

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.001 min
Response: 7087111
Conc: 13.22 ng/ml

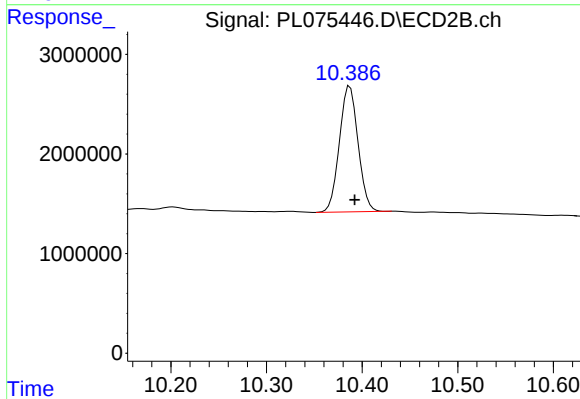

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.005 min
Response: 17175546
Conc: 12.52 ng/ml