

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 12:31
 Operator : AR\AJ
 Sample : N3099-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 15:53:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.641	8662989	23607527	14.740	14.902
28)	SA Decachlor...	11.638	10.386	6126666	15304763	11.426	11.153
Target Compounds							
4)	MA Heptachlor	0.000	6.202f	0	300576	N.D.	0.147 #
7)	B delta-BHC	0.000	6.410	0	214034	N.D.	0.100 #
9)	A Endosulfan I	0.000	7.500f	0	148881	N.D.	0.088 #
10)	B gamma-Chl...	8.411f	7.331f	358948	224586	0.532	0.122 #
13)	MA Dieldrin	0.000	7.762	0	481856	N.D.	0.278 #
14)	MA Endrin	0.000	8.069f	0	157532	N.D.	0.101 #
15)	B Endosulfa...	9.307	0.000	205701	0	0.364	N.D. #
17)	MA 4,4'-DDT	0.000	8.465	0	189463	N.D.	0.132 #
21)	B Endrin ke...	10.187f	0.000	378127	0	0.616	N.D. #
25)	Chlordane-3	8.411	7.331f	358948	224586	3.857	1.272 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 12:31
Operator : AR\AJ
Sample : N3099-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 15:53:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

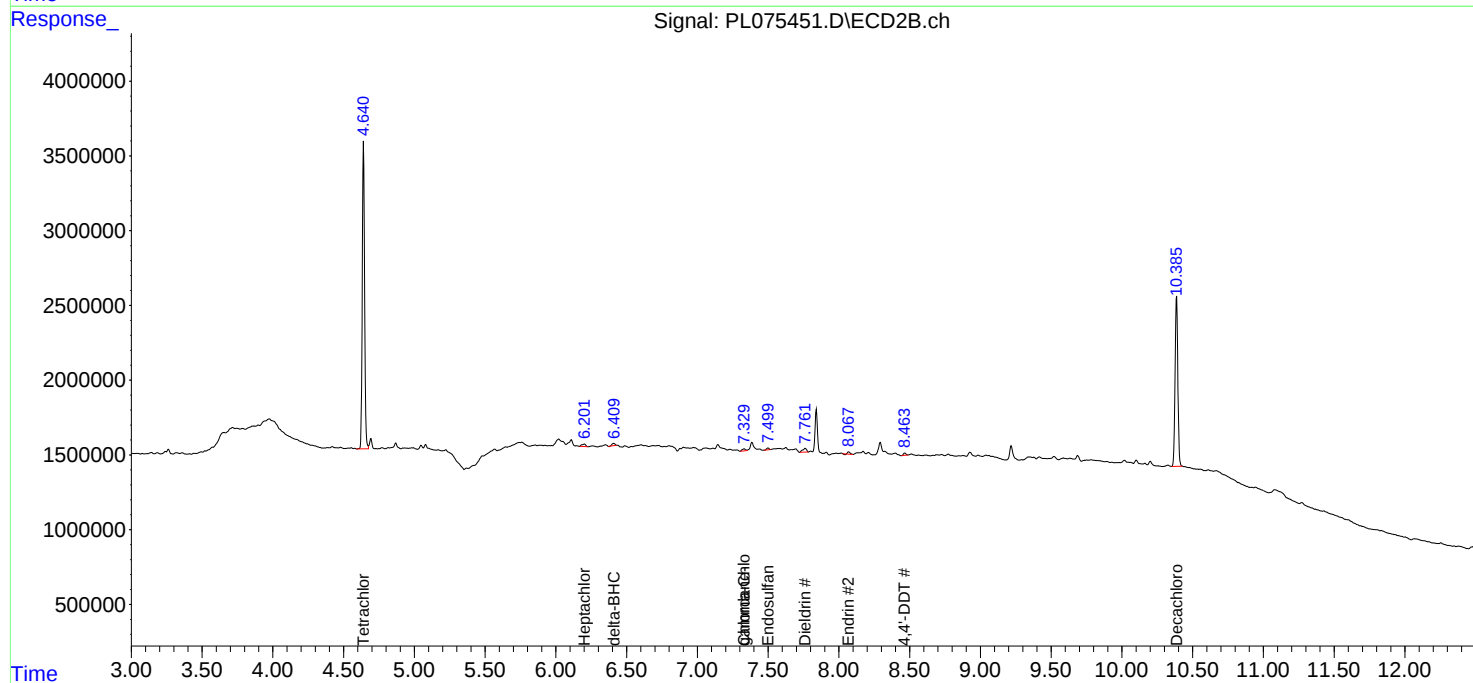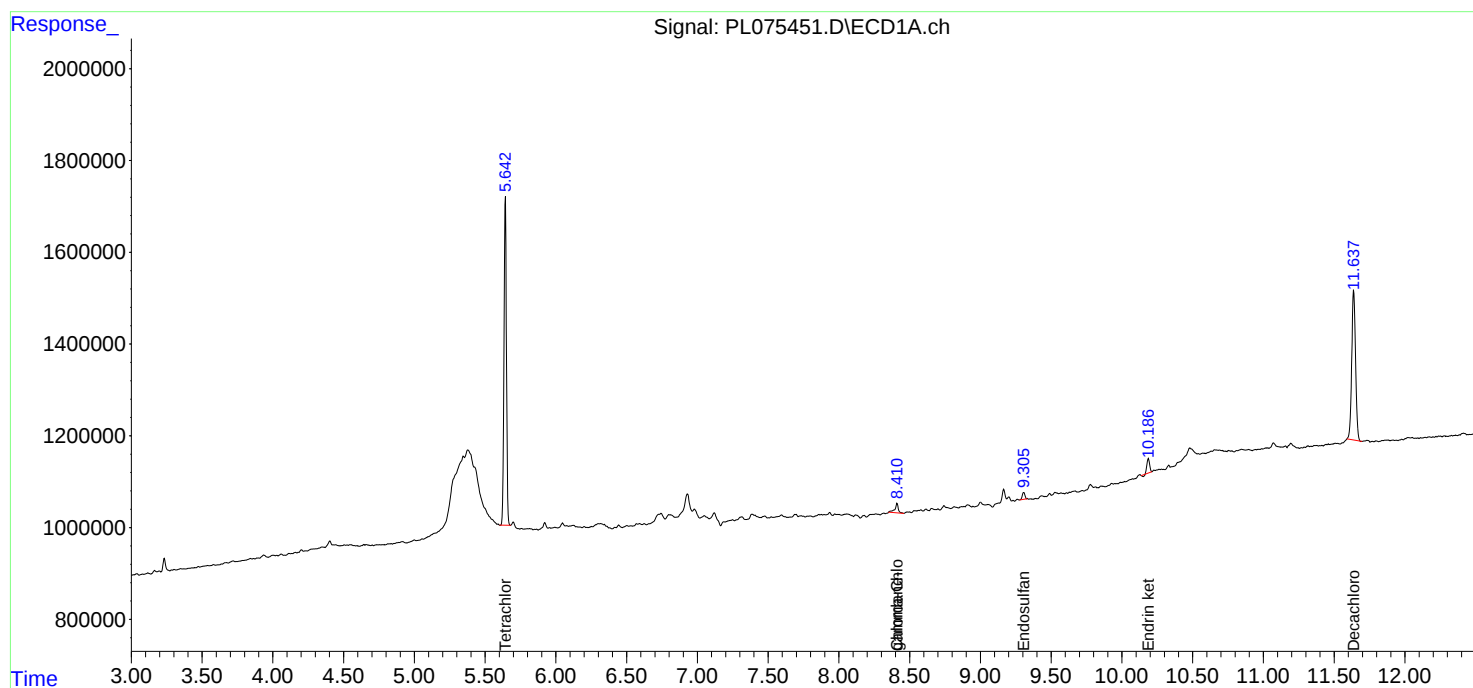


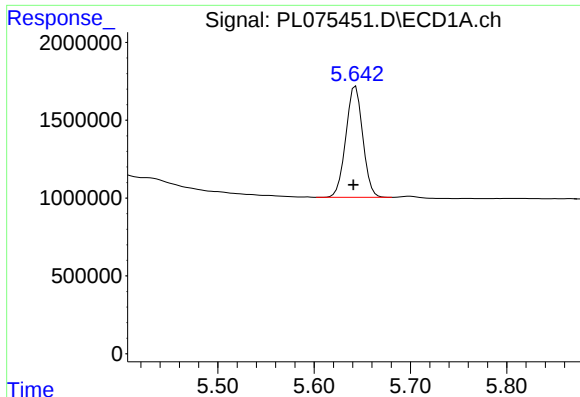

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 8662989
Conc: 14.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

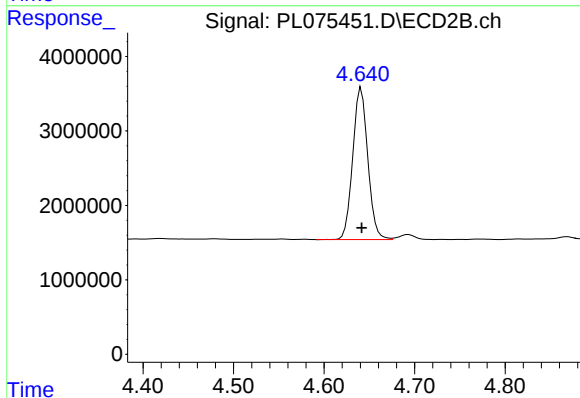


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 23607527
Conc: 14.90 ng/ml

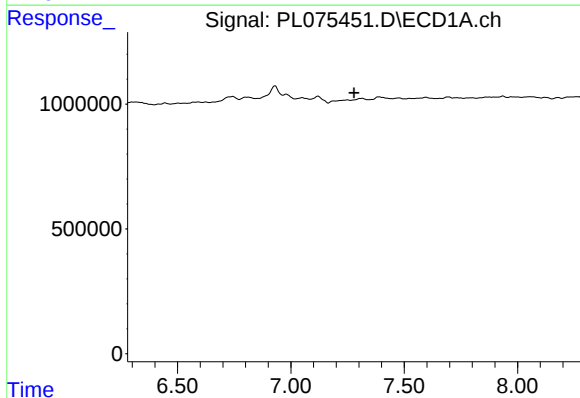


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.279 min
Response: 0
Conc: N.D.

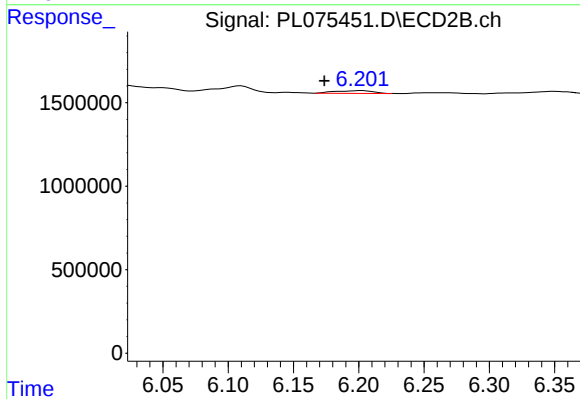

#4 Heptachlor

R.T.: 6.202 min
Delta R.T.: 0.028 min
Response: 300576
Conc: 0.15 ng/ml

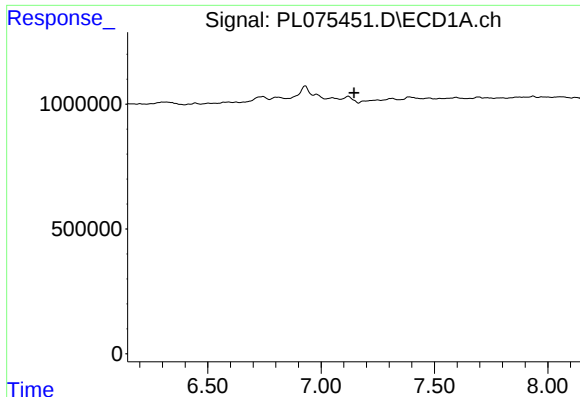

#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#7 delta-BHC


R.T.: 6.410 min
Delta R.T.: 0.006 min
Response: 214034
Conc: 0.10 ng/ml

#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

#9 Endosulfan I


R.T.: 7.500 min
Delta R.T.: 0.025 min
Response: 148881
Conc: 0.09 ng/ml

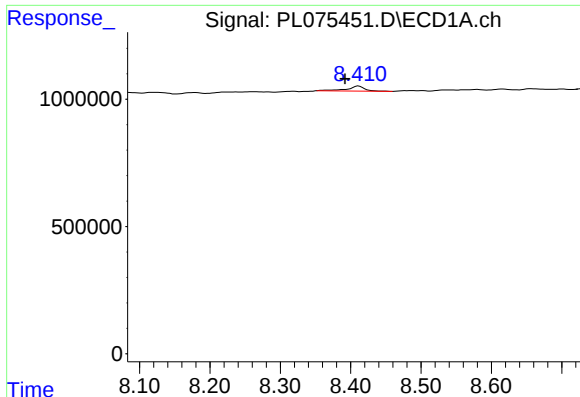

#10 gamma-Chlordane


R.T.: 8.411 min
Delta R.T.: 0.019 min
Response: 358948
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

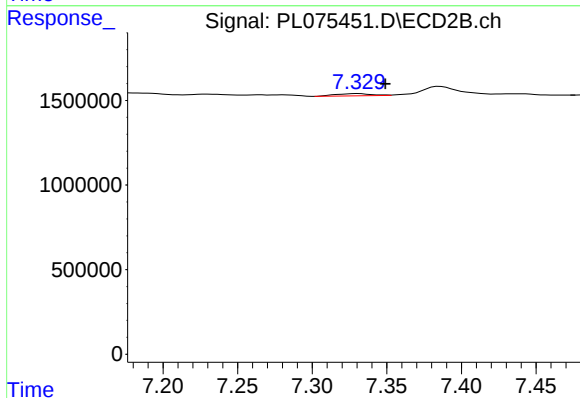


#10 gamma-Chlordane

R.T.: 7.331 min
Delta R.T.: -0.018 min
Response: 224586
Conc: 0.12 ng/ml

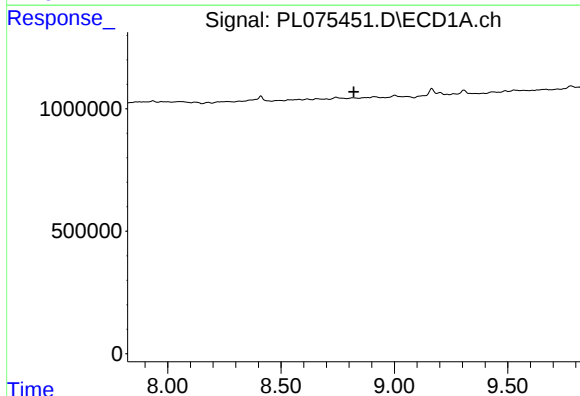


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

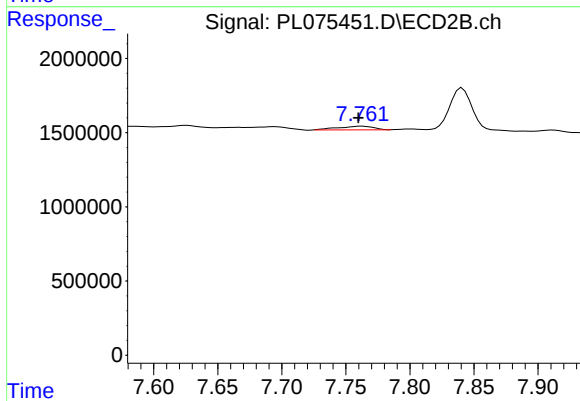

#13 Dieldrin


R.T.: 7.762 min
Delta R.T.: 0.003 min
Response: 481856
Conc: 0.28 ng/ml

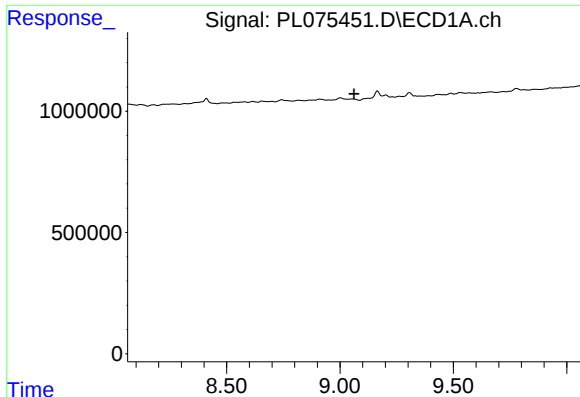

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

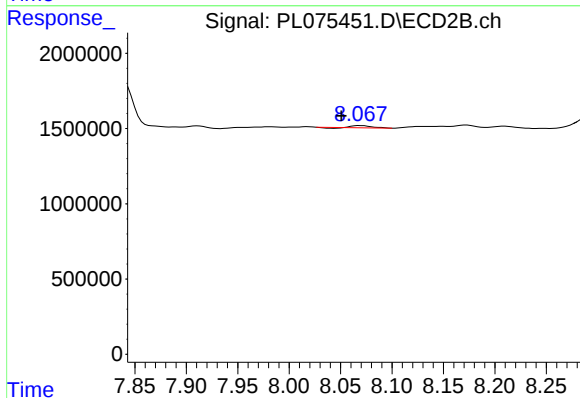


#14 Endrin

R.T.: 8.069 min
Delta R.T.: 0.018 min
Response: 157532
Conc: 0.10 ng/ml

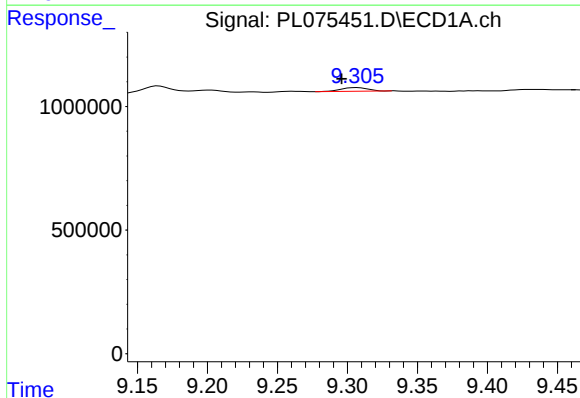


#15 Endosulfan II

R.T.: 9.307 min
Delta R.T.: 0.011 min
Response: 205701
Conc: 0.36 ng/ml

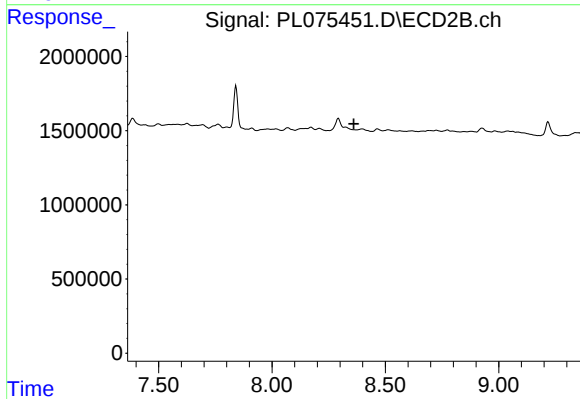

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

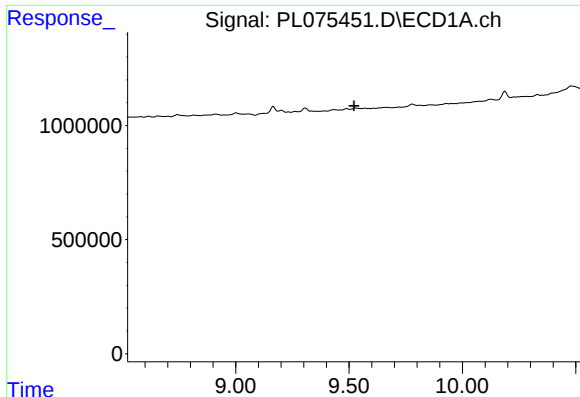

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

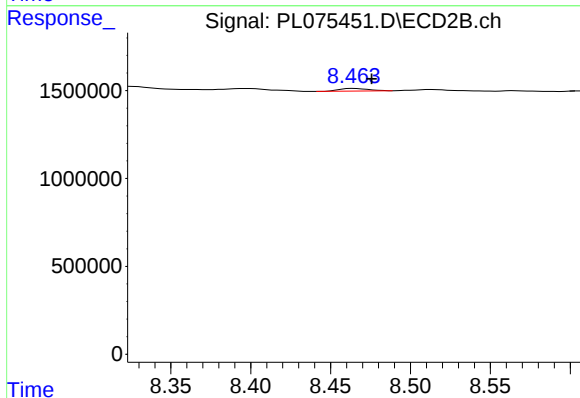


#17 4,4'-DDT

R.T.: 8.465 min
Delta R.T.: -0.011 min
Response: 189463
Conc: 0.13 ng/ml

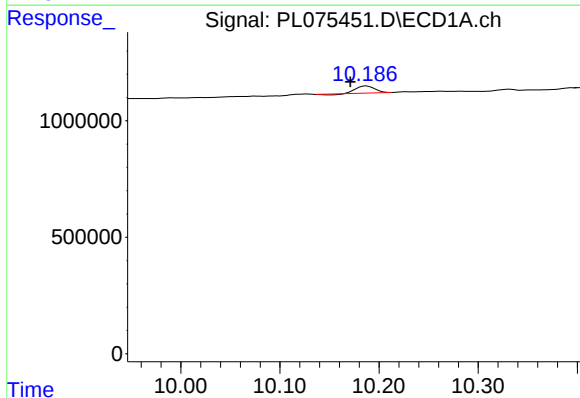


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 378127
Conc: 0.62 ng/ml

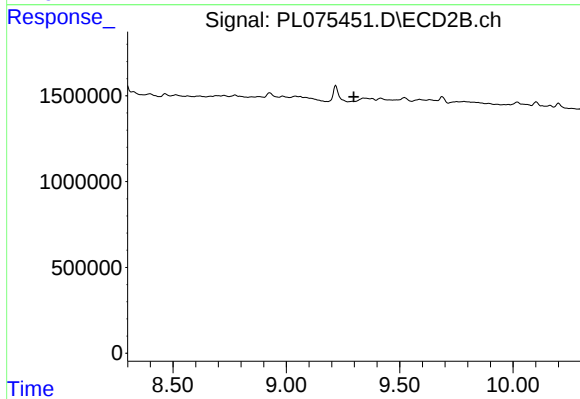

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.298 min
Response: 0
Conc: N.D.

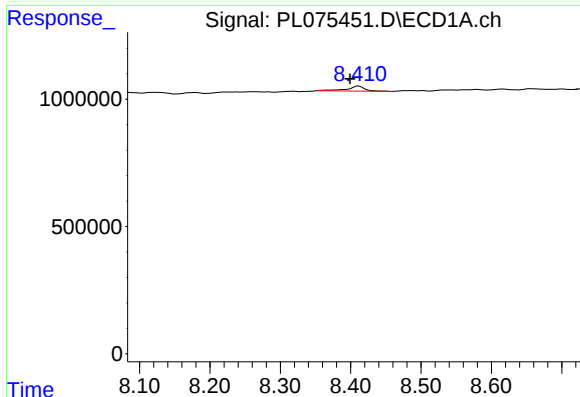

#25 Chlordane-3


R.T.: 8.411 min
Delta R.T.: 0.012 min
Response: 358948
Conc: 3.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

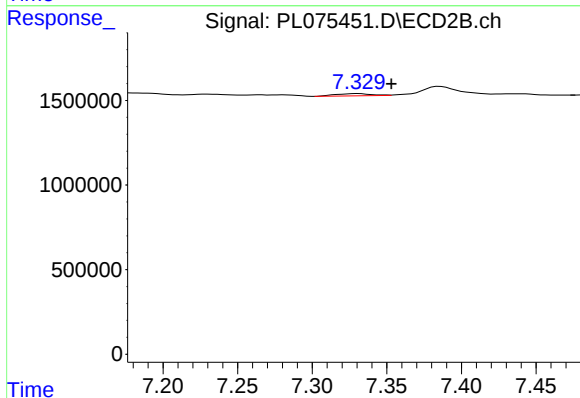


#25 Chlordane-3

R.T.: 7.331 min
Delta R.T.: -0.022 min
Response: 224586
Conc: 1.27 ng/ml

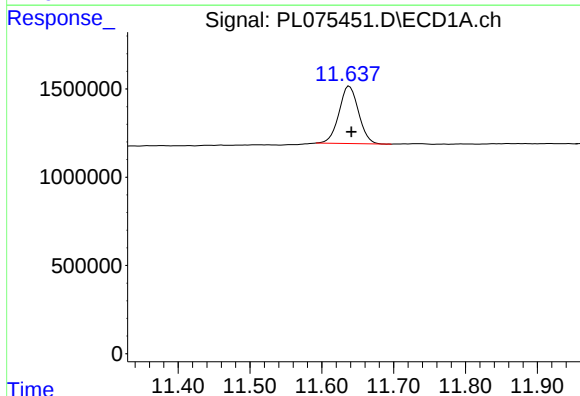

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: -0.003 min
Response: 612666
Conc: 11.43 ng/ml

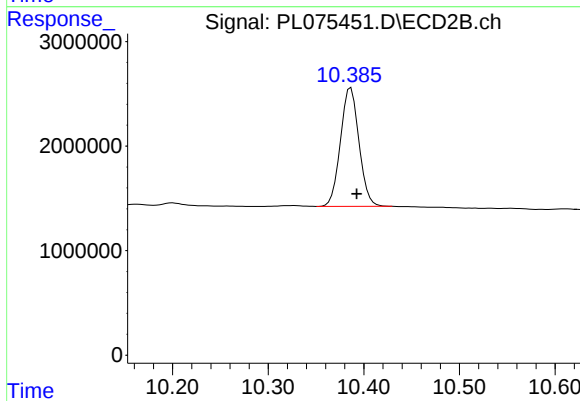

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: -0.006 min
Response: 15304763
Conc: 11.15 ng/ml