

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 14:11
 Operator : AR\AJ
 Sample : N2987-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:37:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.641	6537888	18007217	11.124	11.367
28)	SA Decachlor...	11.640	10.386	5990276	14881455	11.172	10.844
Target Compounds							
7)	B delta-BHC	0.000	6.411	0	321634	N.D.	0.150 #
11)	B alpha-Chl...	0.000	7.394f	0	248791	N.D.	0.136 #
14)	MA Endrin	0.000	8.066	0	317701	N.D.	0.204 #
15)	B Endosulfa...	9.305	0.000	133847	0	0.237	N.D. #
16)	A 4,4'-DDD	9.204	0.000	316484	0	0.640	N.D. #
17)	MA 4,4'-DDT	0.000	8.463	0	662473	N.D.	0.463 #
19)	B Endosulfa...	0.000	8.775	0	518647	N.D.	0.347 #
21)	B Endrin ke...	10.187f	0.000	338036	0	0.551	N.D. #
26)	Chlordane-4	0.000	7.394f	0	248791	N.D.	1.317 #
27)	Chlordane-5	0.000	8.127	0	762818	N.D.	15.287 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 14:11
Operator : AR\AJ
Sample : N2987-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:37:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

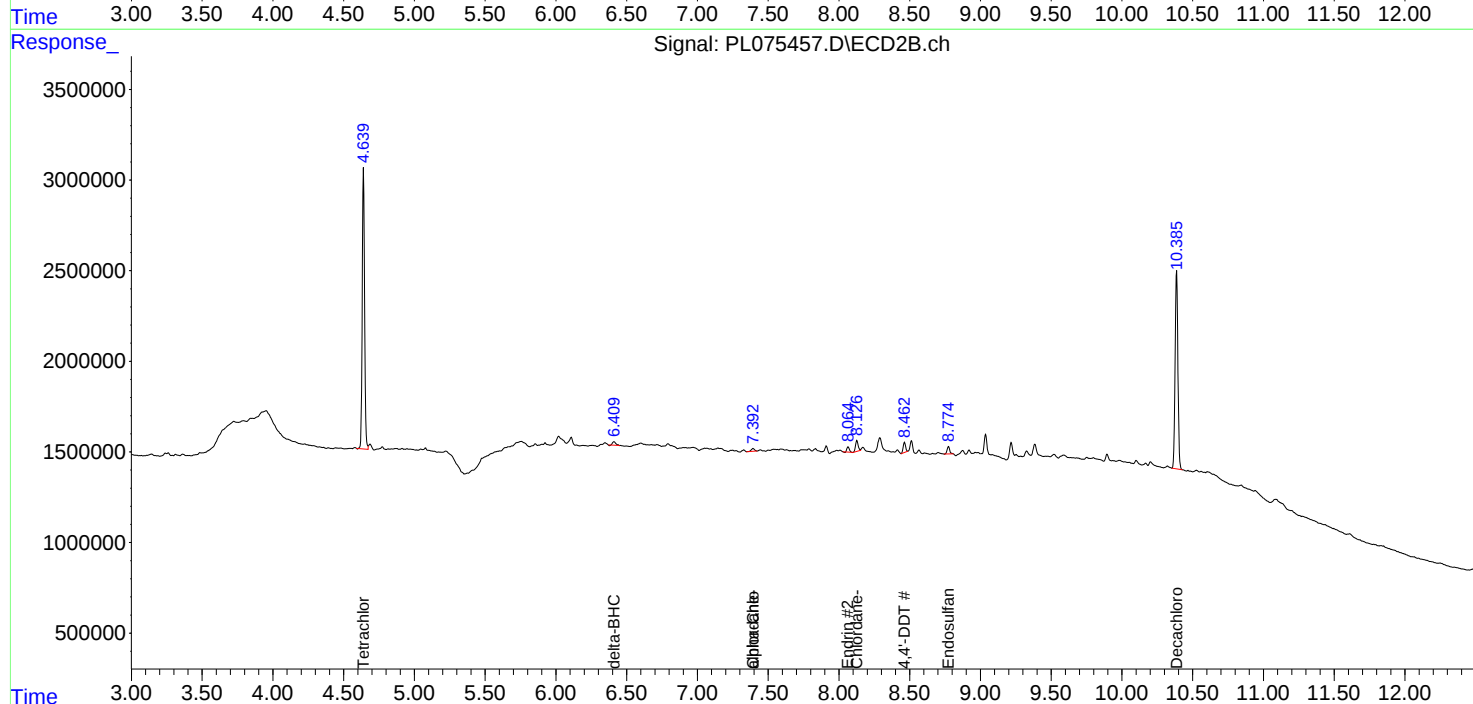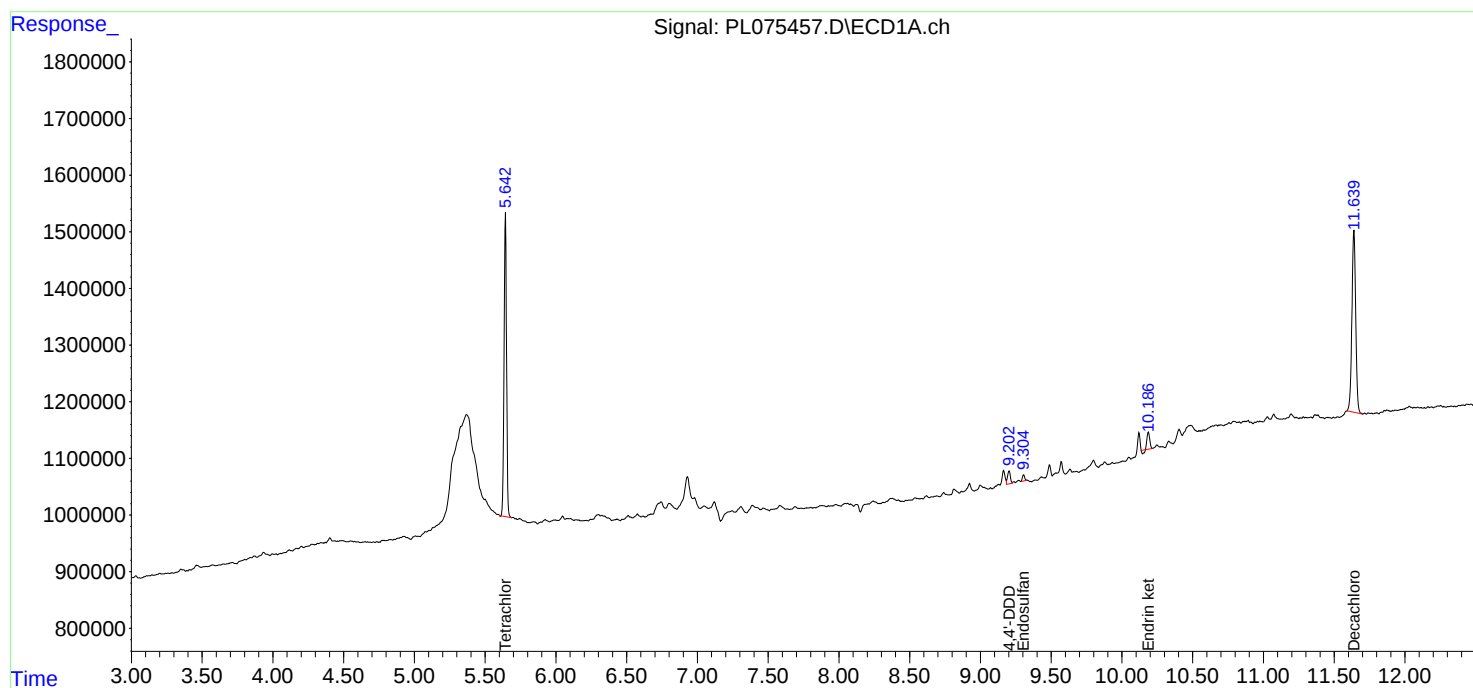


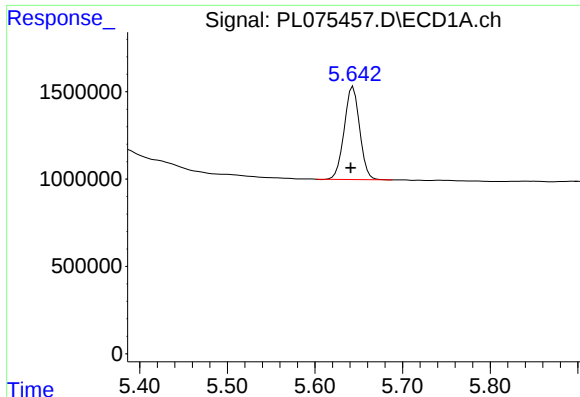

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 6537888
Conc: 11.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

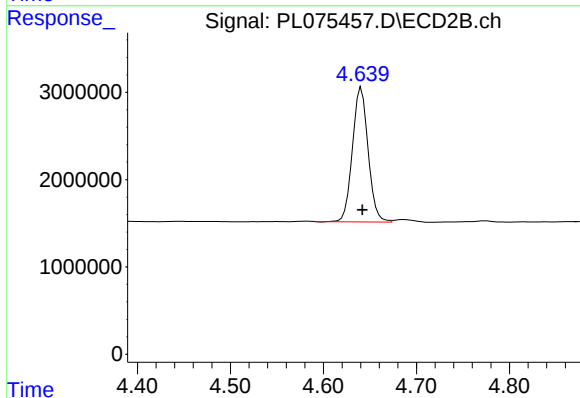


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: -0.001 min
Response: 18007217
Conc: 11.37 ng/ml

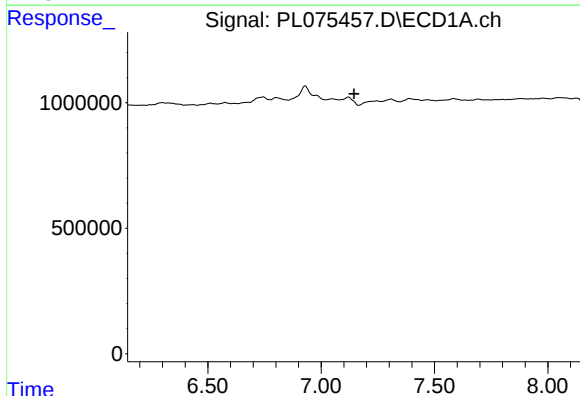


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

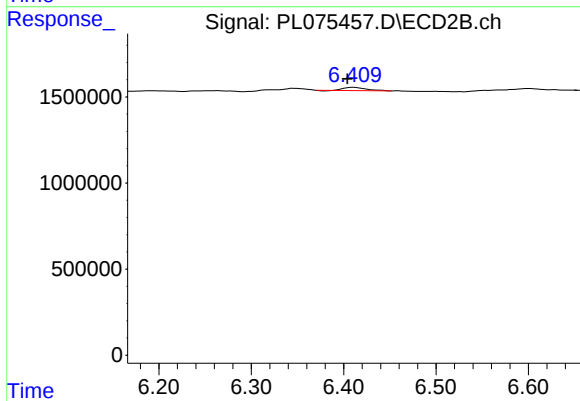

#7 delta-BHC


R.T.: 6.411 min
Delta R.T.: 0.007 min
Response: 321634
Conc: 0.15 ng/ml

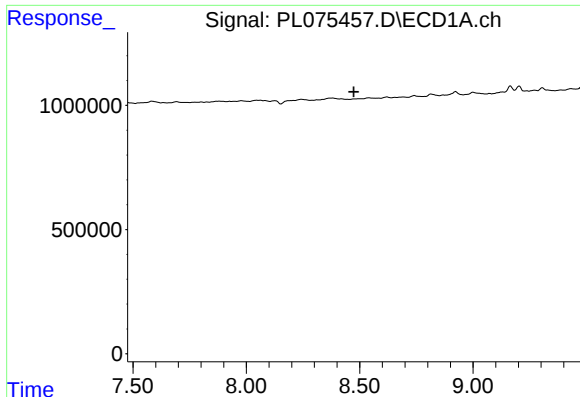

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

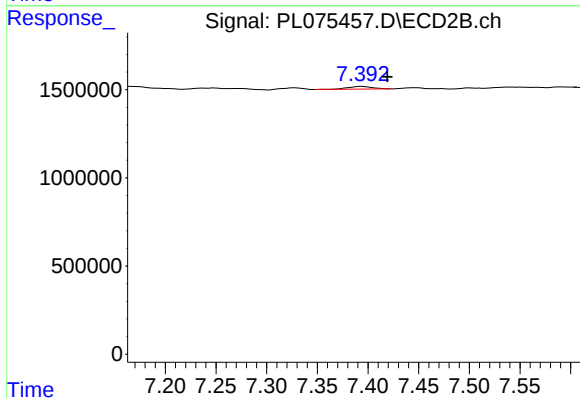


#11 alpha-Chlordane

R.T.: 7.394 min
Delta R.T.: -0.025 min
Response: 248791
Conc: 0.14 ng/ml

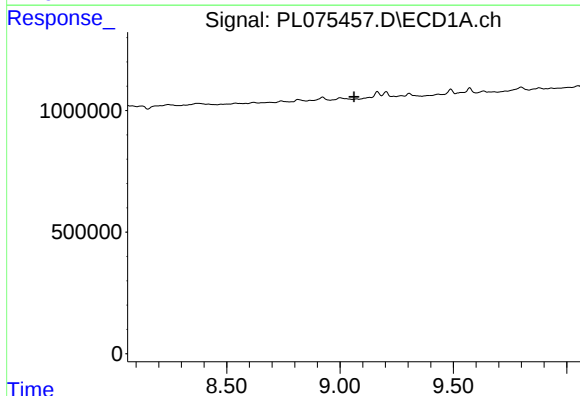


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

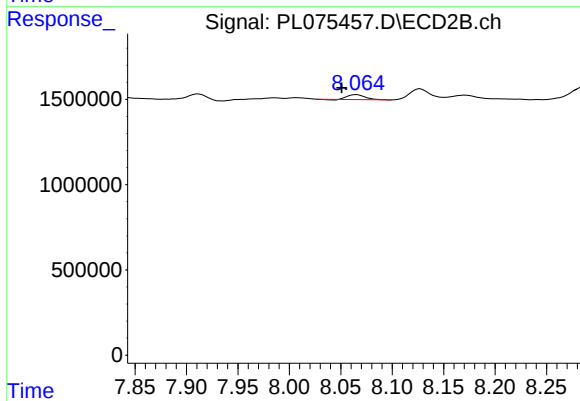

#14 Endrin


R.T.: 8.066 min
Delta R.T.: 0.014 min
Response: 317701
Conc: 0.20 ng/ml

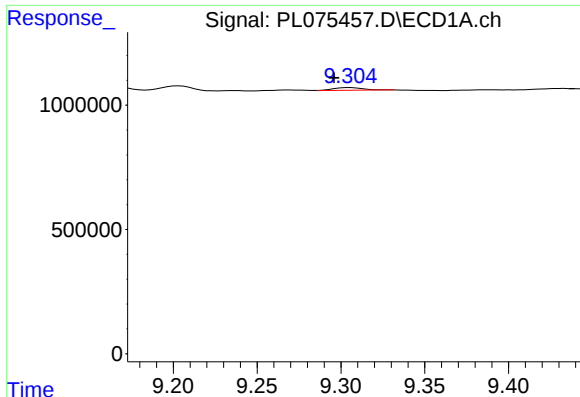

#15 Endosulfan II


R.T.: 9.305 min
Delta R.T.: 0.009 min
Response: 133847
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

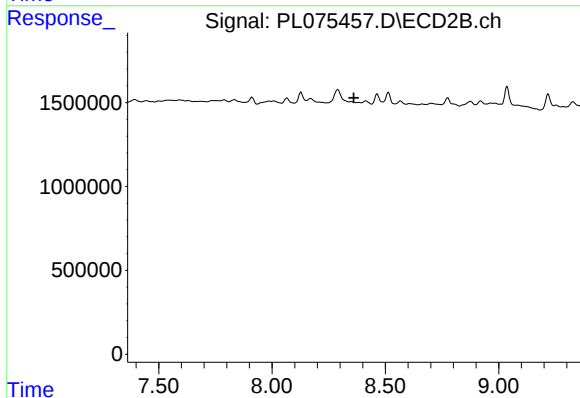


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

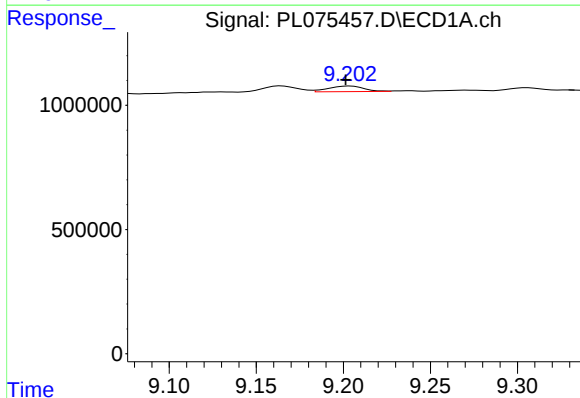


#16 4,4'-DDD

R.T.: 9.204 min
Delta R.T.: 0.002 min
Response: 316484
Conc: 0.64 ng/ml

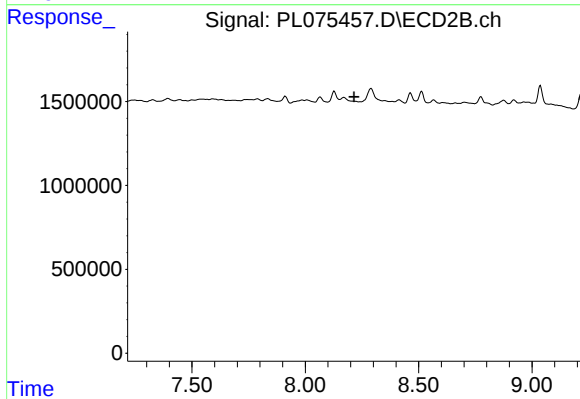

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 8.215 min
Response: 0
Conc: N.D.

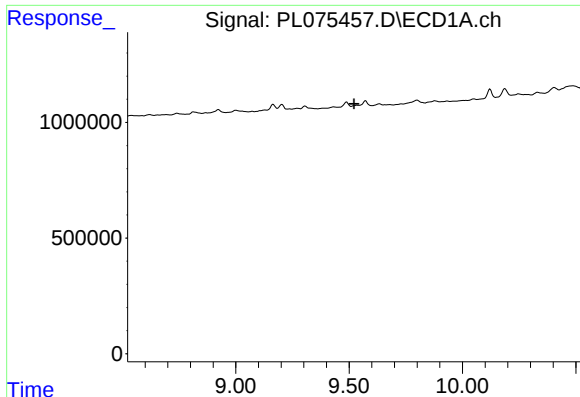

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

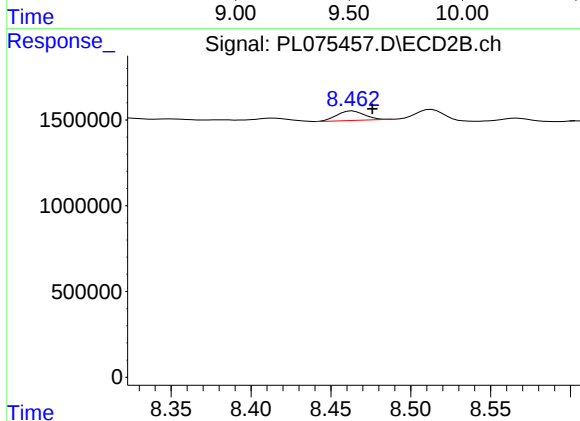


#17 4,4'-DDT

R.T.: 8.463 min
Delta R.T.: -0.013 min
Response: 662473
Conc: 0.46 ng/ml

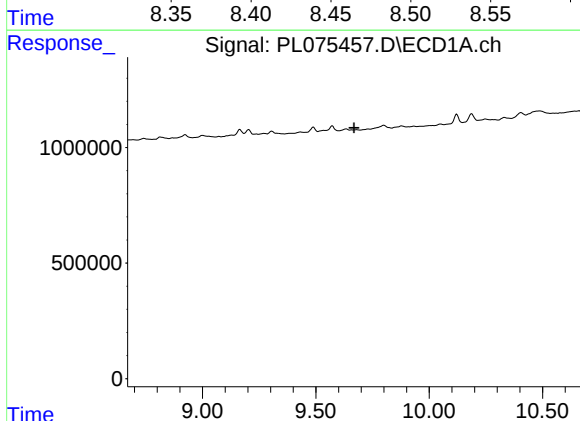


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.669 min
Response: 0
Conc: N.D.

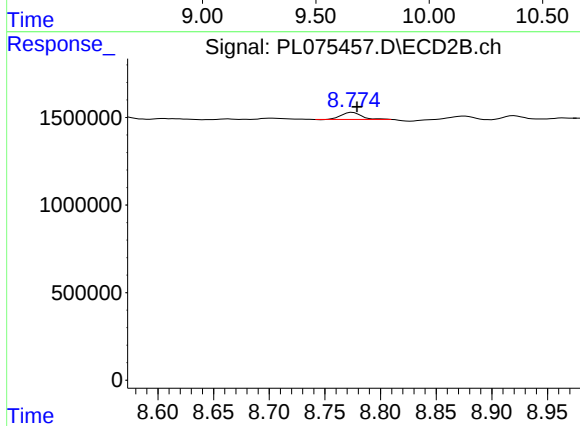

#19 Endosulfan Sulfate


R.T.: 8.775 min
Delta R.T.: -0.004 min
Response: 518647
Conc: 0.35 ng/ml

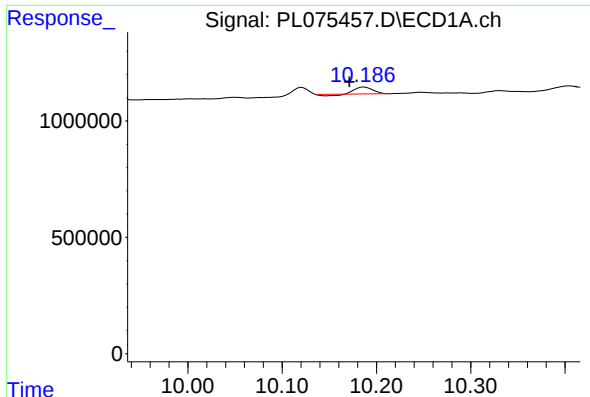

#21 Endrin ketone


R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 338036
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

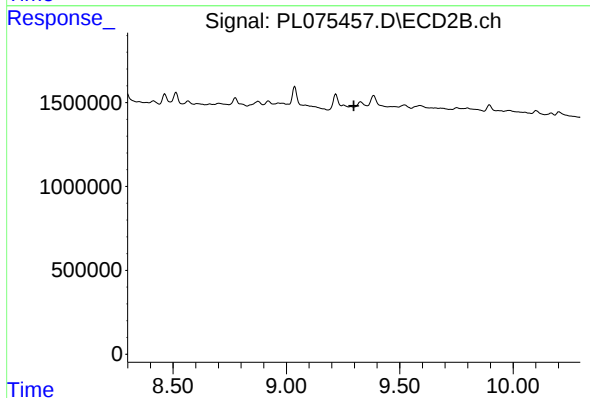


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.297 min
Response: 0
Conc: N.D.

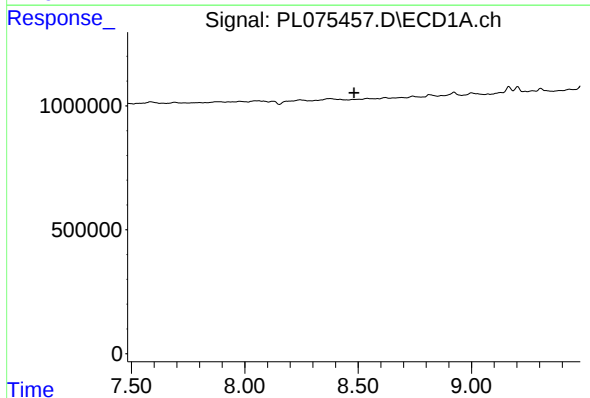


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

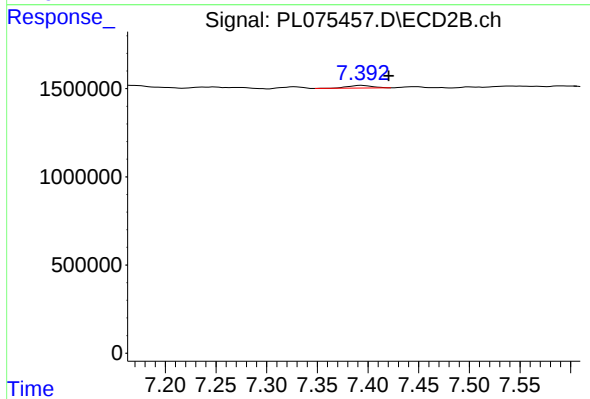

#26 Chlordane-4


R.T.: 7.394 min
Delta R.T.: -0.027 min
Response: 248791
Conc: 1.32 ng/ml

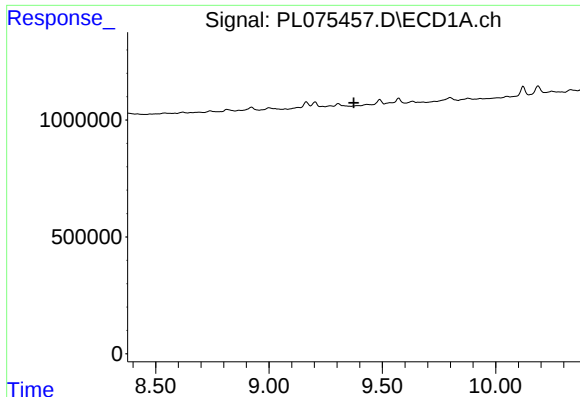

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

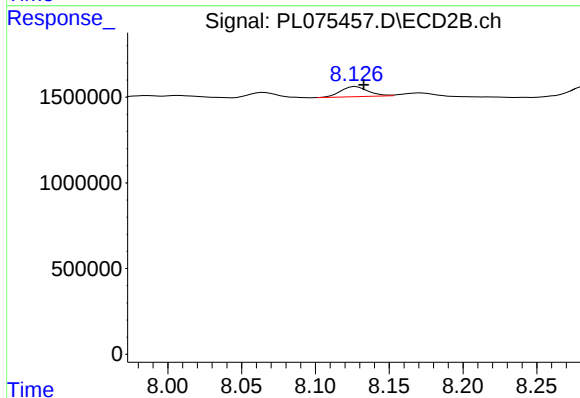


#27 Chlordane-5

R.T.: 8.127 min
Delta R.T.: -0.005 min
Response: 762818
Conc: 15.29 ng/ml

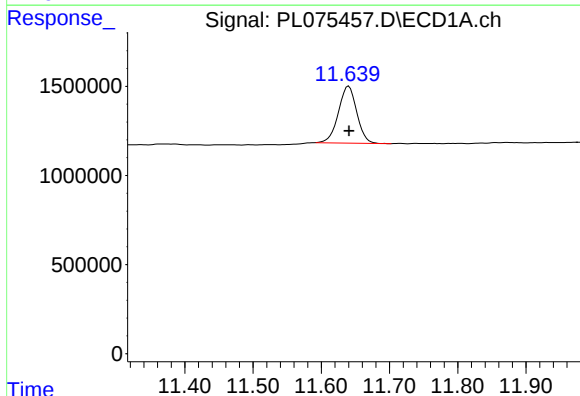

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.000 min
Response: 5990276
Conc: 11.17 ng/ml

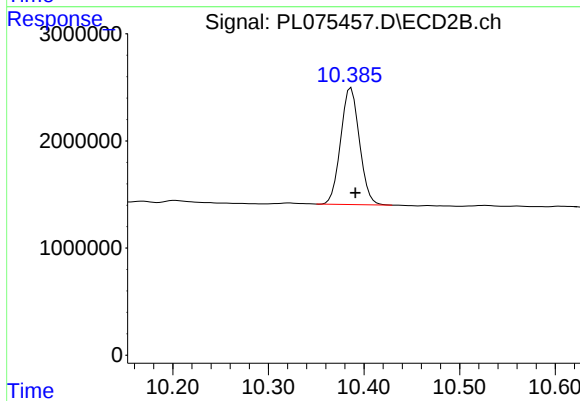

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: -0.005 min
Response: 14881455
Conc: 10.84 ng/ml