

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 14:27
 Operator : AR\AJ
 Sample : N2987-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:37:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.640	6365435	17743875	10.830	11.201
28)	SA Decachlor...	11.640	10.386	5786708	14363345	10.792	10.467
Target Compounds							
7)	B delta-BHC	0.000	6.411	0	523937	N.D.	0.244 #
11)	B alpha-Chl...	0.000	7.391f	0	308540	N.D.	0.169 #
14)	MA Endrin	0.000	8.064	0	277392	N.D.	0.178 #
15)	B Endosulfa...	9.305	0.000	151824	0	0.269	N.D. #
16)	A 4,4'-DDD	9.203	0.000	349533	0	0.707	N.D. #
17)	MA 4,4'-DDT	0.000	8.463	0	711148	N.D.	0.497 #
18)	B Endrin al...	0.000	8.566f	0	158155	N.D.	0.131 #
19)	B Endosulfa...	0.000	8.774	0	571769	N.D.	0.382 #
21)	B Endrin ke...	10.187f	0.000	252119	0	0.411	N.D. #
26)	Chlordane-4	0.000	7.391f	0	308540	N.D.	1.633 #
27)	Chlordane-5	0.000	8.127	0	804089	N.D.	16.114 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 14:27
Operator : AR\AJ
Sample : N2987-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:37:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

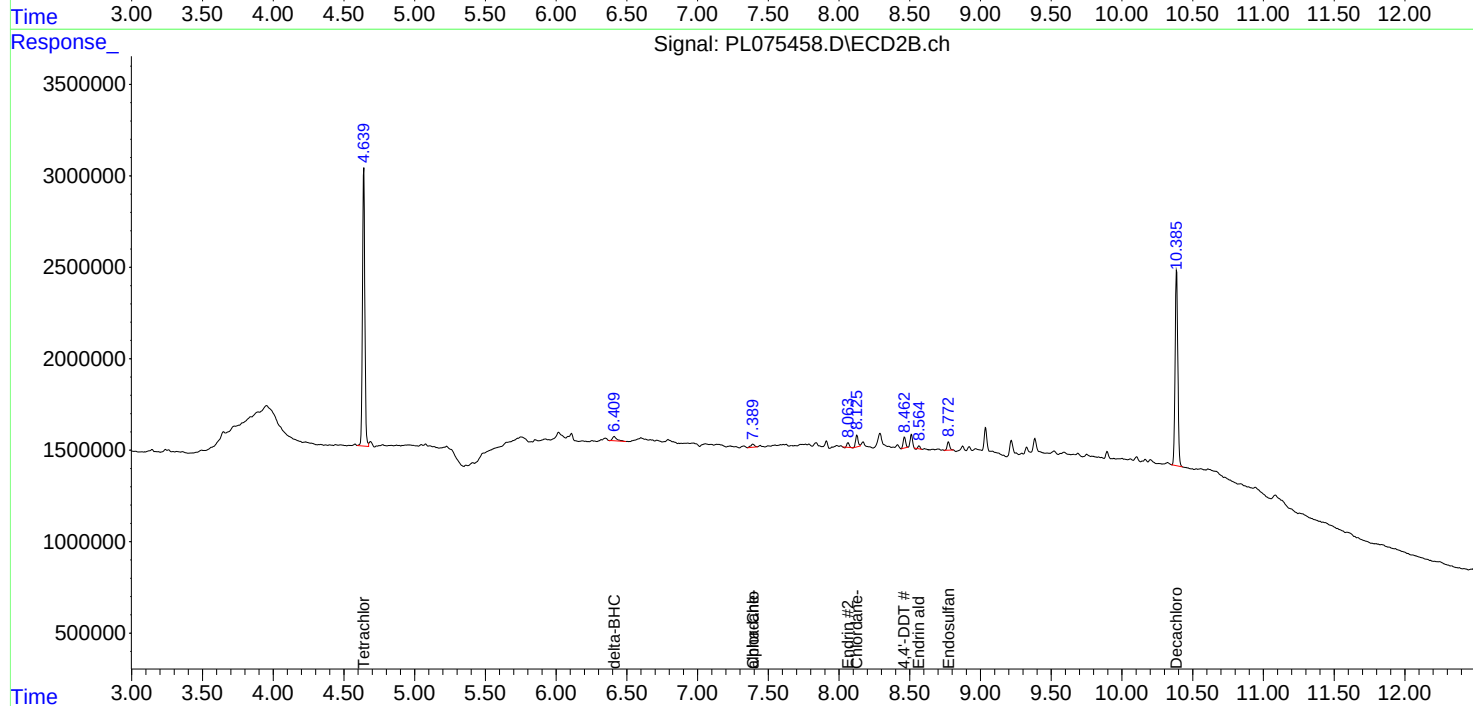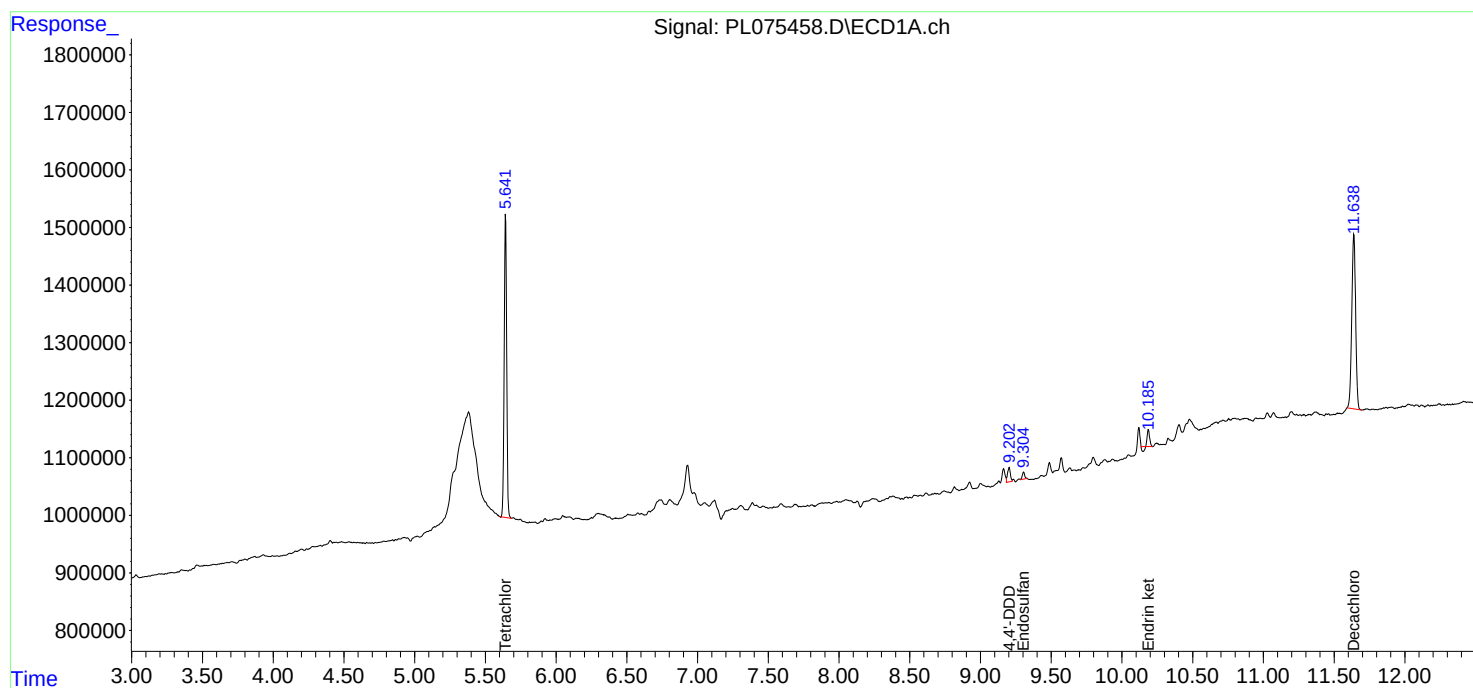


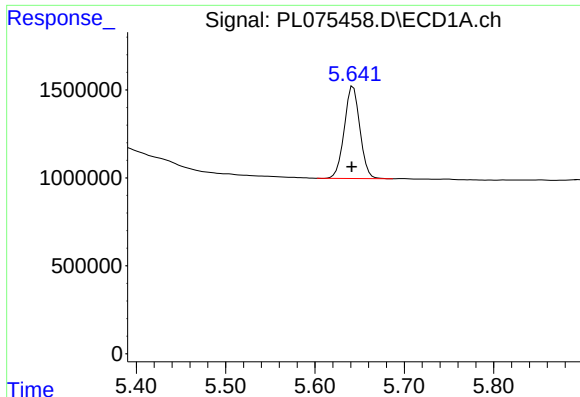

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 6365435
Conc: 10.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

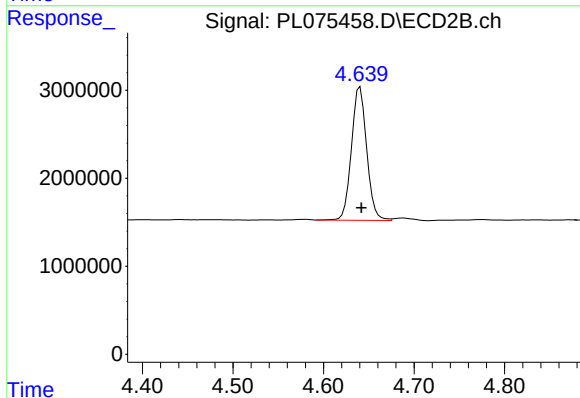


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.002 min
Response: 17743875
Conc: 11.20 ng/ml

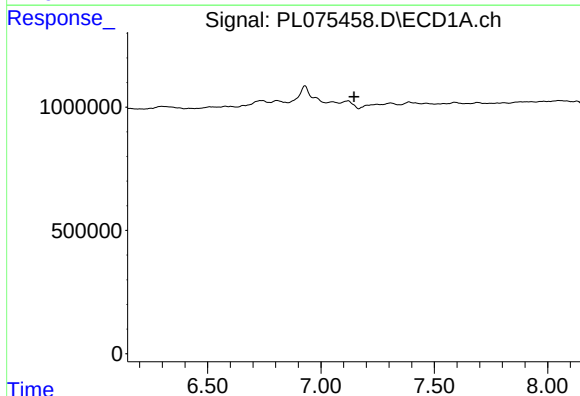


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

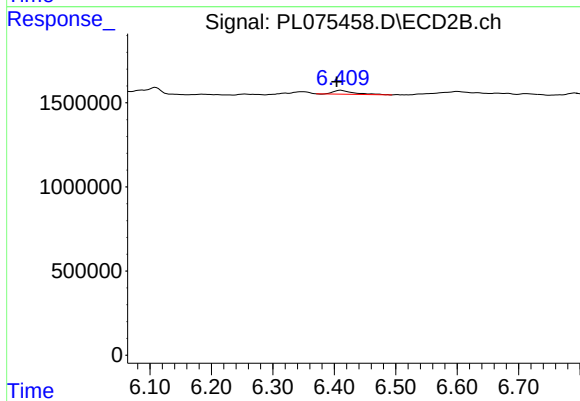

#7 delta-BHC


R.T.: 6.411 min
Delta R.T.: 0.007 min
Response: 523937
Conc: 0.24 ng/ml

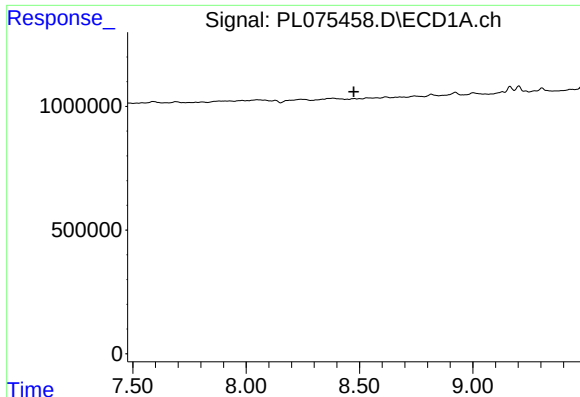

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

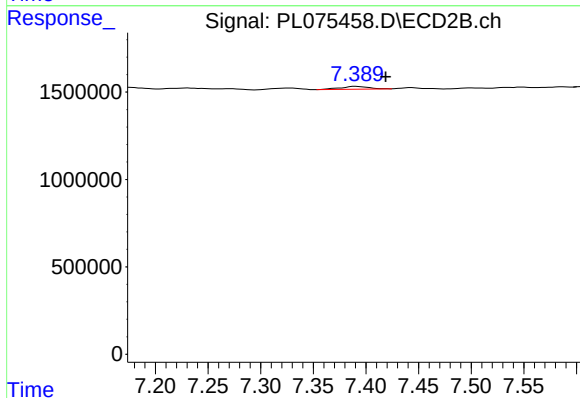


#11 alpha-Chlordane

R.T.: 7.391 min
Delta R.T.: -0.028 min
Response: 308540
Conc: 0.17 ng/ml

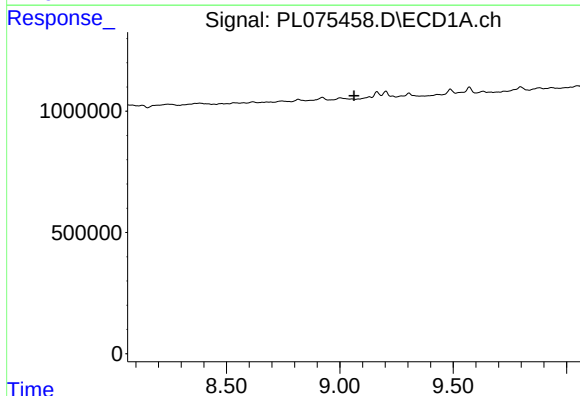


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

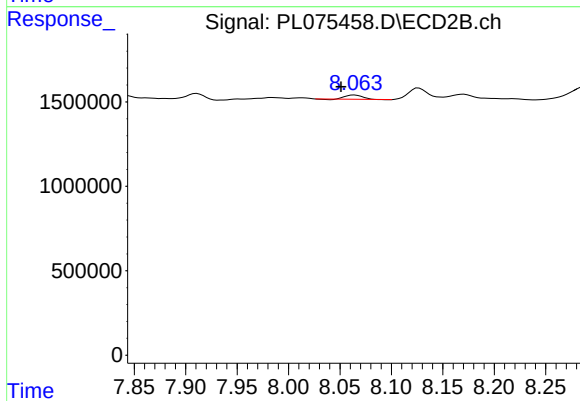

#14 Endrin


R.T.: 8.064 min
Delta R.T.: 0.013 min
Response: 277392
Conc: 0.18 ng/ml

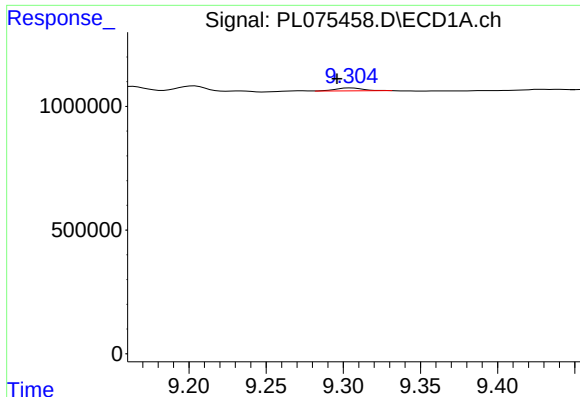

#15 Endosulfan II


R.T.: 9.305 min
Delta R.T.: 0.009 min
Response: 151824
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

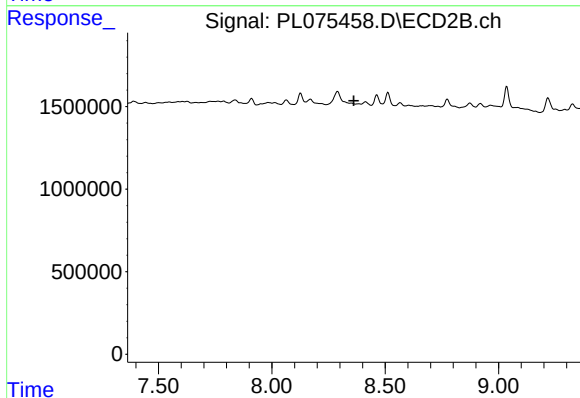


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

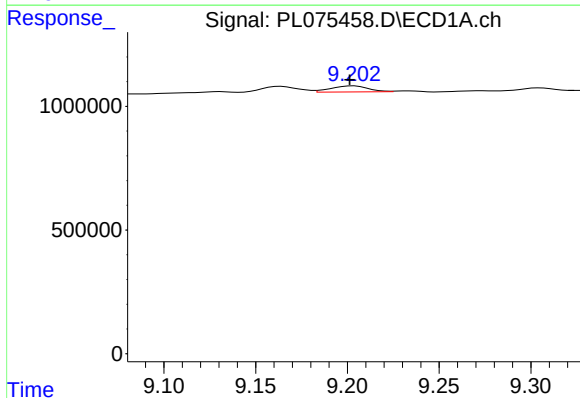


#16 4,4'-DDD

R.T.: 9.203 min
Delta R.T.: 0.002 min
Response: 349533
Conc: 0.71 ng/ml

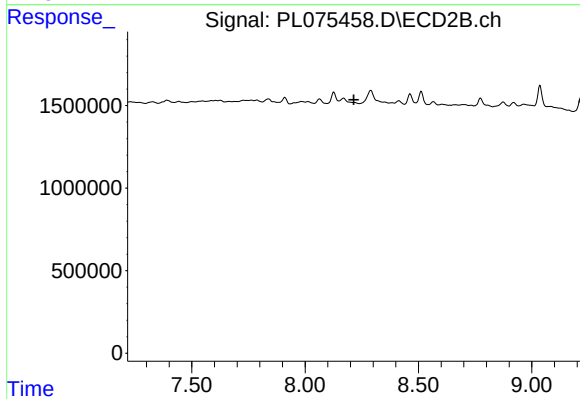

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 8.215 min
Response: 0
Conc: N.D.

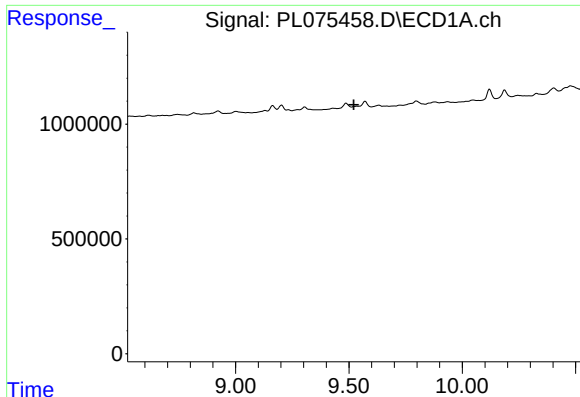

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

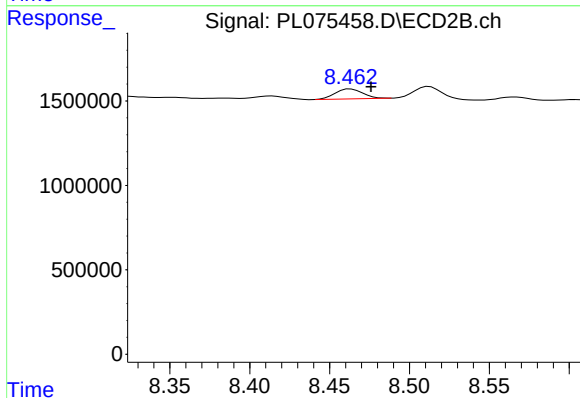


#17 4,4'-DDT

R.T.: 8.463 min
Delta R.T.: -0.013 min
Response: 711148
Conc: 0.50 ng/ml

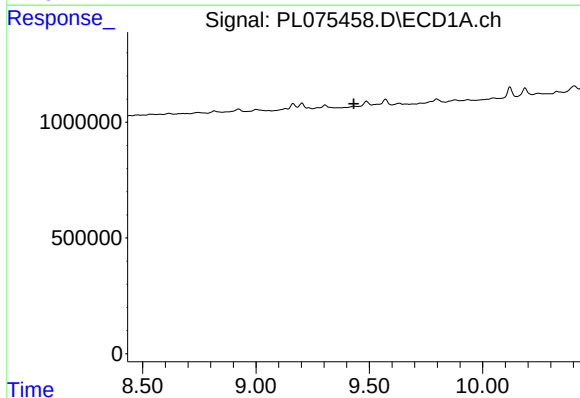


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 9.431 min
Response: 0
Conc: N.D.

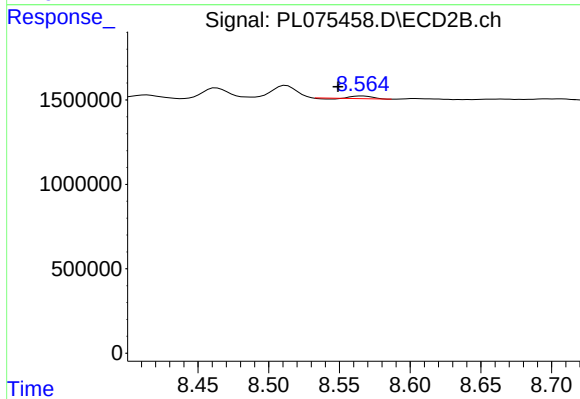

#18 Endrin aldehyde


R.T.: 8.566 min
Delta R.T.: 0.017 min
Response: 158155
Conc: 0.13 ng/ml

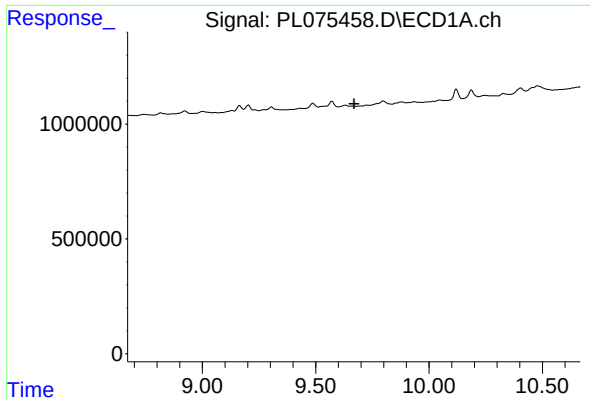

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

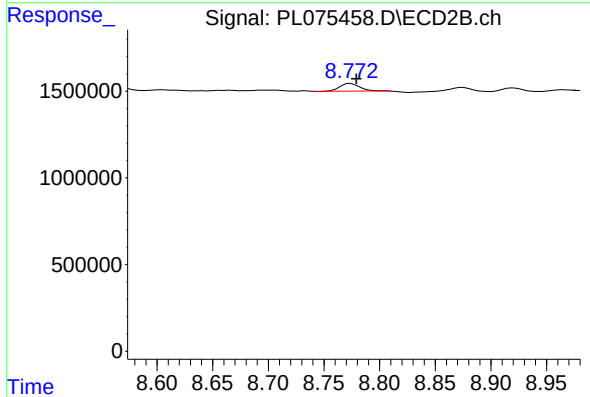


#19 Endosulfan Sulfate

R.T.: 8.774 min
Delta R.T.: -0.005 min
Response: 571769
Conc: 0.38 ng/ml

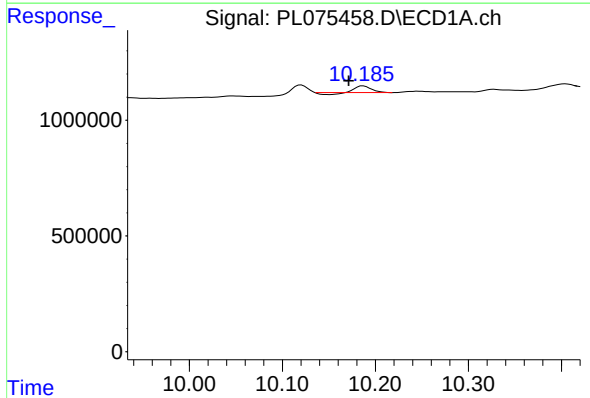


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 252119
Conc: 0.41 ng/ml

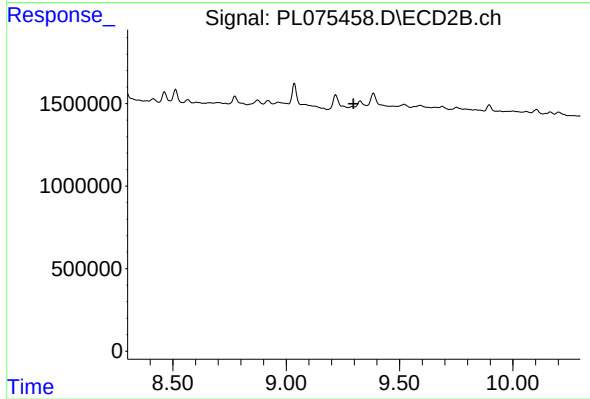

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.297 min
Response: 0
Conc: N.D.

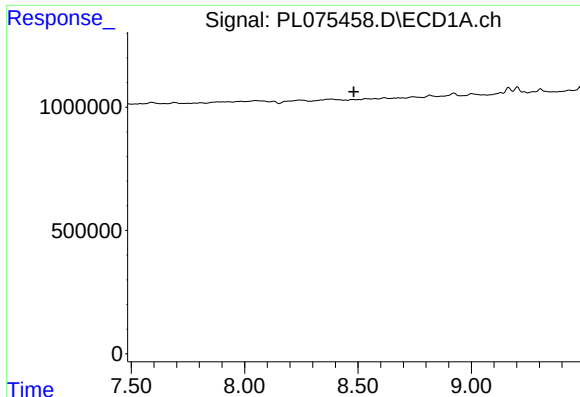

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.482 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

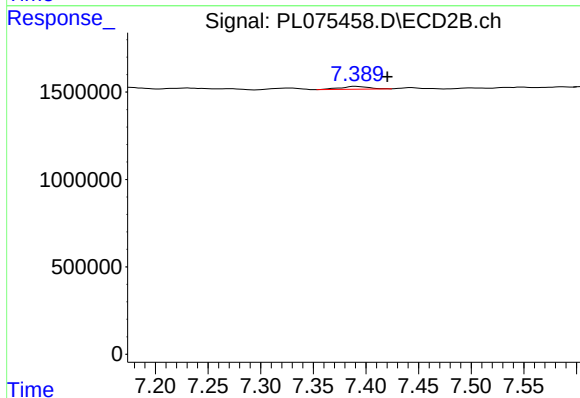


#26 Chlordane-4

R.T.: 7.391 min
Delta R.T.: -0.030 min
Response: 308540
Conc: 1.63 ng/ml

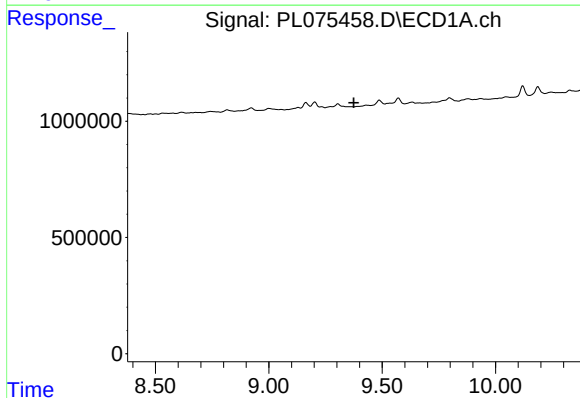


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

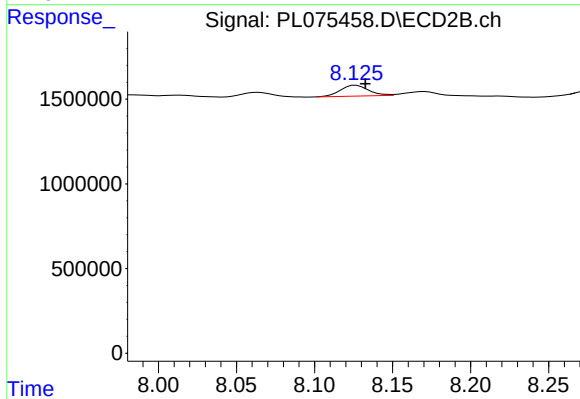

#27 Chlordane-5


R.T.: 8.127 min
Delta R.T.: -0.006 min
Response: 804089
Conc: 16.11 ng/ml

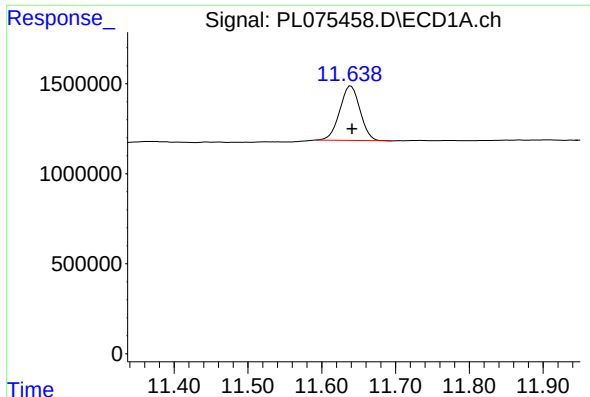

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.001 min
Response: 5786708
Conc: 10.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

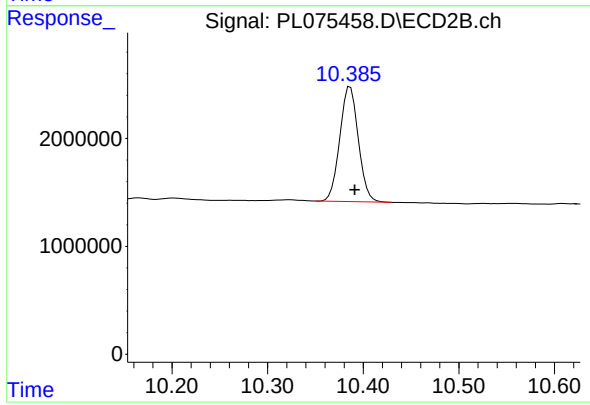

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: -0.005 min
Response: 14363345
Conc: 10.47 ng/ml