

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 17:45
 Operator : AR\AJ
 Sample : N2987-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:40:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.641	11450511	30418390	19.482	19.202
28)	SA Decachlor...	11.641	10.387	9653356	22045820	18.004	16.065
Target Compounds							
7)	B delta-BHC	0.000	6.414	0	351883	N.D.	0.164 #
11)	B alpha-Chl...	0.000	7.397f	0	295858	N.D.	0.162 #
13)	MA Dieldrin	0.000	7.759	0	579489	N.D.	0.334 #
14)	MA Endrin	0.000	8.068f	0	283056	N.D.	0.182 #
15)	B Endosulfa...	9.306	0.000	260010	0	0.461	N.D. #
16)	A 4,4'-DDD	9.201	0.000	158500	0	0.320	N.D. #
17)	MA 4,4'-DDT	0.000	8.467	0	347389	N.D.	0.243 #
19)	B Endosulfa...	9.675	8.774	182270	82208	0.328	0.055 #
26)	Chlordane-4	0.000	7.397f	0	295858	N.D.	1.566 #
27)	Chlordane-5	0.000	8.129	0	190110	N.D.	3.810 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 17:45
Operator : AR\AJ
Sample : N2987-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:40:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

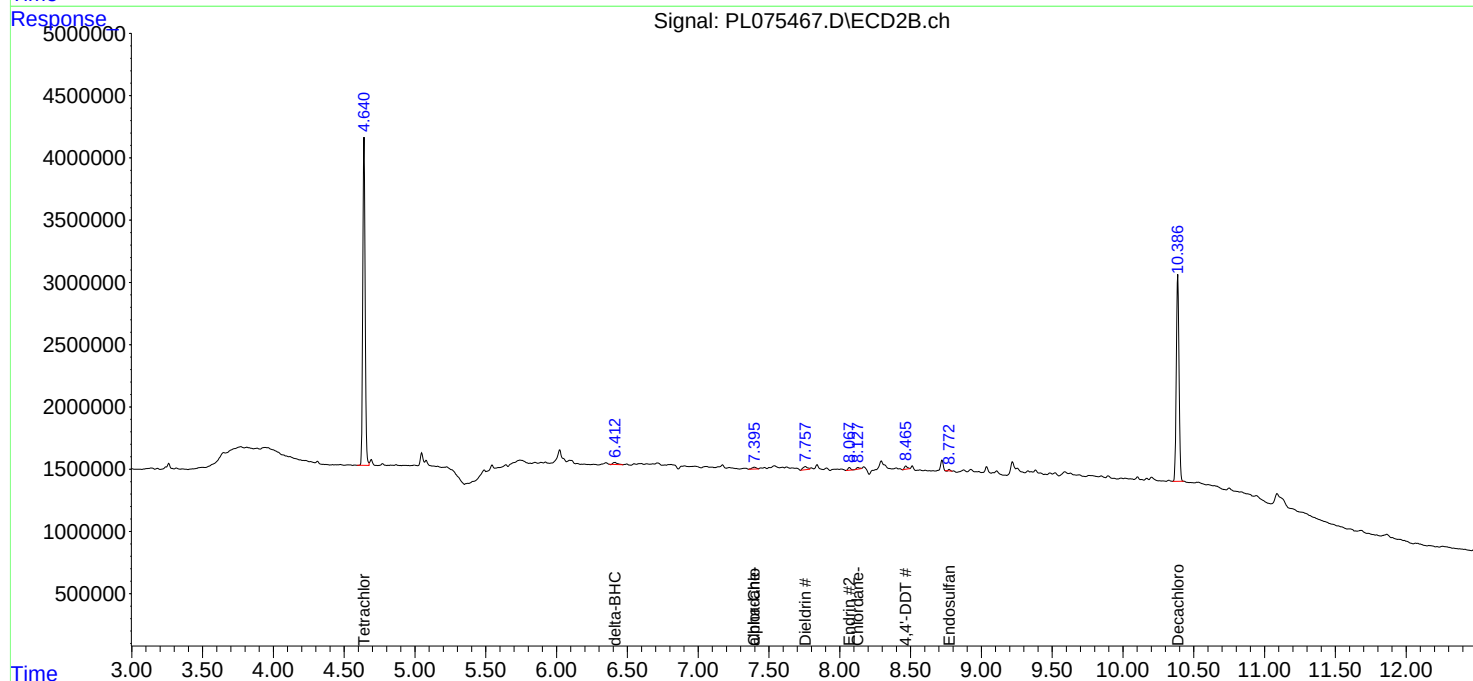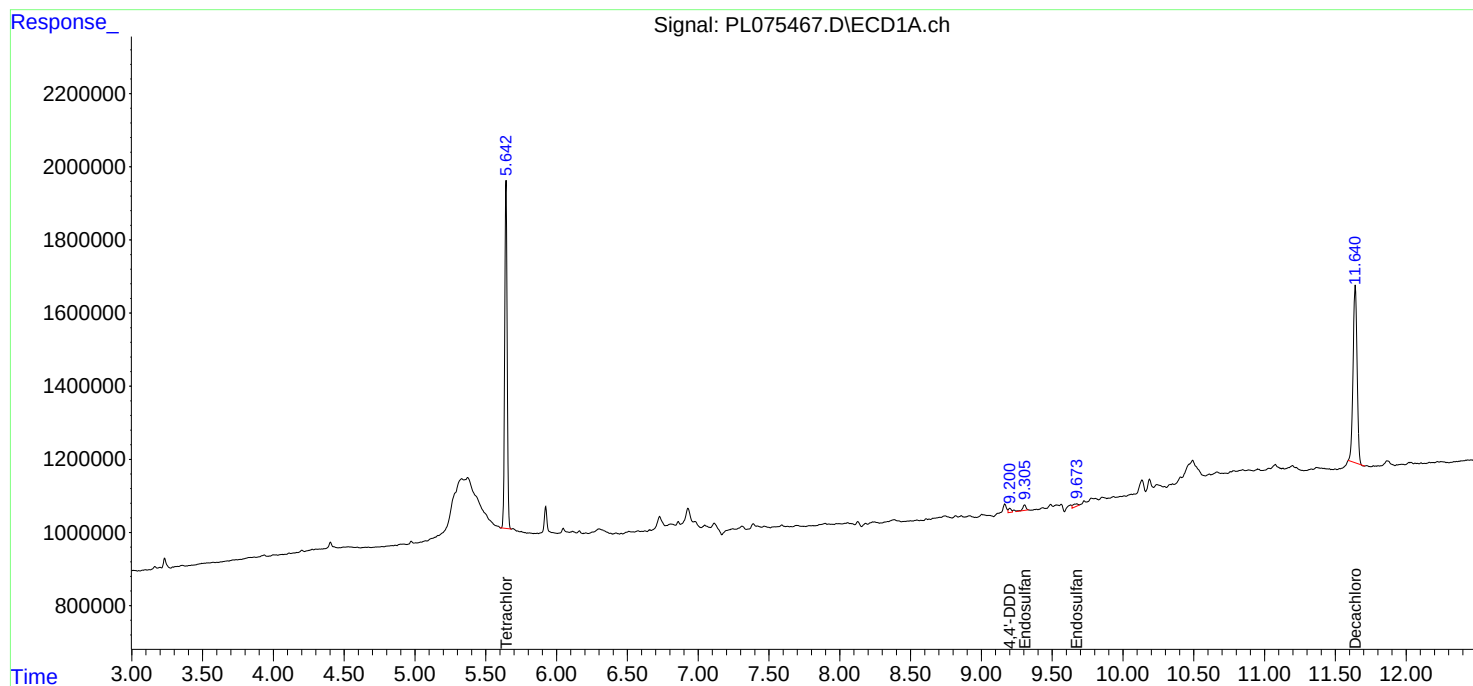


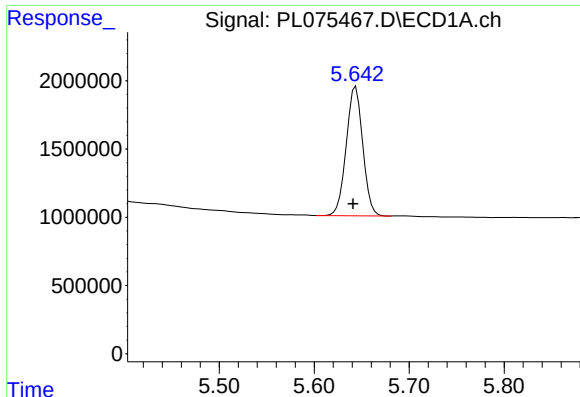

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 11450511
Conc: 19.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

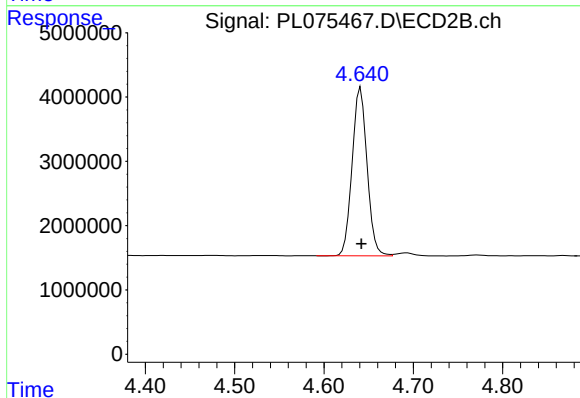


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 30418390
Conc: 19.20 ng/ml

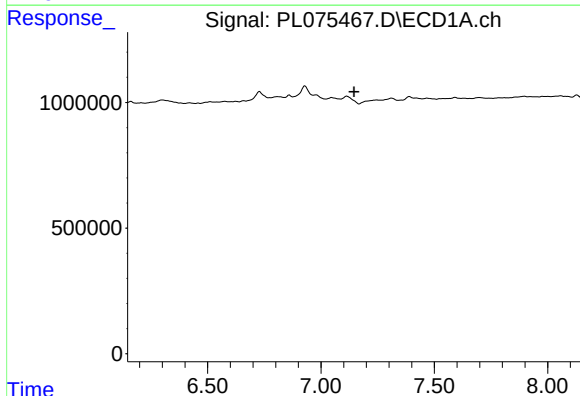


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

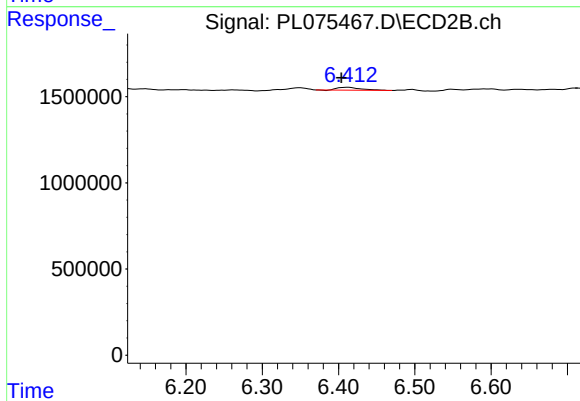

#7 delta-BHC


R.T.: 6.414 min
Delta R.T.: 0.010 min
Response: 351883
Conc: 0.16 ng/ml

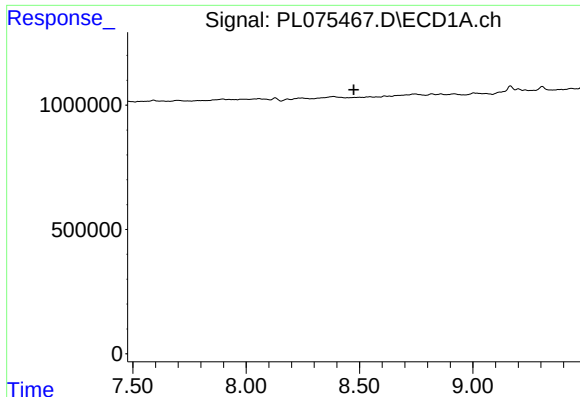

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

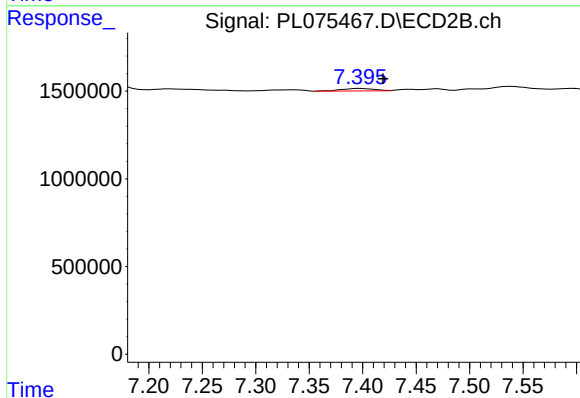


#11 alpha-Chlordane

R.T.: 7.397 min
Delta R.T.: -0.022 min
Response: 295858
Conc: 0.16 ng/ml

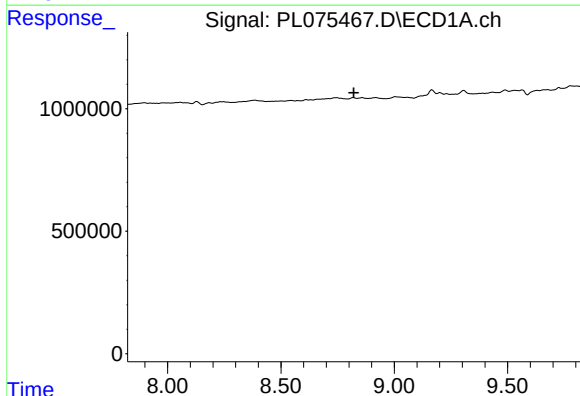


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

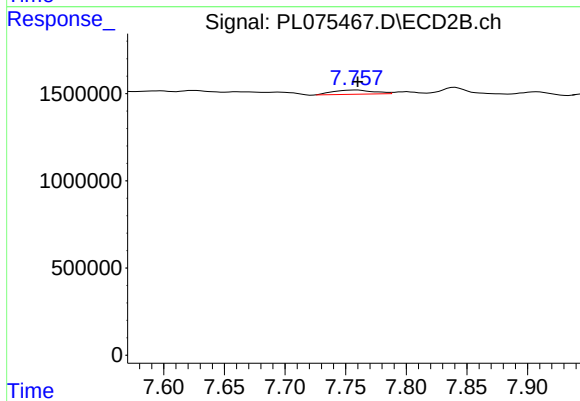

#13 Dieldrin


R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 579489
Conc: 0.33 ng/ml

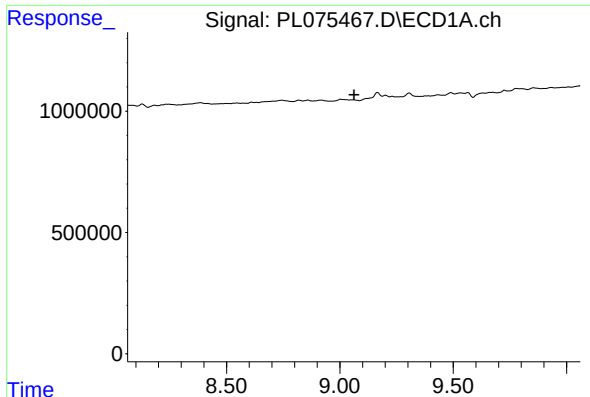

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

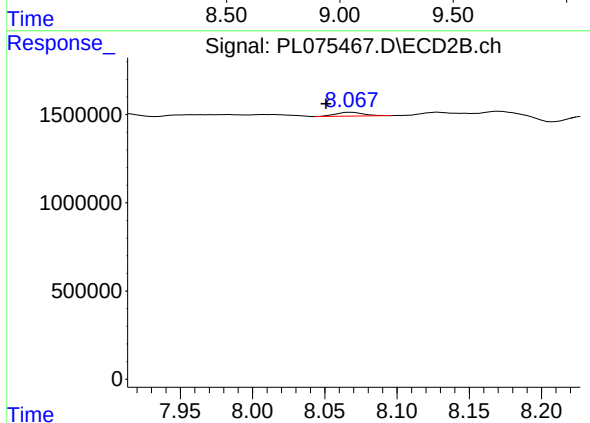


#14 Endrin

R.T.: 8.068 min
Delta R.T.: 0.017 min
Response: 283056
Conc: 0.18 ng/ml

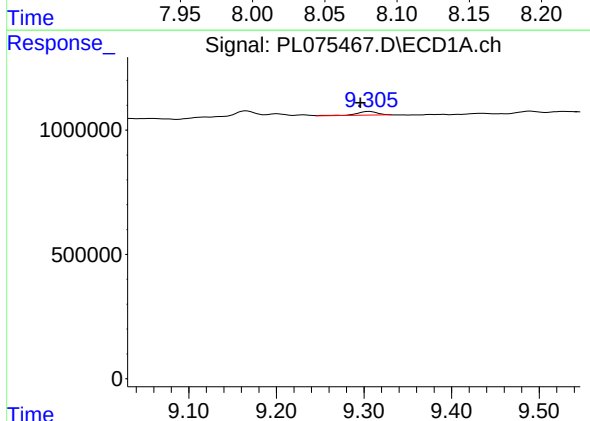


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 260010
Conc: 0.46 ng/ml

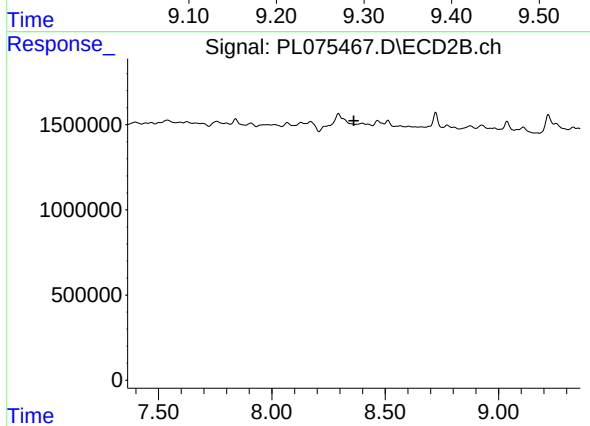

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

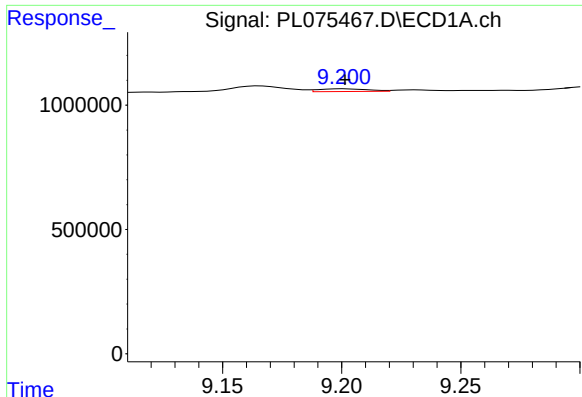

#16 4,4'-DDD


R.T.: 9.201 min
Delta R.T.: 0.000 min
Response: 158500
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

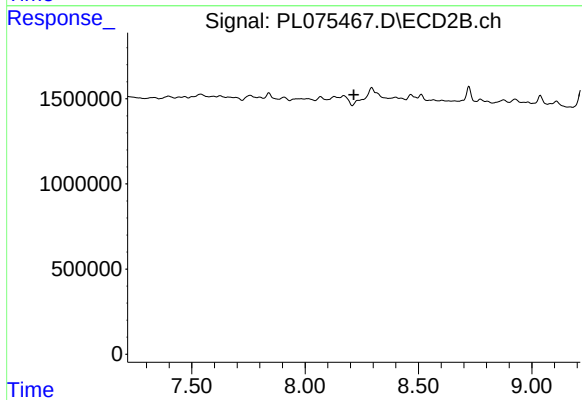


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.215 min
Response: 0
Conc: N.D.

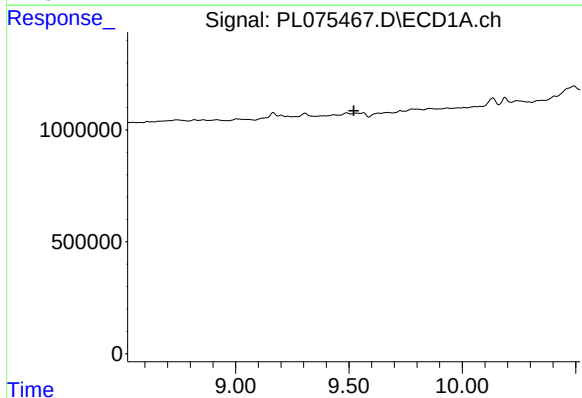


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

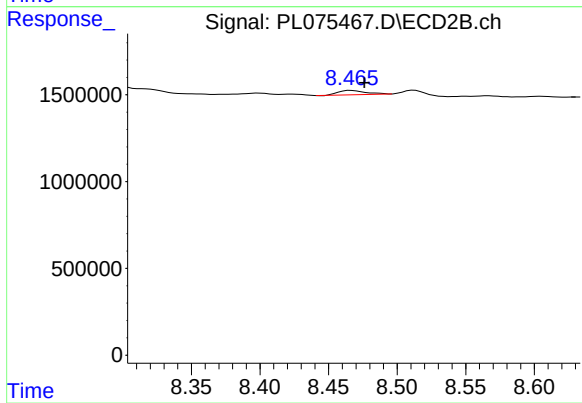

#17 4,4'-DDT


R.T.: 8.467 min
Delta R.T.: -0.009 min
Response: 347389
Conc: 0.24 ng/ml

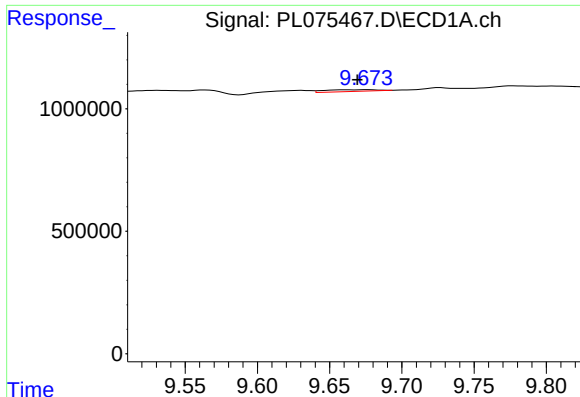

#19 Endosulfan Sulfate


R.T.: 9.675 min
Delta R.T.: 0.006 min
Response: 182270
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

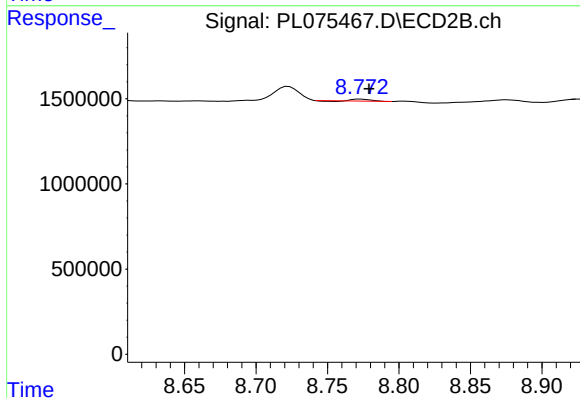


#19 Endosulfan Sulfate

R.T.: 8.774 min
Delta R.T.: -0.005 min
Response: 82208
Conc: 0.05 ng/ml

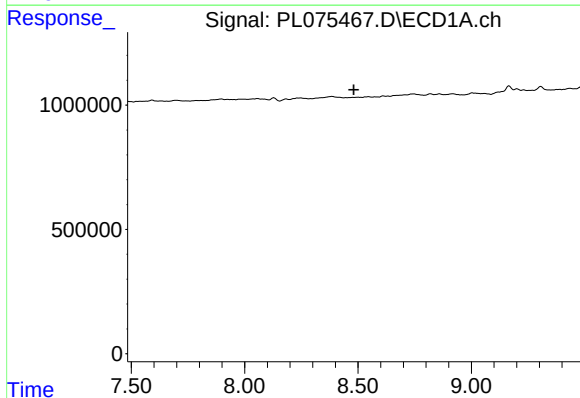


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

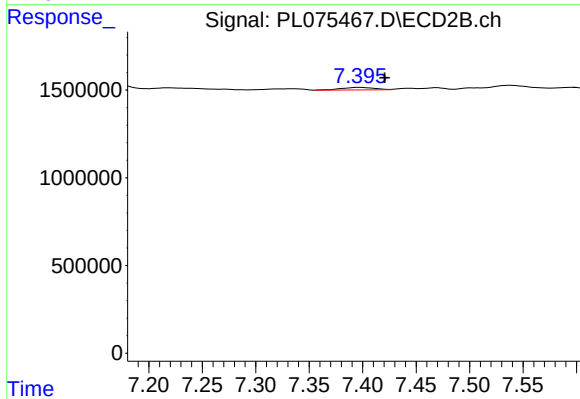

#26 Chlordane-4


R.T.: 7.397 min
Delta R.T.: -0.023 min
Response: 295858
Conc: 1.57 ng/ml

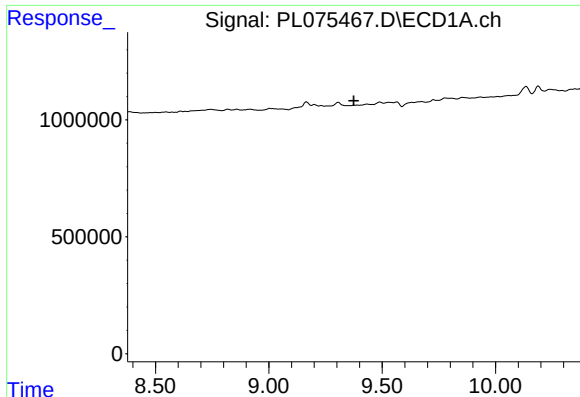

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

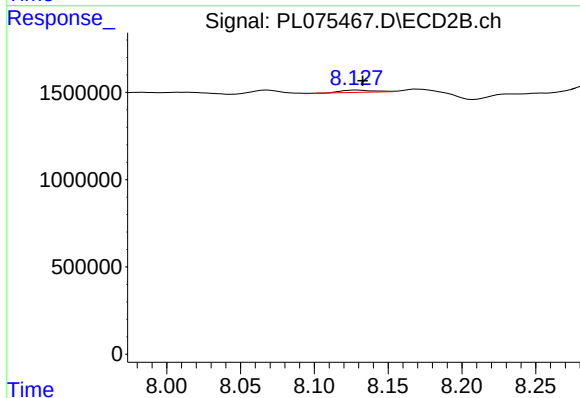


#27 Chlordane-5

R.T.: 8.129 min
Delta R.T.: -0.004 min
Response: 190110
Conc: 3.81 ng/ml

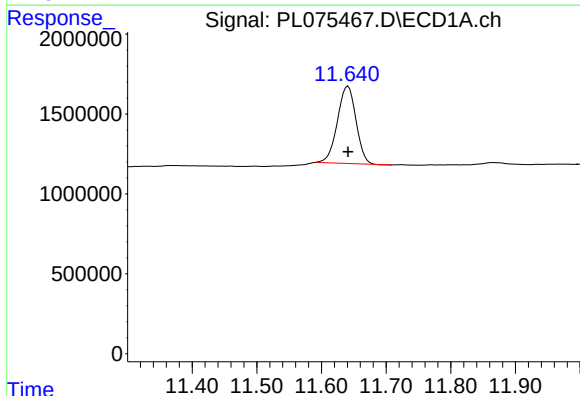

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 9653356
Conc: 18.00 ng/ml

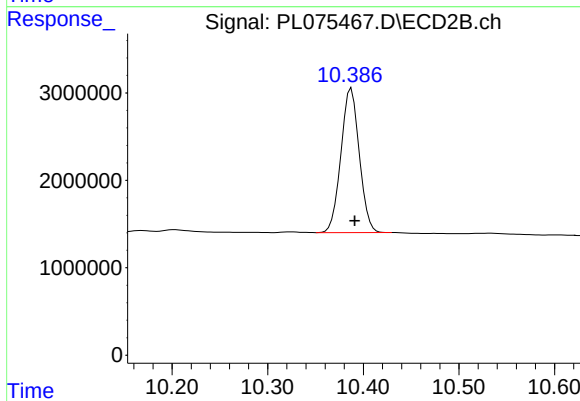

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.004 min
Response: 22045820
Conc: 16.07 ng/ml