

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 18:02
 Operator : AR\AJ
 Sample : N2987-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:40:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.641	11595598	30816846	19.729	19.453
28)	SA Decachlor...	11.640	10.386	8145976	19756669	15.193	14.397
Target Compounds							
5)	MB Aldrin	0.000	6.493	0	888064	N.D.	0.460 #
7)	B delta-BHC	0.000	6.414	0	243061	N.D.	0.113 #
8)	B Heptachlo...	8.126	0.000	3891287	0	5.700	N.D. #
9)	A Endosulfan I	0.000	7.503f	0	127146	N.D.	0.075 #
11)	B alpha-Chl...	0.000	7.443f	0	297545	N.D.	0.163 #
13)	MA Dieldrin	0.000	7.767	0	4540187	N.D.	2.617 #
14)	MA Endrin	0.000	8.070f	0	1253634	N.D.	0.805 #
15)	B Endosulfa...	9.307	8.374	366129	62665	0.649	0.040 #
17)	MA 4,4'-DDT	0.000	8.467	0	224343	N.D.	0.157 #
26)	Chlordane-4	0.000	7.443f	0	297545	N.D.	1.575 #
27)	Chlordane-5	0.000	8.144	0	412792	N.D.	8.272 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 18:02
Operator : AR\AJ
Sample : N2987-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:40:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

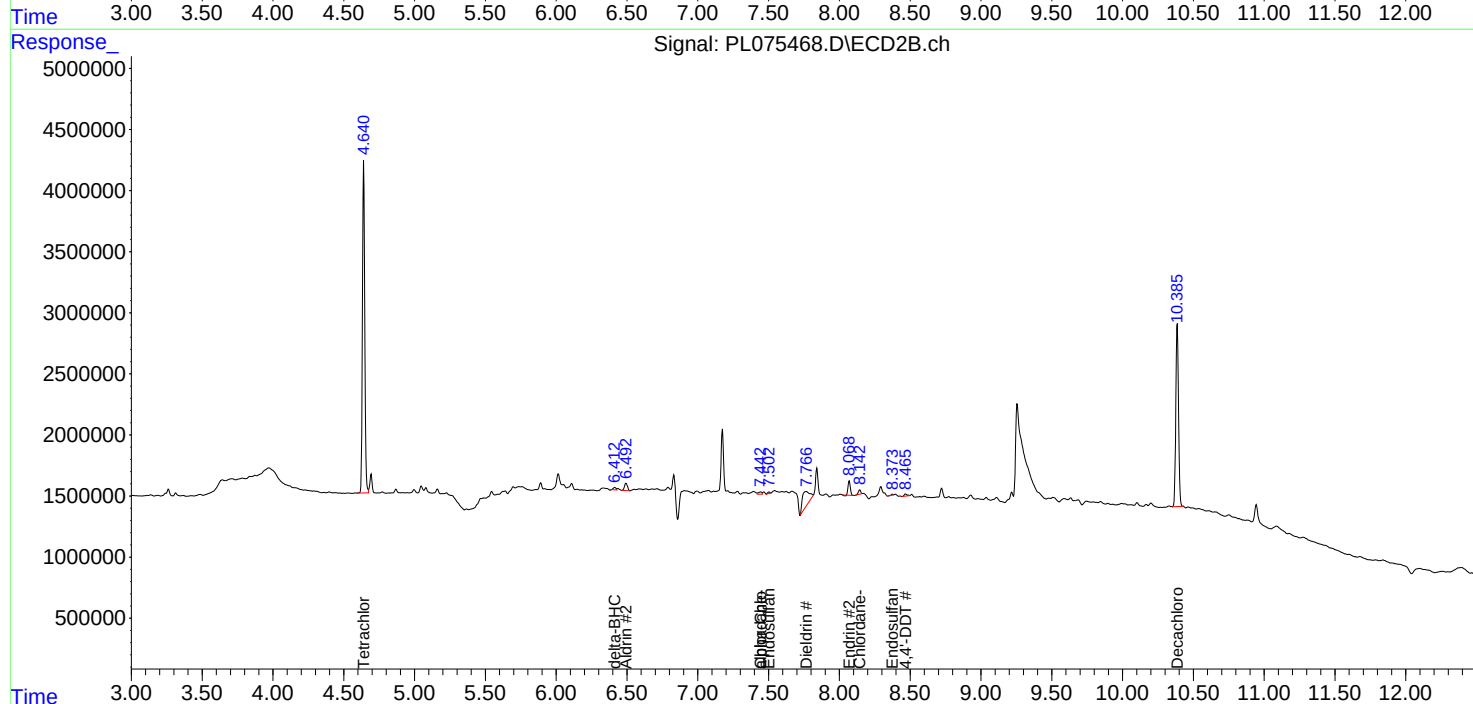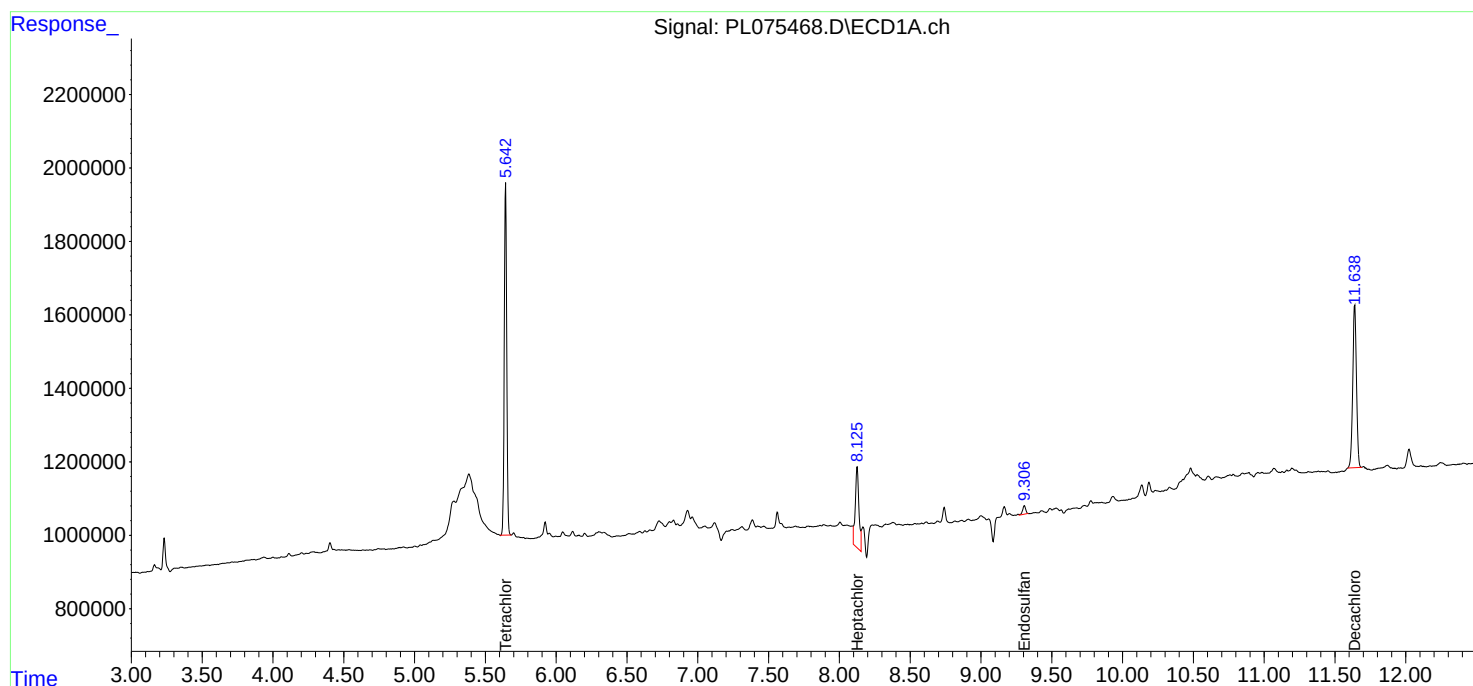


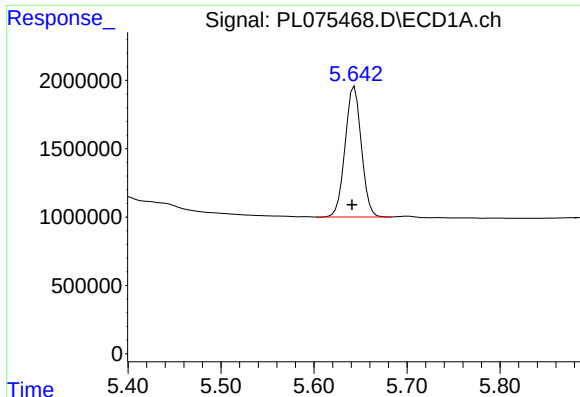

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 11595598
Conc: 19.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

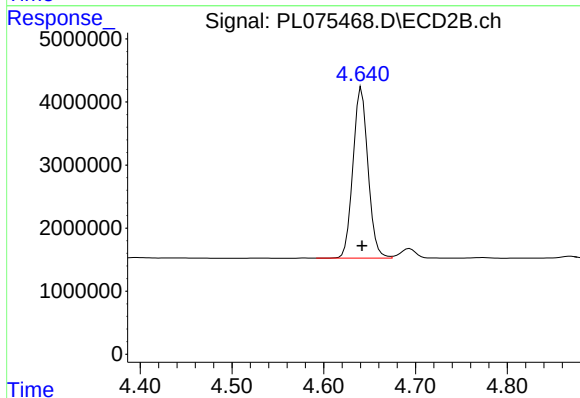


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 30816846
Conc: 19.45 ng/ml

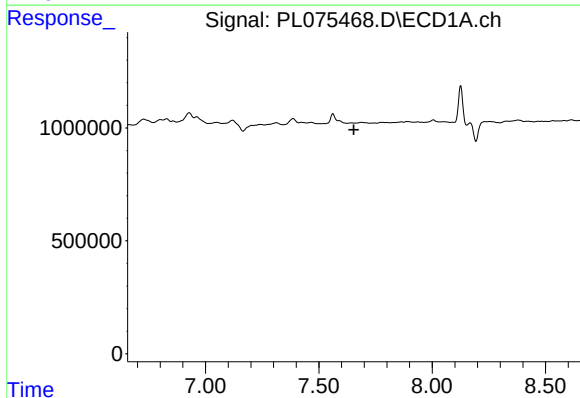


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

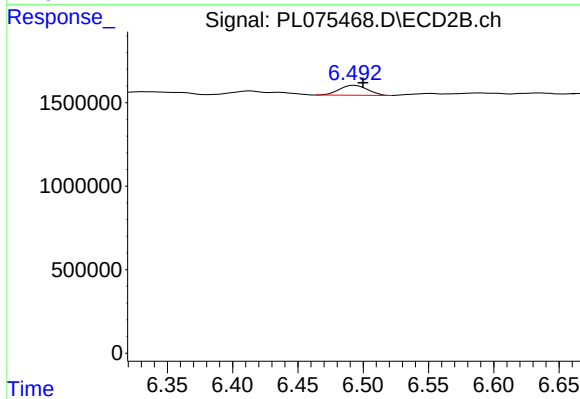

#5 Aldrin


R.T.: 6.493 min
Delta R.T.: -0.007 min
Response: 888064
Conc: 0.46 ng/ml

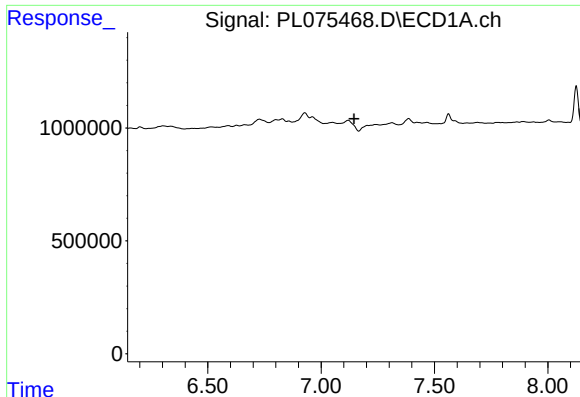

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.146 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

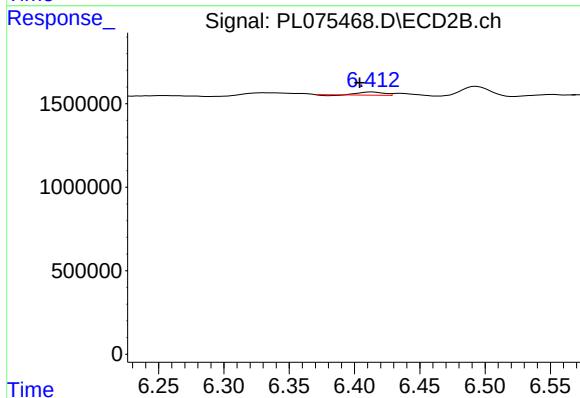


#7 delta-BHC

R.T.: 6.414 min
Delta R.T.: 0.010 min
Response: 243061
Conc: 0.11 ng/ml

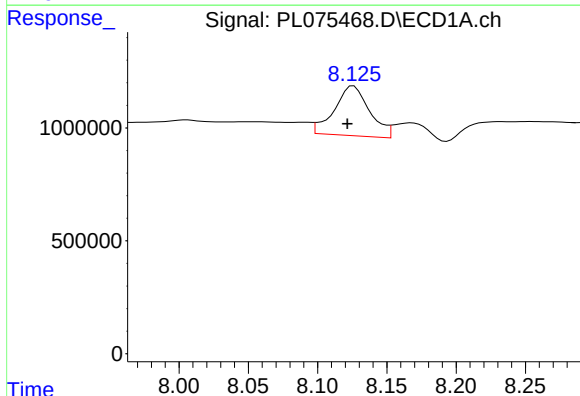


#8 Heptachlor epoxide

R.T.: 8.126 min
Delta R.T.: 0.004 min
Response: 3891287
Conc: 5.70 ng/ml

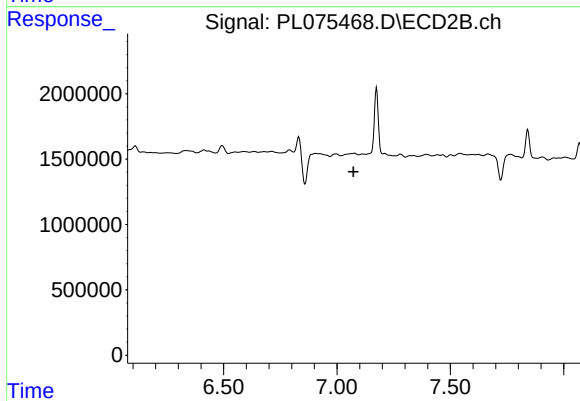

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.073 min
Response: 0
Conc: N.D.

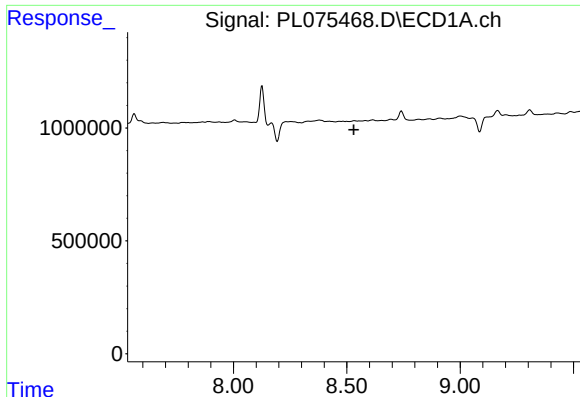

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

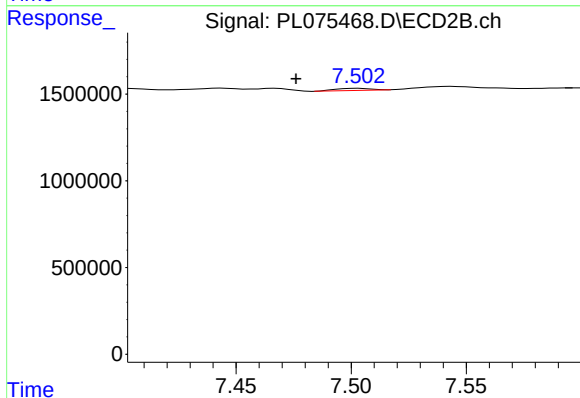


#9 Endosulfan I

R.T.: 7.503 min
Delta R.T.: 0.027 min
Response: 127146
Conc: 0.08 ng/ml

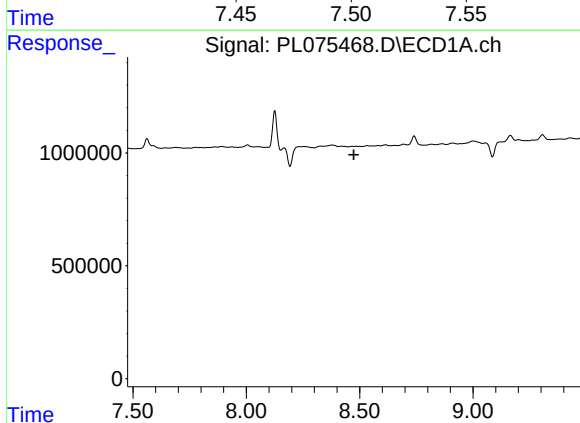


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

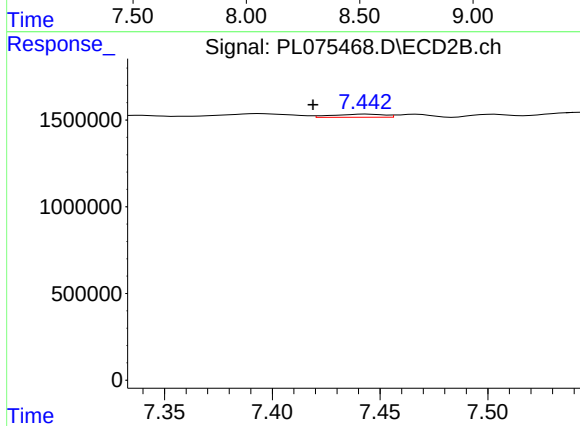

#11 alpha-Chlordane


R.T.: 7.443 min
Delta R.T.: 0.024 min
Response: 297545
Conc: 0.16 ng/ml

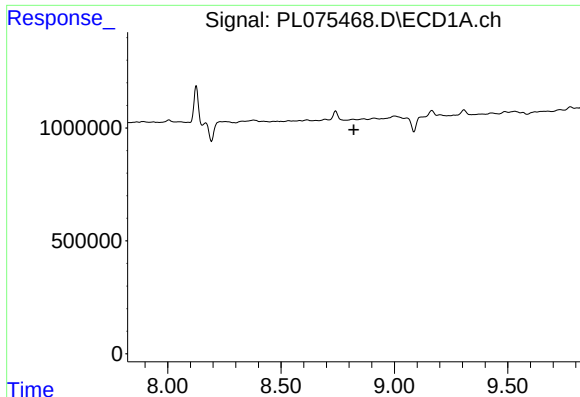

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

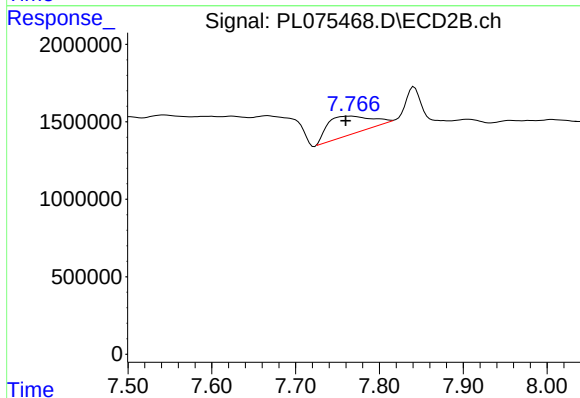


#13 Dieldrin

R.T.: 7.767 min
Delta R.T.: 0.007 min
Response: 4540187
Conc: 2.62 ng/ml

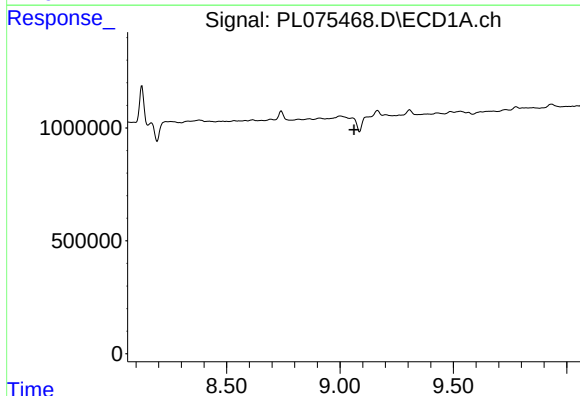


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

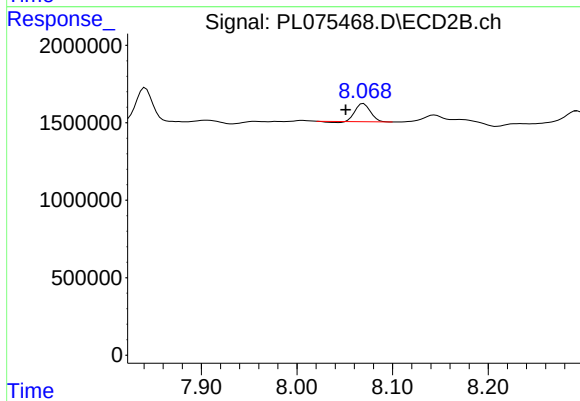

#14 Endrin


R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 1253634
Conc: 0.81 ng/ml

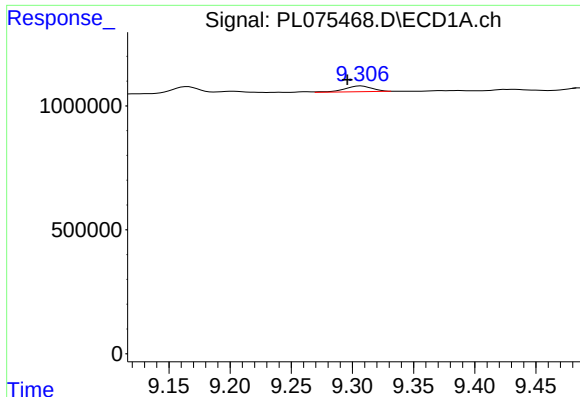

#15 Endosulfan II


R.T.: 9.307 min
Delta R.T.: 0.011 min
Response: 366129
Conc: 0.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

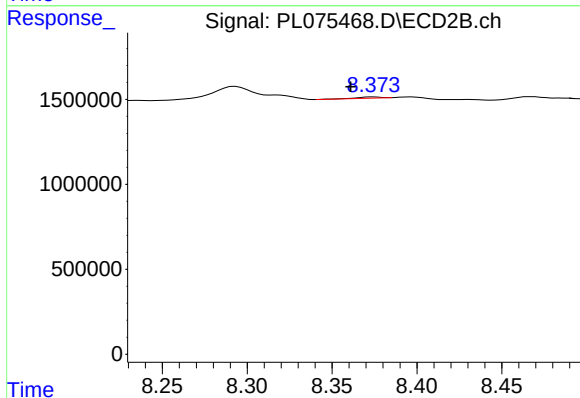


#15 Endosulfan II

R.T.: 8.374 min
Delta R.T.: 0.013 min
Response: 62665
Conc: 0.04 ng/ml

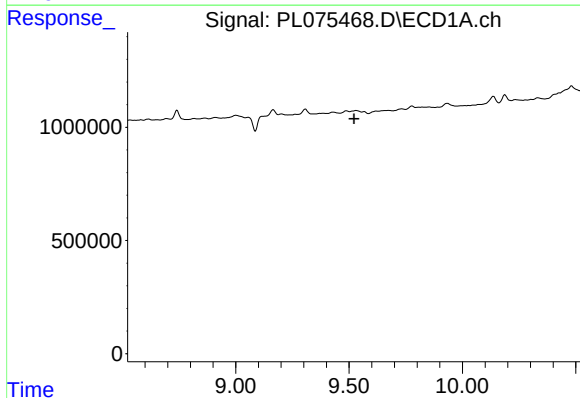


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

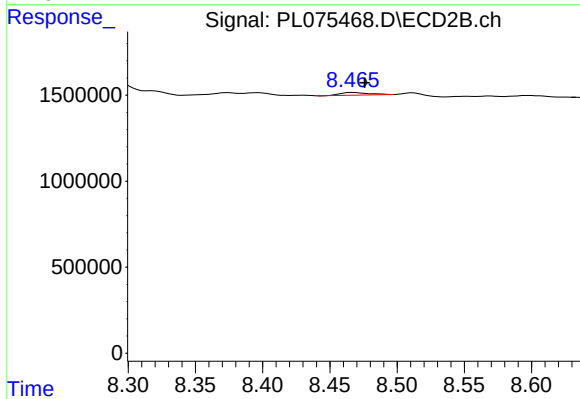

#17 4,4'-DDT


R.T.: 8.467 min
Delta R.T.: -0.009 min
Response: 224343
Conc: 0.16 ng/ml

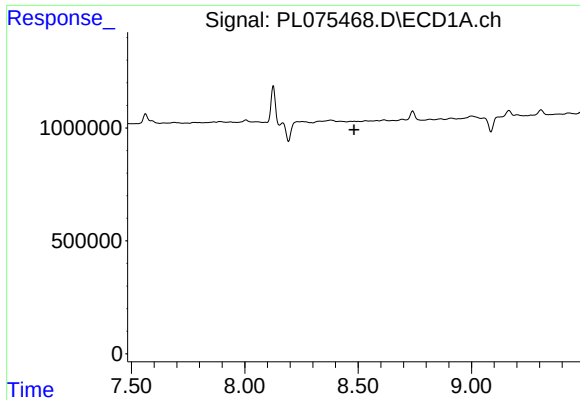

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.482 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

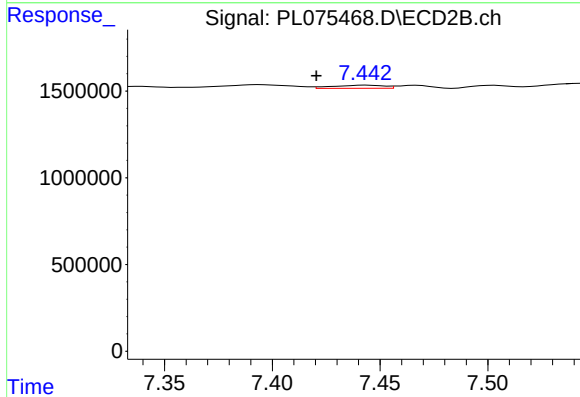


#26 Chlordane-4

R.T.: 7.443 min
Delta R.T.: 0.023 min
Response: 297545
Conc: 1.58 ng/ml

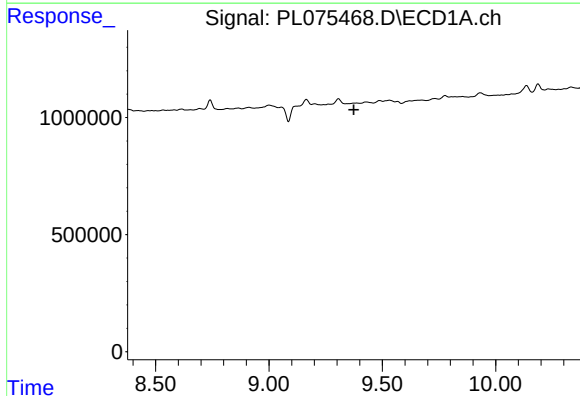


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

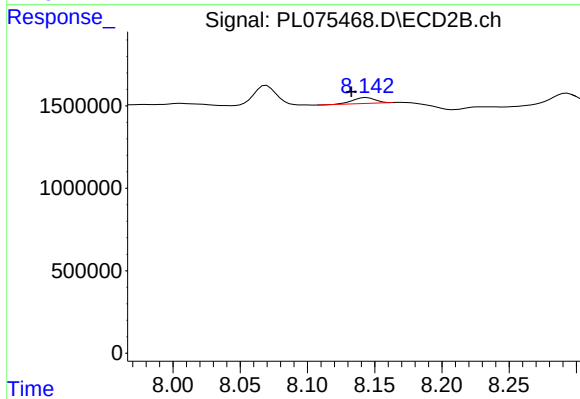

#27 Chlordane-5


R.T.: 8.144 min
Delta R.T.: 0.011 min
Response: 412792
Conc: 8.27 ng/ml

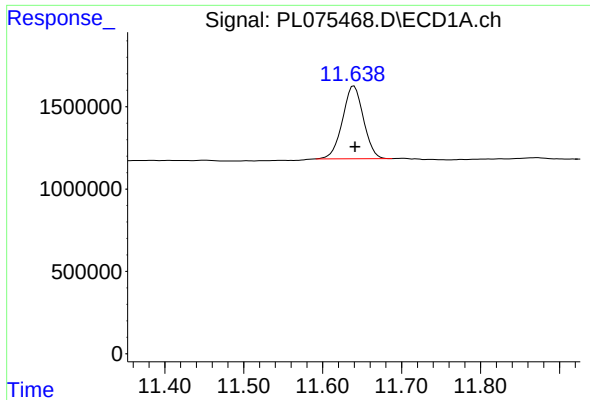

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.001 min
Response: 8145976
Conc: 15.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

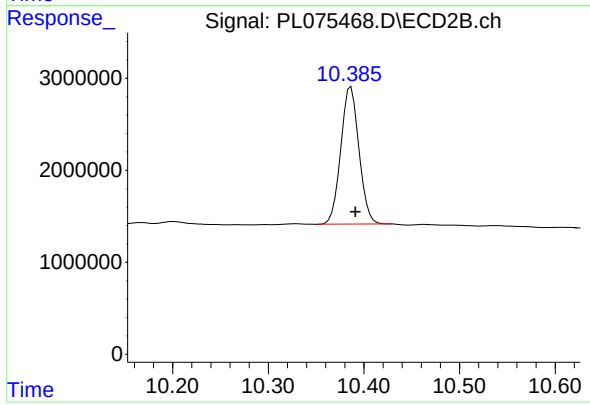

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: -0.005 min
Response: 19756669
Conc: 14.40 ng/ml