

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 19:25
 Operator : AR\AJ
 Sample : 3099-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:42:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.641	9389890	24788777	15.976	15.648
28)	SA Decachlor...	11.639	10.387	7129981	17458123	13.298	12.722
Target Compounds							
4)	MA Heptachlor	0.000	6.203f	0	248372	N.D.	0.122 #
7)	B delta-BHC	0.000	6.413	0	499339	N.D.	0.233 #
8)	B Heptachlo...	8.126	0.000	3401336	0	4.982	N.D. #
9)	A Endosulfan I	0.000	7.499f	0	155017	N.D.	0.092 #
10)	B gamma-Chl...	0.000	7.328f	0	281908	N.D.	0.153 #
13)	MA Dieldrin	0.000	7.763	0	3650495	N.D.	2.104 #
14)	MA Endrin	0.000	8.069f	0	5233415	N.D.	3.362 #
15)	B Endosulfa...	9.306	0.000	210187	0	0.372	N.D. #
17)	MA 4,4'-DDT	0.000	8.465	0	217488	N.D.	0.152 #
21)	B Endrin ke...	10.187f	0.000	403171	0	0.657	N.D. #
25)	Chlordane-3	0.000	7.328f	0	281908	N.D.	1.597 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 19:25
Operator : AR\AJ
Sample : 3099-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:42:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

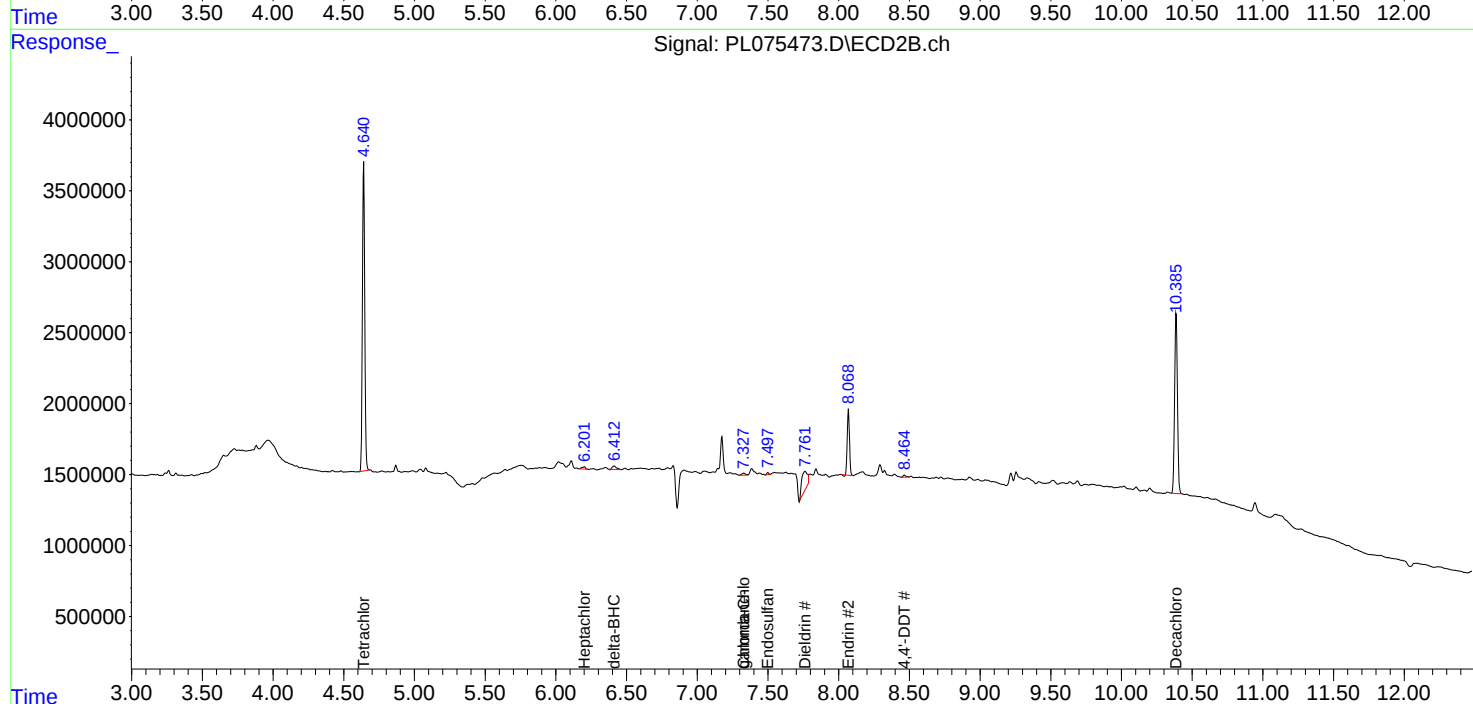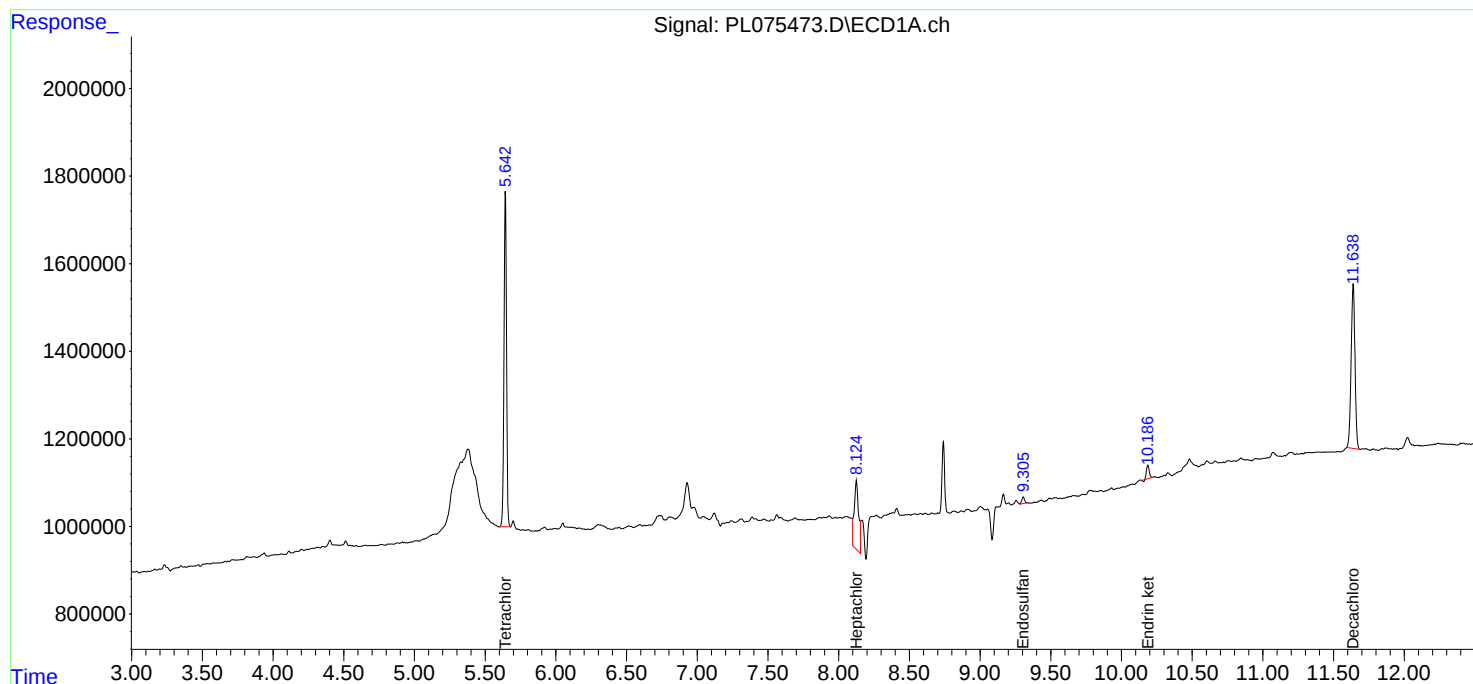


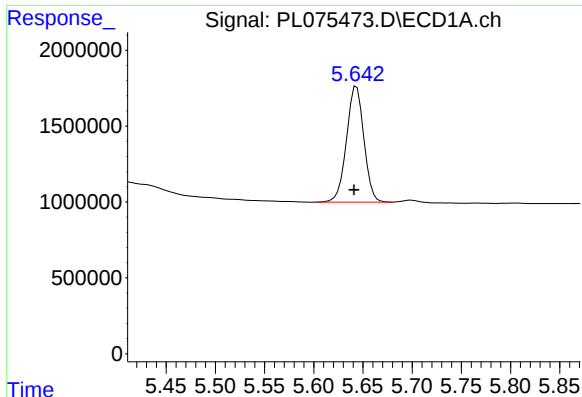

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 9389890
Conc: 15.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

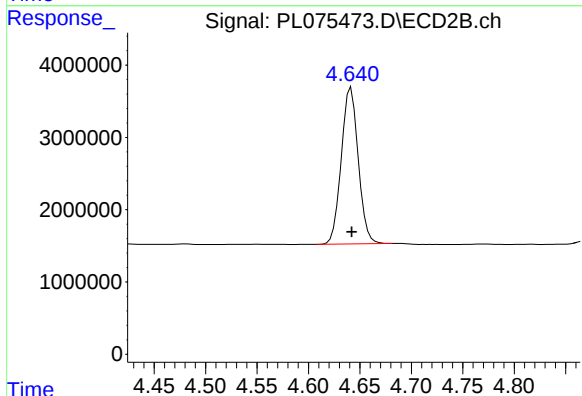


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 24788777
Conc: 15.65 ng/ml

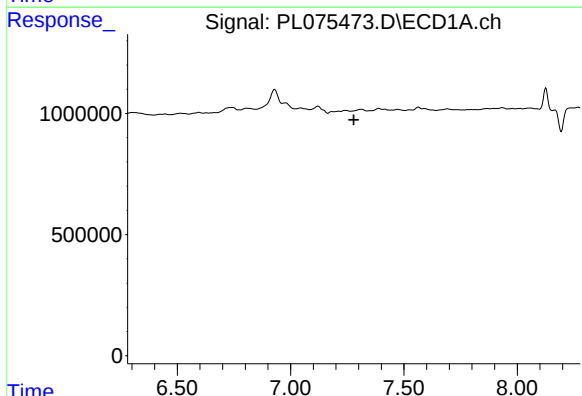


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.279 min
Response: 0
Conc: N.D.

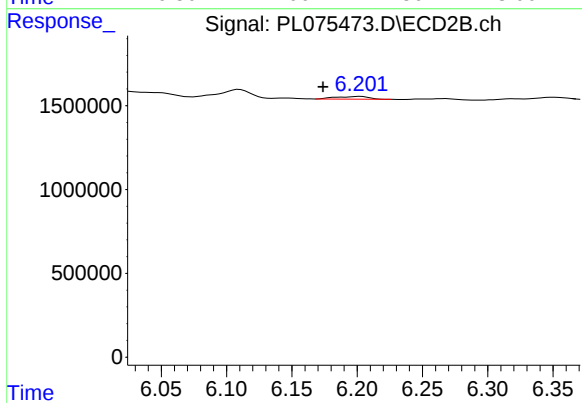

#4 Heptachlor


R.T.: 6.203 min
Delta R.T.: 0.029 min
Response: 248372
Conc: 0.12 ng/ml

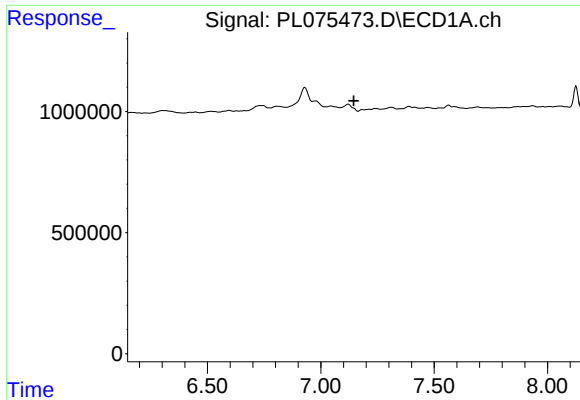

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.146 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

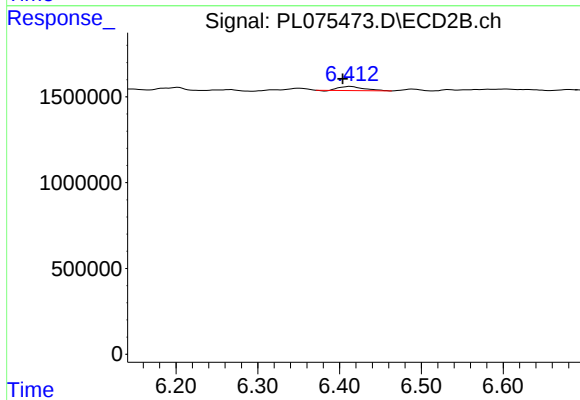


#7 delta-BHC

R.T.: 6.413 min
Delta R.T.: 0.009 min
Response: 499339
Conc: 0.23 ng/ml

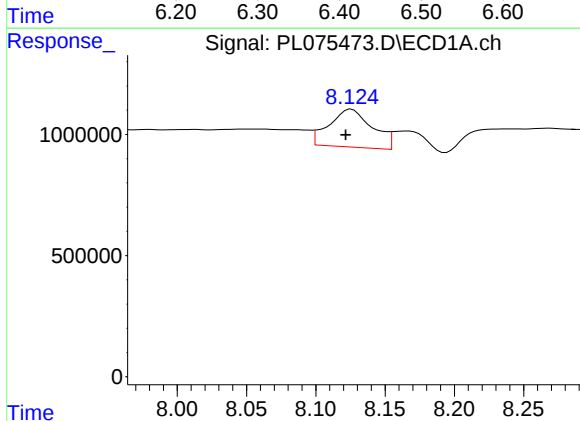


#8 Heptachlor epoxide

R.T.: 8.126 min
Delta R.T.: 0.004 min
Response: 3401336
Conc: 4.98 ng/ml

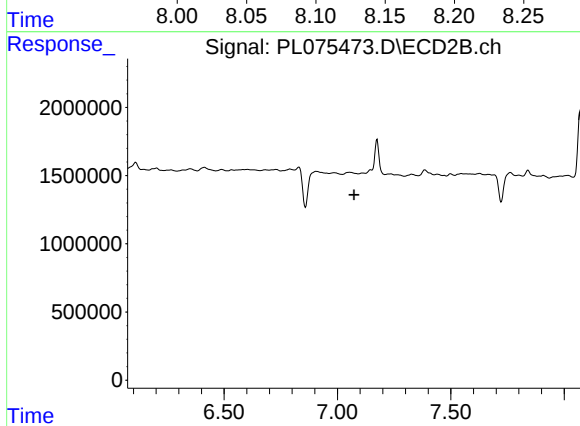

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.073 min
Response: 0
Conc: N.D.

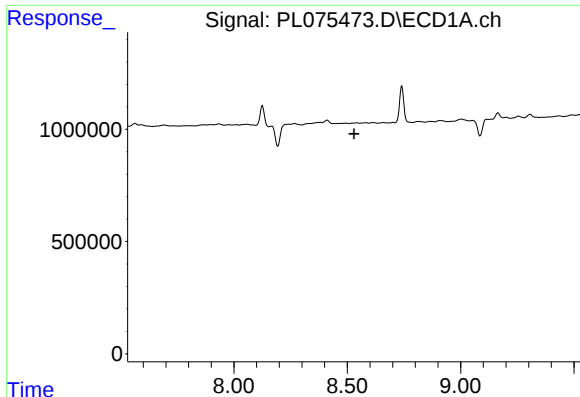

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

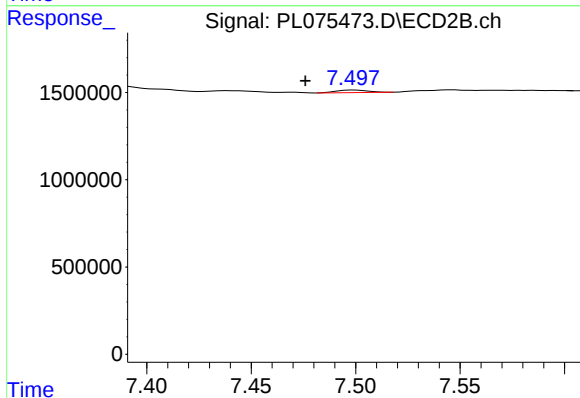


#9 Endosulfan I

R.T.: 7.499 min
Delta R.T.: 0.023 min
Response: 155017
Conc: 0.09 ng/ml

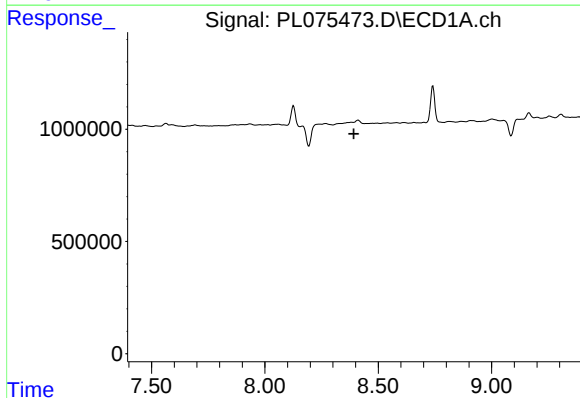


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.392 min
Response: 0
Conc: N.D.

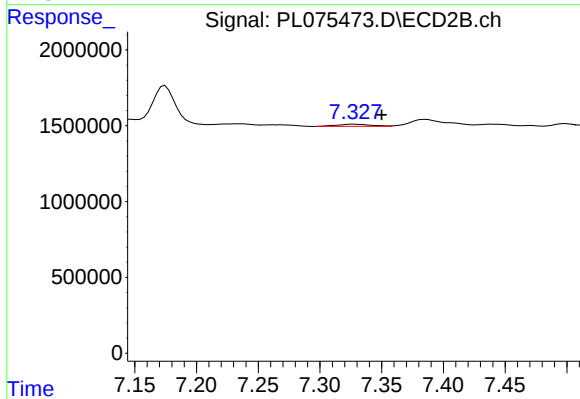

#10 gamma-Chlordane


R.T.: 7.328 min
Delta R.T.: -0.022 min
Response: 281908
Conc: 0.15 ng/ml

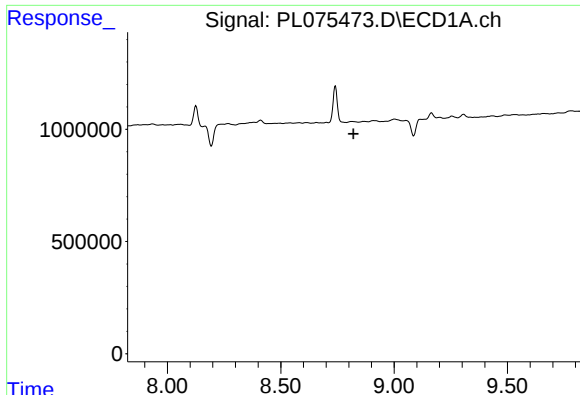

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

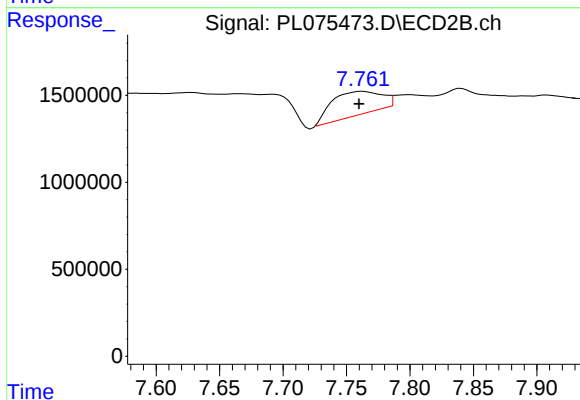


#13 Dieldrin

R.T.: 7.763 min
Delta R.T.: 0.003 min
Response: 3650495
Conc: 2.10 ng/ml

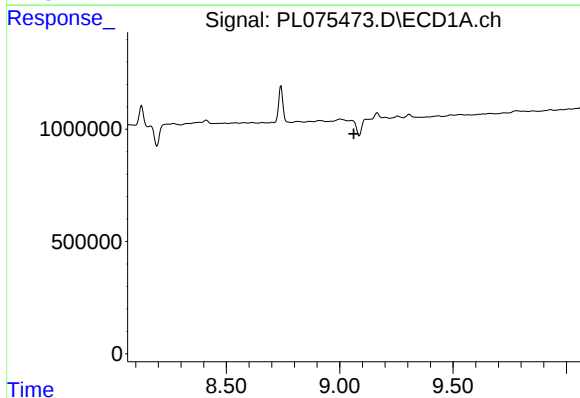


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.062 min
Response: 0
Conc: N.D.

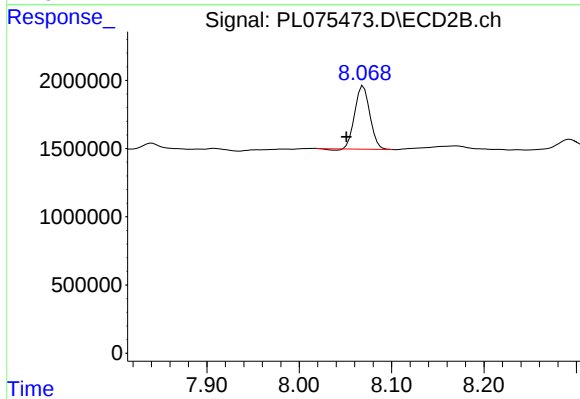

#14 Endrin


R.T.: 8.069 min
Delta R.T.: 0.018 min
Response: 5233415
Conc: 3.36 ng/ml

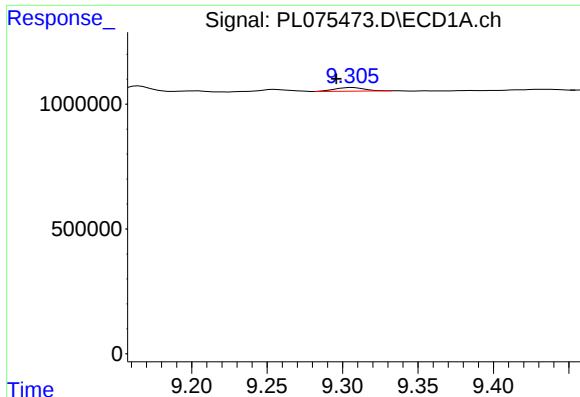

#15 Endosulfan II


R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 210187
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

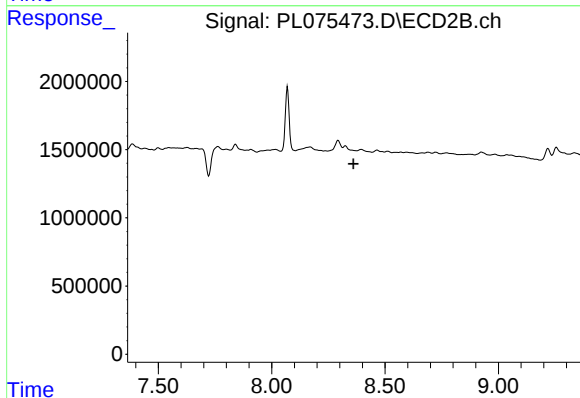


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

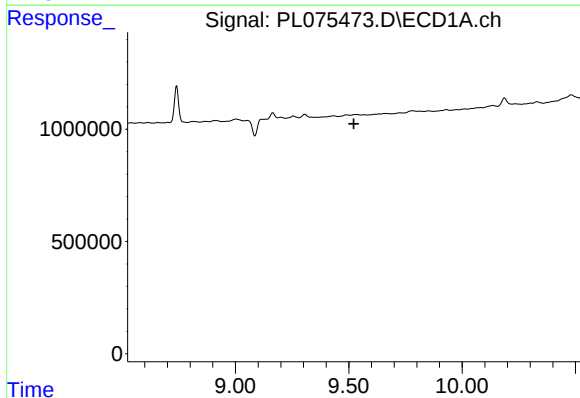


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

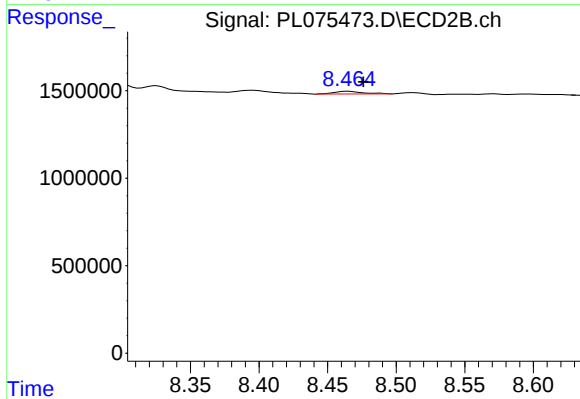

#17 4,4'-DDT


R.T.: 8.465 min
Delta R.T.: -0.011 min
Response: 217488
Conc: 0.15 ng/ml

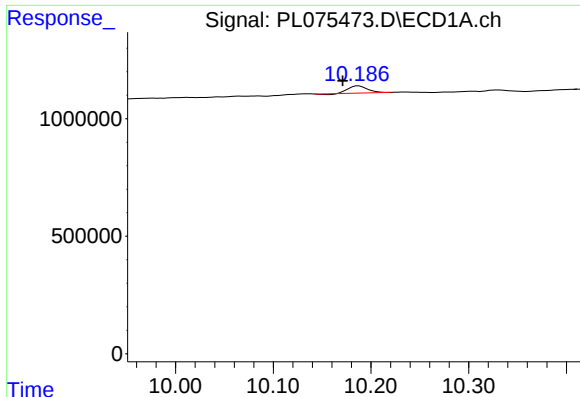

#21 Endrin ketone


R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 403171
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

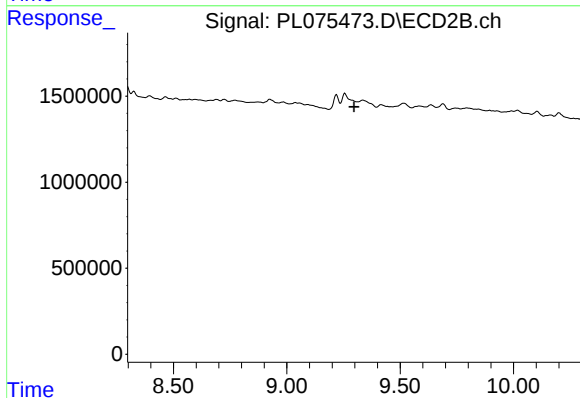


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.297 min
Response: 0
Conc: N.D.

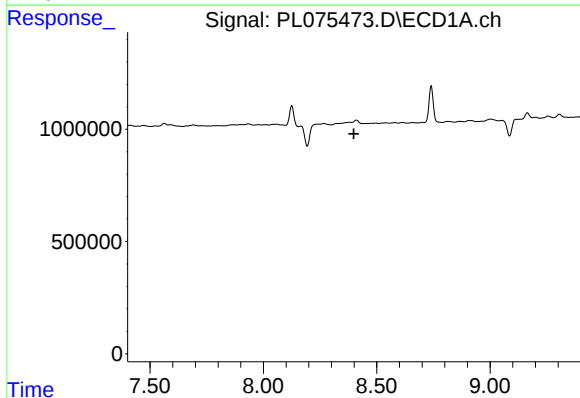


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.399 min
Response: 0
Conc: N.D.

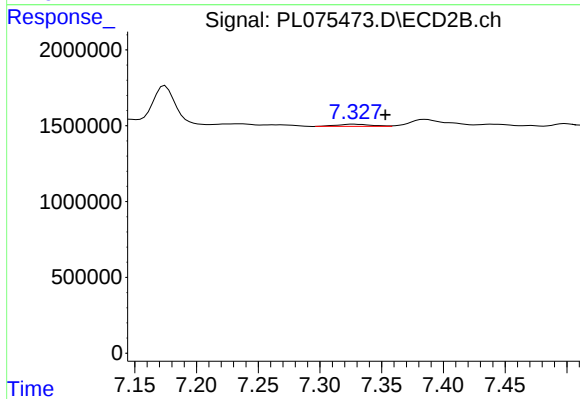

#25 Chlordane-3


R.T.: 7.328 min
Delta R.T.: -0.025 min
Response: 281908
Conc: 1.60 ng/ml

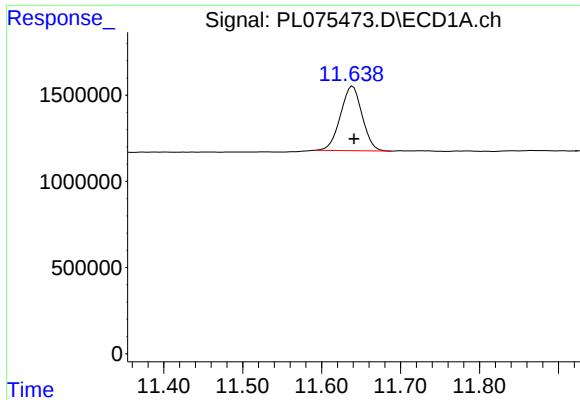

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 7129981
Conc: 13.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

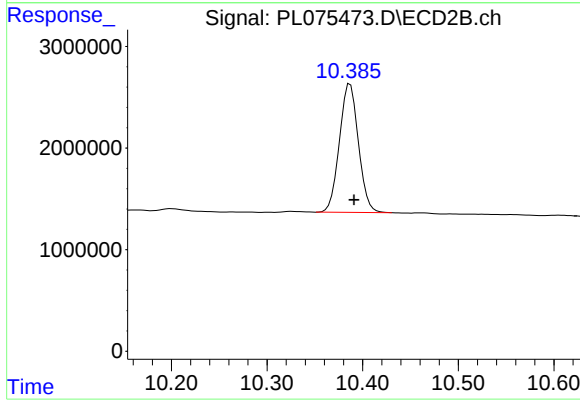

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.004 min
Response: 17458123
Conc: 12.72 ng/ml