

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 21:21
 Operator : AR\AJ
 Sample : N2987-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:45:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	6528267	17641200	11.107	11.136
28)	SA Decachlor...	11.639	10.387	5929028	14652283	11.058	10.677
Target Compounds							
7)	B delta-BHC	0.000	6.413	0	243897	N.D.	0.114 #
11)	B alpha-Chl...	0.000	7.395f	0	230460	N.D.	0.126 #
14)	MA Endrin	0.000	8.066	0	310774	N.D.	0.200 #
15)	B Endosulfa...	9.306	0.000	136594	0	0.242	N.D. #
16)	A 4,4'-DDD	9.203	0.000	343710	0	0.695	N.D. #
17)	MA 4,4'-DDT	0.000	8.464	0	677203	N.D.	0.474 #
19)	B Endosulfa...	0.000	8.775	0	503112	N.D.	0.336 #
21)	B Endrin ke...	10.187f	9.327f	300758	385792	0.490	0.241 #
26)	Chlordane-4	0.000	7.395f	0	230460	N.D.	1.220 #
27)	Chlordane-5	0.000	8.128	0	740701	N.D.	14.843 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 21:21
Operator : AR\AJ
Sample : N2987-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:45:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

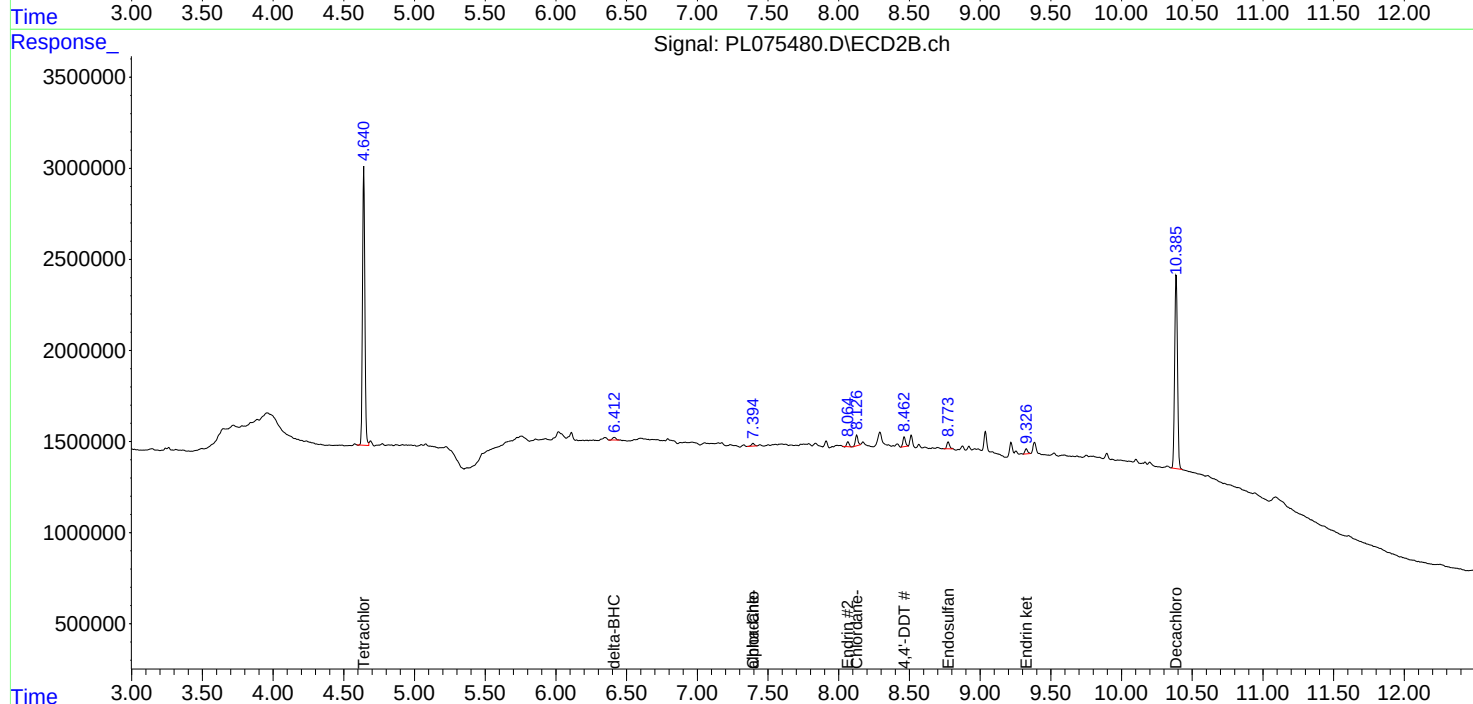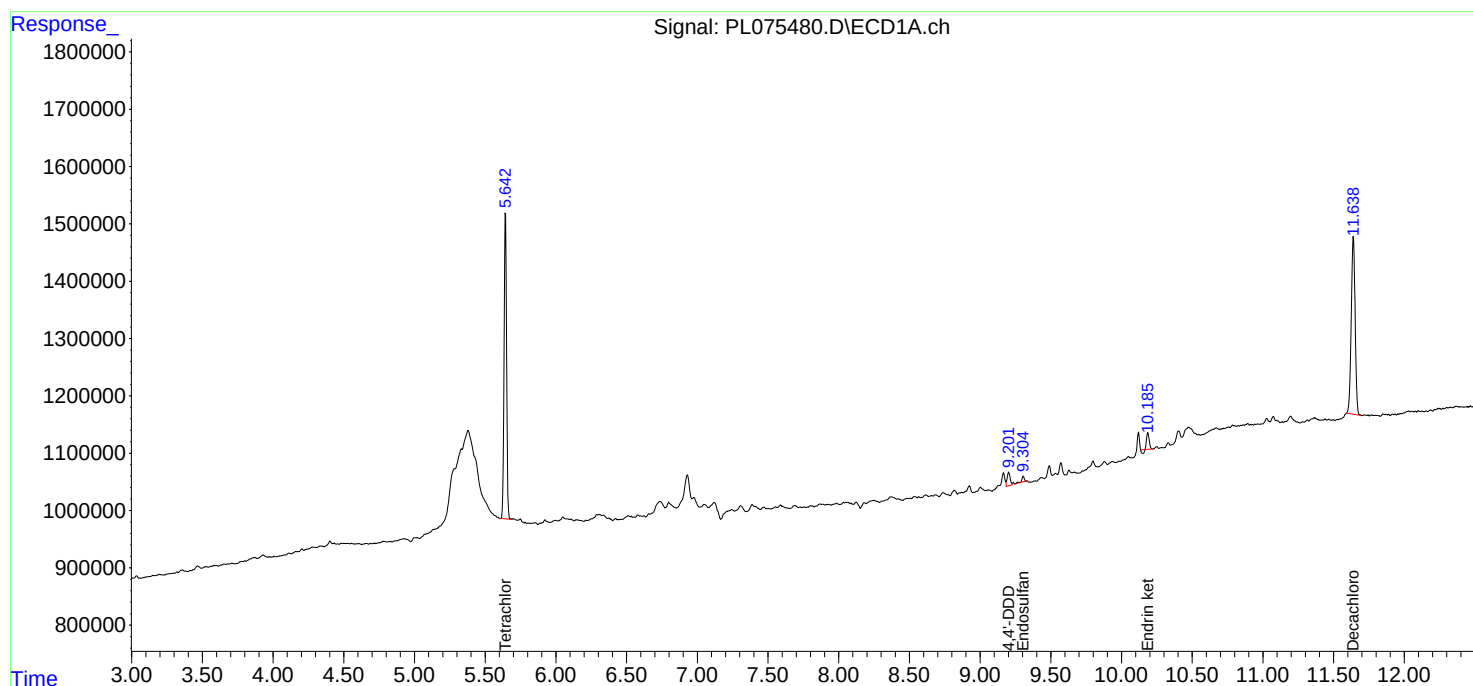


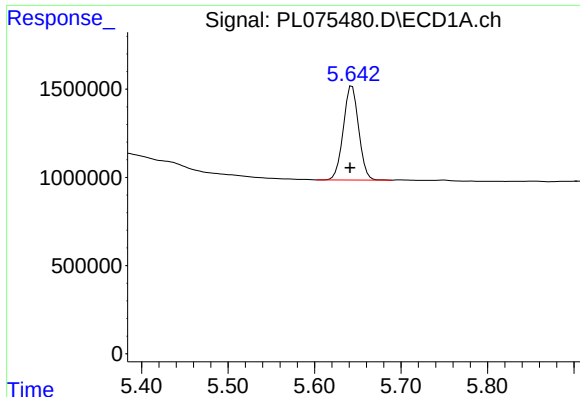

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 6528267
Conc: 11.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

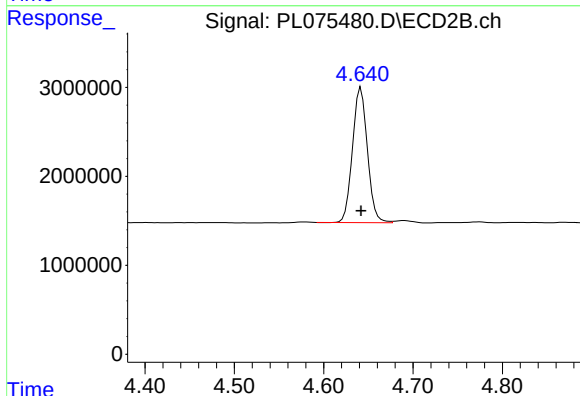


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 17641200
Conc: 11.14 ng/ml

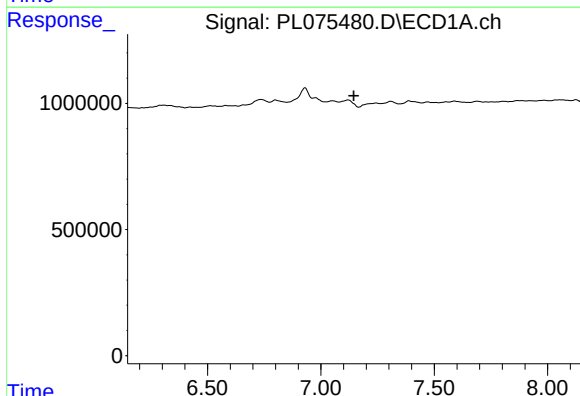


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

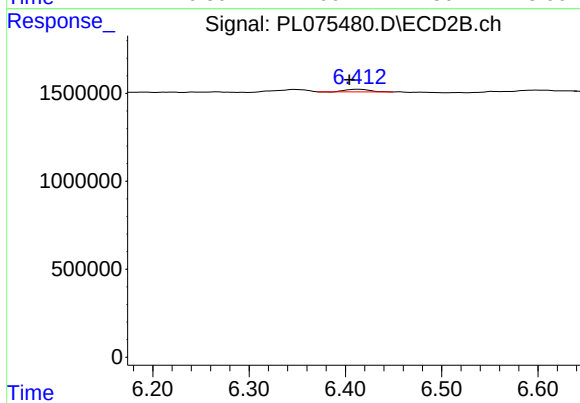

#7 delta-BHC


R.T.: 6.413 min
Delta R.T.: 0.009 min
Response: 243897
Conc: 0.11 ng/ml

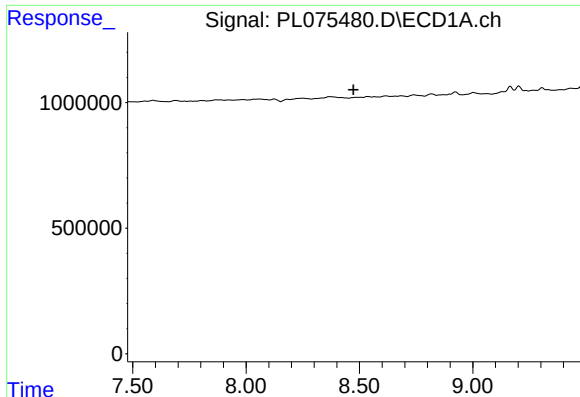

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

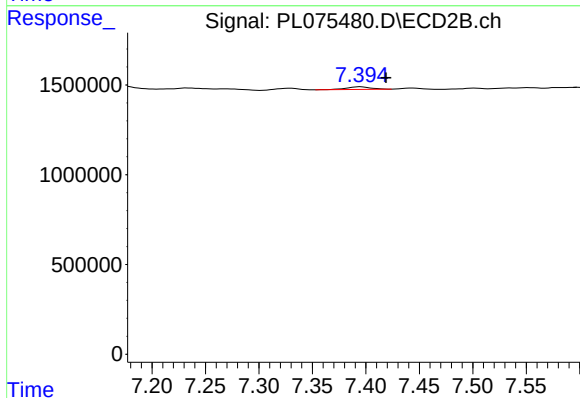


#11 alpha-Chlordane

R.T.: 7.395 min
Delta R.T.: -0.024 min
Response: 230460
Conc: 0.13 ng/ml

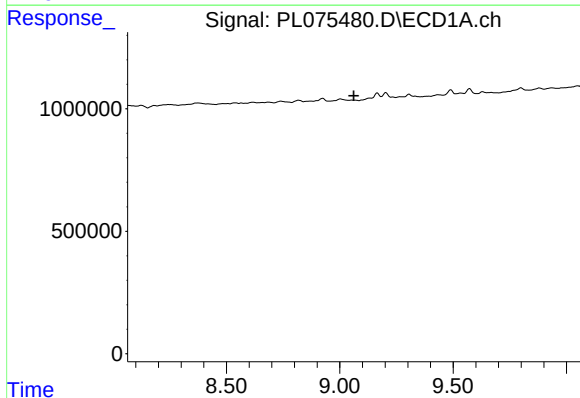


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

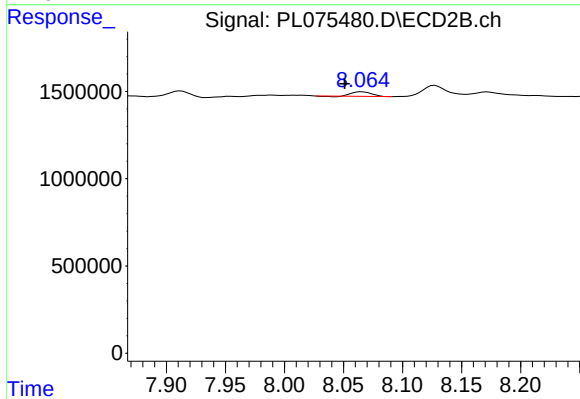

#14 Endrin


R.T.: 8.066 min
Delta R.T.: 0.015 min
Response: 310774
Conc: 0.20 ng/ml

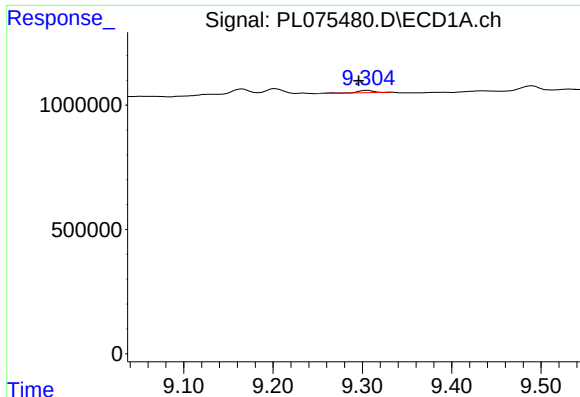

#15 Endosulfan II


R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 136594
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

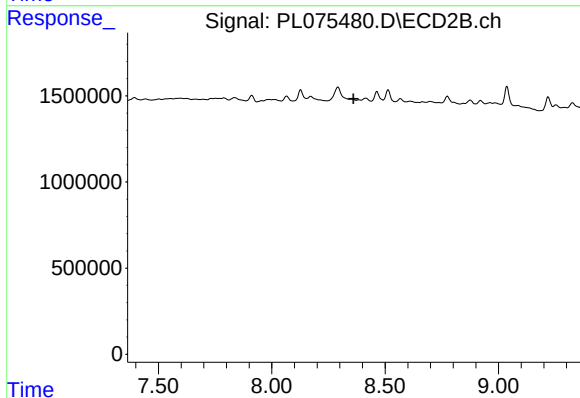


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

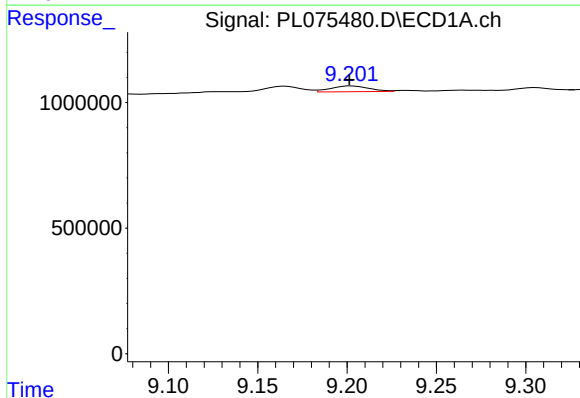


#16 4,4'-DDD

R.T.: 9.203 min
Delta R.T.: 0.001 min
Response: 343710
Conc: 0.69 ng/ml

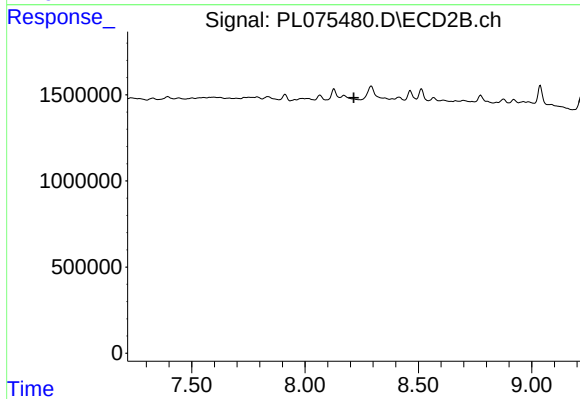

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 8.215 min
Response: 0
Conc: N.D.

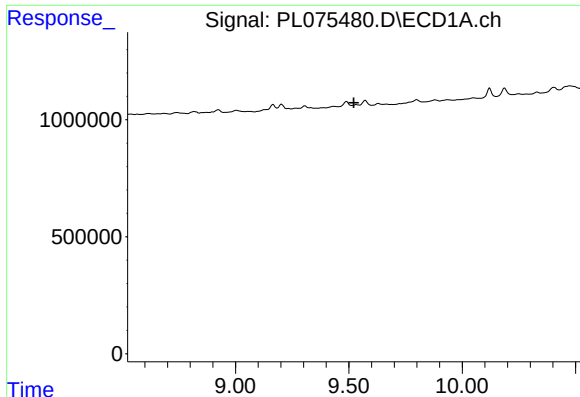

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

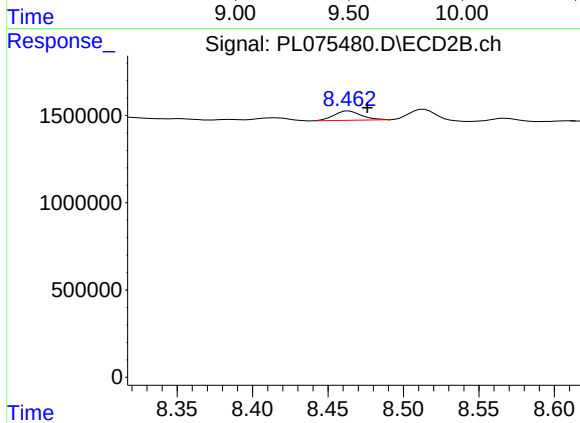


#17 4,4'-DDT

R.T.: 8.464 min
Delta R.T.: -0.012 min
Response: 677203
Conc: 0.47 ng/ml

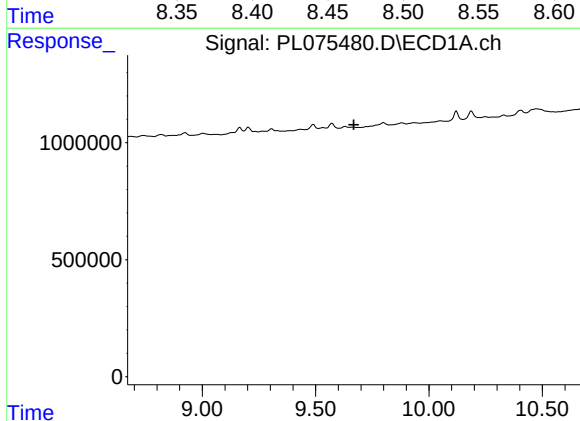


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.669 min
Response: 0
Conc: N.D.

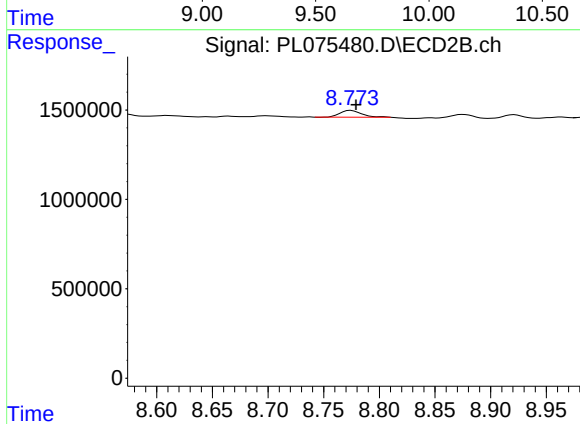

#19 Endosulfan Sulfate


R.T.: 8.775 min
Delta R.T.: -0.004 min
Response: 503112
Conc: 0.34 ng/ml

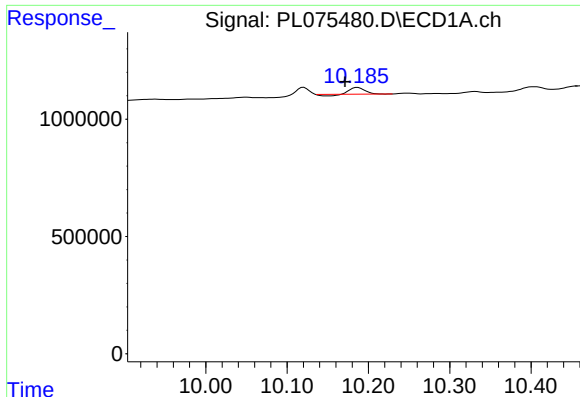

#21 Endrin ketone


R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 300758
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

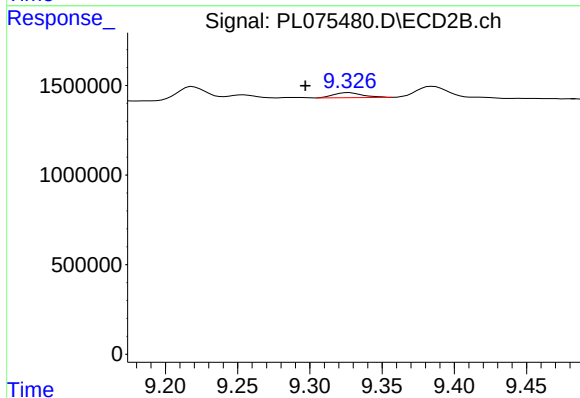


#21 Endrin ketone

R.T.: 9.327 min
Delta R.T.: 0.030 min
Response: 385792
Conc: 0.24 ng/ml

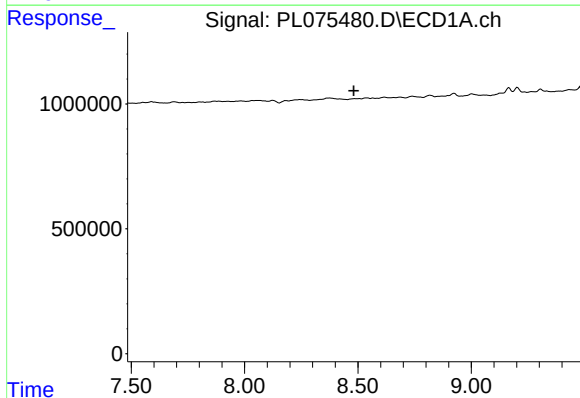


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

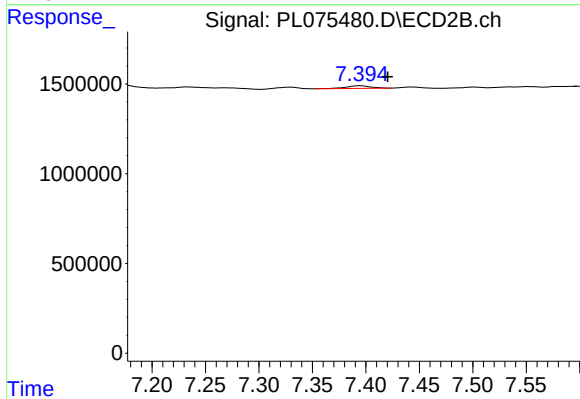

#26 Chlordane-4


R.T.: 7.395 min
Delta R.T.: -0.026 min
Response: 230460
Conc: 1.22 ng/ml

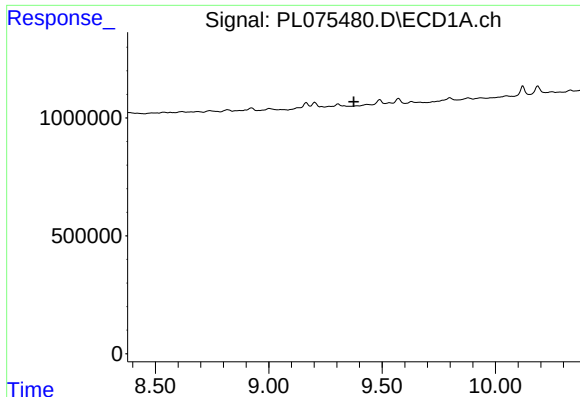

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

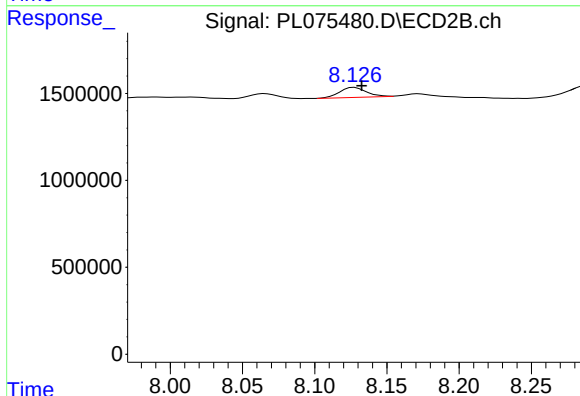


#27 Chlordane-5

R.T.: 8.128 min
Delta R.T.: -0.005 min
Response: 740701
Conc: 14.84 ng/ml

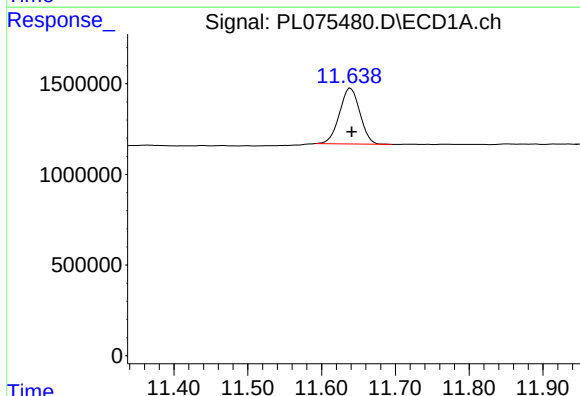

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 5929028
Conc: 11.06 ng/ml

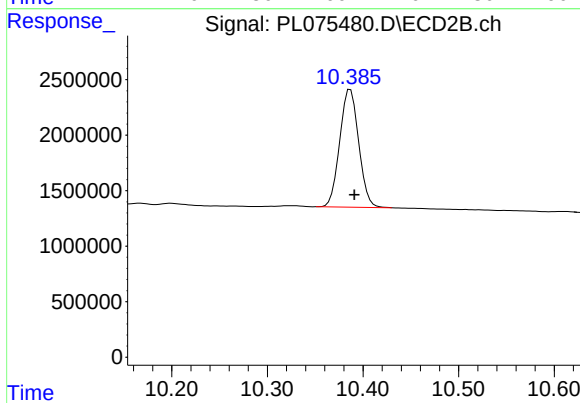

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.004 min
Response: 14652283
Conc: 10.68 ng/ml