

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 21:37
 Operator : AR\AJ
 Sample : N2987-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:46:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.642	6266736	17030475	10.662	10.751
28)	SA Decachlor...	11.639	10.387	5892117	14279421	10.989	10.406
Target Compounds							
7)	B delta-BHC	0.000	6.413	0	339045	N.D.	0.158 #
8)	B Heptachlo...	8.126	0.000	1595362	0	2.337	N.D. #
13)	MA Dieldrin	0.000	7.764	0	1393514	N.D.	0.803 #
14)	MA Endrin	0.000	8.069f	0	781459	N.D.	0.502 #
15)	B Endosulfa...	9.306	0.000	117520	0	0.208	N.D. #
16)	A 4,4'-DDD	9.204	0.000	430908	0	0.871	N.D. #
17)	MA 4,4'-DDT	0.000	8.464	0	690786	N.D.	0.483 #
19)	B Endosulfa...	0.000	8.775	0	484675	N.D.	0.324 #
21)	B Endrin ke...	10.187f	0.000	187282	0	0.305	N.D. #
27)	Chlordane-5	0.000	8.128	0	772760	N.D.	15.486 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 21:37
Operator : AR\AJ
Sample : N2987-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:46:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

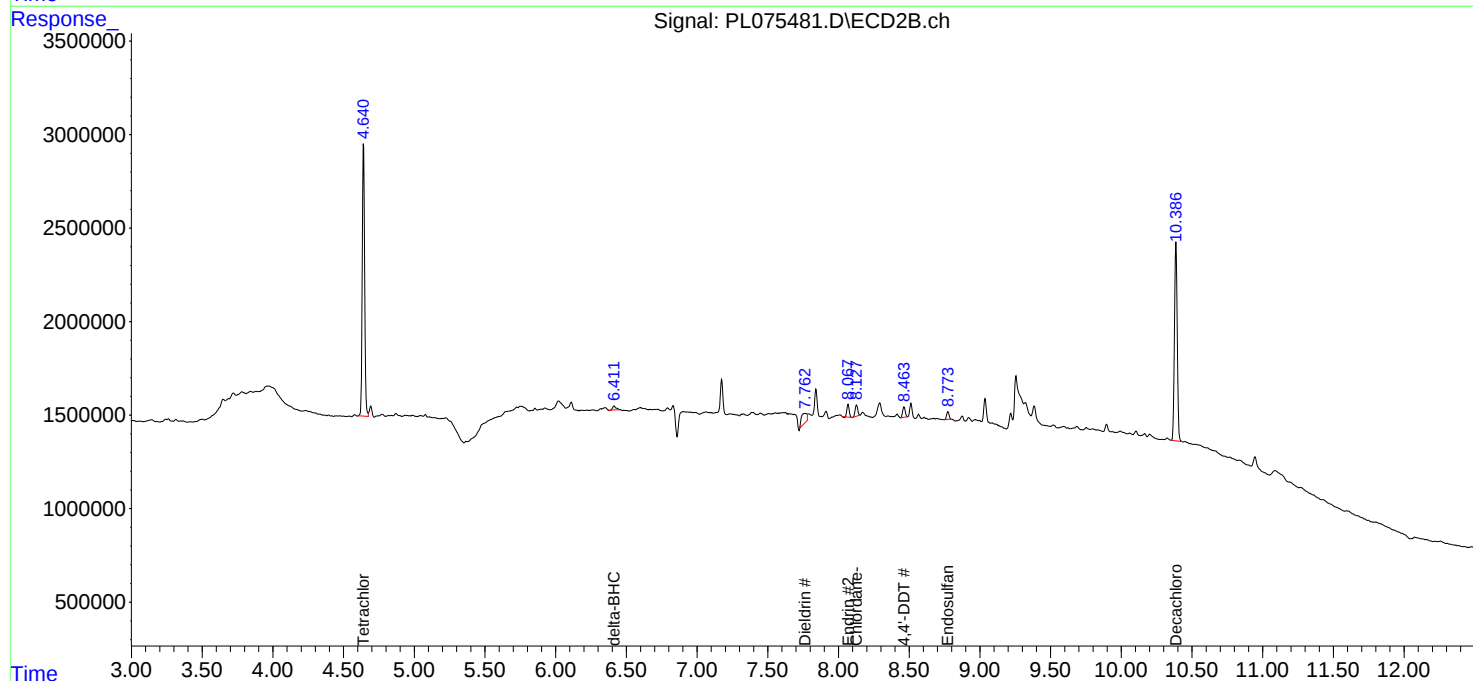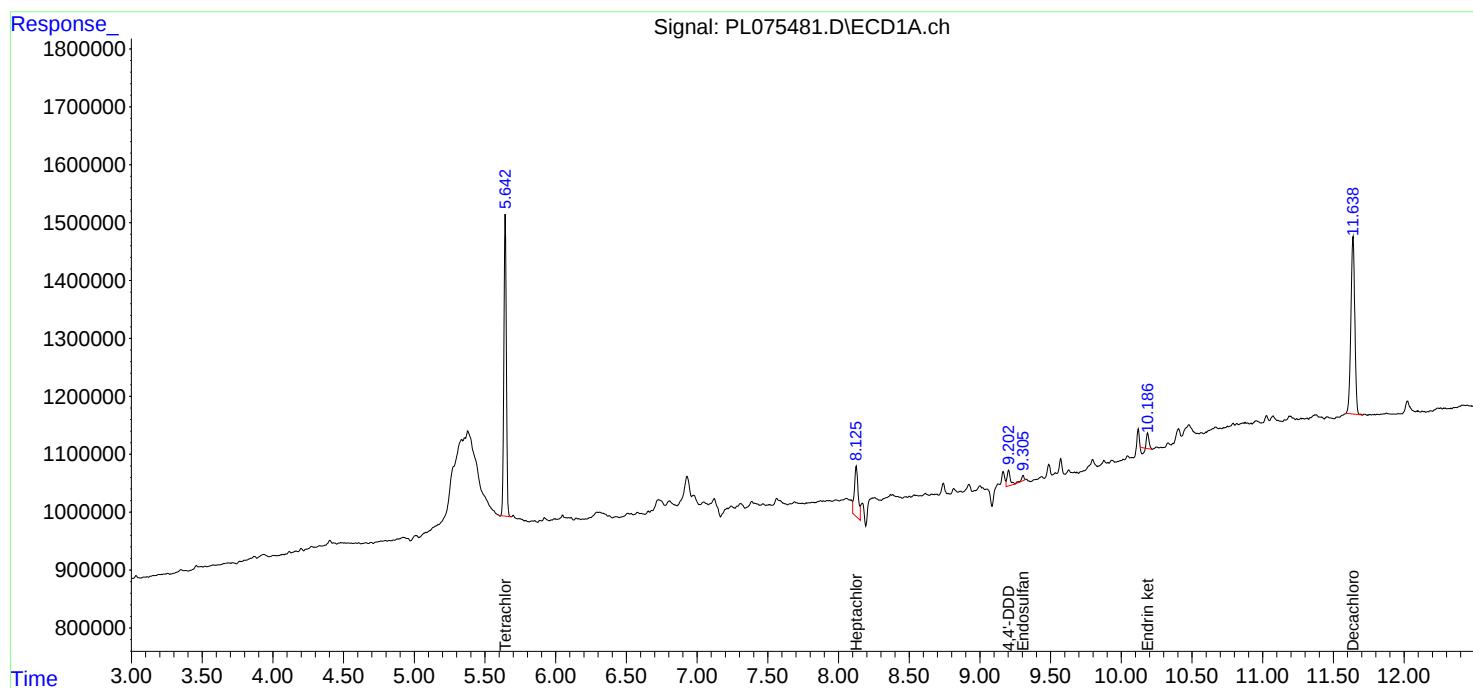


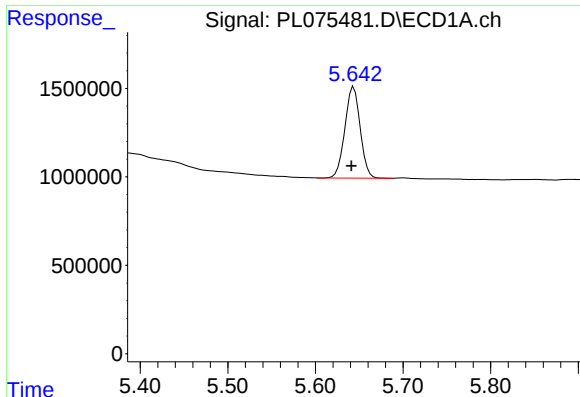

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 6266736
Conc: 10.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

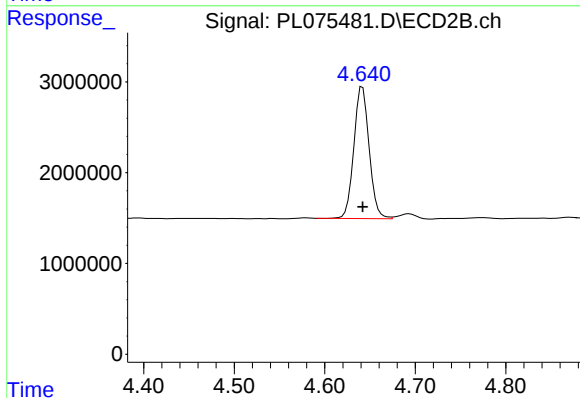


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 17030475
Conc: 10.75 ng/ml

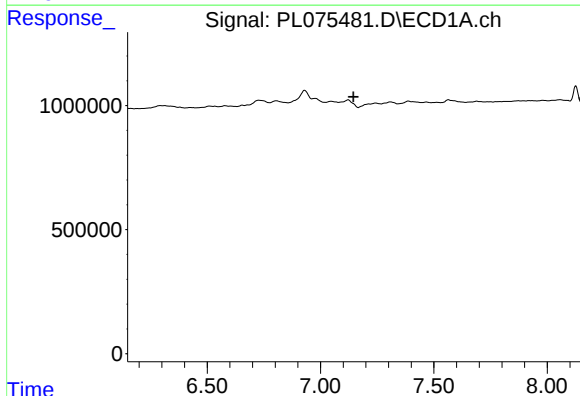


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

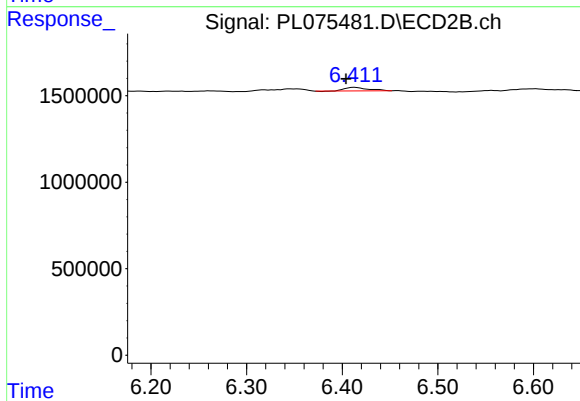

#7 delta-BHC


R.T.: 6.413 min
Delta R.T.: 0.009 min
Response: 339045
Conc: 0.16 ng/ml

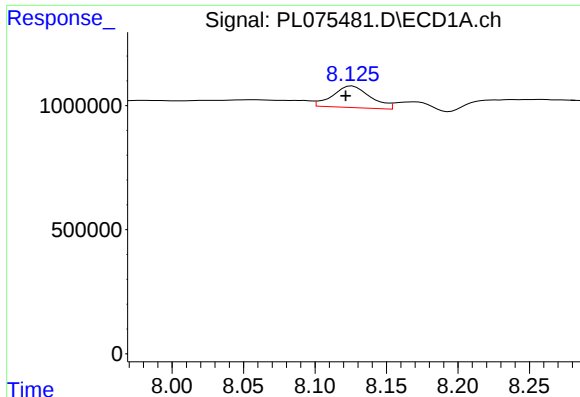

#8 Heptachlor epoxide


R.T.: 8.126 min
Delta R.T.: 0.004 min
Response: 1595362
Conc: 2.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

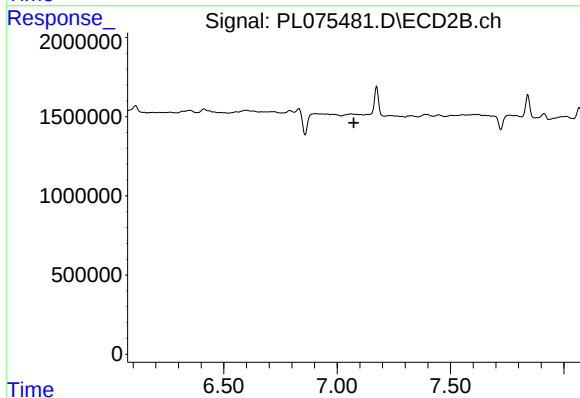


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.073 min
Response: 0
Conc: N.D.

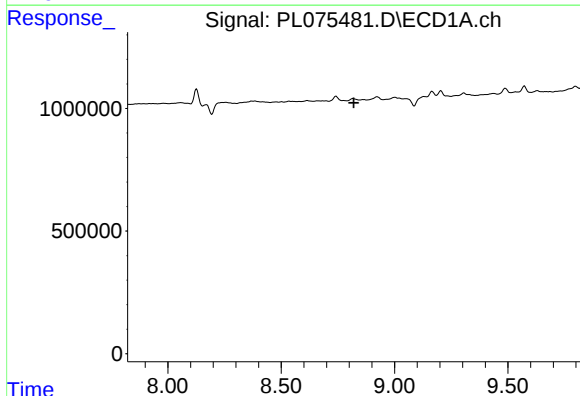


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

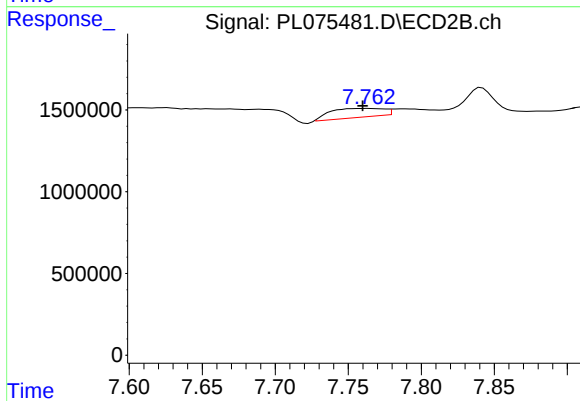

#13 Dieldrin


R.T.: 7.764 min
Delta R.T.: 0.004 min
Response: 1393514
Conc: 0.80 ng/ml

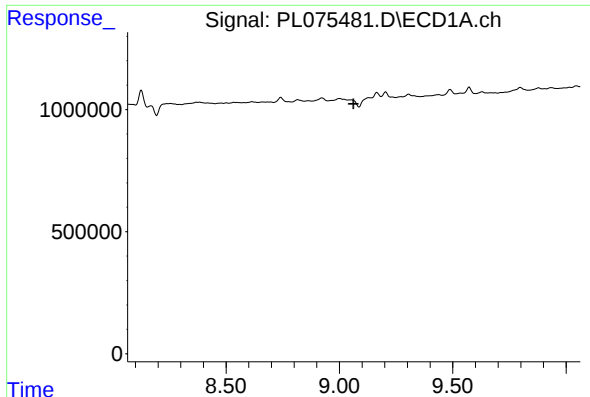

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

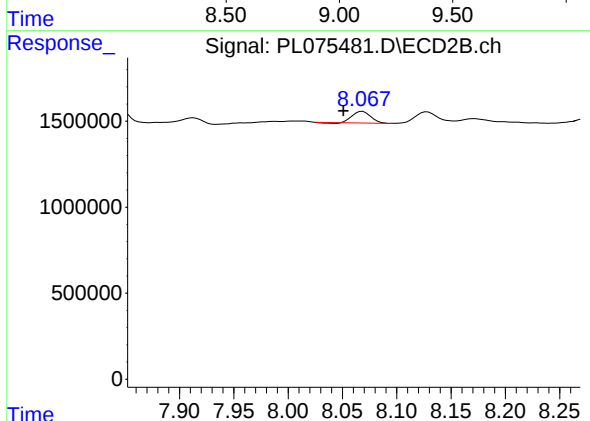


#14 Endrin

R.T.: 8.069 min
Delta R.T.: 0.018 min
Response: 781459
Conc: 0.50 ng/ml

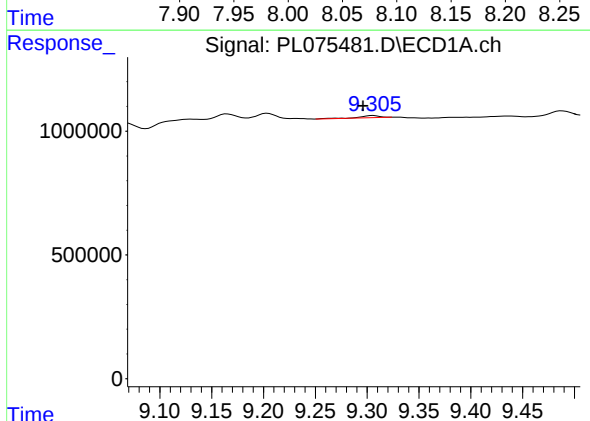


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 117520
Conc: 0.21 ng/ml

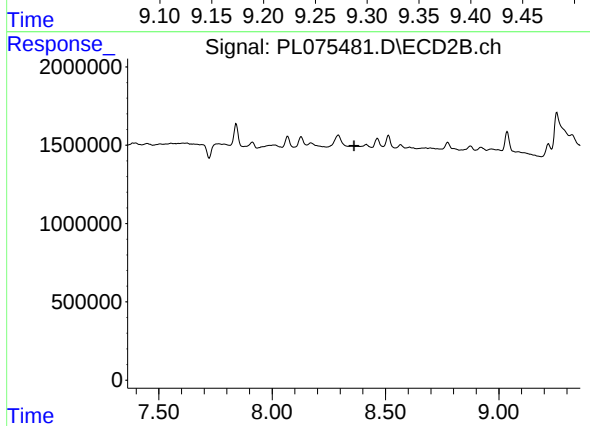

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

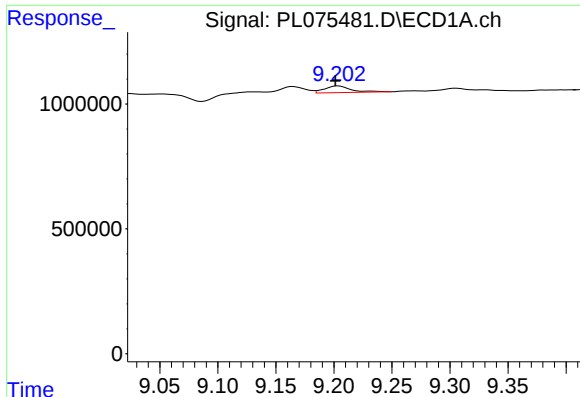

#16 4,4'-DDD


R.T.: 9.204 min
Delta R.T.: 0.003 min
Response: 430908
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

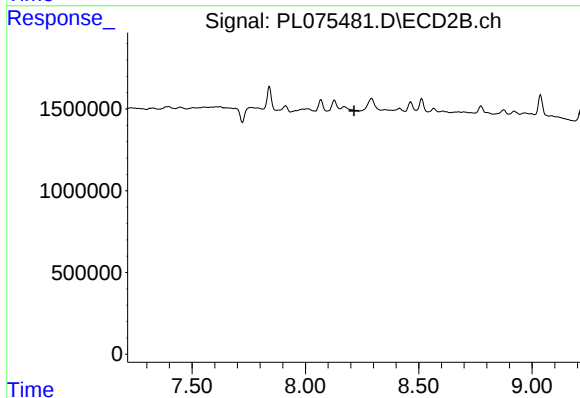


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.215 min
Response: 0
Conc: N.D.

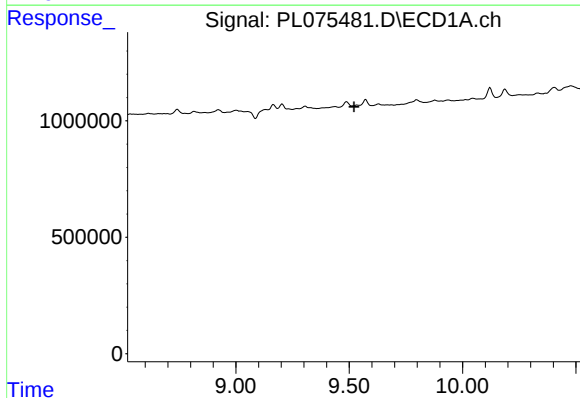


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

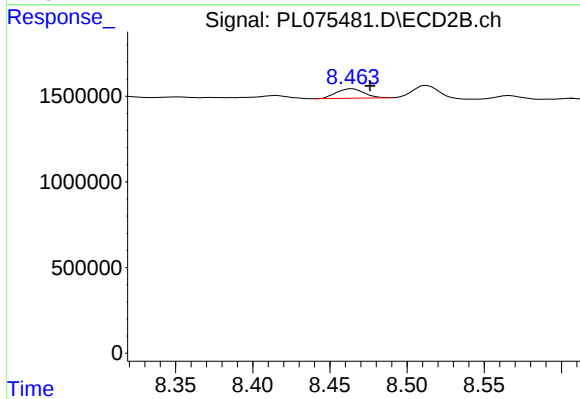

#17 4,4'-DDT


R.T.: 8.464 min
Delta R.T.: -0.012 min
Response: 690786
Conc: 0.48 ng/ml

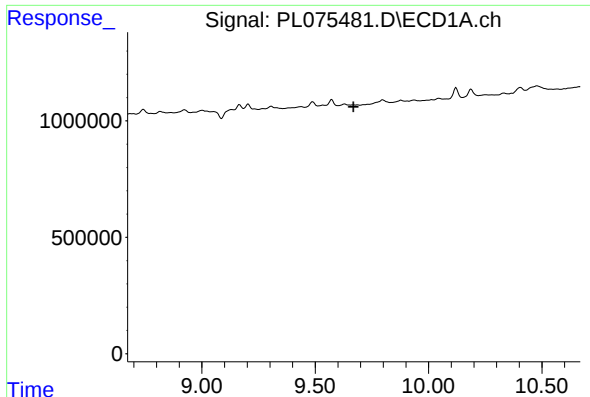

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

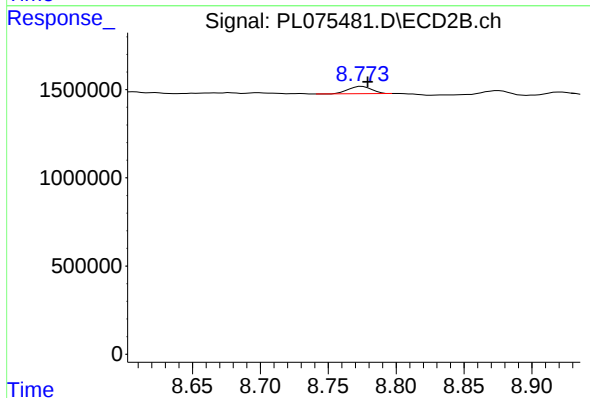


#19 Endosulfan Sulfate

R.T.: 8.775 min
Delta R.T.: -0.004 min
Response: 484675
Conc: 0.32 ng/ml

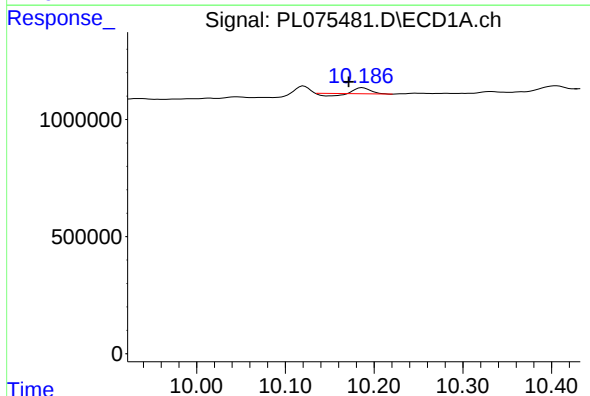


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 187282
Conc: 0.31 ng/ml

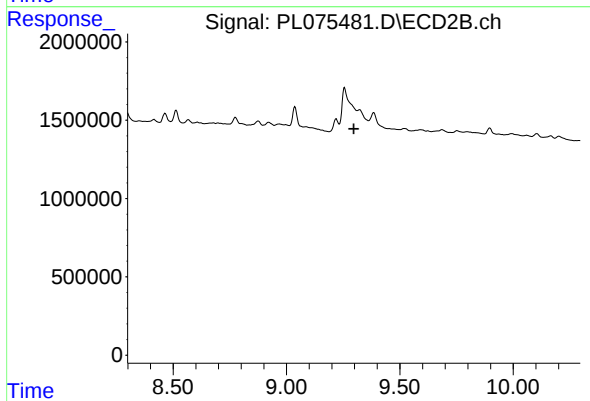

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.297 min
Response: 0
Conc: N.D.

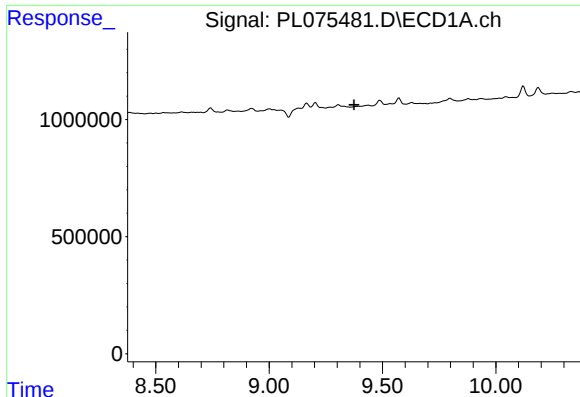

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

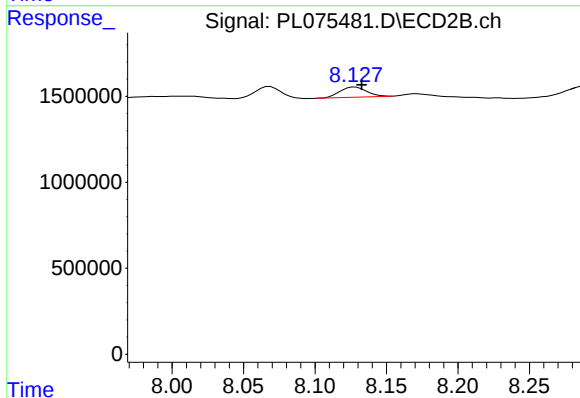


#27 Chlordane-5

R.T.: 8.128 min
Delta R.T.: -0.005 min
Response: 772760
Conc: 15.49 ng/ml

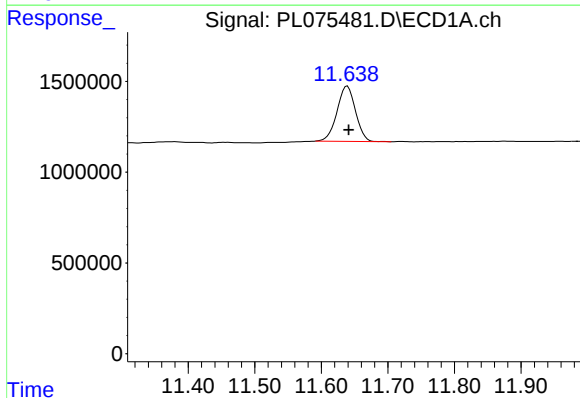

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 5892117
Conc: 10.99 ng/ml

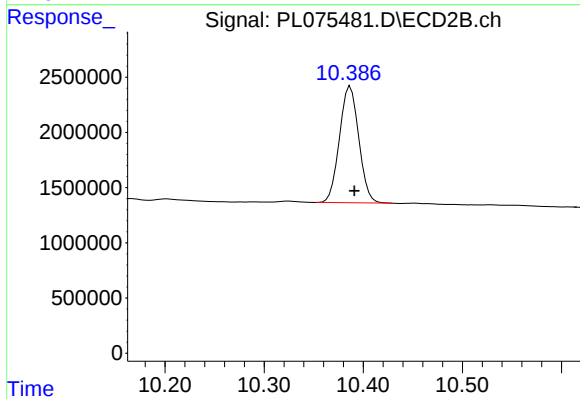

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.004 min
Response: 14279421
Conc: 10.41 ng/ml